

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051925\
 Data File : VX046256.D
 Acq On : 19 May 2025 10:39
 Operator : JC/MD
 Sample : VX0519MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0519MBL01

Quant Time: May 19 23:06:09 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 06 07:12:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.537	168	63875	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.751	114	126268	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	121867	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	52500	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	64149	53.869	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	107.740%
35) Dibromofluoromethane	5.379	113	46655	51.311	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.620%
50) Toluene-d8	8.647	98	158856	50.477	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	100.960%
62) 4-Bromofluorobenzene	11.079	95	61486	50.934	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	101.860%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051925\
Data File : VX046256.D
Acq On : 19 May 2025 10:39
Operator : JC/MD
Sample : VX0519MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0519MBL01

Quant Time: May 19 23:06:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
Quant Title : SW846 8260
QLast Update : Tue May 06 07:12:22 2025
Response via : Initial Calibration




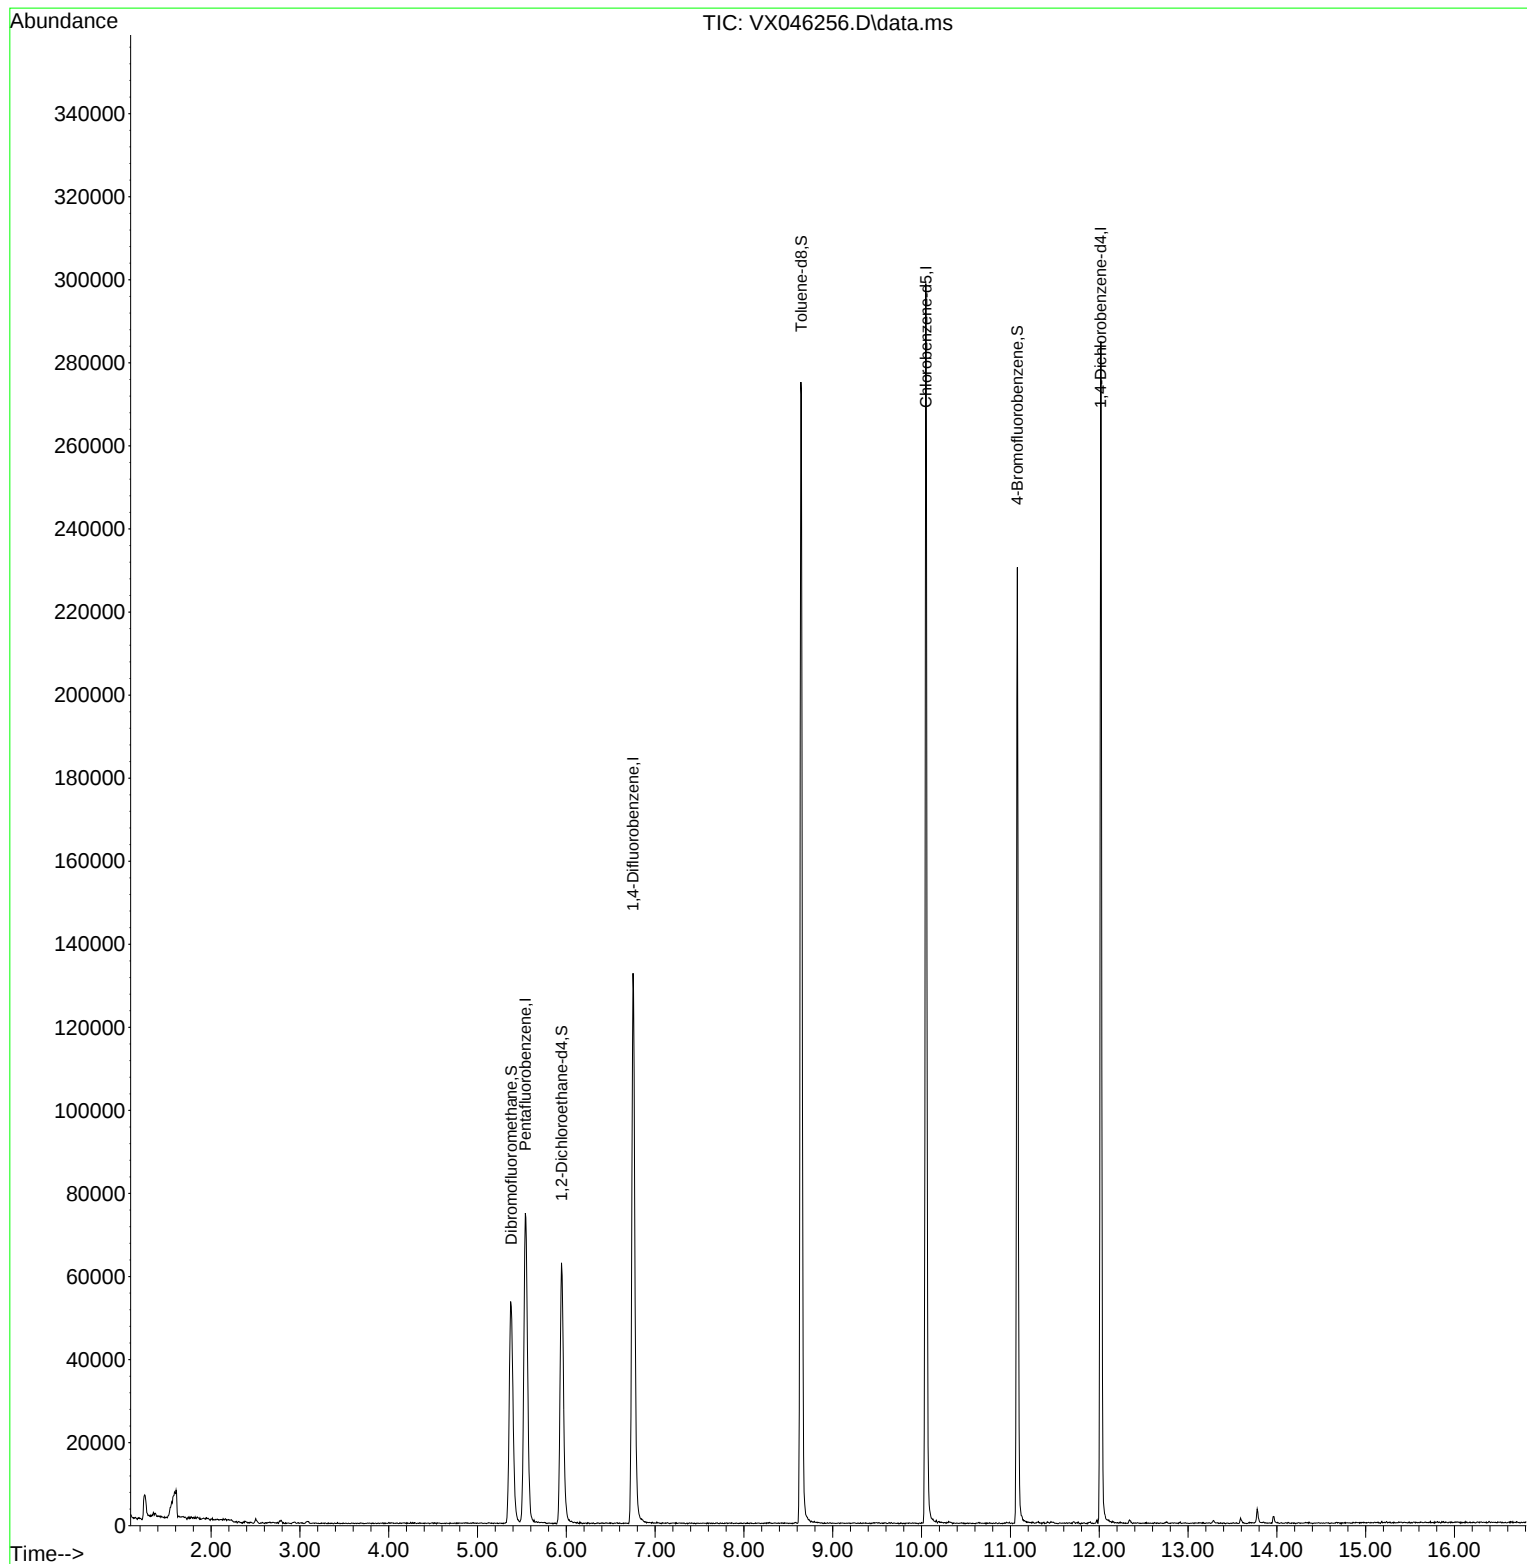




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.537 min Scan# 71
Delta R.T. -0.007 min
Lab File: VX046256.D
Acq: 19 May 2025 10:39




Instrument :
MSVOA_X
ClientSampleId :
VX0519MBL01


Tgt Ion:168 Resp: 63875
Ion Ratio Lower Upper
168 100
99 71.0 54.9 82.3

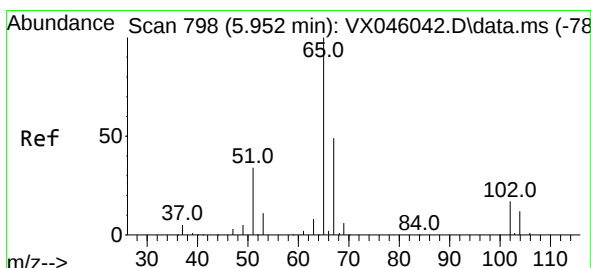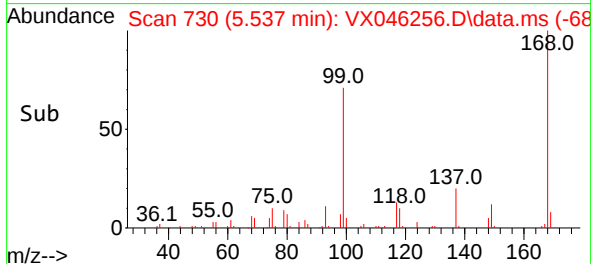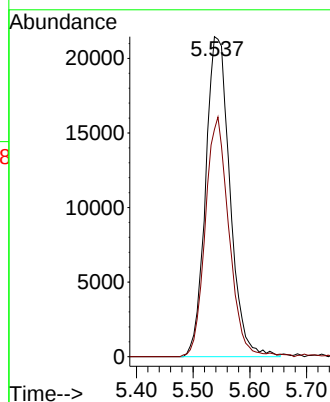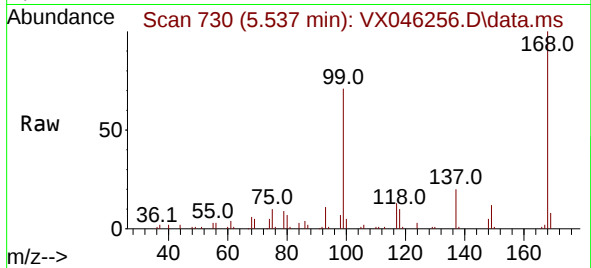

#33
1,2-Dichloroethane-d4
Concen: 53.869 ug/l
RT: 5.946 min Scan# 797
Delta R.T. -0.006 min
Lab File: VX046256.D
Acq: 19 May 2025 10:39

Tgt Ion: 65 Resp: 64149
Ion Ratio Lower Upper
65 100
67 49.4 0.0 99.0

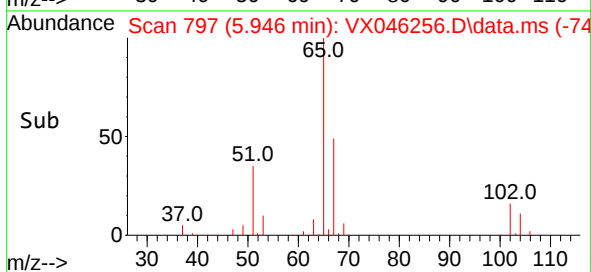
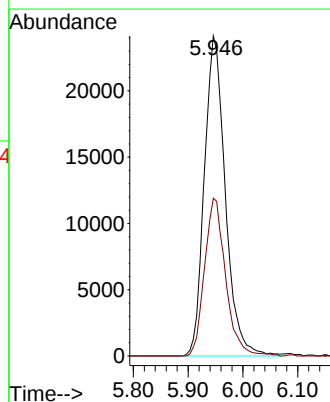
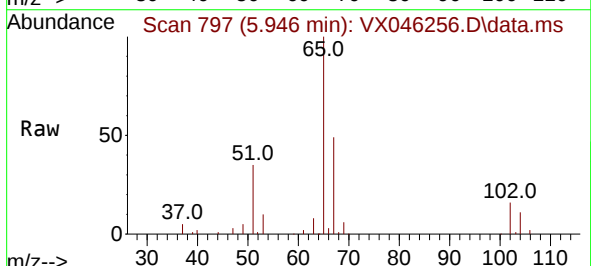


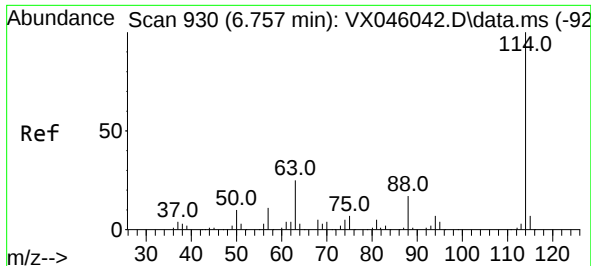

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.751 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX046256.D
Acq: 19 May 2025 10:39




Instrument :
MSVOA_X
ClientSampleId :
VX0519MBL01


Tgt Ion:114 Resp: 126268
Ion Ratio Lower Upper
114 100
63 23.9 0.0 49.2
88 18.0 0.0 33.6

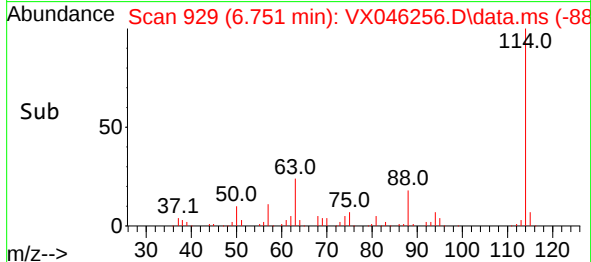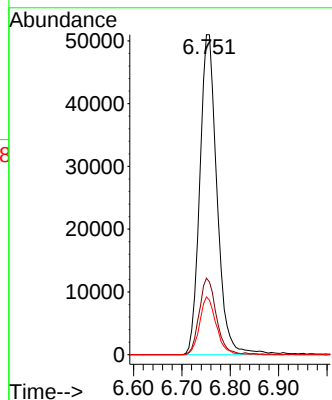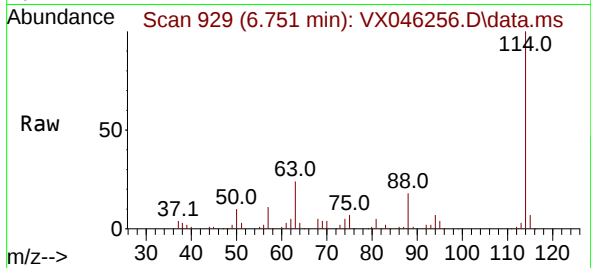

#35
Dibromofluoromethane
Concen: 51.311 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX046256.D
Acq: 19 May 2025 10:39

Tgt Ion:113 Resp: 46655
Ion Ratio Lower Upper
113 100
111 105.3 83.1 124.7
192 17.3 13.3 19.9


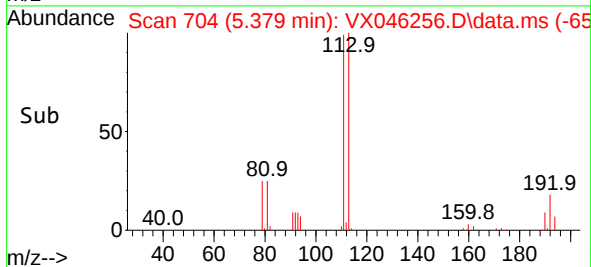
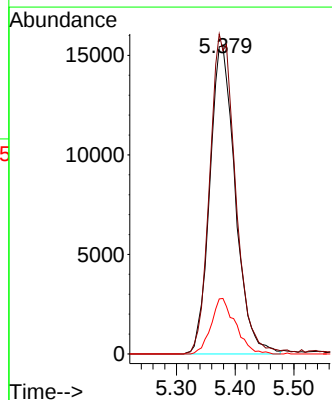
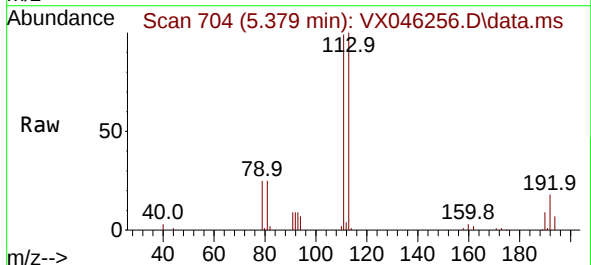


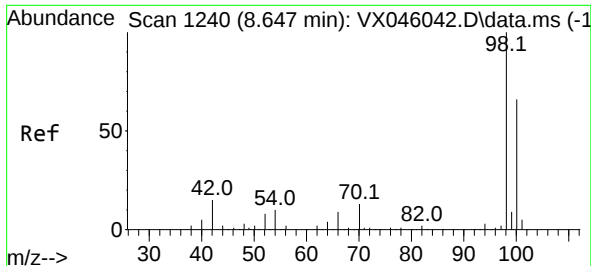

#50
Toluene-d8
Concen: 50.477 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX046256.D
Acq: 19 May 2025 10:39




Instrument :
MSVOA_X
ClientSampleId :
VX0519MBL01


Tgt Ion: 98 Resp: 158856
Ion Ratio Lower Upper
98 100
100 65.4 53.5 80.3

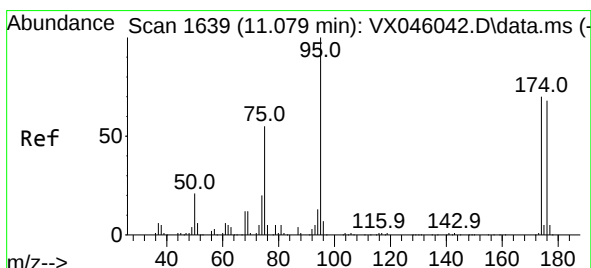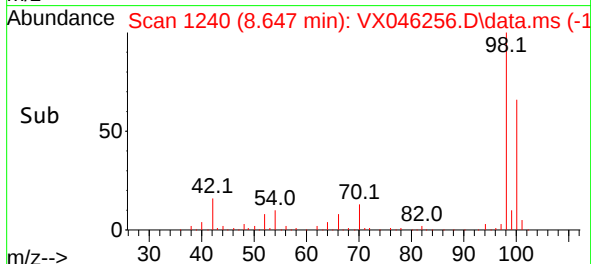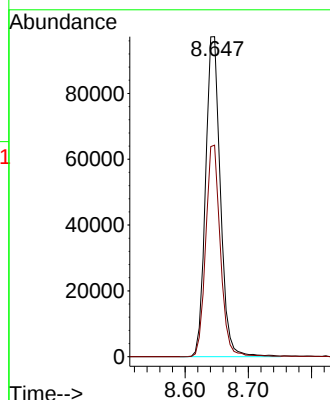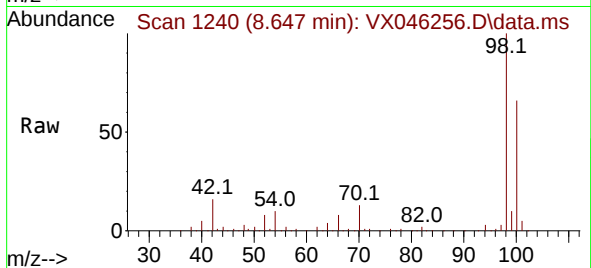

#62
4-Bromofluorobenzene
Concen: 50.934 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX046256.D
Acq: 19 May 2025 10:39

Tgt Ion: 95 Resp: 61486
Ion Ratio Lower Upper
95 100
174 67.8 0.0 135.8
176 64.7 0.0 131.4


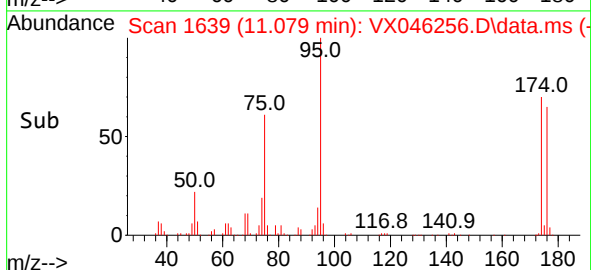
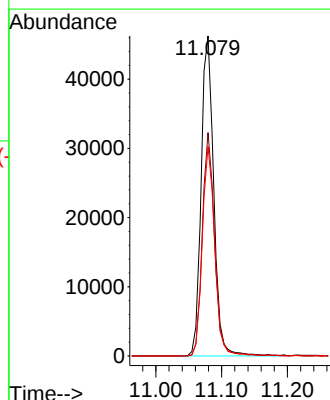
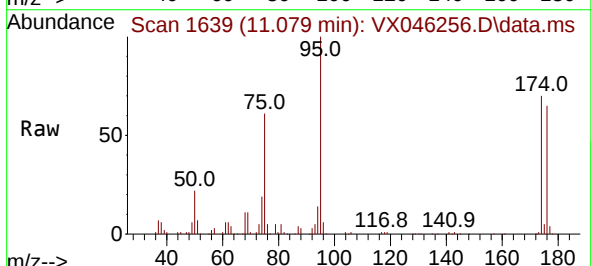


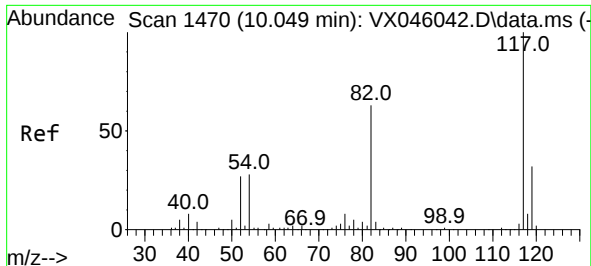

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VX046256.D
Acq: 19 May 2025 10:39

Instrument :
MSVOA_X
ClientSampleId :
VX0519MBL01

Tgt Ion:117 Resp: 121867
Ion Ratio Lower Upper
117 100
82 60.0 50.6 76.0
119 31.3 25.8 38.6

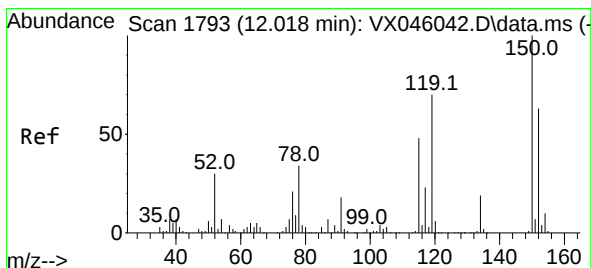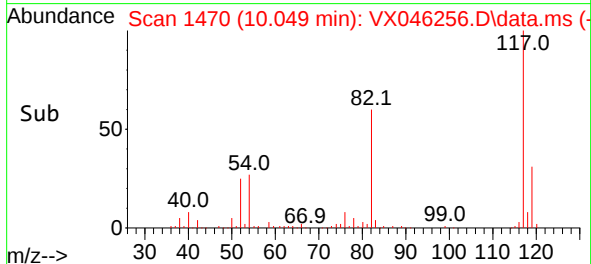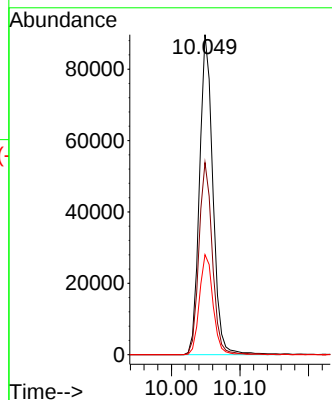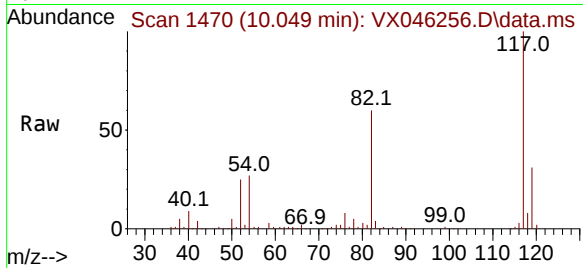

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX046256.D
Acq: 19 May 2025 10:39

Tgt Ion:152 Resp: 52500
Ion Ratio Lower Upper
152 100
115 66.1 46.9 140.7
150 154.0 0.0 351.0

