

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX052019\
 Data File : VX009725.D
 Acq On : 20 May 2019 14:52
 Operator : JC/SP
 Sample : K2952-06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB202-GW-698-700

Quant Time: May 21 08:19:06 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 09 07:31:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	176590	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	280910	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	248059	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	103850	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	116816	48.46	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.92%	
35) Dibromofluoromethane	5.50	113	85820	48.60	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.20%	
50) Toluene-d8	8.71	98	354674	49.75	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.50%	
62) 4-Bromofluorobenzene	11.13	95	117312	45.28	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.56%	
Target Compounds						
16) Acetone	2.44	43	13116	10.133	ug/l	93
52) Toluene	8.79	92	6890	1.403	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX052019\
Data File : VX009725.D
Acq On : 20 May 2019 14:52
Operator : JC/SP
Sample : K2952-06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB202-GW-698-700

Quant Time: May 21 08:19:06 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
Quant Title : SW846 8260
QLast Update : Thu May 09 07:31:15 2019
Response via : Initial Calibration

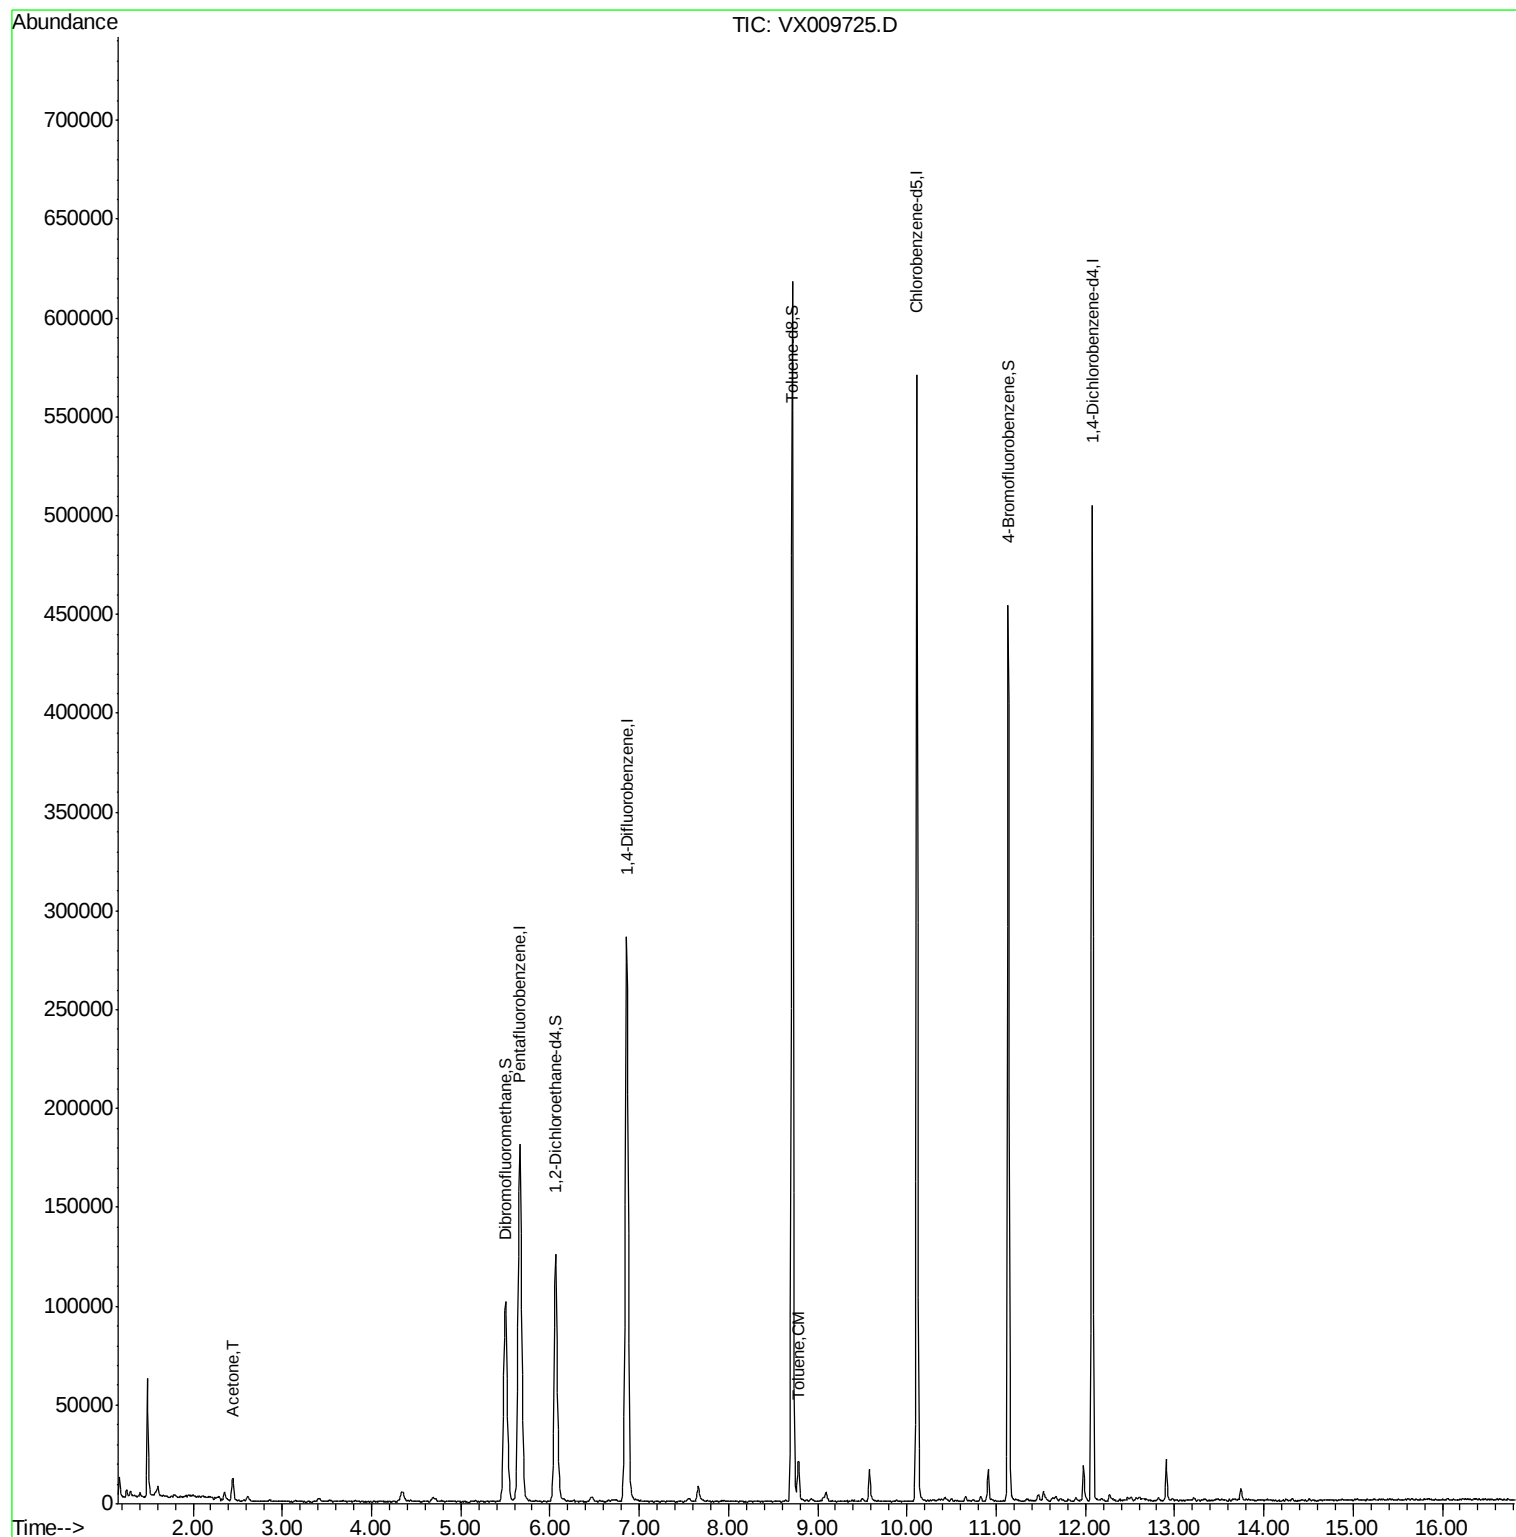

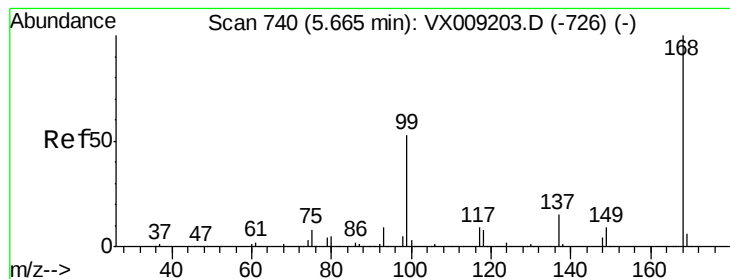

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.00 min

Lab File: VX009725.D

Acq: 20 May 2019 14:52

Instrument :

MSVOA_X

ClientSampleId :


BP-VPB202-GW-698-700

Tot Ion:168 Resp: 176590

Ion Ratio Lower Upper




168 100

99 53.2 42.3 63.5

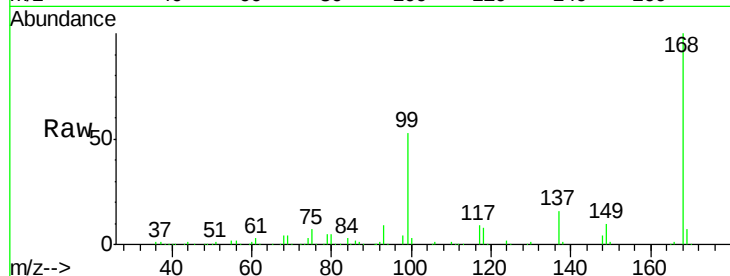

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

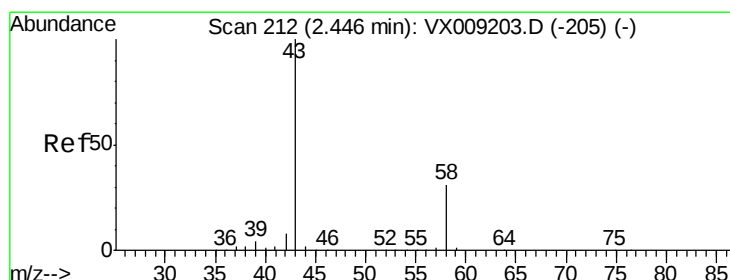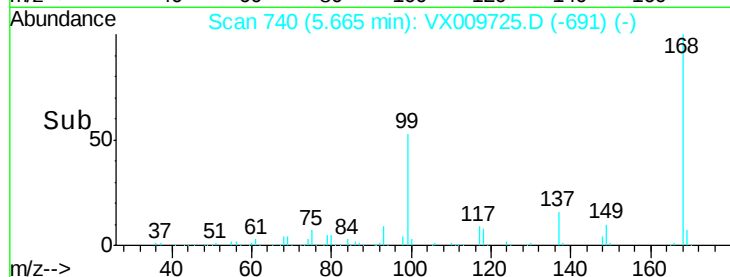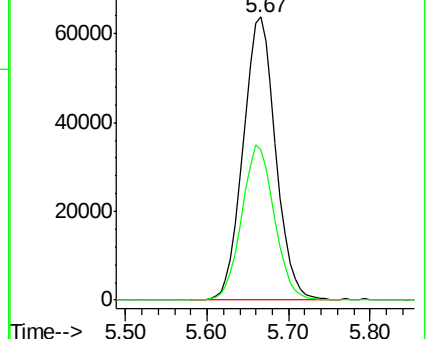

#16

Acetone

Concen: 10.133 ug/l

RT: 2.44 min Scan# 211

Delta R.T. -0.01 min

Lab File: VX009725.D


Acq: 20 May 2019 14:52

Tgt Ion: 43 Resp: 13116

Ion Ratio Lower Upper



43 100

58 27.5 24.9 37.3

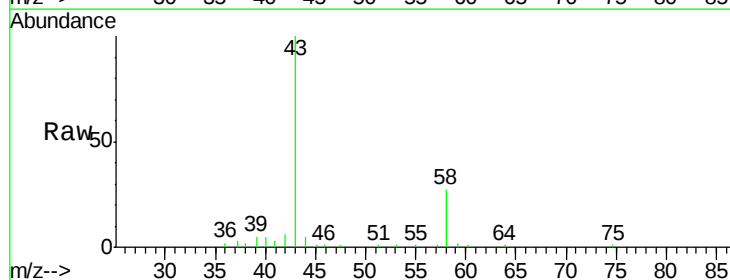

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

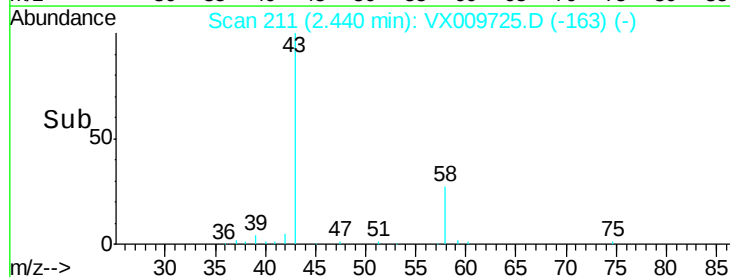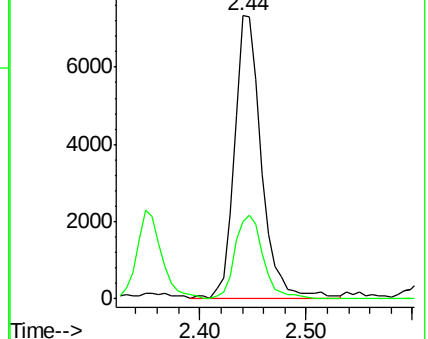



#33

1,2-Dichloroethane-d4

Concen: 48.458 ug/l

RT: 6.06 min Scan# 805

Delta R.T. 0.00 min

Lab File: VX009725.D

Acq: 20 May 2019 14:52

Instrument :

MSVOA_X

ClientSampleId :


BP-VPB202-GW-698-700

Tot Ion: 65 Resp: 116816

Ion Ratio Lower Upper




65 100

67 53.6 0.0 106.6

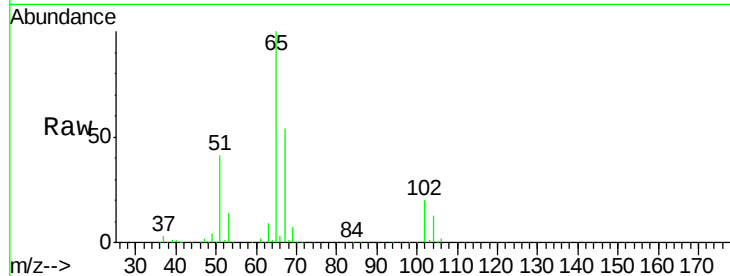

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

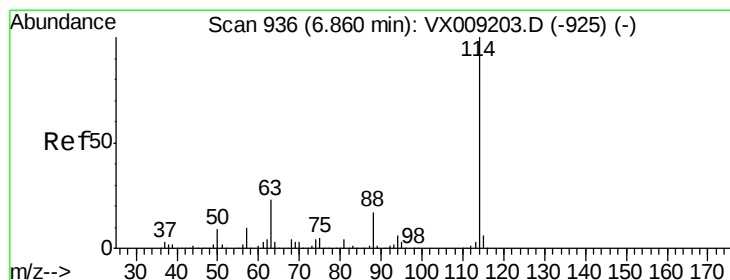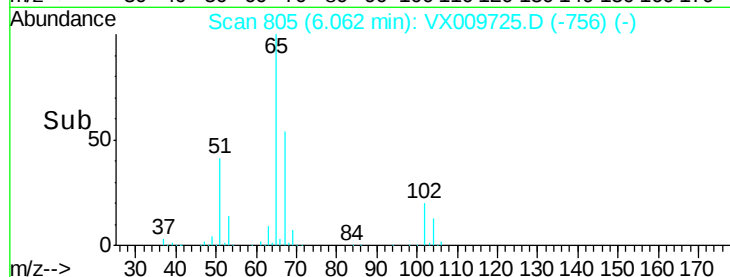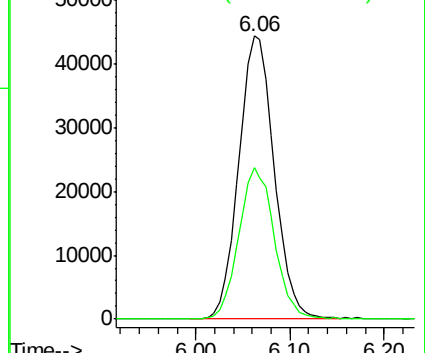

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. 0.00 min

Lab File: VX009725.D

Acq: 20 May 2019 14:52


Tgt Ion: 114 Resp: 280910

Ion Ratio Lower Upper

114 100

63 23.0 0.0 45.6



88 16.7 0.0 33.2

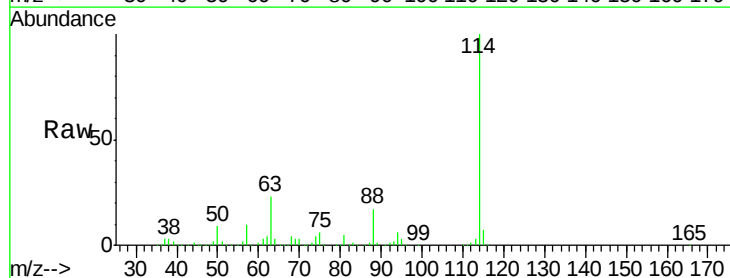


Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0



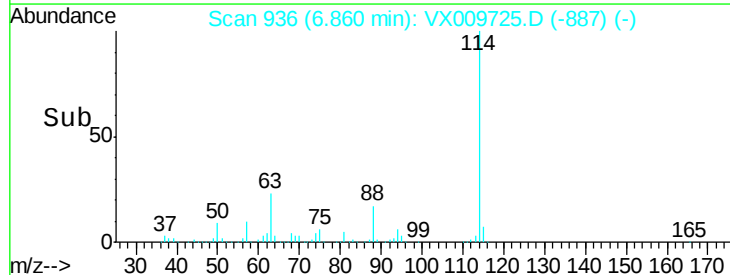
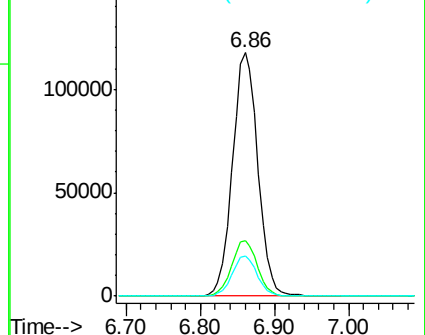


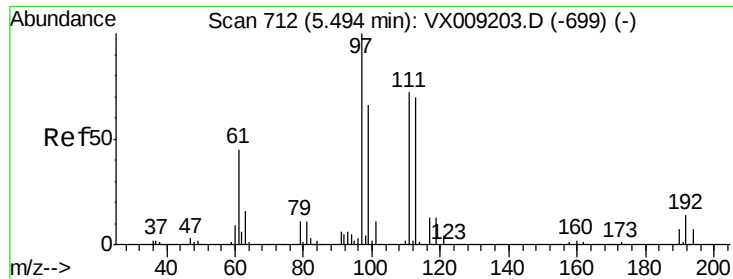

#35
 Dibromofluoromethane
 Concen: 48.598 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. 0.01 min
 Lab File: VX009725.D
 Acq: 20 May 2019 14:52




Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB202-GW-698-700


Tot Ion:113 Resp: 85820
 Ion Ratio Lower Upper
 113 100
 111 103.5 82.8 124.2
 192 22.3 17.0 25.6

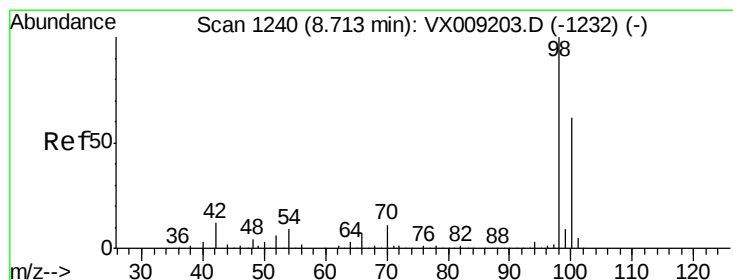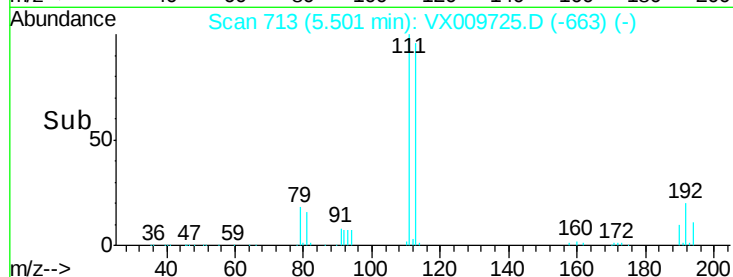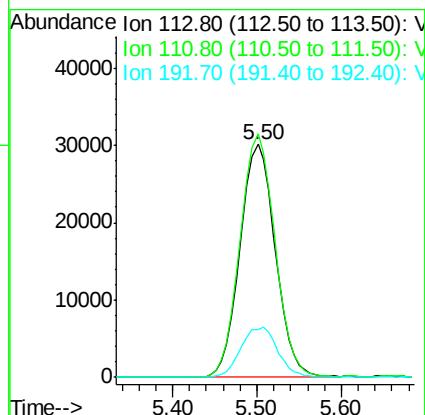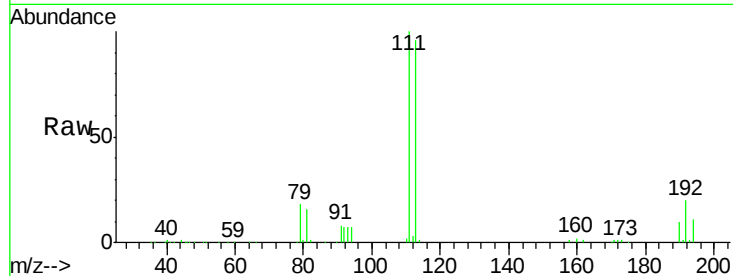

#50
 Toluene-d8
 Concen: 49.748 ug/l
 RT: 8.71 min Scan# 1240
 Delta R.T. 0.00 min
 Lab File: VX009725.D
 Acq: 20 May 2019 14:52

Tgt Ion: 98 Resp: 354674
 Ion Ratio Lower Upper
 98 100
 100 63.9 51.2 76.8

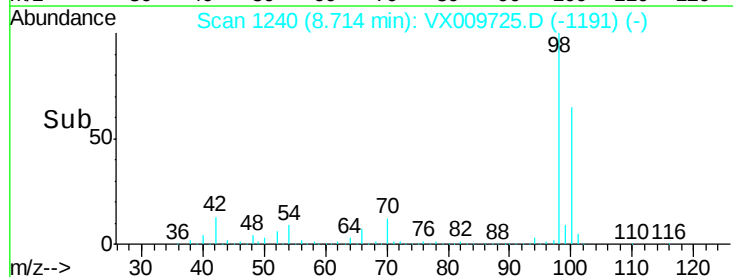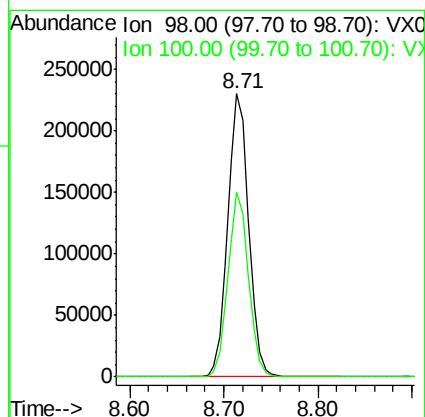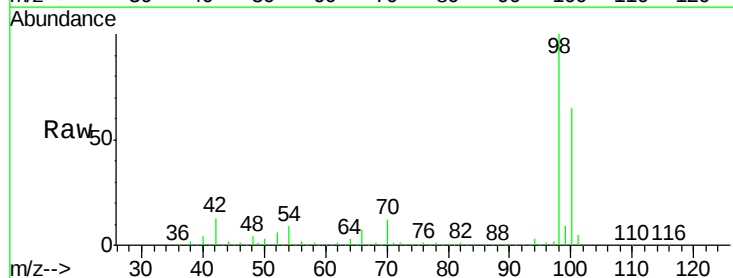

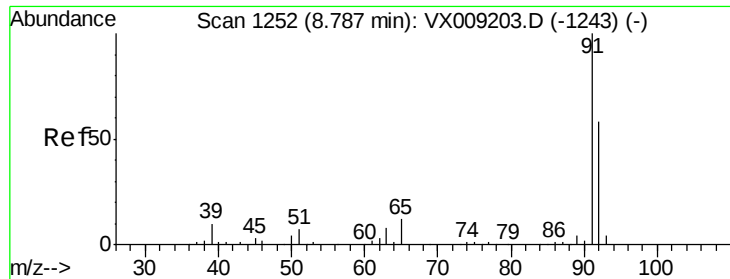

#52

Toluene

Concen: 1.403 ug/l

RT: 8.79 min Scan# 1252

Delta R.T. 0.00 min

Lab File: VX009725.D

Acq: 20 May 2019 14:52

Instrument :

MSVOA_X

ClientSampleId :


BP-VPB202-GW-698-700

Tot Ion: 92 Resp: 6890

Ion Ratio Lower Upper




92 100

91 179.6 138.8 208.2

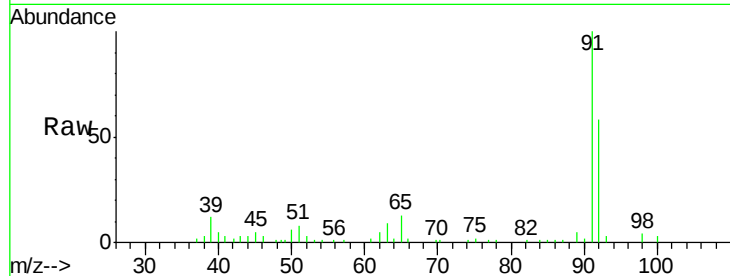

Abundance Ion 92.00 (91.70 to 92.70): VX0

Ion 91.00 (90.70 to 91.70): VX0

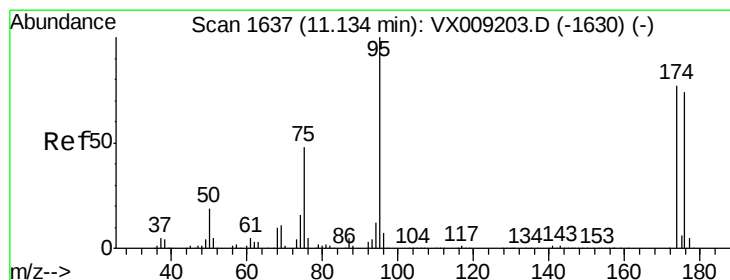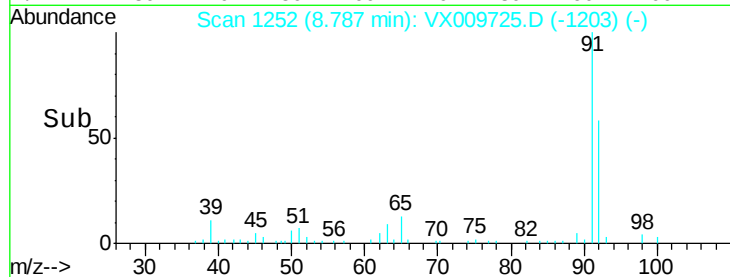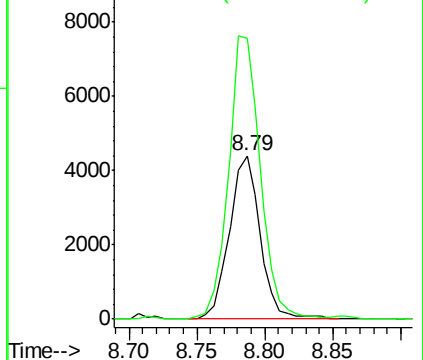

#62

4-Bromofluorobenzene

Concen: 45.284 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.00 min

Lab File: VX009725.D

Acq: 20 May 2019 14:52


Tgt Ion: 95 Resp: 117312

Ion Ratio Lower Upper

95 100

174 81.6 0.0 161.6



176 79.8 0.0 159.2

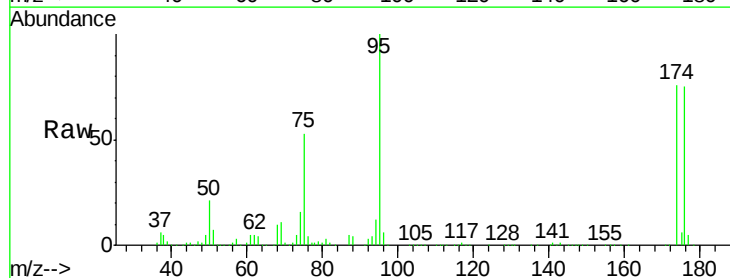


Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V



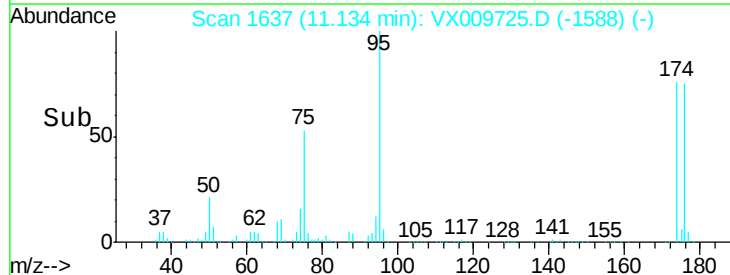
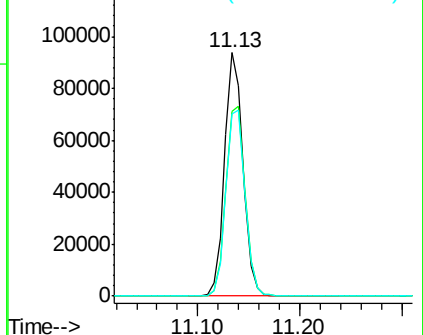


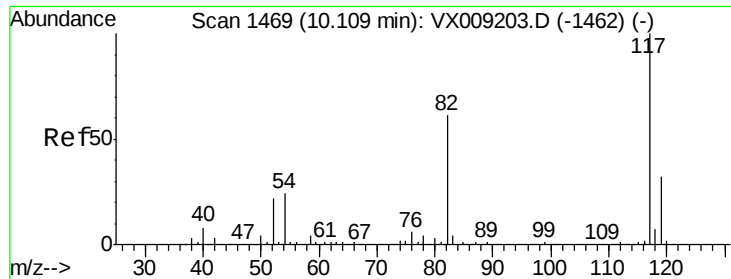

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. 0.00 min
Lab File: VX009725.D
Acq: 20 May 2019 14:52

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB202-GW-698-700

Tot Ion:117 Resp: 248059
Ion Ratio Lower Upper
117 100
82 58.9 48.8 73.2
119 31.9 25.8 38.6

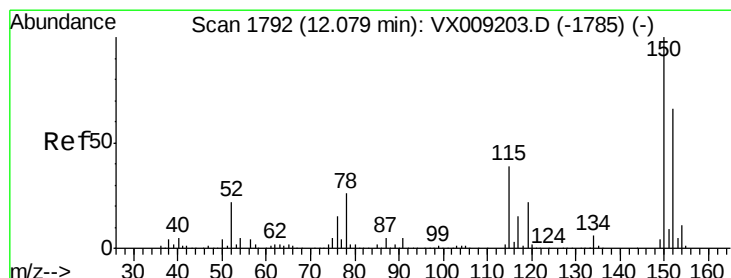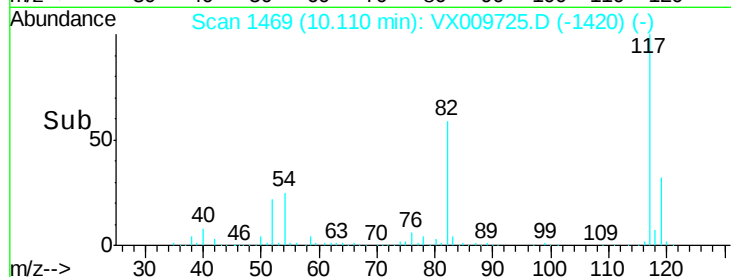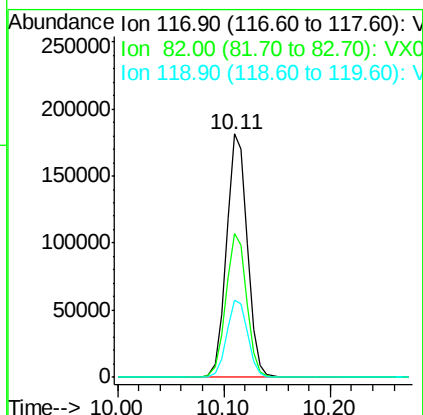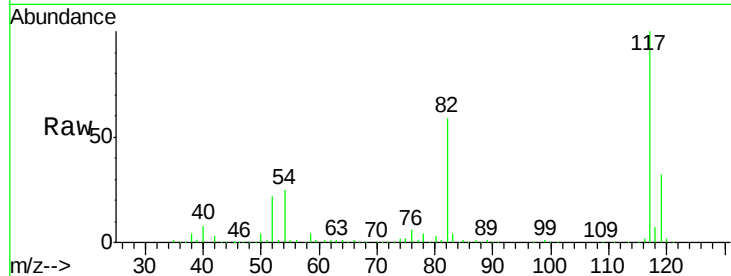

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. 0.00 min
Lab File: VX009725.D
Acq: 20 May 2019 14:52

Tgt Ion:152 Resp: 103850
Ion Ratio Lower Upper
152 100
115 59.0 41.2 123.6
150 157.8 0.0 346.4

