

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX052019\
 Data File : VX009728.D
 Acq On : 20 May 2019 16:03
 Operator : JC/SP
 Sample : K2952-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB202-TB-20190516

Quant Time: May 21 08:24:21 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 09 07:31:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	169584	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	272169	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	239173	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	97260	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.06	65	115464	49.88	ug/l	0.00
Spiked Amount			Recovery	=	99.76%	
35) Dibromofluoromethane	5.50	113	83332	48.70	ug/l	0.00
Spiked Amount			Recovery	=	97.40%	
50) Toluene-d8	8.71	98	344996	49.94	ug/l	0.00
Spiked Amount			Recovery	=	99.88%	
62) 4-Bromofluorobenzene	11.13	95	111915	44.59	ug/l	0.00
Spiked Amount			Recovery	=	89.18%	


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX052019\
Data File : VX009728.D
Acq On : 20 May 2019 16:03
Operator : JC/SP
Sample : K2952-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB202-TB-20190516

Quant Time: May 21 08:24:21 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
Quant Title : SW846 8260
QLast Update : Thu May 09 07:31:15 2019
Response via : Initial Calibration

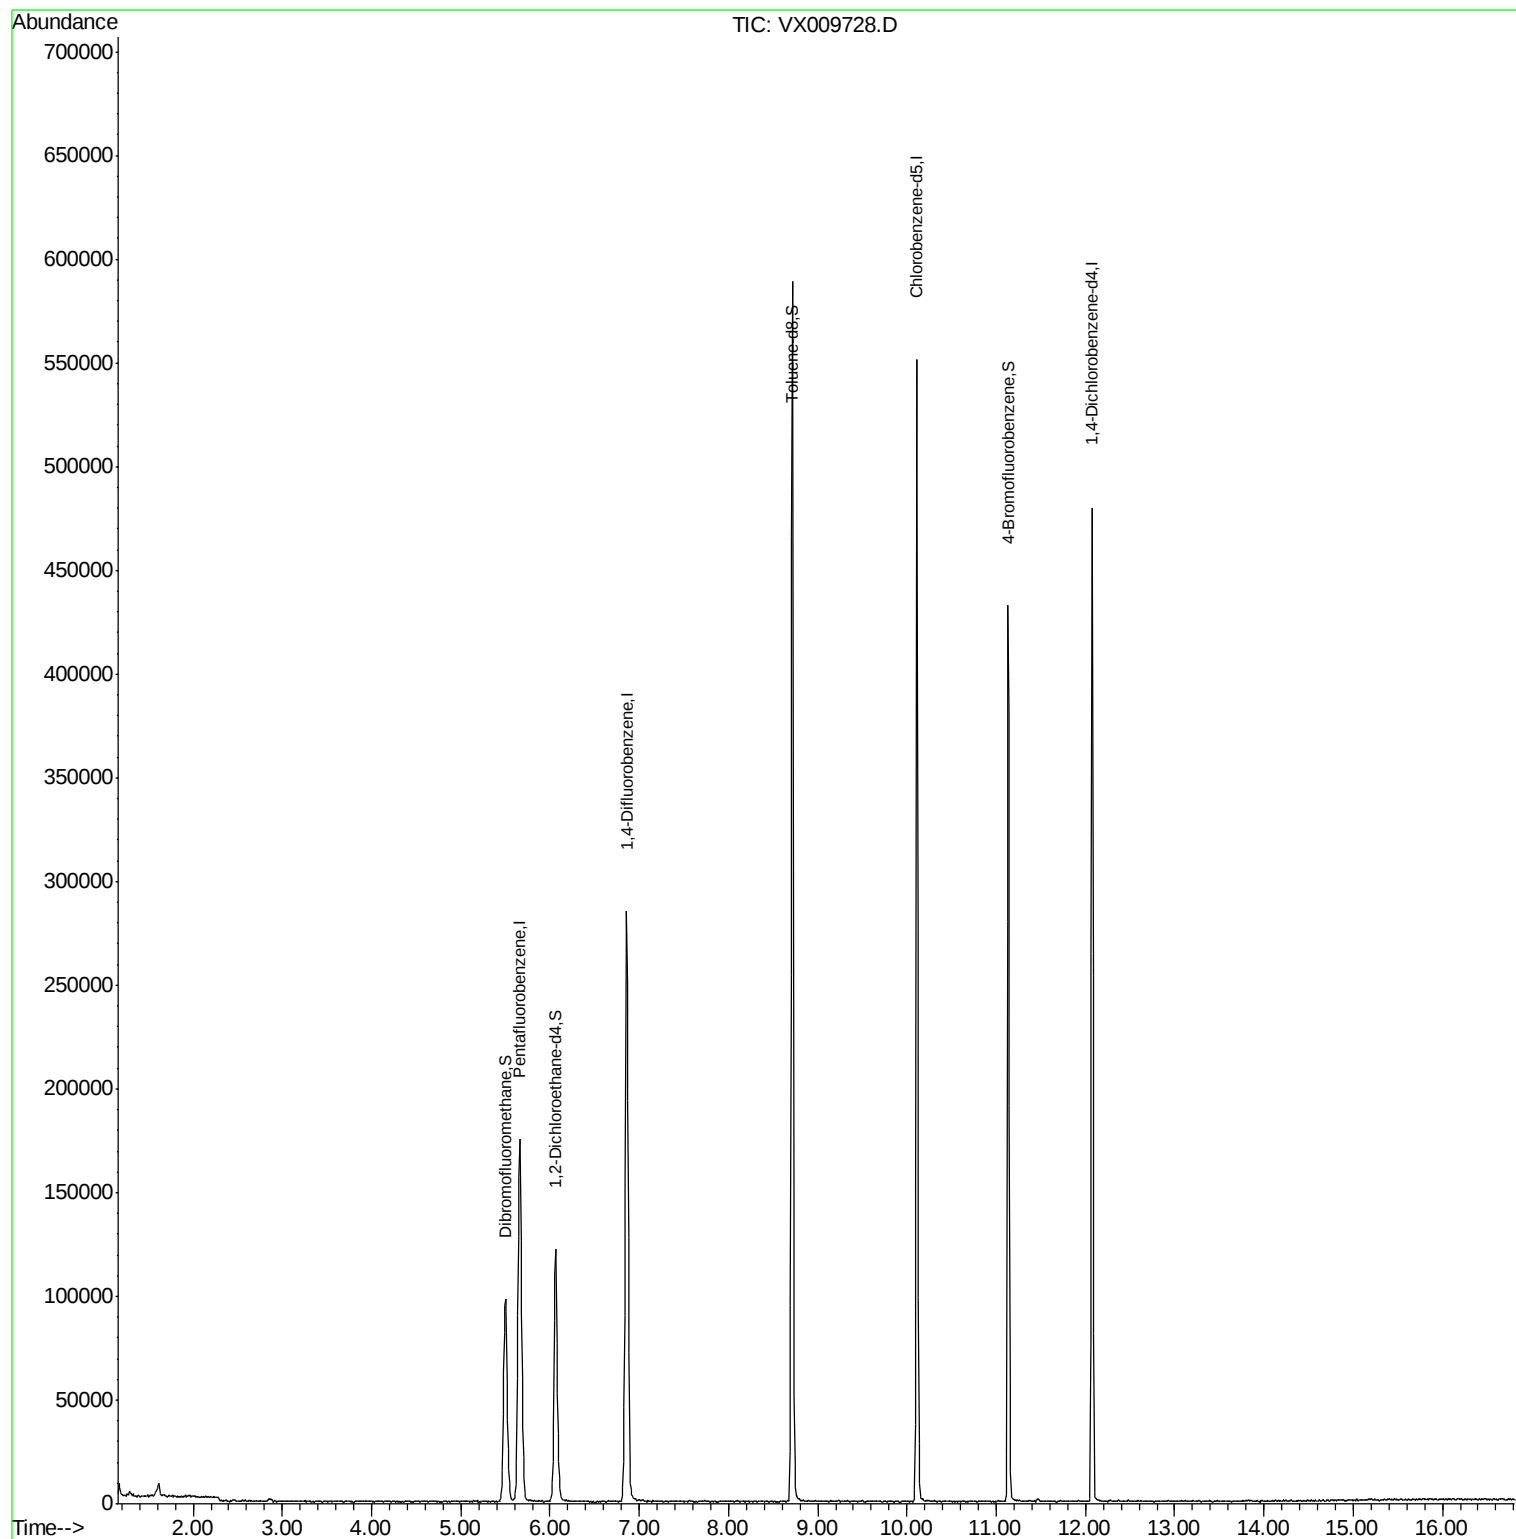



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.01 min

Lab File: VX009728.D

Acq: 20 May 2019 16:03

Instrument :

MSVOA_X

ClientSampleId :


BP-VPB202-TB-20190516

Tot Ion:168 Resp: 169584

Ion Ratio Lower Upper

168 100

99 57.1 42.3 63.5

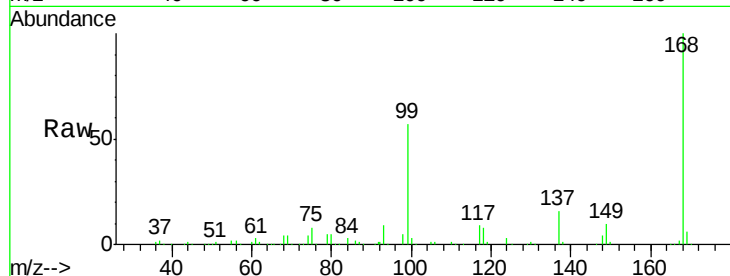

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.66



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

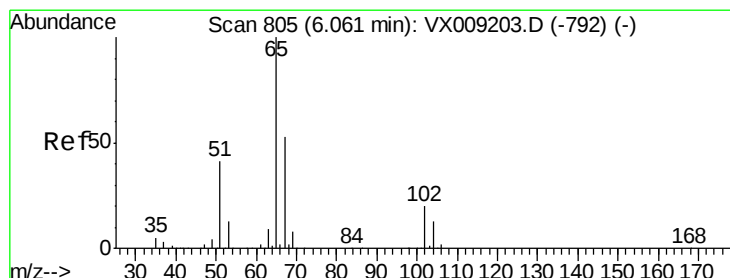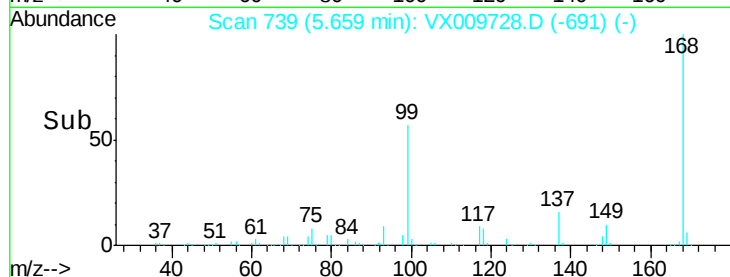

#33

1,2-Dichloroethane-d4

Concen: 49.876 ug/l

RT: 6.06 min Scan# 805

Delta R.T. 0.00 min

Lab File: VX009728.D


Acq: 20 May 2019 16:03

Tgt Ion: 65 Resp: 115464

Ion Ratio Lower Upper

65 100

67 53.0 0.0 106.6

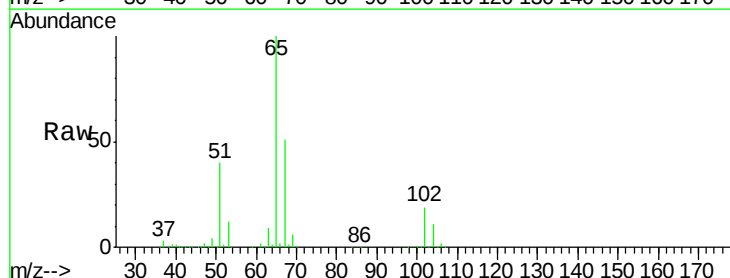

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.06

50000

40000


30000


20000

10000

0

Time--> 5.90 6.00 6.10 6.20




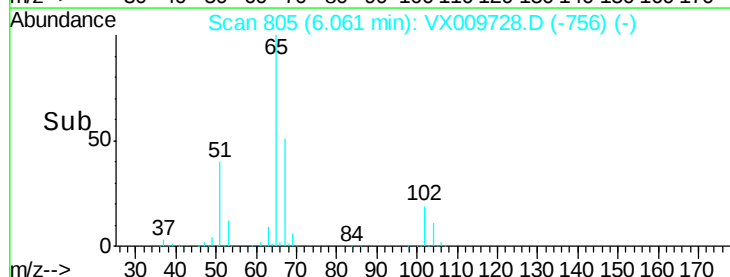


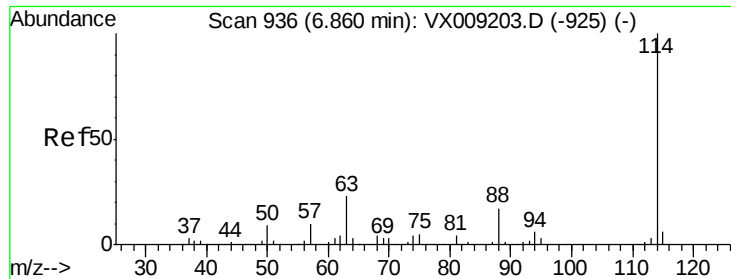

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. 0.00 min
 Lab File: VX009728.D
 Acq: 20 May 2019 16:03




Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB202-TB-20190516


Tot Ion:114	Resp:	272169
Ion Ratio	Lower	Upper
114 100		
63 22.7	0.0	45.6
88 16.5	0.0	33.2

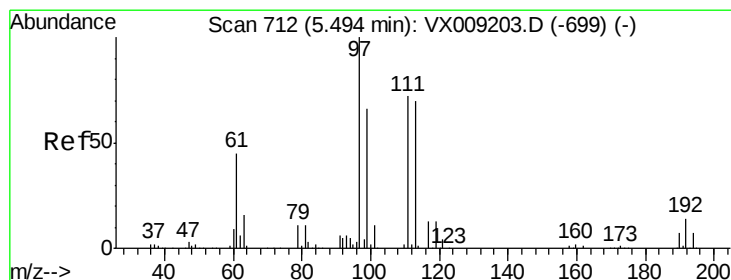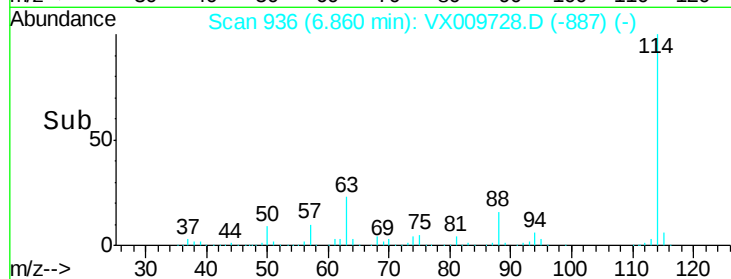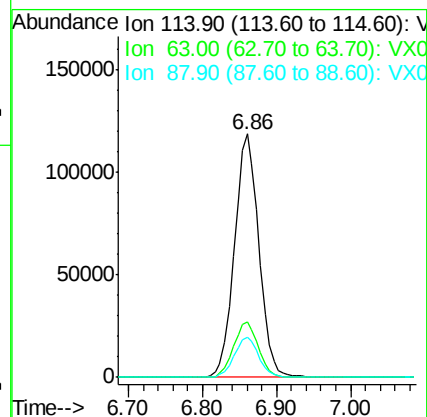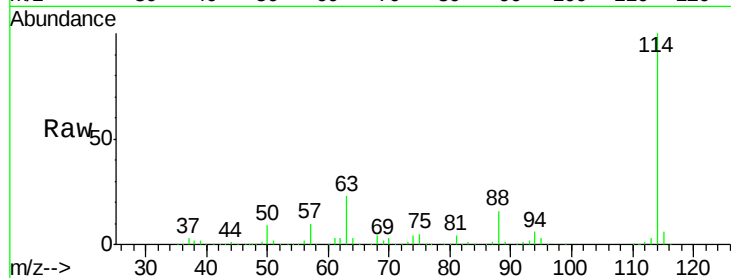

#35
 Dibromofluoromethane
 Concen: 48.705 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. 0.01 min
 Lab File: VX009728.D
 Acq: 20 May 2019 16:03

Tgt Ion:113	Resp:	83332
Ion Ratio	Lower	Upper
113 100		
111 102.2	82.8	124.2
192 21.4	17.0	25.6

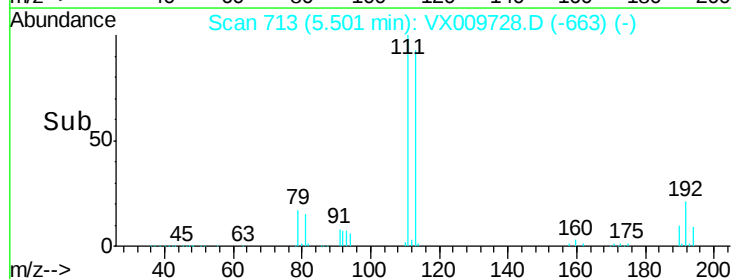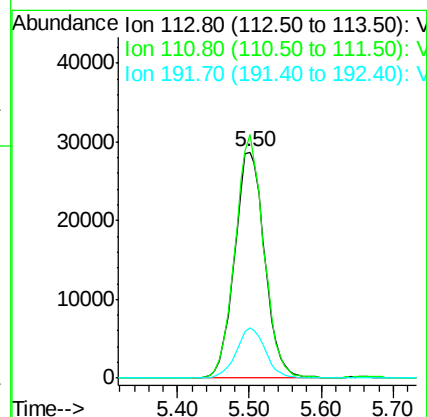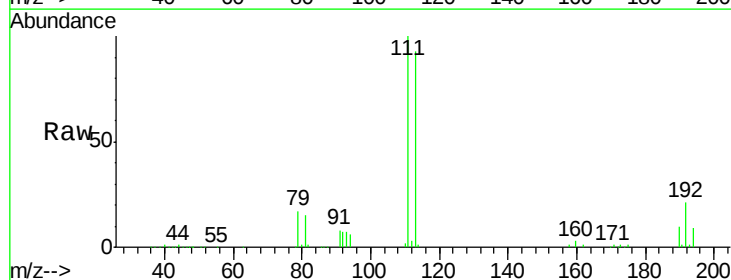

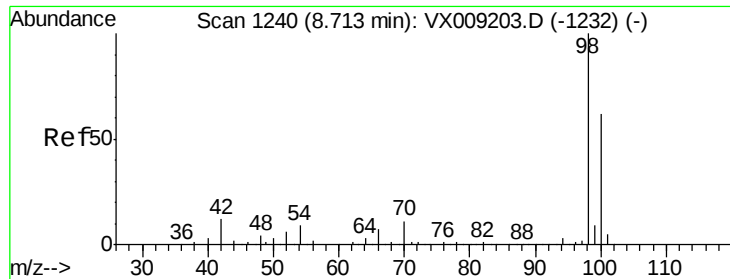

#50

Toluene-d8

Concen: 49.945 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX009728.D

Acq: 20 May 2019 16:03

Instrument :

MSVOA_X

ClientSampleId :


BP-VPB202-TB-20190516

Tot Ion: 98 Resp: 344996

Ion Ratio Lower Upper

98 100

100 63.8 51.2 76.8

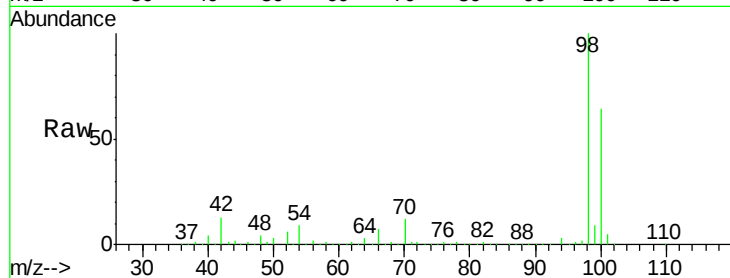

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

8.71

250000

200000



150000

100000

50000

0

Time--> 8.60 8.70 8.80

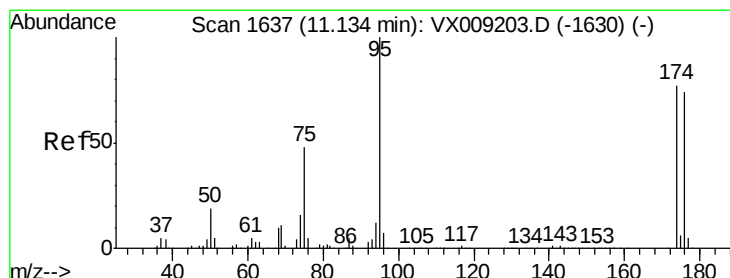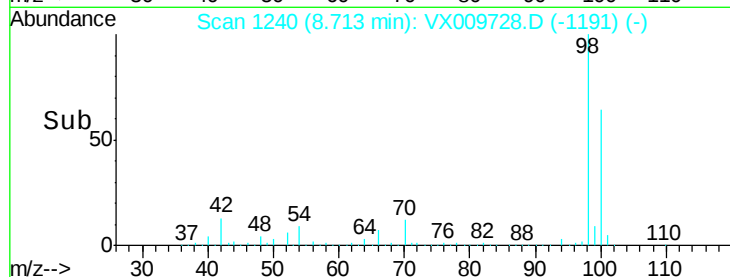

#62

4-Bromofluorobenzene

Concen: 44.588 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.00 min

Lab File: VX009728.D

Acq: 20 May 2019 16:03


Tgt Ion: 95 Resp: 111915

Ion Ratio Lower Upper

95 100

174 80.3 0.0 161.6

176 78.9 0.0 159.2

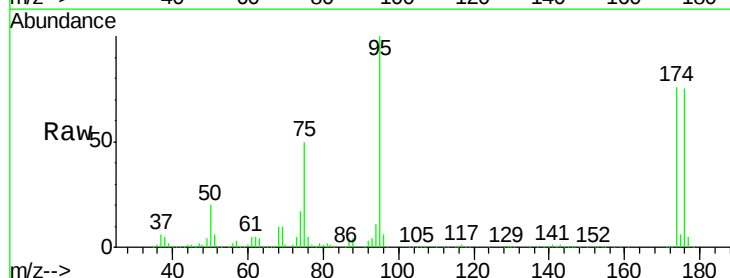

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

120000

100000

80000


60000


40000

20000

0

Time--> 11.10 11.20

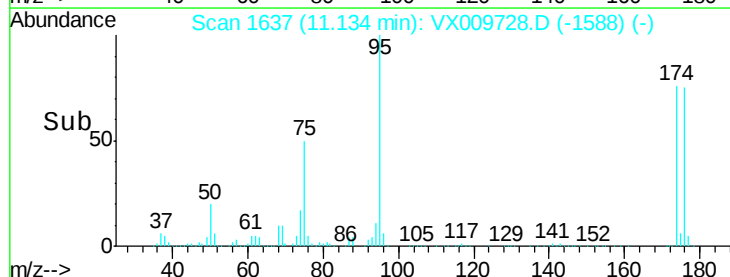


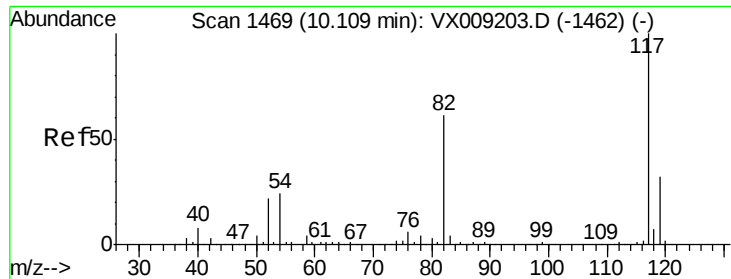




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. 0.00 min
Lab File: VX009728.D
Acq: 20 May 2019 16:03

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB202-TB-20190516

Tot Ion:117 Resp: 239173
Ion Ratio Lower Upper
117 100
82 60.5 48.8 73.2
119 31.5 25.8 38.6

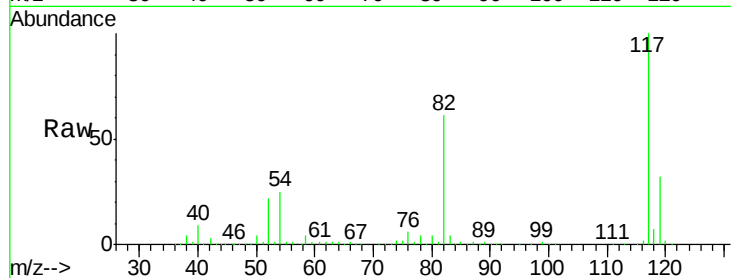


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

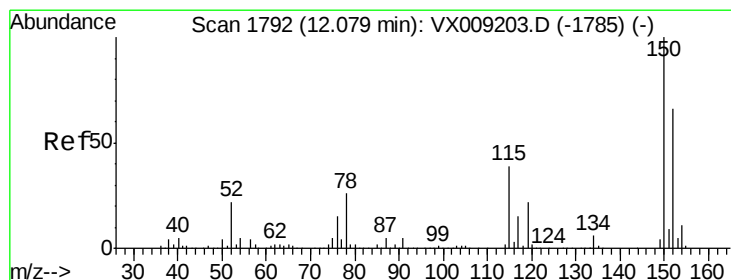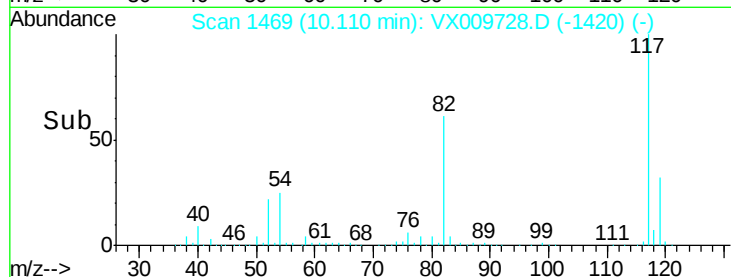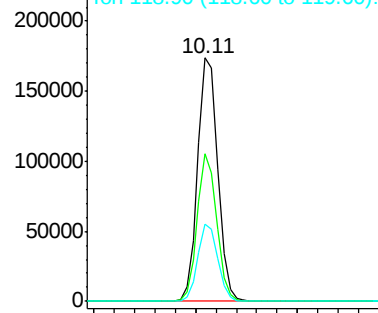

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. 0.00 min
Lab File: VX009728.D
Acq: 20 May 2019 16:03

Tgt Ion:152 Resp: 97260
Ion Ratio Lower Upper
152 100
115 58.8 41.2 123.6
150 156.6 0.0 346.4

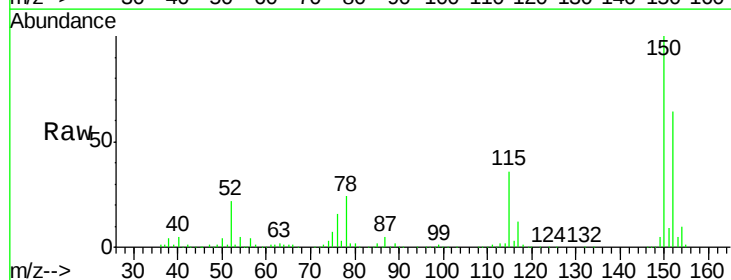

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

