

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052022\
 Data File : VX028882.D
 Acq On : 21 May 2022 04:34
 Operator : JC/MD
 Sample : N2970-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP01-20220519

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Title : SW846 8260

Signal : TIC: VX028882.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	26	31	44	rBV	29492	104761	6.03%	0.517%
2	2.782	270	278	283	rBV2	22838	50690	2.92%	0.250%
3	3.105	322	331	341	rBV2	44209	99081	5.71%	0.489%
4	4.495	542	559	570	rBV3	15885	50935	2.93%	0.251%
5	5.391	695	706	718	rBV	201952	589024	33.93%	2.906%
6	5.556	722	733	742	rBV	336214	960393	55.33%	4.738%
7	5.848	769	781	789	rBV6	23162	73617	4.24%	0.363%
8	5.958	789	799	822	rVV	222656	601010	34.62%	2.965%
9	6.165	824	833	842	rVV3	21535	82925	4.78%	0.409%
10	6.257	842	848	857	rVV4	23715	71205	4.10%	0.351%
11	6.763	920	931	945	rBV	542170	1282966	73.91%	6.330%
12	7.129	981	991	1004	rVB2	43245	94480	5.44%	0.466%
13	7.373	1020	1031	1042	rBV3	50231	124823	7.19%	0.616%
14	7.775	1089	1097	1105	rVB2	42132	86046	4.96%	0.425%
15	7.958	1117	1127	1140	rVB3	47290	104587	6.02%	0.516%
16	8.324	1180	1187	1193	rBV2	27458	52671	3.03%	0.260%
17	8.604	1226	1233	1235	rBV2	25340	42010	2.42%	0.207%
18	8.653	1235	1241	1254	rVB	1112321	1735892	100.00%	8.564%
19	8.775	1254	1261	1266	rBV	78597	131396	7.57%	0.648%
20	8.976	1289	1294	1302	rVB	150381	245044	14.12%	1.209%
21	9.104	1306	1315	1321	rBV	57863	95246	5.49%	0.470%
22	9.512	1374	1382	1387	rBV2	40798	70637	4.07%	0.348%
23	9.622	1394	1400	1404	rBV	78650	123572	7.12%	0.610%
24	9.836	1428	1435	1448	rVB	24771	44808	2.58%	0.221%
25	10.055	1465	1471	1478	rBV	1118285	1475198	84.98%	7.278%
26	10.128	1478	1483	1488	rVV	33421	51840	2.99%	0.256%
27	10.281	1503	1508	1517	rVV4	44014	114634	6.60%	0.566%
28	10.457	1532	1537	1542	rBV	29086	41728	2.40%	0.206%
29	10.598	1547	1560	1566	rBV4	50880	135628	7.81%	0.669%
30	10.756	1578	1586	1588	rBV2	27064	53221	3.07%	0.263%
31	10.781	1588	1590	1595	rVB	36665	39446	2.27%	0.195%
32	10.860	1597	1603	1610	rBV4	32172	58850	3.39%	0.290%
33	11.085	1634	1640	1644	rBV	861137	1132090	65.22%	5.585%
34	11.128	1644	1647	1651	rVB2	36783	47865	2.76%	0.236%
35	11.226	1659	1663	1667	rVB3	45984	62538	3.60%	0.309%
36	11.622	1722	1728	1734	rVB3	35014	57206	3.30%	0.282%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052022\
 Data File : VX028882.D
 Acq On : 21 May 2022 04:34
 Operator : JC/MD
 Sample : N2970-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP01-20220519

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Title : SW846 8260

37	11.713	1739	1743	1747	rBV2	40214	49159	2.83%	0.243%
38	11.866	1760	1768	1770	rBV	125907	178042	10.26%	0.878%
39	11.890	1770	1772	1778	rVB	140376	162375	9.35%	0.801%
40	12.024	1789	1794	1799	rBV	1114749	1378597	79.42%	6.801%
41	12.177	1815	1819	1825	rVB	42939	55063	3.17%	0.272%
42	12.250	1825	1831	1834	rBV	59019	75400	4.34%	0.372%
43	12.311	1834	1841	1852	rVB4	100642	186958	10.77%	0.922%
44	12.408	1852	1857	1862	rBV	110392	144773	8.34%	0.714%
45	12.603	1880	1889	1892	rBV3	47783	80994	4.67%	0.400%
46	12.646	1892	1896	1902	rVB2	102831	167727	9.66%	0.827%
47	12.725	1902	1909	1912	rBV3	72058	130846	7.54%	0.646%
48	12.762	1912	1915	1920	rVB	60948	72069	4.15%	0.356%
49	12.841	1920	1928	1933	rVB2	249326	398419	22.95%	1.966%
50	12.902	1933	1938	1940	rBV	156596	214790	12.37%	1.060%
51	12.926	1940	1942	1947	rVB2	86942	109167	6.29%	0.539%
52	13.030	1954	1959	1965	rVB2	83547	120963	6.97%	0.597%
53	13.140	1966	1977	1982	rBV2	222877	335174	19.31%	1.654%
54	13.195	1982	1986	1991	rVB	93851	104903	6.04%	0.518%
55	13.250	1991	1995	1998	rBV	55093	72944	4.20%	0.360%
56	13.292	1998	2002	2007	rVB2	76765	106533	6.14%	0.526%
57	13.347	2007	2011	2015	rBV3	53104	62332	3.59%	0.308%
58	13.396	2015	2019	2030	rVB4	81306	153131	8.82%	0.755%
59	13.518	2034	2039	2045	rBV4	57843	123671	7.12%	0.610%
60	13.585	2045	2050	2053	rBV3	166719	243422	14.02%	1.201%
61	13.621	2053	2056	2057	rVV	167502	206201	11.88%	1.017%
62	13.640	2057	2059	2061	rVV	225884	301821	17.39%	1.489%
63	13.664	2061	2063	2067	rVB	346976	364019	20.97%	1.796%
64	13.749	2073	2077	2081	rBV	232495	286141	16.48%	1.412%
65	13.798	2081	2085	2090	rVB3	63381	104281	6.01%	0.514%
66	13.853	2090	2094	2098	rVB2	103994	137172	7.90%	0.677%
67	13.926	2098	2106	2110	rBV4	182642	355626	20.49%	1.755%
68	13.975	2110	2114	2117	rVV2	112899	158894	9.15%	0.784%
69	14.006	2117	2119	2122	rVB	49180	50144	2.89%	0.247%
70	14.067	2126	2129	2132	rBV3	61550	75157	4.33%	0.371%
71	14.103	2132	2135	2139	rVB	100704	107126	6.17%	0.529%
72	14.182	2142	2148	2150	rBV	60071	91493	5.27%	0.451%
73	14.213	2150	2153	2157	rVB	97646	109764	6.32%	0.542%
74	14.292	2163	2166	2167	rBV2	41947	46706	2.69%	0.230%
75	14.323	2167	2171	2174	rVB	163660	205205	11.82%	1.012%
76	14.371	2174	2179	2184	rVB2	114689	184790	10.65%	0.912%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052022\
 Data File : VX028882.D
 Acq On : 21 May 2022 04:34
 Operator : JC/MD
 Sample : N2970-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP01-20220519

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Title : SW846 8260

77	14.420	2184	2187	2192	rVB2	67519	83138	4.79%	0.410%
78	14.481	2192	2197	2206	rBV2	235690	419415	24.16%	2.069%
79	14.585	2210	2214	2216	rBV3	39708	70448	4.06%	0.348%
80	14.670	2224	2228	2233	rBV2	216183	285213	16.43%	1.407%
81	14.725	2233	2237	2240	rVB	78885	89395	5.15%	0.441%
82	14.792	2243	2248	2252	rBV	194813	292745	16.86%	1.444%
83	14.853	2255	2258	2261	rVB2	29657	31587	1.82%	0.156%
84	14.883	2261	2263	2266	rBV	33614	46749	2.69%	0.231%
85	14.981	2276	2279	2283	rVB3	35495	48443	2.79%	0.239%
86	15.048	2286	2290	2294	rBV3	29315	46771	2.69%	0.231%
87	15.182	2307	2312	2319	rVV3	79025	152759	8.80%	0.754%
88	15.255	2319	2324	2330	rVB4	53970	88310	5.09%	0.436%
89	15.408	2346	2349	2353	rVB2	45273	55862	3.22%	0.276%
90	15.481	2358	2361	2364	rVV3	25541	40076	2.31%	0.198%
91	15.524	2364	2368	2375	rVV6	29048	76722	4.42%	0.379%
92	15.597	2375	2380	2386	rVV	167818	267082	15.39%	1.318%
93	15.652	2386	2389	2395	rVB4	24657	42908	2.47%	0.212%
94	15.731	2395	2402	2408	rBV2	83257	152938	8.81%	0.755%
95	15.810	2410	2415	2418	rVV2	40459	71265	4.11%	0.352%
96	15.847	2418	2421	2428	rVV2	29343	44482	2.56%	0.219%
97	15.987	2439	2444	2450	rBV	24529	36846	2.12%	0.182%
98	16.091	2456	2461	2470	rVB3	21303	41719	2.40%	0.206%
99	16.304	2491	2496	2504	rVV5	23660	52874	3.05%	0.261%
100	16.603	2540	2545	2552	rVB4	13477	31433	1.81%	0.155%


Sum of corrected areas: 20269235

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052022\
Data File : VX028882.D
Acq On : 21 May 2022 04:34
Operator : JC/MD
Sample : N2970-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP01-20220519

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

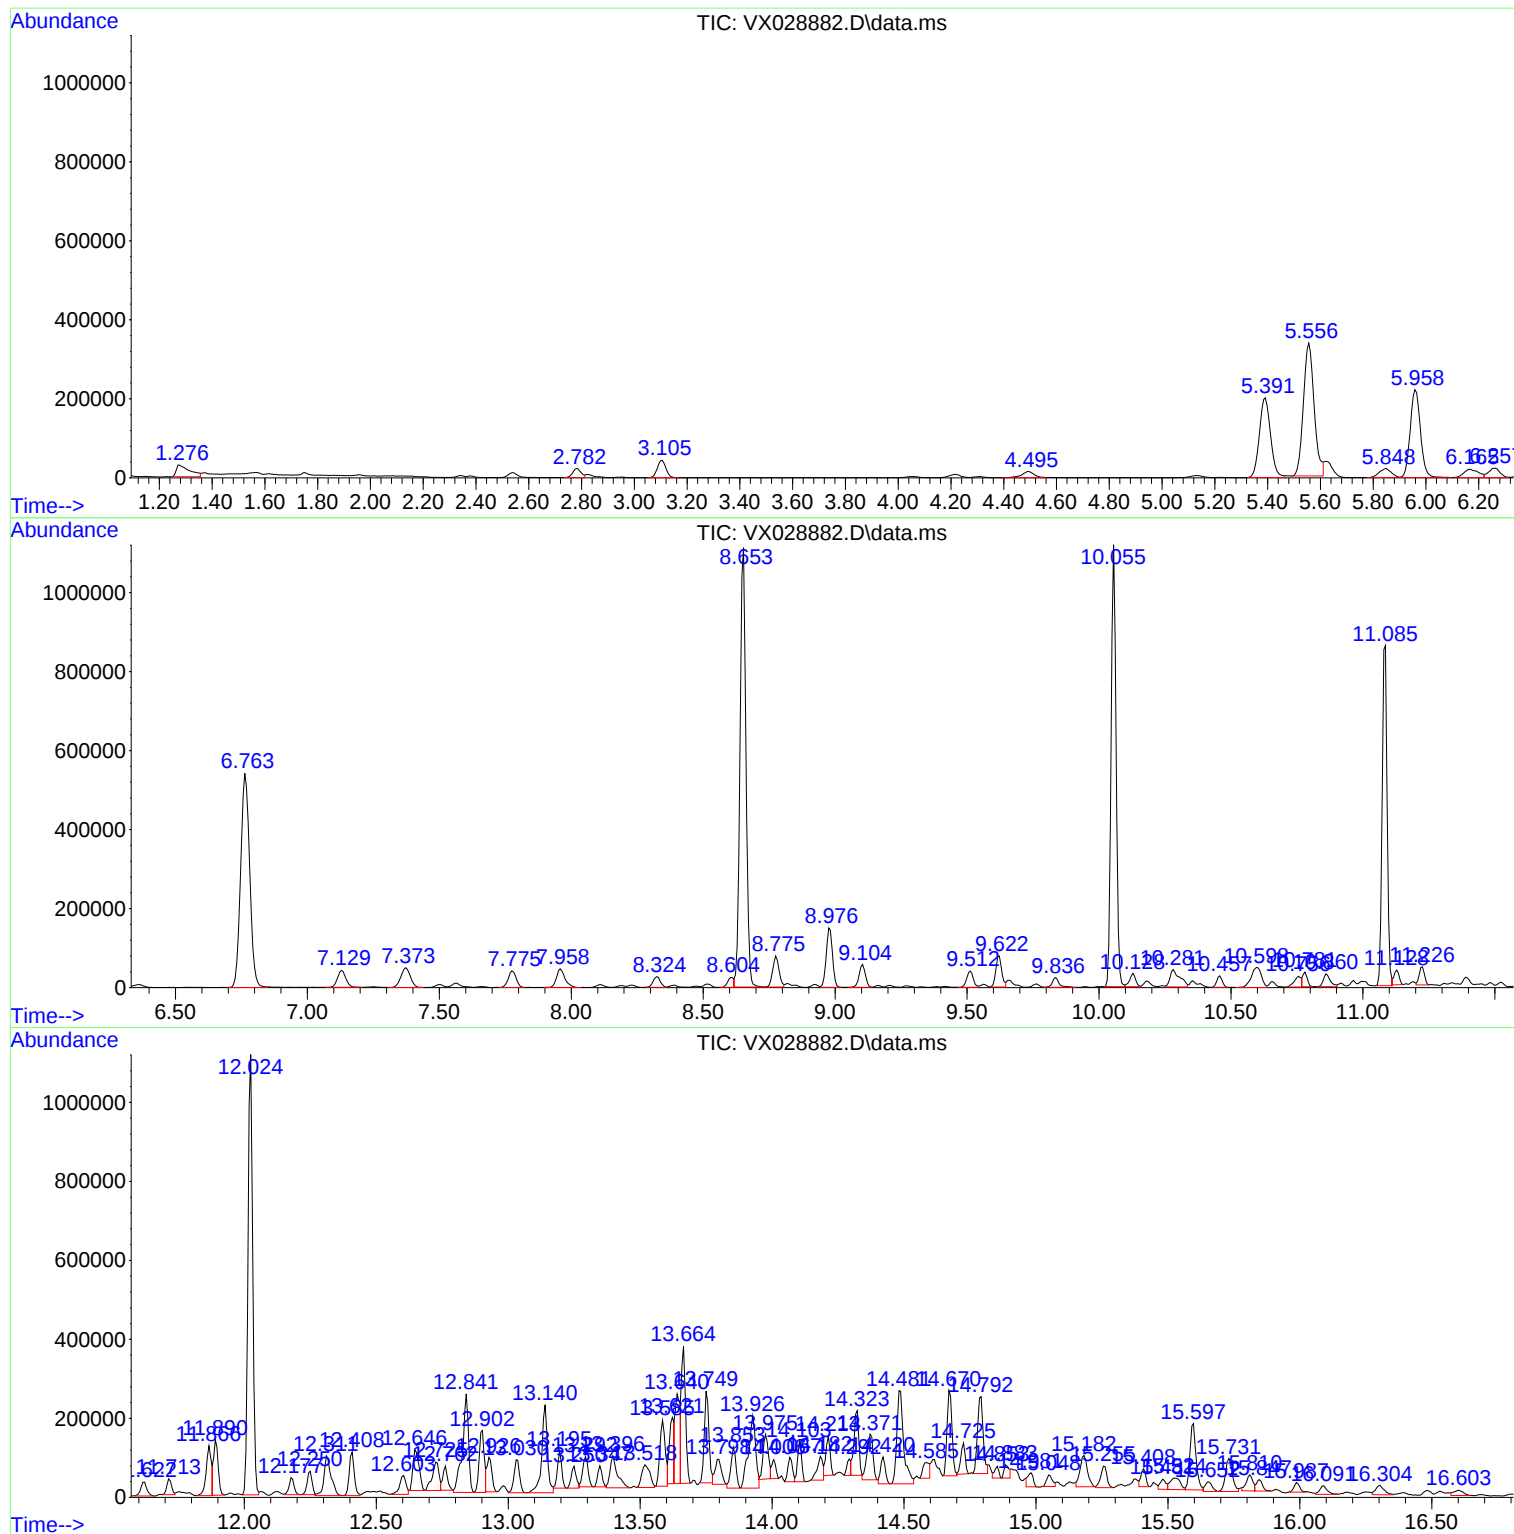

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052022\
Data File : VX028882.D
Acq On : 21 May 2022 04:34
Operator : JC/MD
Sample : N2970-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP01-20220519

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052022\
Data File : VX028882.D
Acq On : 21 May 2022 04:34
Operator : JC/MD
Sample : N2970-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP01-20220519

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------