

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX052120\  
 Data File : VX016396.D  
 Acq On : 21 May 2020 19:58  
 Operator : JC/SP  
 Sample : L2732-05  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 KY038PS034-200520

Integration Parameters: RTEINT.P

Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X050420W.M  
 Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.471       | 707           | 719         | 734          | rBV      | 121026         | 339753        | 29.98%          | 5.595%        |
| 2         | 5.629       | 734           | 745         | 761          | rVB      | 218580         | 613307        | 54.11%          | 10.100%       |
| 3         | 6.038       | 801           | 812         | 826          | rBV      | 130502         | 346751        | 30.60%          | 5.710%        |
| 4         | 6.836       | 930           | 943         | 955          | rBV      | 334389         | 800959        | 70.67%          | 13.190%       |
| 5         | 8.696       | 1241          | 1248        | 1260         | rBV      | 724364         | 1133345       | 100.00%         | 18.664%       |
| 6         | 10.098      | 1472          | 1478        | 1486         | rBV      | 749210         | 1005793       | 88.75%          | 16.563%       |
| 7         | 11.122      | 1640          | 1646        | 1659         | rBV      | 630153         | 804443        | 70.98%          | 13.247%       |
| 8         | 12.061      | 1795          | 1800        | 1808         | rBV      | 846252         | 1028140       | 90.72%          | 16.931%       |


Sum of corrected areas: 6072491

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX052120\  
Data File : VX016396.D  
Acq On : 21 May 2020 19:58  
Operator : JC/SP  
Sample : L2732-05  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
KY038PS034-200520

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X050420W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

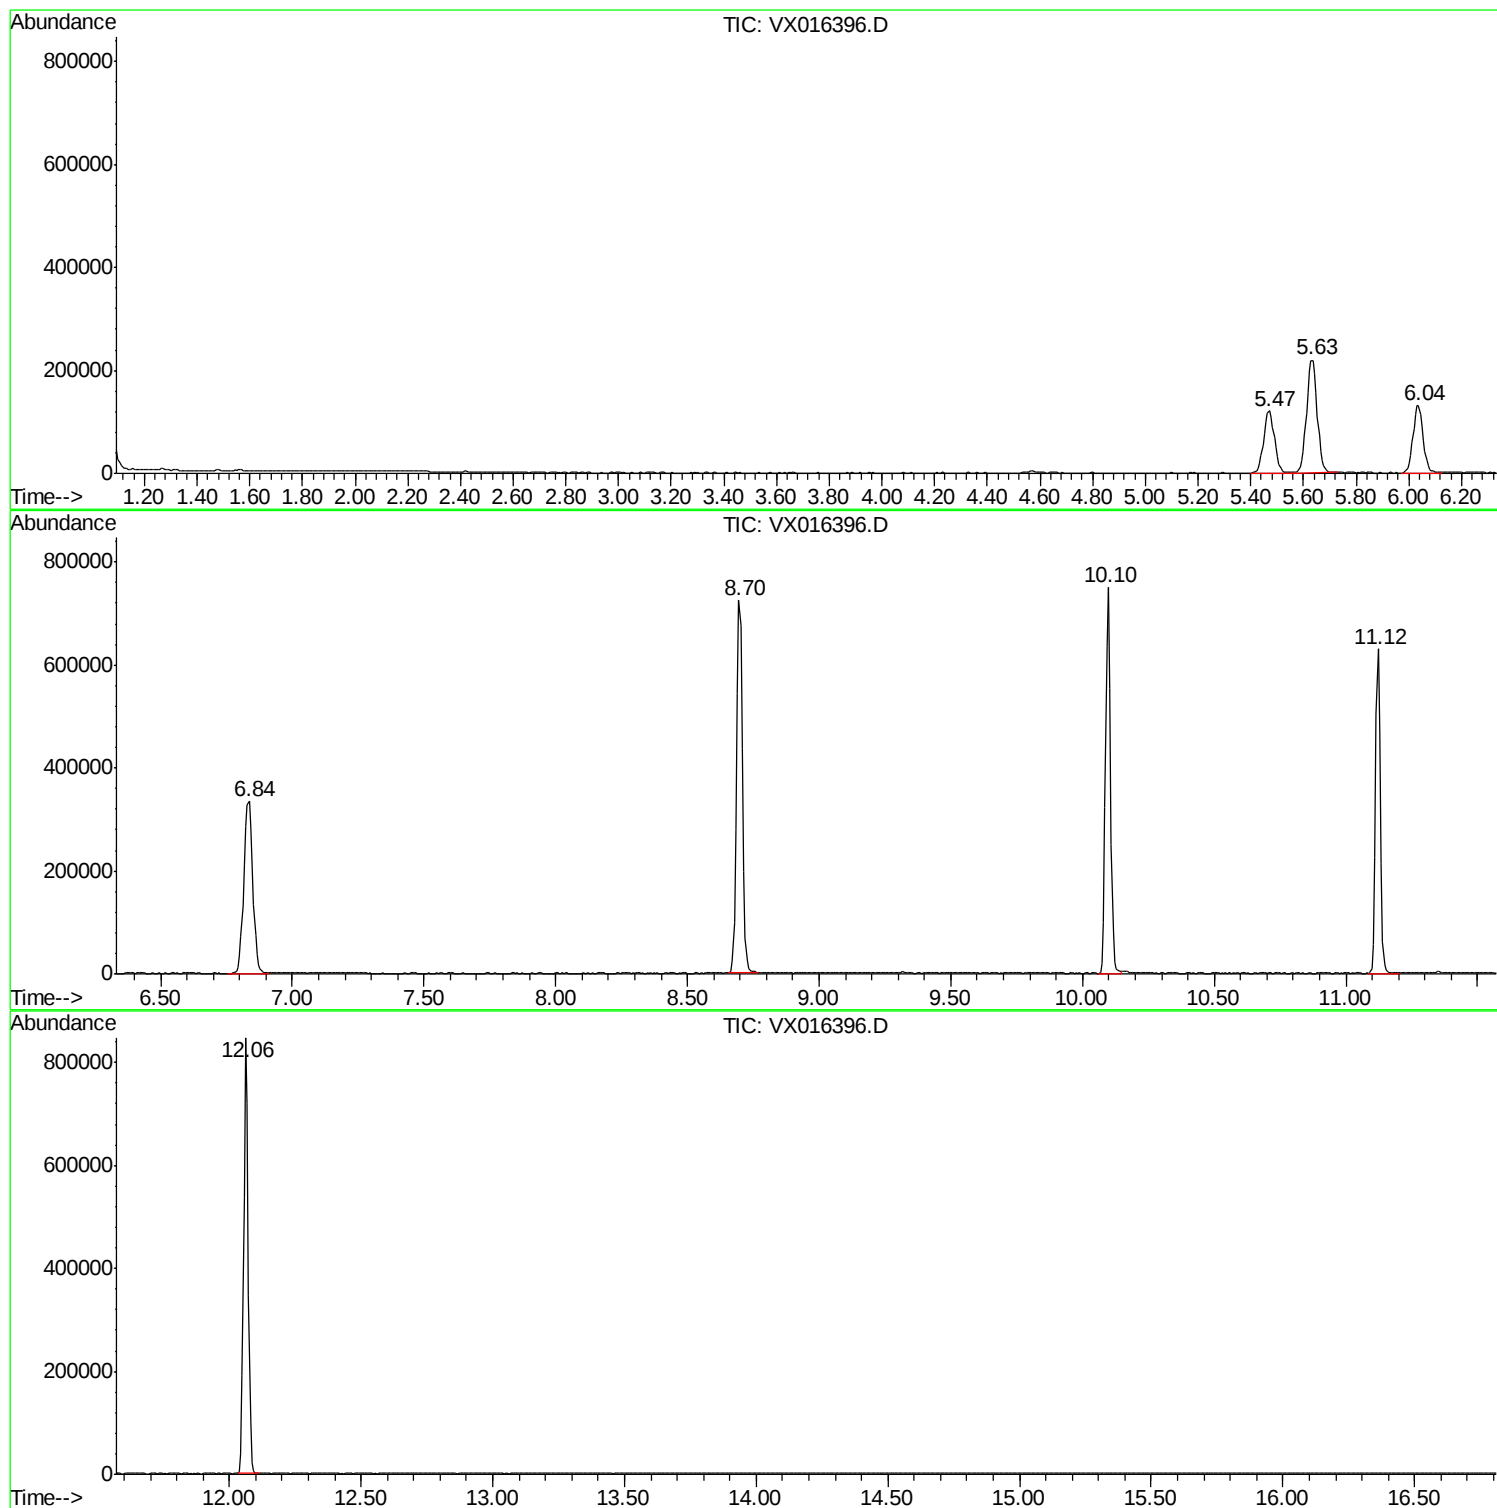

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX052120\  
Data File : VX016396.D  
Acq On : 21 May 2020 19:58  
Operator : JC/SP  
Sample : L2732-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
KY038PS034-200520

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X050420W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX052120\  
Data File : VX016396.D  
Acq On : 21 May 2020 19:58  
Operator : JC/SP  
Sample : L2732-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
KY038PS034-200520

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X050420W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |