

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052121\
 Data File : VX022118.D
 Acq On : 21 May 2021 16:16
 Operator : JC/MD
 Sample : M2480-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WASTE-WATER-NO-FEEDS

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M

Title : SW846 8260

Signal : TIC: VX022118.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.453	56	60	70	rBV	127968	144120	31.03%	5.362%
2	2.068	157	161	166	rVB2	3346	4976	1.07%	0.185%
3	2.391	209	214	223	rVB	23018	41697	8.98%	1.551%
4	2.556	235	241	247	rBV2	2736	4869	1.05%	0.181%
5	4.251	509	519	526	rBV4	2995	8057	1.73%	0.300%
6	4.580	559	573	585	rBV	13002	37406	8.05%	1.392%
7	4.690	585	591	601	rVB2	7244	20116	4.33%	0.748%
8	5.025	637	646	655	rBV	28681	84709	18.24%	3.152%
9	5.104	655	659	671	rVB2	6379	18601	4.00%	0.692%
10	5.403	696	708	719	rBV3	50471	147757	31.81%	5.497%
11	5.568	724	735	748	rBV	80799	224580	48.35%	8.355%
12	5.970	791	801	814	rBV	63303	163014	35.10%	6.065%
13	6.775	921	933	947	rBV	141229	335086	72.15%	12.467%
14	7.671	1073	1080	1088	rVB6	2326	5085	1.09%	0.189%
15	8.659	1234	1242	1252	rBV	288593	464459	100.00%	17.280%
16	10.061	1466	1472	1489	rVB	270791	380285	81.88%	14.148%
17	10.945	1613	1617	1622	rBV	11563	15653	3.37%	0.582%
18	11.030	1624	1631	1635	rBV2	4776	6811	1.47%	0.253%
19	11.085	1635	1640	1647	rBV	218306	267138	57.52%	9.939%
20	12.024	1789	1794	1801	rBV	253965	313433	67.48%	11.661%




Sum of corrected areas: 2687852

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052121\
Data File : VX022118.D
Acq On : 21 May 2021 16:16
Operator : JC/MD
Sample : M2480-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WASTE-WATER-NO-FEEDS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

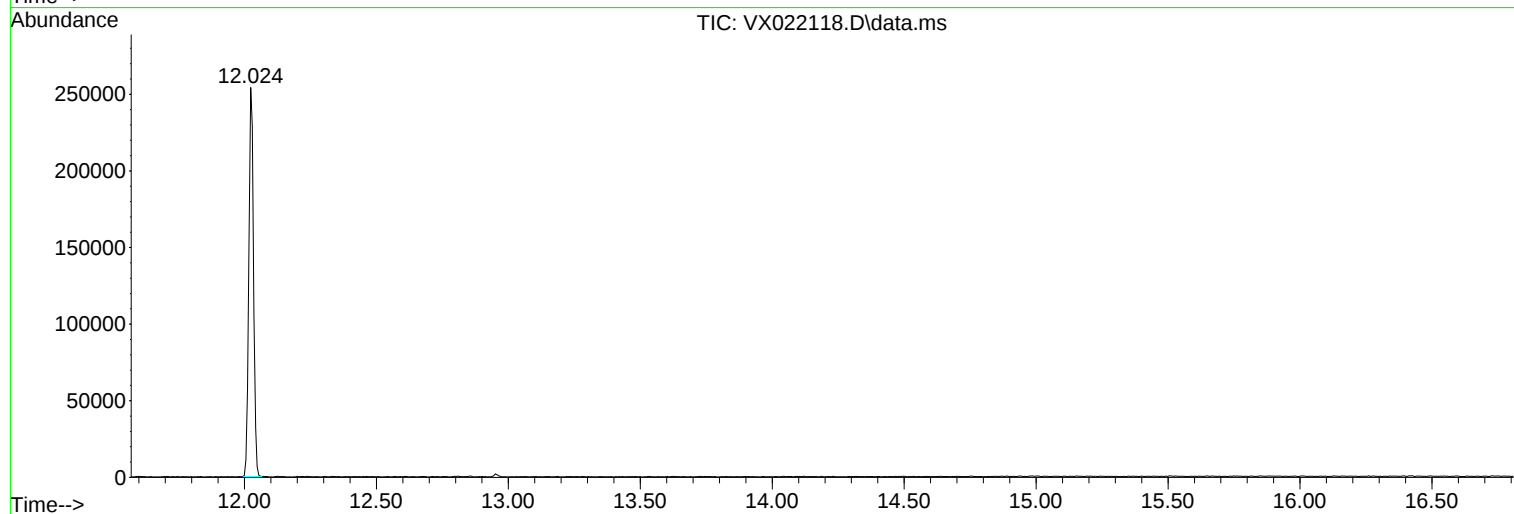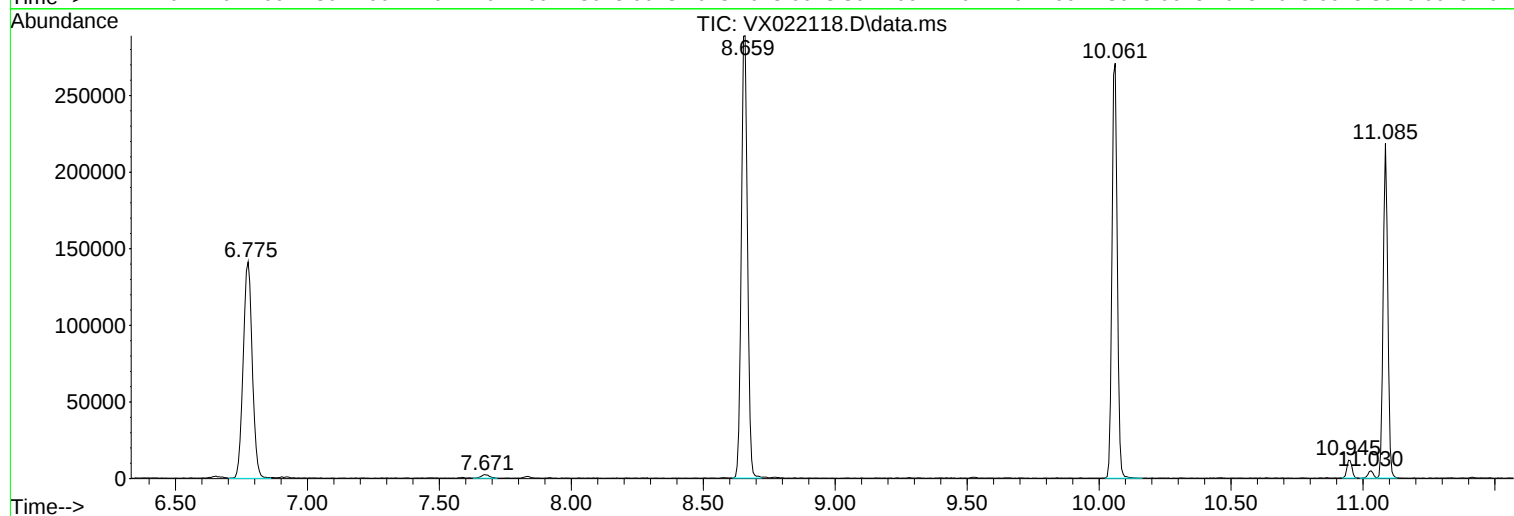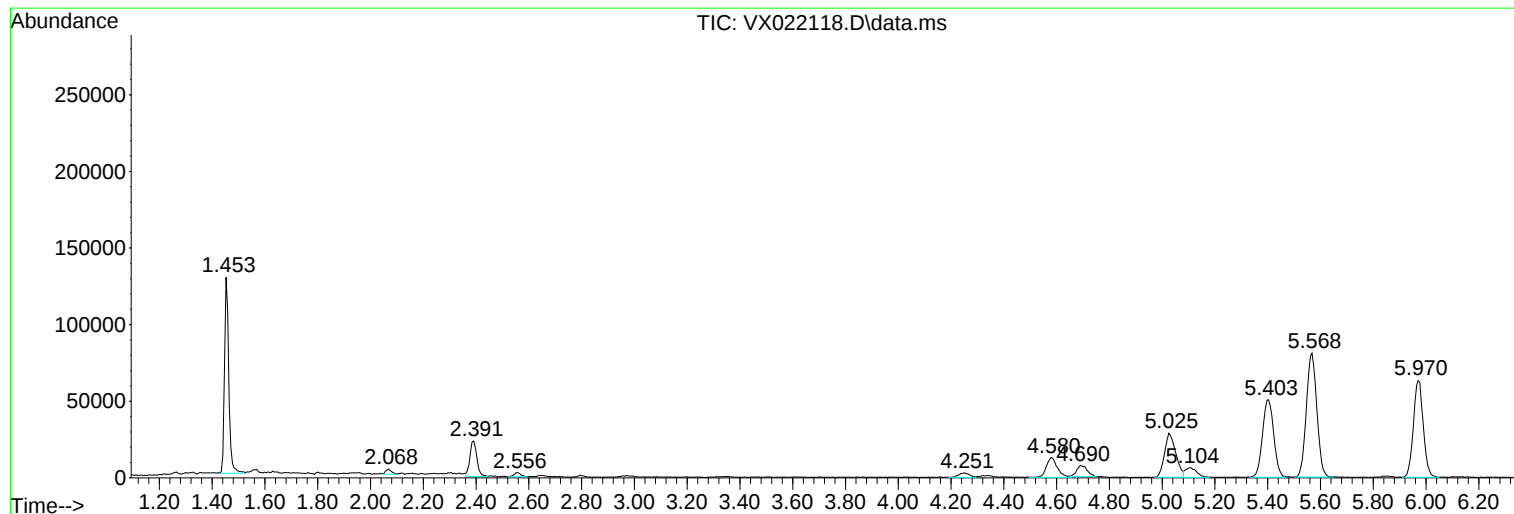

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052121\
Data File : VX022118.D
Acq On : 21 May 2021 16:16
Operator : JC/MD
Sample : M2480-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WASTE-WATER-NO-FEEDS










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Acetaldehyde Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.453	32.09 ug/l	144120	Pentafluorobenzene	5.568

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Acetaldehyde	44	C2H4O	000075-07-0	64
2			Ethylene oxide	44	C2H4O	000075-21-8	9
3			Propane	44	C3H8	000074-98-6	5
4			Alanine	89	C3H7NO2	000056-41-7	4
5			Carbon dioxide	44	CO2	000124-38-9	3

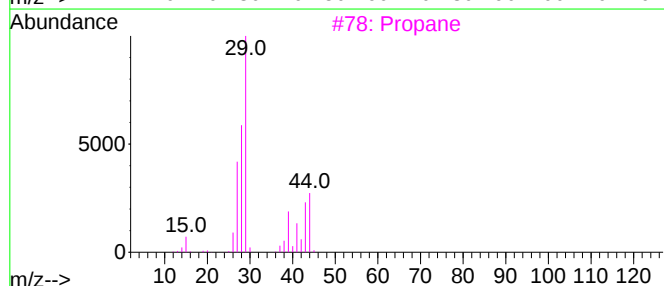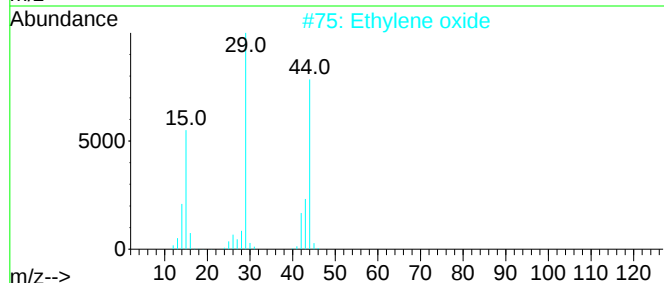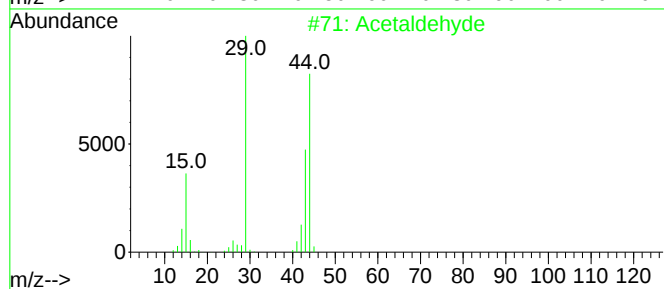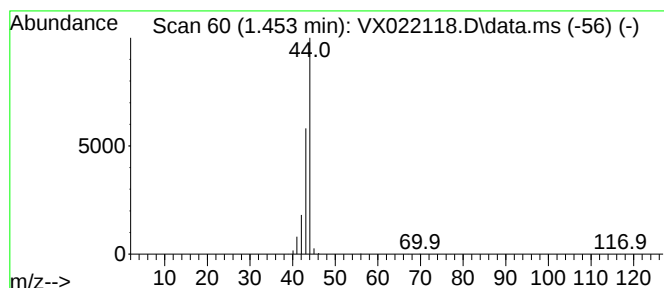

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052121\
Data File : VX022118.D
Acq On : 21 May 2021 16:16
Operator : JC/MD
Sample : M2480-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WASTE-WATER-NO-FEEDS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Acetaldehyde	1.453	32.1	ug/l	144120	1	5.568	224580	50.0