

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052121\
 Data File : VX022121.D
 Acq On : 21 May 2021 17:26
 Operator : JC/MD
 Sample : M2481-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DI-WATER

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M

Title : SW846 8260

Signal : TIC: VX022121.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.111	647	660	673	rBV4	10490	32794	7.37%	1.463%
2	5.397	697	707	719	rBV2	49843	142093	31.93%	6.340%
3	5.562	722	734	750	rVB3	75506	213717	48.02%	9.536%
4	5.971	791	801	815	rVB2	60920	156849	35.25%	6.998%
5	6.769	920	932	944	rBV	135439	322663	72.51%	14.396%
6	8.653	1234	1241	1250	rBV	287634	445013	100.00%	19.855%
7	10.055	1465	1471	1480	rBV	269311	369549	83.04%	16.488%
8	11.085	1634	1640	1651	rBV	209443	259522	58.32%	11.579%
9	12.024	1789	1794	1801	rVB	240824	299075	67.21%	13.344%




Sum of corrected areas: 2241275

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052121\
Data File : VX022121.D
Acq On : 21 May 2021 17:26
Operator : JC/MD
Sample : M2481-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DI-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

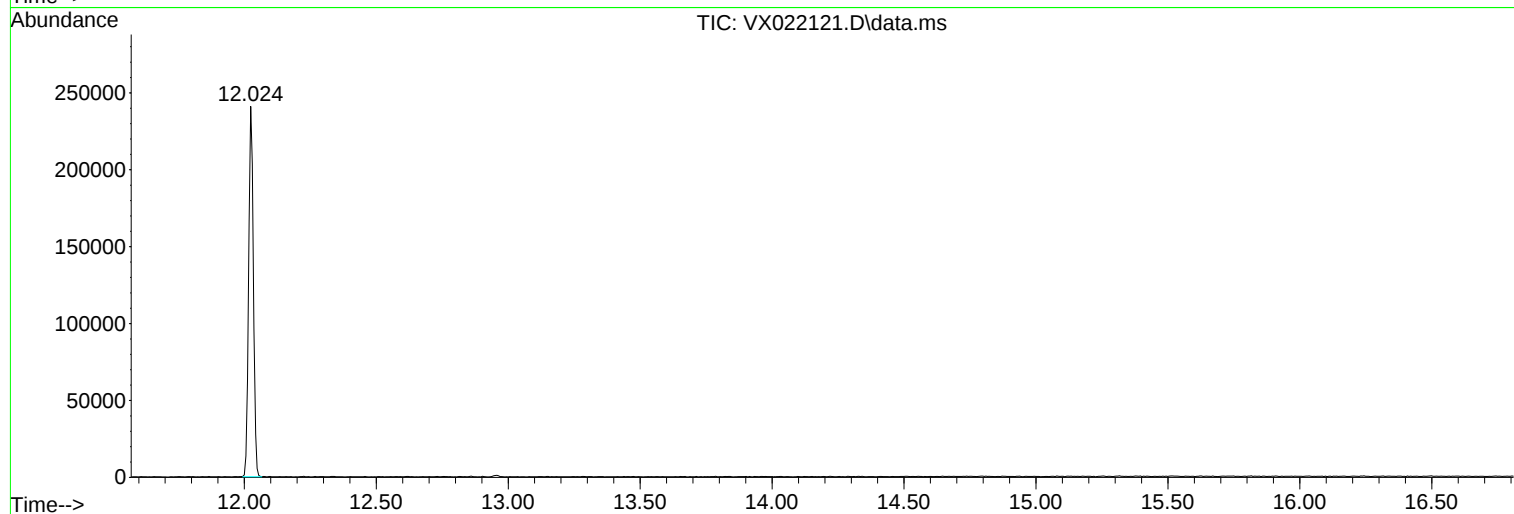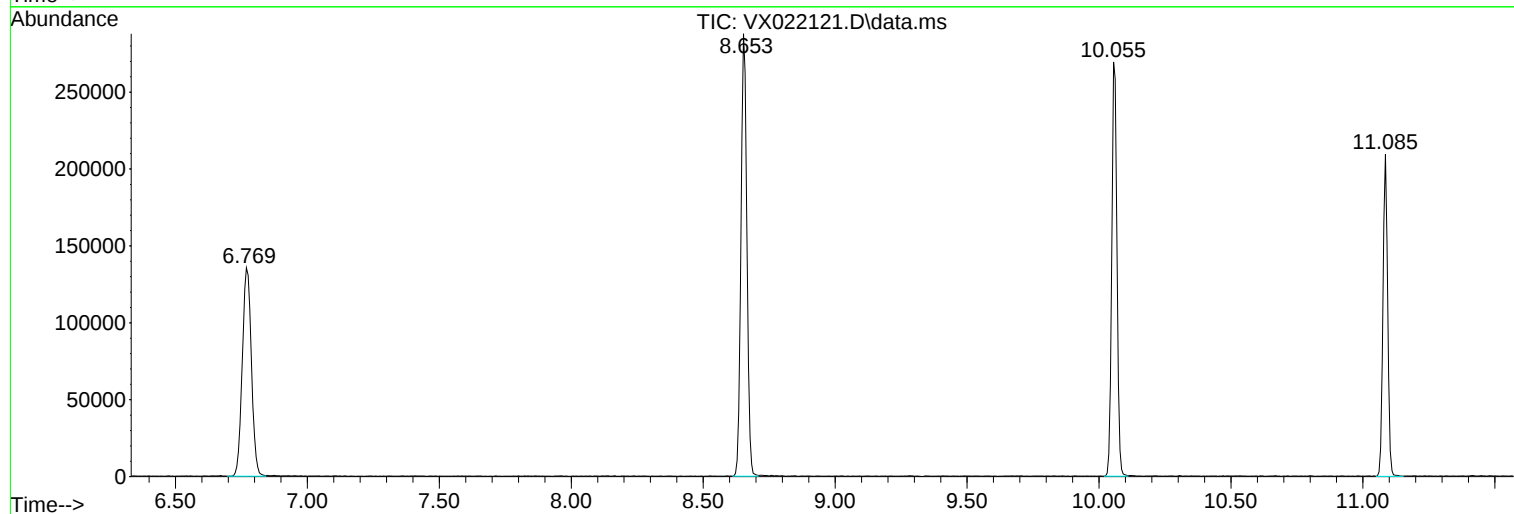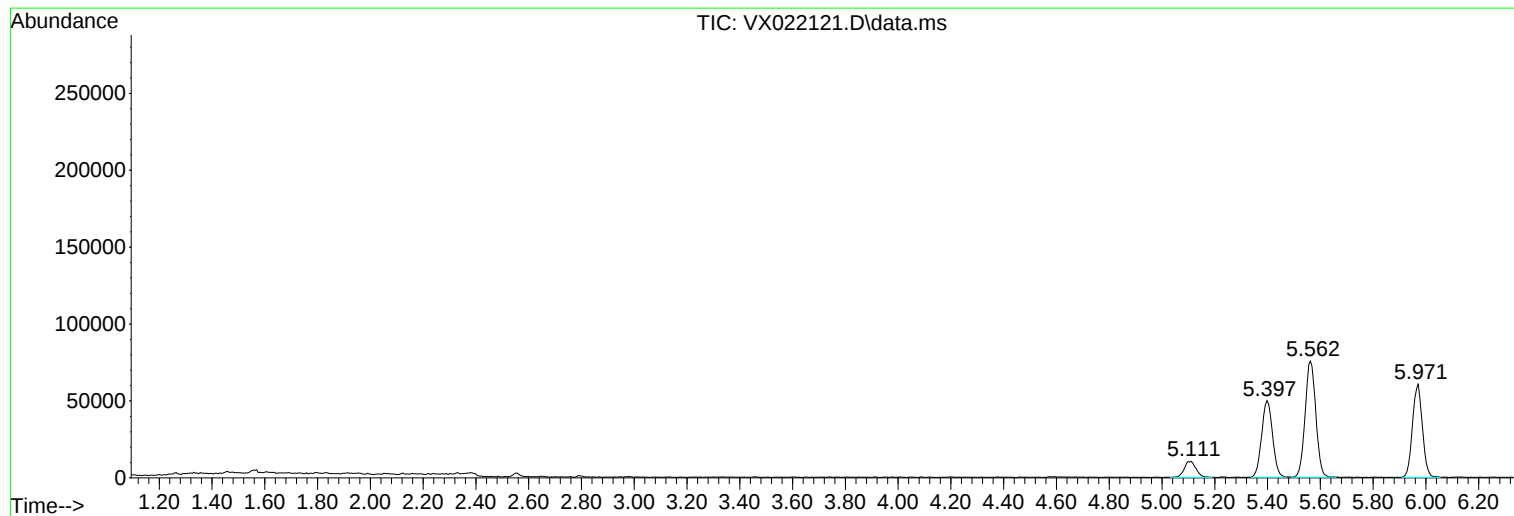

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052121\
Data File : VX022121.D
Acq On : 21 May 2021 17:26
Operator : JC/MD
Sample : M2481-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DI-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052121\
Data File : VX022121.D
Acq On : 21 May 2021 17:26
Operator : JC/MD
Sample : M2481-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DI-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
