

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052121\
 Data File : VX022136.D
 Acq On : 22 May 2021 00:31
 Operator : JC/MD
 Sample : M2420-03
 Misc : 5.07g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CONCESSION-CP-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M

Title : SW846 8260

Signal : TIC: VX022136.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.569	69	79	80	rBV6	4893	11044	2.63%	0.510%
2	2.953	298	306	314	rBV2	7568	18612	4.43%	0.860%
3	5.397	697	707	719	rBV2	43661	126189	30.04%	5.831%
4	5.556	723	733	746	rVB	71785	203357	48.40%	9.396%
5	5.964	790	800	814	rBV	56232	144417	34.38%	6.673%
6	6.769	921	932	942	rBV	124241	297985	70.93%	13.768%
7	8.653	1234	1241	1254	rVV	275917	420118	100.00%	19.412%
8	8.763	1254	1259	1266	rVB4	2860	4957	1.18%	0.229%
9	10.061	1466	1472	1478	rBV	248006	349908	83.29%	16.168%
10	11.085	1635	1640	1652	rVB	204645	259898	61.86%	12.009%
11	12.024	1789	1794	1803	rVB	265295	327768	78.02%	15.145%




Sum of corrected areas: 2164253

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052121\
Data File : VX022136.D
Acq On : 22 May 2021 00:31
Operator : JC/MD
Sample : M2420-03
Misc : 5.07g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CONCESSION-CP-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

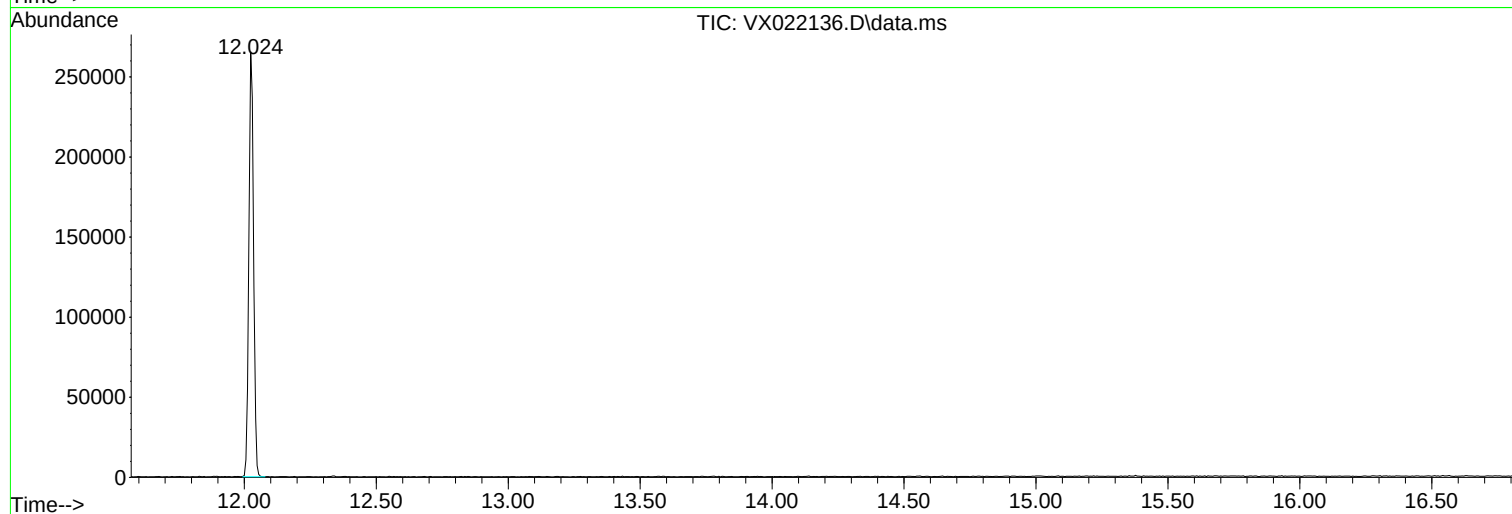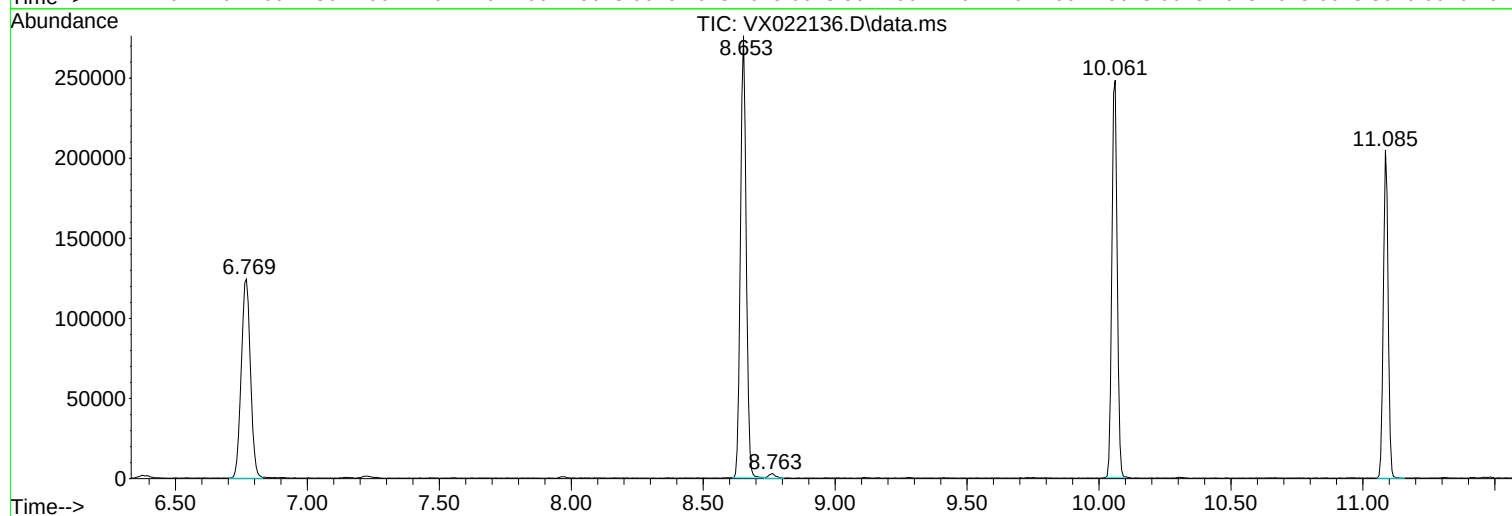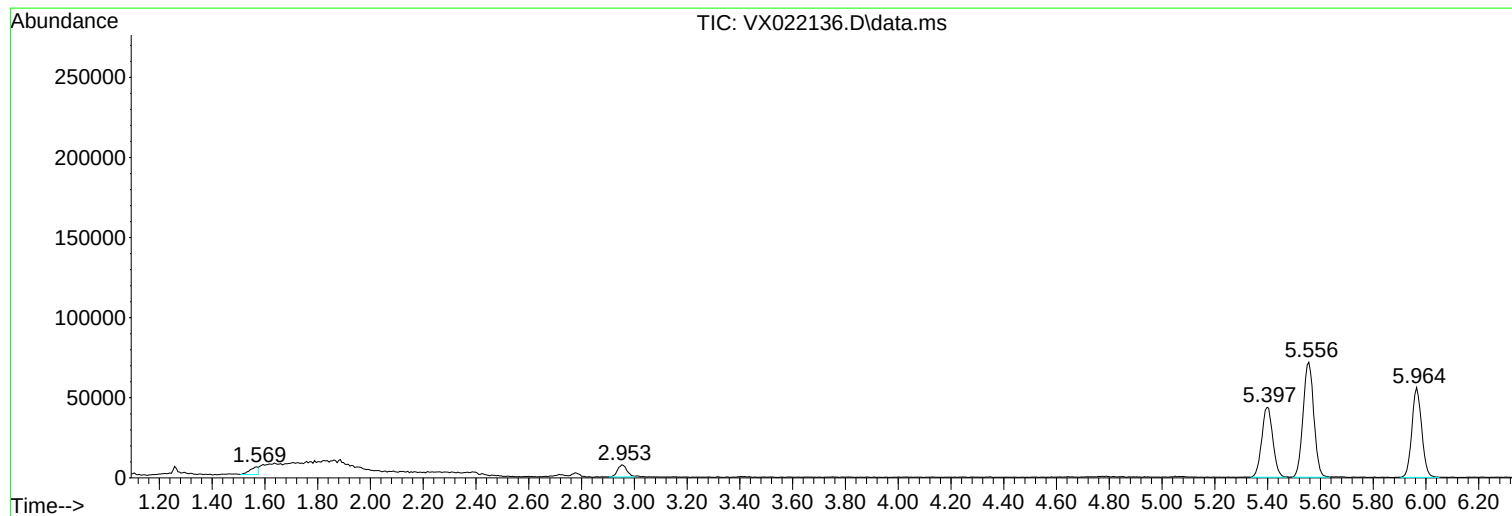

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052121\
Data File : VX022136.D
Acq On : 22 May 2021 00:31
Operator : JC/MD
Sample : M2420-03
Misc : 5.07g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CONCESSION-CP-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052121\
Data File : VX022136.D
Acq On : 22 May 2021 00:31
Operator : JC/MD
Sample : M2420-03
Misc : 5.07g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CONCESSION-CP-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc