
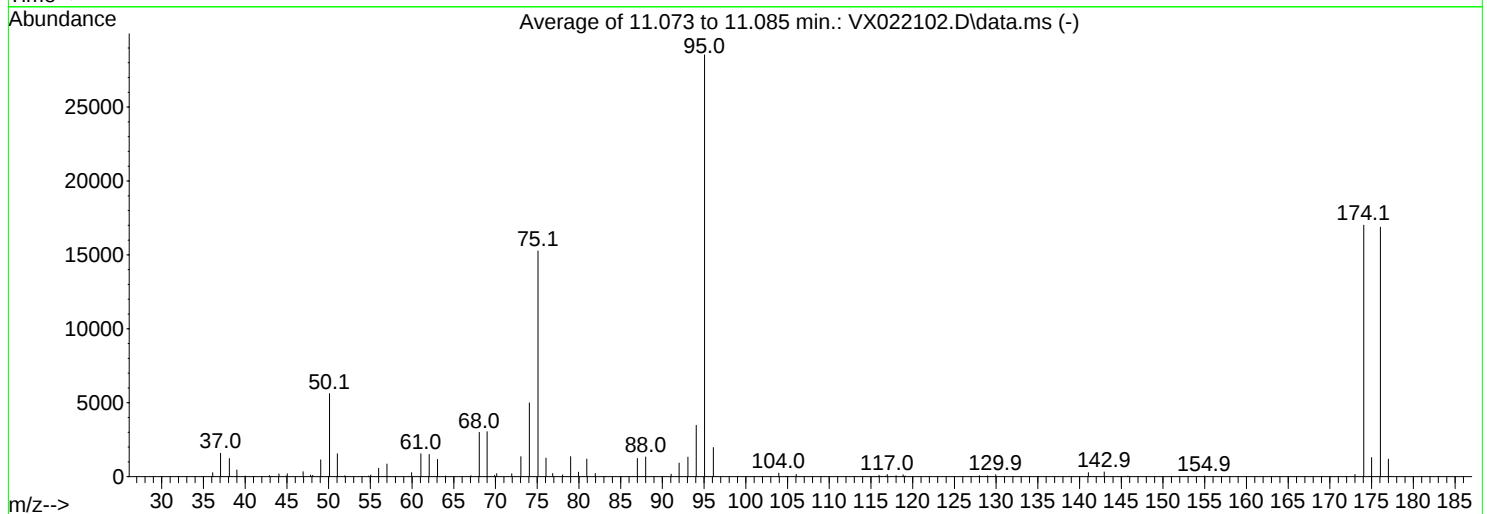


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052121\
 Data File : VX022102.D
 Acq On : 21 May 2021 09:20
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Title : SW846 8260
 Last Update : Wed May 19 14:23:10 2021

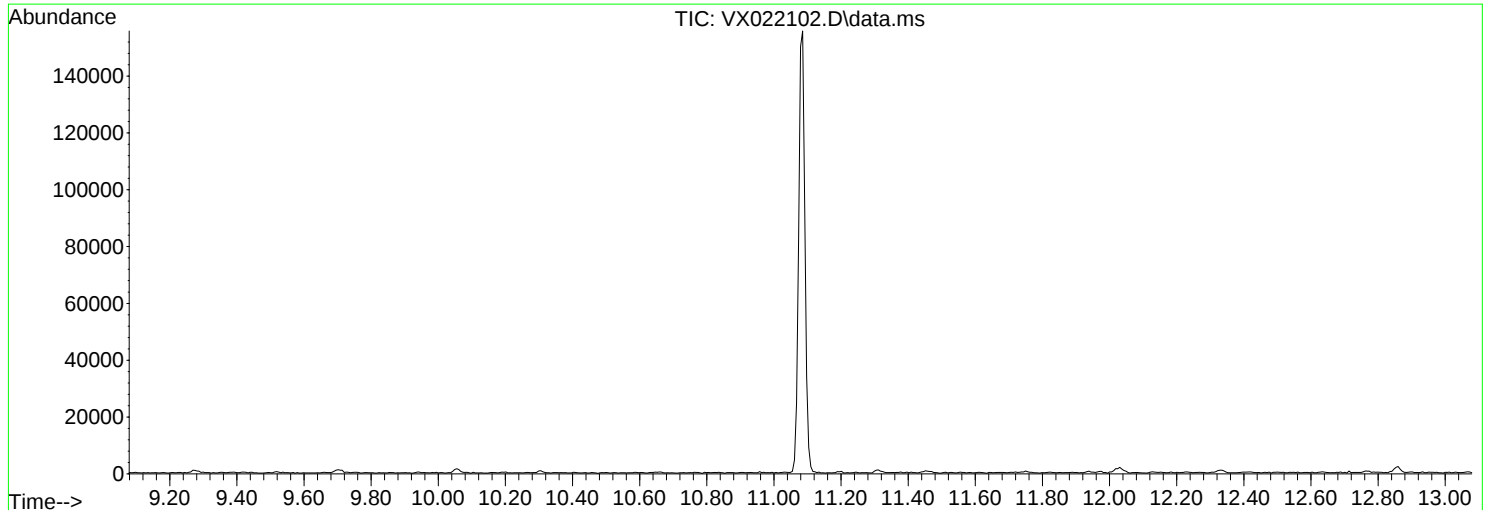

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	5616	PASS
75	95	30	60	53.5	15270	PASS
95	95	100	100	100.0	28531	PASS
96	95	5	9	6.9	1968	PASS
173	174	0.00	2	0.8	136	PASS
174	95	50	100	59.6	17016	PASS
175	174	5	9	7.6	1288	PASS
176	174	95	101	99.2	16875	PASS
177	176	5	9	7.0	1179	PASS