
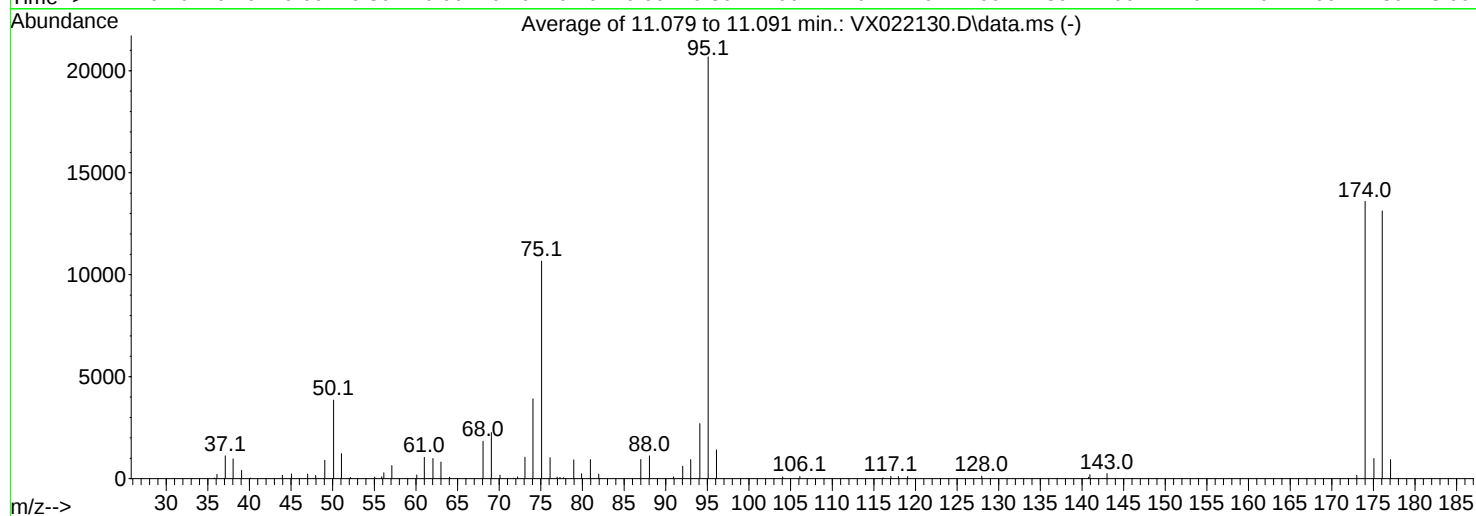


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052121\
 Data File : VX022130.D
 Acq On : 21 May 2021 20:59
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Title : SW846 8260
 Last Update : Wed May 19 14:23:10 2021

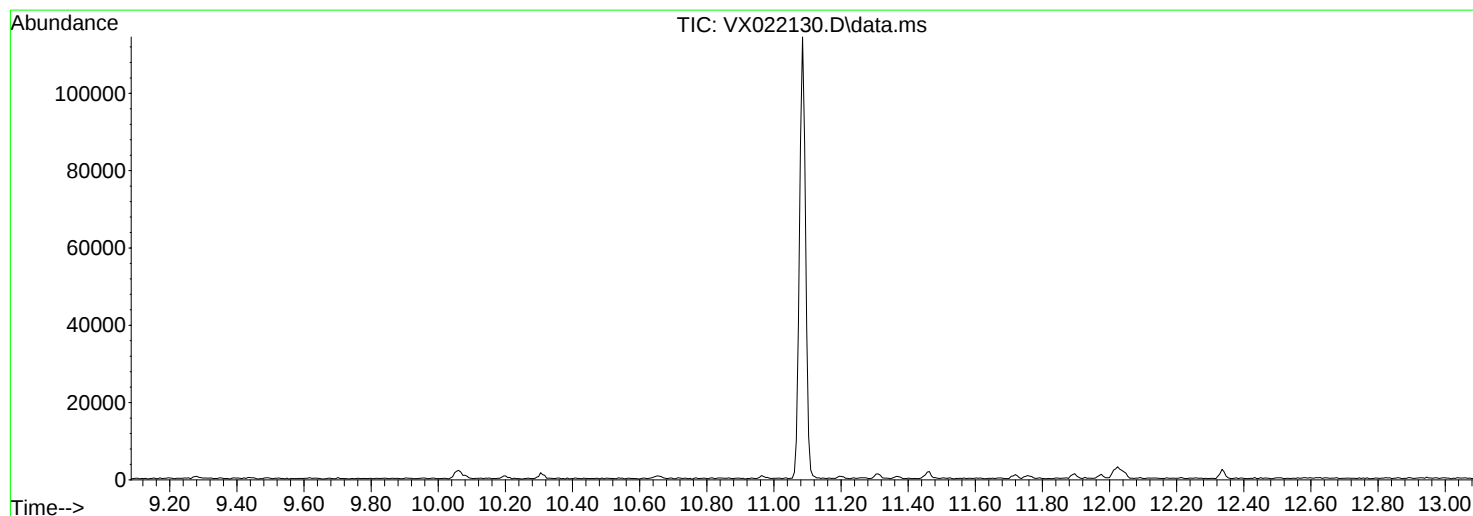

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	3849	PASS
75	95	30	60	51.6	10669	PASS
95	95	100	100	100.0	20683	PASS
96	95	5	9	6.8	1411	PASS
173	174	0.00	2	1.2	168	PASS
174	95	50	100	65.7	13595	PASS
175	174	5	9	7.3	992	PASS
176	174	95	101	96.5	13125	PASS
177	176	5	9	7.1	932	PASS