

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX052219\
 Data File : VX009798.D
 Acq On : 22 May 2019 12:50
 Operator : JC/SP
 Sample : K2970-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-11-S

Quant Time: May 23 07:38:01 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 09 07:31:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	167113	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	269242	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	234717	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	94849	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.06	65	115885	50.80	ug/l	0.00
Spiked Amount			Recovery	=	101.60%	
35) Dibromofluoromethane	5.50	113	83643	49.42	ug/l	0.00
Spiked Amount			Recovery	=	98.84%	
50) Toluene-d8	8.71	98	342051	50.06	ug/l	0.00
Spiked Amount			Recovery	=	100.12%	
62) 4-Bromofluorobenzene	11.13	95	108956	43.88	ug/l	0.00
Spiked Amount			Recovery	=	87.76%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Acetone	2.44	43	10748	8.774	ug/l	94
18) Methyl Acetate	2.78	43	4538	1.558	ug/l	99
20) Methylene Chloride	2.85	84	16977	8.560	ug/l	97
43) Isopropyl Acetate	6.45	43	11312	2.029	ug/l	97
95) Naphthalene	13.83	128	11961	1.730	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX052219\
Data File : VX009798.D
Acq On : 22 May 2019 12:50
Operator : JC/SP
Sample : K2970-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-11-S

Quant Time: May 23 07:38:01 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
Quant Title : SW846 8260
QLast Update : Thu May 09 07:31:15 2019
Response via : Initial Calibration

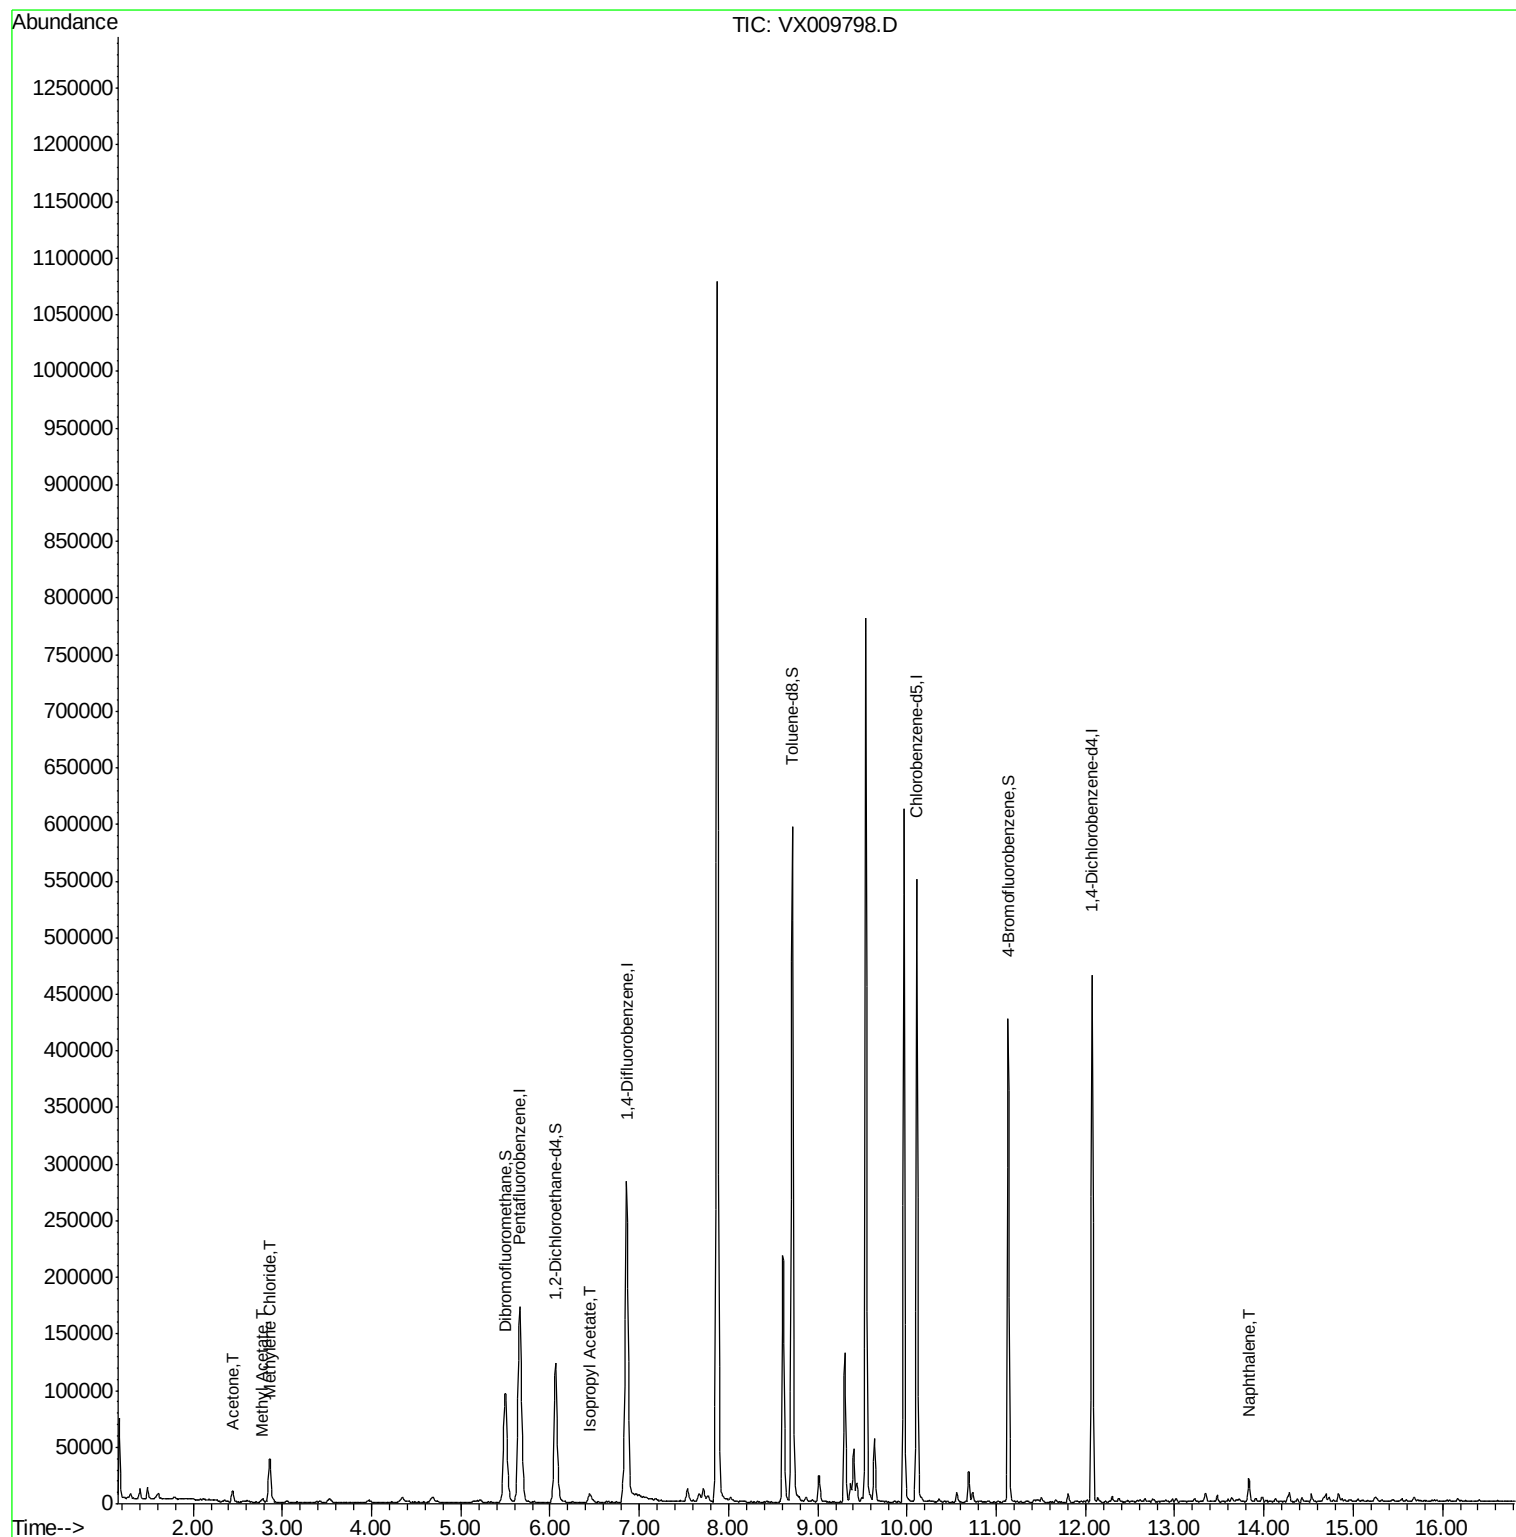



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.00 min

Lab File: VX009798.D

Acq: 22 May 2019 12:50


Instrument :
MSVOA_X
ClientSampleId :
TP-11-S

Tot Ion:168 Resp: 167113

Ion Ratio Lower Upper




168 100

99 54.0 42.3 63.5

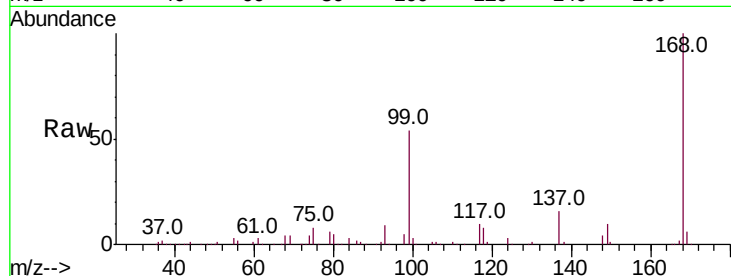

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

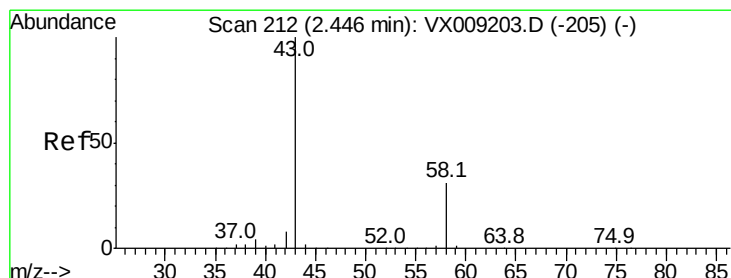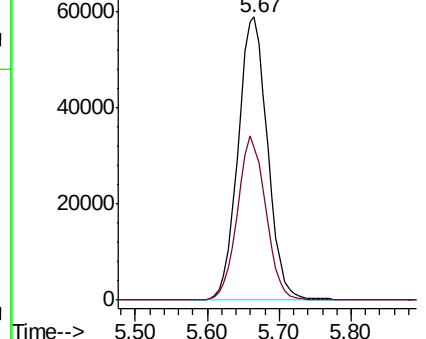

#16

Acetone

Concen: 8.774 ug/l

RT: 2.44 min Scan# 211

Delta R.T. -0.01 min

Lab File: VX009798.D


Acq: 22 May 2019 12:50

Tgt Ion: 43 Resp: 10748

Ion Ratio Lower Upper



43 100


58 28.1 24.9 37.3

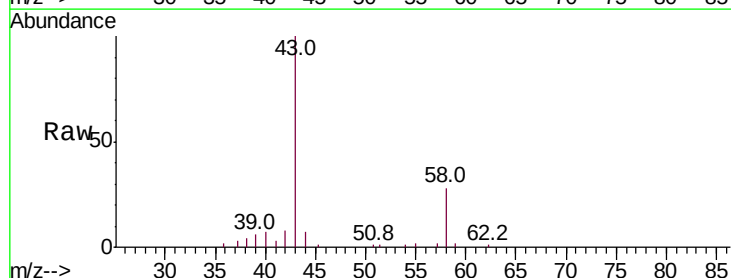

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0




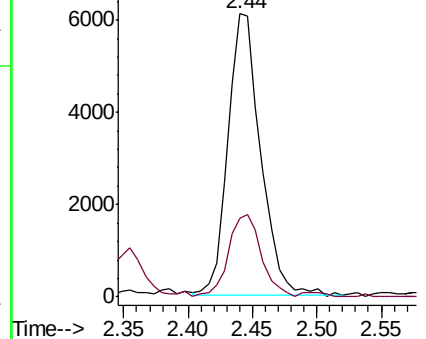


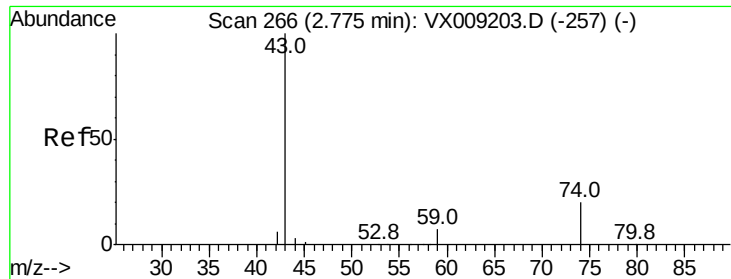

#18
Methvl Acetate
Concen: 1.558 ug/l
RT: 2.78 min Scan# 266
Delta R.T. 0.00 min
Lab File: VX009798.D
Acq: 22 May 2019 12:50




Instrument :
MSVOA_X
ClientSampled :
TP-11-S


Tot Ion: 43 Resp: 4538
Ion Ratio Lower Upper
43 100
74 20.6 16.2 24.4

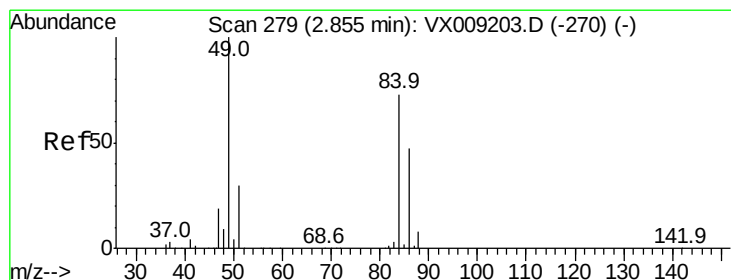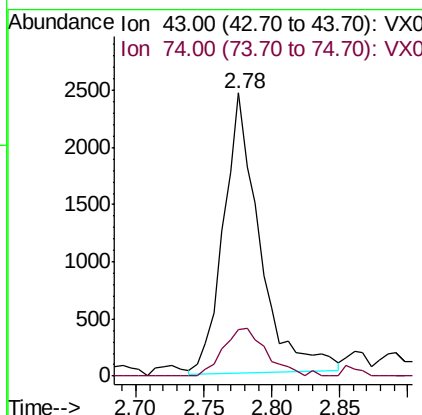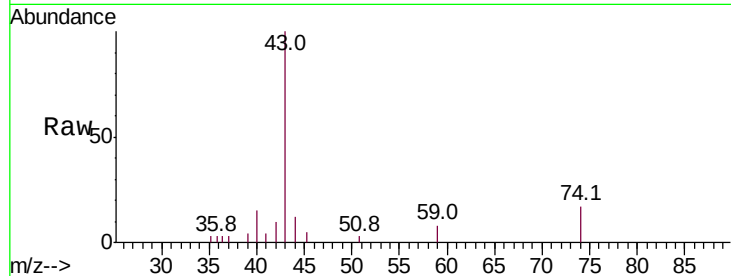

#20
Methylene Chloride
Concen: 8.560 ug/l
RT: 2.85 min Scan# 279
Delta R.T. 0.00 min
Lab File: VX009798.D
Acq: 22 May 2019 12:50

Tgt Ion: 84 Resp: 16977
Ion Ratio Lower Upper
84 100
49 141.7 109.9 164.9
51 42.1 32.7 49.1
86 63.0 52.0 78.0


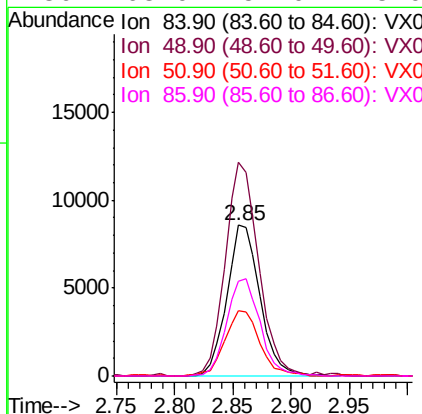

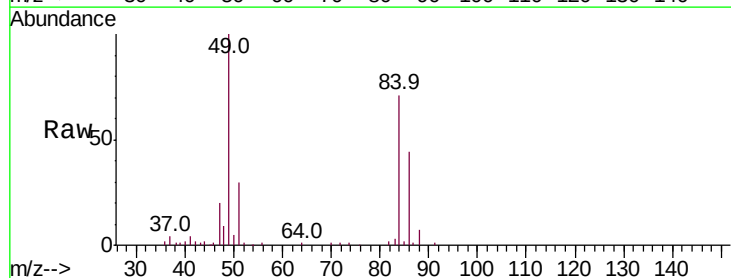


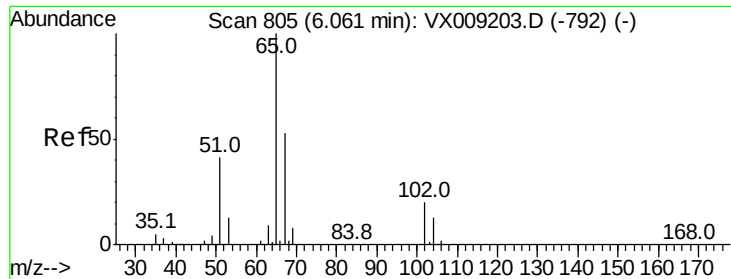

#33
 1,2-Dichloroethane-d4
 Concen: 50.798 ug/l
 RT: 6.06 min Scan# 805
 Delta R.T. 0.00 min
 Lab File: VX009798.D
 Acq: 22 May 2019 12:50




Instrument :
 MSVOA_X
 ClientSampleId :
 TP-11-S


Tot Ion: 65 Resp: 115885
 Ion Ratio Lower Upper
 65 100
 67 53.0 0.0 106.6

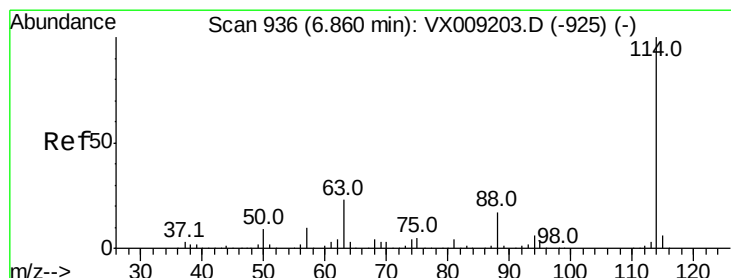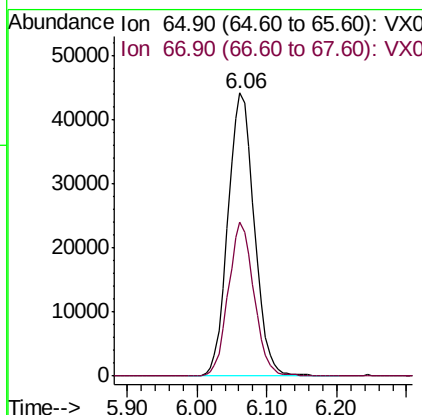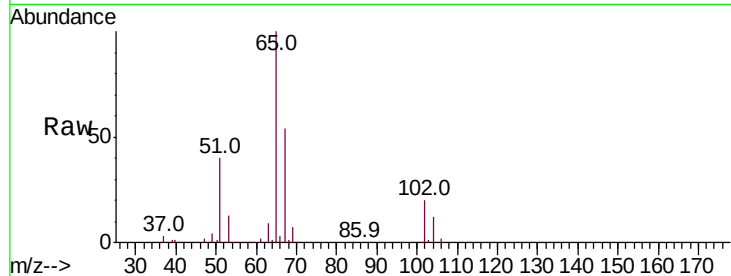

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. 0.00 min
 Lab File: VX009798.D
 Acq: 22 May 2019 12:50

Tgt Ion:114 Resp: 269242
 Ion Ratio Lower Upper
 114 100
 63 23.6 0.0 45.6
 88 17.0 0.0 33.2

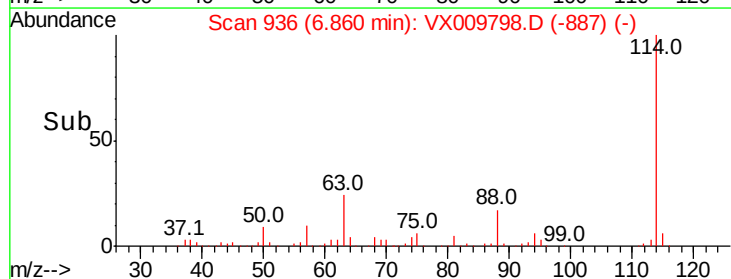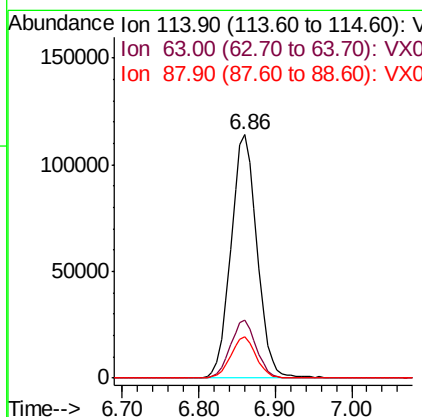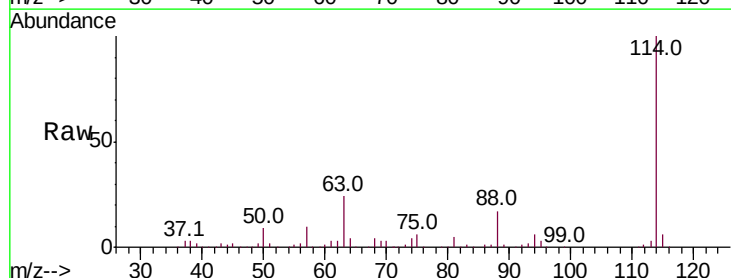

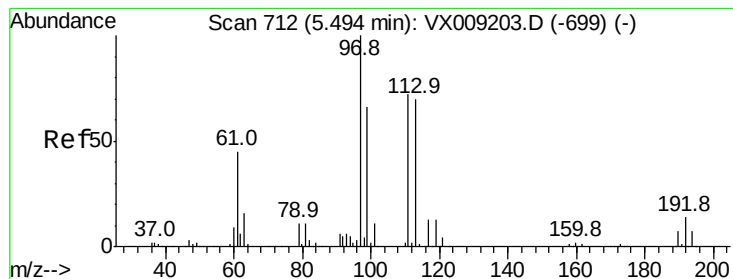

#35

Dibromofluoromethane

Concen: 49.418 ug/l

RT: 5.50 min Scan# 713

Delta R.T. 0.01 min

Lab File: VX009798.D

Acq: 22 May 2019 12:50

Instrument :

MSVOA_X

ClientSampleId :

TP-11-S


Tot Ion:113 Resp: 83643

Ion Ratio Lower Upper

113 100

111 103.8 82.8 124.2




192 21.5 17.0 25.6

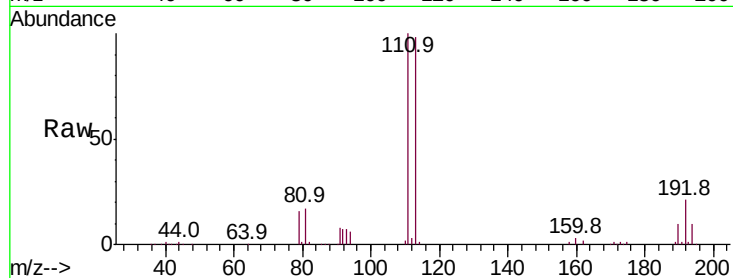

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

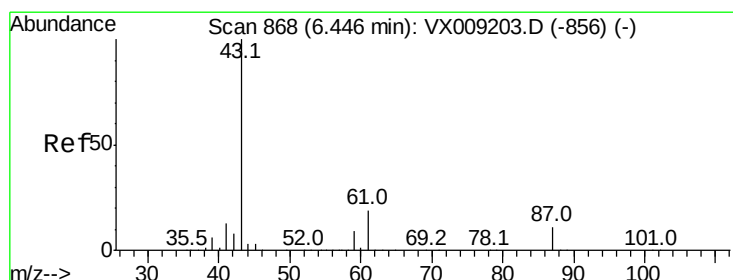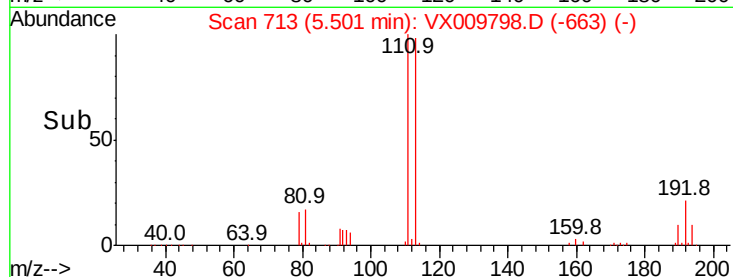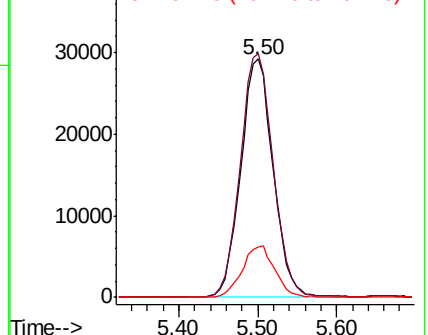

#43

Isopropyl Acetate

Concen: 2.029 ug/l

RT: 6.45 min Scan# 868

Delta R.T. 0.00 min

Lab File: VX009798.D

Acq: 22 May 2019 12:50


Tgt Ion: 43 Resp: 11312

Ion Ratio Lower Upper

43 100

61 20.1 15.1 22.7



87 12.2 9.0 13.6

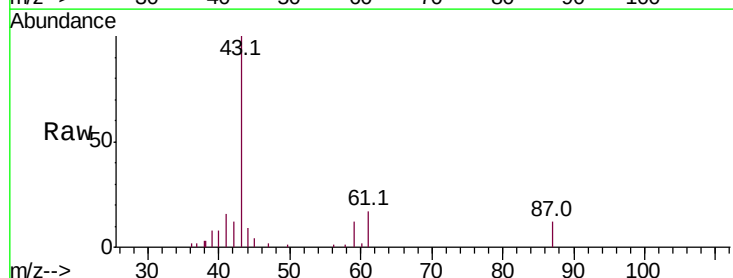


Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

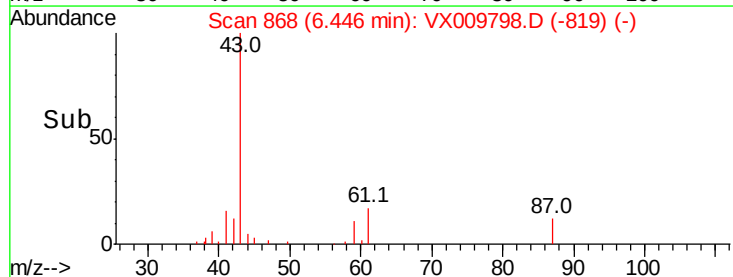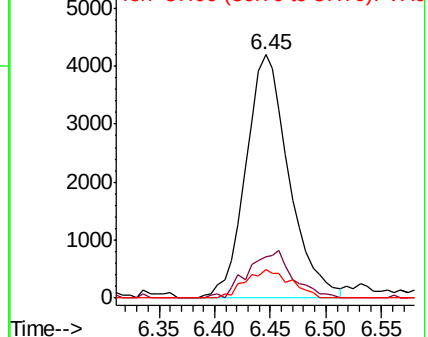

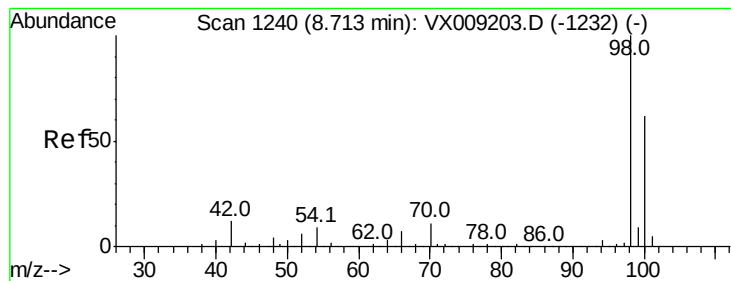

#50

Toluene-d8

Concen: 50.057 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX009798.D

Acq: 22 May 2019 12:50

Instrument :

MSVOA_X

ClientSampleId :


TP-11-S

Tot Ion: 98 Resp: 342051

Ion Ratio Lower Upper

98 100

100 64.2 51.2 76.8

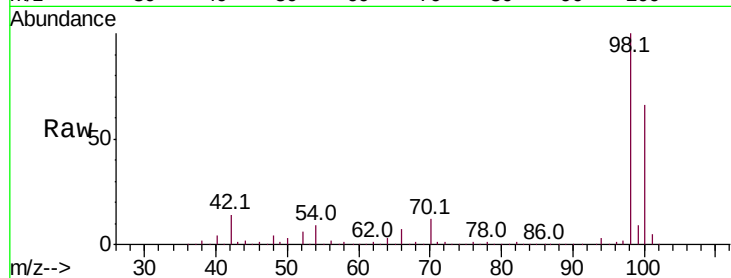

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

8.71

250000

200000



150000

100000

50000

0

Time-->

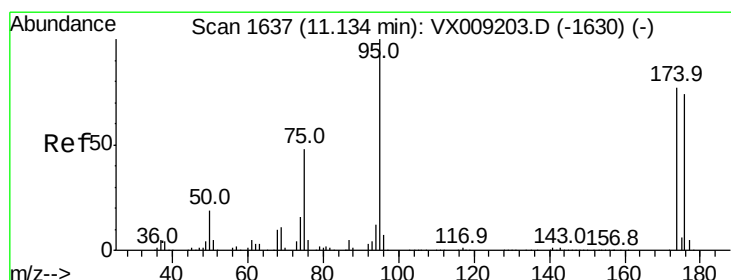

#62

4-Bromofluorobenzene

Concen: 43.881 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.00 min

Lab File: VX009798.D

Acq: 22 May 2019 12:50


Tgt Ion: 95 Resp: 108956

Ion Ratio Lower Upper

95 100

174 82.2 0.0 161.6

176 79.2 0.0 159.2

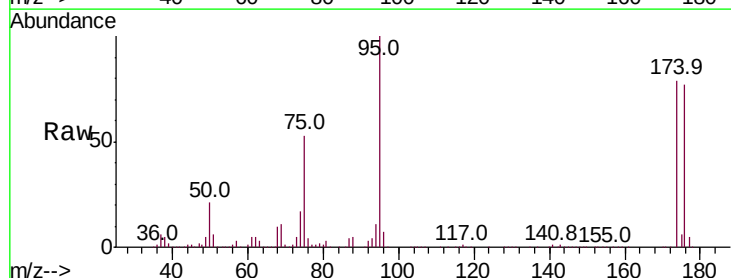

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

120000

100000

80000


60000


40000

20000

0

Time-->









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. 0.00 min
Lab File: VX009798.D
Acq: 22 May 2019 12:50

Instrument :
MSVOA_X
ClientSampled :
TP-11-S

Tot Ion:117 Resp: 234717
Ion Ratio Lower Upper
117 100
82 60.3 48.8 73.2
119 32.1 25.8 38.6

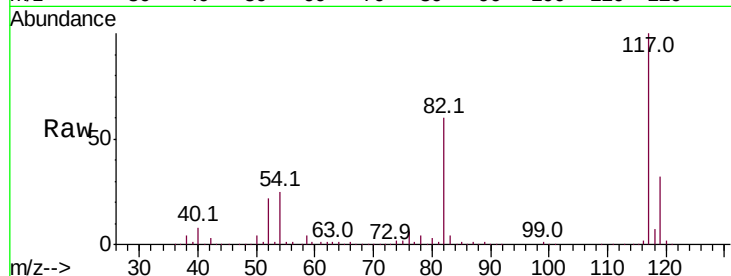


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

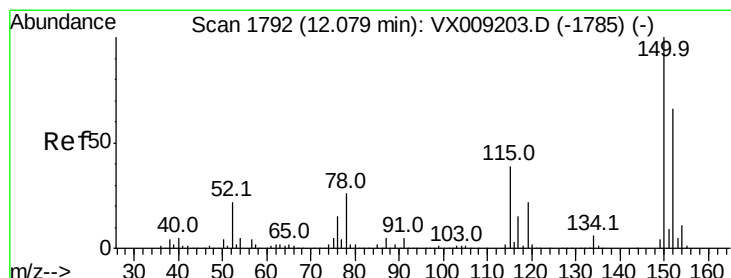
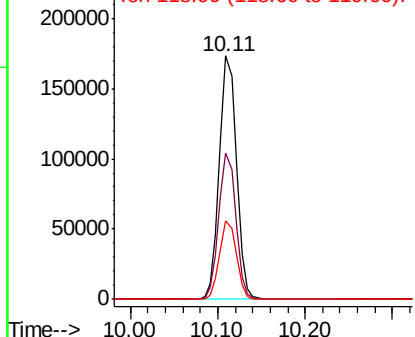



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. 0.00 min
Lab File: VX009798.D
Acq: 22 May 2019 12:50

Tgt Ion:152 Resp: 94849
Ion Ratio Lower Upper
152 100
115 58.8 41.2 123.6
150 158.1 0.0 346.4

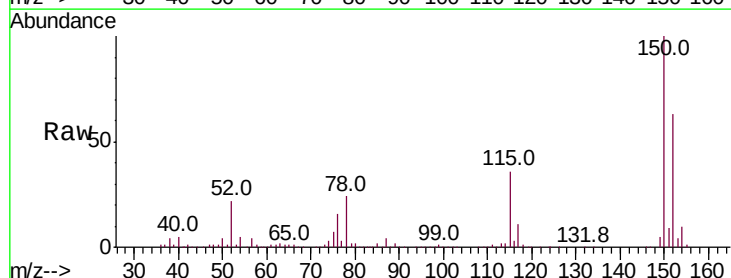

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

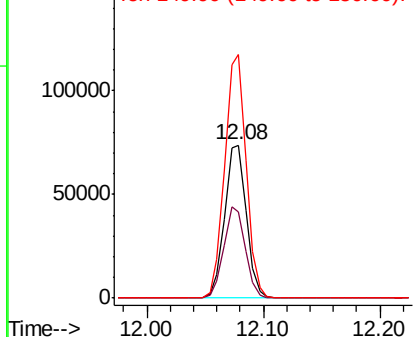

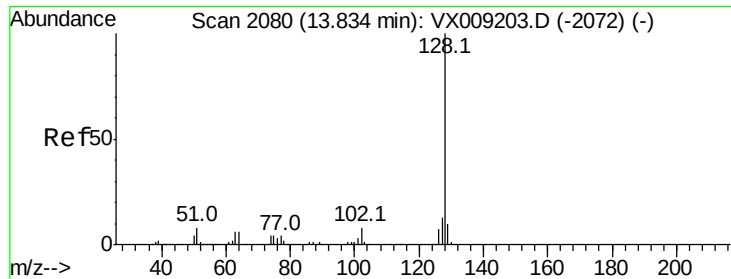

#95
 Naphthalene
 Concen: 1.730 ug/l
 RT: 13.83 min Scan# 2079
 Delta R.T. -0.01 min
 Lab File: VX009798.D
 Acq: 22 May 2019 12:50

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-11-S

Tot Ion	Ratio	Lower	Upper
128	100		
127	13.4	10.4	15.6
129	11.8	8.6	13.0

