

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052224\
 Data File : VX041597.D
 Acq On : 22 May 2024 12:58
 Operator : JC/MD
 Sample : P2494-25 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 5

Quant Time: May 23 03:40:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 08 06:03:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	175816	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	259251	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	248276	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	134052	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	95417	49.852	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	99.700%
35) Dibromofluoromethane	5.385	113	80402	45.764	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	91.520%
50) Toluene-d8	8.647	98	298539	53.688	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	107.380%
62) 4-Bromofluorobenzene	11.079	95	115813	53.802	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	107.600%


Target Compounds				Qvalue		
5) Bromomethane	1.593	94	291	0.326	ug/l	# 48
11) Tert butyl alcohol	2.977	59	139	0.363	ug/l	# 78
13) Acrolein	2.245	56	102	0.336	ug/l	90
16) Acetone	2.392	43	5254	2.359	ug/l	99
20) Methylene Chloride	2.794	84	1154	0.695	ug/l	# 69
25) 2-Butanone	4.605	43	322	0.260	ug/l	# 51
31) Cyclohexane	5.458	56	676	0.293	ug/l	87
36) 1,1-Dichloropropene	5.544	75	11014	5.243	ug/l	# 51
38) Carbon Tetrachloride	5.544	117	15514	6.446	ug/l	# 15
39) Methylcyclohexane	7.373	83	704	0.285	ug/l	95
40) Benzene	6.037	78	99598	15.379	ug/l	99
43) Isopropyl Acetate	6.361	43	5612	1.424	ug/l	93
51) 4-Methyl-2-Pentanone	8.555	43	3818	1.614	ug/l	# 42
52) Toluene	8.720	92	74372	18.773	ug/l	96
53) t-1,3-Dichloropropene	8.714	75	875	2.790	ug/l	# 1
54) cis-1,3-Dichloropropene	8.549	75	1406	0.623	ug/l	# 56
59) 2-Hexanone	9.488	43	2508	1.326	ug/l	# 55
67) Ethyl Benzene	10.195	91	18615	2.239	ug/l	96
68) m/p-Xylenes	10.299	106	40406	12.134	ug/l	98
69) o-Xylene	10.640	106	44773	14.043	ug/l	93
70) Styrene	10.659	104	10906	2.085	ug/l	# 49
73) Isopropylbenzene	10.963	105	2090	0.255	ug/l	91
76) 1,2,3-Trichloropropane	11.079	75	59101	27.053	ug/l	# 39
78) n-propylbenzene	11.305	91	2676	0.311	ug/l	97
79) 2-Chlorotoluene	11.378	91	2353	0.425	ug/l	# 42
80) 1,3,5-Trimethylbenzene	11.451	105	20168	3.023	ug/l	93
81) trans-1,4-Dichloro-2-b...	11.079	75	59101	73.689	ug/l	# 5
82) 4-Chlorotoluene	11.451	91	2463	0.392	ug/l	# 46
84) 1,2,4-Trimethylbenzene	11.750	105	53497	7.970	ug/l	95
85) sec-Butylbenzene	11.750	105	53497	6.535	ug/l	# 57
90) Hexachloroethane	12.548	117	877	0.713	ug/l	# 17
95) Naphthalene	13.774	128	1001535	109.045	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052224\
Data File : VX041597.D
Acq On : 22 May 2024 12:58
Operator : JC/MD
Sample : P2494-25 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
5

Quant Time: May 23 03:40:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
Quant Title : SW846 8260
QLast Update : Wed May 08 06:03:16 2024
Response via : Initial Calibration




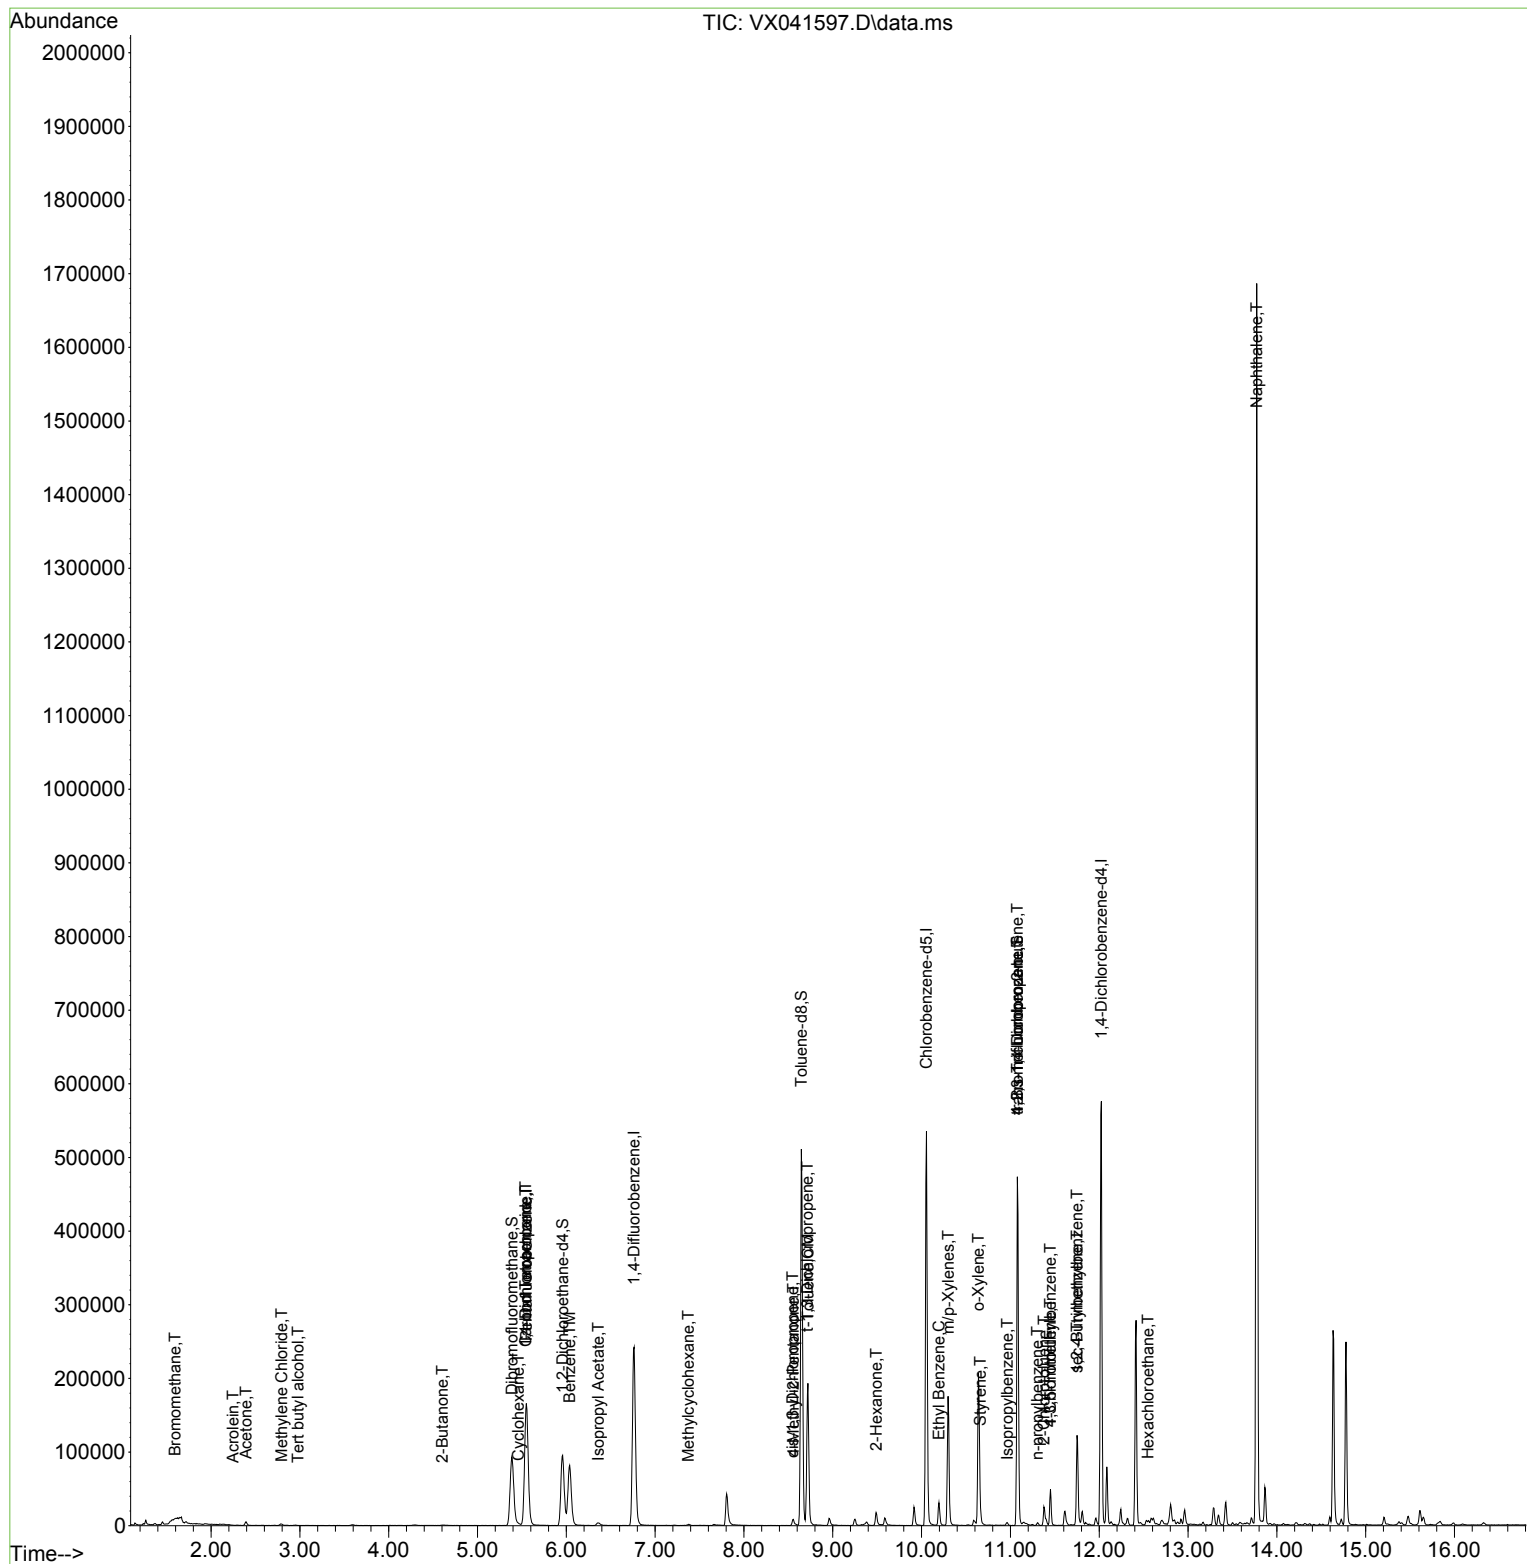




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX041597.D
Acq: 22 May 2024 12:58




Instrument :
MSVOA_X
ClientSampleId :
5


Tgt Ion:168 Resp: 175816
Ion Ratio Lower Upper
168 100
99 48.9 56.6 85.0#

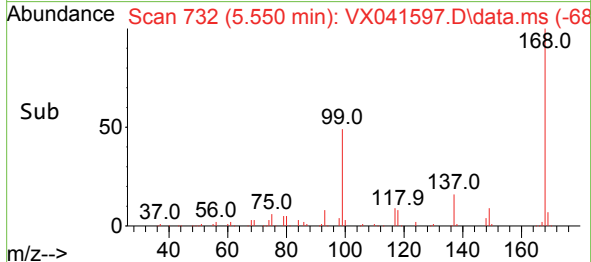

#5
Bromomethane
Concen: 0.326 ug/l
RT: 1.593 min Scan# 83
Delta R.T. -0.006 min
Lab File: VX041597.D
Acq: 22 May 2024 12:58

Tgt Ion: 94 Resp: 291
Ion Ratio Lower Upper
94 100
96 43.5 74.6 111.8#

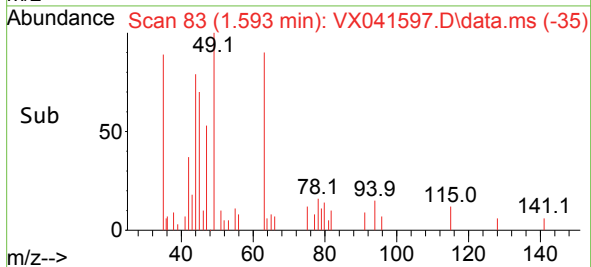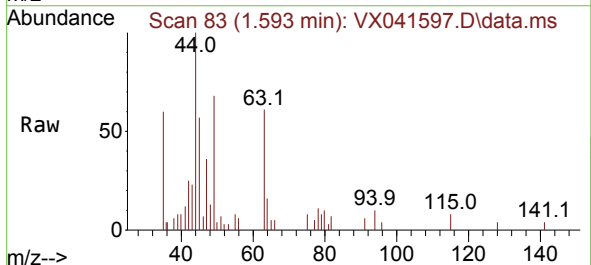

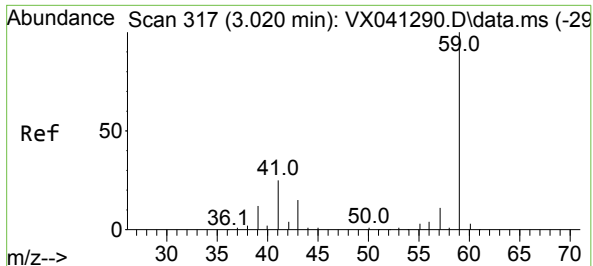

#11

Tert butyl alcohol

Concen: 0.363 ug/l

RT: 2.977 min Scan# 31

Delta R.T. -0.043 min

Lab File: VX041597.D

Acq: 22 May 2024 12:58

Instrument :

MSVOA_X

ClientSampleId :





5

Tgt Ion: 59 Resp: 139

Ion Ratio Lower Upper

59 100

57 0.0 6.0 9.0#

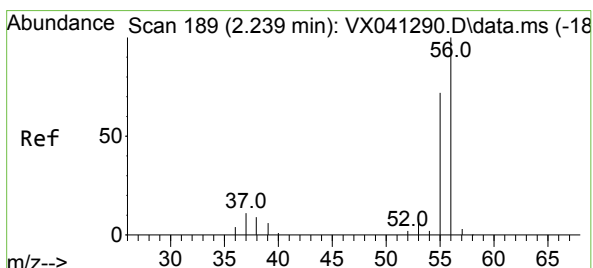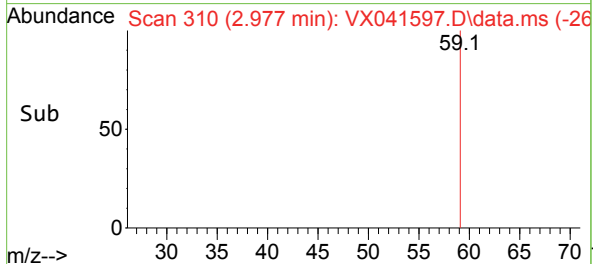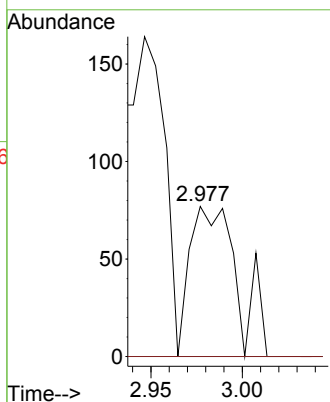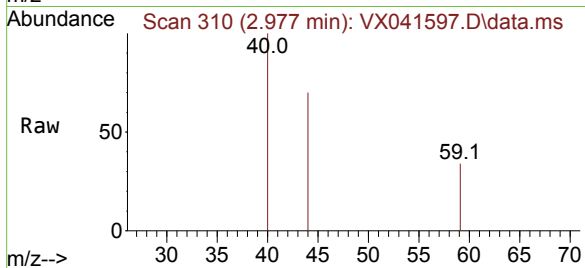

#13

Acrolein

Concen: 0.336 ug/l

RT: 2.245 min Scan# 190

Delta R.T. 0.006 min

Lab File: VX041597.D




Acq: 22 May 2024 12:58


Tgt Ion: 56 Resp: 102

Ion Ratio Lower Upper

56 100

55 62.7 57.1 85.7

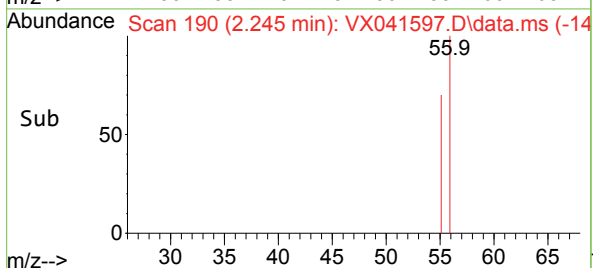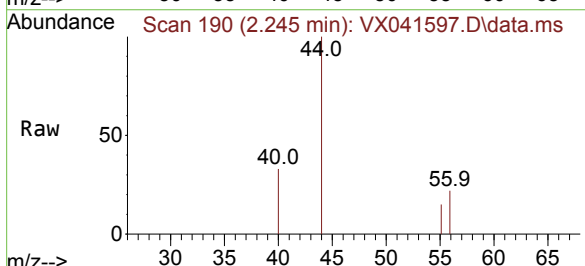



#16

Acetone

Concen: 2.359 ug/l

RT: 2.392 min Scan# 214

Delta R.T. -0.000 min

Lab File: VX041597.D

Acq: 22 May 2024 12:58

Instrument :

MSVOA_X

ClientSampleId :





5

Tgt Ion: 43 Resp: 5254

Ion Ratio Lower Upper

43 100

58 27.7 21.9 32.9

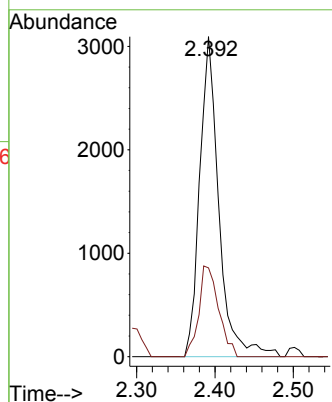

#20

Methylene Chloride

Concen: 0.695 ug/l

RT: 2.794 min Scan# 280

Delta R.T. 0.006 min

Lab File: VX041597.D

Acq: 22 May 2024 12:58

Tgt Ion: 84 Resp: 1154




Ion Ratio Lower Upper


84 100

49 86.0 103.6 155.4#

51 31.0 33.8 50.6#

86 42.0 49.4 74.0#

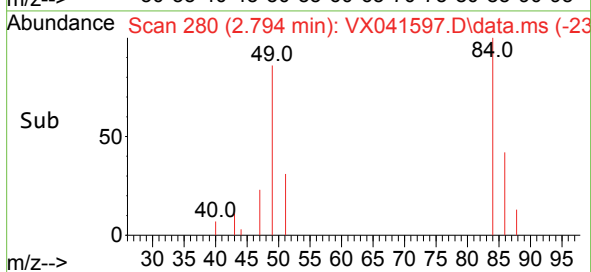

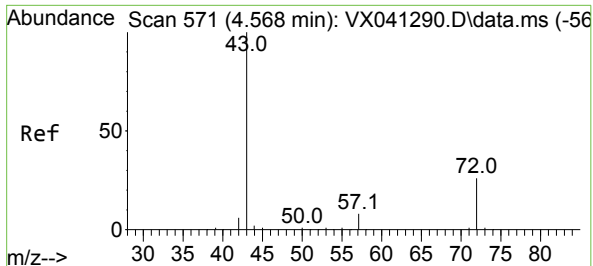

#25

2-Butanone

Concen: 0.260 ug/l

RT: 4.605 min Scan# 51

Delta R.T. 0.037 min

Lab File: VX041597.D

Acq: 22 May 2024 12:58

Instrument :

MSVOA_X

ClientSampleId :





5

Tgt Ion: 43 Resp: 322

Ion Ratio Lower Upper

43 100

72 0.0 19.4 29.2#

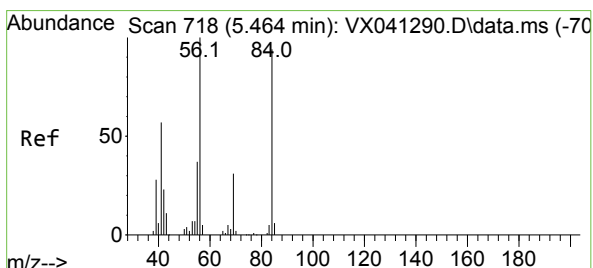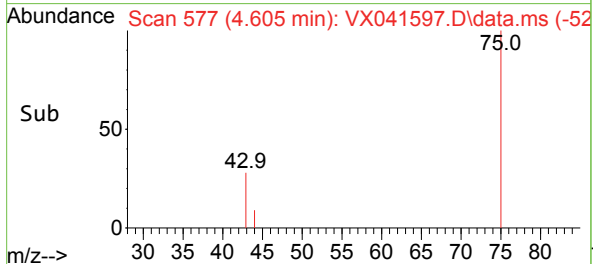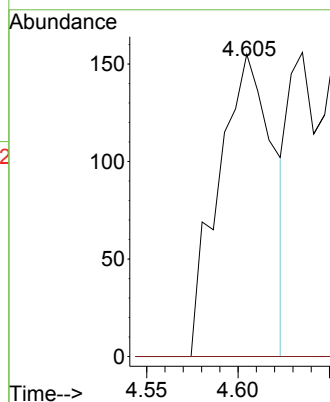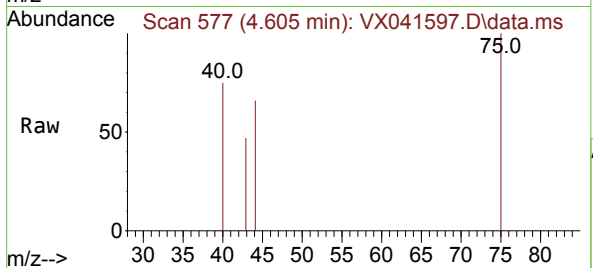

#31

Cyclohexane

Concen: 0.293 ug/l

RT: 5.458 min Scan# 717

Delta R.T. -0.006 min

Lab File: VX041597.D

Acq: 22 May 2024 12:58




Tgt Ion: 56 Resp: 676


Ion Ratio Lower Upper

56 100

69 26.5 23.4 35.2

84 68.7 65.9 98.9

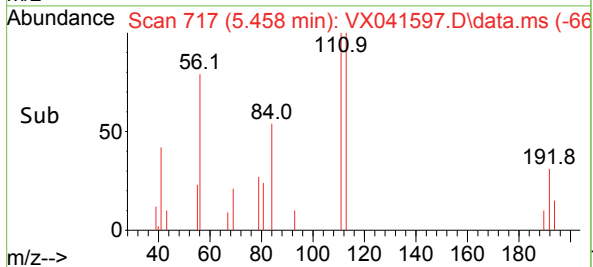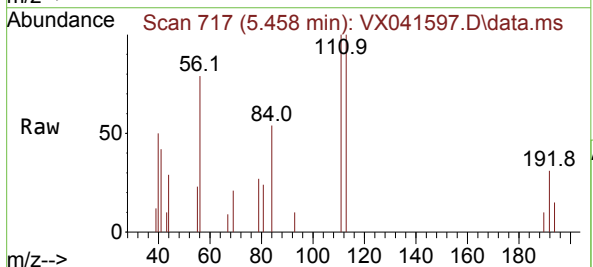



#33

1,2-Dichloroethane-d4

Concen: 49.852 ug/l

RT: 5.958 min Scan# 798

Delta R.T. 0.006 min

Lab File: VX041597.D

Acq: 22 May 2024 12:58

Instrument :

MSVOA_X

ClientSampleId :





5

Tgt Ion: 65 Resp: 95417

Ion Ratio Lower Upper

65 100

67 50.9 0.0 100.2

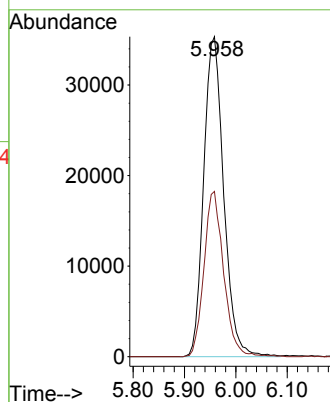

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.006 min

Lab File: VX041597.D

Acq: 22 May 2024 12:58




Tgt Ion: 114 Resp: 259251


Ion Ratio Lower Upper

114 100

63 19.3 0.0 45.0

88 15.3 0.0 36.6







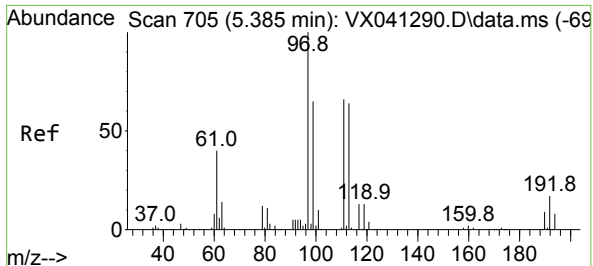

#35
Dibromofluoromethane
Concen: 45.764 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX041597.D
Acq: 22 May 2024 12:58




Instrument :
MSVOA_X
ClientSampleId :
5


Tgt Ion:113 Resp: 80402
Ion Ratio Lower Upper
113 100
111 100.9 82.9 124.3
192 24.9 13.3 19.9#

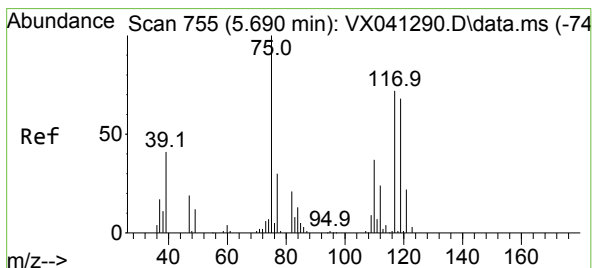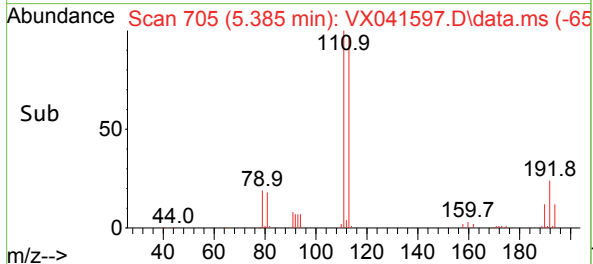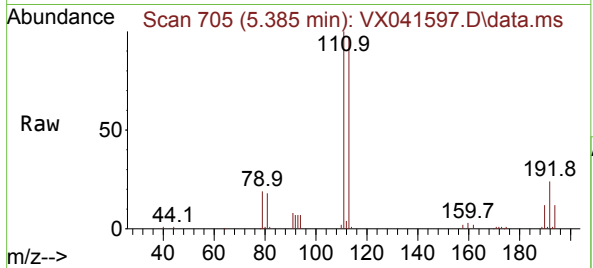

#36
1,1-Dichloropropene
Concen: 5.243 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.146 min
Lab File: VX041597.D
Acq: 22 May 2024 12:58


Tgt Ion: 75 Resp: 11014
Ion Ratio Lower Upper
75 100
110 9.3 17.0 50.9#
77 0.0 24.7 37.1#

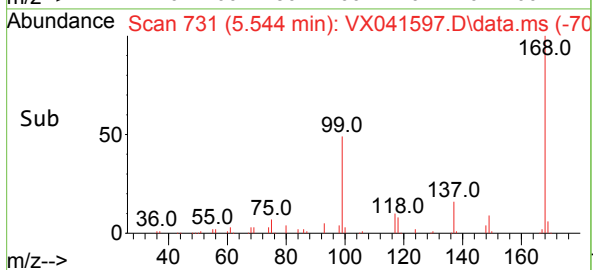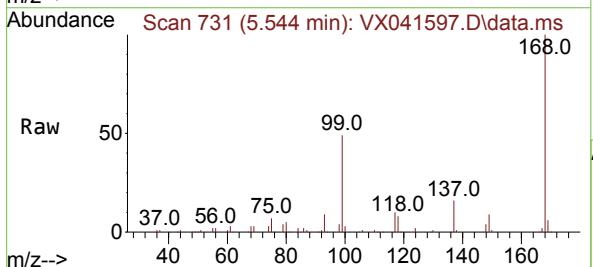






#38
Carbon Tetrachloride
Concen: 6.446 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX041597.D
Acq: 22 May 2024 12:58


Instrument :
MSVOA_X
ClientSampleId :
5





Tgt Ion:117 Resp: 15514
Ion Ratio Lower Upper
117 100
119 4.5 78.2 117.2#
121 0.0 24.4 36.6#




#39
Methylcyclohexane
Concen: 0.285 ug/l
RT: 7.373 min Scan# 1031
Delta R.T. -0.000 min
Lab File: VX041597.D
Acq: 22 May 2024 12:58

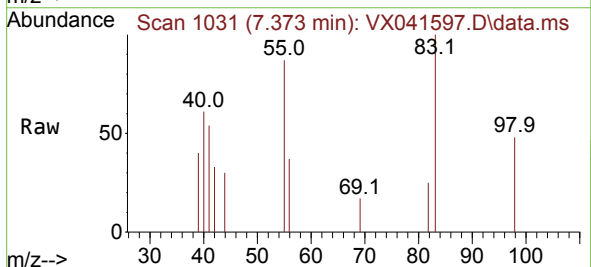

Tgt Ion: 83 Resp: 704
Ion Ratio Lower Upper
83 100
55 86.6 64.6 97.0
98 48.0 36.7 55.1

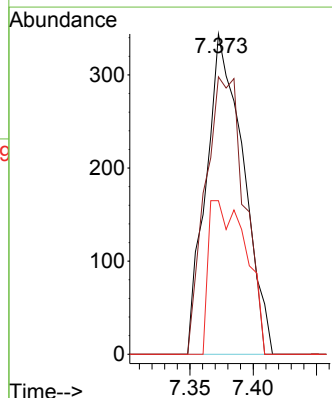

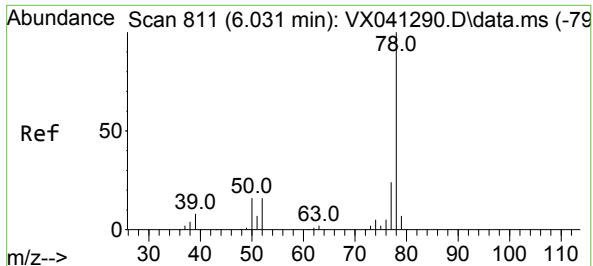

#40

Benzene

Concen: 15.379 ug/l

RT: 6.037 min Scan# 811

Delta R.T. 0.006 min

Lab File: VX041597.D

Acq: 22 May 2024 12:58

Instrument :

MSVOA_X

ClientSampleId :





5

Tgt Ion: 78 Resp: 99598

Ion Ratio Lower Upper

78 100

77 23.7 19.3 28.9

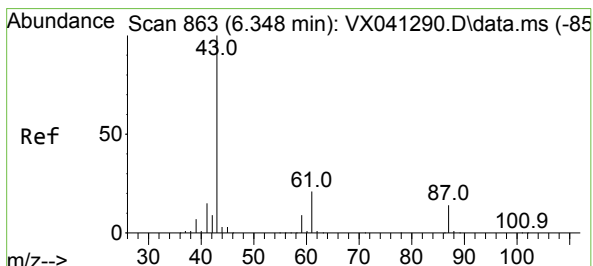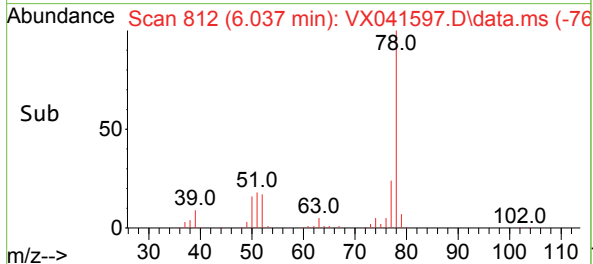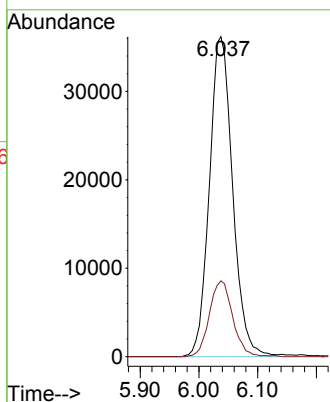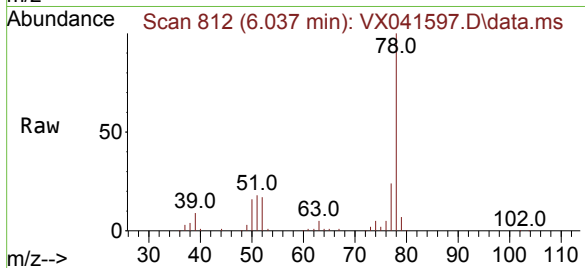

#43

Isopropyl Acetate

Concen: 1.424 ug/l

RT: 6.361 min Scan# 865

Delta R.T. 0.012 min

Lab File: VX041597.D

Acq: 22 May 2024 12:58




Tgt Ion: 43 Resp: 5612


Ion Ratio Lower Upper

43 100

61 15.5 15.2 22.8

87 10.2 9.8 14.6


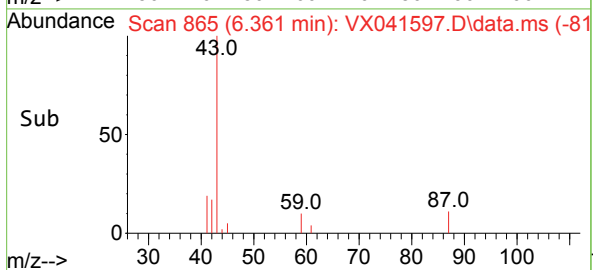

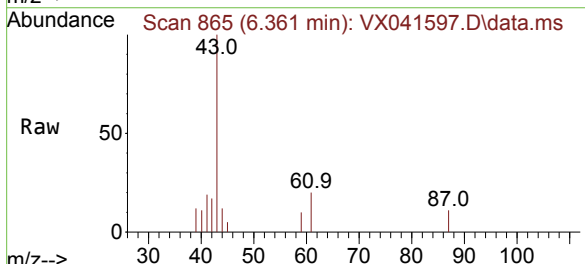




#50
Toluene-d8
Concen: 53.688 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX041597.D
Acq: 22 May 2024 12:58




Instrument :
MSVOA_X
ClientSampleId :
5


Tgt Ion: 98 Resp: 298539
Ion Ratio Lower Upper
98 100
100 66.5 53.1 79.7

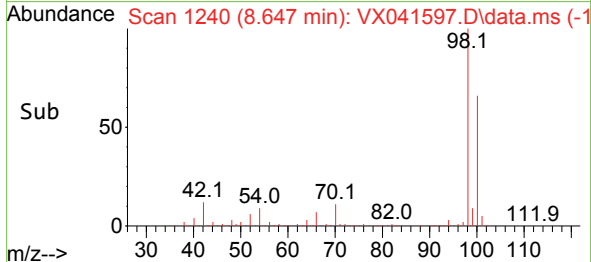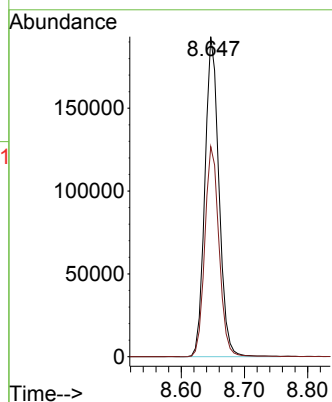

#51
4-Methyl-2-Pentanone
Concen: 1.614 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. -0.024 min
Lab File: VX041597.D
Acq: 22 May 2024 12:58

Tgt Ion: 43 Resp: 3818
Ion Ratio Lower Upper
43 100
58 2.8 30.4 45.6#


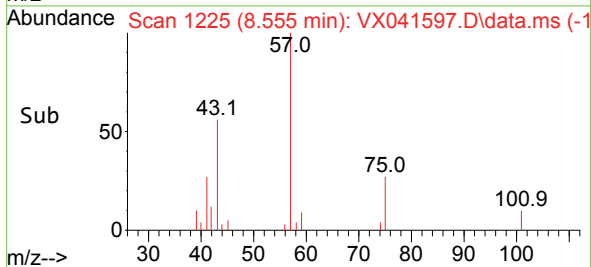

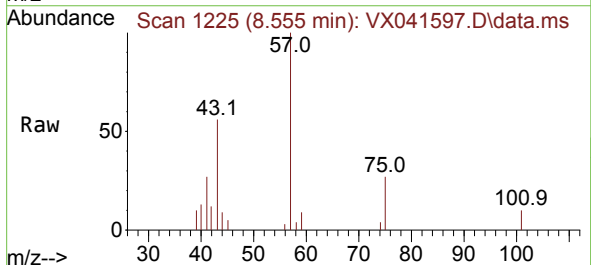




#52
Toluene
Concen: 18.773 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX041597.D
Acq: 22 May 2024 12:58




Instrument :
MSVOA_X
ClientSampleId :
5


Tgt Ion: 92 Resp: 74372
Ion Ratio Lower Upper
92 100
91 173.0 134.2 201.2

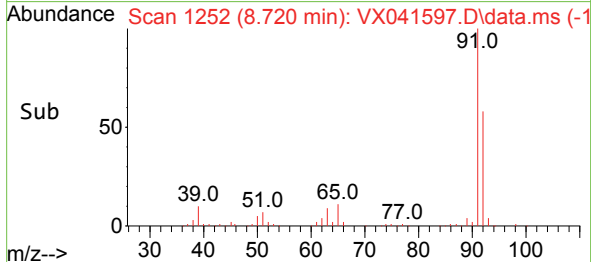

#53
t-1,3-Dichloropropene
Concen: 2.790 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. -0.262 min
Lab File: VX041597.D
Acq: 22 May 2024 12:58

Tgt Ion: 75 Resp: 875
Ion Ratio Lower Upper
75 100
77 153.6 25.7 38.5#


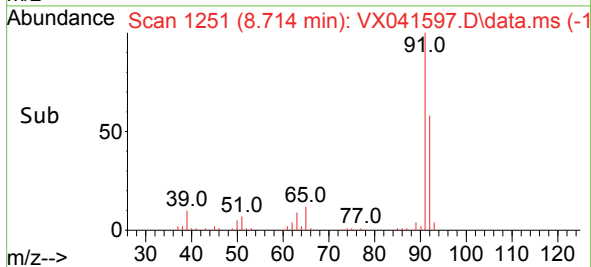

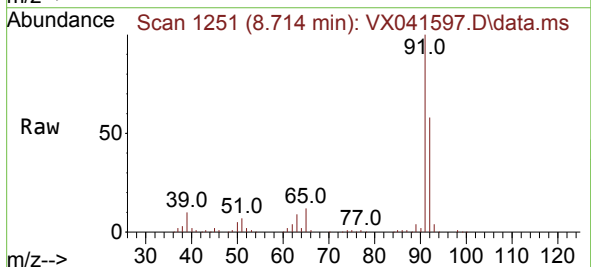




#54
 cis-1,3-Dichloropropene
 Concen: 0.623 ug/l
 RT: 8.549 min Scan# 1194
 Delta R.T. 0.183 min
 Lab File: VX041597.D
 Acq: 22 May 2024 12:58




Instrument :
 MSVOA_X
 ClientSampleId :
 5


Tgt Ion: 75 Resp: 1406
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.3 37.9#
 39 31.3 46.7 70.1#



#59
 2-Hexanone
 Concen: 1.326 ug/l
 RT: 9.488 min Scan# 1378
 Delta R.T. 0.055 min
 Lab File: VX041597.D
 Acq: 22 May 2024 12:58

Tgt Ion: 43 Resp: 2508
 Ion Ratio Lower Upper
 43 100
 58 20.5 26.2 78.5#


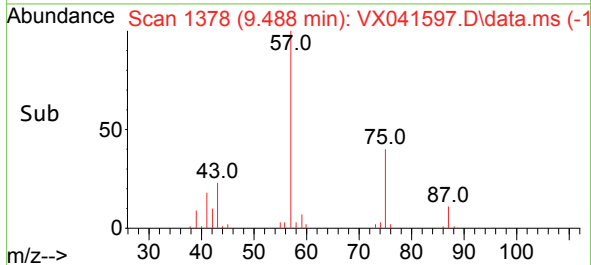

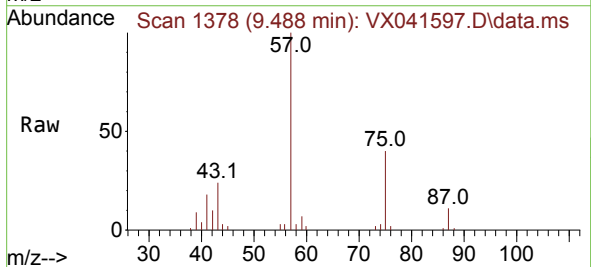




#62
4-Bromofluorobenzene
Concen: 53.802 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX041597.D
Acq: 22 May 2024 12:58




Instrument :
MSVOA_X
ClientSampleId :
5


Tgt Ion: 95 Resp: 115813
Ion Ratio Lower Upper
95 100
174 96.7 0.0 135.6
176 95.7 0.0 131.0

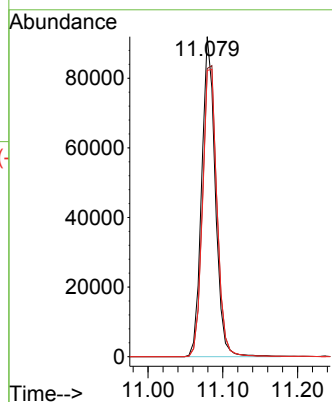

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX041597.D
Acq: 22 May 2024 12:58

Tgt Ion: 117 Resp: 248276
Ion Ratio Lower Upper
117 100
82 52.1 46.2 69.4
119 32.2 25.5 38.3

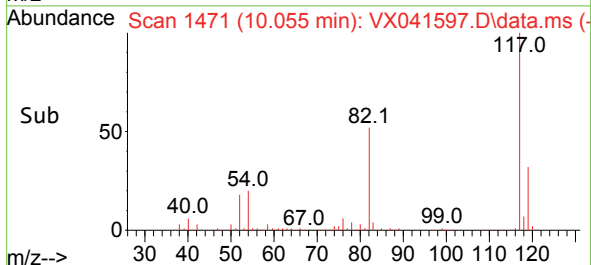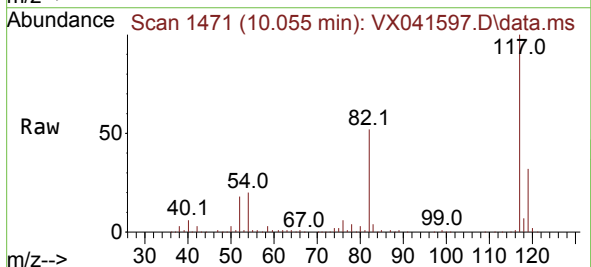



#67

Ethyl Benzene

Concen: 2.239 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. -0.000 min

Lab File: VX041597.D

Acq: 22 May 2024 12:58

Instrument :

MSVOA_X

ClientSampleId :





5

Tgt Ion: 91 Resp: 18615

Ion Ratio Lower Upper

91 100

106 29.1 24.9 37.3



#68

m/p-Xylenes

Concen: 12.134 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. -0.000 min

Lab File: VX041597.D




Acq: 22 May 2024 12:58


Tgt Ion: 106 Resp: 40406

Ion Ratio Lower Upper

106 100

91 203.2 165.5 248.3

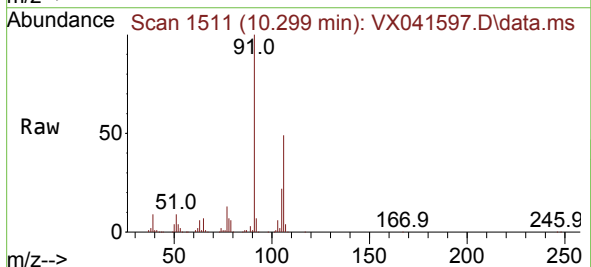



#69

o-Xylene

Concen: 14.043 ug/l

RT: 10.640 min Scan# 1567

Delta R.T. -0.000 min

Lab File: VX041597.D

Acq: 22 May 2024 12:58

Instrument :

MSVOA_X

ClientSampleId :





5

Tgt Ion:106 Resp: 44773

Ion Ratio Lower Upper

106 100

91 206.5 108.9 326.8



#70

Styrene

Concen: 2.085 ug/l

RT: 10.659 min Scan# 1570

Delta R.T. 0.006 min

Lab File: VX041597.D

Acq: 22 May 2024 12:58




Tgt Ion:104 Resp: 10906


Ion Ratio Lower Upper

104 100

78 92.6 43.6 65.4#

103 89.4 43.6 65.4#


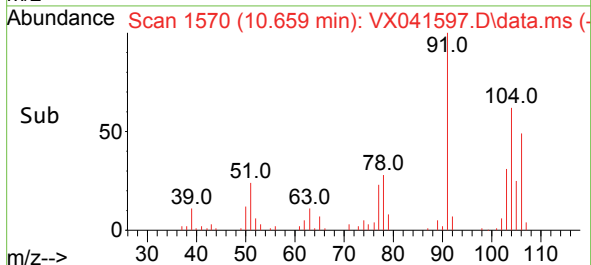
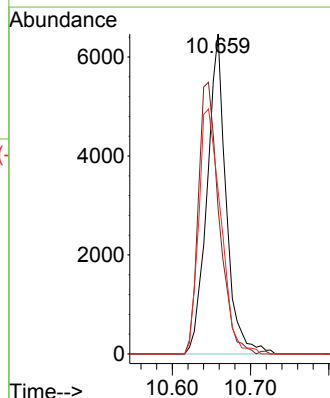
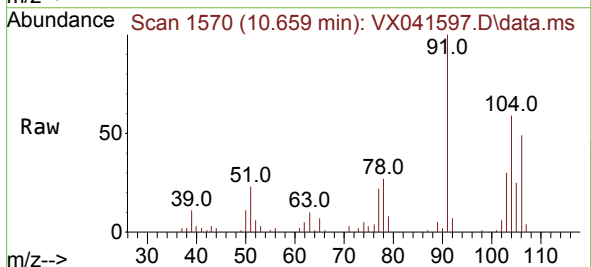




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX041597.D
 Acq: 22 May 2024 12:58




Instrument :
 MSVOA_X
 ClientSampleId :
 5


Tgt Ion:152 Resp: 134052
 Ion Ratio Lower Upper
 152 100
 115 53.5 43.3 129.9
 150 154.7 0.0 345.0

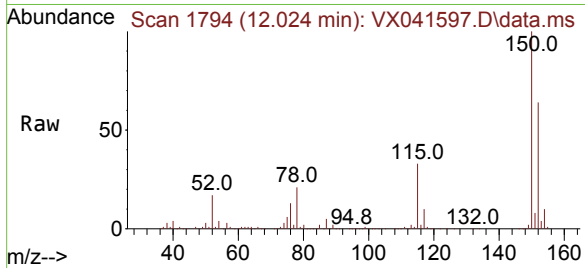

#73
 Isopropylbenzene
 Concen: 0.255 ug/l
 RT: 10.963 min Scan# 1620
 Delta R.T. -0.000 min
 Lab File: VX041597.D
 Acq: 22 May 2024 12:58

Tgt Ion:105 Resp: 2090
 Ion Ratio Lower Upper
 105 100
 120 30.4 12.9 38.6

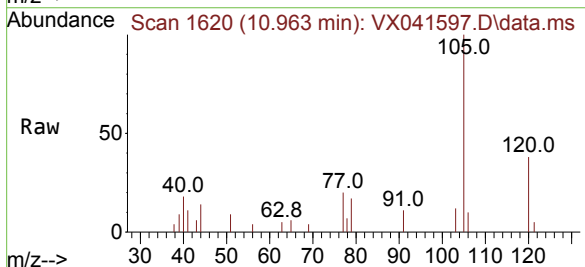



#76

1,2,3-Trichloropropane

Concen: 27.053 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.159 min

Lab File: VX041597.D

Acq: 22 May 2024 12:58

Instrument :

MSVOA_X

ClientSampleId :





5

Tgt Ion: 75 Resp: 59101

Ion Ratio Lower Upper

75 100

77 1.2 19.1 57.5#

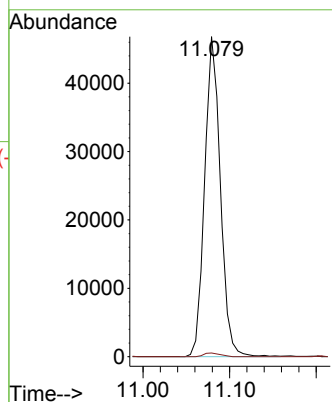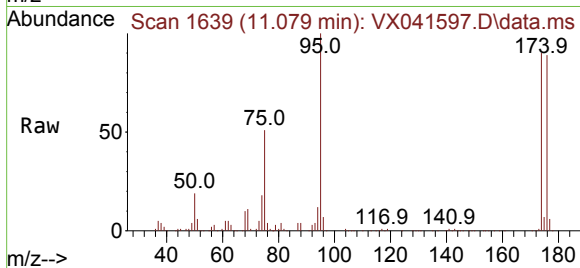

#78

n-propylbenzene

Concen: 0.311 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.000 min

Lab File: VX041597.D




Acq: 22 May 2024 12:58


Tgt Ion: 91 Resp: 2676

Ion Ratio Lower Upper

91 100

120 24.1 11.5 34.4

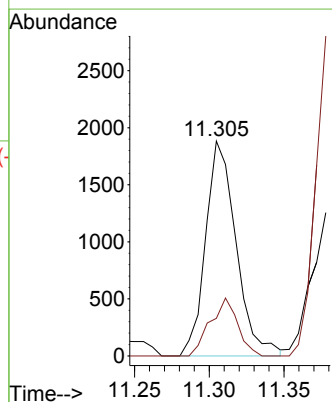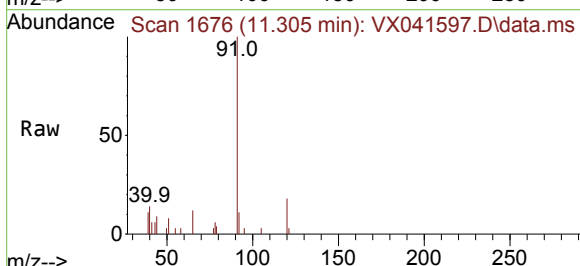



#79

2-Chlorotoluene

Concen: 0.425 ug/l

RT: 11.378 min Scan# 1

Delta R.T. 0.012 min

Lab File: VX041597.D

Acq: 22 May 2024 12:58

Instrument :

MSVOA_X

ClientSampleId :





5

Tgt Ion: 91 Resp: 2353

Ion Ratio Lower Upper

91 100

126 0.0 16.3 48.8#

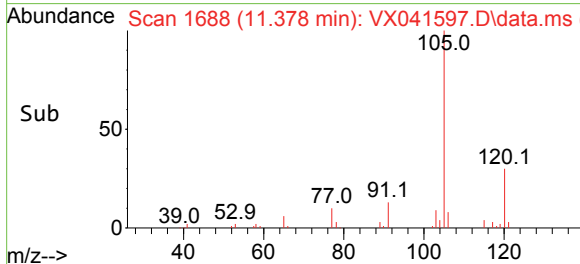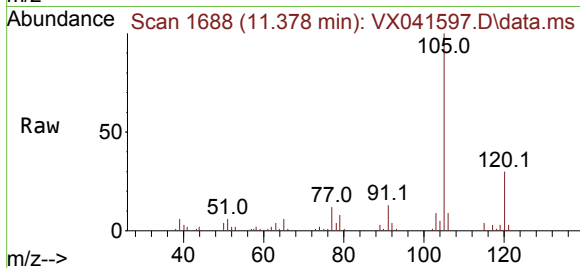

#80

1,3,5-Trimethylbenzene

Concen: 3.023 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. -0.000 min

Lab File: VX041597.D




Acq: 22 May 2024 12:58


Tgt Ion: 105 Resp: 20168

Ion Ratio Lower Upper

105 100

120 53.1 24.1 72.3


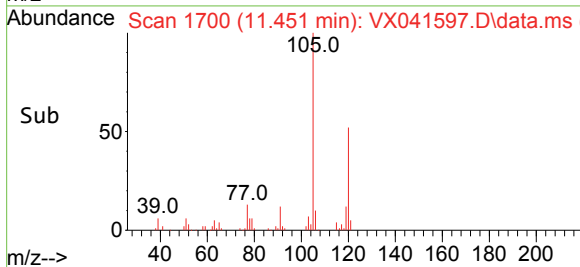

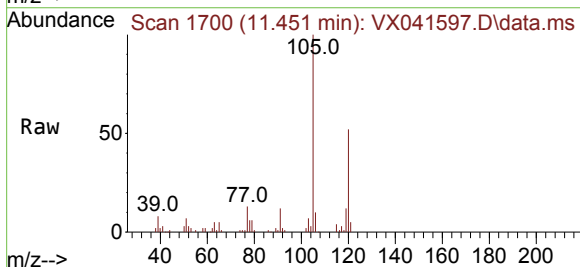




#81
trans-1,4-Dichloro-2-butene
Concen: 73.689 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX041597.D
Acq: 22 May 2024 12:58




Instrument :
MSVOA_X
ClientSampleId :
5


Tgt Ion: 75 Resp: 59101
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

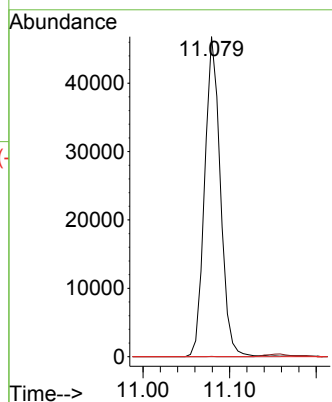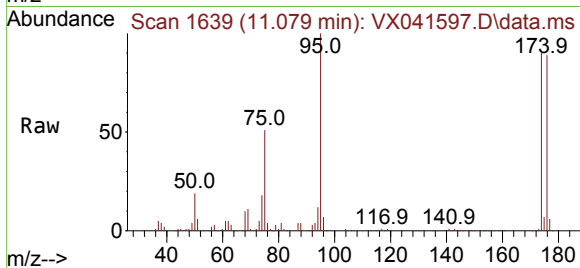

#82
4-Chlorotoluene
Concen: 0.392 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX041597.D
Acq: 22 May 2024 12:58

Tgt Ion: 91 Resp: 2463
Ion Ratio Lower Upper
91 100
126 0.0 14.2 42.6#

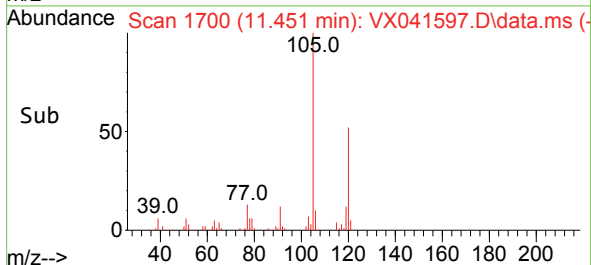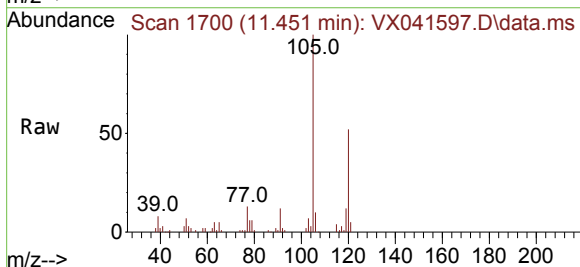



#84

1,2,4-Trimethylbenzene

Concen: 7.970 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX041597.D

Acq: 22 May 2024 12:58

Instrument :

MSVOA_X

ClientSampleId :





5

Tgt Ion:105 Resp: 53497

Ion Ratio Lower Upper

105 100

120 39.4 21.2 63.6

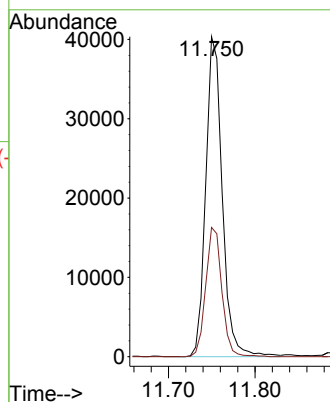

#85

sec-Butylbenzene

Concen: 6.535 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.140 min

Lab File: VX041597.D




Acq: 22 May 2024 12:58


Tgt Ion:105 Resp: 53497

Ion Ratio Lower Upper

105 100

134 0.0 9.8 29.4#




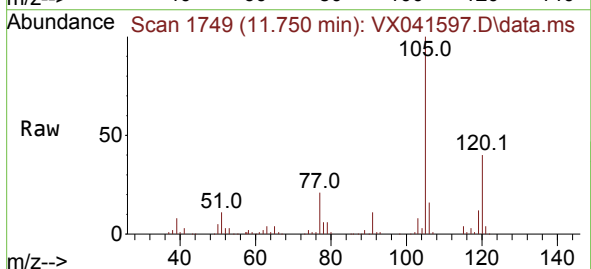




#90
Hexachloroethane
Concen: 0.713 ug/l
RT: 12.548 min Scan# 117
Delta R.T. 0.012 min
Lab File: VX041597.D
Acq: 22 May 2024 12:58

Instrument :
MSVOA_X
ClientSampleId :
5

Tgt Ion:117 Resp: 877
Ion Ratio Lower Upper
117 100
201 0.0 32.9 98.6#

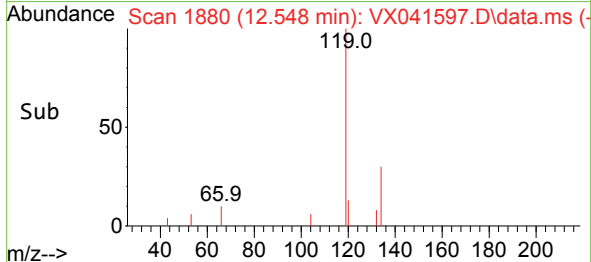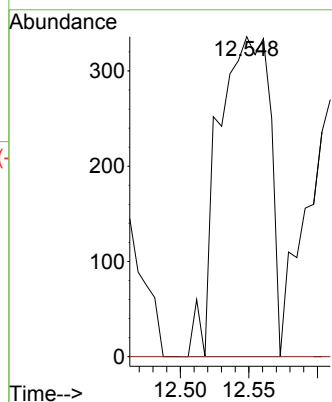

#95
Naphthalene
Concen: 109.045 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX041597.D
Acq: 22 May 2024 12:58

Tgt Ion:128 Resp: 1001535
Ion Ratio Lower Upper
128 100
127 13.2 10.3 15.5
129 11.2 8.8 13.2

