

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX052319\
 Data File : VX009870.D
 Acq On : 23 May 2019 19:48
 Operator : JC/SP
 Sample : K3000-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S36-0157

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.410	38	42	48	rVB	19794	23737	2.43%	0.442%
2	1.611	66	75	79	rBV10	5824	13885	1.42%	0.258%
3	2.446	207	212	223	rVB	6567	14126	1.45%	0.263%
4	2.611	232	239	246	rBV	21308	39385	4.04%	0.733%
5	3.166	323	330	343	rBV	23094	49442	5.07%	0.920%
6	4.598	554	565	574	rBV4	4190	13317	1.37%	0.248%
7	5.501	698	713	724	rBV2	99550	287909	29.52%	5.359%
8	5.659	729	739	757	rVB	182031	519989	53.32%	9.679%
9	6.062	792	805	814	rBV	128903	336909	34.54%	6.271%
10	6.147	814	819	832	rVB2	15269	42552	4.36%	0.792%
11	6.860	926	936	950	rBV	294283	698420	71.61%	13.000%
12	8.714	1233	1240	1248	rVV	634251	975306	100.00%	18.154%
13	8.781	1248	1251	1260	rVV3	8641	15242	1.56%	0.284%
14	8.872	1260	1266	1272	rVB	7972	13066	1.34%	0.243%
15	10.110	1457	1469	1481	rBV2	612417	943503	96.74%	17.562%
16	10.250	1488	1492	1498	rBV2	8285	13737	1.41%	0.256%
17	10.360	1504	1510	1515	rBV	11386	17048	1.75%	0.317%
18	10.695	1561	1565	1570	rBV	10144	15213	1.56%	0.283%
19	11.134	1631	1637	1644	rBV	476888	613799	62.93%	11.425%
20	12.073	1786	1791	1800	rBV	542684	714888	73.30%	13.307%
21	15.633	2366	2375	2380	rBV3	5737	10875	1.12%	0.202%


Sum of corrected areas: 5372348

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX052319\
Data File : VX009870.D
Acq On : 23 May 2019 19:48
Operator : JC/SP
Sample : K3000-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S36-0157

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

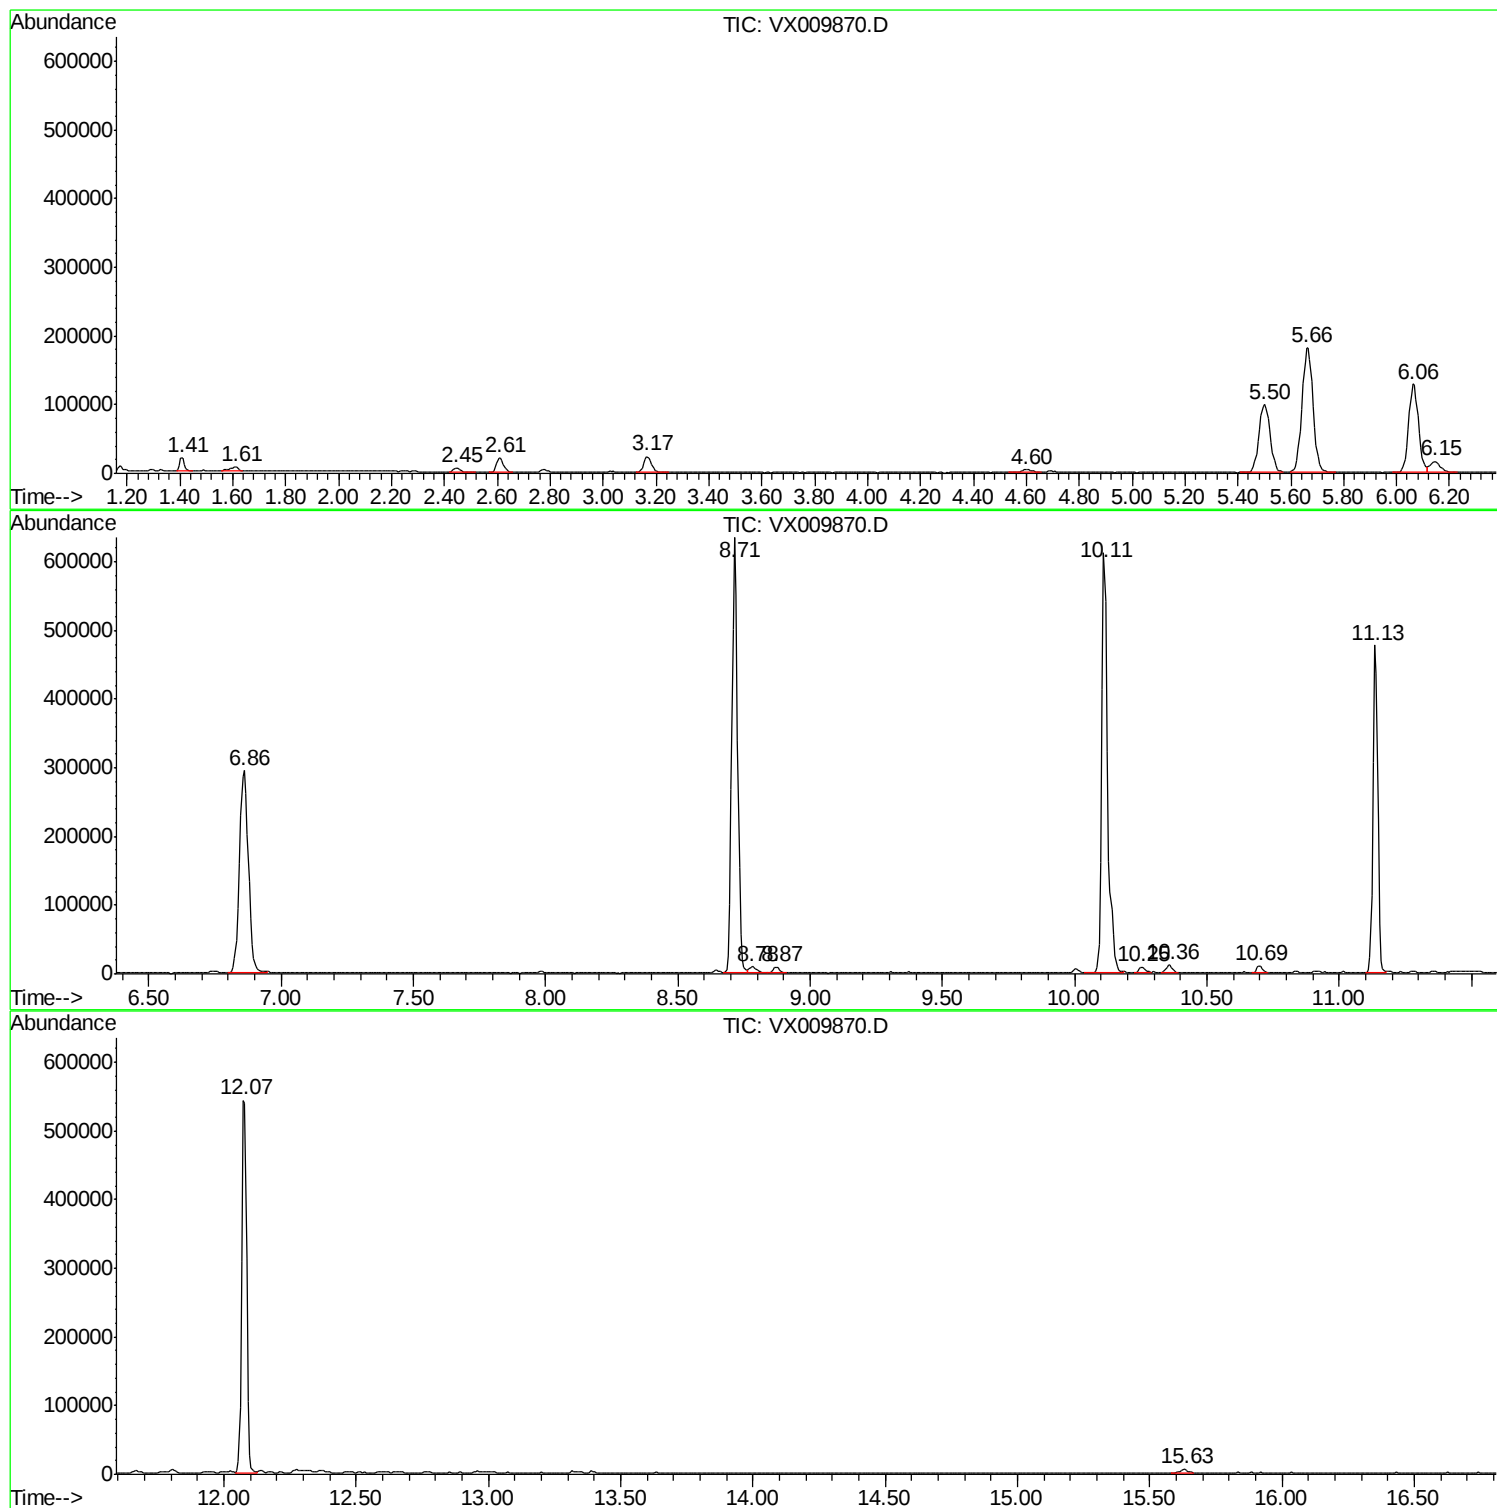

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX052319\
Data File : VX009870.D
Acq On : 23 May 2019 19:48
Operator : JC/SP
Sample : K3000-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S36-0157

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX052319\
Data File : VX009870.D
Acq On : 23 May 2019 19:48
Operator : JC/SP
Sample : K3000-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S36-0157

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc