
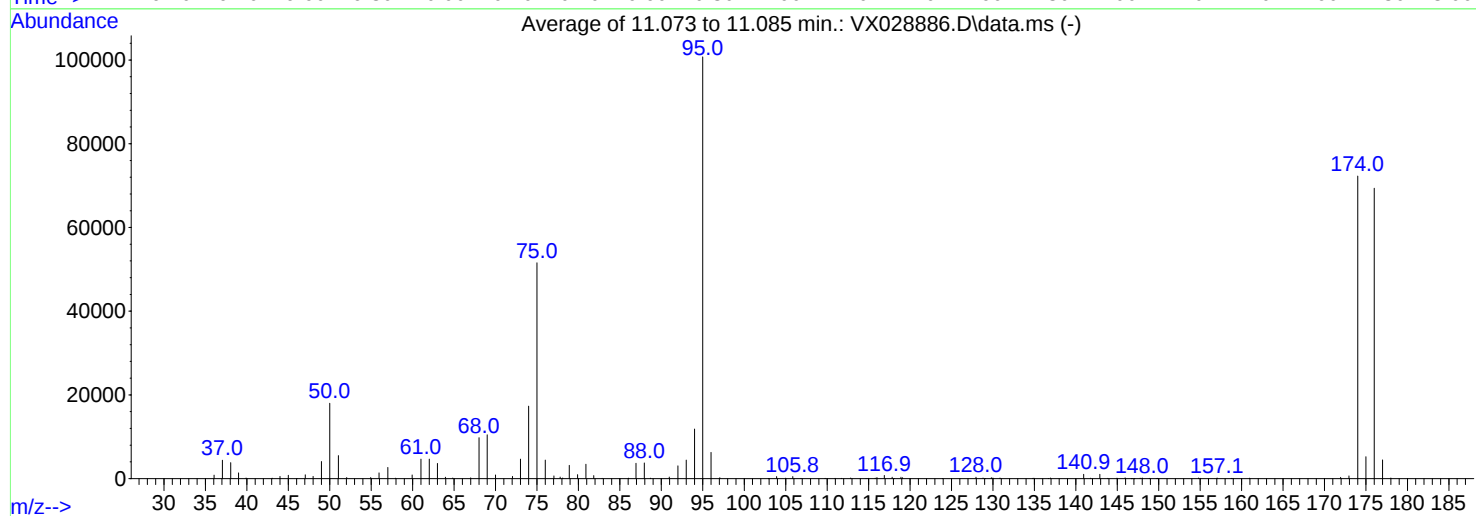


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052322\
 Data File : VX028886.D
 Acq On : 23 May 2022 09:33
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Title : SW846 8260
 Last Update : Thu May 12 14:58:53 2022

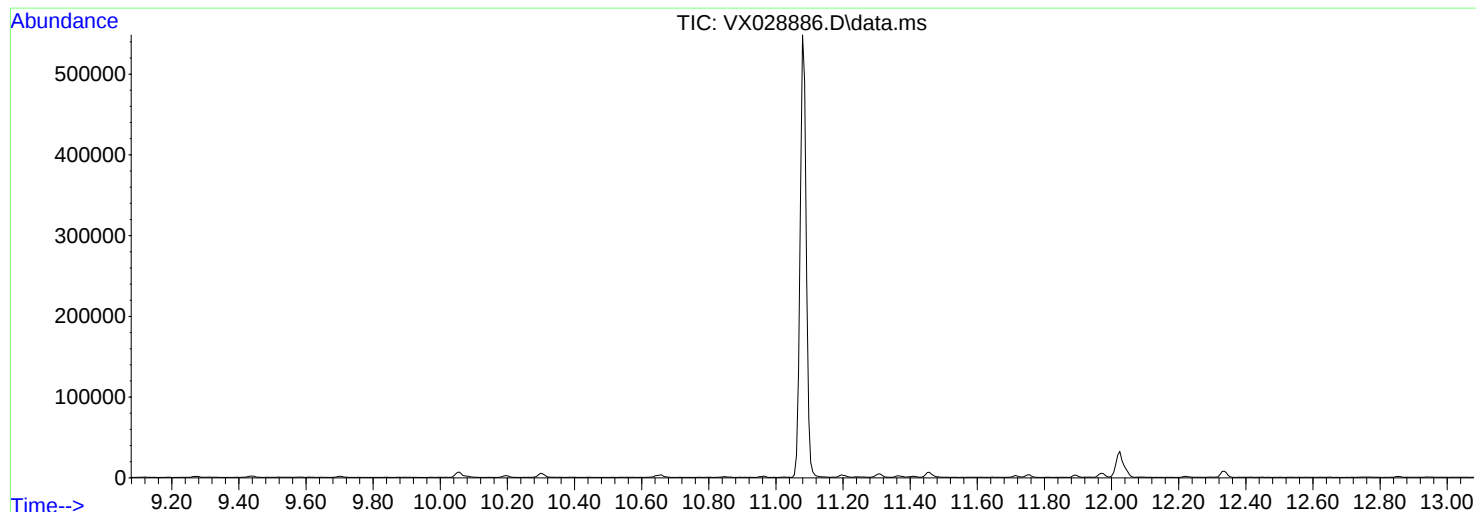

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	18020	PASS
75	95	30	60	51.2	51555	PASS
95	95	100	100	100.0	100757	PASS
96	95	5	9	6.2	6278	PASS
173	174	0.00	2	0.9	654	PASS
174	95	50	100	71.7	72256	PASS
175	174	5	9	7.2	5236	PASS
176	174	95	101	96.0	69371	PASS
177	176	5	9	6.5	4484	PASS