

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052323\
 Data File : VX035818.D
 Acq On : 23 May 2023 16:52
 Operator : JC/MD
 Sample : 02830-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SEMI-ANNUAL-CONDENSATE

Quant Time: May 24 05:50:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X052323W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Tue May 23 11:36:37 2023
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :John Carlone 05/25/2023
 Supervised By :Mahesh Dadoda 05/25/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	4.898	128	33368	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	6.763	114	196150	30.000	ug/l	0.00
57) Chlorobenzene-d5	10.055	117	177002	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	5.958	65	86470	31.188	ug/l	0.00
Spiked Amount 30.000	Range 91 - 110		Recovery = 103.967%			
60) 4-Bromofluorobenzene	11.079	95	92643	31.192	ug/l	0.00
Spiked Amount 30.000	Range 63 - 112		Recovery = 103.967%			
63) Toluene-d8	8.647	98	238729	30.509	ug/l	0.00
Spiked Amount 30.000	Range 91 - 112		Recovery = 101.700%			
Target Compounds						
					Qvalue	
8) Diethyl Ether	2.130	74	7646	6.167	ug/l	98
15) Acetone	2.398	58	906842	2558.847	ug/l	98
16) Carbon Disulfide	2.514	76	2316	0.638	ug/l #	94
22) cis-1,2-Dichloroethene	4.489	96	1740	0.746	ug/l #	60
23) tert-Butyl Alcohol	3.014	59	3256570	7529.720	ug/l #	100
30) 2-Butanone	4.574	43	5963341	3335.109	ug/l	99
34) Benzene	6.038	78	270396	31.380	ug/l	98
45) 1,4-Dioxane	7.714	88	81984	1552.887	ug/l	94
58) 4-Methyl-2-Pentanone	8.574	43	245987	71.549	ug/l	99
59) 2-Hexanone	9.433	43	102376	39.574	ug/l	95
62) Toluene	8.720	91	910607	99.900	ug/l	99
64) Chlorobenzene	10.080	112	62999	10.913	ug/l	90
66) Ethyl Benzene	10.195	91	520492	51.058	ug/l	98
67) m/p-Xylenes	10.299	106	200076	51.852	ug/l	99
68) o-Xylene	10.640	106	110748	28.694	ug/l	100
70) Isopropylbenzene	10.964	105	67107	6.812	ug/l	100
74) n-propylbenzene	11.305	91	53518	4.557	ug/l	99
76) 1,3,5-Trimethylbenzene	11.451	105	107559	12.855	ug/l	100
80) 1,2,4-Trimethylbenzene	11.750	105	390423	46.431	ug/l	98
81) sec-Butylbenzene	11.890	105	20470m	2.007	ug/l	
82) p-Isopropyltoluene	12.012	119	2156506	254.176	ug/l	98
83) 1,3-Dichlorobenzene	11.969	146	3777	0.834	ug/l	84
84) 1,4-Dichlorobenzene	12.043	146	364873	80.250	ug/l	100
85) n-Butylbenzene	12.323	91	29623m	3.925	ug/l	
87) 1,2-Dichlorobenzene	12.335	146	15173	3.419	ug/l	94
89) 1,2,4-Trichlorobenzene	13.591	180	3949	1.485	ug/l #	81
91) Naphthalene	13.780	128	2859969	310.708	ug/l	99
92) 1,2,3-Trichlorobenzene	13.963	180	2171	0.817	ug/l #	68

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052323\
Data File : VX035818.D
Acq On : 23 May 2023 16:52
Operator : JC/MD
Sample : 02830-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
SEMI-ANNUAL-CONDENSATE

Quant Time: May 24 05:50:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X052323W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Tue May 23 11:36:37 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : John Carlone 05/25/2023
Supervised By : Mahesh Dadoda 05/25/2023

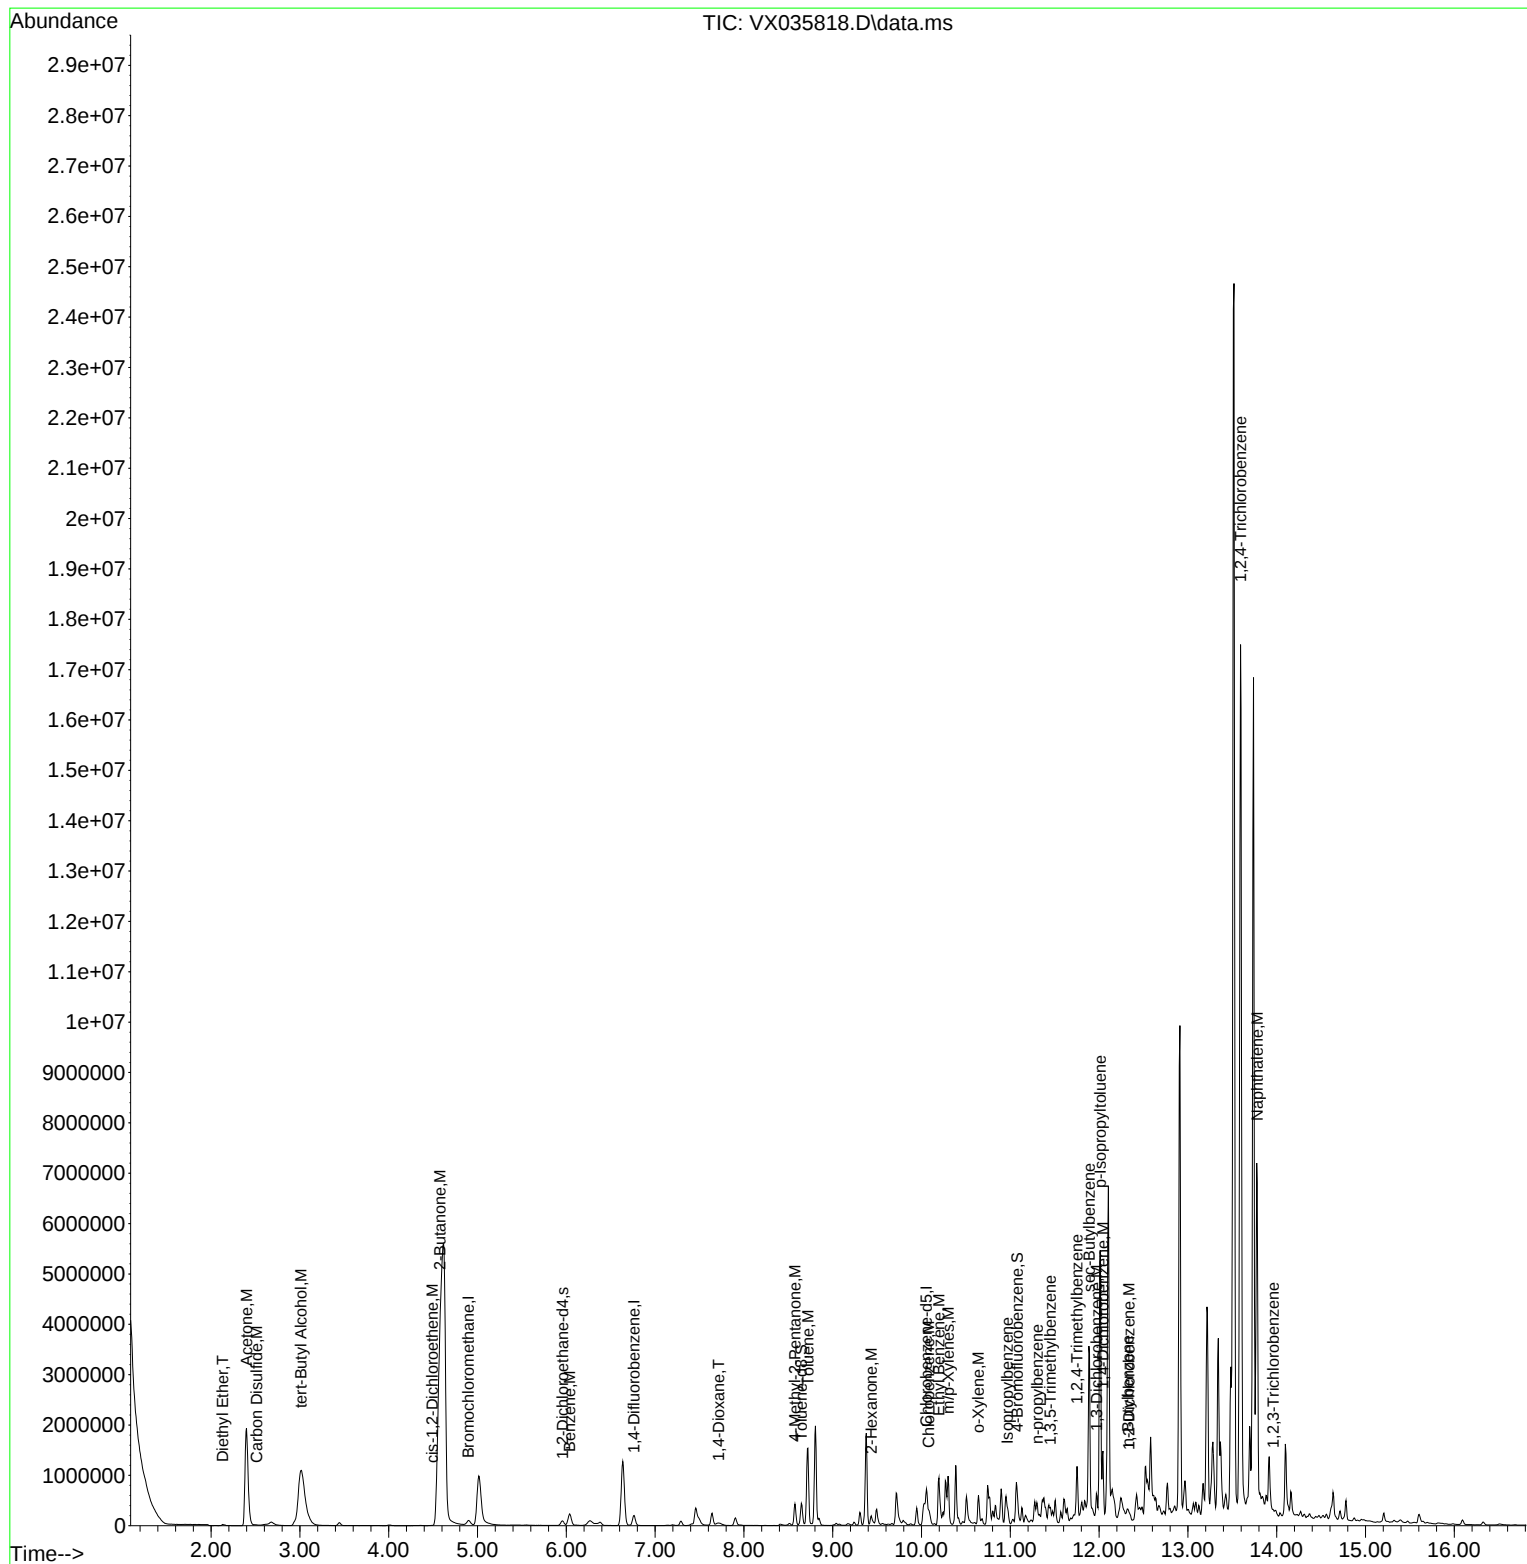



#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 4.898 min Scan# 61
Delta R.T. 0.007 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52




Instrument :
MSVOA_X
ClientSampleId :
SEMI-ANNUAL-CONDENSATE



Tgt Ion:128 Resp: 3336
Ion Ratio Lower Upper
128 100
49 180.7 0.0 428.8
130 126.0 0.0 310.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2023
Supervised By :Mahesh Dadoda 05/25/2023

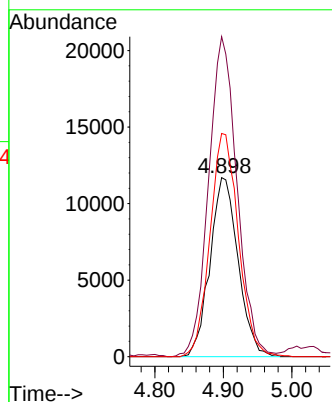

#8
Diethyl Ether
Concen: 6.167 ug/l
RT: 2.130 min Scan# 171
Delta R.T. -0.006 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52

Tgt Ion: 74 Resp: 7646
Ion Ratio Lower Upper
74 100
45 104.3 20.5 184.5

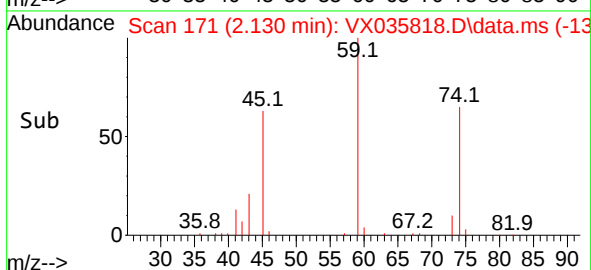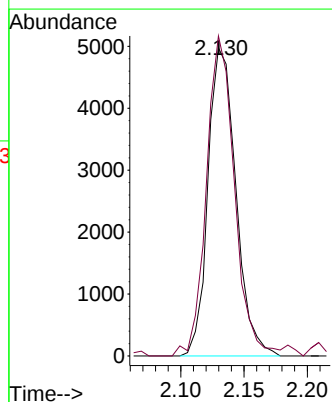



#15

Acetone

Concen: 2558.847 ug/l

RT: 2.398 min Scan# 216

Delta R.T. -0.006 min

Lab File: VX035818.D

Acq: 23 May 2023 16:52

Instrument :

MSVOA_X

ClientSampleId :

SEMI-ANNUAL-CONDENSATE

Tgt Ion: 58 Resp: 90684

Ion Ratio Lower Upper

58 100





43 333.8 270.8 406.2

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/25/2023

Supervised By :Mahesh Dadoda 05/25/2023

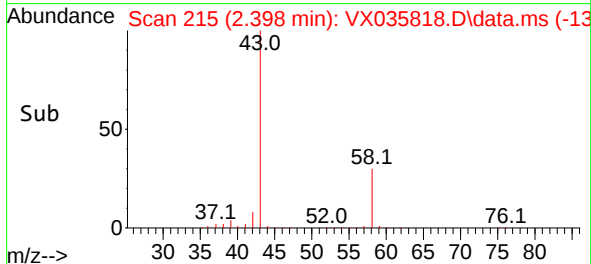

#16

Carbon Disulfide

Concen: 0.638 ug/l

RT: 2.514 min Scan# 234

Delta R.T. 0.000 min

Lab File: VX035818.D




Acq: 23 May 2023 16:52


Tgt Ion: 76 Resp: 2316

Ion Ratio Lower Upper

76 100


78 11.1 7.0 10.6#

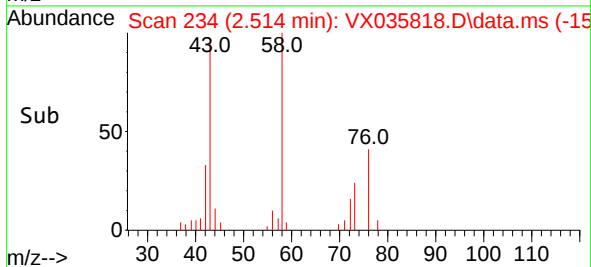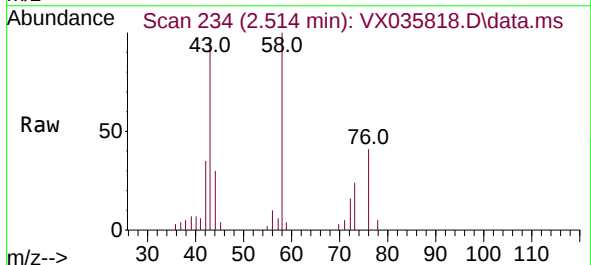



#22
 cis-1,2-Dichloroethene
 Concen: 0.746 ug/l
 RT: 4.489 min Scan# 511
 Delta R.T. 0.000 min
 Lab File: VX035818.D
 Acq: 23 May 2023 16:52




Instrument :
 MSVOA_X
 ClientSampleId :
 SEMI-ANNUAL-CONDENSATE



Tgt Ion: 96 Resp: 1740
 Ion Ratio Lower Upper
 96 100
 61 96.3 121.7 182.5
 98 40.9 52.2 78.2




Manual Integrations
 APPROVED


Reviewed By :John Carlone 05/25/2023
 Supervised By :Mahesh Dadoda 05/25/2023

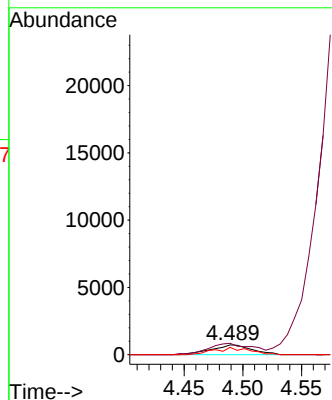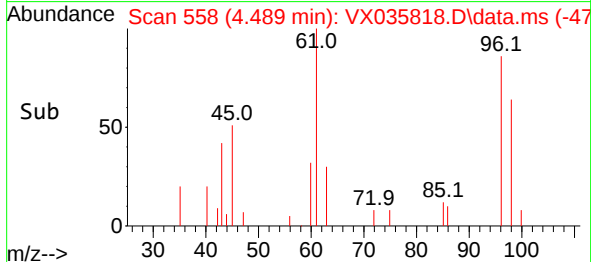

#23
 tert-Butyl Alcohol
 Concen: 7529.720 ug/l
 RT: 3.014 min Scan# 316
 Delta R.T. -0.018 min
 Lab File: VX035818.D
 Acq: 23 May 2023 16:52

Tgt Ion: 59 Resp: 3256570
 Ion Ratio Lower Upper
 59 100
 52 0.2 0.2 0.4

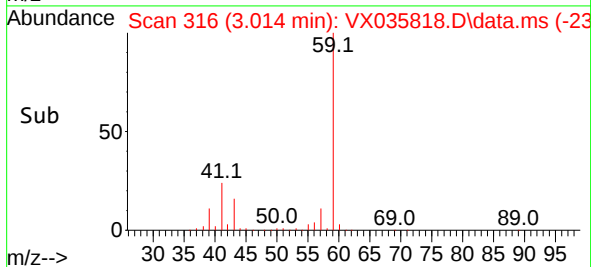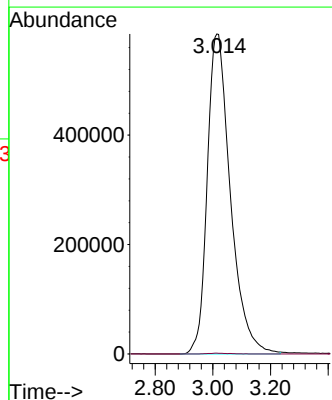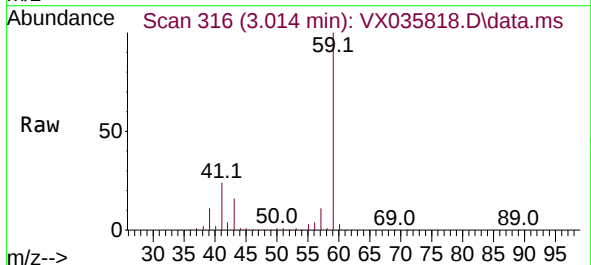



#27

1,2-Dichloroethane-d4

Concen: 31.188 ug/l

RT: 5.958 min Scan# 798

Delta R.T. 0.006 min

Lab File: VX035818.D

Acq: 23 May 2023 16:52

Instrument :

MSVOA_X

ClientSampleId :

SEMI-ANNUAL-CONDENSATE

Tgt Ion: 65 Resp: 86470

Ion Ratio Lower Upper

65 100





67 51.5 40.9 61.3

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/25/2023

Supervised By :Mahesh Dadoda 05/25/2023

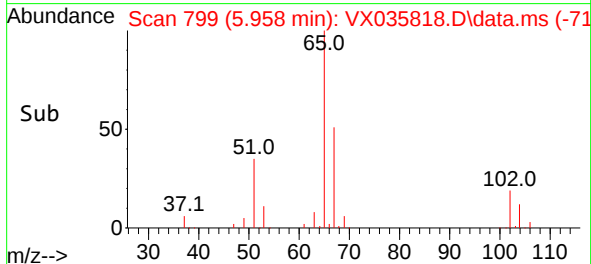

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.006 min

Lab File: VX035818.D

Acq: 23 May 2023 16:52




Tgt Ion:114 Resp: 196150


Ion Ratio Lower Upper

114 100

63 22.0 18.0 27.0


88 16.3 13.3 19.9

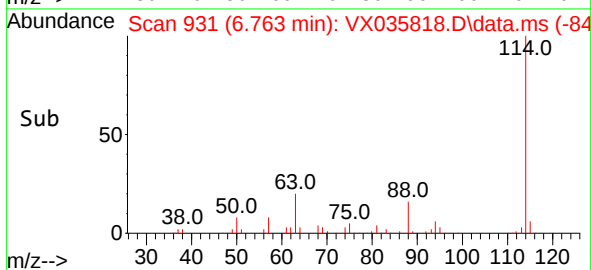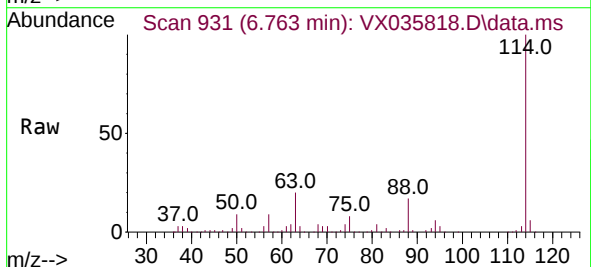



#30
2-Butanone
Concen: 3335.109 ug/l
RT: 4.574 min Scan# 51
Delta R.T. 0.000 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52




Instrument :
MSVOA_X
ClientSampleId :
SEMI-ANNUAL-CONDENSATE




Tgt Ion: 43 Resp: 596334
Ion Ratio Lower Upper
43 100
57 8.2 6.3 9.5
72 24.1 19.6 29.4

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/25/2023
Supervised By :Mahesh Dadoda 05/25/2023

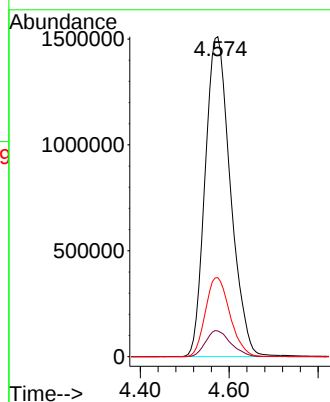


#34
Benzene
Concen: 31.380 ug/l
RT: 6.038 min Scan# 812
Delta R.T. 0.000 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52




Tgt Ion: 78 Resp: 270396
Ion Ratio Lower Upper
78 100
77 23.1 19.0 28.4
51 17.1 14.6 21.8

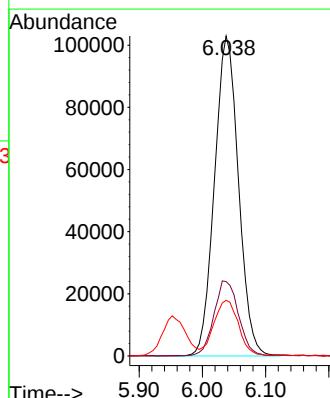



#45
1,4-Dioxane
Concen: 1552.887 ug/l
RT: 7.714 min Scan# 1092
Delta R.T. -0.030 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52




Instrument :
MSVOA_X
ClientSampleId :
SEMI-ANNUAL-CONDENSATE



Tgt Ion: 88 Resp: 81984
Ion Ratio Lower Upper
88 100
43 29.8 26.5 39.7
58 65.1 55.6 83.4




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2023
Supervised By :Mahesh Dadoda 05/25/2023

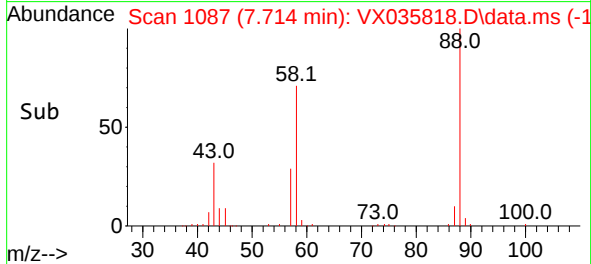

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52

Tgt Ion:117 Resp: 177002
Ion Ratio Lower Upper
117 100
82 58.6 45.8 68.8
119 32.4 25.4 38.0

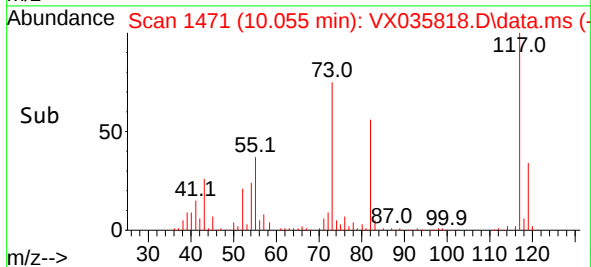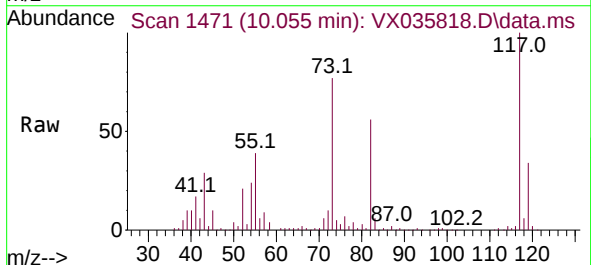

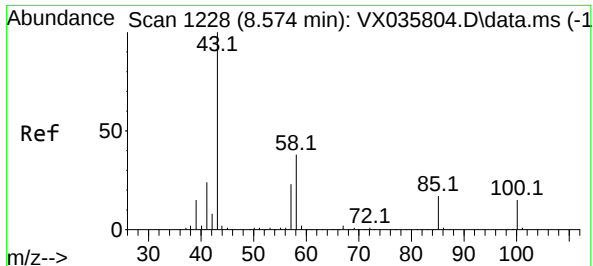

#58

4-Methyl-2-Pentanone

Concen: 71.549 ug/l

RT: 8.574 min Scan# 1228

Delta R.T. 0.000 min

Lab File: VX035818.D


Acq: 23 May 2023 16:52

Instrument :

MSVOA_X

ClientSampleId :

SEMI-ANNUAL-CONDENSATE

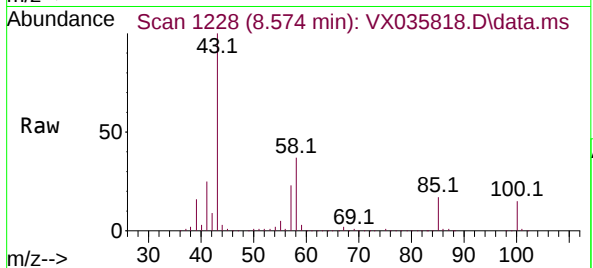

Tgt Ion: 43 Resp: 24598




Ion	Ratio	Lower	Upper
43	100		
58	38.3	29.9	44.9
85	16.7	13.2	19.8

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/25/2023

Supervised By :Mahesh Dadoda 05/25/2023

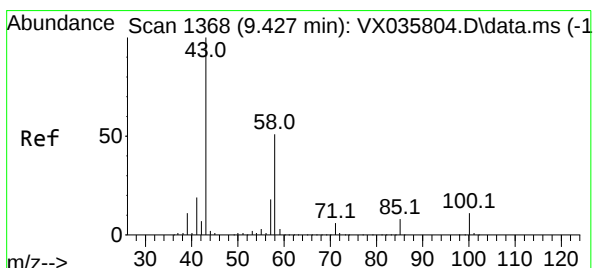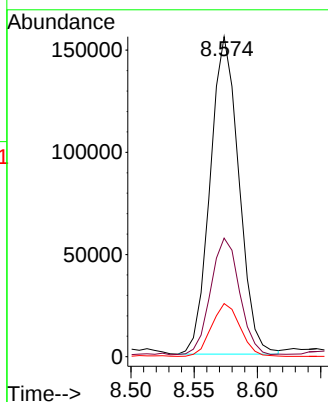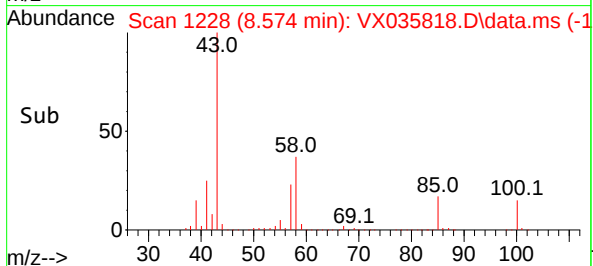

#59

2-Hexanone

Concen: 39.574 ug/l

RT: 9.433 min Scan# 1369




Delta R.T. 0.006 min


Lab File: VX035818.D

Acq: 23 May 2023 16:52

Tgt Ion: 43 Resp: 102376


Ion	Ratio	Lower	Upper
43	100		
58	49.5	41.7	62.5
57	21.7	14.7	22.1

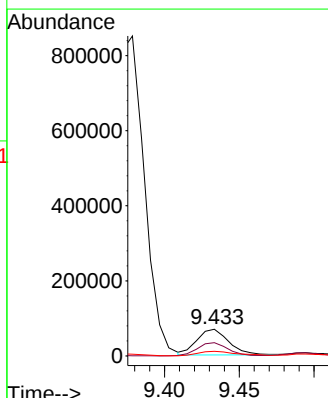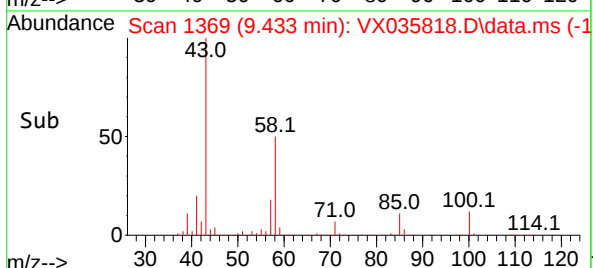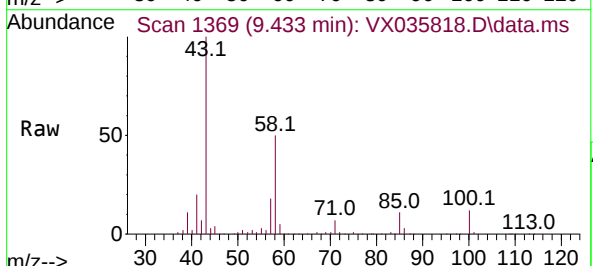



#60
4-Bromofluorobenzene
Concen: 31.192 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52




Instrument : MSVOA_X
ClientSampleId : SEMI-ANNUAL-CONDENSATE



Tgt Ion: 95 Resp: 92643
Ion Ratio Lower Upper
95 100
174 70.0 0.2 0.4
176 67.7 0.2 0.2




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2023
Supervised By :Mahesh Dadoda 05/25/2023

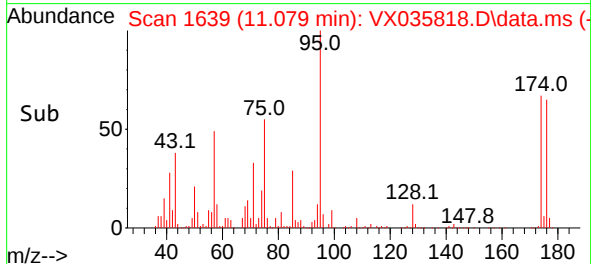

#62
Toluene
Concen: 99.900 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.000 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52


Tgt Ion: 91 Resp: 910607
Ion Ratio Lower Upper
91 100
92 58.7 46.5 69.7

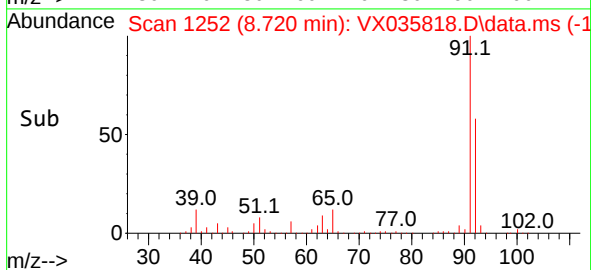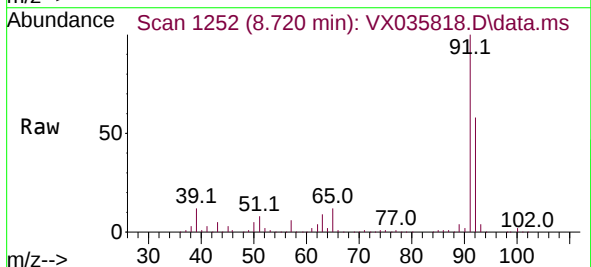



#63
Toluene-d8
Concen: 30.509 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52




Instrument :
MSVOA_X
ClientSampleId :
SEMI-ANNUAL-CONDENSATE



Tgt Ion: 98 Resp: 238729
Ion Ratio Lower Upper
98 100
100 65.1 52.1 78.1




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2023
Supervised By :Mahesh Dadoda 05/25/2023

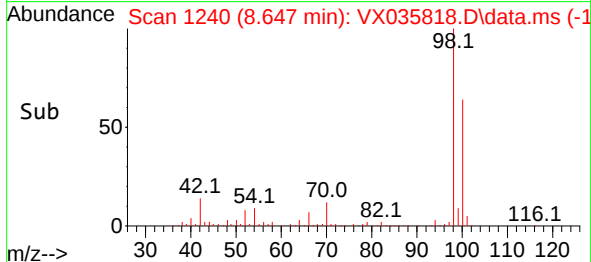

#64
Chlorobenzene
Concen: 10.913 ug/l
RT: 10.080 min Scan# 1475
Delta R.T. 0.000 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52


Tgt Ion:112 Resp: 62999
Ion Ratio Lower Upper
112 100
114 38.0 25.8 38.8

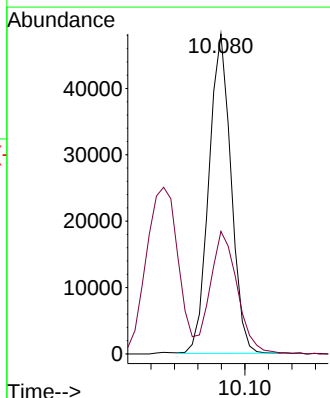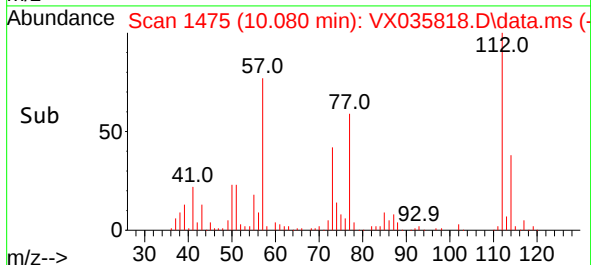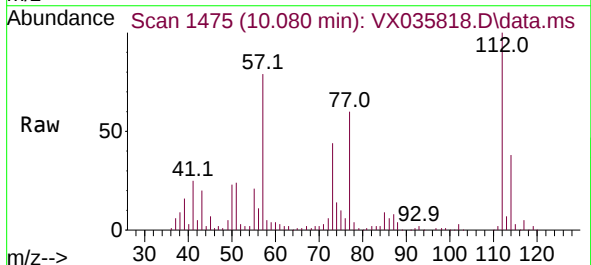



#66
Ethyl Benzene
Concen: 51.058 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52




Instrument :
MSVOA_X
ClientSampleId :
SEMI-ANNUAL-CONDENSATE




Tgt Ion: 91 Resp: 520492
Ion Ratio Lower Upper
91 100
106 31.7 24.4 36.6

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/25/2023
Supervised By :Mahesh Dadoda 05/25/2023

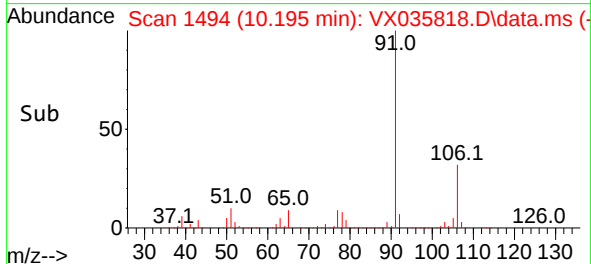


#67
m/p-Xylenes
Concen: 51.852 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52

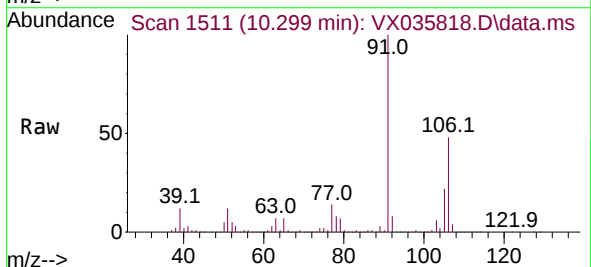

Tgt Ion:106 Resp: 200076
Ion Ratio Lower Upper
106 100
91 207.9 167.4 251.2

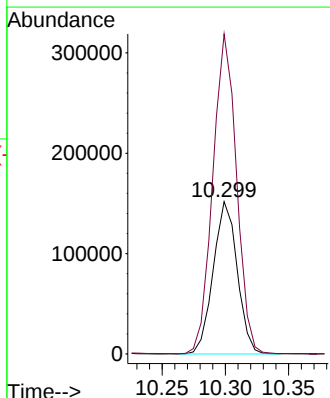







#68
o-Xylene
Concen: 28.694 ug/l
RT: 10.640 min Scan# 11074
Delta R.T. 0.000 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52

Instrument :
MSVOA_X
ClientSampleId :
SEMI-ANNUAL-CONDENSATE

Tgt Ion:106 Resp: 11074
Ion Ratio Lower Upper
106 100
91 218.5 108.9 326.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2023
Supervised By :Mahesh Dadoda 05/25/2023

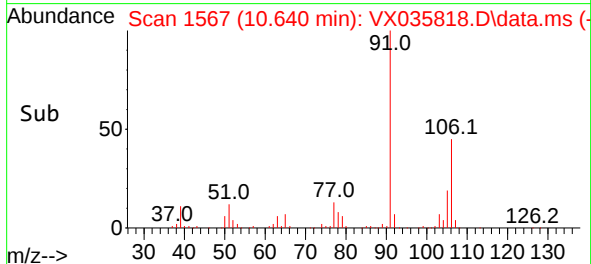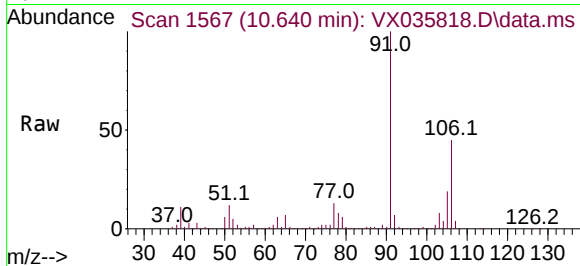

#70
Isopropylbenzene
Concen: 6.812 ug/l
RT: 10.964 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52

Tgt Ion:105 Resp: 67107
Ion Ratio Lower Upper
105 100
120 26.5 18.5 34.3

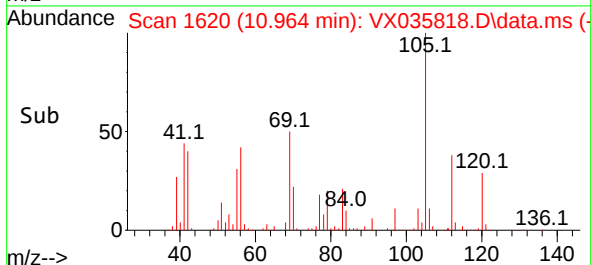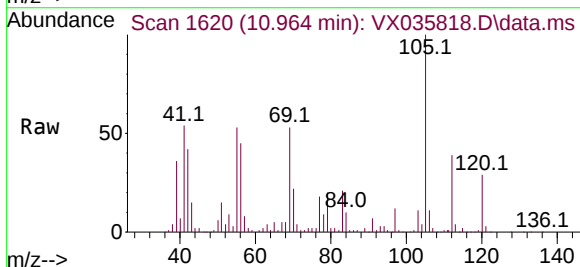







#74
n-propylbenzene
Concen: 4.557 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.000 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52

Instrument :
MSVOA_X
ClientSampleId :
SEMI-ANNUAL-CONDENSATE

Tgt Ion: 91 Resp: 53518
Ion Ratio Lower Upper
91 100
120 22.9 0.0 44.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2023
Supervised By :Mahesh Dadoda 05/25/2023

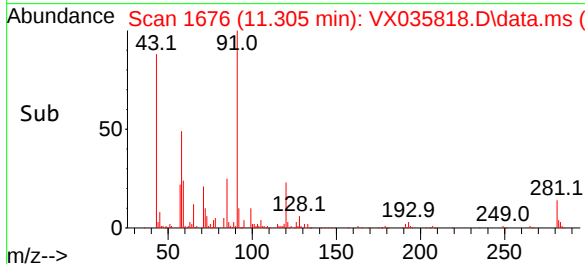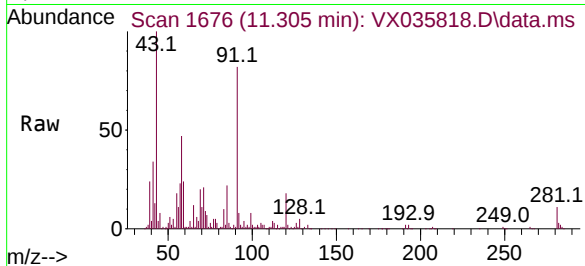

#76
1,3,5-Trimethylbenzene
Concen: 12.855 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52


Tgt Ion:105 Resp: 107559
Ion Ratio Lower Upper
105 100
120 48.2 0.0 96.4

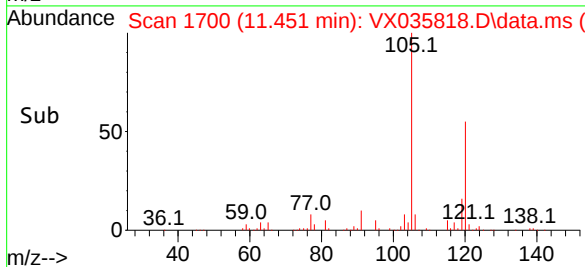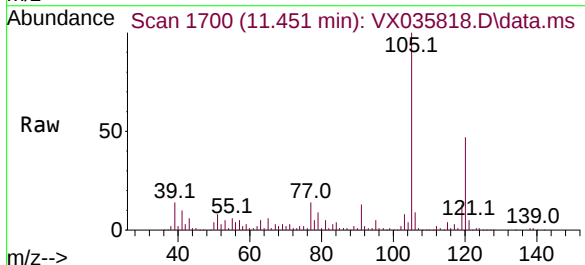



#80
1,2,4-Trimethylbenzene
Concen: 46.431 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52




Instrument :
MSVOA_X
ClientSampleId :
SEMI-ANNUAL-CONDENSATE



Tgt Ion:105 Resp: 390423
Ion Ratio Lower Upper
105 100
120 46.7 0.0 90.4




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2023
Supervised By :Mahesh Dadoda 05/25/2023

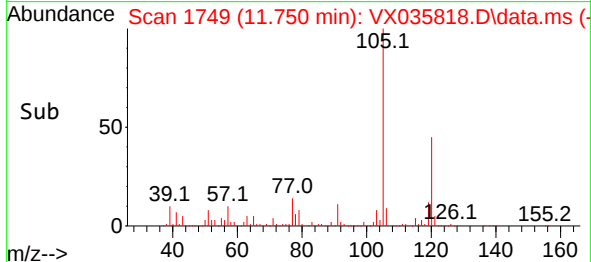

#81
sec-Butylbenzene
Concen: 2.007 ug/l m
RT: 11.890 min Scan# 1772
Delta R.T. 0.000 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52

Tgt Ion:105 Resp: 20470
Ion Ratio Lower Upper
105 100
134 11.0 0.0 40.2

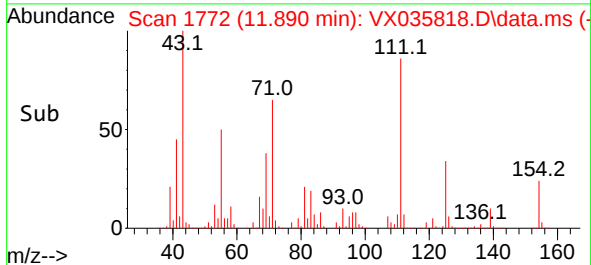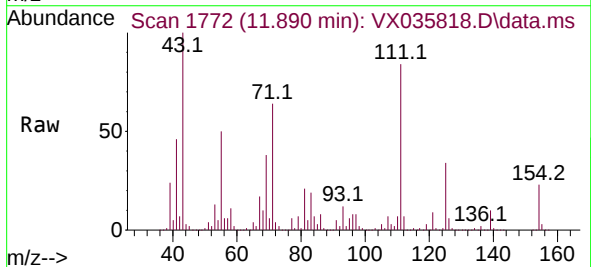



#82

p-Isopropyltoluene

Concen: 254.176 ug/l

RT: 12.012 min Scan# 1792

Delta R.T. 0.006 min

Lab File: VX035818.D


Acq: 23 May 2023 16:52

Instrument :

MSVOA_X

ClientSampleId :

SEMI-ANNUAL-CONDENSATE

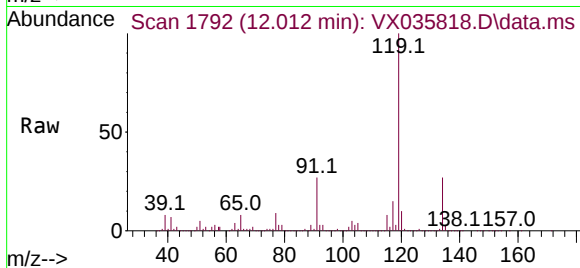

Tgt Ion:119 Resp: 2156500

Ion Ratio Lower Upper

119 100

134 26.4 0.0 52.2



91 27.1 0.0 51.0

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/25/2023

Supervised By :Mahesh Dadoda 05/25/2023

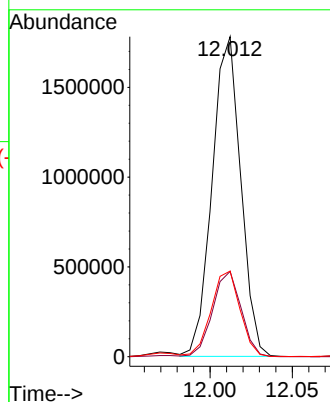

#83

1,3-Dichlorobenzene

Concen: 0.834 ug/l

RT: 11.969 min Scan# 1785

Delta R.T. 0.000 min

Lab File: VX035818.D

Acq: 23 May 2023 16:52




Tgt Ion:146 Resp: 3777


Ion Ratio Lower Upper

146 100

111 23.4 20.6 61.9

148 69.4 31.6 94.7

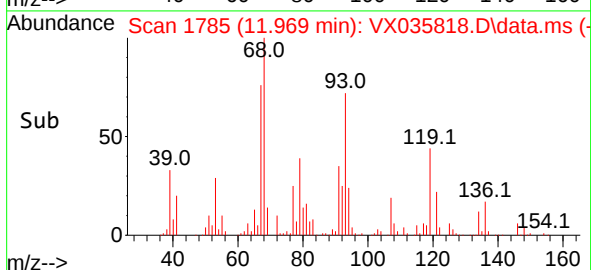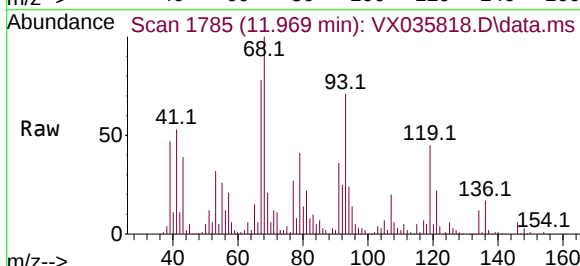



#84

1,4-Dichlorobenzene

Concen: 80.250 ug/l

RT: 12.043 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX035818.D

Acq: 23 May 2023 16:52

Instrument :

MSVOA_X

ClientSampleId :





SEMI-ANNUAL-CONDENSATE

Tgt Ion:146 Resp: 36487
 Ion Ratio Lower Upper
 146 100
 111 40.4 20.3 60.9
 148 63.3 31.8 95.3

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/25/2023
 Supervised By :Mahesh Dadoda 05/25/2023

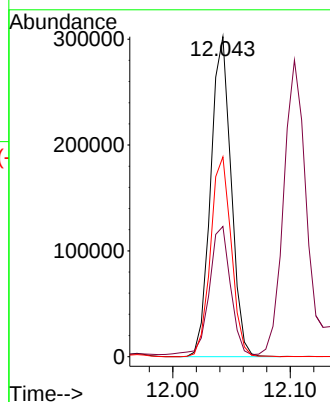

#85

n-Butylbenzene

Concen: 3.925 ug/l m




RT: 12.323 min Scan# 1843


Delta R.T. -0.006 min

Lab File: VX035818.D

Acq: 23 May 2023 16:52


Tgt Ion: 91 Resp: 29623
 Ion Ratio Lower Upper
 91 100
 92 15.7 0.0 107.6
 134 30.8 0.0 49.8

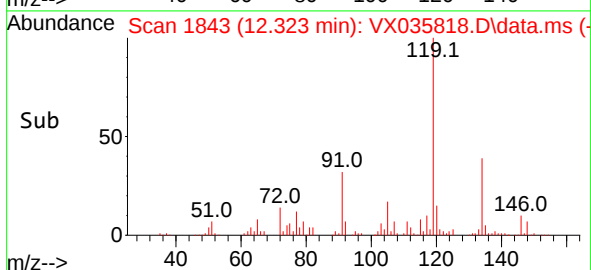

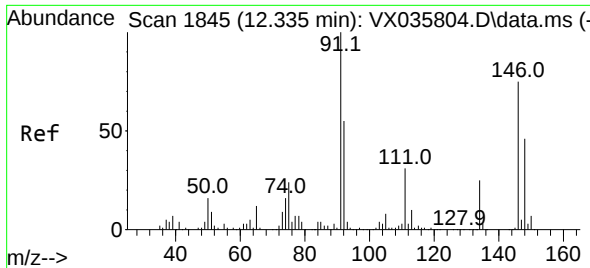

#87
1,2-Dichlorobenzene
Concen: 3.419 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52




Instrument :
MSVOA_X
ClientSampleId :
SEMI-ANNUAL-CONDENSATE

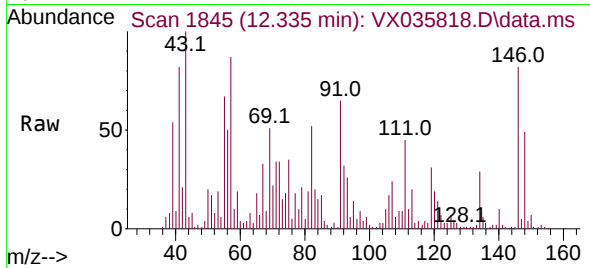


Tgt Ion:146 Resp: 1517
Ion Ratio Lower Upper
146 100
111 52.9 21.3 64.0
148 63.3 31.7 95.1

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/25/2023
Supervised By :Mahesh Dadoda 05/25/2023

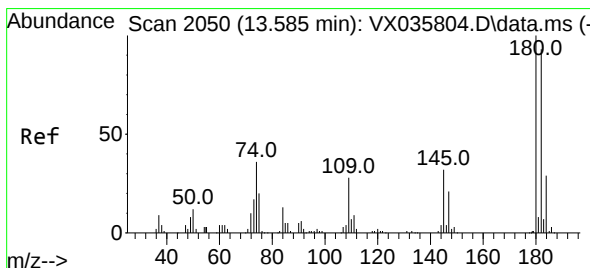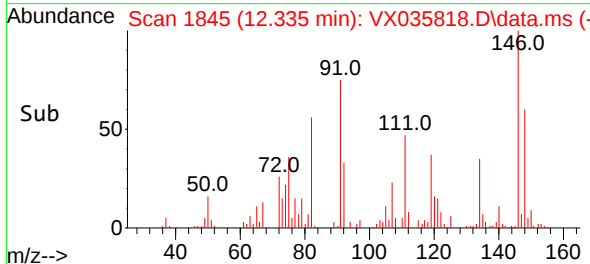


#89
1,2,4-Trichlorobenzene
Concen: 1.485 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. 0.006 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52

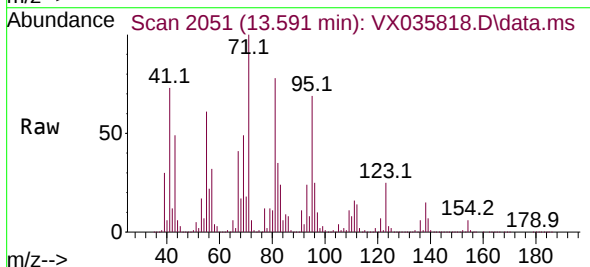


Tgt Ion:180 Resp: 3949
Ion Ratio Lower Upper
180 100
182 92.1 75.8 113.8
145 68.7 25.8 38.6#

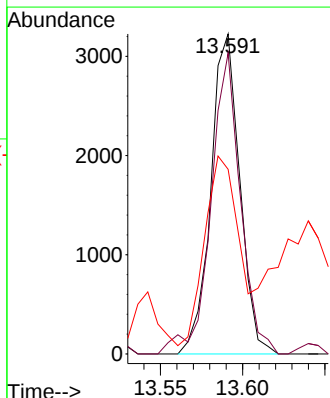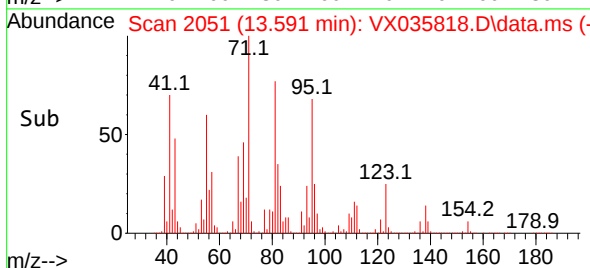

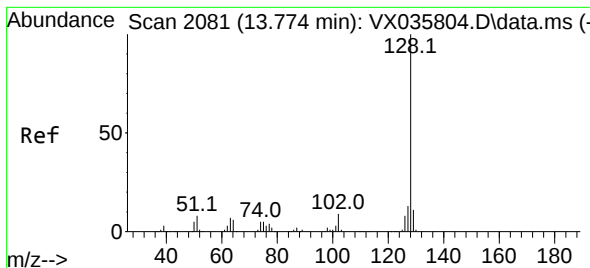

#91
Naphthalene
Concen: 310.708 ug/l
RT: 13.780 min Scan# 2081
Delta R.T. 0.006 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52




Instrument :
MSVOA_X
ClientSampleId :
SEMI-ANNUAL-CONDENSATE

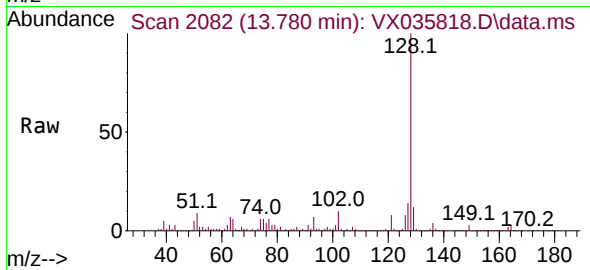

Tgt Ion:128 Resp: 285996
Ion Ratio Lower Upper
128 100
127 13.4 10.3 15.5
129 11.4 8.8 13.2

Manual Integrations
APPROVED

Reviewed By :John Carlone 05/25/2023
Supervised By :Mahesh Dadoda 05/25/2023

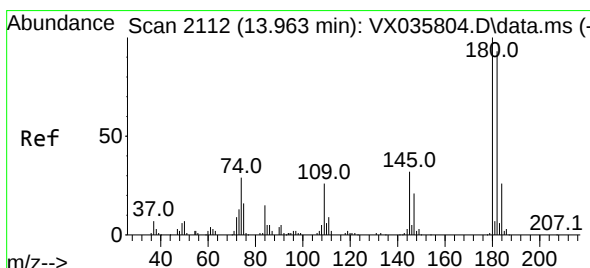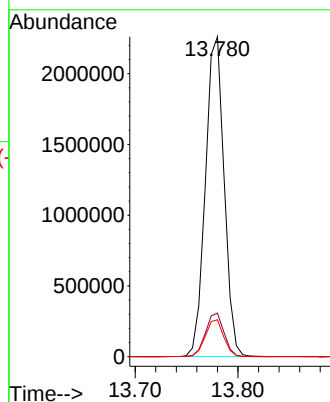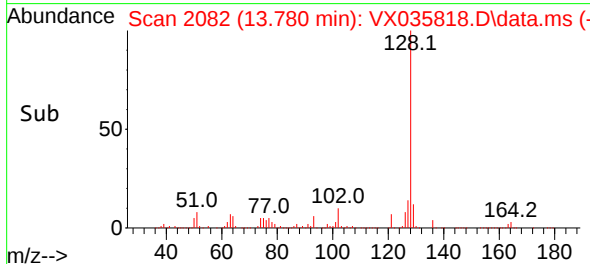

#92
1,2,3-Trichlorobenzene
Concen: 0.817 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. 0.000 min
Lab File: VX035818.D
Acq: 23 May 2023 16:52

Tgt Ion:180 Resp: 2171
Ion Ratio Lower Upper
180 100
182 90.7 0.0 191.0
145 96.5 0.0 66.8#

