

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052323\
 Data File : VX035820.D
 Acq On : 23 May 2023 17:39
 Operator : JC/MD
 Sample : 02899-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TWP01

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X052323W.M

Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VX035820.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.398	209	215	227	rVB3	2723	7354	1.13%	0.277%
2	4.897	614	625	640	rBV2	85921	251731	38.71%	9.478%
3	5.550	724	732	743	rVB3	5194	13656	2.10%	0.514%
4	5.952	788	798	812	rBV2	90938	245797	37.79%	9.254%
5	6.763	918	931	946	rBV	202516	489471	75.26%	18.429%
6	8.647	1234	1240	1251	rBV	416789	650367	100.00%	24.486%
7	10.055	1465	1471	1482	rBV	411357	554117	85.20%	20.863%
8	11.079	1633	1639	1649	rBV	316553	398999	61.35%	15.022%
9	13.585	2046	2050	2055	rBV6	6577	10127	1.56%	0.381%
10	13.731	2070	2074	2078	rBV2	18885	25491	3.92%	0.960%
11	13.774	2078	2081	2089	rVB2	5713	8929	1.37%	0.336%




Sum of corrected areas: 2656039

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052323\
Data File : VX035820.D
Acq On : 23 May 2023 17:39
Operator : JC/MD
Sample : 02899-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TWP01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X052323W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

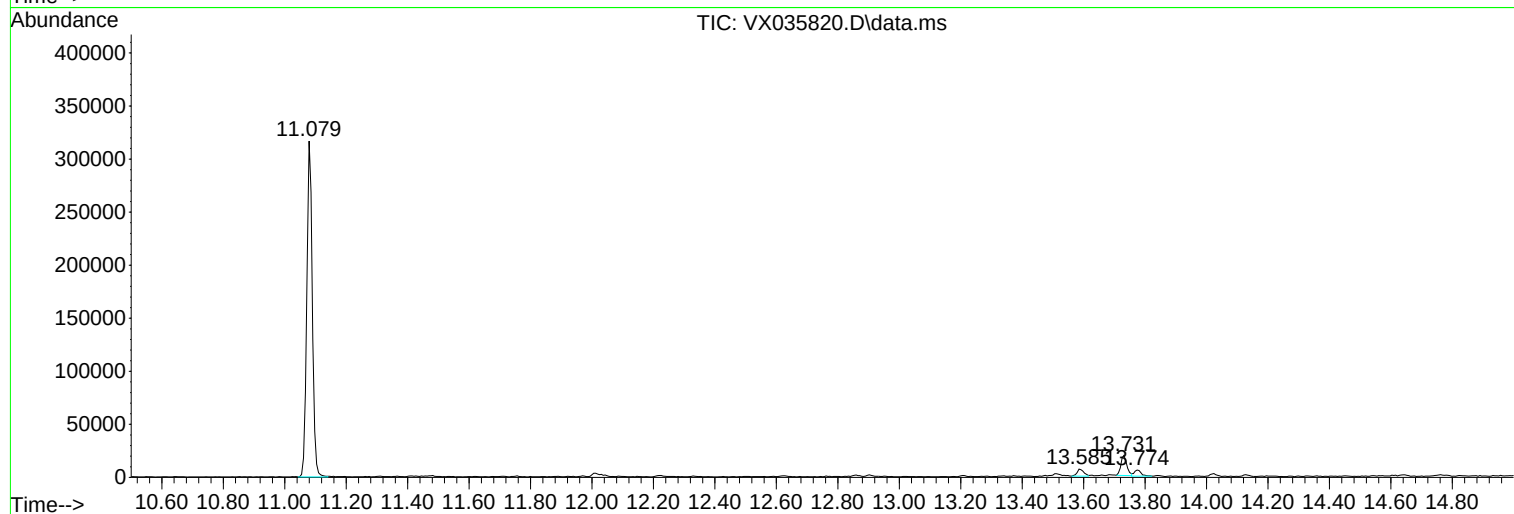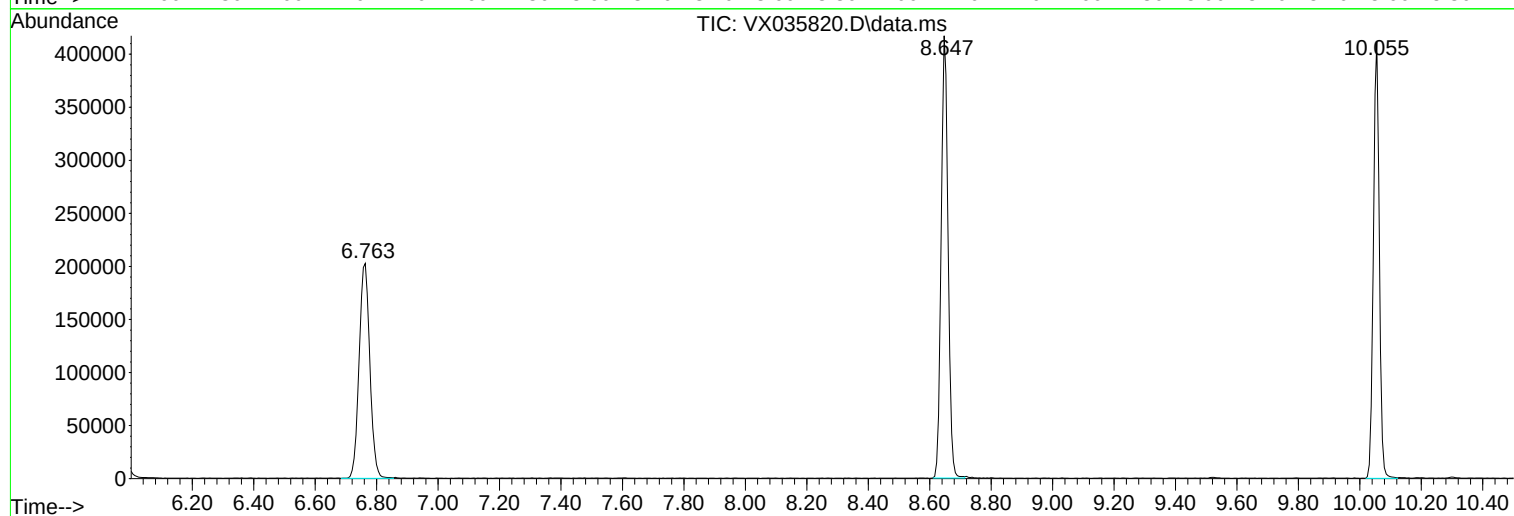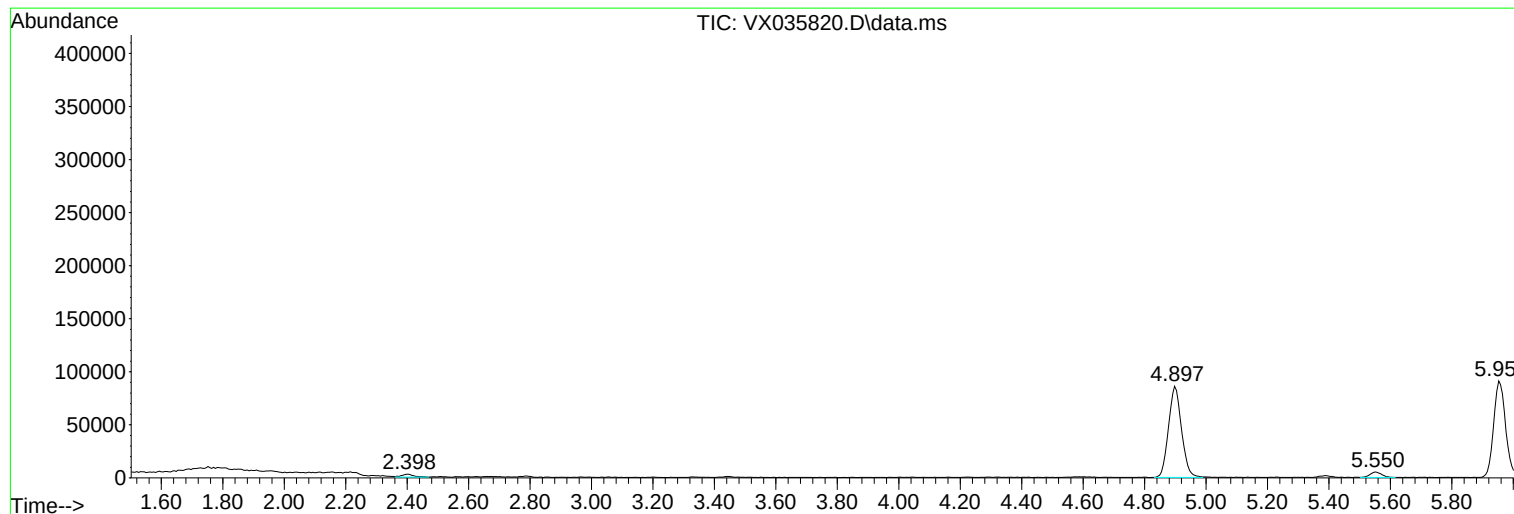

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052323\
Data File : VX035820.D
Acq On : 23 May 2023 17:39
Operator : JC/MD
Sample : 02899-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TWP01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X052323W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052323\
Data File : VX035820.D
Acq On : 23 May 2023 17:39
Operator : JC/MD
Sample : 02899-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TWP01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X052323W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------