
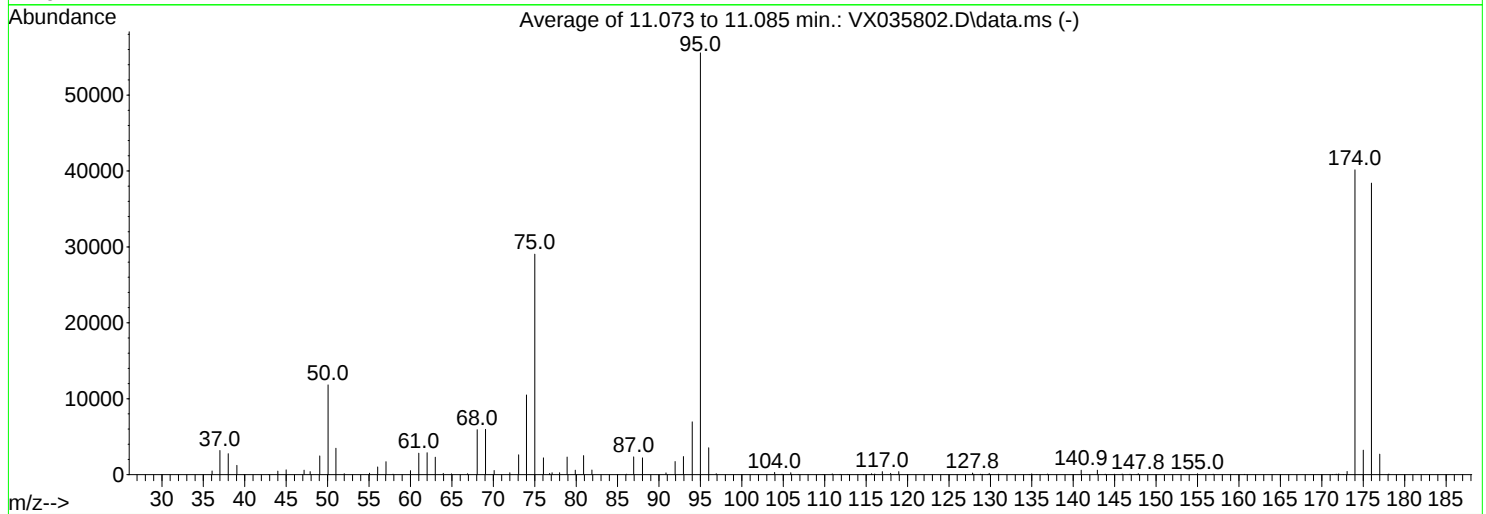


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052323\
 Data File : VX035802.D
 Acq On : 23 May 2023 08:24
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X052323W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue May 23 11:36:37 2023

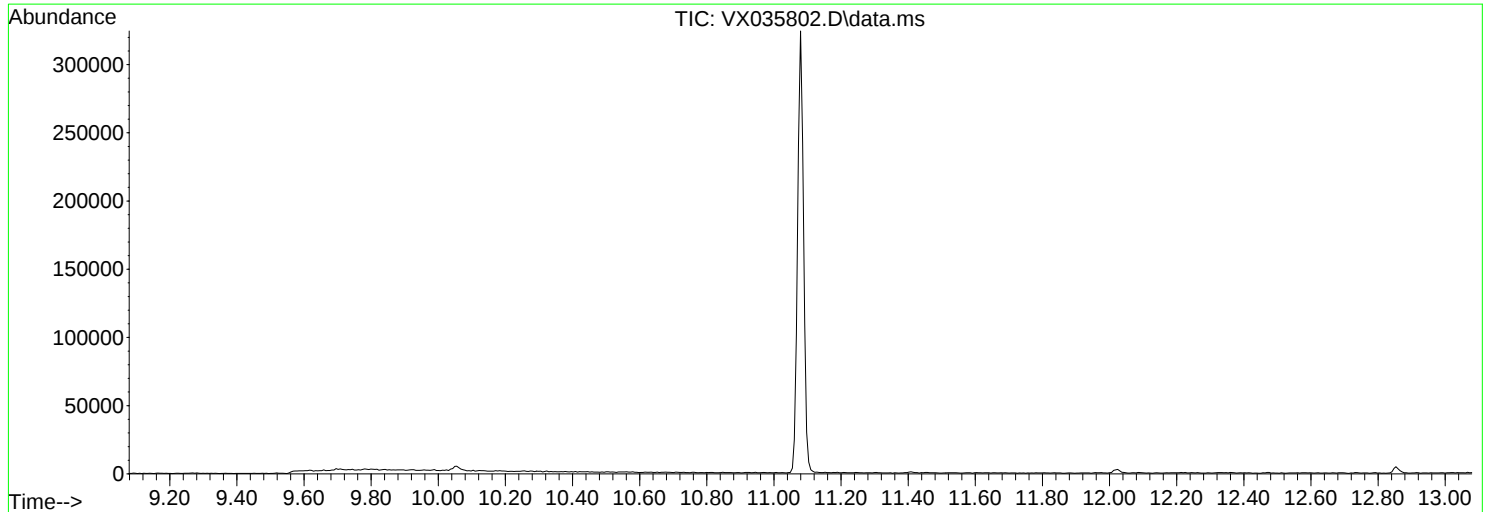

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	11835	PASS
75	95	30	60	52.3	29045	PASS
95	95	100	100	100.0	55565	PASS
96	95	5	9	6.4	3550	PASS
173	174	0.00	2	1.1	425	PASS
174	95	50	100	72.3	40163	PASS
175	174	5	9	8.0	3231	PASS
176	174	95	101	95.6	38403	PASS
177	176	5	9	7.0	2703	PASS