

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX052419\
 Data File : VX009890.D
 Acq On : 24 May 2019 16:34
 Operator : JC/SP
 Sample : K3032-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S32-0652

Quant Time: May 25 00:14:55 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 09 07:31:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	173348	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	279630	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	249772	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	108254	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.06	65	120328	50.85	ug/l	0.00
Spiked Amount			Recovery	=	101.70%	
35) Dibromofluoromethane	5.50	113	85962	48.90	ug/l	0.00
Spiked Amount			Recovery	=	97.80%	
50) Toluene-d8	8.71	98	356376	50.22	ug/l	0.00
Spiked Amount			Recovery	=	100.44%	
62) 4-Bromofluorobenzene	11.13	95	120092	46.57	ug/l	0.00
Spiked Amount			Recovery	=	93.14%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.40	50	16332	7.489	ug/l #	43
4) Vinyl Chloride	1.41	62	2924722	1375.269	ug/l	97
5) Bromomethane	1.65	94	276	0.216	ug/l #	80
10) Methyl Iodide	2.51	142	219	4.699	ug/l #	53
11) Tert butyl alcohol	3.03	59	2227	4.066	ug/l	95
12) 1,1-Dichloroethene	2.38	96	1560	0.959	ug/l #	78
16) Acetone	2.44	43	4020	3.164	ug/l	100
17) Carbon Disulfide	2.57	76	2452	0.537	ug/l #	62
20) Methylene Chloride	2.85	84	511	0.248	ug/l #	79
21) trans-1,2-Dichloroethene	3.17	96	18247	10.344	ug/l	97
25) 2-Butanone	4.70	43	729	0.369	ug/l #	53
27) cis-1,2-Dichloroethene	4.60	96	357824	169.950	ug/l	91
28) Bromochloromethane	5.04	49	40	Below Cal	#	20
31) Cyclohexane	5.67	56	4147	1.185	ug/l #	1
36) 1,1-Dichloropropene	5.66	75	13862	5.334	ug/l #	50
38) Carbon Tetrachloride	5.67	117	16376	6.936	ug/l #	15
40) Benzene	6.15	78	1911	0.238	ug/l	100
44) Trichloroethene	7.21	130	5217	2.683	ug/l	90
49) 1,4-Dioxane	7.86	88	23	0.395	ug/l #	1
65) Chlorobenzene	10.14	112	2403	0.481	ug/l	92
69) o-Xylene	10.70	106	1121	0.338	ug/l	98
76) 1,2,3-Trichloropropane	11.13	75	62672	24.958	ug/l #	34
81) trans-1,4-Dichloro-2-buten	11.13	75	62672	63.858	ug/l #	10
90) Hexachloroethane	12.70	117	336	0.287	ug/l #	7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX052419\
Data File : VX009890.D
Acq On : 24 May 2019 16:34
Operator : JC/SP
Sample : K3032-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S32-0652

Quant Time: May 25 00:14:55 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
Quant Title : SW846 8260
QLast Update : Thu May 09 07:31:15 2019
Response via : Initial Calibration

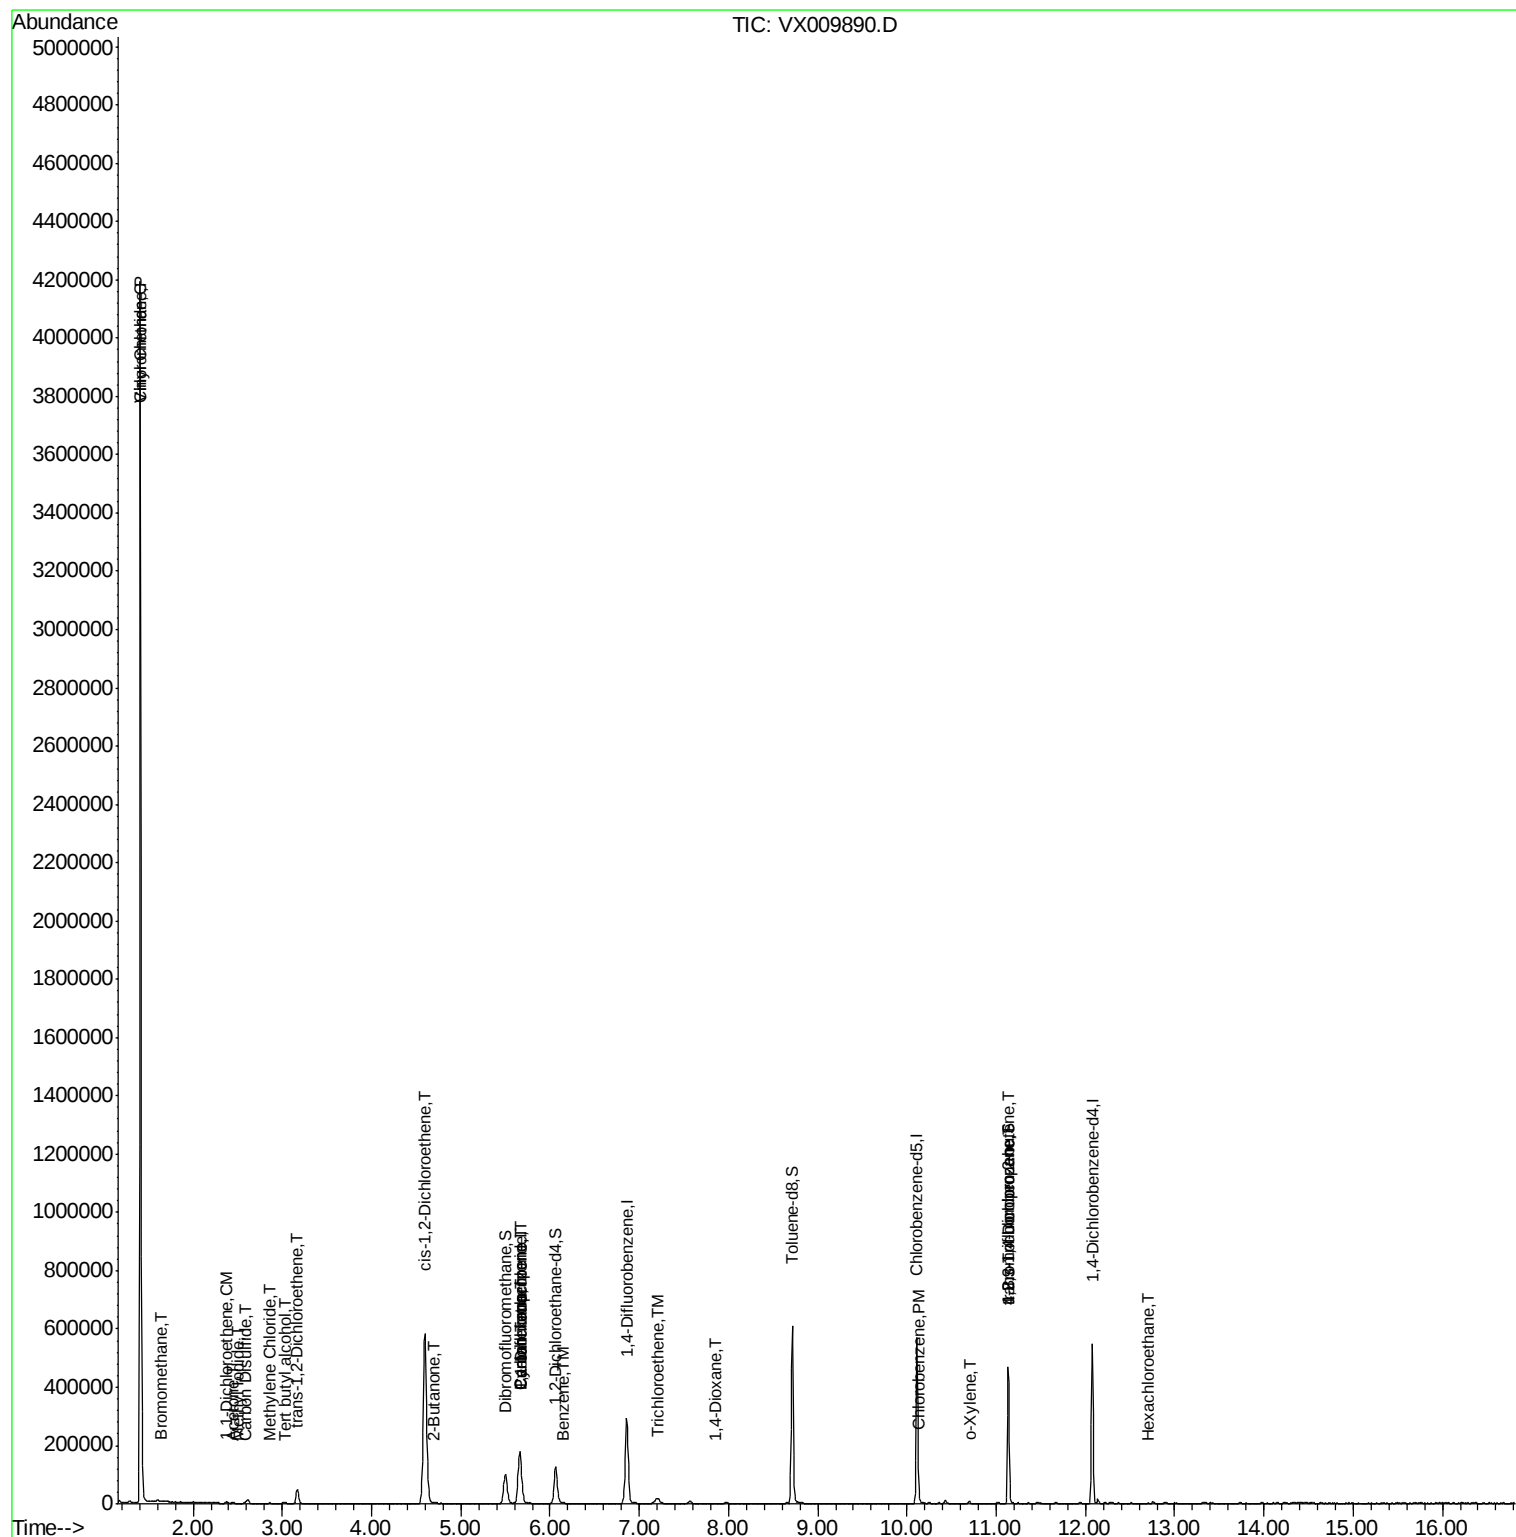



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.00 min

Lab File: VX009890.D

Acq: 24 May 2019 16:34

Instrument :

MSVOA_X

ClientSampleId :


S32-0652

Tot Ion:168 Resp: 173348

Ion Ratio Lower Upper

168 100

99 54.7 42.3 63.5



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

60000



40000

20000

0

Time-->

5.50 5.60 5.70 5.80 5.90



#3

Chloromethane

Concen: 7.489 ug/l

RT: 1.40 min Scan# 41

Delta R.T. 0.08 min

Lab File: VX009890.D


Acq: 24 May 2019 16:34

Tgt Ion: 50 Resp: 16332

Ion Ratio Lower Upper

50 100

52 0.6 25.9 38.9#



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

1.40

15000


10000


5000

0

Time-->

1.35 1.40 1.45





#4

Vinyl Chloride

Concen: 1375.269 ug/l

RT: 1.41 min Scan# 42

Delta R.T. -0.00 min

Lab File: VX009890.D

Acq: 24 May 2019 16:34

Instrument :

MSVOA_X

ClientSampled :





S32-0652

Tot Ion: 62 Resp: 2924722

Ion Ratio Lower Upper

62 100

64 32.3 24.6 36.8

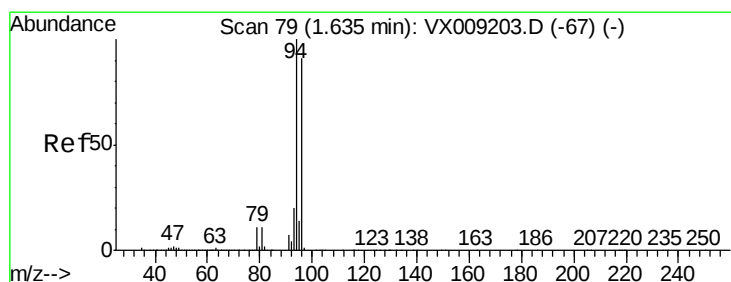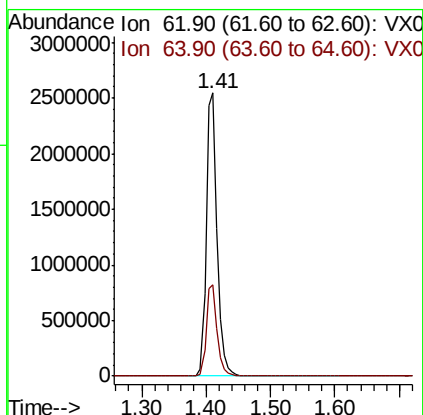

#5

Bromomethane

Concen: 0.216 ug/l

RT: 1.65 min Scan# 81

Delta R.T. 0.01 min

Lab File: VX009890.D




Acq: 24 May 2019 16:34


Tgt Ion: 94 Resp: 276

Ion Ratio Lower Upper

94 100

96 72.0 73.0 109.6#

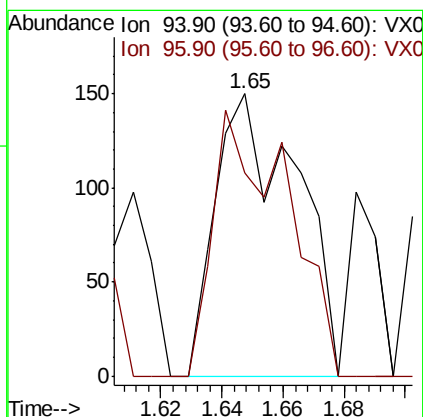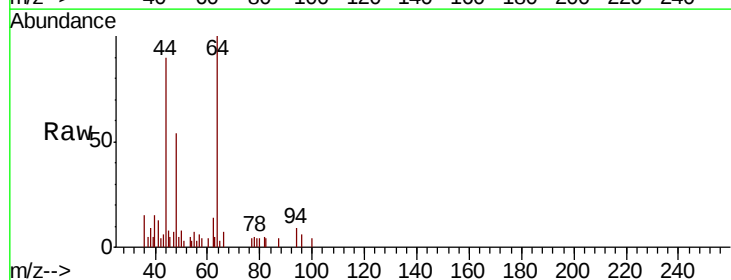







#10
Methvl Iodide
Concen: 4.699 ug/l
RT: 2.51 min Scan# 223
Delta R.T. 0.01 min
Lab File: VX009890.D
Acq: 24 May 2019 16:34

Instrument :
MSVOA_X
ClientSampleId :
S32-0652

Tot Ion:142 Resp: 219
Ion Ratio Lower Upper
142 100
127 9.1 32.7 49.1#
141 0.0 11.5 17.3#




Abundance Ion 141.80 (141.50 to 142.50): V
Ion 126.80 (126.50 to 127.50): V
Ion 140.80 (140.50 to 141.50): V

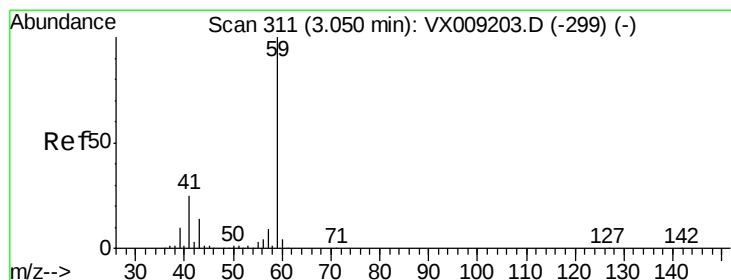
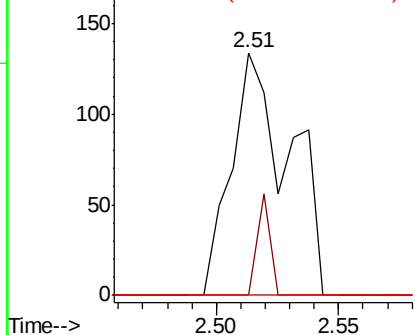



#11
Tert butyl alcohol
Concen: 4.066 ug/l
RT: 3.03 min Scan# 307
Delta R.T. -0.02 min
Lab File: VX009890.D
Acq: 24 May 2019 16:34

Tgt Ion: 59 Resp: 2227
Ion Ratio Lower Upper
59 100
57 8.4 8.2 12.2



Abundance Ion 59.00 (58.70 to 59.70): VX0
Ion 57.00 (56.70 to 57.70): VX0



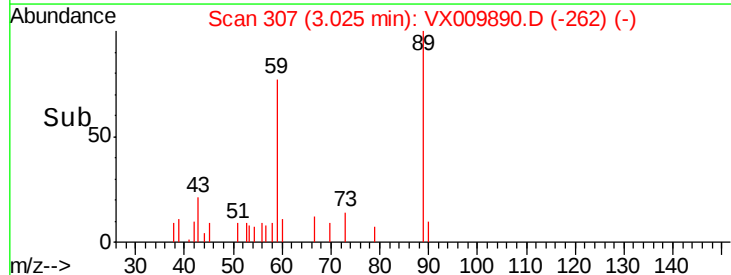
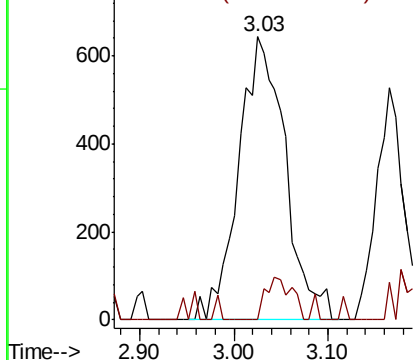




#12
 1,1-Dichloroethene
 Concen: 0.959 ug/l
 RT: 2.38 min Scan# 201
 Delta R.T. 0.01 min
 Lab File: VX009890.D
 Acq: 24 May 2019 16:34




Instrument :
 MSVOA_X
 ClientSampled :
 S32-0652


Tot Ion	Ratio	Lower	Upper
96	100		
61	143.8	144.3	216.5#
98	54.2	50.3	75.5

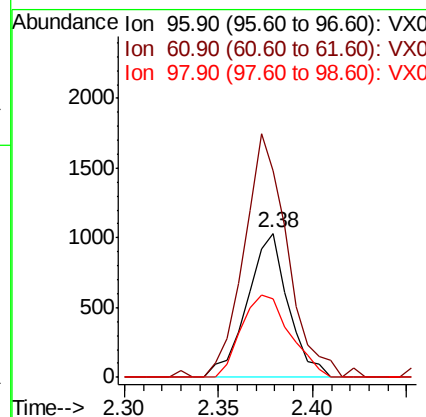

#16
 Acetone
 Concen: 3.164 ug/l
 RT: 2.44 min Scan# 211
 Delta R.T. -0.01 min
 Lab File: VX009890.D
 Acq: 24 May 2019 16:34

Tgt Ion	Ratio	Lower	Upper
43	100		
58	31.3	24.9	37.3

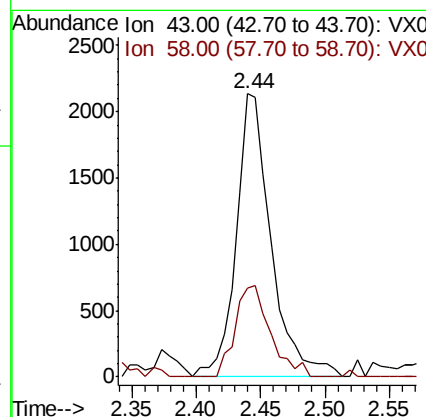



#17

Carbon Disulfide

Concen: 0.537 ug/l

RT: 2.57 min Scan# 233

Delta R.T. 0.01 min

Lab File: VX009890.D

Acq: 24 May 2019 16:34

Instrument :

MSVOA_X

ClientSampled :


S32-0652

Tot Ion: 76 Resp: 2452

Ion Ratio Lower Upper




76 100

78 23.1 7.4 11.0#



Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

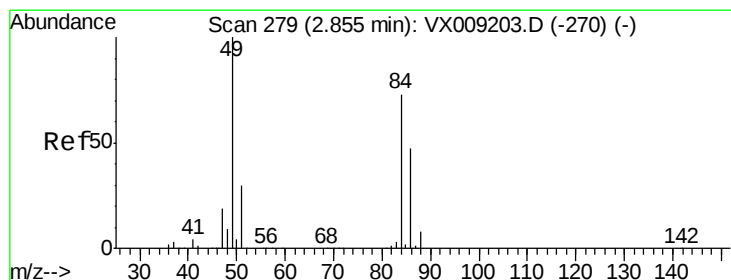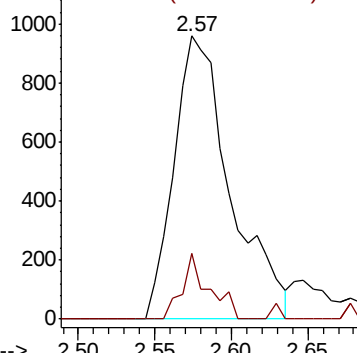

#20

Methylene Chloride

Concen: 0.248 ug/l

RT: 2.85 min Scan# 279

Delta R.T. -0.00 min

Lab File: VX009890.D

Acq: 24 May 2019 16:34

Tgt Ion: 84 Resp: 511


Ion Ratio Lower Upper

84 100

49 152.7 109.9 164.9

51 66.5 32.7 49.1#

86 44.2 52.0 78.0#






Abundance Ion 83.90 (83.60 to 84.60): VX0

Ion 48.90 (48.60 to 49.60): VX0

Ion 50.90 (50.60 to 51.60): VX0

Ion 85.90 (85.60 to 86.60): VX0

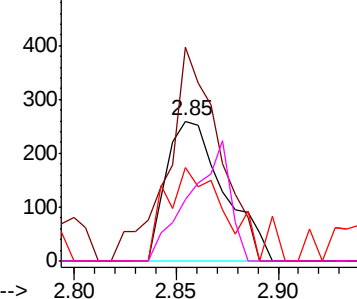



#21

trans-1,2-Dichloroethene

Concen: 10.344 ug/l

RT: 3.17 min Scan# 330

Delta R.T. 0.01 min

Lab File: VX009890.D

Acq: 24 May 2019 16:34

Instrument :

MSVOA_X

ClientSampleId :

S32-0652


Tot Ion: 96 Resp: 18247

Ion Ratio Lower Upper




96 100

61 158.8 124.5 186.7

98 65.1 50.4 75.6

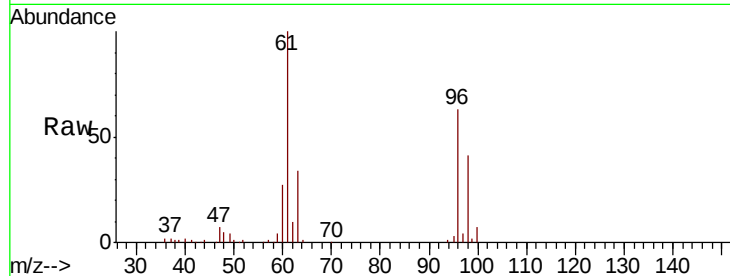

Abundance Ion 95.90 (95.60 to 96.60): VX0
Ion 60.90 (60.60 to 61.60): VX0
Ion 97.90 (97.60 to 98.60): VX0

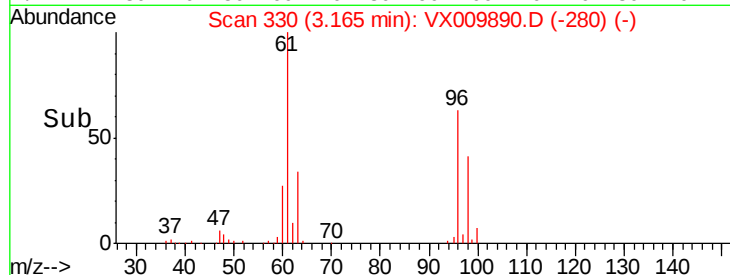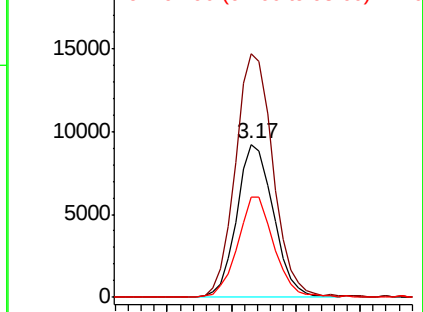

#25

2-Butanone

Concen: 0.369 ug/l

RT: 4.70 min Scan# 581

Delta R.T. 0.02 min

Lab File: VX009890.D


Acq: 24 May 2019 16:34

Tgt Ion: 43 Resp: 729



Ion Ratio Lower Upper


43 100

72 0.0 18.2 27.2#



Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 72.00 (71.70 to 72.70): VX0

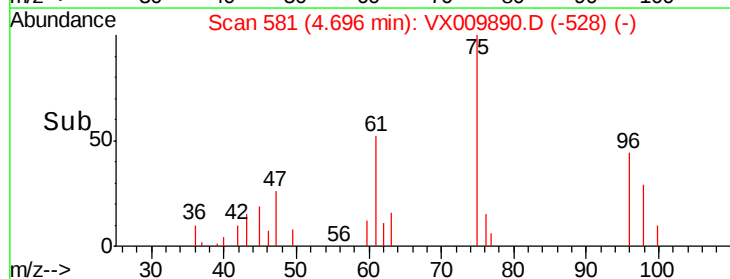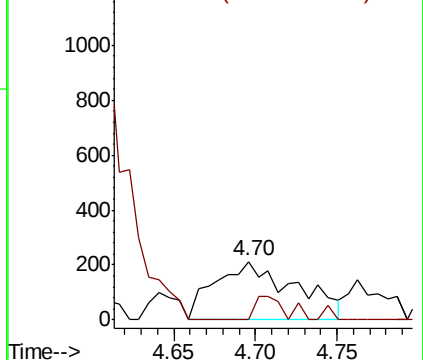




#27

cis-1,2-Dichloroethene
 Concen: 169.950 ug/l
 RT: 4.60 min Scan# 565
 Delta R.T. 0.01 min
 Lab File: VX009890.D
 Acq: 24 May 2019 16:34

Instrument :
 MSVOA_X
 ClientSampled :
 S32-0652

Tot Ion	96	Resp	357824
Ion	Ratio	Lower	Upper
96	100		
61	145.4	0.0	324.0
98	63.7	0.0	130.4






Abundance

Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0


Ion 97.90 (97.60 to 98.60): VX0

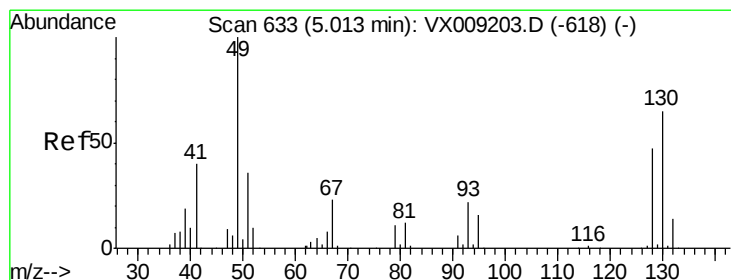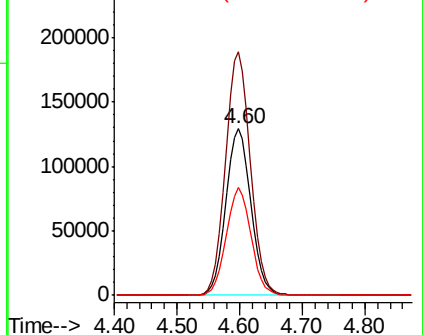

#28

Bromochloromethane
 Concen: Below Cal
 RT: 5.04 min Scan# 638
 Delta R.T. 0.03 min
 Lab File: VX009890.D
 Acq: 24 May 2019 16:34

Tgt Ion	49	Resp	40
Ion	Ratio	Lower	Upper
49	100		
129	0.0	0.0	3.8
130	0.0	51.2	76.8#






Abundance

Ion 48.90 (48.60 to 49.60): VX0

Ion 128.80 (128.50 to 129.50): V

Ion 129.80 (129.50 to 130.50): V

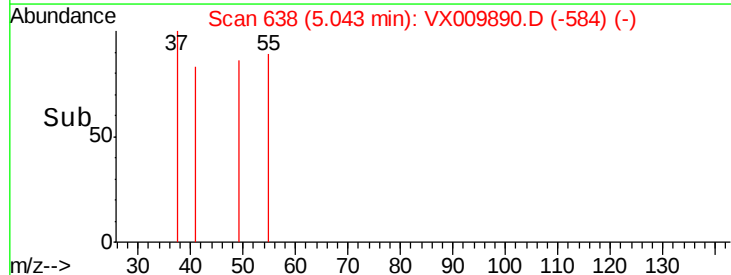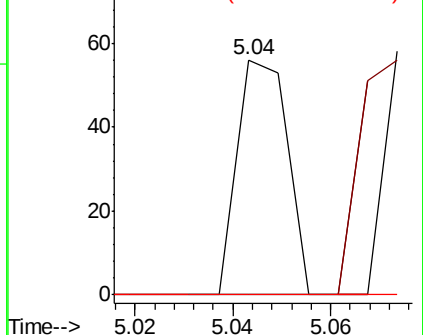







#31
Cyclohexane
Concen: 1.185 ug/l
RT: 5.67 min Scan# 740
Delta R.T. 0.09 min
Lab File: VX009890.D
Acq: 24 May 2019 16:34

Instrument :
MSVOA_X
ClientSampled :
S32-0652

Tot Ion: 56 Resp: 4147
Ion Ratio Lower Upper
56 100
69 174.7 23.4 35.0#
84 144.6 61.9 92.9#




Abundance Ion 56.00 (55.70 to 56.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 84.00 (83.70 to 84.70): VX0

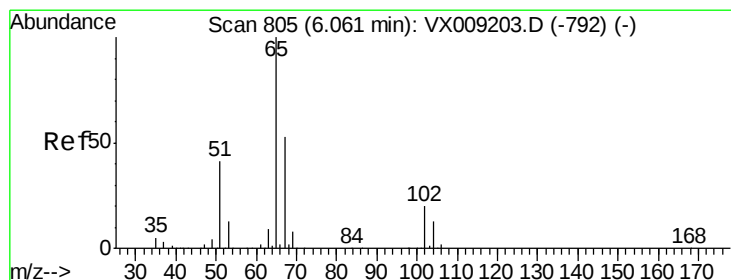
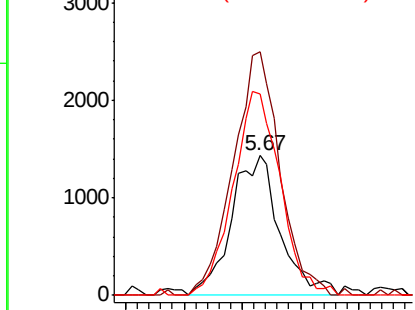



#33
1,2-Dichloroethane-d4
Concen: 50.848 ug/l
RT: 6.06 min Scan# 805
Delta R.T. -0.00 min
Lab File: VX009890.D
Acq: 24 May 2019 16:34

Tgt Ion: 65 Resp: 120328
Ion Ratio Lower Upper
65 100
67 53.1 0.0 106.6



Abundance Ion 64.90 (64.60 to 65.60): VX0
Ion 66.90 (66.60 to 67.60): VX0




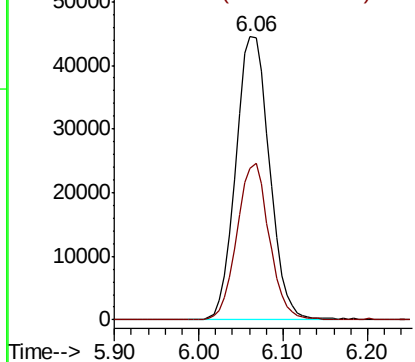




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. -0.00 min
 Lab File: VX009890.D
 Acq: 24 May 2019 16:34




Instrument :
 MSVOA_X
 ClientSampleId :
 S32-0652


Tot Ion	Ratio	Lower	Upper
114	100		
63	22.8	0.0	45.6
88	16.9	0.0	33.2

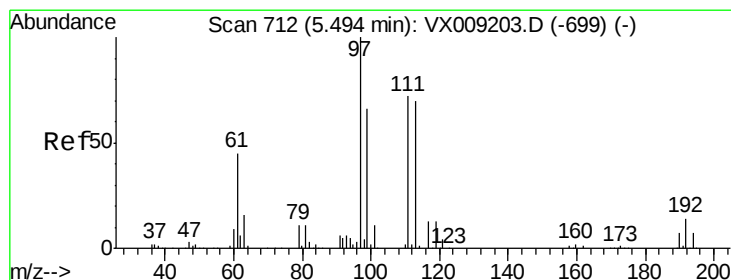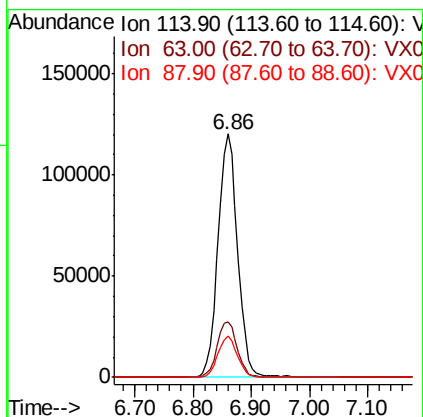

#35
 Dibromofluoromethane
 Concen: 48.901 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. 0.01 min
 Lab File: VX009890.D
 Acq: 24 May 2019 16:34

Tgt Ion	Ratio	Lower	Upper
113	100		
111	103.6	82.8	124.2
192	21.7	17.0	25.6

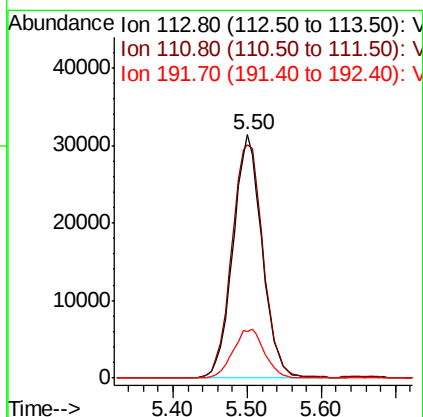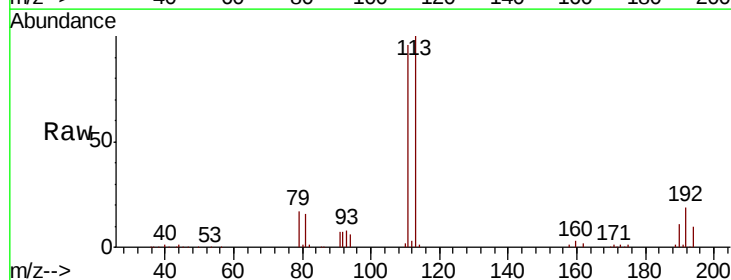

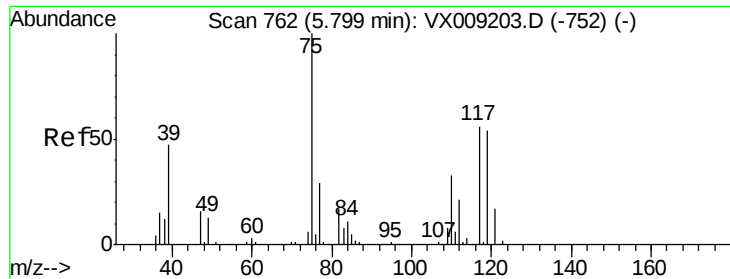

#36

1,1-Dichloropropene

Concen: 5.334 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.14 min

Lab File: VX009890.D

Acq: 24 May 2019 16:34

Instrument :

MSVOA_X

ClientSampleId :

S32-0652


Tot Ion: 75 Resp: 13862

Ion Ratio Lower Upper

75 100

110 9.0 16.9 50.6#




77 0.0 24.8 37.2#

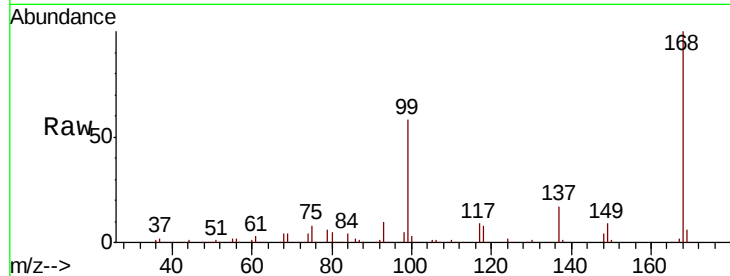

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

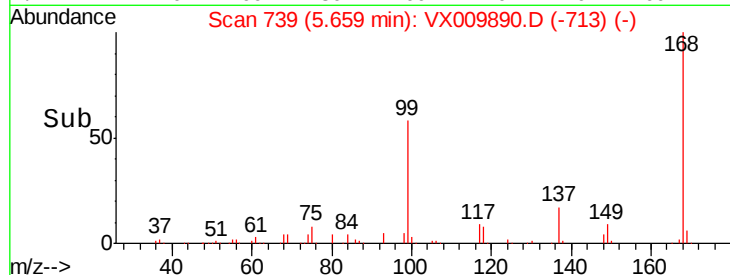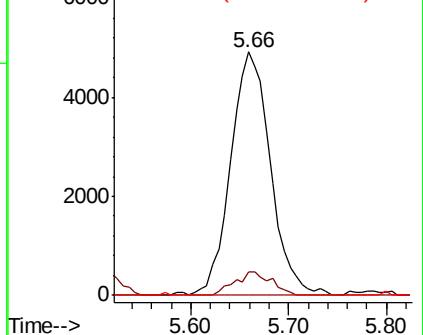

#38

Carbon Tetrachloride

Concen: 6.936 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.12 min

Lab File: VX009890.D

Acq: 24 May 2019 16:34


Tgt Ion: 117 Resp: 16376

Ion Ratio Lower Upper

117 100

119 4.6 77.5 116.3#



121 0.0 24.7 37.1#




Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

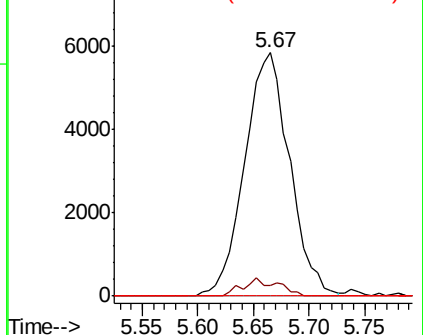



#40

Benzene

Concen: 0.238 ug/l

RT: 6.15 min Scan# 819

Delta R.T. 0.01 min

Lab File: VX009890.D

Acq: 24 May 2019 16:34

Instrument :

MSVOA_X

ClientSampled :


S32-0652

Tot Ion: 78 Resp: 1911

Ion Ratio Lower Upper

78 100

77 23.5 18.8 28.2



Abundance Ion 78.00 (77.70 to 78.70): VX0

Ion 77.00 (76.70 to 77.70): VX0

6.15

800



600

400

200

0

Time-->



#44

Trichloroethene

Concen: 2.683 ug/l

RT: 7.21 min Scan# 994

Delta R.T. -0.00 min

Lab File: VX009890.D


Acq: 24 May 2019 16:34

Tgt Ion:130 Resp: 5217

Ion Ratio Lower Upper

130 100

95 109.1 0.0 199.2



Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

7.21

3000

2500

2000


1500


1000

500

0

Time-->





#49

1,4-Dioxane

Concen: 0.395 ug/l

RT: 7.86 min Scan# 1100

Delta R.T. 0.12 min

Lab File: VX009890.D

Acq: 24 May 2019 16:34

Instrument :

MSVOA_X

ClientSampleId :

S32-0652


Tot Ion: 88 Resp: 23

Ion Ratio Lower Upper

88 100

43 834.8 28.6 42.8#




58 0.0 61.7 92.5#

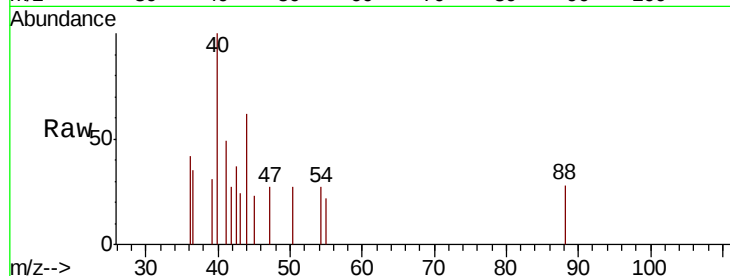

Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

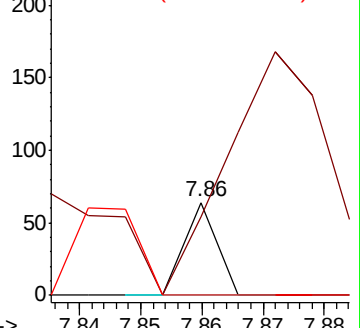

#50

Toluene-d8

Concen: 50.215 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX009890.D


Acq: 24 May 2019 16:34

Tgt Ion: 98 Resp: 356376

Ion Ratio Lower Upper



98 100


100 63.6 51.2 76.8



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

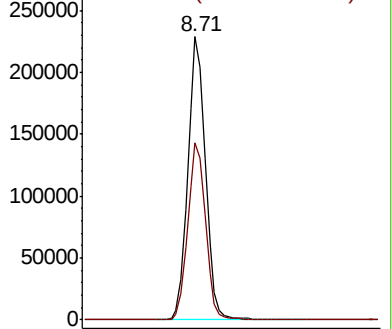



#62

4-Bromofluorobenzene

Concen: 46.570 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.00 min

Lab File: VX009890.D

Acq: 24 May 2019 16:34

Instrument :

MSVOA_X

ClientSampleId :

S32-0652


Tot Ion: 95 Resp: 120092

Ion Ratio Lower Upper

95 100

174 81.0 0.0 161.6




176 78.4 0.0 159.2

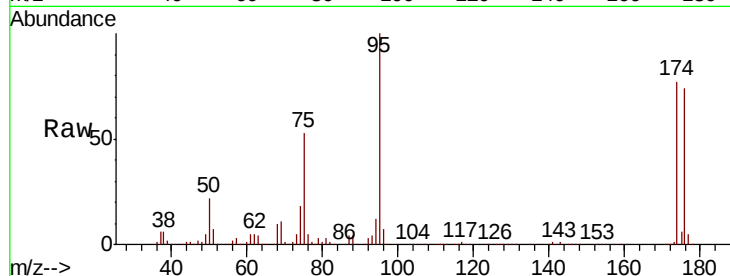

Abundance Ion 94.90 (94.60 to 95.60): VX009890.D (-1588) (-)

Ion 173.80 (173.50 to 174.50): VX009890.D (-1588) (-)

Ion 175.80 (175.50 to 176.50): VX009890.D (-1588) (-)

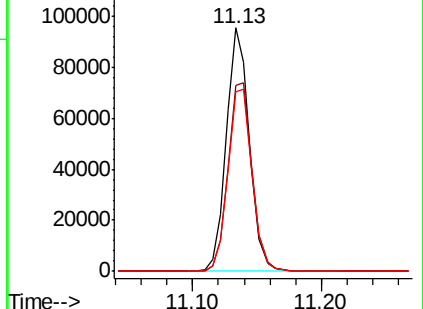

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. -0.00 min

Lab File: VX009890.D

Acq: 24 May 2019 16:34


Tgt Ion: 117 Resp: 249772

Ion Ratio Lower Upper

117 100

82 60.5 48.8 73.2



119 32.2 25.8 38.6




Abundance Ion 116.90 (116.60 to 117.60): VX009890.D (-1420) (-)

Ion 82.00 (81.70 to 82.70): VX009890.D (-1420) (-)

Ion 118.90 (118.60 to 119.60): VX009890.D (-1420) (-)



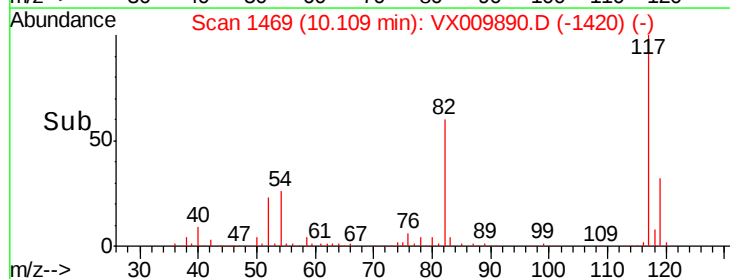
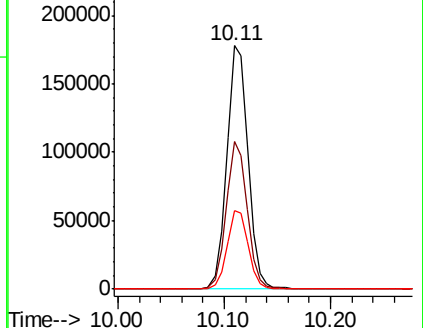




#65
Chlorobenzene
Concen: 0.481 ug/l
RT: 10.14 min Scan# 1474
Delta R.T. 0.01 min
Lab File: VX009890.D
Acq: 24 May 2019 16:34




Instrument :
MSVOA_X
ClientSampleId :
S32-0652


Tot Ion:112 Resp: 2403
Ion Ratio Lower Upper
112 100
114 36.3 25.5 38.3

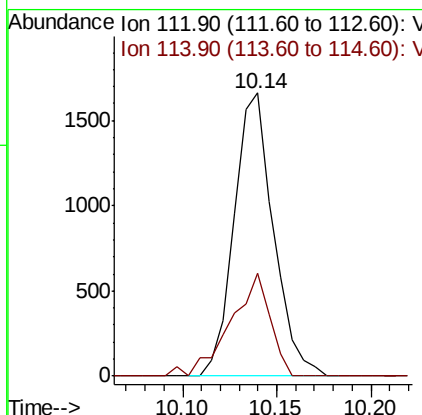

#69
o-Xylene
Concen: 0.338 ug/l
RT: 10.70 min Scan# 1566
Delta R.T. -0.00 min
Lab File: VX009890.D
Acq: 24 May 2019 16:34

Tgt Ion:106 Resp: 1121
Ion Ratio Lower Upper
106 100
91 215.3 109.5 328.4

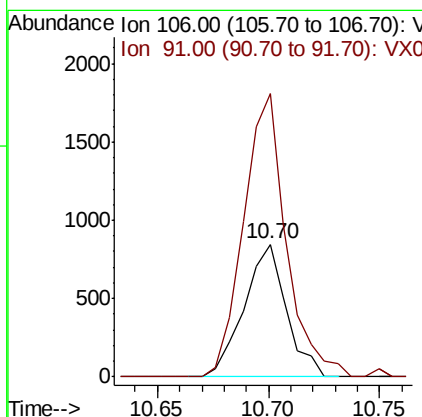

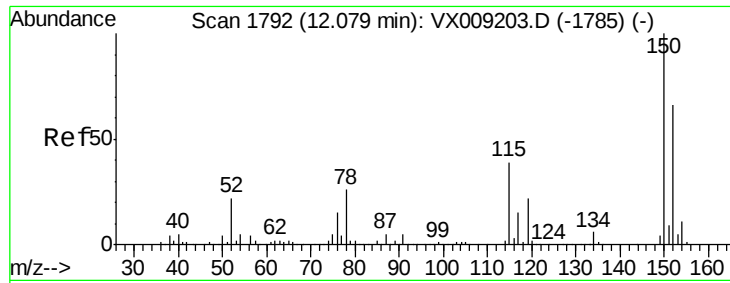

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX009890.D

Acq: 24 May 2019 16:34

Instrument :

MSVOA_X

ClientSampleId :

S32-0652


Tot Ion:152 Resp: 108254

Ion Ratio Lower Upper

152 100

115 58.9 41.2 123.6




150 157.2 0.0 346.4

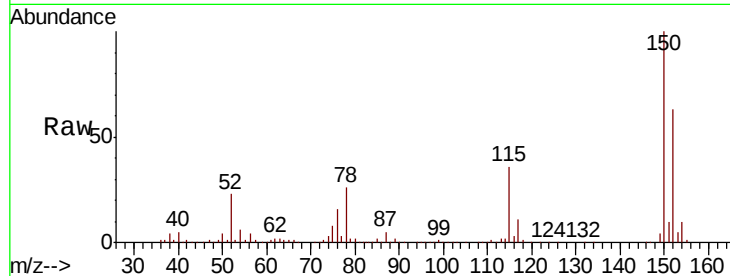

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

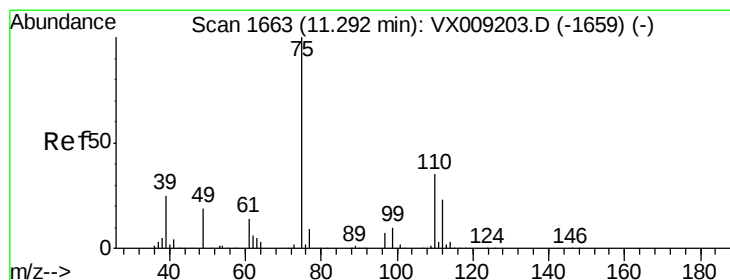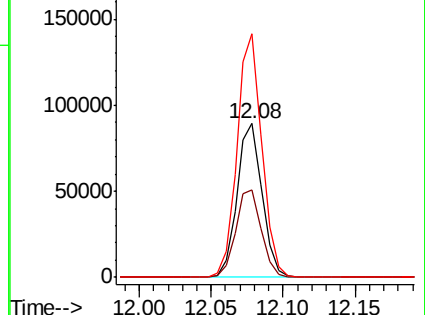

#76

1,2,3-Trichloropropane

Concen: 24.958 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.16 min

Lab File: VX009890.D


Acq: 24 May 2019 16:34

Tgt Ion: 75 Resp: 62672

Ion Ratio Lower Upper



75 100


77 1.3 22.1 66.1#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

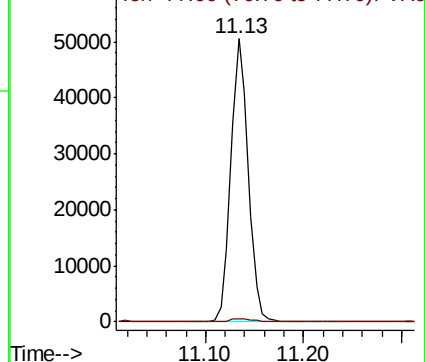

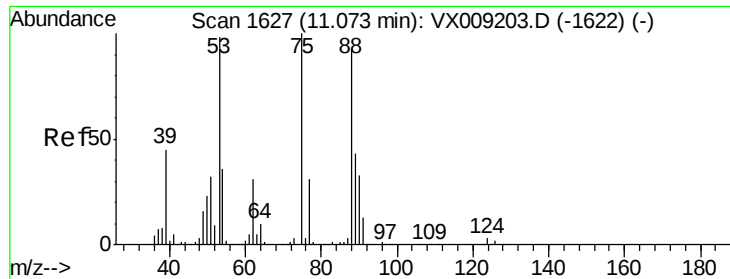

#81

trans-1,4-Dichloro-2-butene

Concen: 63.858 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.06 min

Lab File: VX009890.D

Acq: 24 May 2019 16:34

Instrument :

MSVOA_X

ClientSampleId :

S32-0652


Tot Ion: 75 Resp: 62672

Ion Ratio Lower Upper

75 100

53 0.1 79.0 118.6#




89 0.0 34.7 52.1#

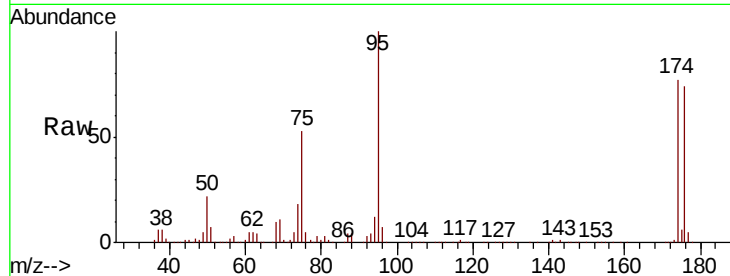

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

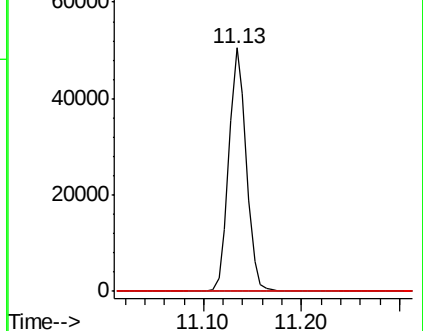

#90

Hexachloroethane

Concen: 0.287 ug/l

RT: 12.70 min Scan# 1894

Delta R.T. 0.10 min

Lab File: VX009890.D


Acq: 24 May 2019 16:34

Tgt Ion: 117 Resp: 336

Ion Ratio Lower Upper

117 100

201 0.0 42.3 126.9#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 200.70 (200.40 to 201.40): V

