

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052421\
 Data File : VX022158.D
 Acq On : 24 May 2021 19:21
 Operator : JC/MD
 Sample : M2504-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-104

Quant Time: May 25 02:09:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 19 14:23:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	70194	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	144410	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	125477	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	51212	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	55745	51.48	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	102.96%
35) Dibromofluoromethane	5.397	113	44599	48.70	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.40%
50) Toluene-d8	8.653	98	178339	50.55	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	101.10%
62) 4-Bromofluorobenzene	11.085	95	62941	48.27	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	96.54%


Target Compounds						Qvalue
5) Bromomethane	1.618	94	190	0.33	ug/l #	62
6) Chloroethane	1.691	64	805	1.39	ug/l #	43
10) Methyl Iodide	2.447	142	218	0.24	ug/l #	80
11) Tert butyl alcohol	2.947	59	313	1.26	ug/l #	73
13) Acrolein	2.258	56	80	0.49	ug/l #	14
16) Acetone	2.392	43	1189	2.52	ug/l #	83
18) Methyl Acetate	2.709	43	438	0.35	ug/l #	47
20) Methylene Chloride	2.794	84	269	0.26	ug/l #	68
25) 2-Butanone	4.568	43	174	0.23	ug/l #	45
31) Cyclohexane	5.483	56	550	0.40	ug/l #	77
36) 1,1-Dichloropropene	5.568	75	6599	4.94	ug/l #	46
38) Carbon Tetrachloride	5.562	117	7635	5.84	ug/l #	15
39) Methylcyclohexane	7.391	83	633	0.42	ug/l #	84
40) Benzene	6.056	78	1169	0.28	ug/l #	84
55) 1,1,2-Trichloroethane	9.104	97	225	0.21	ug/l #	15
60) Dibromochloromethane	9.275	129	710	0.69	ug/l #	11
64) Tetrachloroethene	9.281	164	787	0.96	ug/l #	73
67) Ethyl Benzene	10.195	91	20864	4.34	ug/l	99
68) m/p-Xylenes	10.311	106	13338	7.34	ug/l	98
73) Isopropylbenzene	10.970	105	1483	0.34	ug/l	97
76) 1,2,3-Trichloropropane	11.085	75	31897	25.25	ug/l #	38
78) n-propylbenzene	11.305	91	3467	0.68	ug/l	96
79) 2-Chlorotoluene	11.384	91	1550	0.50	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.457	105	6455	1.80	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.085	75	31897	59.82	ug/l #	12
82) 4-Chlorotoluene	11.457	91	903	0.25	ug/l #	45
84) 1,2,4-Trimethylbenzene	11.756	105	21361	5.91	ug/l	100
85) sec-Butylbenzene	11.756	105	21361	4.88	ug/l #	57
89) n-Butylbenzene	12.329	91	733	0.21	ug/l #	66
90) Hexachloroethane	12.561	117	139	0.23	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	12.695	75	62	0.20	ug/l #	1
95) Naphthalene	13.780	128	10803	2.70	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052421\
Data File : VX022158.D
Acq On : 24 May 2021 19:21
Operator : JC/MD
Sample : M2504-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-104

Quant Time: May 25 02:09:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260
QLast Update : Wed May 19 14:23:10 2021
Response via : Initial Calibration




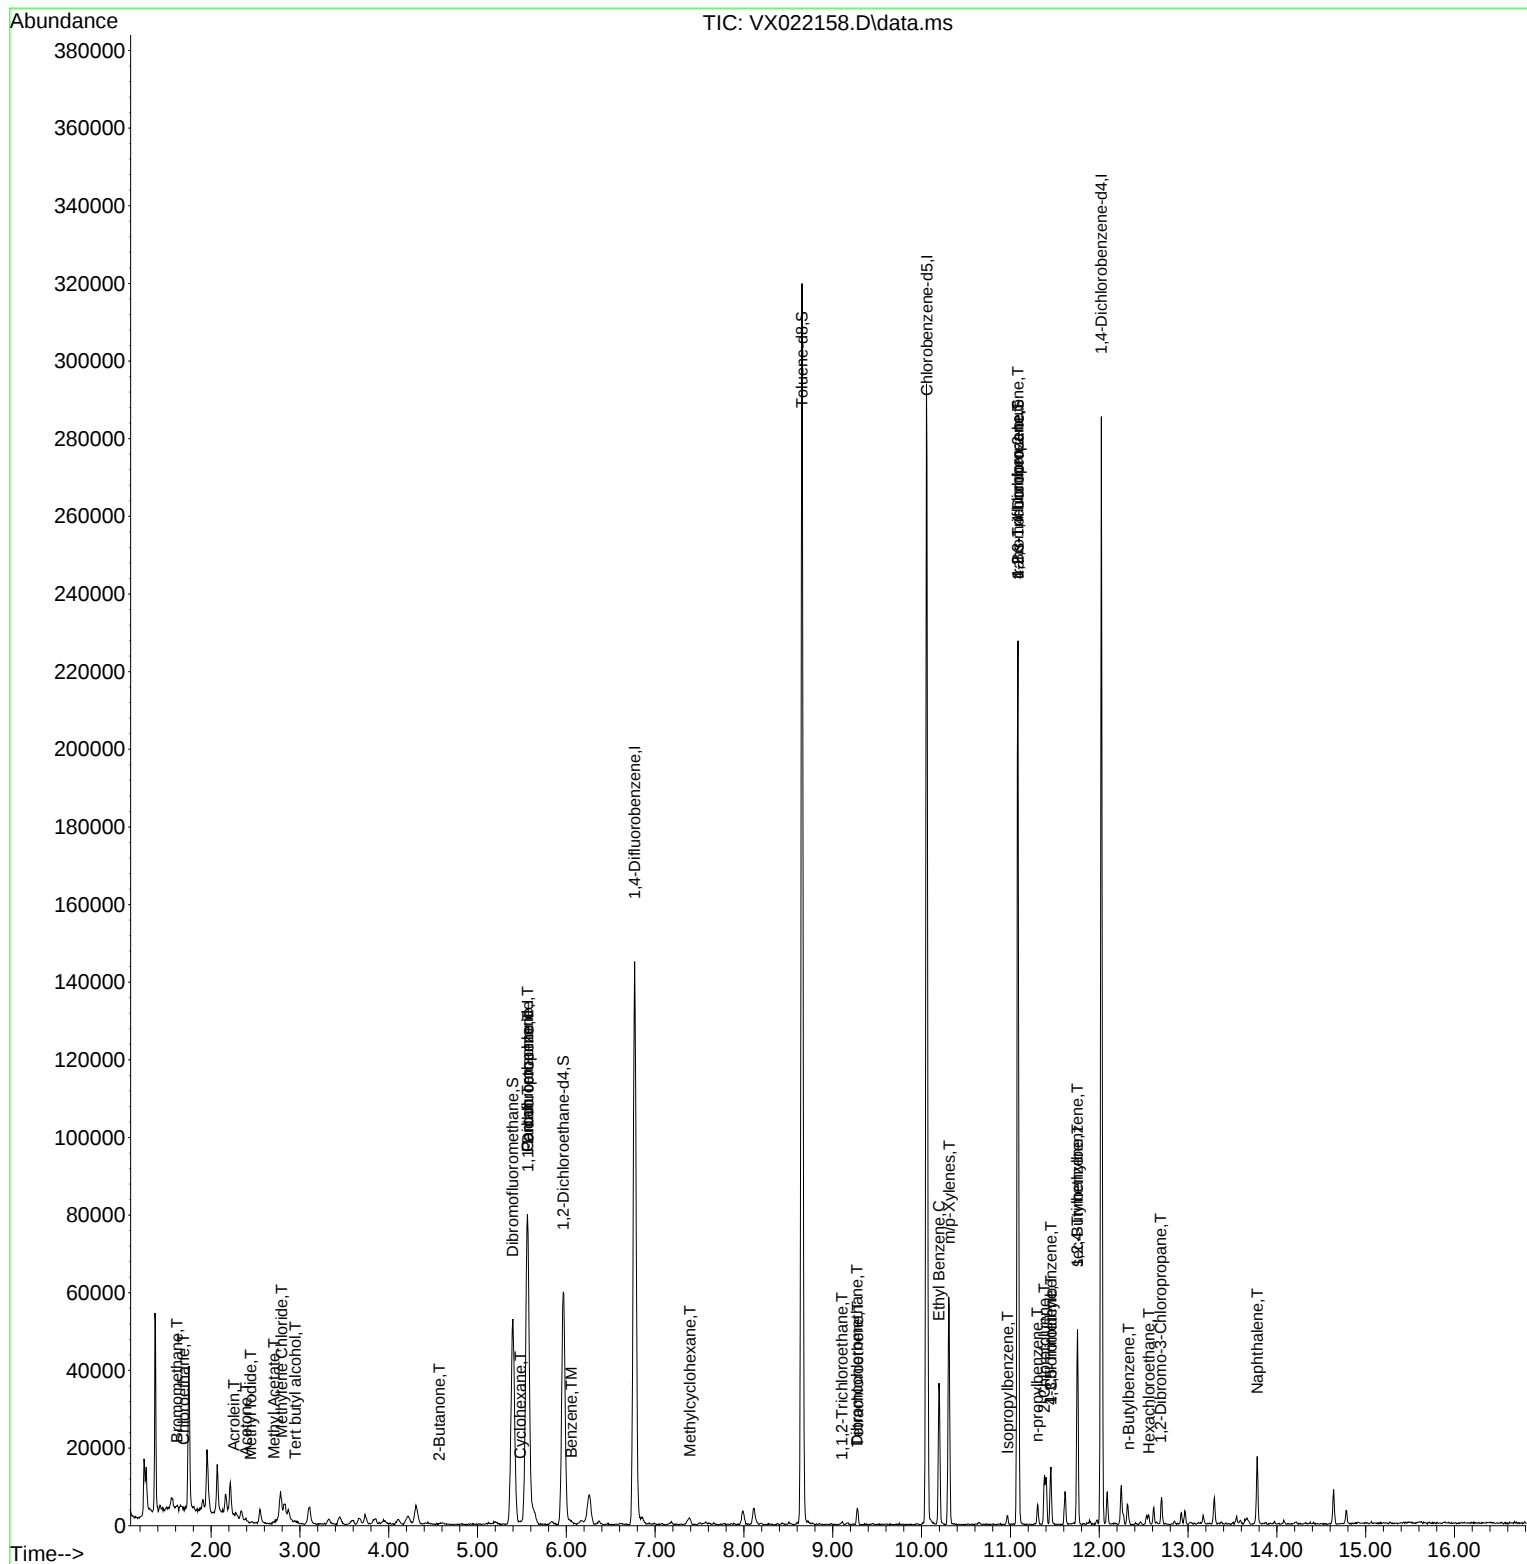




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21




Instrument :
MSVOA_X
ClientSampleId :
MW-104


Tgt Ion:168 Resp: 70194
Ion Ratio Lower Upper
168 100
99 66.1 45.8 68.6



#5
Bromomethane
Concen: 0.33 ug/l
RT: 1.618 min Scan# 87
Delta R.T. 0.006 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Tgt Ion: 94 Resp: 190
Ion Ratio Lower Upper
94 100
96 58.8 76.4 114.6#


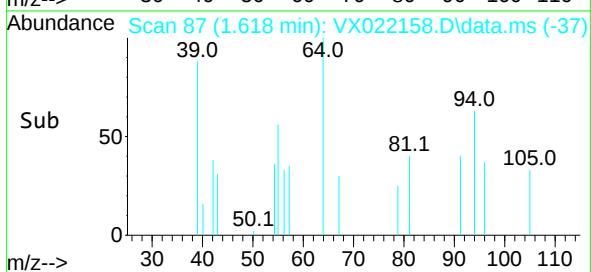

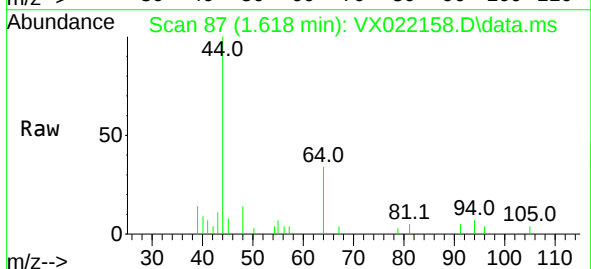


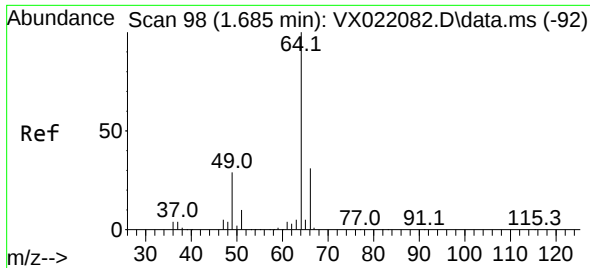

#6
Chloroethane
Concen: 1.39 ug/l
RT: 1.691 min Scan# 99
Delta R.T. 0.006 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21




Instrument :
MSVOA_X
ClientSampled :
MW-104


Tgt Ion: 64 Resp: 805
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.0#

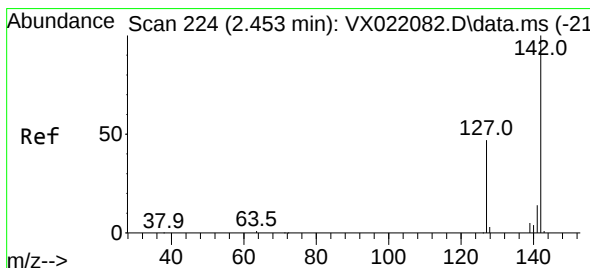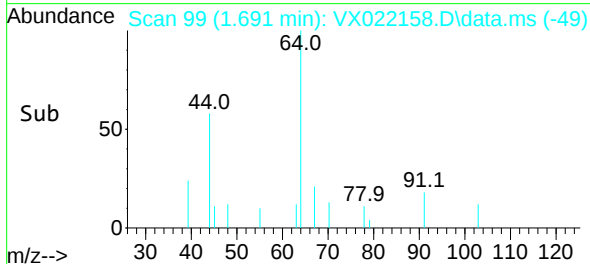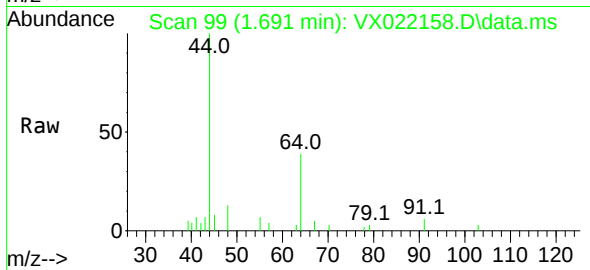

#10
Methyl Iodide
Concen: 0.24 ug/l
RT: 2.447 min Scan# 223
Delta R.T. -0.006 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Tgt Ion: 142 Resp: 218
Ion Ratio Lower Upper
142 100
127 32.1 33.3 49.9#
141 0.0 11.4 17.0#

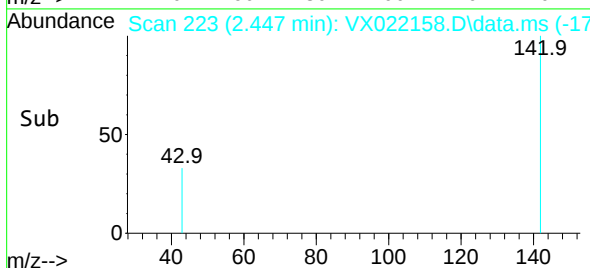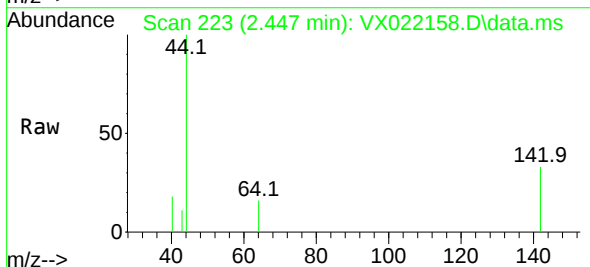




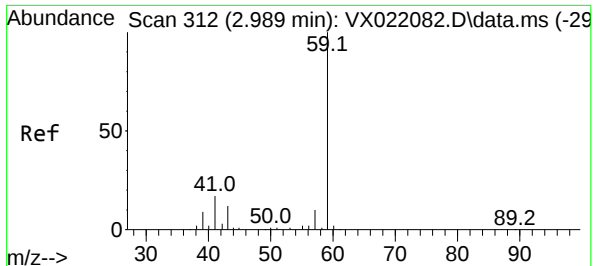


#11

Tert butyl alcohol
Concen: 1.26 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.042 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Instrument :
MSVOA_X
ClientSampled :
MW-104




Tgt Ion: 59 Resp: 313
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#

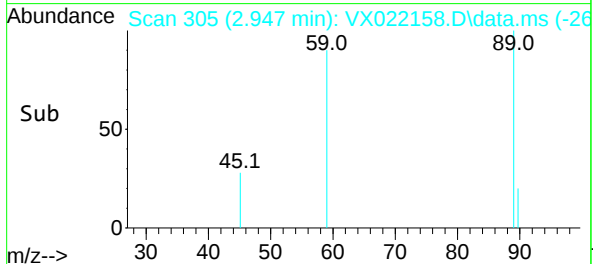


#13

Acrolein
Concen: 0.49 ug/l
RT: 2.258 min Scan# 192
Delta R.T. 0.018 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Tgt Ion: 56 Resp: 80
Ion Ratio Lower Upper
56 100
55 0.0 56.4 84.6#


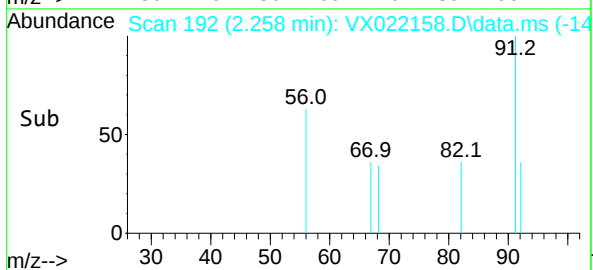

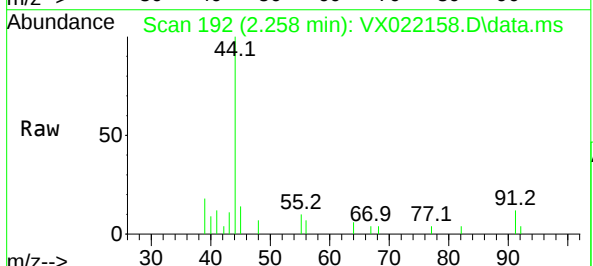


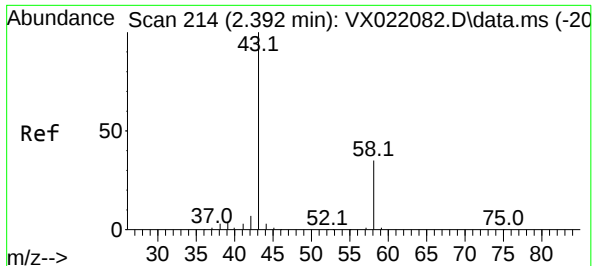

#16
Acetone
Concen: 2.52 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.000 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21




Instrument :
MSVOA_X
ClientSampled :
MW-104


Tgt Ion: 43 Resp: 1189
Ion Ratio Lower Upper
43 100
58 24.9 27.8 41.8#

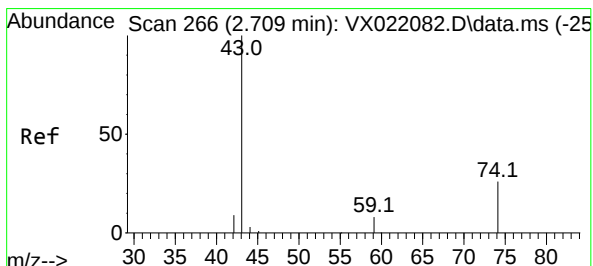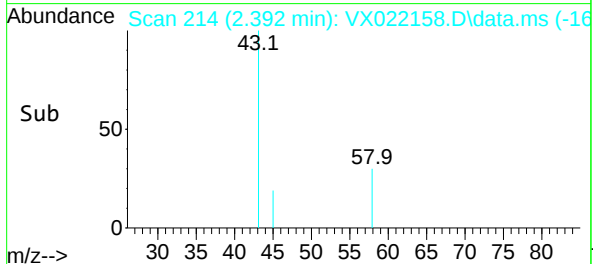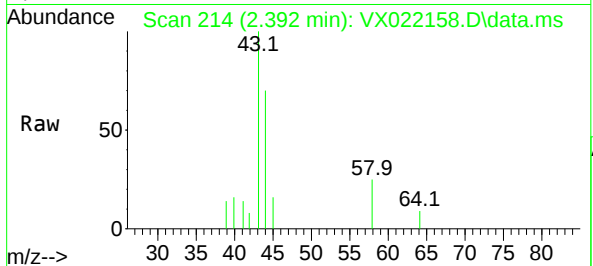

#18
Methyl Acetate
Concen: 0.35 ug/l
RT: 2.709 min Scan# 266
Delta R.T. -0.000 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Tgt Ion: 43 Resp: 438
Ion Ratio Lower Upper
43 100
74 0.0 21.9 32.9#

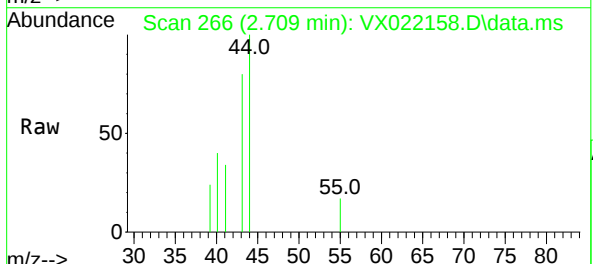







#20
Methylene Chloride
Concen: 0.26 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Instrument :
MSVOA_X
ClientSampleId :
MW-104

Tgt Ion: 84 Resp: 269




Ion	Ratio	Lower	Upper
84	100		
49	126.2	88.6	132.8
51	32.3	27.0	40.6
86	124.4	50.3	75.5#




#25
2-Butanone
Concen: 0.23 ug/l
RT: 4.568 min Scan# 571
Delta R.T. 0.000 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Tgt Ion: 43 Resp: 174

Ion	Ratio	Lower	Upper
43	100		
72	0.0	23.7	35.5#









#31
Cyclohexane
Concen: 0.40 ug/l
RT: 5.483 min Scan# 721
Delta R.T. -0.000 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21




Instrument :
MSVOA_X
ClientSampleId :
MW-104


Tgt Ion: 56 Resp: 550
Ion Ratio Lower Upper
56 100
69 44.3 25.3 37.9#
84 67.4 71.4 107.0#

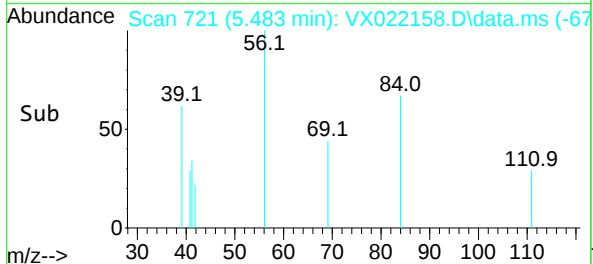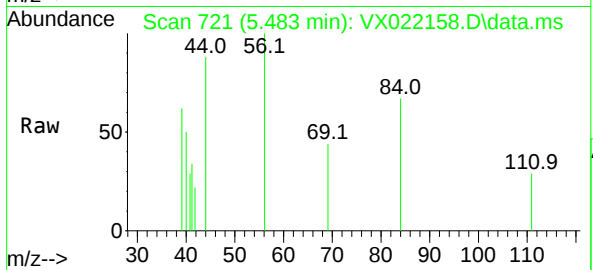

#33
1,2-Dichloroethane-d4
Concen: 51.48 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Tgt Ion: 65 Resp: 55745
Ion Ratio Lower Upper
65 100
67 53.6 0.0 105.4




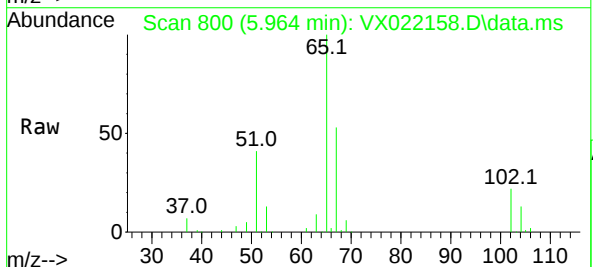


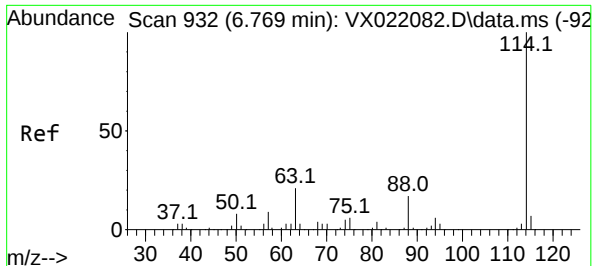

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21




Instrument :
MSVOA_X
ClientSampleId :
MW-104


Tgt Ion:114 Resp: 144410
Ion Ratio Lower Upper
114 100
63 21.0 0.0 40.8
88 16.6 0.0 32.8

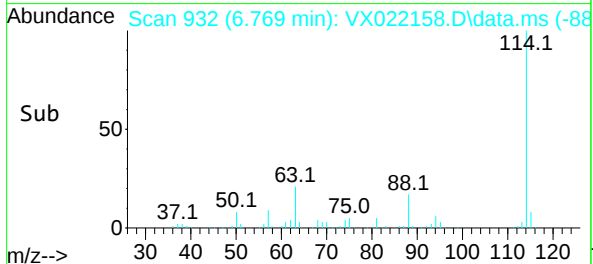

#35
Dibromofluoromethane
Concen: 48.70 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.006 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Tgt Ion:113 Resp: 44599
Ion Ratio Lower Upper
113 100
111 101.9 81.9 122.9
192 16.7 16.7 25.1

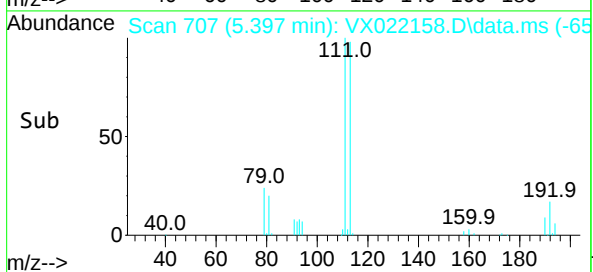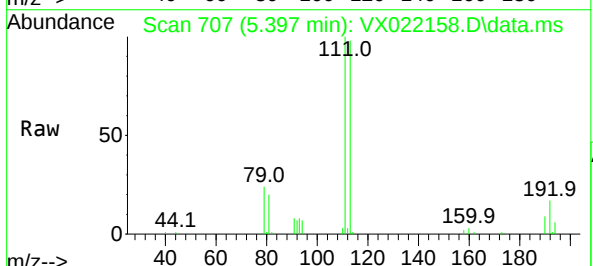

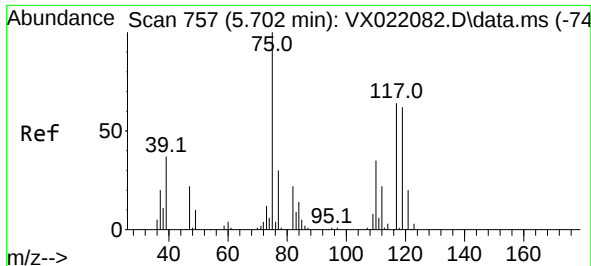

#36

1,1-Dichloropropene

Concen: 4.94 ug/l

RT: 5.568 min Scan# 735

Delta R.T. -0.134 min

Lab File: VX022158.D

Acq: 24 May 2021 19:21

Tgt Ion: 75 Resp: 6599

Ion Ratio Lower Upper

75 100

110 6.0 18.1 54.4#





77 0.0 25.3 37.9#

Instrument :

MSVOA_X

ClientSampleId :

MW-104

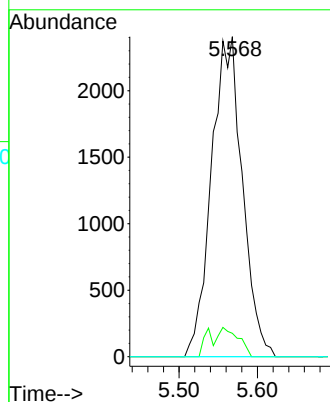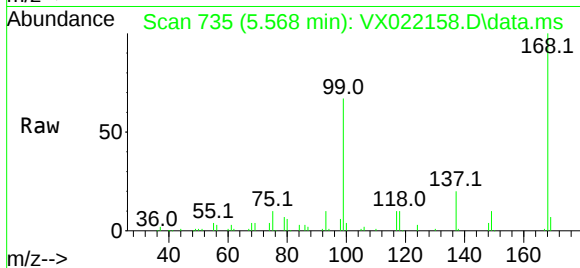

#38

Carbon Tetrachloride

Concen: 5.84 ug/l

RT: 5.562 min Scan# 734

Delta R.T. -0.128 min

Lab File: VX022158.D

Acq: 24 May 2021 19:21




Tgt Ion: 117 Resp: 7635


Ion Ratio Lower Upper

117 100

119 4.1 76.2 114.2#

121 0.0 24.8 37.2#

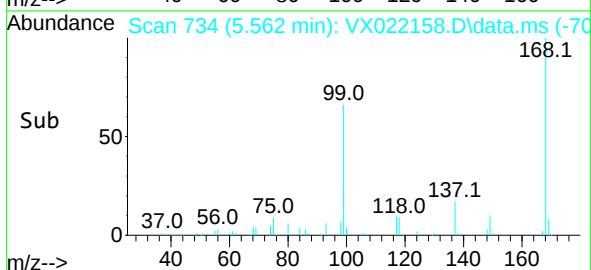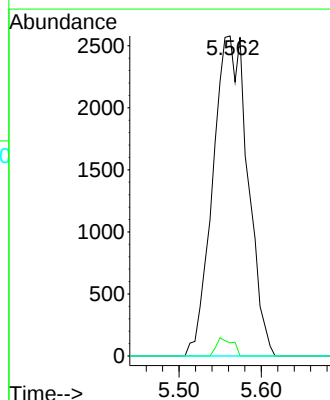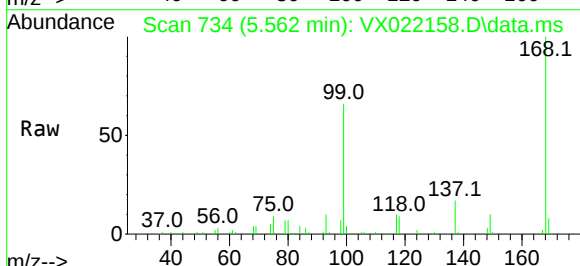



#39

Methylcyclohexane

Concen: 0.42 ug/l

RT: 7.391 min Scan# 1034





Delta R.T. 0.006 min

Lab File: VX022158.D

Acq: 24 May 2021 19:21

Tgt Ion:	83	Resp:	633
Ion	Ratio	Lower	Upper
83	100		
55	84.5	58.9	88.3
98	33.3	38.1	57.1#

Instrument :
MSVOA_X
ClientSampleId :
MW-104

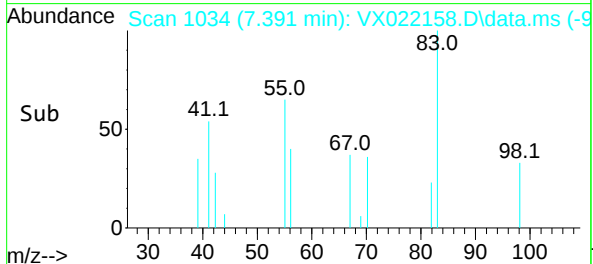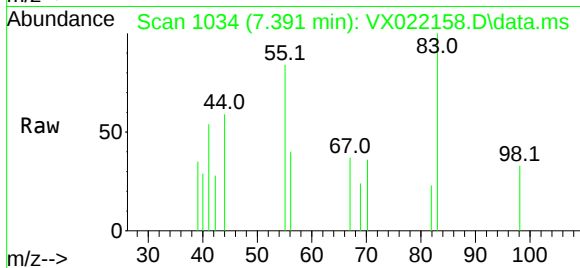

#40

Benzene

Concen: 0.28 ug/l




RT: 6.056 min Scan# 815


Delta R.T. 0.012 min

Lab File: VX022158.D

Acq: 24 May 2021 19:21

Tgt Ion:	78	Resp:	1169
Ion	Ratio	Lower	Upper
78	100		
77	31.7	18.9	28.3#


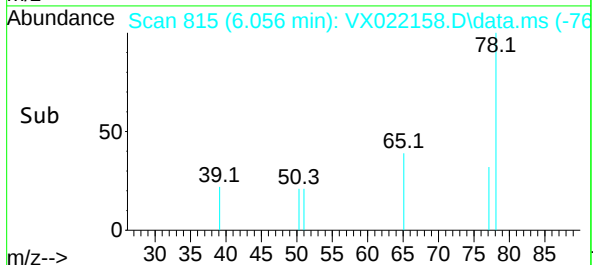

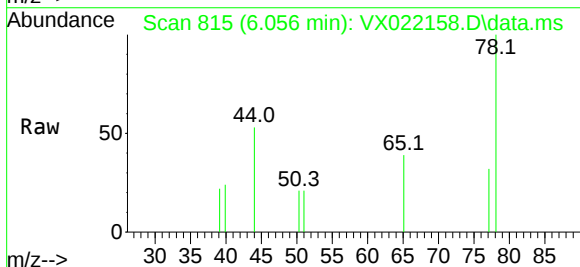




#50
Toluene-d8
Concen: 50.55 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21




Instrument :
MSVOA_X
ClientSampleId :
MW-104


Tgt Ion: 98 Resp: 178339
Ion Ratio Lower Upper
98 100
100 64.7 51.9 77.9

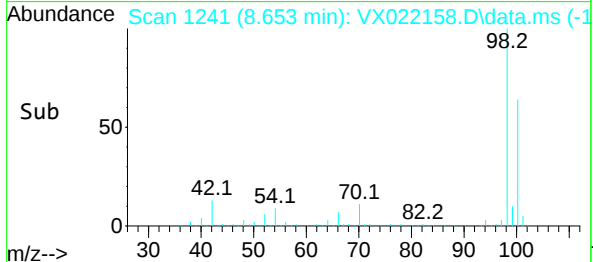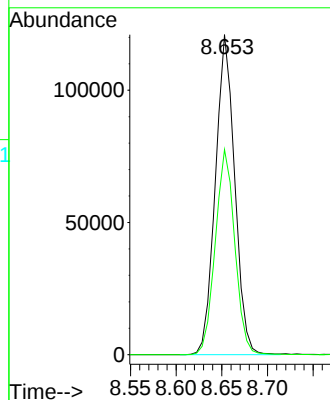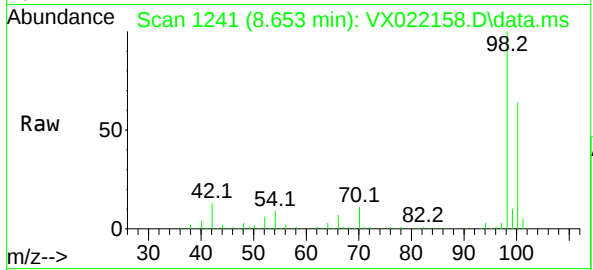

#55
1,1,2-Trichloroethane
Concen: 0.21 ug/l
RT: 9.104 min Scan# 1315
Delta R.T. -0.055 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Tgt Ion: 97 Resp: 225
Ion Ratio Lower Upper
97 100
83 0.0 69.3 103.9#
85 0.0 44.3 66.5#
99 0.0 50.3 75.5#



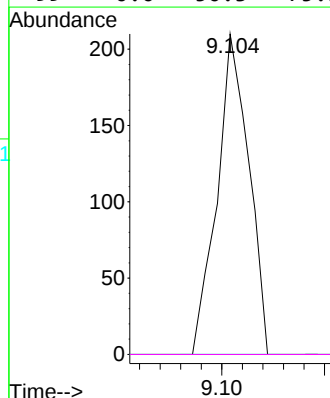
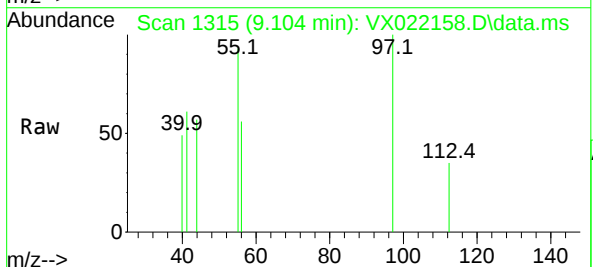


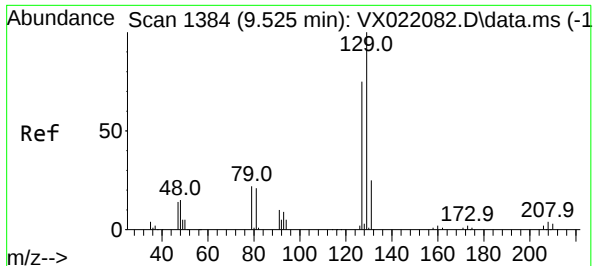

#60
Dibromochloromethane
Concen: 0.69 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.250 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21




Instrument :
MSVOA_X
ClientSampleId :
MW-104


Tgt Ion:129 Resp: 710
Ion Ratio Lower Upper
129 100
127 0.0 38.4 115.2#

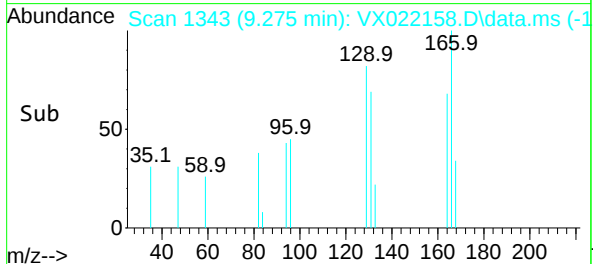

#62
4-Bromofluorobenzene
Concen: 48.27 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Tgt Ion: 95 Resp: 62941
Ion Ratio Lower Upper
95 100
174 62.9 0.0 154.6
176 60.7 0.0 155.8


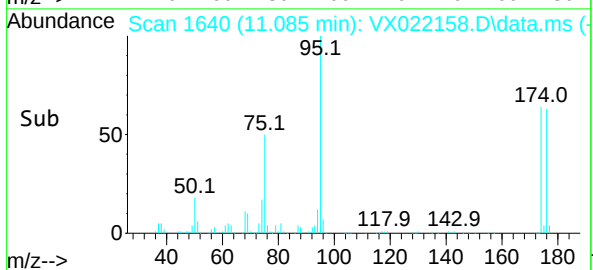

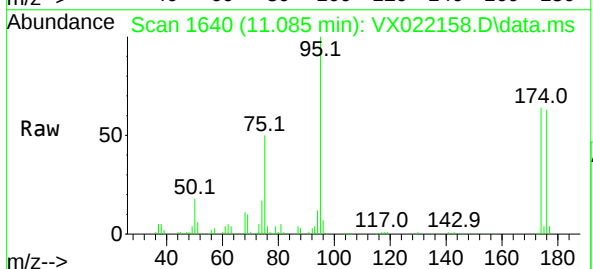




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. 0.000 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21




Instrument :
MSVOA_X
ClientSampleId :
MW-104


Tgt Ion:117 Resp: 125477
Ion Ratio Lower Upper
117 100
82 55.1 47.4 71.2
119 31.8 26.6 39.8

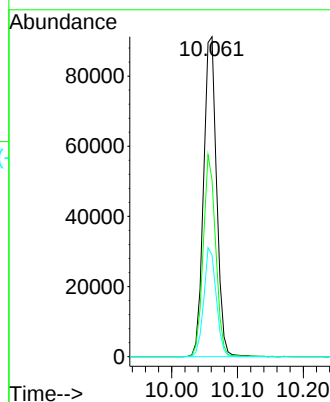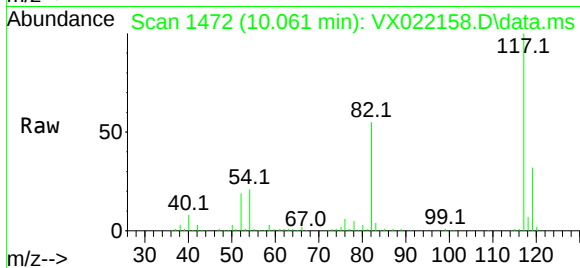

#64
Tetrachloroethene
Concen: 0.96 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. 0.006 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Tgt Ion:164 Resp: 787
Ion Ratio Lower Upper
164 100
166 87.6 103.4 155.2#
129 55.6 70.8 106.2#
131 85.1 72.5 108.7


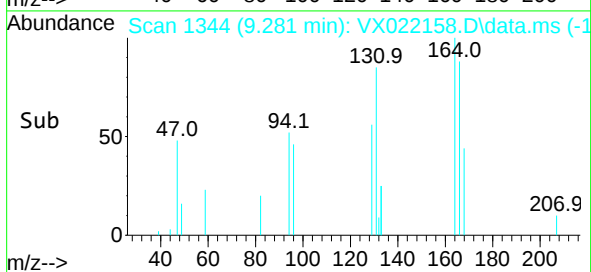
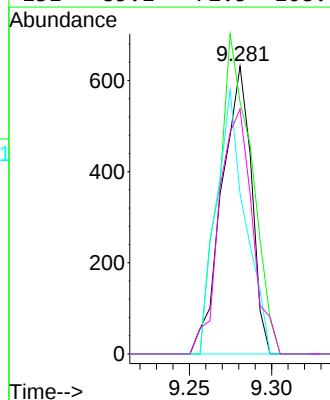
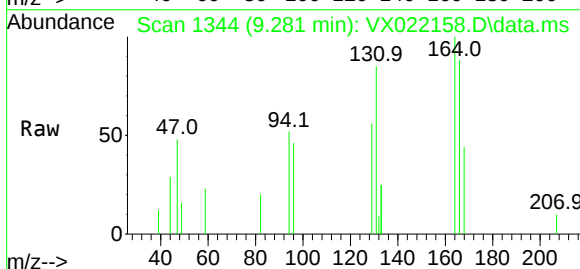




#67
Ethyl Benzene
Concen: 4.34 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21




Instrument :
MSVOA_X
ClientSampleId :
MW-104


Tgt Ion: 91 Resp: 20864
Ion Ratio Lower Upper
91 100
106 31.3 24.6 37.0

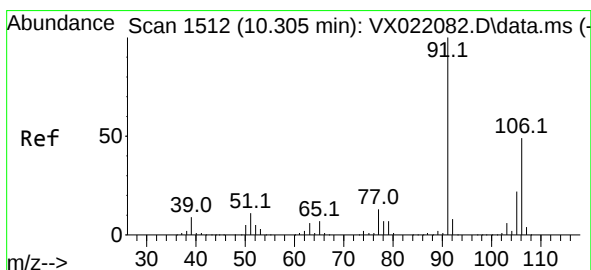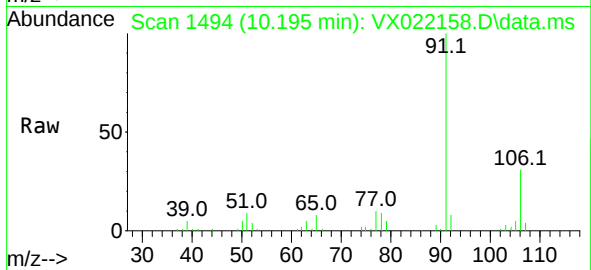

#68
m/p-Xylenes
Concen: 7.34 ug/l
RT: 10.311 min Scan# 1513
Delta R.T. 0.006 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Tgt Ion: 106 Resp: 13338
Ion Ratio Lower Upper
106 100
91 201.2 162.8 244.2


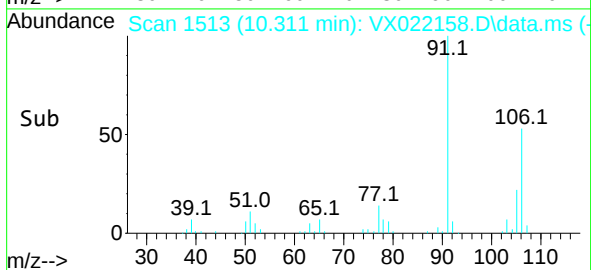

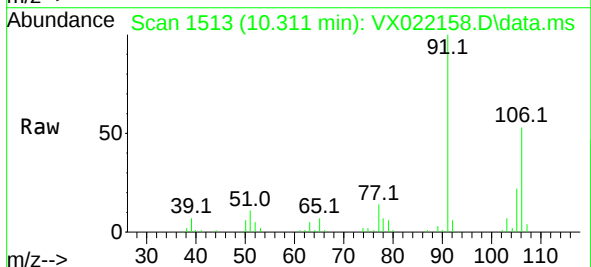




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21




Instrument :
MSVOA_X
ClientSampleId :
MW-104


Tgt Ion:152 Resp: 51212
Ion Ratio Lower Upper
152 100
115 67.6 41.1 123.3
150 159.1 0.0 349.0

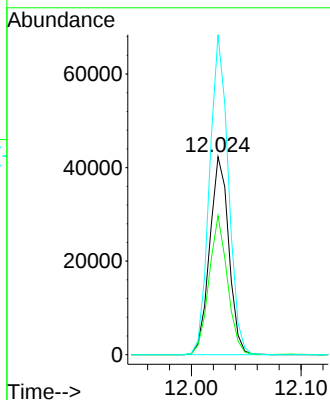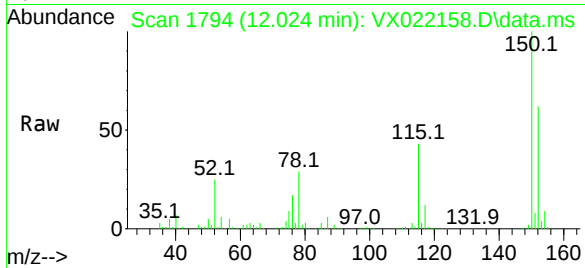

#73
Isopropylbenzene
Concen: 0.34 ug/l
RT: 10.970 min Scan# 1621
Delta R.T. 0.006 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Tgt Ion:105 Resp: 1483
Ion Ratio Lower Upper
105 100
120 25.1 13.2 39.6


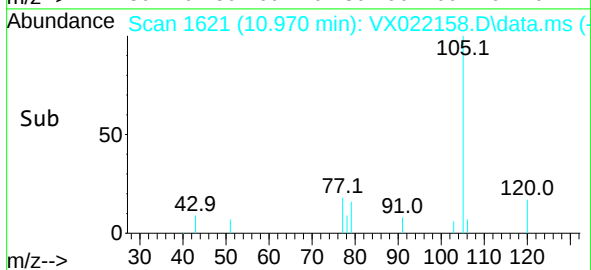
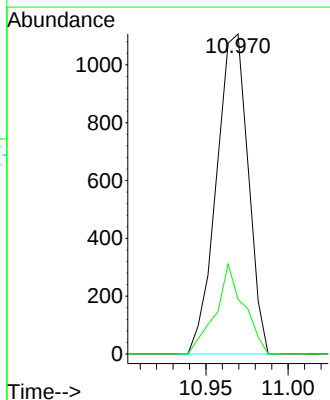
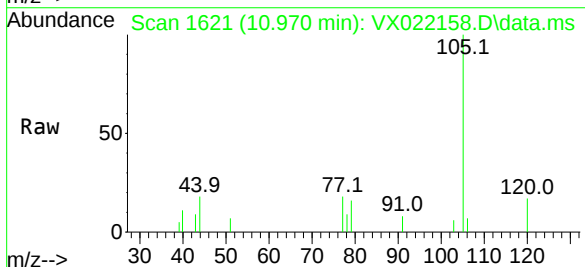




#76
1,2,3-Trichloropropane
Concen: 25.25 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21




Instrument :
MSVOA_X
ClientSampled :
MW-104


Tgt Ion: 75 Resp: 31897
Ion Ratio Lower Upper
75 100
77 0.9 19.1 57.5#



#78
n-propylbenzene
Concen: 0.68 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Tgt Ion: 91 Resp: 3467
Ion Ratio Lower Upper
91 100
120 21.2 11.5 34.5









#79
2-Chlorotoluene
Concen: 0.50 ug/l
RT: 11.384 min Scan# 1689
Delta R.T. 0.018 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21




Instrument :
MSVOA_X
ClientSampled :
MW-104


Tgt Ion: 91 Resp: 1550
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.8#

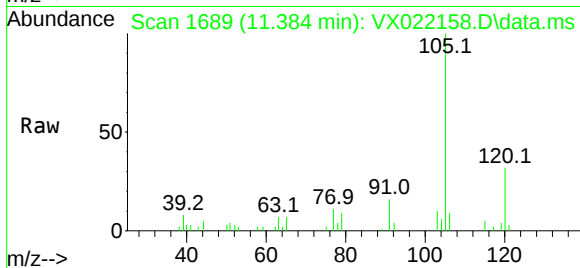

#80
1,3,5-Trimethylbenzene
Concen: 1.80 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Tgt Ion: 105 Resp: 6455
Ion Ratio Lower Upper
105 100
120 49.0 23.8 71.5


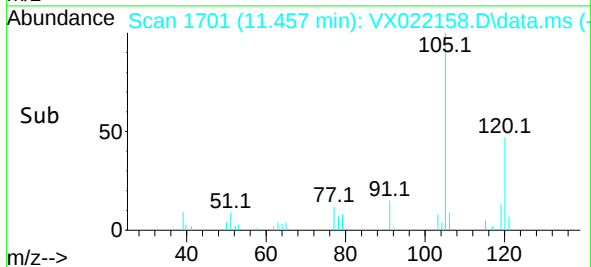

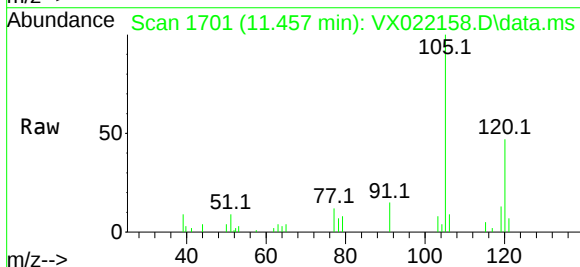




#81
trans-1,4-Dichloro-2-butene
Concen: 59.82 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.060 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21




Instrument :
MSVOA_X
ClientSampleId :
MW-104


Tgt Ion: 75 Resp: 31897
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#

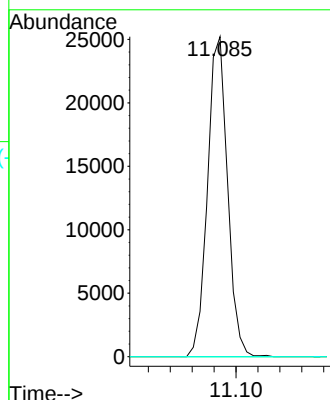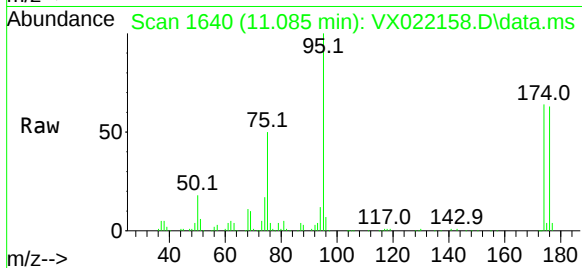

#82
4-Chlorotoluene
Concen: 0.25 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Tgt Ion: 91 Resp: 903
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#


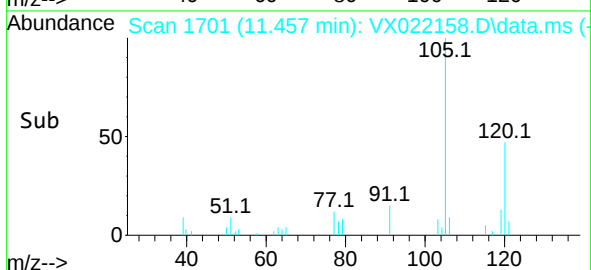
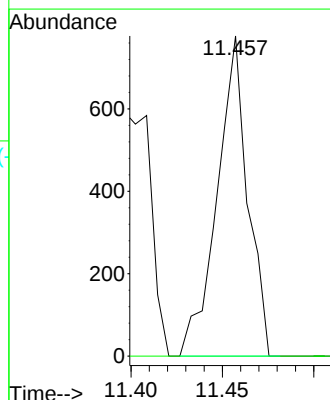
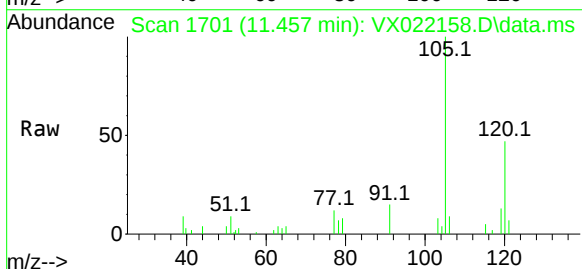


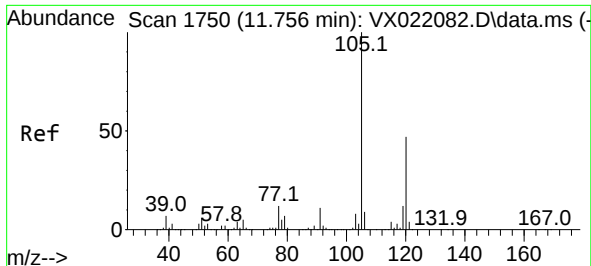

#84
1,2,4-Trimethylbenzene
Concen: 5.91 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21




Instrument :
MSVOA_X
ClientSampleId :
MW-104


Tgt Ion:105 Resp: 21361
Ion Ratio Lower Upper
105 100
120 45.0 22.4 67.3

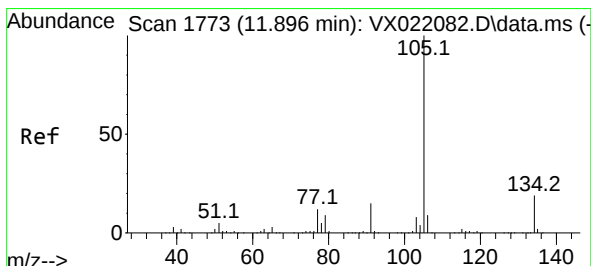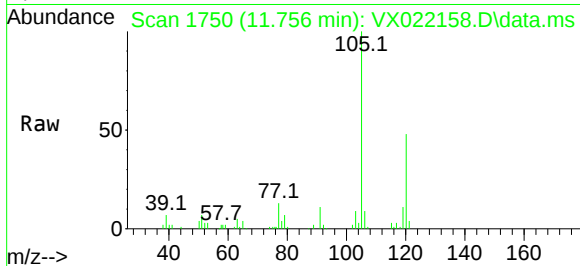

#85
sec-Butylbenzene
Concen: 4.88 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.140 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Tgt Ion:105 Resp: 21361
Ion Ratio Lower Upper
105 100
134 0.0 10.0 29.8#


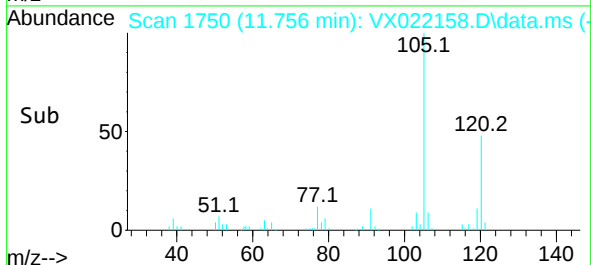

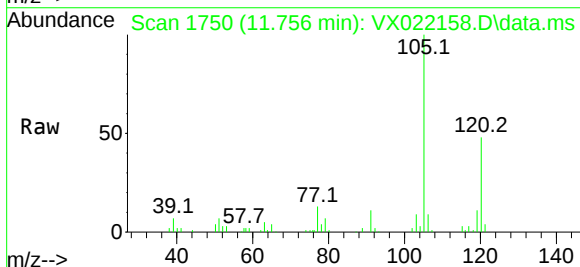




#89
n-Butylbenzene
Concen: 0.21 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. -0.006 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21




Instrument :
MSVOA_X
ClientSampled :
MW-104


Tgt Ion: 91 Resp: 733
Ion Ratio Lower Upper
91 100
92 36.3 27.4 82.0
134 0.0 13.2 39.5#

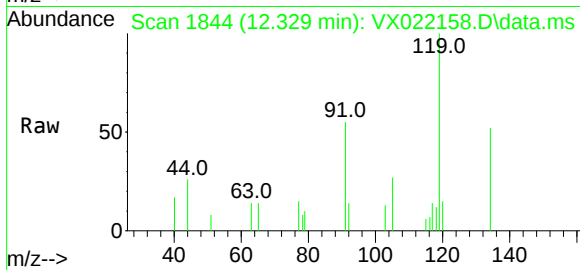

#90
Hexachloroethane
Concen: 0.23 ug/l
RT: 12.561 min Scan# 1882
Delta R.T. 0.018 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Tgt Ion: 117 Resp: 139
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#


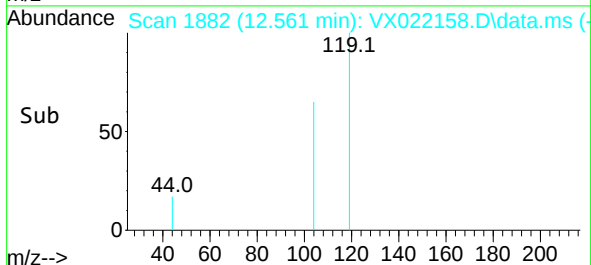

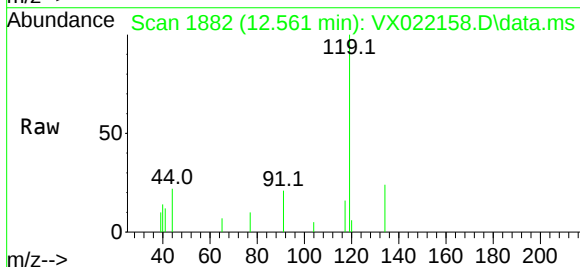




#92
1,2-Dibromo-3-Chloropropane
Concen: 0.20 ug/l
RT: 12.695 min Scan# 1904
Delta R.T. -0.250 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Instrument :
MSVOA_X
ClientSampleId :
MW-104

Tgt Ion: 75 Resp: 62
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#

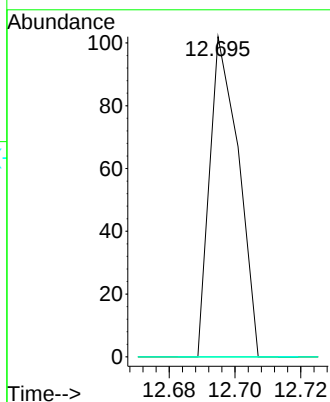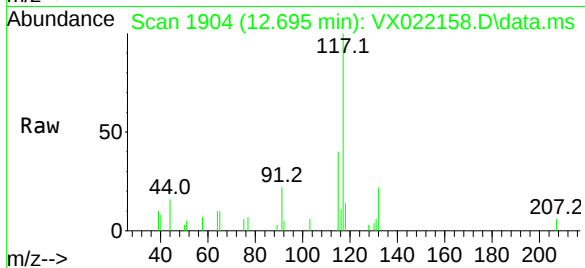

#95
Naphthalene
Concen: 2.70 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX022158.D
Acq: 24 May 2021 19:21

Tgt Ion: 128 Resp: 10803
Ion Ratio Lower Upper
128 100
127 11.5 10.3 15.5
129 11.1 8.8 13.2

