

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052422\
 Data File : VX028933.D
 Acq On : 24 May 2022 19:48
 Operator : JC/MD
 Sample : N2980-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Quant Time: May 25 01:52:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 12 14:58:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	335395	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	598451	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	566692	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	263412	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	231595	50.374	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	100.740%
35) Dibromofluoromethane	5.385	113	196726	50.173	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	100.340%
50) Toluene-d8	8.653	98	711985	48.163	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	96.320%
62) 4-Bromofluorobenzene	11.079	95	276159	50.016	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	100.040%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052422\
Data File : VX028933.D
Acq On : 24 May 2022 19:48
Operator : JC/MD
Sample : N2980-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Time: May 25 01:52:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260
QLast Update : Thu May 12 14:58:53 2022
Response via : Initial Calibration




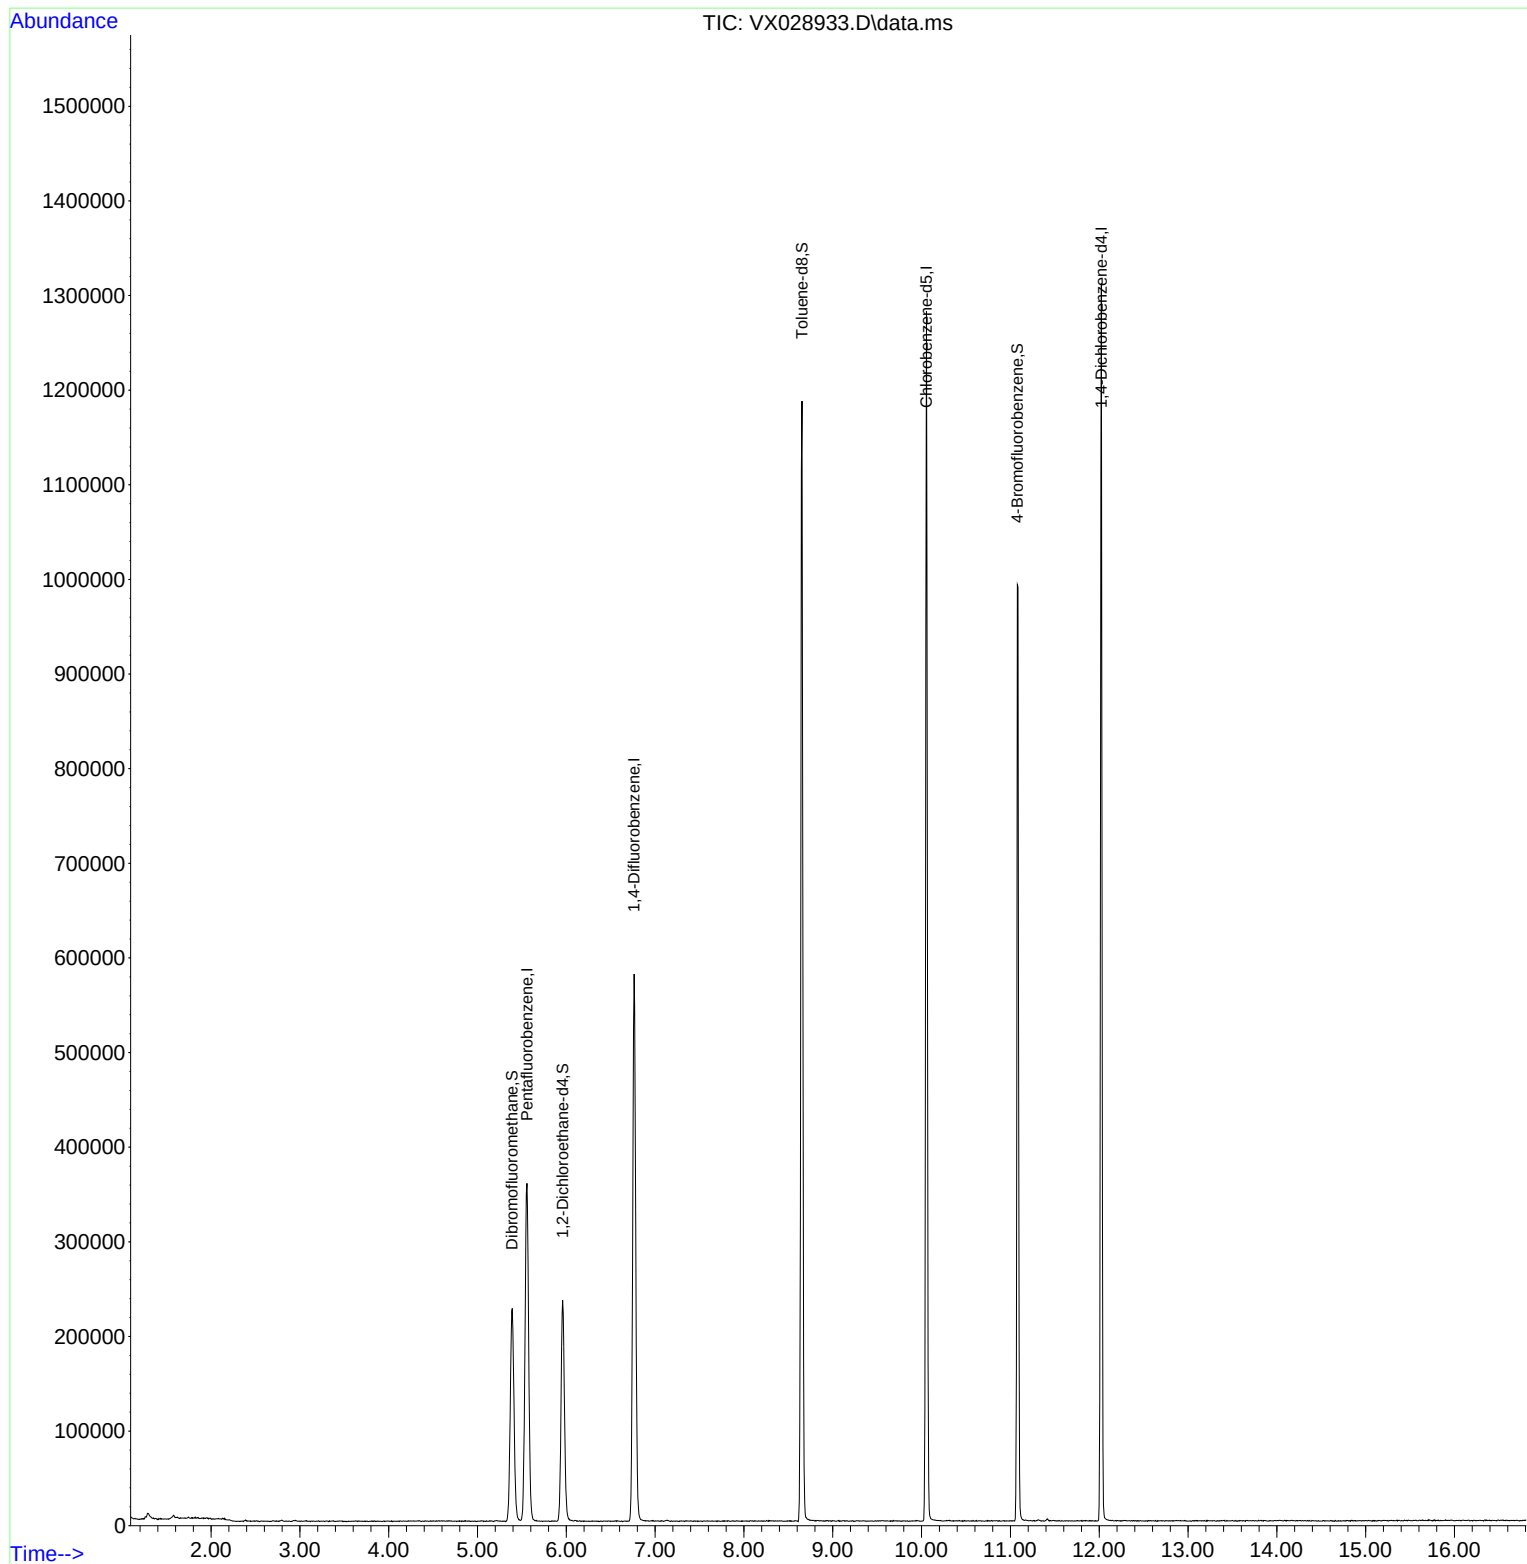


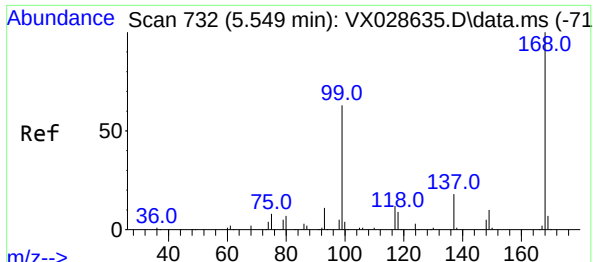

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.007 min
Lab File: VX028933.D
Acq: 24 May 2022 19:48




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion:168 Resp: 335395
Ion Ratio Lower Upper
168 100
99 60.8 41.7 62.5

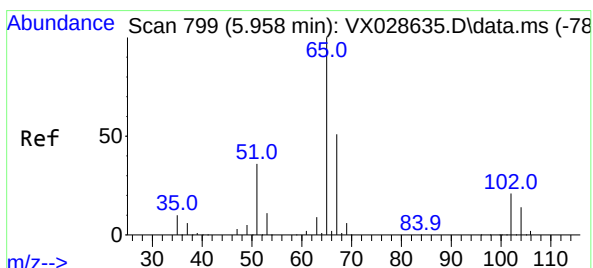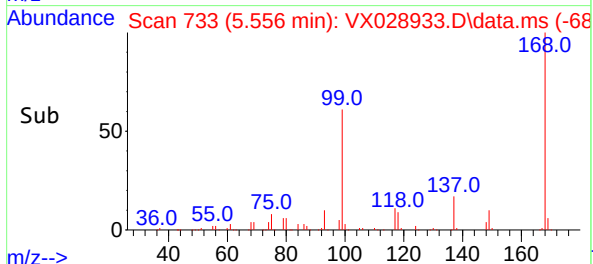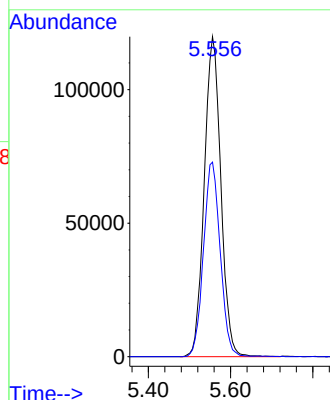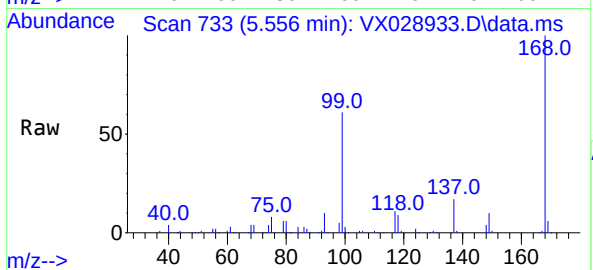

#33
1,2-Dichloroethane-d4
Concen: 50.374 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028933.D
Acq: 24 May 2022 19:48

Tgt Ion: 65 Resp: 231595
Ion Ratio Lower Upper
65 100
67 50.6 0.0 107.4

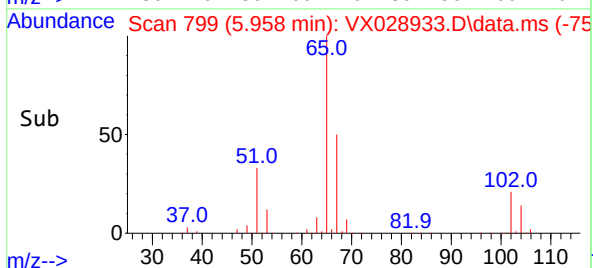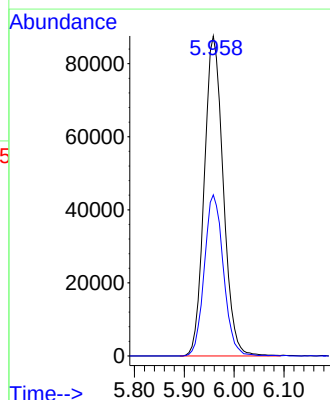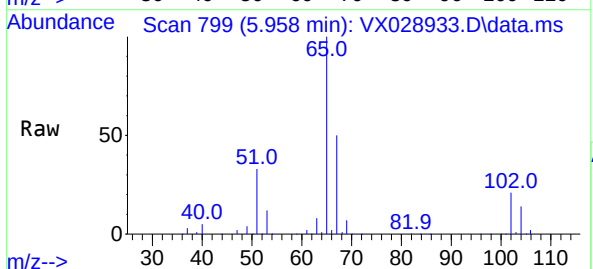




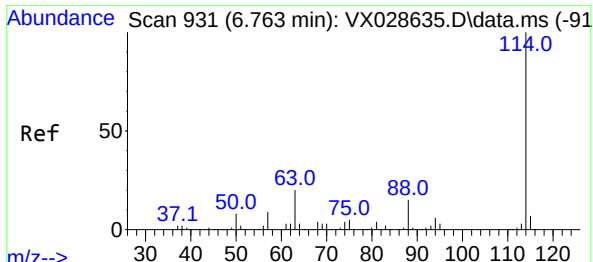


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX028933.D
Acq: 24 May 2022 19:48

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Tgt Ion:114 Resp: 598451




Ion	Ratio	Lower	Upper
114	100		
63	20.0	0.0	36.8
88	16.8	0.0	32.4

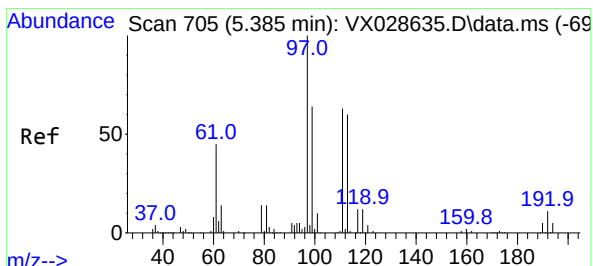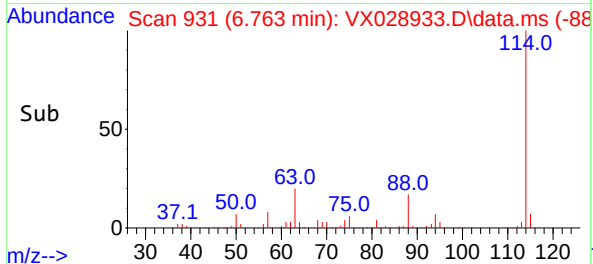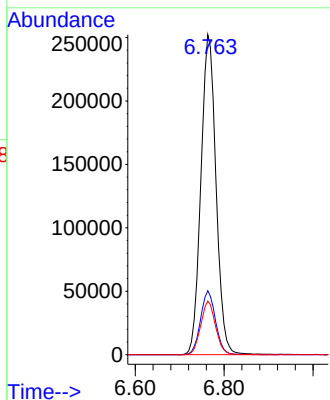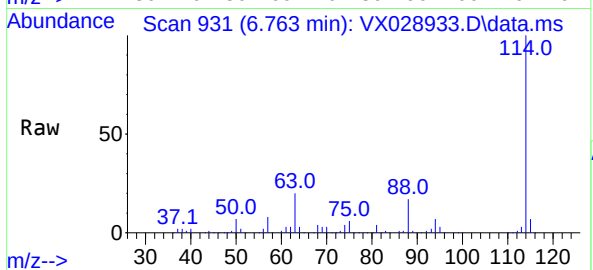


#35
Dibromofluoromethane
Concen: 50.173 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX028933.D
Acq: 24 May 2022 19:48

Tgt Ion:113 Resp: 196726

Ion	Ratio	Lower	Upper
113	100		
111	103.1	82.8	124.2
192	19.1	16.9	25.3


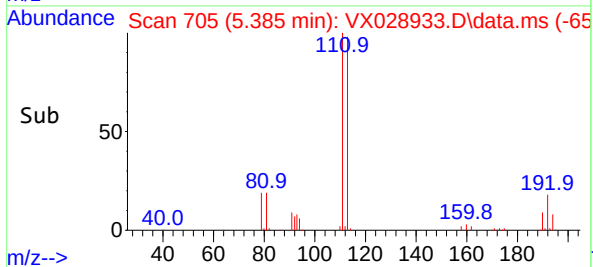
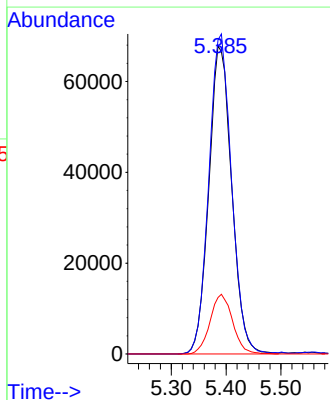
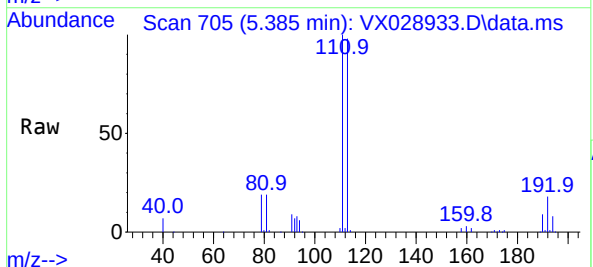


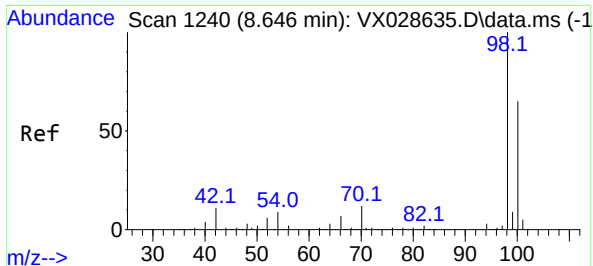

#50
Toluene-d8
Concen: 48.163 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.007 min
Lab File: VX028933.D
Acq: 24 May 2022 19:48




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion: 98 Resp: 711985
Ion Ratio Lower Upper
98 100
100 66.7 52.6 78.8

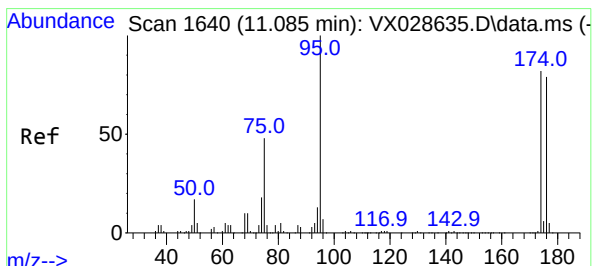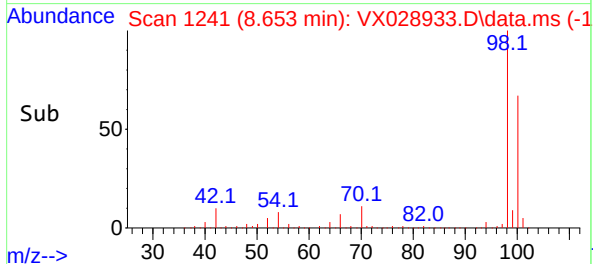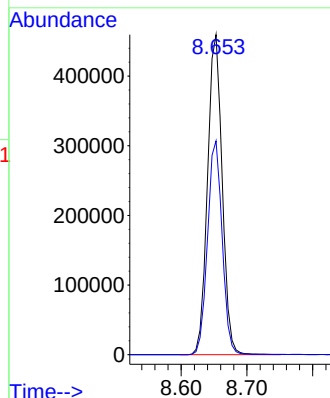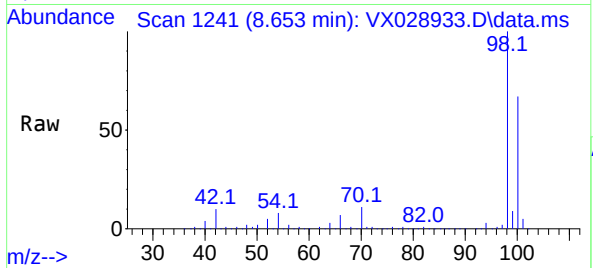

#62
4-Bromofluorobenzene
Concen: 50.016 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX028933.D
Acq: 24 May 2022 19:48

Tgt Ion: 95 Resp: 276159
Ion Ratio Lower Upper
95 100
174 76.6 0.0 163.0
176 73.9 0.0 155.0


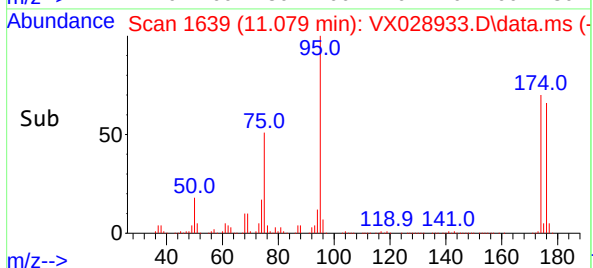
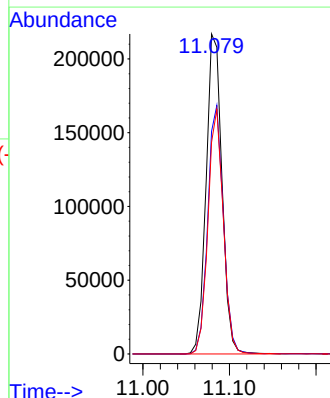
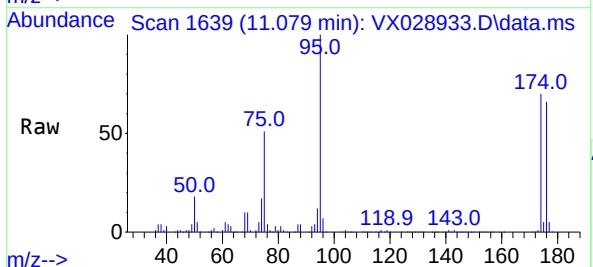


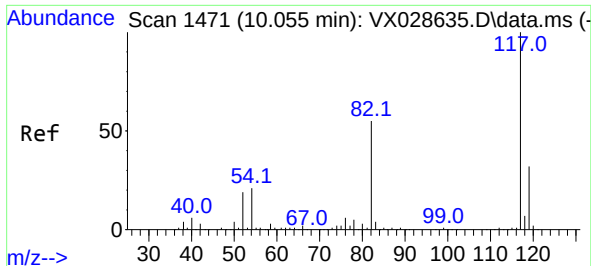

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028933.D
Acq: 24 May 2022 19:48

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Tgt Ion:117 Resp: 566692
Ion Ratio Lower Upper
117 100
82 55.8 41.8 62.8
119 32.9 24.8 37.2

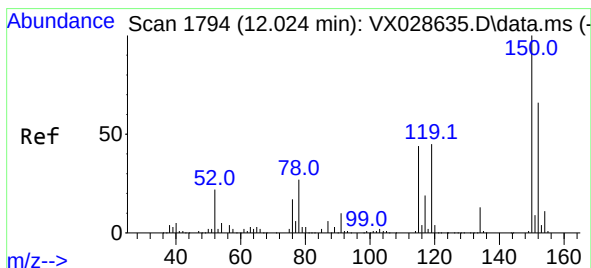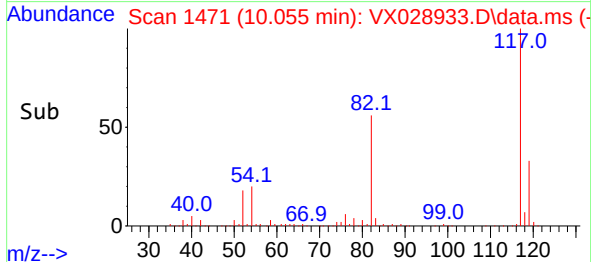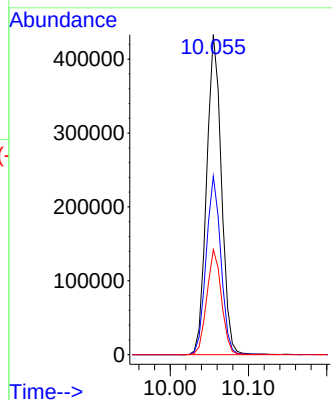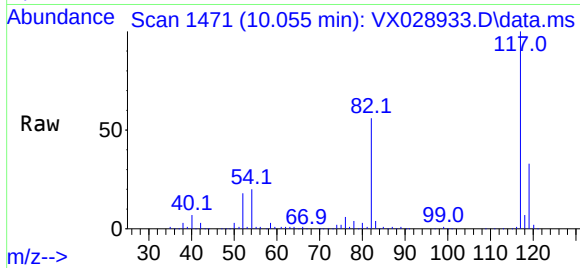

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX028933.D
Acq: 24 May 2022 19:48

Tgt Ion:152 Resp: 263412
Ion Ratio Lower Upper
152 100
115 61.6 37.5 112.7
150 156.6 0.0 338.2

