

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052422\
 Data File : VX028921.D
 Acq On : 24 May 2022 15:08
 Operator : JC/MD
 Sample : N2943-17DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-38IDL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M

Title : SW846 8260

Signal : TIC: VX028921.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.946	296	305	314	rBV	30643	72011	3.87%	0.640%
2	3.111	322	332	349	rBV	398854	930206	49.93%	8.266%
3	4.568	558	571	585	rVB2	8526	30538	1.64%	0.271%
4	5.391	694	706	721	rBV	222734	657328	35.28%	5.841%
5	5.556	721	733	750	rVB	363981	1022919	54.90%	9.090%
6	5.958	789	799	814	rBV	233180	617841	33.16%	5.490%
7	6.763	920	931	945	rBV	582413	1374588	73.78%	12.214%
8	8.653	1233	1241	1256	rBV	1189858	1863078	100.00%	16.555%
9	10.055	1465	1471	1484	rBV	1301294	1698766	91.18%	15.095%
10	11.085	1634	1640	1650	rBV	1027660	1336882	71.76%	11.879%
11	12.024	1788	1794	1801	rBV	1331453	1649617	88.54%	14.658%




Sum of corrected areas: 11253774

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052422\
Data File : VX028921.D
Acq On : 24 May 2022 15:08
Operator : JC/MD
Sample : N2943-17DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-38IDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

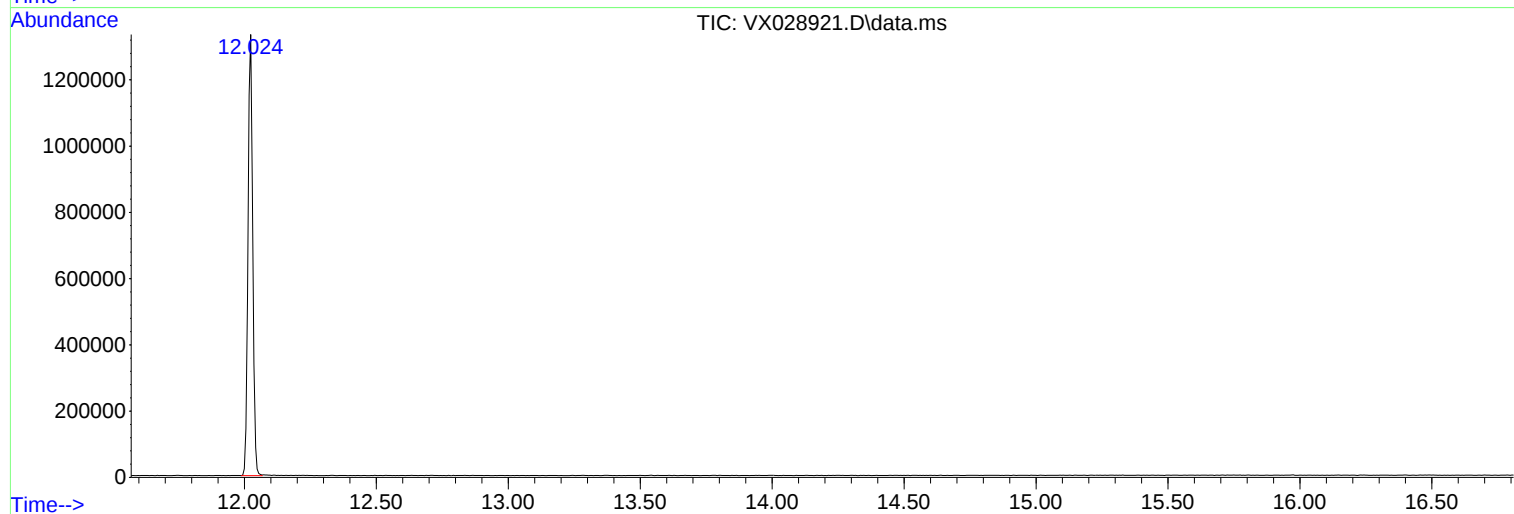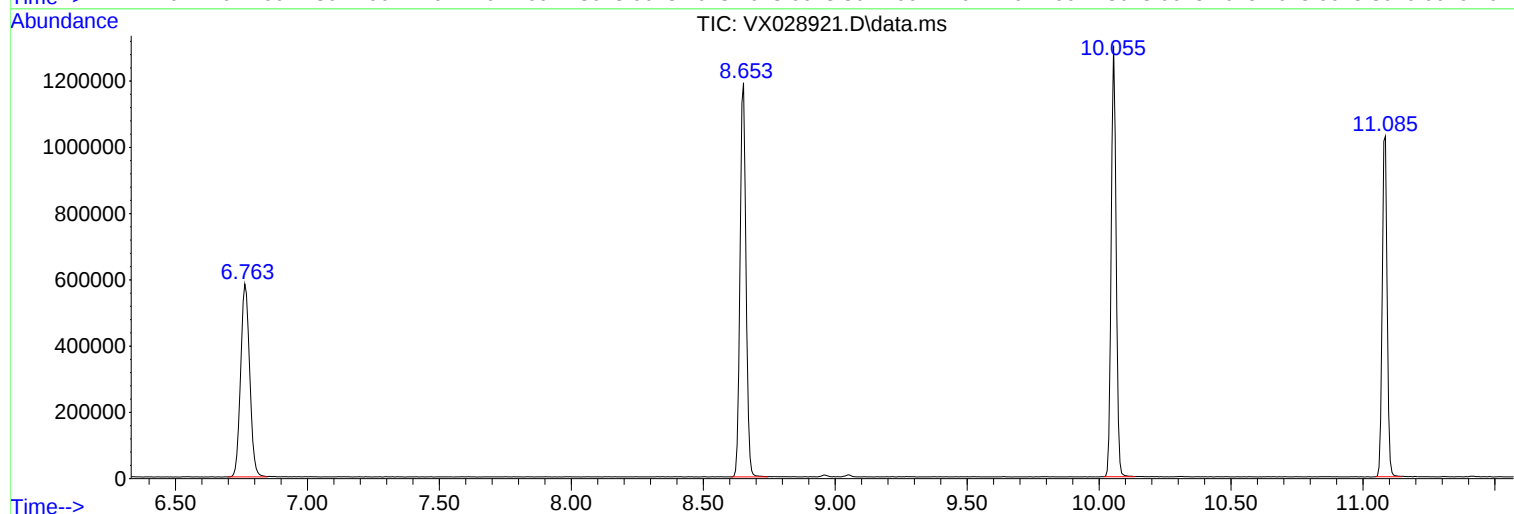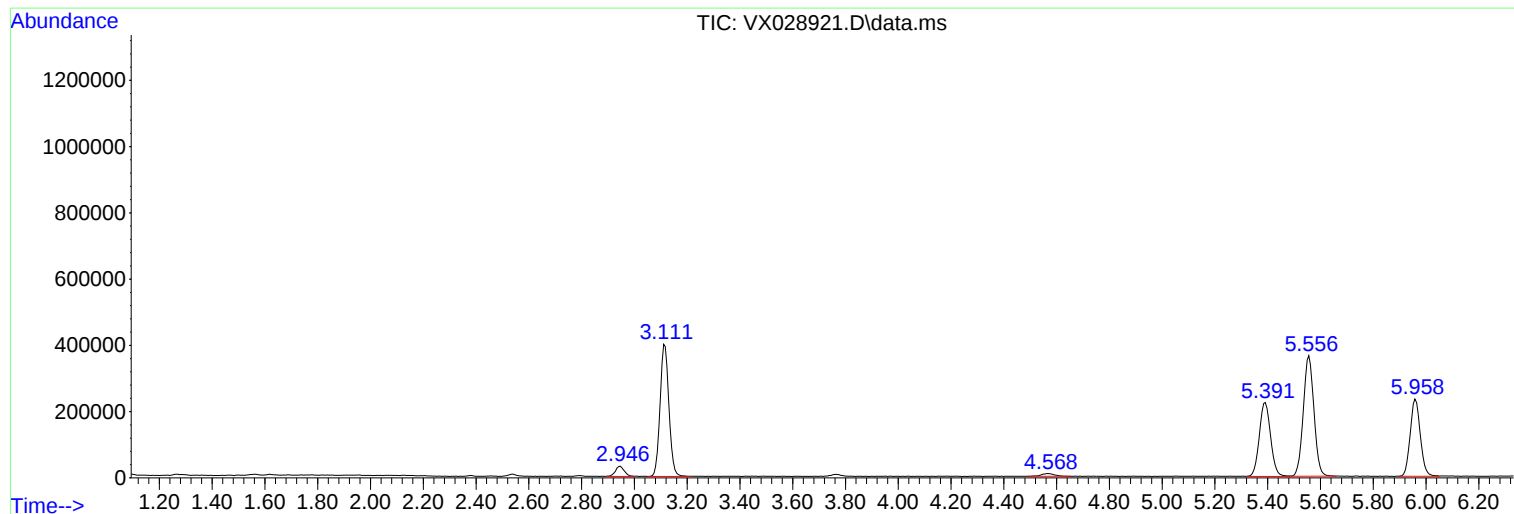

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052422\
Data File : VX028921.D
Acq On : 24 May 2022 15:08
Operator : JC/MD
Sample : N2943-17DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-38IDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052422\
Data File : VX028921.D
Acq On : 24 May 2022 15:08
Operator : JC/MD
Sample : N2943-17DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-38IDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc