

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052422\
 Data File : VX028928.D
 Acq On : 24 May 2022 17:52
 Operator : JC/MD
 Sample : N2970-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 28S-20220519

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Title : SW846 8260

Signal : TIC: VX028928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	23	28	43	rBV	37971	129952	6.84%	0.581%
2	2.782	269	278	283	rBV2	25770	58883	3.10%	0.263%
3	3.099	321	330	343	rVB	49687	114595	6.03%	0.512%
4	4.209	503	512	521	rBV5	9719	30253	1.59%	0.135%
5	4.489	543	558	569	rBV5	10927	38398	2.02%	0.172%
6	5.385	693	705	717	rBV	228904	668130	35.16%	2.988%
7	5.556	723	733	742	rBV	361653	1038258	54.65%	4.643%
8	5.849	766	781	790	rBV5	25244	85681	4.51%	0.383%
9	5.958	790	799	816	rVB	234966	626319	32.96%	2.801%
10	6.166	823	833	842	rBV5	22664	88576	4.66%	0.396%
11	6.263	842	849	857	rVV4	26884	77538	4.08%	0.347%
12	6.763	920	931	946	rBV	586851	1393903	73.36%	6.234%
13	7.373	1021	1031	1040	rBV2	56372	140657	7.40%	0.629%
14	7.775	1089	1097	1106	rVB	48081	99669	5.25%	0.446%
15	7.958	1119	1127	1140	rVB2	51734	117492	6.18%	0.525%
16	8.324	1179	1187	1193	rBV3	30582	59365	3.12%	0.265%
17	8.604	1225	1233	1235	rBV2	28631	48571	2.56%	0.217%
18	8.653	1235	1241	1252	rVB	1176578	1899997	100.00%	8.497%
19	8.775	1254	1261	1266	rBV	89024	145121	7.64%	0.649%
20	8.976	1288	1294	1301	rVB	171774	278064	14.63%	1.244%
21	9.104	1306	1315	1321	rBV	64839	106432	5.60%	0.476%
22	9.513	1375	1382	1387	rBV2	45807	73040	3.84%	0.327%
23	9.622	1394	1400	1404	rBV	84975	134573	7.08%	0.602%
24	9.659	1404	1406	1416	rVB3	19891	34787	1.83%	0.156%
25	9.836	1428	1435	1441	rBV2	27312	45136	2.38%	0.202%
26	10.055	1465	1471	1478	rBV	1320067	1714297	90.23%	7.667%
27	10.128	1478	1483	1488	rVV	36913	55566	2.92%	0.249%
28	10.281	1503	1508	1517	rBV3	42252	110557	5.82%	0.494%
29	10.458	1532	1537	1542	rBV2	32322	46412	2.44%	0.208%
30	10.604	1548	1561	1566	rBV4	55304	148676	7.83%	0.665%
31	10.756	1578	1586	1587	rBV2	29851	48068	2.53%	0.215%
32	10.781	1587	1590	1595	rVB	39301	52891	2.78%	0.237%
33	10.860	1598	1603	1610	rBV4	32440	60930	3.21%	0.272%
34	11.079	1634	1639	1644	rBV	1037076	1359889	71.57%	6.082%
35	11.128	1644	1647	1651	rVB	41450	53993	2.84%	0.241%
36	11.226	1659	1663	1667	rVB2	49379	66734	3.51%	0.298%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052422\
 Data File : VX028928.D
 Acq On : 24 May 2022 17:52
 Operator : JC/MD
 Sample : N2970-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 28S-20220519

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Title : SW846 8260

37	11.390	1686	1690	1696	rVB6	19094	30121	1.59%	0.135%
38	11.616	1719	1727	1734	rBV3	38082	65446	3.44%	0.293%
39	11.713	1734	1743	1746	rBV	46099	66898	3.52%	0.299%
40	11.866	1760	1768	1770	rBV	135398	196653	10.35%	0.879%
41	11.890	1770	1772	1778	rVB	148835	173524	9.13%	0.776%
42	12.024	1789	1794	1799	rBV	1375840	1703755	89.67%	7.620%
43	12.177	1814	1819	1824	rVV	47530	61746	3.25%	0.276%
44	12.250	1825	1831	1835	rVV	67927	84624	4.45%	0.378%
45	12.311	1835	1841	1851	rVB4	112355	204857	10.78%	0.916%
46	12.408	1851	1857	1862	rBV	114479	156314	8.23%	0.699%
47	12.597	1880	1888	1892	rBV3	49754	88043	4.63%	0.394%
48	12.646	1892	1896	1902	rVV2	118714	205618	10.82%	0.920%
49	12.725	1902	1909	1912	rVV3	88829	165361	8.70%	0.740%
50	12.762	1912	1915	1920	rVV	71633	96826	5.10%	0.433%
51	12.841	1920	1928	1933	rVB2	266644	431904	22.73%	1.932%
52	12.902	1933	1938	1940	rBV	170793	237049	12.48%	1.060%
53	12.927	1940	1942	1947	rVB3	92736	116400	6.13%	0.521%
54	13.030	1955	1959	1964	rVB2	89567	126655	6.67%	0.566%
55	13.140	1966	1977	1982	rBV2	234860	358976	18.89%	1.605%
56	13.195	1982	1986	1991	rVB	96615	112806	5.94%	0.504%
57	13.250	1991	1995	1998	rBV	57167	82289	4.33%	0.368%
58	13.292	1998	2002	2007	rVB2	85281	115656	6.09%	0.517%
59	13.347	2007	2011	2015	rBV2	55839	66295	3.49%	0.296%
60	13.396	2015	2019	2030	rVB4	86549	161454	8.50%	0.722%
61	13.518	2034	2039	2045	rBV5	65641	141082	7.43%	0.631%
62	13.585	2045	2050	2053	rBV2	188572	269772	14.20%	1.206%
63	13.622	2053	2056	2057	rVV2	182953	224475	11.81%	1.004%
64	13.640	2057	2059	2061	rVV	247646	325659	17.14%	1.456%
65	13.664	2061	2063	2068	rVB	365422	384648	20.24%	1.720%
66	13.750	2073	2077	2081	rBV	247766	303536	15.98%	1.357%
67	13.798	2081	2085	2090	rVB2	66806	103720	5.46%	0.464%
68	13.853	2090	2094	2098	rVB2	106444	144060	7.58%	0.644%
69	13.926	2098	2106	2110	rBV5	198611	381366	20.07%	1.706%
70	13.975	2110	2114	2117	rVV2	125064	166846	8.78%	0.746%
71	14.006	2117	2119	2122	rVB	55366	53810	2.83%	0.241%
72	14.067	2126	2129	2132	rBV3	61957	75313	3.96%	0.337%
73	14.103	2132	2135	2139	rVB	107955	118929	6.26%	0.532%
74	14.182	2142	2148	2150	rBV	65232	103983	5.47%	0.465%
75	14.213	2150	2153	2157	rVB	105472	117072	6.16%	0.524%
76	14.292	2163	2166	2167	rBV3	43448	47190	2.48%	0.211%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052422\
 Data File : VX028928.D
 Acq On : 24 May 2022 17:52
 Operator : JC/MD
 Sample : N2970-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 28S-20220519

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Title : SW846 8260

77	14.317	2167	2170	2174	rVB	170504	215600	11.35%	0.964%
78	14.371	2174	2179	2184	rVB2	126896	198730	10.46%	0.889%
79	14.420	2184	2187	2192	rVB	73809	90462	4.76%	0.405%
80	14.481	2192	2197	2206	rBV2	257419	460696	24.25%	2.060%
81	14.591	2210	2215	2216	rBV4	37893	68581	3.61%	0.307%
82	14.670	2224	2228	2233	rBV2	228774	308080	16.21%	1.378%
83	14.725	2233	2237	2241	rVV	82232	96971	5.10%	0.434%
84	14.786	2243	2247	2251	rVV	205428	304892	16.05%	1.364%
85	14.853	2255	2258	2260	rVB2	32779	34244	1.80%	0.153%
86	14.884	2260	2263	2269	rBV3	37442	80919	4.26%	0.362%
87	14.981	2276	2279	2285	rVB3	37516	51922	2.73%	0.232%
88	15.048	2286	2290	2299	rVV5	30039	69515	3.66%	0.311%
89	15.182	2307	2312	2319	rVV2	86897	167949	8.84%	0.751%
90	15.262	2319	2325	2330	rVB3	55996	89051	4.69%	0.398%
91	15.408	2346	2349	2353	rVB2	47790	60298	3.17%	0.270%
92	15.530	2364	2369	2375	rVB6	25998	58909	3.10%	0.263%
93	15.597	2375	2380	2386	rVB2	165015	256165	13.48%	1.146%
94	15.652	2386	2389	2396	rVB5	24601	40025	2.11%	0.179%
95	15.731	2396	2402	2408	rBV2	84374	150462	7.92%	0.673%
96	15.810	2408	2415	2418	rBV2	39619	66086	3.48%	0.296%
97	15.847	2418	2421	2425	rVB	28015	39017	2.05%	0.174%
98	15.987	2439	2444	2449	rBV2	22132	35810	1.88%	0.160%
99	16.091	2456	2461	2468	rVB3	22119	41237	2.17%	0.184%
100	16.304	2491	2496	2505	rVB6	24954	52515	2.76%	0.235%




Sum of corrected areas: 22360270

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052422\
Data File : VX028928.D
Acq On : 24 May 2022 17:52
Operator : JC/MD
Sample : N2970-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
28S-20220519

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

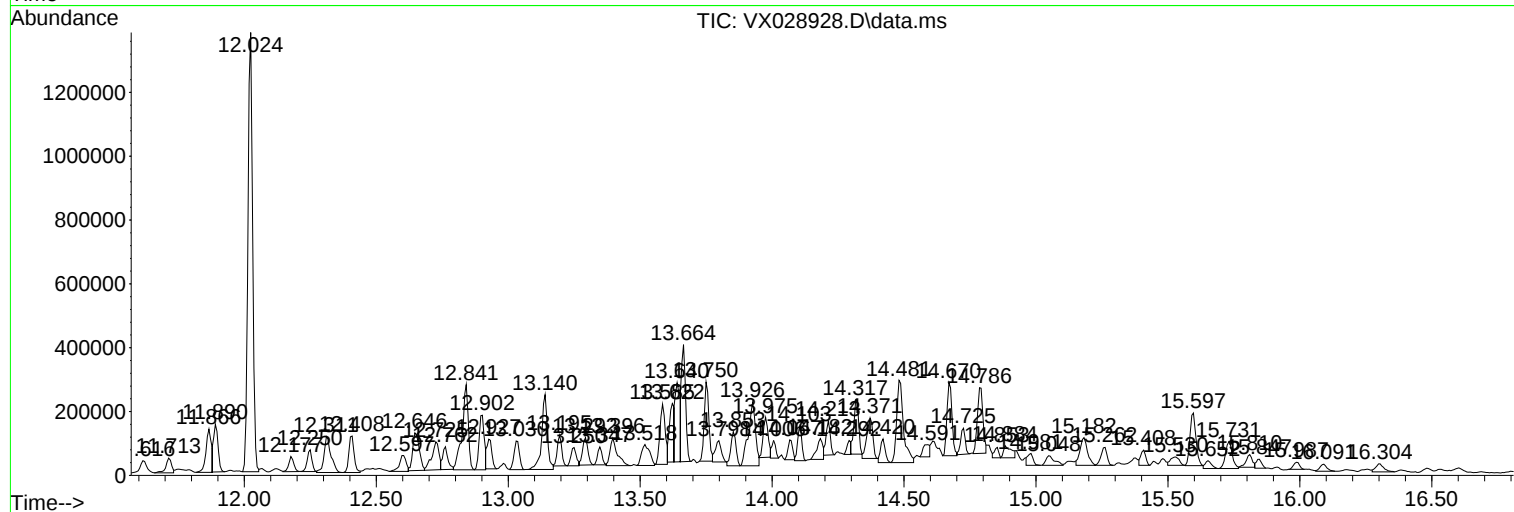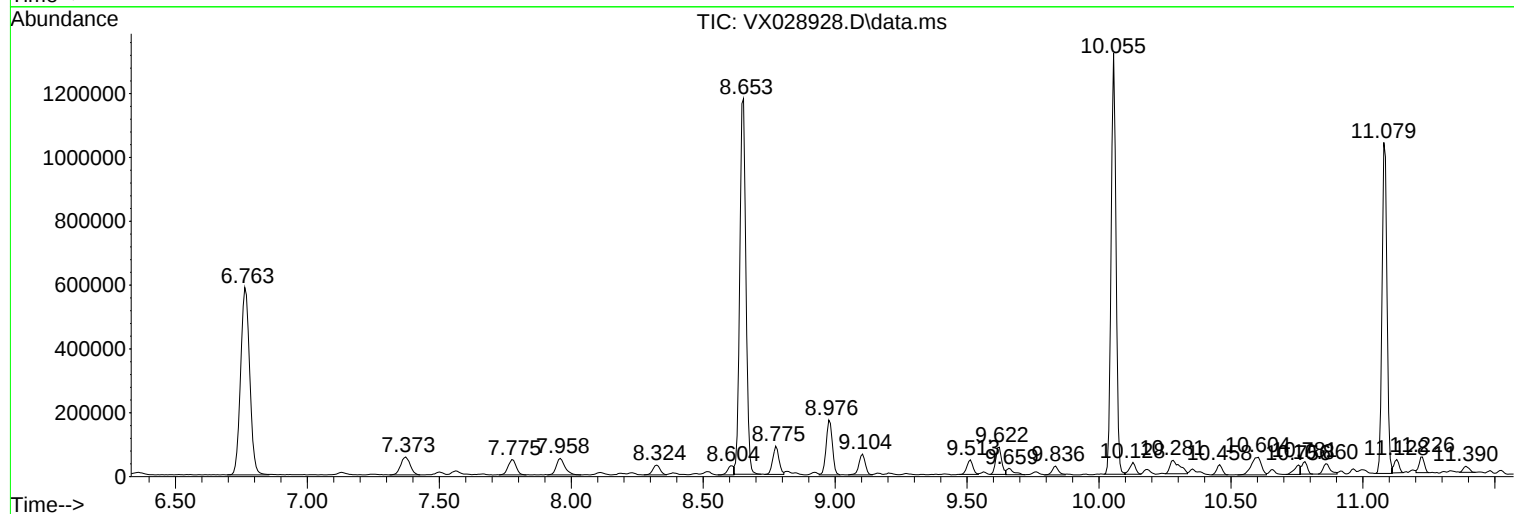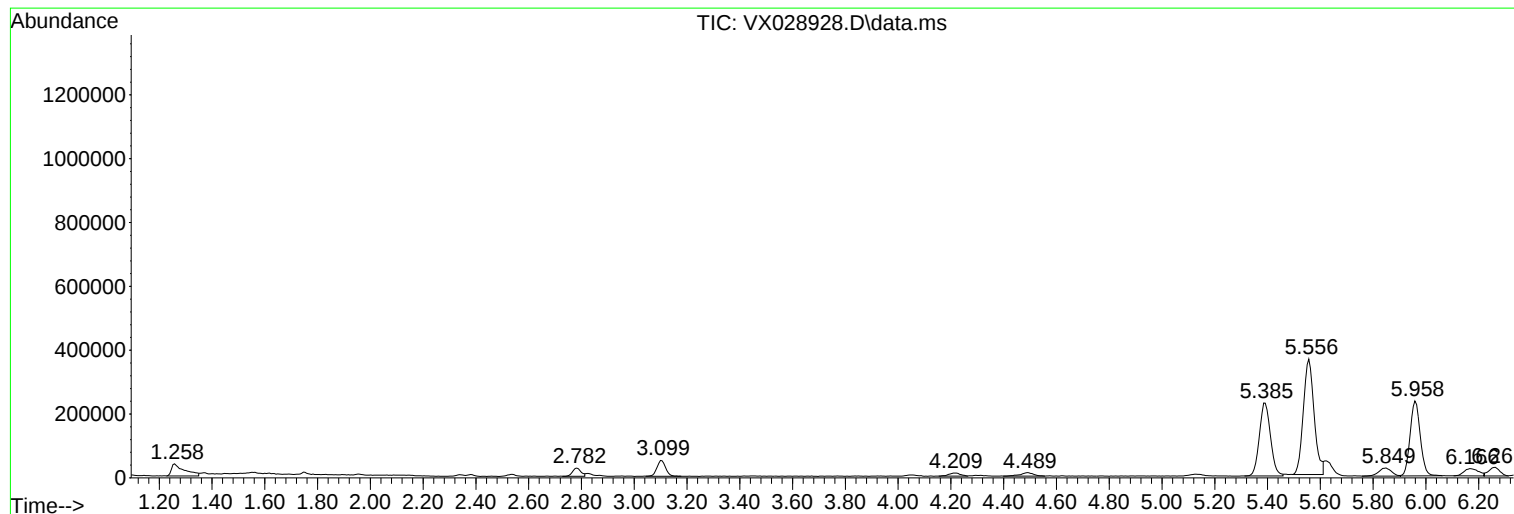

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052422\
Data File : VX028928.D
Acq On : 24 May 2022 17:52
Operator : JC/MD
Sample : N2970-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
28S-20220519

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052422\
Data File : VX028928.D
Acq On : 24 May 2022 17:52
Operator : JC/MD
Sample : N2970-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
28S-20220519

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------