

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052423\
Data File : VX035831.D
Acq On : 24 May 2023 13:15
Operator : JC/MD
Sample : 02860-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-DUP-03-05162023

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M

Title : SW846 8260

Signal : TIC: VX035831.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	692	705	721	rBV	123930	364442	19.18%	4.797%
2	5.549	721	732	746	rVB	204198	576490	30.34%	7.588%
3	5.952	787	798	813	rBV	146729	394127	20.75%	5.188%
4	6.763	920	931	950	rBV	332098	798224	42.02%	10.507%
5	7.122	980	990	1004	rBV	866519	1899797	100.00%	25.007%
6	8.646	1233	1240	1249	rBV	636035	998448	52.56%	13.143%
7	9.518	1378	1383	1392	rBV	25843	38922	2.05%	0.512%
8	10.055	1465	1471	1482	rBV	678928	918971	48.37%	12.096%
9	11.079	1634	1639	1651	rVB	575287	710704	37.41%	9.355%
10	12.018	1788	1793	1804	rBV	687934	896875	47.21%	11.806%




Sum of corrected areas: 7597000

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052423\
Data File : VX035831.D
Acq On : 24 May 2023 13:15
Operator : JC/MD
Sample : 02860-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-DUP-03-05162023

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

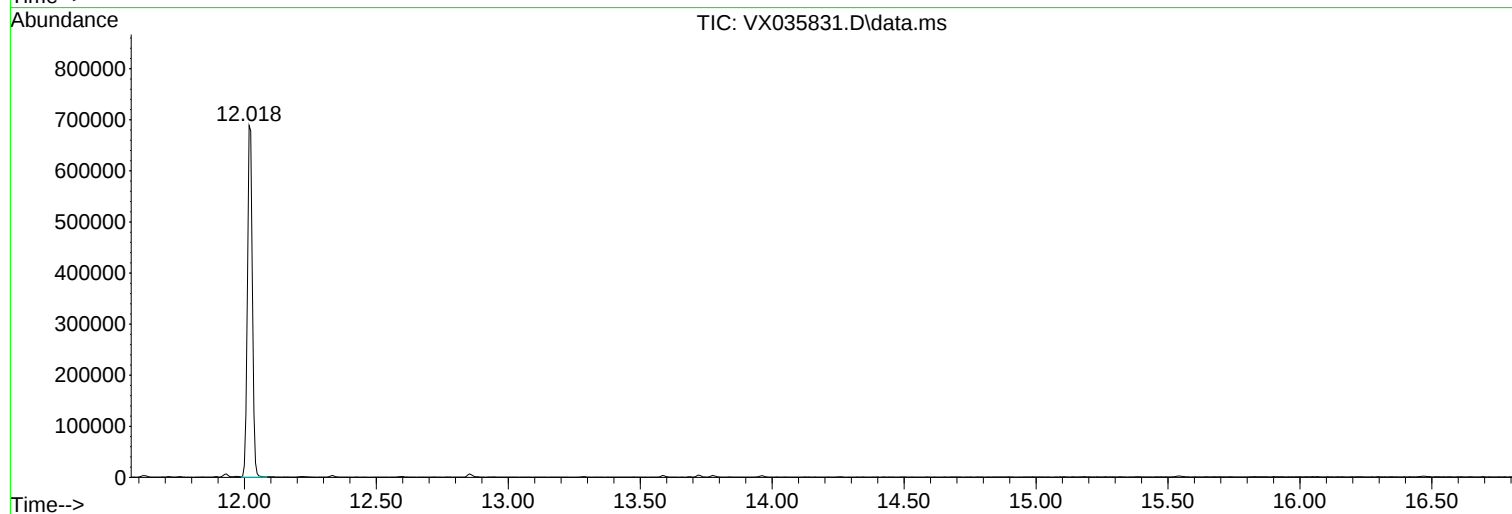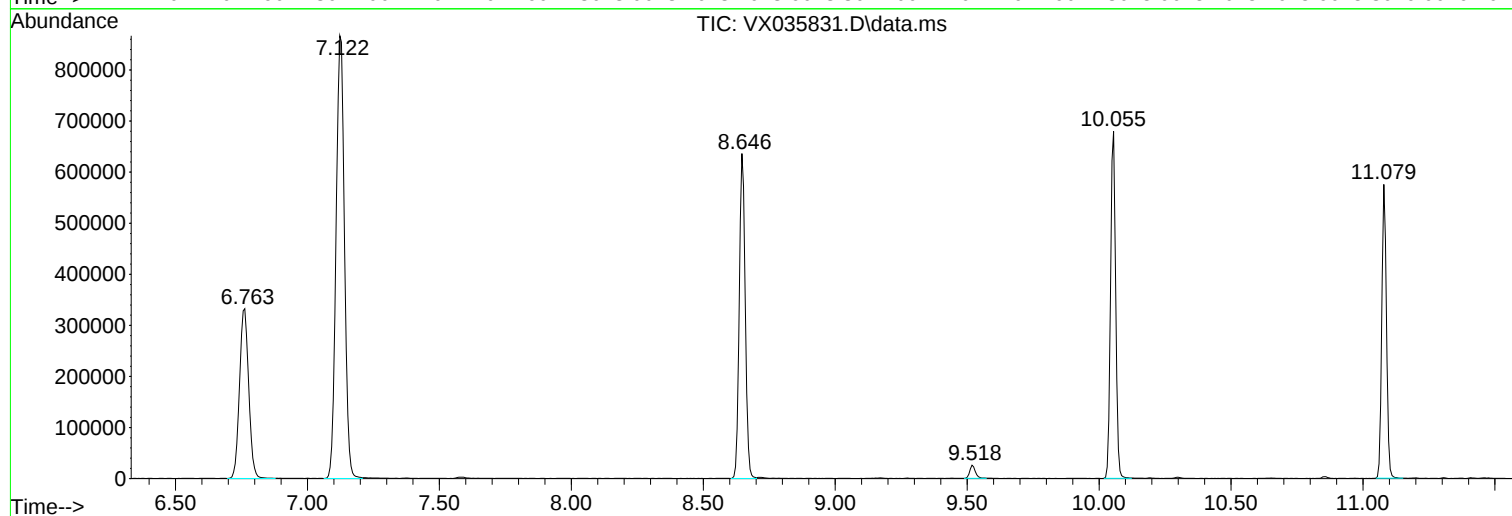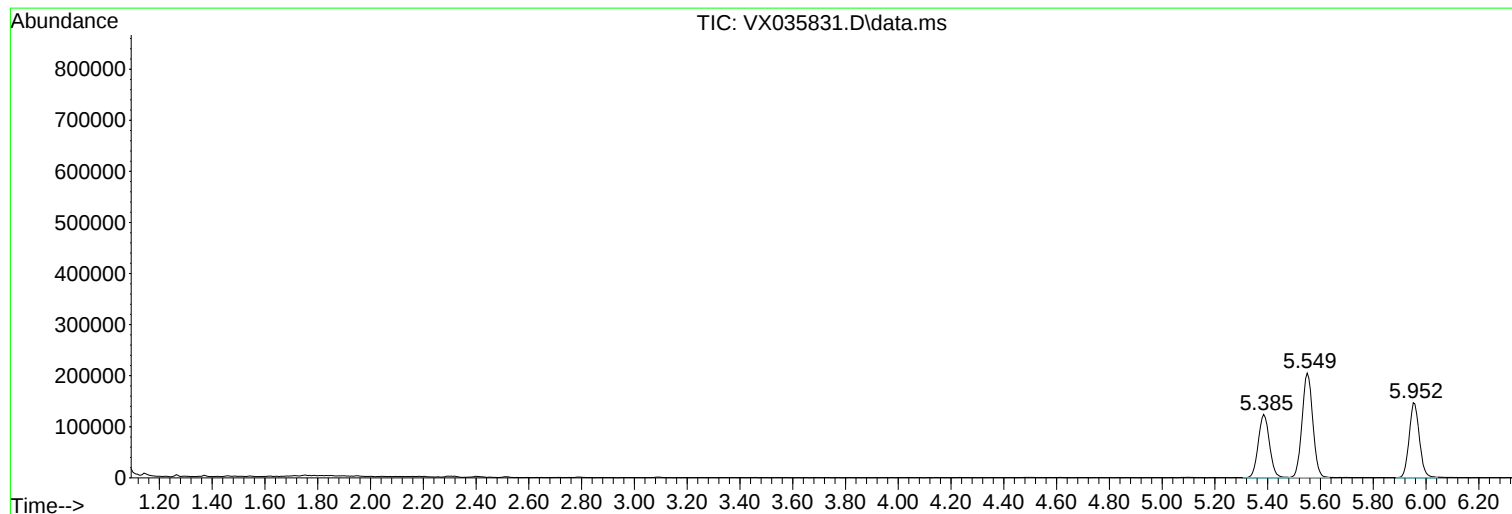

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052423\
Data File : VX035831.D
Acq On : 24 May 2023 13:15
Operator : JC/MD
Sample : 02860-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-DUP-03-05162023

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052423\
Data File : VX035831.D
Acq On : 24 May 2023 13:15
Operator : JC/MD
Sample : 02860-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-DUP-03-05162023

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------