



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX052423\  
Data File : VX035824.D  
Acq On : 24 May 2023 08:44  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051123W.M  
Title : SW846 8260  
Last Update : Thu May 11 13:57:54 2023

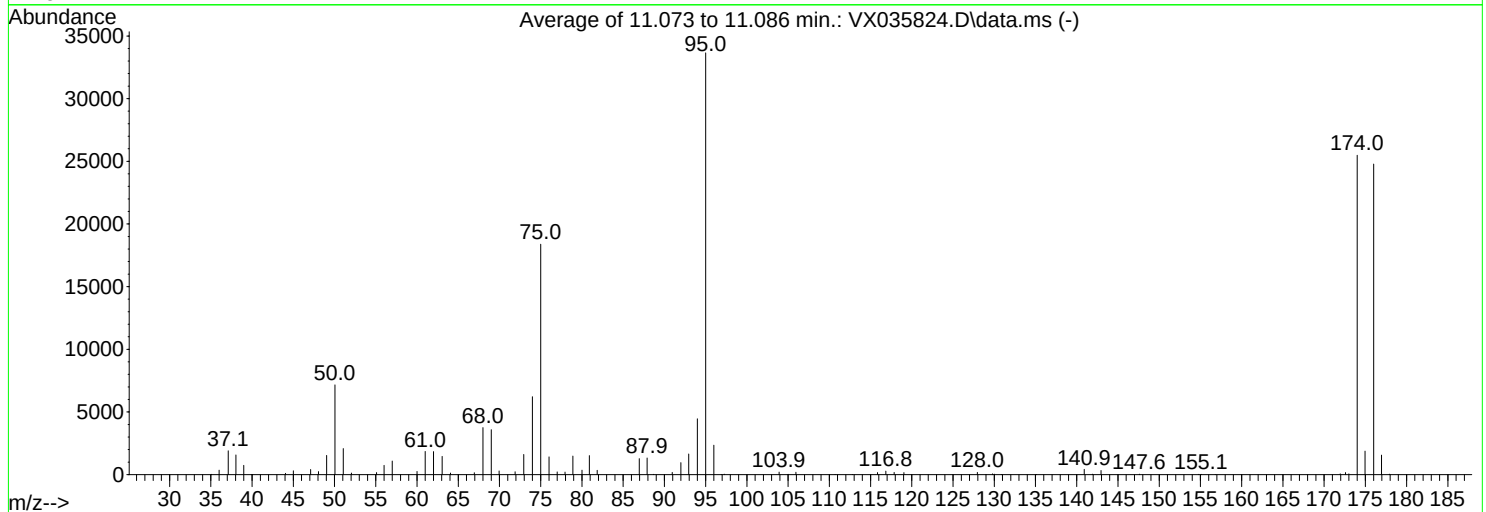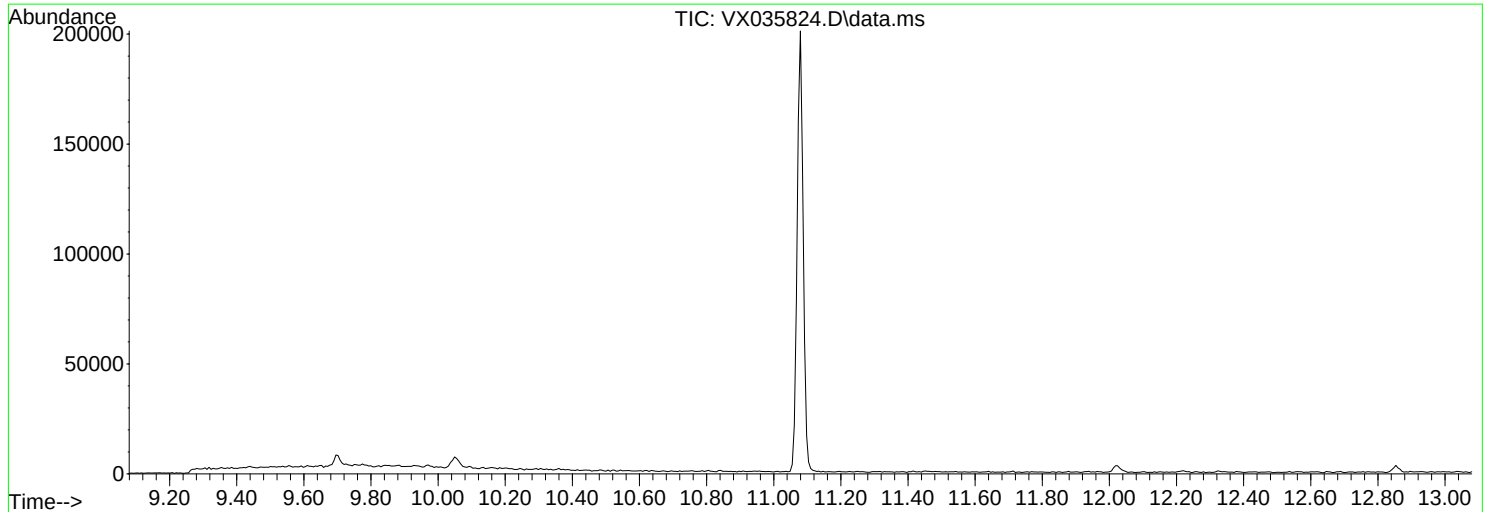

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 21.3  | 7161  | PASS      |
| 75     | 95      | 30     | 60     | 54.6  | 18384 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 33656 | PASS      |
| 96     | 95      | 5      | 9      | 7.0   | 2349  | PASS      |
| 173    | 174     | 0.00   | 2      | 0.2   | 62    | PASS      |
| 174    | 95      | 50     | 100    | 75.7  | 25483 | PASS      |
| 175    | 174     | 5      | 9      | 7.3   | 1873  | PASS      |
| 176    | 174     | 95     | 101    | 97.2  | 24776 | PASS      |
| 177    | 176     | 5      | 9      | 6.3   | 1554  | PASS      |