

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052424\
 Data File : VX041646.D
 Acq On : 24 May 2024 11:48
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK

Quant Time: May 25 04:21:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 08 06:03:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	142875	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.757	114	210502	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	207331	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	107631	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	79308	50.989	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 101.980%	
35) Dibromofluoromethane	5.385	113	65689	46.049	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 92.100%	
50) Toluene-d8	8.647	98	247121	54.733	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 109.460%	
62) 4-Bromofluorobenzene	11.079	95	94275	53.939	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 107.880%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052424\
Data File : VX041646.D
Acq On : 24 May 2024 11:48
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK

Quant Time: May 25 04:21:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
Quant Title : SW846 8260
QLast Update : Wed May 08 06:03:16 2024
Response via : Initial Calibration




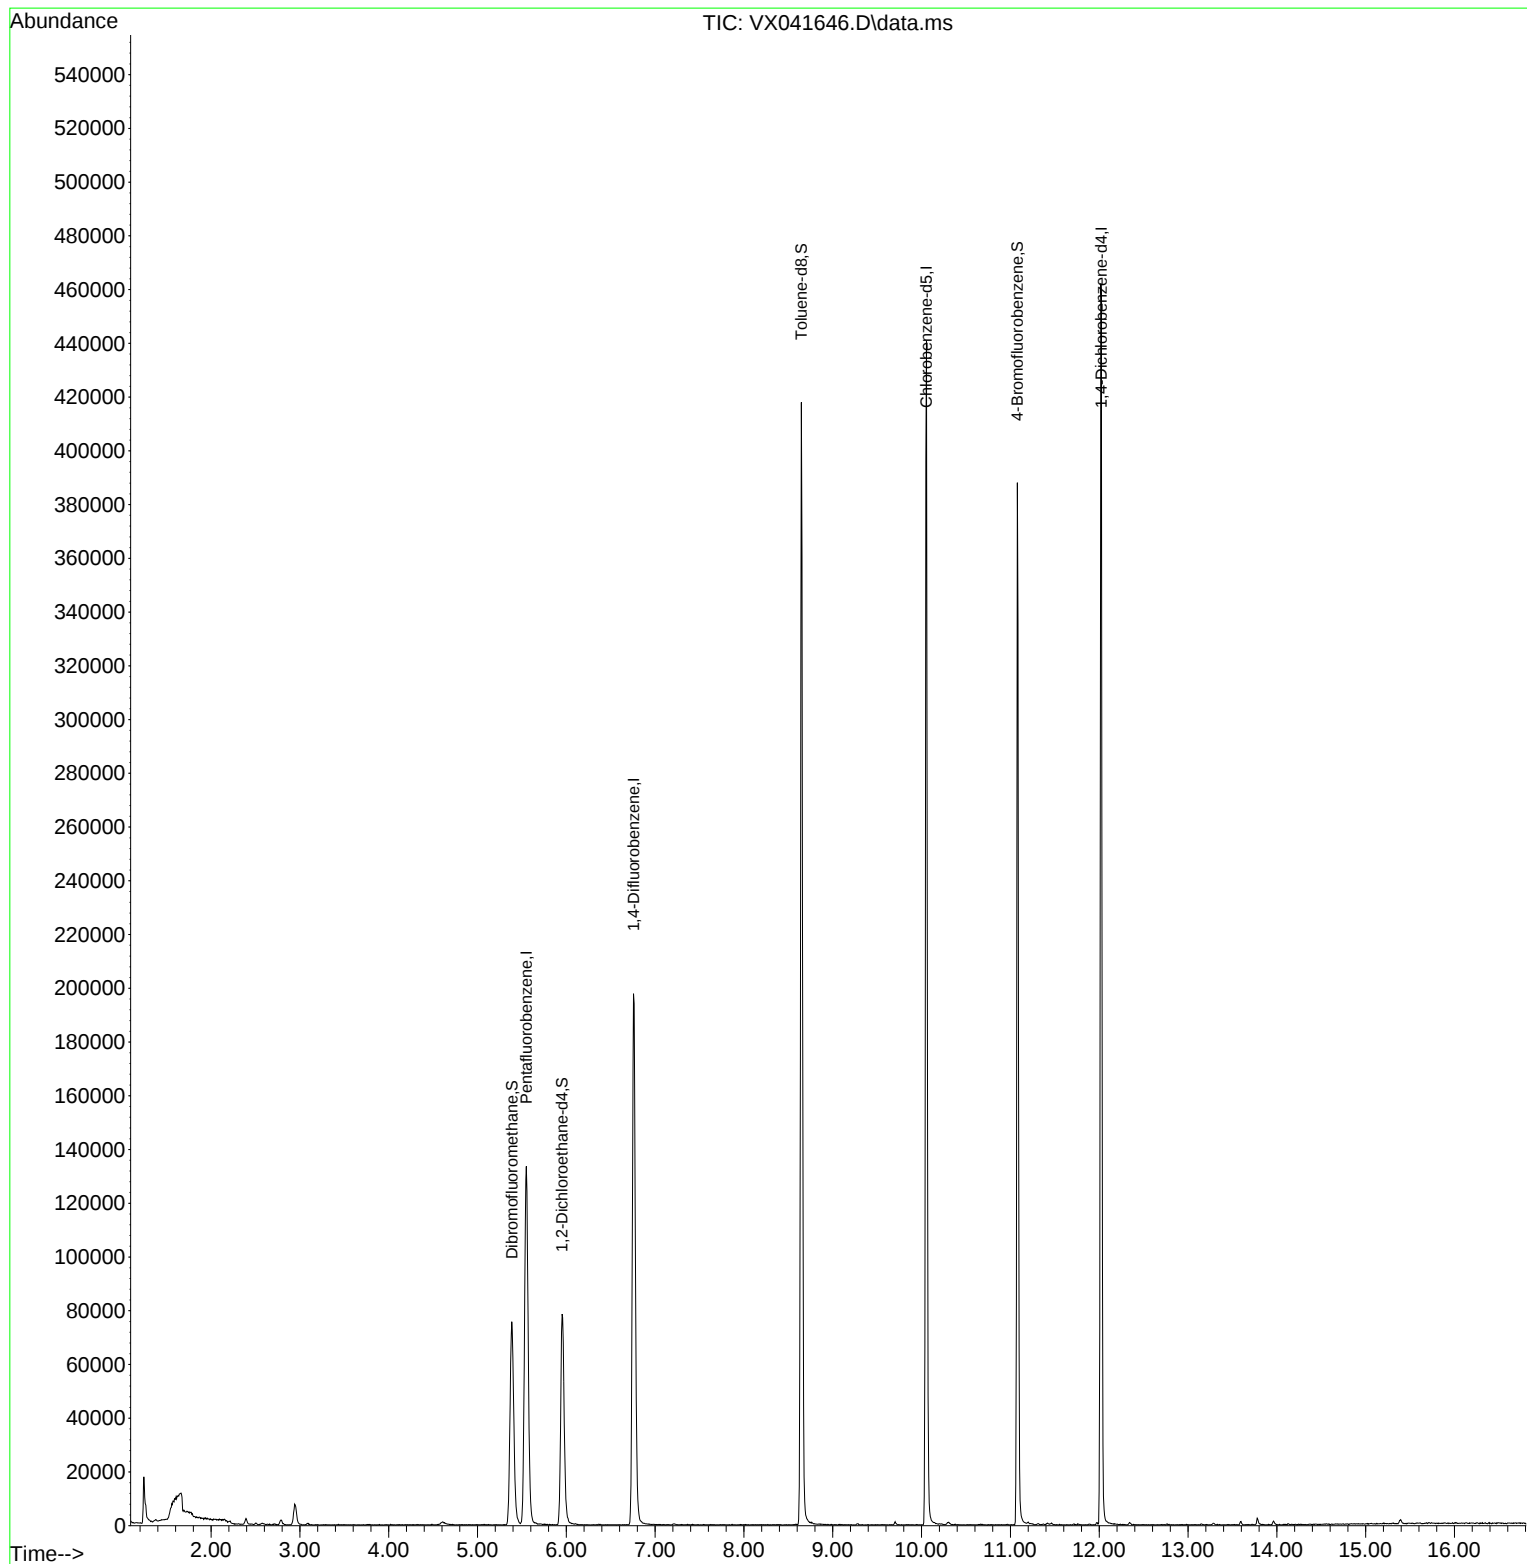


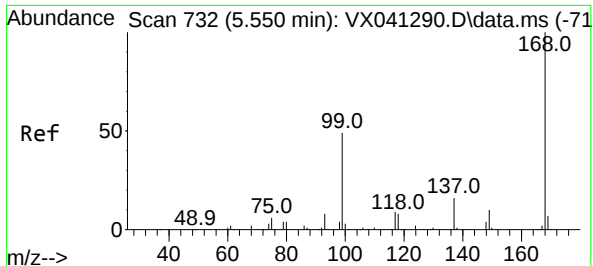

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX041646.D
Acq: 24 May 2024 11:48




Instrument :
MSVOA_X
ClientSampleId :
VIBLK


Tgt Ion:168 Resp: 142875
Ion Ratio Lower Upper
168 100
99 47.6 56.6 85.0#

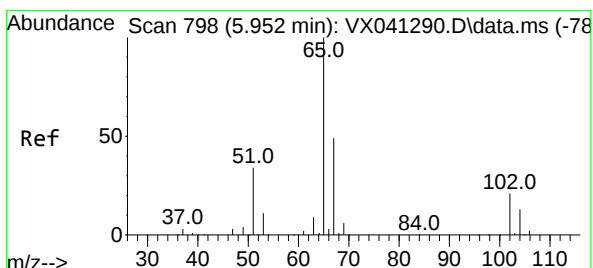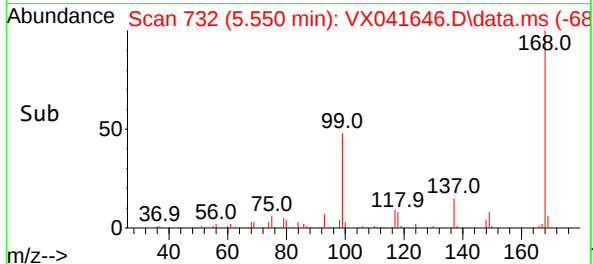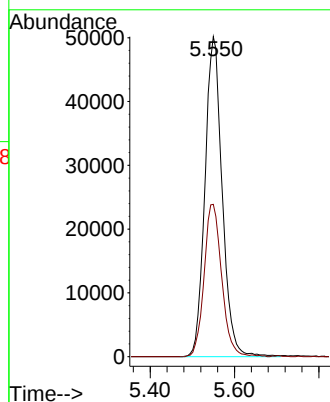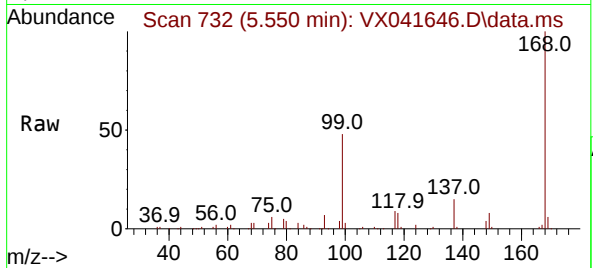

#33
1,2-Dichloroethane-d4
Concen: 50.989 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX041646.D
Acq: 24 May 2024 11:48

Tgt Ion: 65 Resp: 79308
Ion Ratio Lower Upper
65 100
67 51.6 0.0 100.2


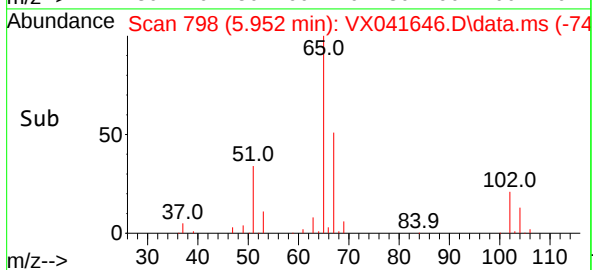
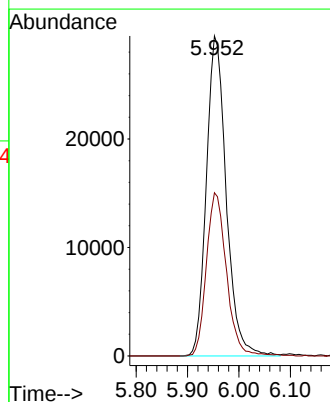
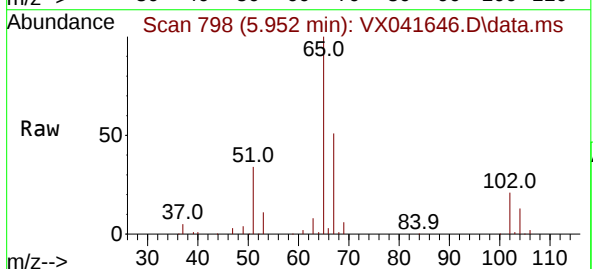


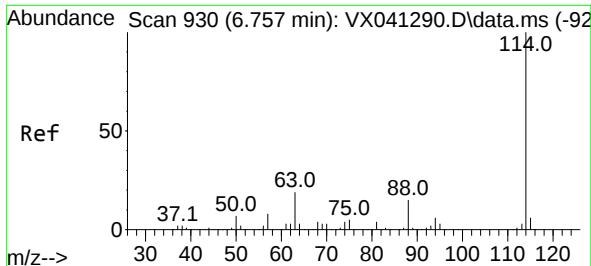

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX041646.D
Acq: 24 May 2024 11:48




Instrument :
MSVOA_X
ClientSampleId :
VIBLK


Tgt Ion:114 Resp: 210502
Ion Ratio Lower Upper
114 100
63 20.3 0.0 45.0
88 15.8 0.0 36.6

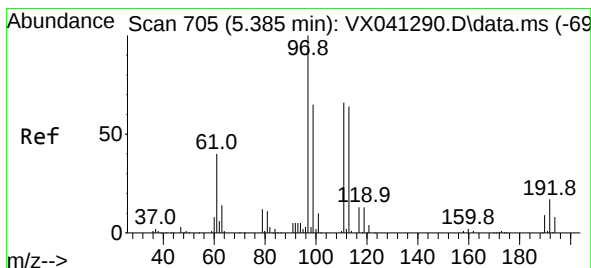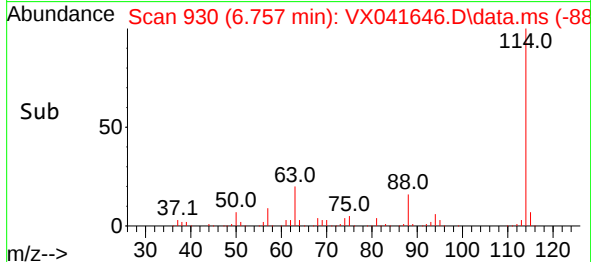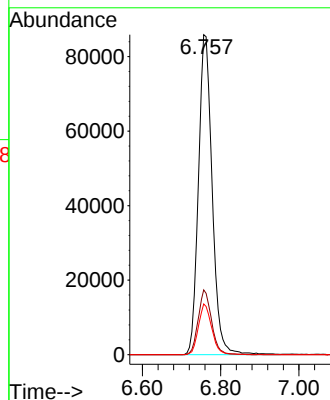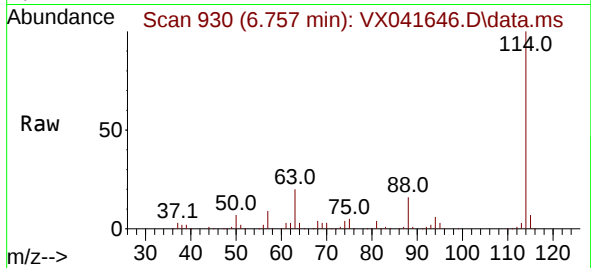

#35
Dibromofluoromethane
Concen: 46.049 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX041646.D
Acq: 24 May 2024 11:48

Tgt Ion:113 Resp: 65689
Ion Ratio Lower Upper
113 100
111 101.8 82.9 124.3
192 24.6 13.3 19.9#


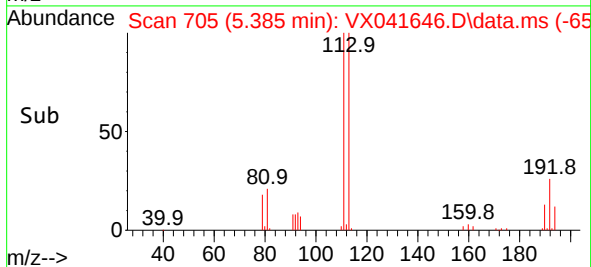
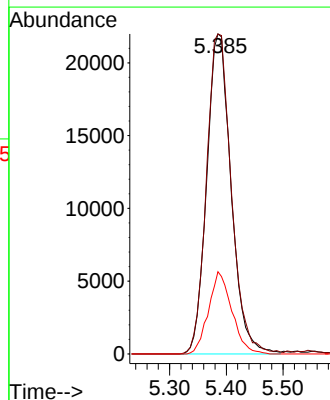
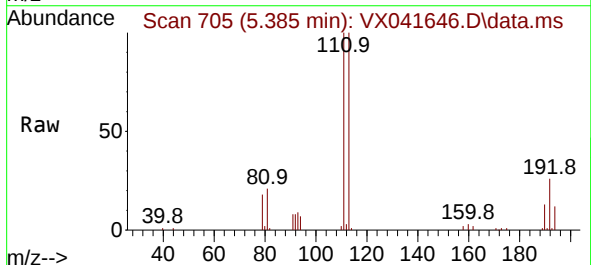


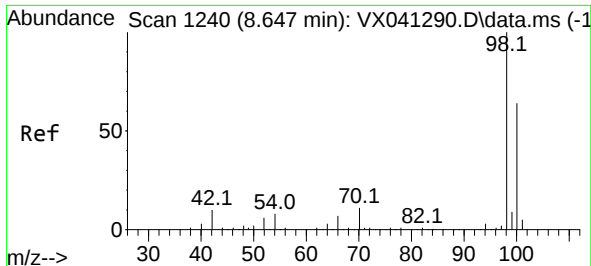

#50
Toluene-d8
Concen: 54.733 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX041646.D
Acq: 24 May 2024 11:48




Instrument :
MSVOA_X
ClientSampleId :
VIBLK


Tgt Ion: 98 Resp: 247121
Ion Ratio Lower Upper
98 100
100 66.4 53.1 79.7

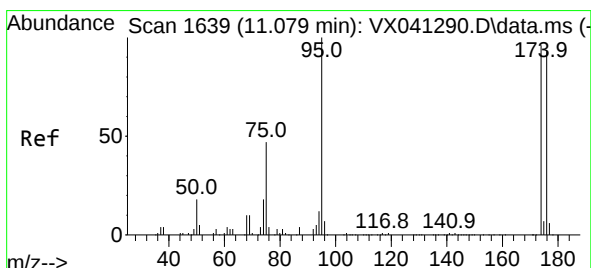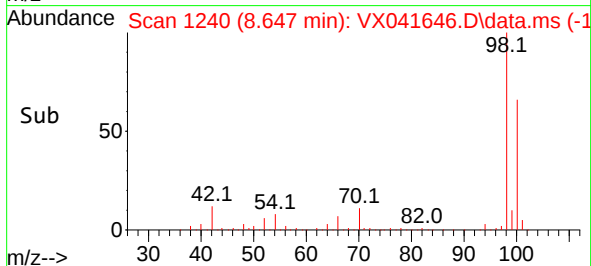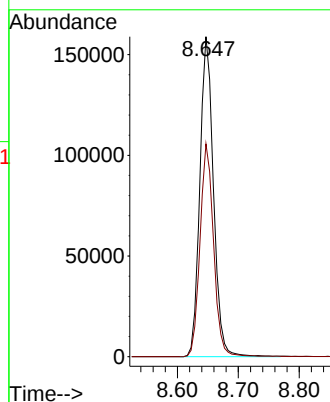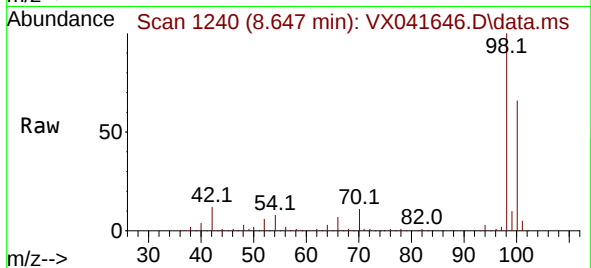

#62
4-Bromofluorobenzene
Concen: 53.939 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX041646.D
Acq: 24 May 2024 11:48

Tgt Ion: 95 Resp: 94275
Ion Ratio Lower Upper
95 100
174 98.6 0.0 135.6
176 95.3 0.0 131.0


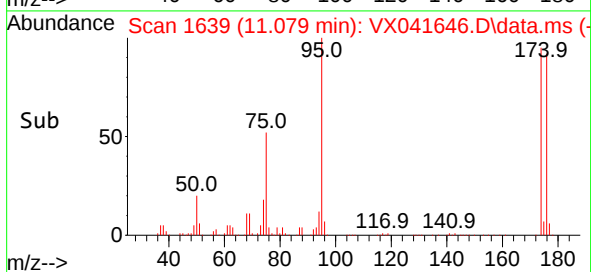
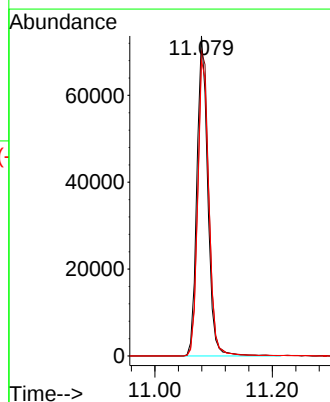
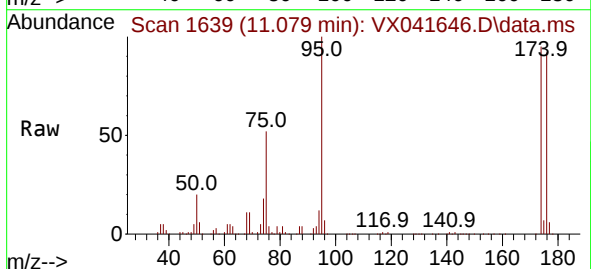


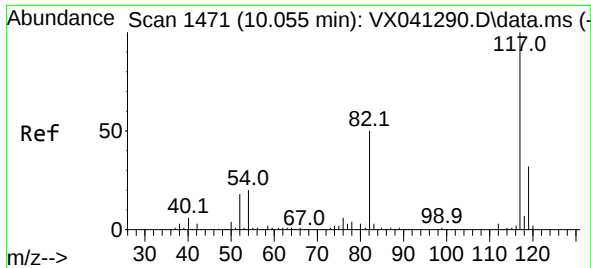

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX041646.D
Acq: 24 May 2024 11:48

Instrument :
MSVOA_X
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 207331
Ion Ratio Lower Upper
117 100
82 52.0 46.2 69.4
119 31.8 25.5 38.3

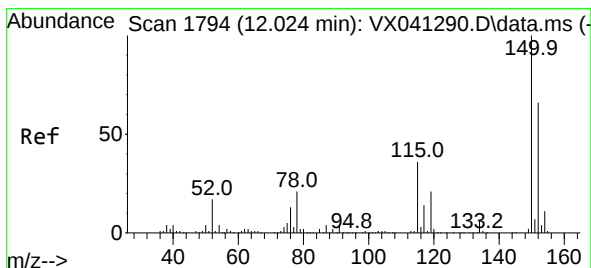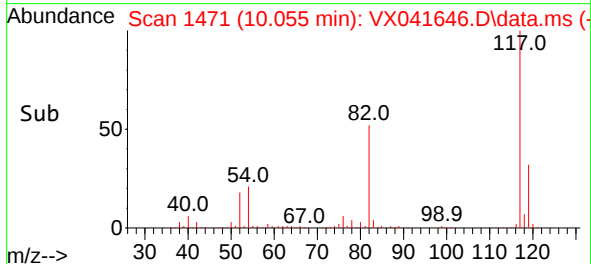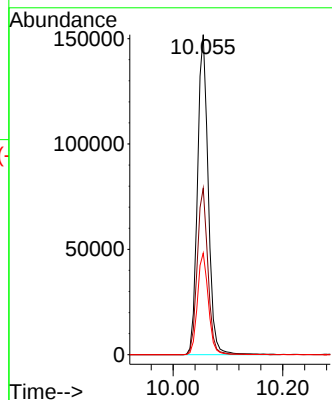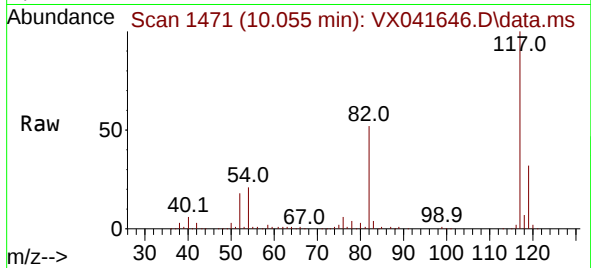

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX041646.D
Acq: 24 May 2024 11:48

Tgt Ion:152 Resp: 107631
Ion Ratio Lower Upper
152 100
115 54.0 43.3 129.9
150 155.6 0.0 345.0

