
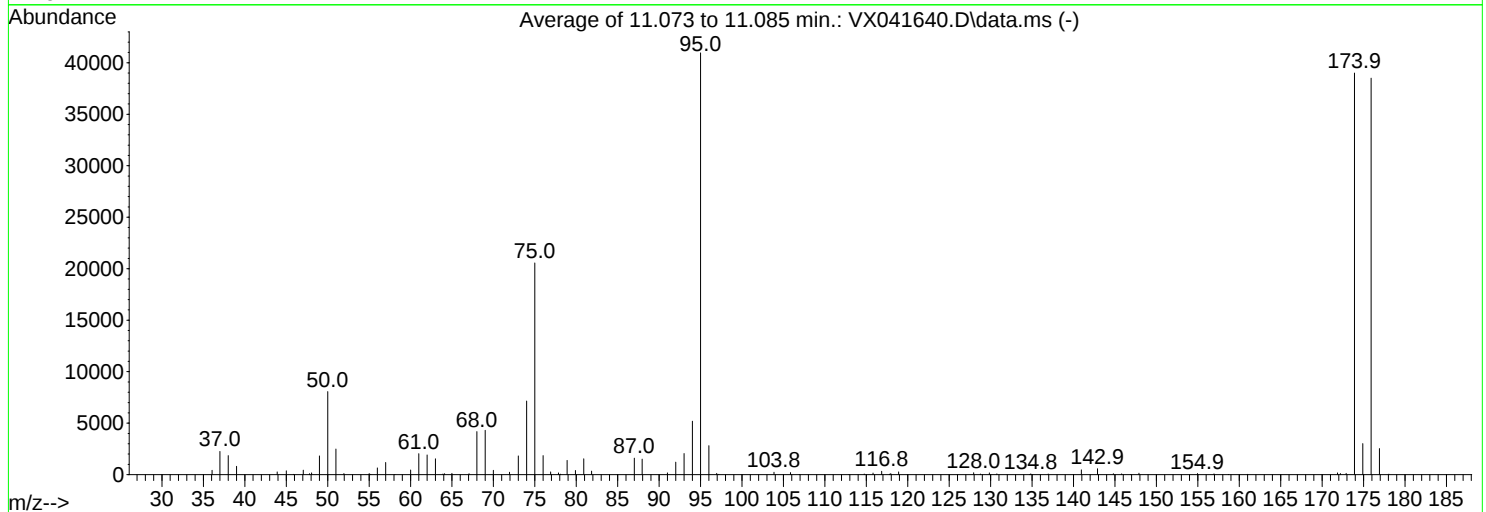


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052424\
Data File : VX041640.D
Acq On : 24 May 2024 08:19
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
Title : SW846 8260
Last Update : Wed May 08 06:03:16 2024

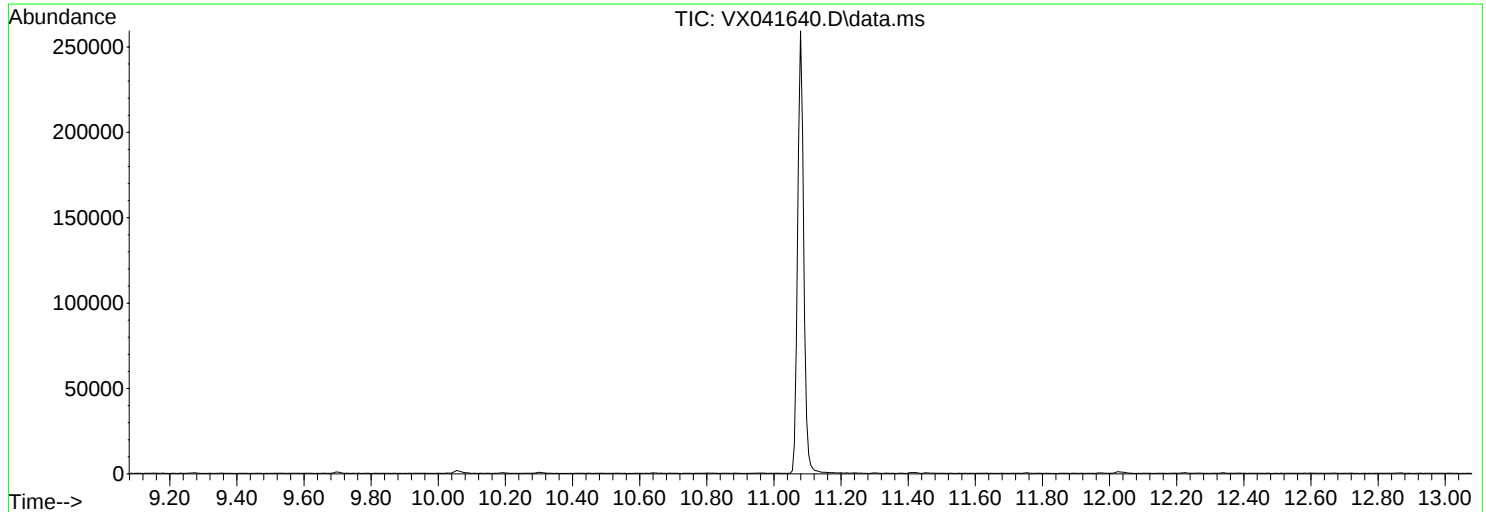

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	8070	PASS
75	95	30	60	50.2	20563	PASS
95	95	100	100	100.0	40963	PASS
96	95	5	9	6.9	2819	PASS
173	174	0.00	2	0.3	120	PASS
174	95	50	100	95.2	39005	PASS
175	174	5	9	7.7	3013	PASS
176	174	95	101	98.7	38504	PASS
177	176	5	9	6.6	2533	PASS