

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052522\
 Data File : VX028955.D
 Acq On : 25 May 2022 17:01
 Operator : JC/MD
 Sample : N3034-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FD-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M

Title : SW846 8260

Signal : TIC: VX028955.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	20	25	32	rBV	33240	56870	3.22%	0.553%
2	1.495	63	67	72	rBV	25875	31074	1.76%	0.302%
3	2.379	207	212	221	rBV	25289	41585	2.35%	0.404%
4	2.532	228	237	246	rBV	11330	22927	1.30%	0.223%
5	2.946	298	305	317	rVB4	7835	21078	1.19%	0.205%
6	5.391	687	706	721	rBV	216129	635402	35.95%	6.179%
7	5.556	721	733	750	rVB	336636	948887	53.68%	9.227%
8	5.958	787	799	814	rBV	223116	591759	33.48%	5.754%
9	6.763	921	931	950	rBV	545876	1288726	72.91%	12.532%
10	7.129	983	991	1005	rVB	38368	86881	4.92%	0.845%
11	8.653	1234	1241	1260	rBV	1135194	1767590	100.00%	17.188%
12	10.055	1465	1471	1486	rBV	1218666	1619903	91.64%	15.752%
13	11.085	1634	1640	1649	rBV	976246	1265553	71.60%	12.306%
14	12.024	1788	1794	1803	rBV	1374273	1634856	92.49%	15.897%
15	12.219	1821	1826	1833	rBV	94015	137012	7.75%	1.332%
16	12.780	1913	1918	1921	rBV4	14157	22724	1.29%	0.221%
17	12.829	1921	1926	1929	rVV6	21304	44371	2.51%	0.431%
18	12.853	1929	1930	1935	rVB	21025	22243	1.26%	0.216%
19	13.140	1969	1977	1986	rVB4	15927	44451	2.51%	0.432%




Sum of corrected areas: 10283892

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052522\
Data File : VX028955.D
Acq On : 25 May 2022 17:01
Operator : JC/MD
Sample : N3034-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FD-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

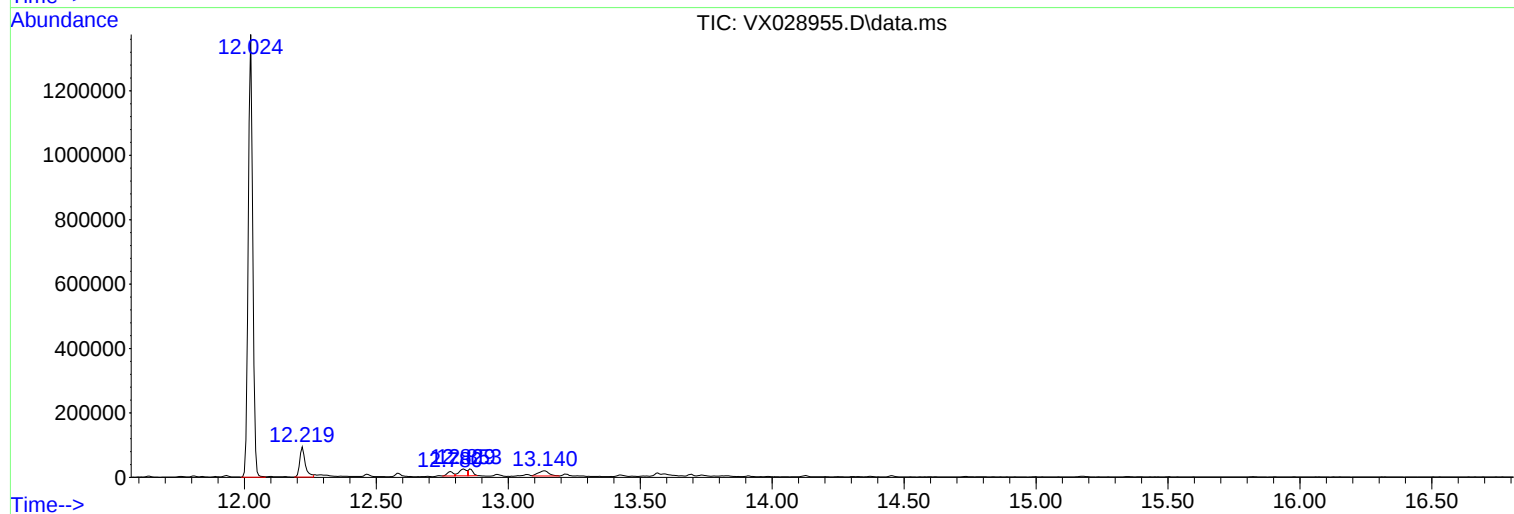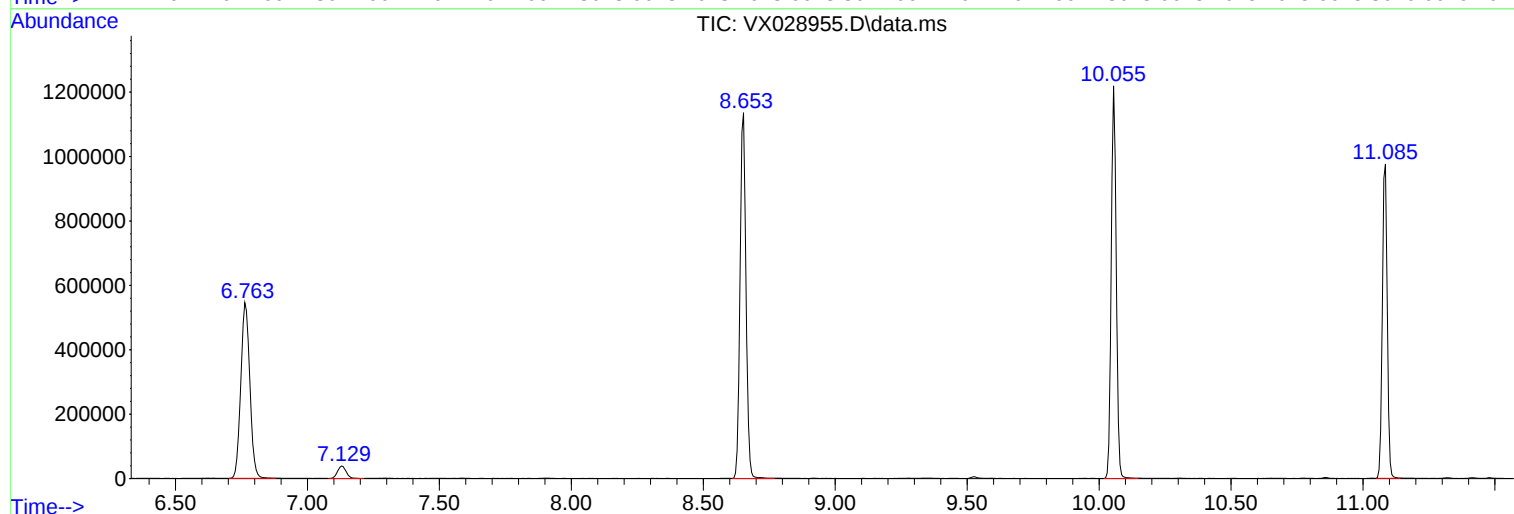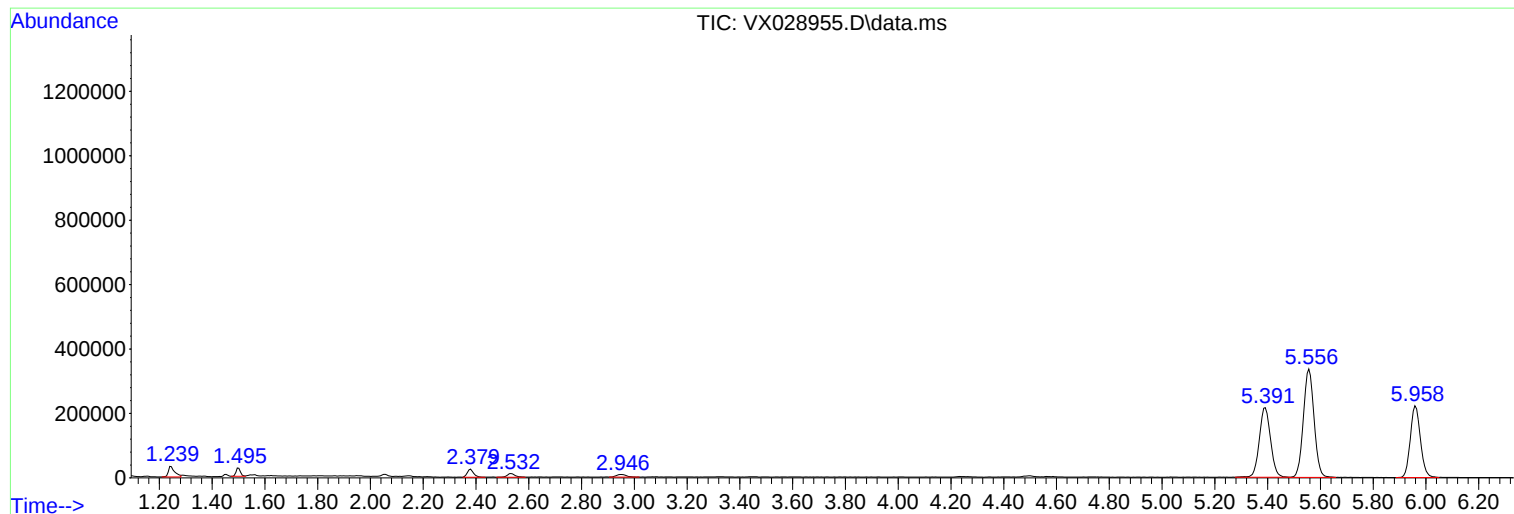

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052522\
Data File : VX028955.D
Acq On : 25 May 2022 17:01
Operator : JC/MD
Sample : N3034-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FD-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052522\
Data File : VX028955.D
Acq On : 25 May 2022 17:01
Operator : JC/MD
Sample : N3034-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FD-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------