

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX052522\  
Data File : VX028974.D  
Acq On : 26 May 2022 01:32  
Operator : JC/MD  
Sample : N3003-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 41 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
13S-20220523

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051222W.M

Title : SW846 8260

Signal : TIC: VX028974.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.391       | 692           | 706         | 721          | rBV2     | 224042         | 654551        | 34.98%          | 6.450%        |
| 2         | 5.556       | 721           | 733         | 750          | rVB      | 355602         | 1002791       | 53.59%          | 9.881%        |
| 3         | 5.958       | 787           | 799         | 815          | rBV      | 234046         | 613656        | 32.79%          | 6.047%        |
| 4         | 6.763       | 920           | 931         | 947          | rBV      | 576617         | 1368640       | 73.14%          | 13.486%       |
| 5         | 8.653       | 1234          | 1241        | 1258         | rBV      | 1209796        | 1871374       | 100.00%         | 18.439%       |
| 6         | 10.055      | 1465          | 1471        | 1490         | rBV      | 1272036        | 1697807       | 90.73%          | 16.729%       |
| 7         | 11.085      | 1634          | 1640        | 1651         | rBV      | 1002461        | 1318546       | 70.46%          | 12.992%       |
| 8         | 12.024      | 1788          | 1794        | 1803         | rBV      | 1334438        | 1621461       | 86.65%          | 15.977%       |




Sum of corrected areas: 10148826

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX052522\  
Data File : VX028974.D  
Acq On : 26 May 2022 01:32  
Operator : JC/MD  
Sample : N3003-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 41 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
13S-20220523

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051222W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

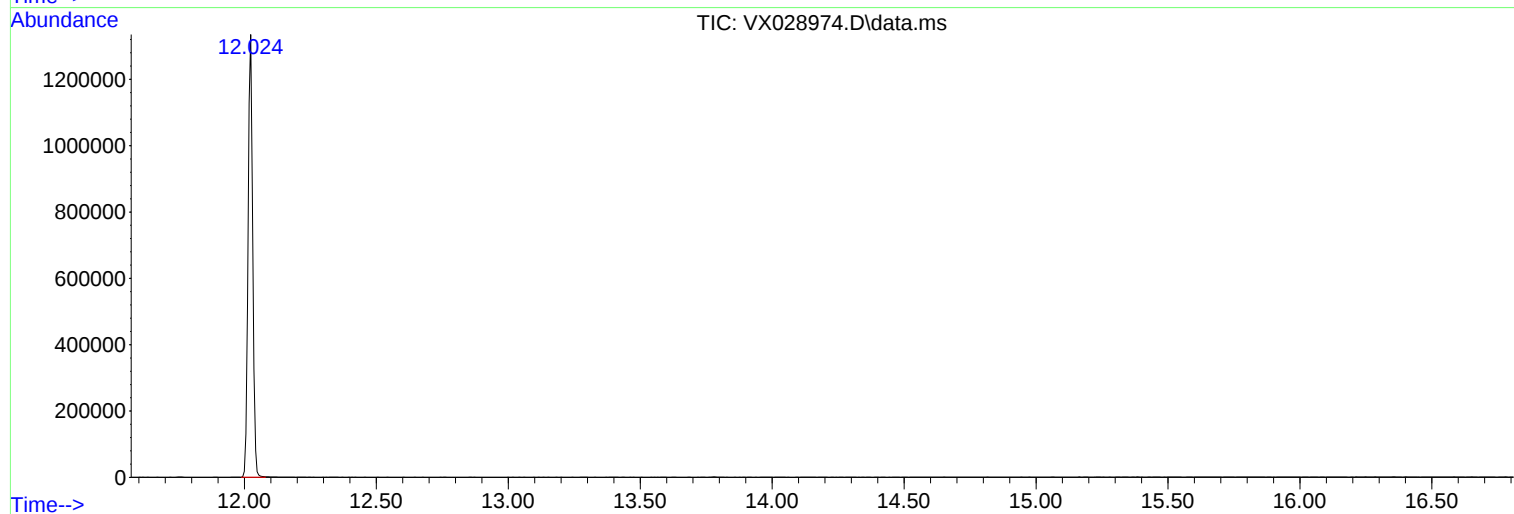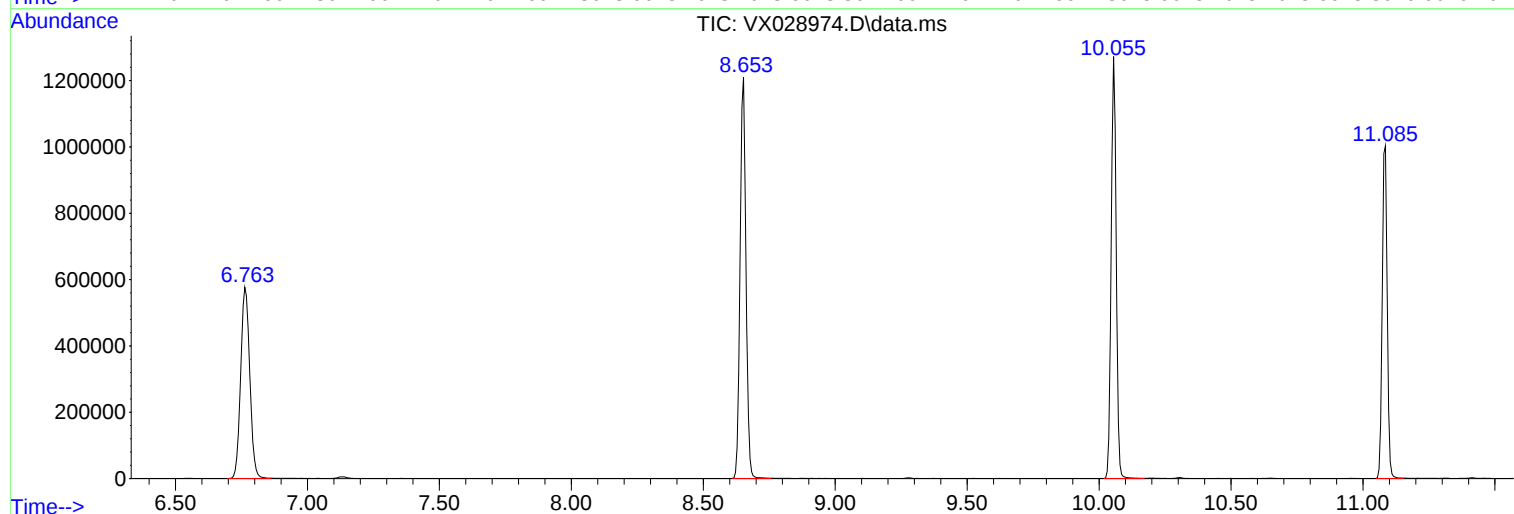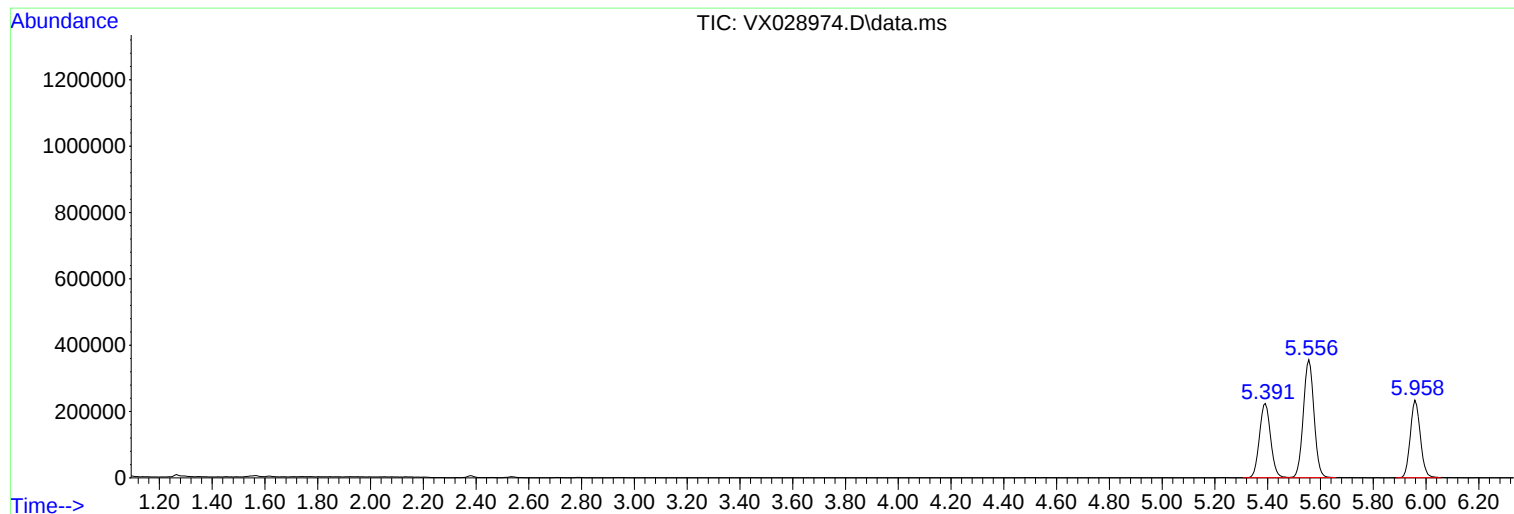

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX052522\  
Data File : VX028974.D  
Acq On : 26 May 2022 01:32  
Operator : JC/MD  
Sample : N3003-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 41 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
13S-20220523

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051222W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX052522\  
Data File : VX028974.D  
Acq On : 26 May 2022 01:32  
Operator : JC/MD  
Sample : N3003-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 41 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
13S-20220523

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051222W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|