

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052523\
 Data File : VX035860.D
 Acq On : 25 May 2023 17:54
 Operator : JC/MD
 Sample : 02881-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SOIL-REF-6

Quant Time: May 26 07:25:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 11 13:57:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	247209	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	477739	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	430093	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	209227	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	215060	49.867	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	99.740%
35) Dibromofluoromethane	5.385	113	159970	49.651	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.300%
50) Toluene-d8	8.647	98	527238	44.297	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	88.600%#
62) 4-Bromofluorobenzene	11.079	95	223121	46.557	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	93.120%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052523\
Data File : VX035860.D
Acq On : 25 May 2023 17:54
Operator : JC/MD
Sample : 02881-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Quant Time: May 26 07:25:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260
QLast Update : Thu May 11 13:57:54 2023
Response via : Initial Calibration




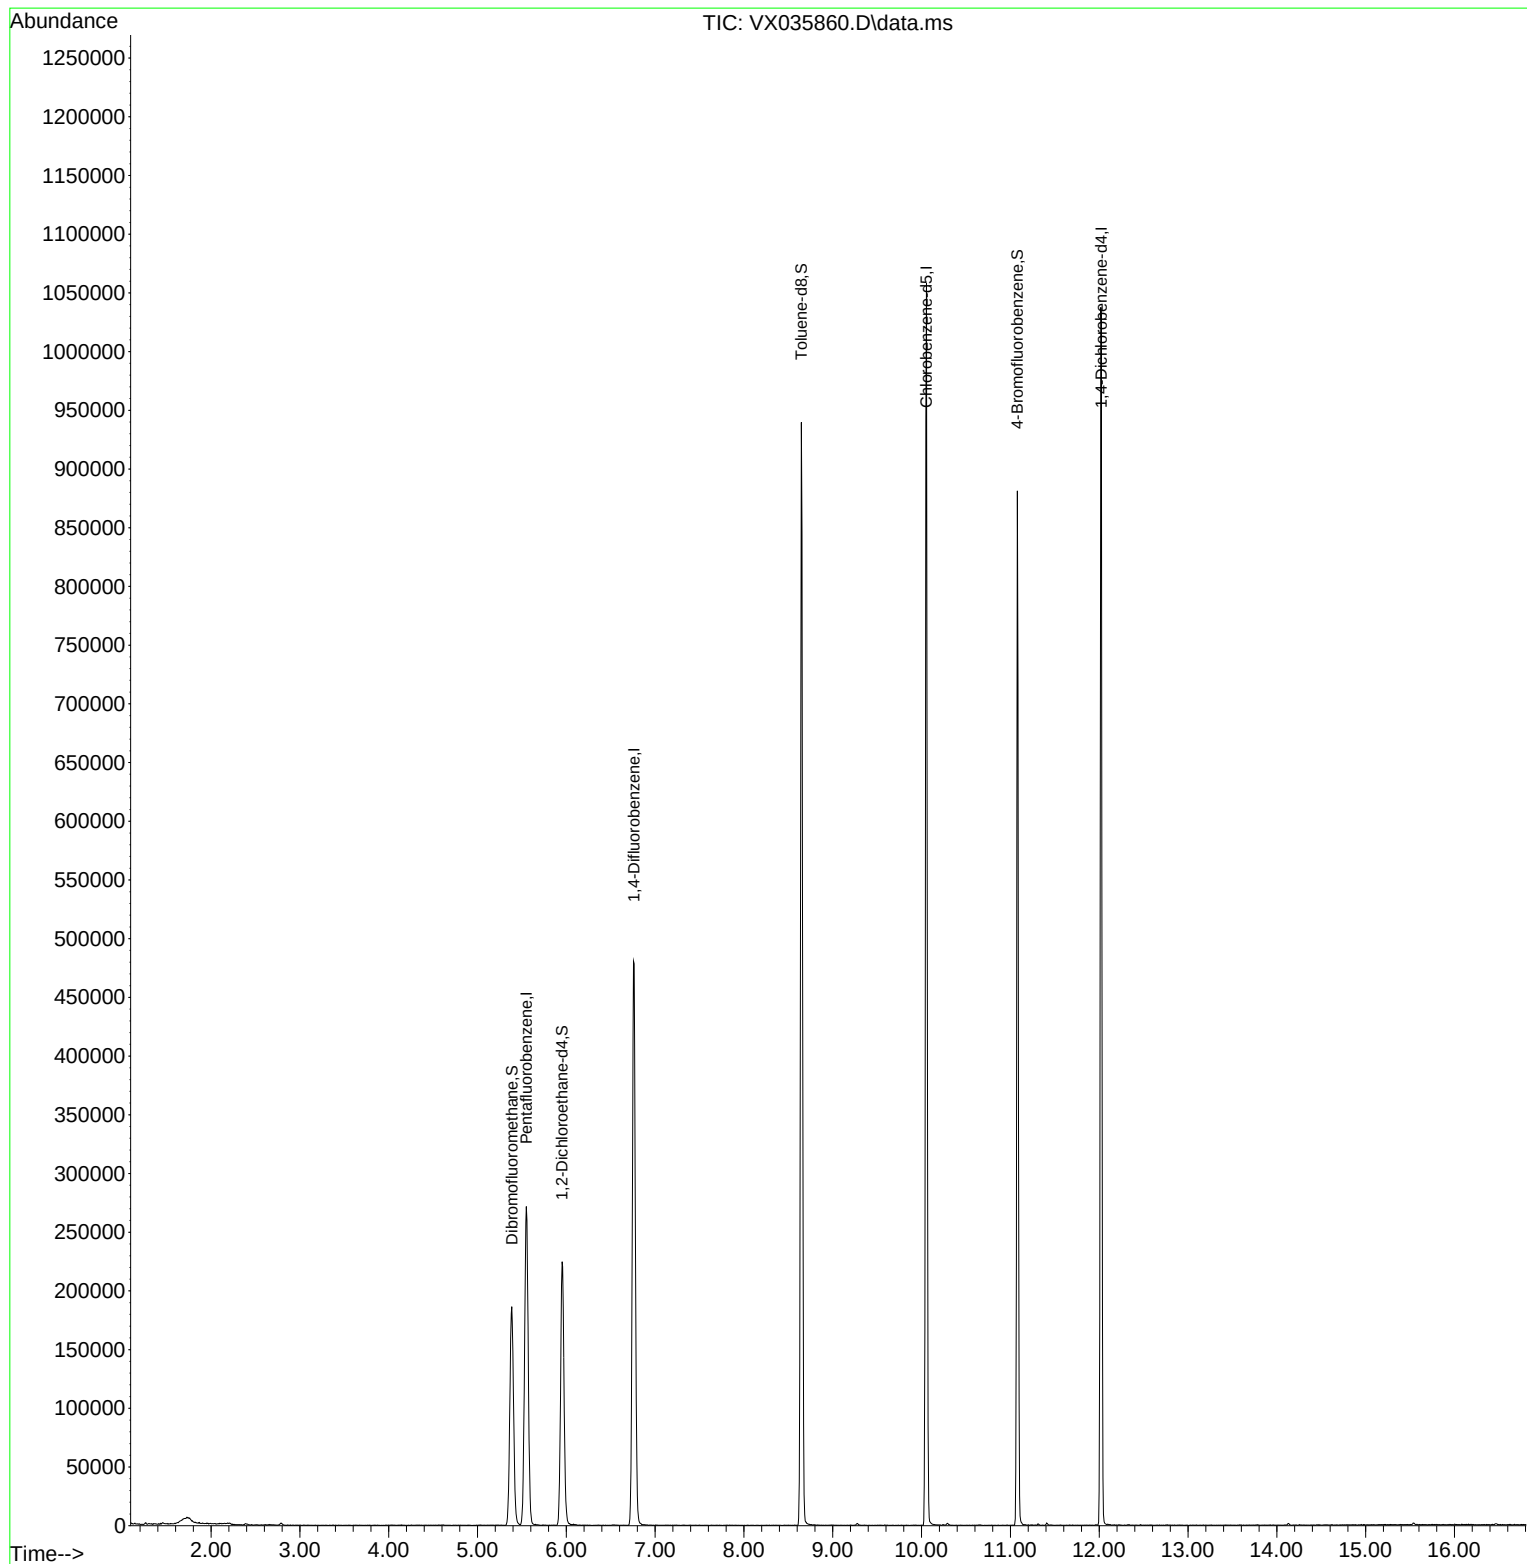


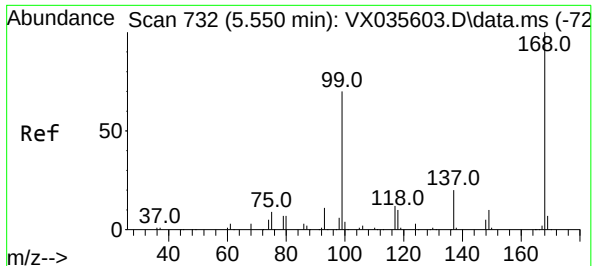

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX035860.D
Acq: 25 May 2023 17:54




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion:168 Resp: 247209
Ion Ratio Lower Upper
168 100
99 62.0 45.7 68.5

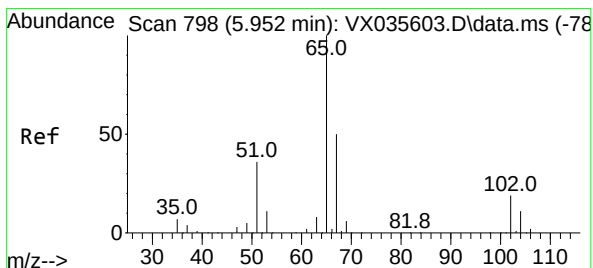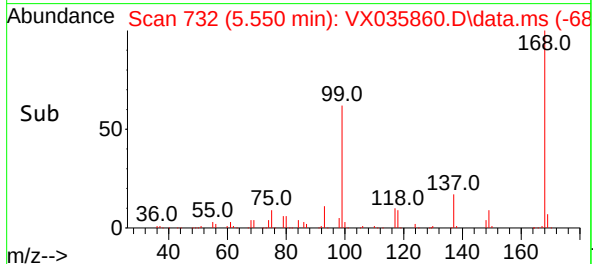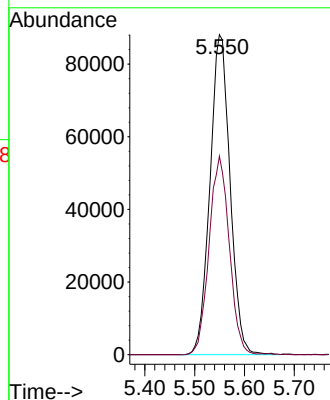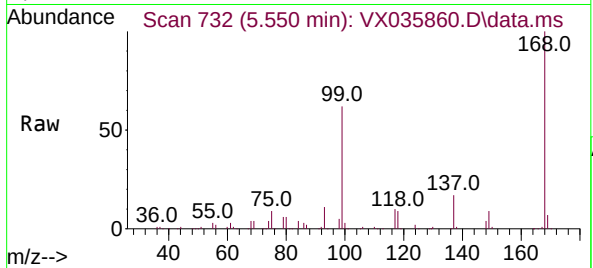

#33
1,2-Dichloroethane-d4
Concen: 49.867 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX035860.D
Acq: 25 May 2023 17:54

Tgt Ion: 65 Resp: 215060
Ion Ratio Lower Upper
65 100
67 50.7 0.0 104.0


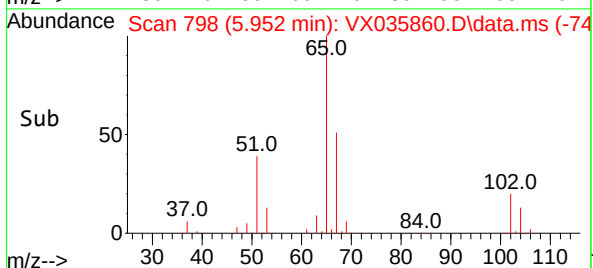
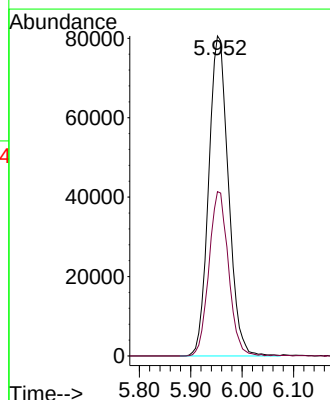
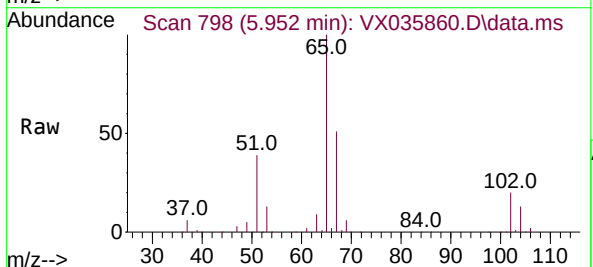


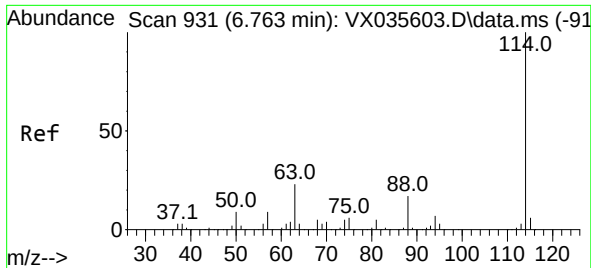

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX035860.D
Acq: 25 May 2023 17:54




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion:114 Resp: 477739
Ion Ratio Lower Upper
114 100
63 22.1 0.0 42.2
88 16.1 0.0 33.2

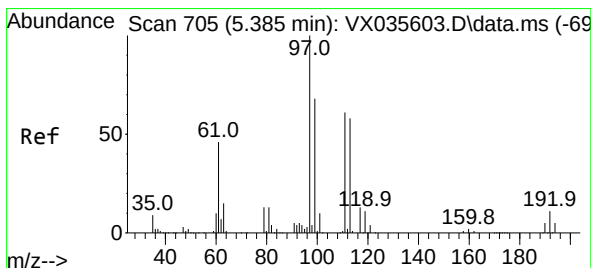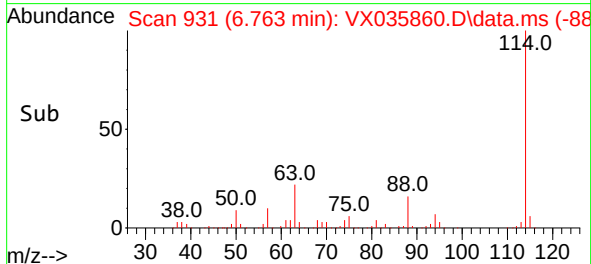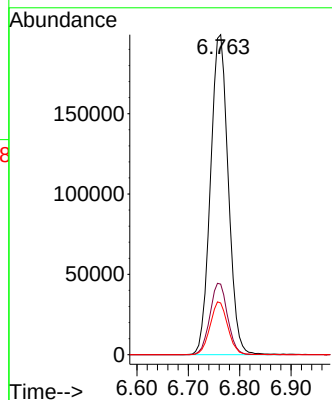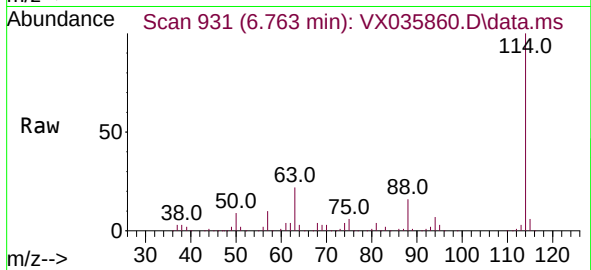

#35
Dibromofluoromethane
Concen: 49.651 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX035860.D
Acq: 25 May 2023 17:54

Tgt Ion:113 Resp: 159970
Ion Ratio Lower Upper
113 100
111 104.6 83.7 125.5
192 17.7 15.4 23.2


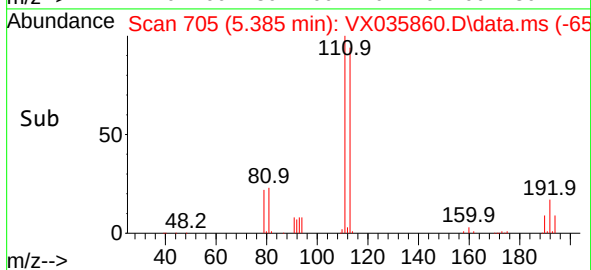
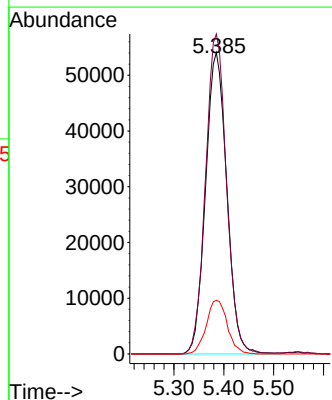
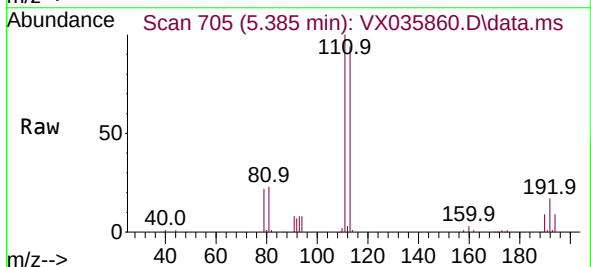


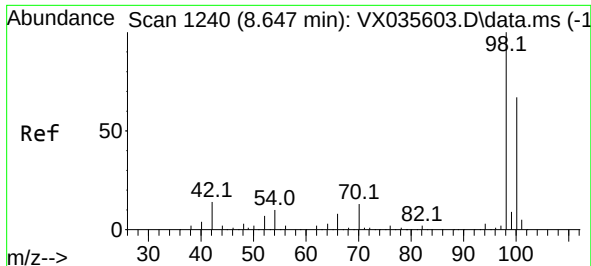

#50
Toluene-d8
Concen: 44.297 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX035860.D
Acq: 25 May 2023 17:54




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion: 98 Resp: 527238
Ion Ratio Lower Upper
98 100
100 66.1 52.5 78.7

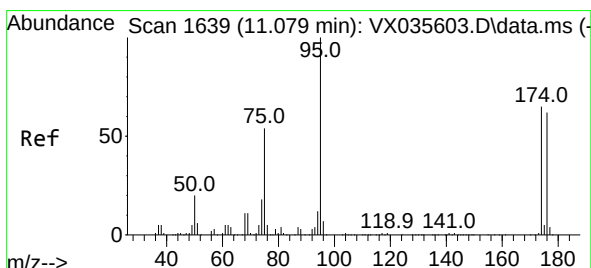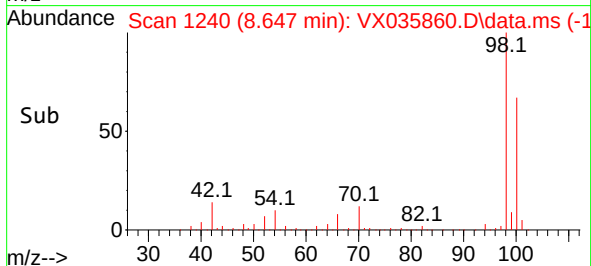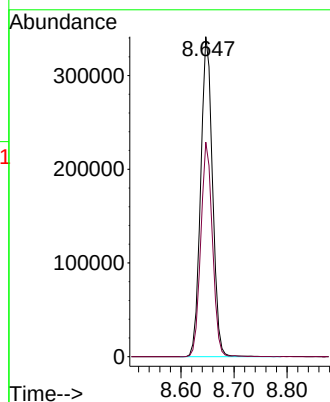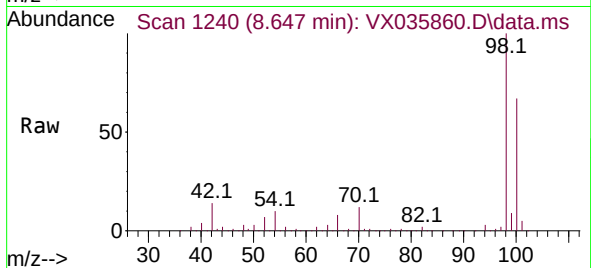

#62
4-Bromofluorobenzene
Concen: 46.557 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX035860.D
Acq: 25 May 2023 17:54

Tgt Ion: 95 Resp: 223121
Ion Ratio Lower Upper
95 100
174 68.9 0.0 147.4
176 67.5 0.0 140.6


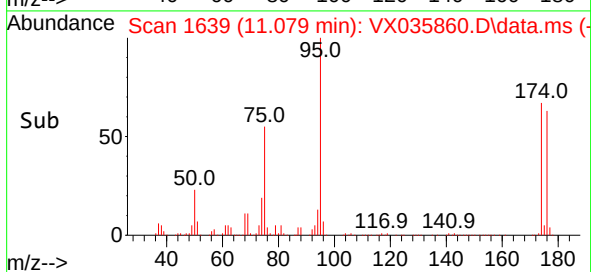
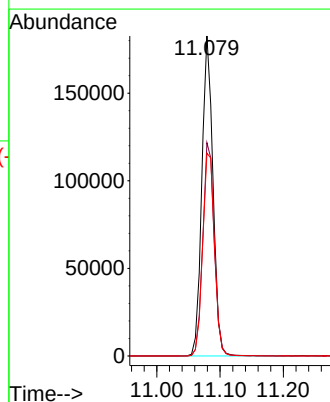
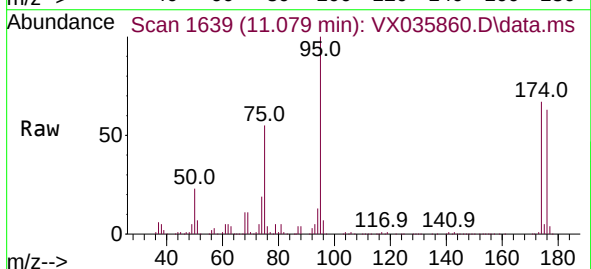


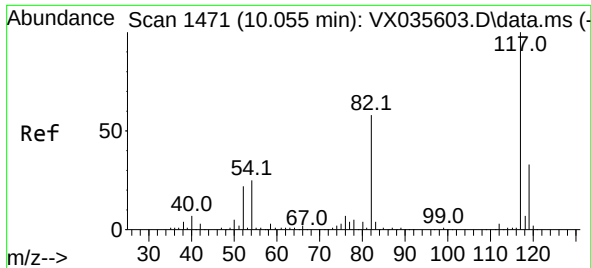

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX035860.D
Acq: 25 May 2023 17:54

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Tgt Ion:117 Resp: 430093
Ion Ratio Lower Upper
117 100
82 59.1 45.0 67.4
119 32.1 26.0 39.0

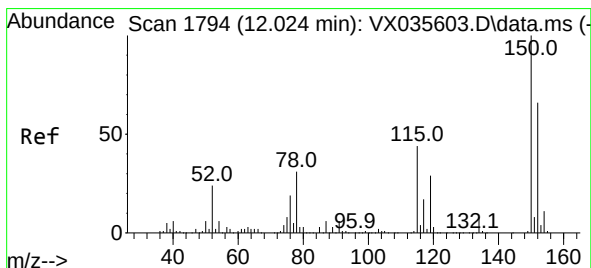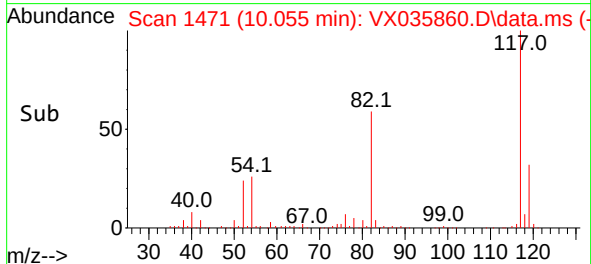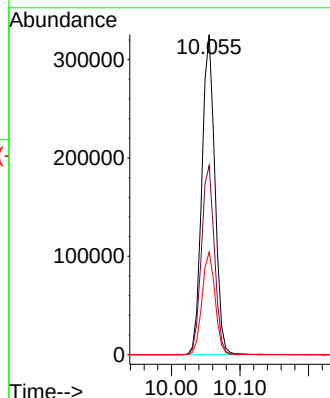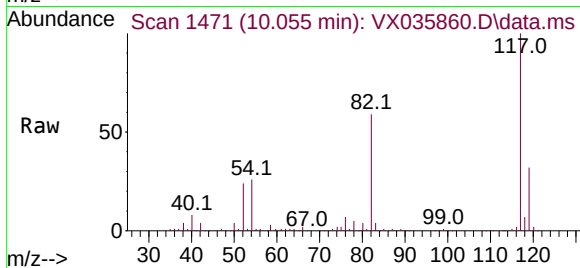

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX035860.D
Acq: 25 May 2023 17:54

Tgt Ion:152 Resp: 209227
Ion Ratio Lower Upper
152 100
115 61.8 45.0 135.0
150 153.5 0.0 352.4

