

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052621\
 Data File : VX022184.D
 Acq On : 25 May 2021 18:37
 Operator : JC/MD
 Sample : VX0526WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0526WBL01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML052621WMA.M
 Title : VOC Analysis

Signal : TIC: VX022184.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	54	rVB	104774	99323	13.60%	1.872%
2	1.666	91	95	104	rVB	74613	95005	13.01%	1.790%
3	2.306	195	200	212	rVB	155463	257613	35.29%	4.855%
4	2.508	231	233	236	rBV2	1120	1460	0.20%	0.028%
5	2.794	275	280	285	rBV4	1711	2902	0.40%	0.055%
6	2.959	302	307	315	rVB2	2142	4698	0.64%	0.089%
7	3.440	385	386	389	rBV2	291	294	0.04%	0.006%
8	3.538	401	402	406	rBV2	197	216	0.03%	0.004%
9	3.684	424	426	429	rVB	262	234	0.03%	0.004%
10	4.105	494	495	500	rVB2	351	354	0.05%	0.007%
11	4.147	500	502	503	rBV2	293	222	0.03%	0.004%
12	4.324	529	531	533	rBV	201	208	0.03%	0.004%
13	4.471	544	555	569	rBV	60832	169975	23.28%	3.203%
14	4.952	633	634	637	rVB2	337	270	0.04%	0.005%
15	5.068	641	653	668	rVV	96207	288107	39.46%	5.430%
16	5.172	668	670	673	rVV2	427	451	0.06%	0.008%
17	5.391	704	706	709	rVB3	346	375	0.05%	0.007%
18	5.483	718	721	723	rBV	419	397	0.05%	0.007%
19	5.537	729	730	732	rBV	309	260	0.04%	0.005%
20	5.806	772	774	776	rBV	228	223	0.03%	0.004%
21	5.885	784	787	789	rBV2	265	374	0.05%	0.007%
22	5.976	791	802	819	rVV3	247669	730079	100.00%	13.759%
23	6.409	872	873	874	rBV	449	224	0.03%	0.004%
24	6.617	903	907	909	rBV2	241	274	0.04%	0.005%
25	6.769	922	932	943	rBV	151612	366239	50.16%	6.902%
26	6.860	945	947	948	rBV	309	233	0.03%	0.004%
27	7.116	981	989	997	rVB7	3508	7894	1.08%	0.149%
28	7.244	1008	1010	1013	rVV2	387	307	0.04%	0.006%
29	7.318	1013	1022	1038	rVB	150190	330114	45.22%	6.221%
30	7.482	1046	1049	1053	rBV3	438	740	0.10%	0.014%
31	7.811	1100	1103	1107	rVV	489	653	0.09%	0.012%
32	7.921	1119	1121	1129	rVB4	1080	2018	0.28%	0.038%
33	8.330	1181	1188	1198	rBV	107743	172314	23.60%	3.247%
34	8.427	1202	1204	1206	rVV	242	306	0.04%	0.006%
35	8.476	1208	1212	1219	rVB3	821	1522	0.21%	0.029%
36	8.653	1233	1241	1248	rBV	380652	584518	80.06%	11.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052621\
 Data File : VX022184.D
 Acq On : 25 May 2021 18:37
 Operator : JC/MD
 Sample : VX0526WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0526WBL01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML052621WMA.M
 Title : VOC Analysis

37	8.726	1249	1253	1259	rVB2	6245	9370	1.28%	0.177%
38	8.836	1269	1271	1274	rVV	283	265	0.04%	0.005%
39	8.951	1285	1290	1303	rVB	76831	114526	15.69%	2.158%
40	9.153	1321	1323	1325	rBV2	300	293	0.04%	0.006%
41	9.275	1341	1343	1348	rBV3	1030	1314	0.18%	0.025%
42	9.390	1356	1362	1379	rBV	265165	373961	51.22%	7.048%
43	9.500	1379	1380	1385	rVB3	349	238	0.03%	0.004%
44	9.707	1408	1414	1415	rBV3	546	781	0.11%	0.015%
45	10.055	1466	1471	1481	rBV	310636	436179	59.74%	8.220%
46	10.195	1490	1494	1499	rVB2	921	1277	0.17%	0.024%
47	10.305	1508	1512	1519	rBV3	1585	2416	0.33%	0.046%
48	10.439	1532	1534	1538	rVB	392	429	0.06%	0.008%
49	10.469	1538	1539	1540	rBV	375	211	0.03%	0.004%
50	10.524	1547	1548	1550	rBV	205	193	0.03%	0.004%
51	10.652	1566	1569	1575	rVB4	1222	1904	0.26%	0.036%
52	10.726	1579	1581	1585	rBV2	244	292	0.04%	0.006%
53	10.774	1585	1589	1592	rBV2	198	276	0.04%	0.005%
54	10.805	1592	1594	1597	rBV	266	218	0.03%	0.004%
55	10.963	1618	1620	1625	rVB2	748	759	0.10%	0.014%
56	11.085	1636	1640	1643	rBV2	285	469	0.06%	0.009%
57	11.122	1643	1646	1652	rVB2	2039	2789	0.38%	0.053%
58	11.195	1652	1658	1666	rBV	265546	344654	47.21%	6.495%
59	11.280	1670	1672	1674	rBV	418	309	0.04%	0.006%
60	11.305	1674	1676	1678	rVB3	542	399	0.05%	0.008%
61	11.360	1683	1685	1686	rBV	205	201	0.03%	0.004%
62	11.463	1698	1702	1703	rBV2	725	837	0.11%	0.016%
63	11.628	1727	1729	1731	rVB2	376	308	0.04%	0.006%
64	11.713	1741	1743	1744	rVV	288	257	0.04%	0.005%
65	11.756	1746	1750	1755	rVB4	3000	4192	0.57%	0.079%
66	11.847	1761	1765	1768	rVB3	441	654	0.09%	0.012%
67	11.890	1770	1772	1775	rVV	251	200	0.03%	0.004%
68	11.939	1775	1780	1783	rVV3	1148	1550	0.21%	0.029%
69	11.975	1783	1786	1789	rVV	1509	1556	0.21%	0.029%
70	12.024	1789	1794	1807	rVV	316959	393806	53.94%	7.422%
71	12.128	1808	1811	1813	rVV3	877	1166	0.16%	0.022%
72	12.152	1813	1815	1819	rVB2	1683	1675	0.23%	0.032%
73	12.225	1824	1827	1828	rBV	403	388	0.05%	0.007%
74	12.323	1837	1843	1849	rBV	379258	473247	64.82%	8.919%
75	12.433	1858	1861	1863	rBV2	467	501	0.07%	0.009%
76	12.487	1868	1870	1876	rVB2	326	321	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052621\
 Data File : VX022184.D
 Acq On : 25 May 2021 18:37
 Operator : JC/MD
 Sample : VX0526WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0526WBL01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML052621WMA.M
 Title : VOC Analysis

77	12.658	1894	1898	1902	rVB2	278	359	0.05%	0.007%
78	12.719	1907	1908	1911	rBV2	327	346	0.05%	0.007%
79	12.817	1922	1924	1927	rVB2	232	232	0.03%	0.004%
80	12.865	1930	1932	1934	rBV2	231	209	0.03%	0.004%
81	13.048	1961	1962	1966	rVB2	326	311	0.04%	0.006%
82	13.091	1967	1969	1970	rVB	347	216	0.03%	0.004%
83	13.115	1970	1973	1976	rBV3	1324	1473	0.20%	0.028%
84	13.347	2007	2011	2013	rBV2	209	328	0.04%	0.006%
85	13.591	2048	2051	2055	rVB	1597	1567	0.21%	0.030%
86	13.780	2080	2082	2087	rVB	906	1039	0.14%	0.020%
87	13.896	2099	2101	2106	rBV2	337	477	0.07%	0.009%
88	13.963	2110	2112	2118	rVB3	825	938	0.13%	0.018%
89	14.140	2136	2141	2142	rBV2	404	387	0.05%	0.007%
90	14.359	2174	2177	2178	rBV2	352	341	0.05%	0.006%
91	14.438	2188	2190	2192	rBV2	283	299	0.04%	0.006%
92	14.560	2207	2210	2215	rVB3	381	440	0.06%	0.008%
93	14.786	2246	2247	2250	rVB2	355	244	0.03%	0.005%
94	14.938	2270	2272	2274	rBV	345	356	0.05%	0.007%
95	15.213	2315	2317	2320	rVB3	338	384	0.05%	0.007%
96	15.456	2355	2357	2358	rBV	329	218	0.03%	0.004%
97	15.828	2417	2418	2421	rBV2	466	363	0.05%	0.007%
98	15.871	2424	2425	2427	rVV2	380	214	0.03%	0.004%
99	16.328	2499	2500	2502	rBV	406	275	0.04%	0.005%
100	16.621	2547	2548	2550	rBV	327	301	0.04%	0.006%


Sum of corrected areas: 5306094

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052621\
Data File : VX022184.D
Acq On : 25 May 2021 18:37
Operator : JC/MD
Sample : VX0526WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0526WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML052621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

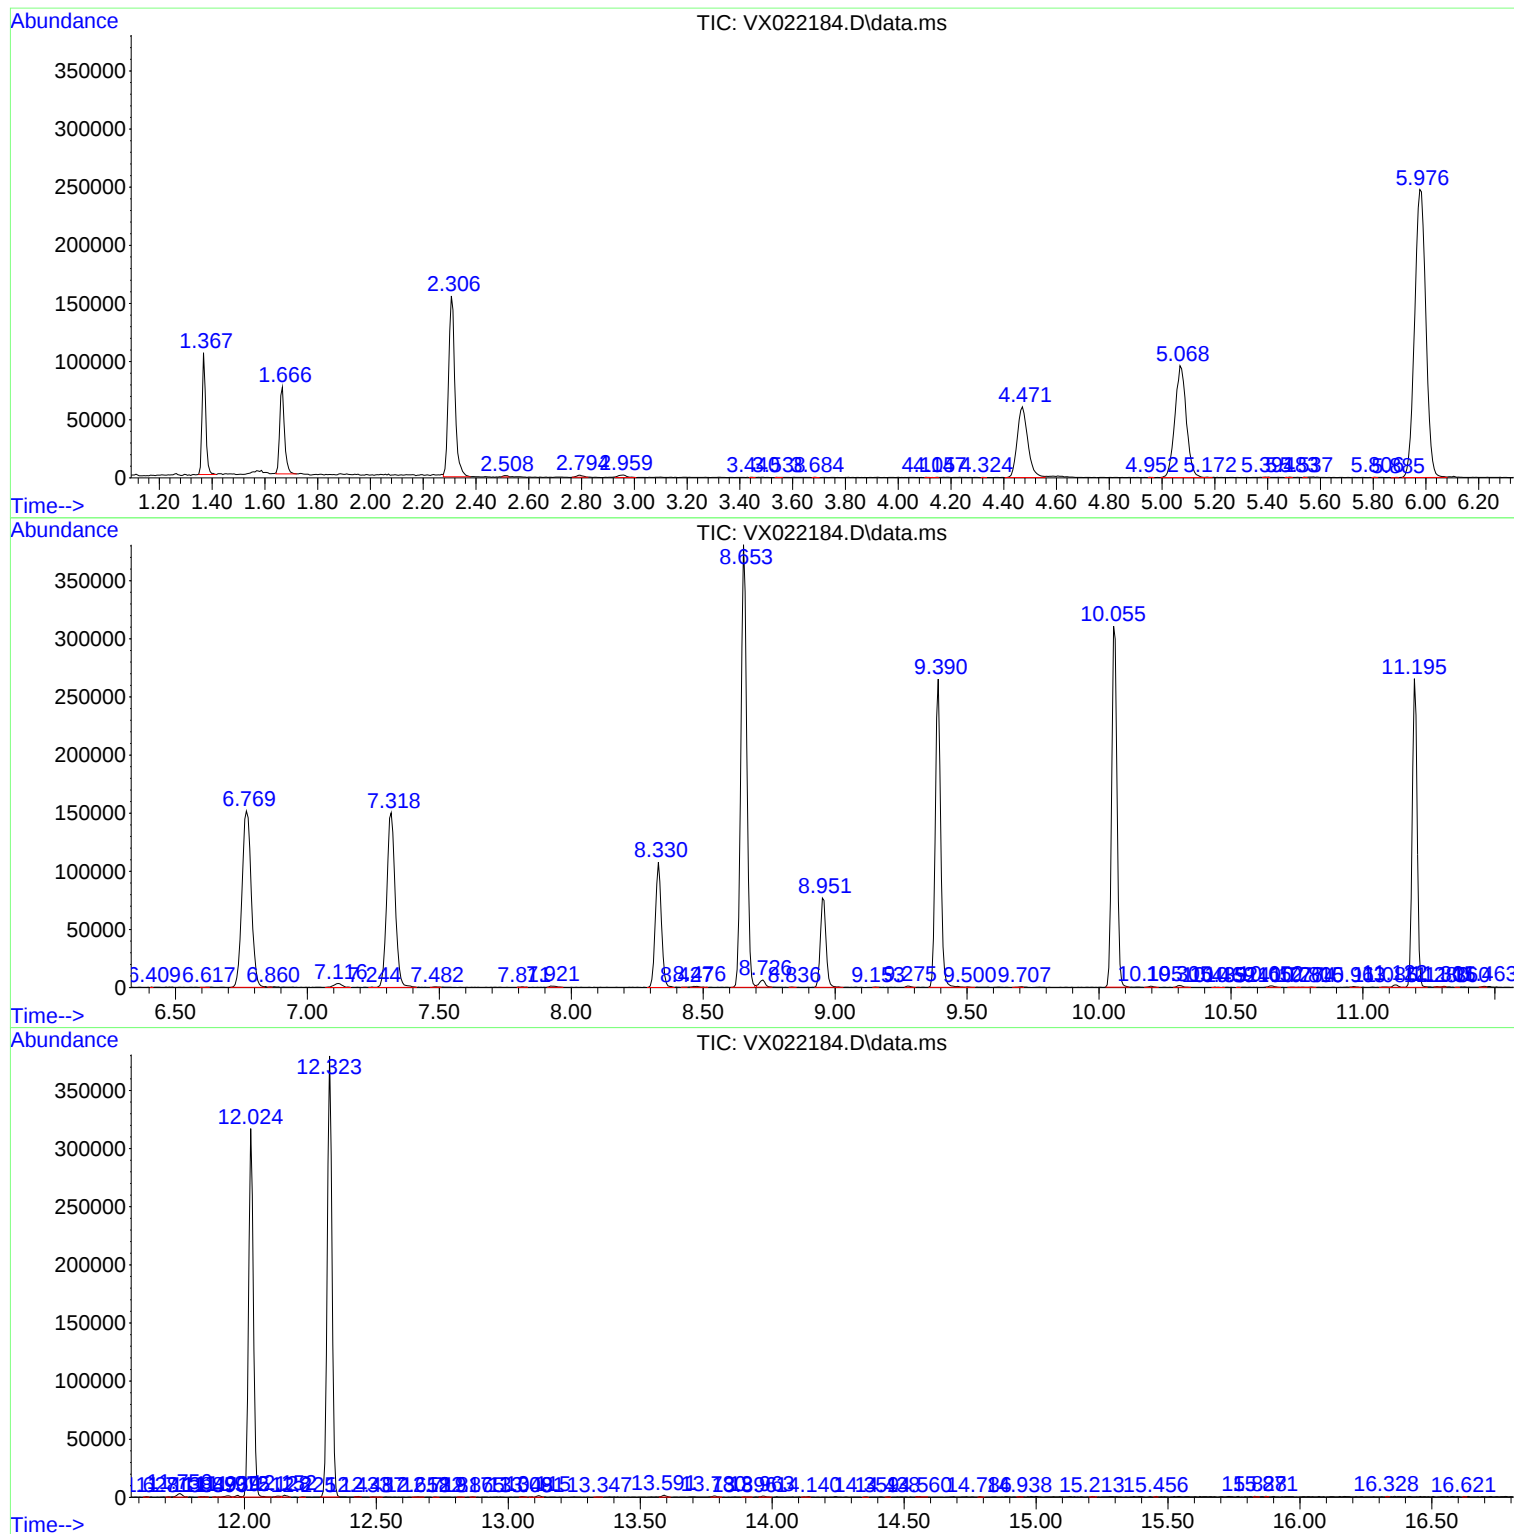

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052621\
Data File : VX022184.D
Acq On : 25 May 2021 18:37
Operator : JC/MD
Sample : VX0526WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0526WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM052621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052621\
Data File : VX022184.D
Acq On : 25 May 2021 18:37
Operator : JC/MD
Sample : VX0526WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0526WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML052621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
