
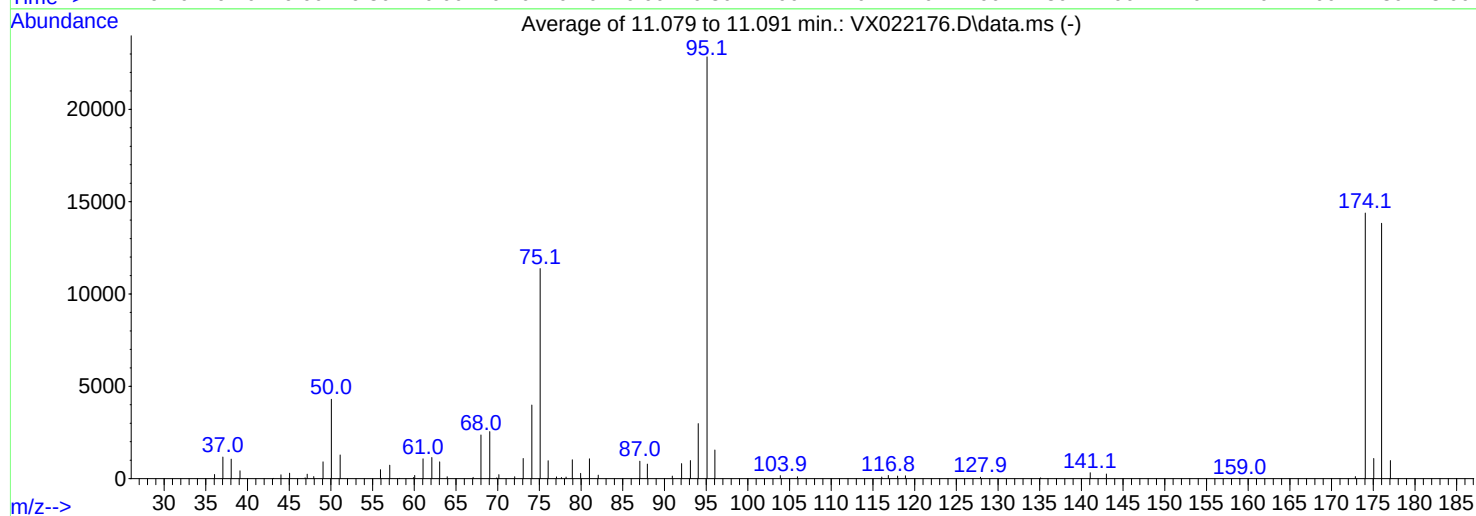


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052621\
 Data File : VX022176.D
 Acq On : 25 May 2021 15:02
 Operator : JC/MD
 Sample : BFB74
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB174

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM052621WMA.M
 Title : VOC Analysis
 Last Update : Tue May 25 17:28:06 2021

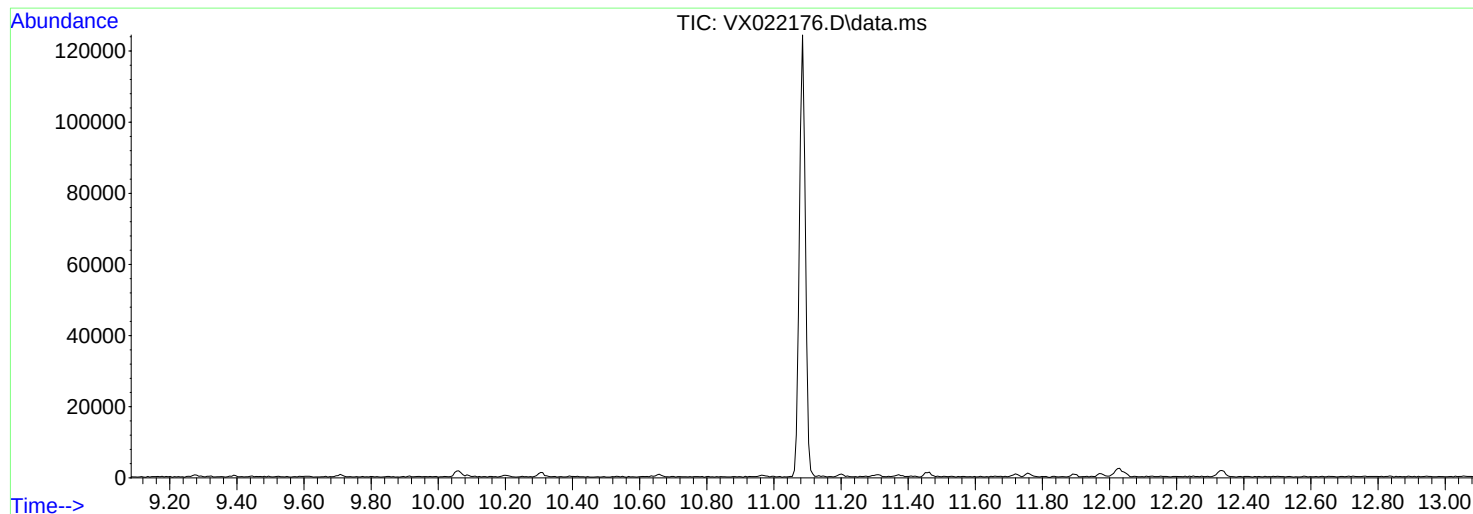

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	4294	PASS
75	95	30	80	49.8	11379	PASS
95	95	100	100	100.0	22843	PASS
96	95	5	9	6.8	1555	PASS
173	174	0.00	2	0.8	114	PASS
174	95	50	120	63.0	14387	PASS
175	174	5	9	7.6	1089	PASS
176	174	95	101	96.1	13828	PASS
177	176	5	9	7.1	980	PASS

m/z	Abundance
40.00	137.0
44.00	165.0

Instrument :
MSVOA_X
ClientSampleId :
BFB174

m/z	Abundance
36.10	200.0
37.00	901.0
38.10	893.0
39.10	326.0
40.00	141.0
44.10	303.0
45.10	171.0
46.90	124.0
47.10	126.0
47.90	129.0
49.10	702.0
50.10	3170.0
51.10	907.0
55.90	395.0
57.00	566.0
60.00	263.0
61.00	944.0
62.10	923.0
63.00	714.0
63.90	118.0
68.00	1799.0
69.00	1935.0
69.90	137.0
72.10	84.0
73.10	1085.0
74.10	3259.0
75.10	9125.0
76.10	477.0
77.10	131.0
78.20	129.0
79.00	920.0
80.00	230.0
81.00	860.0
82.00	180.0
87.00	639.0
87.90	581.0
90.90	150.0
91.90	495.0
92.20	546.0
93.20	800.0
94.10	2491.0
95.10	18648.0
96.10	1362.0
104.00	101.0
106.00	98.0
116.10	107.0
116.90	144.0
118.00	91.0
118.80	189.0
127.80	109.0
141.00	288.0
143.10	226.0
172.90	144.0
174.10	13947.0
175.00	1171.0
176.00	13940.0
177.10	969.0

Instrument :
MSVOA_X
ClientSampleId :
BFB174

m/z	Abundance
36.00	214.0
37.00	1228.0
38.00	1201.0
39.10	444.0
39.90	96.0
43.10	55.0
44.00	410.0
45.00	484.0
47.10	426.0
48.00	84.0
49.10	950.0
50.00	5314.0
51.10	1720.0
56.00	506.0
57.10	761.0
60.10	257.0
61.10	1225.0
62.10	1243.0
63.10	1289.0
63.90	123.0
66.90	69.0
68.00	2817.0
69.10	3132.0
70.20	248.0
71.90	79.0
73.10	1262.0
74.10	4530.0
75.10	14544.0
76.00	1355.0
77.10	97.0
77.70	82.0
78.20	137.0
78.90	1127.0
80.00	341.0
81.00	1258.0
82.00	185.0
87.10	1151.0
87.90	983.0
91.00	127.0
92.10	812.0
93.10	1043.0
94.00	3238.0
95.10	28016.0
96.00	1727.0
103.90	207.0
105.80	99.0
116.10	100.0
116.80	197.0
118.00	150.0
119.00	132.0
128.00	135.0
135.10	74.0
140.90	195.0
141.10	192.0
143.00	293.0
159.00	52.0
172.80	90.0
174.00	17360.0
175.00	1224.0
176.00	16608.0
177.10	1000.0

Instrument :
MSVOA_X
ClientSampleId :
BFB174

m/z	Abundance
36.00	257.0
37.10	1384.0
38.10	1067.0
39.10	518.0
40.00	138.0
44.00	416.0
45.10	226.0
47.30	177.0
48.00	127.0
49.00	1076.0
50.10	4399.0
51.10	1226.0
56.00	545.0
57.10	863.0
58.20	56.0
59.90	178.0
61.00	1053.0
62.10	1265.0
63.10	734.0
64.10	74.0
67.10	149.0
68.00	2471.0
69.00	2565.0
70.10	415.0
72.10	144.0
73.00	917.0
74.10	4178.0
75.10	10467.0
76.10	1069.0
77.00	65.0
77.60	88.0
78.90	1018.0
79.90	288.0
81.00	1114.0
82.10	206.0
87.00	1037.0
88.00	801.0
91.00	145.0
92.00	581.0
93.00	1096.0
94.10	3202.0
95.10	21864.0
96.10	1575.0
103.90	192.0
106.00	109.0
116.00	52.0
116.90	171.0
117.90	163.0
118.90	143.0
135.10	58.0
141.10	275.0
142.90	224.0
172.90	108.0
174.00	11853.0
175.10	871.0
176.00	10937.0
177.00	972.0

Instrument :
MSVOA_X
ClientSampleId :
BFB174