

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052622\
 Data File : VX028995.D
 Acq On : 26 May 2022 13:42
 Operator : JC/MD
 Sample : N3002-01 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-08DL

Quant Time: May 27 07:33:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 12 14:58:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	334990	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	600918	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	580508	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	284716	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	221800	48.302	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	96.600%		
35) Dibromofluoromethane	5.385	113	196133	49.816	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	99.640%		
50) Toluene-d8	8.653	98	712049	47.970	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	95.940%		
62) 4-Bromofluorobenzene	11.079	95	292057	52.678	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	105.360%		
Target Compounds					Qvalue	
5) Bromomethane	1.612	94	1387	Below Cal		91
6) Chloroethane	1.679	64	567	Below Cal		90
10) Methyl Iodide	2.465	142	1074	0.240 ug/l #		91
11) Tert butyl alcohol	2.947	59	11855	4.324 ug/l #		76
16) Acetone	2.380	43	1213	0.616 ug/l		100
19) Methyl tert-butyl Ether	3.117	73	2799	0.228 ug/l #		35
20) Methylene Chloride	2.788	84	1853	0.448 ug/l		94
31) Cyclohexane	5.477	56	2243	0.352 ug/l #		81
36) 1,1-Dichloropropene	5.556	75	25864	4.374 ug/l #		50
38) Carbon Tetrachloride	5.550	117	34367	5.775 ug/l #		15
39) Methylcyclohexane	7.373	83	2614	0.385 ug/l #		90
40) Benzene	6.044	78	14268	0.840 ug/l		95
44) Trichloroethene	7.123	130	1392	0.302 ug/l		66
52) Toluene	8.720	92	13160	1.204 ug/l		97
53) t-1,3-Dichloropropene	8.994	75	43	1.647 ug/l #		43
67) Ethyl Benzene	10.195	91	317370	14.378 ug/l		99
68) m/p-Xylenes	10.299	106	479921	55.845 ug/l		98
69) o-Xylene	10.640	106	236643	27.968 ug/l		99
70) Styrene	10.640	104	11855	0.863 ug/l #		1
73) Isopropylbenzene	10.964	105	15866	0.735 ug/l		99
76) 1,2,3-Trichloropropane	11.079	75	143491	21.520 ug/l #		38
78) n-propylbenzene	11.305	91	41517	1.662 ug/l		100
79) 2-Chlorotoluene	11.378	91	36883	2.409 ug/l #		41
80) 1,3,5-Trimethylbenzene	11.451	105	95347	5.300 ug/l		100
81) trans-1,4-Dichloro-2-b...	11.079	75	143491	63.100 ug/l #		15
82) 4-Chlorotoluene	11.451	91	10829	0.612 ug/l #		48
83) tert-Butylbenzene	11.976	119	4656	0.267 ug/l		72
84) 1,2,4-Trimethylbenzene	11.750	105	397401	22.027 ug/l		100
85) sec-Butylbenzene	11.750	105	397401	18.495 ug/l #		56
86) p-Isopropyltoluene	11.976	119	4656	0.258 ug/l		95
89) n-Butylbenzene	12.323	91	7180	0.460 ug/l #		11
90) Hexachloroethane	12.616	117	2691	0.923 ug/l #		10
95) Naphthalene	13.774	128	128669	6.360 ug/l		100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_X
ClientSampleId :
MW-08DL

Quant Time: May 27 07:33:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260
QLast Update : Thu May 12 14:58:53 2022
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.007 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-08DL


Tgt Ion:168 Resp: 334990
Ion Ratio Lower Upper
168 100
99 59.2 41.7 62.5

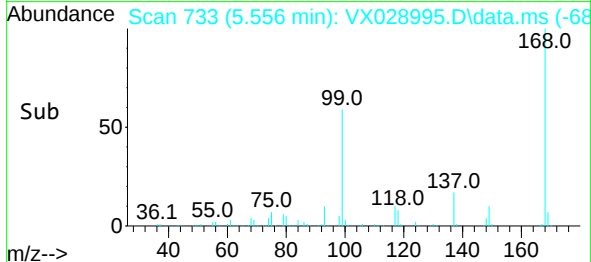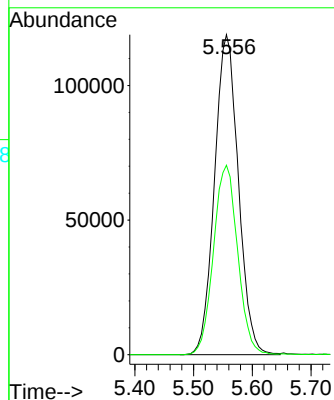

#5
Bromomethane
Concen: Below Cal
RT: 1.612 min Scan# 86
Delta R.T. 0.013 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42

Tgt Ion: 94 Resp: 1387
Ion Ratio Lower Upper
94 100
96 85.7 75.3 112.9


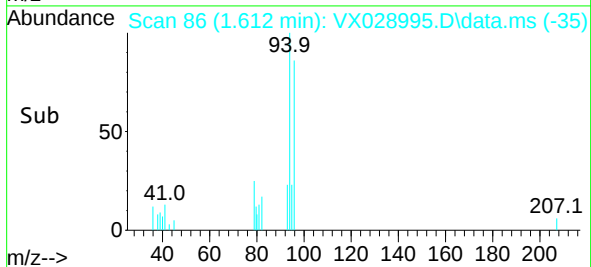
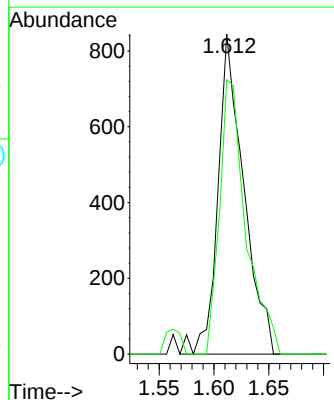
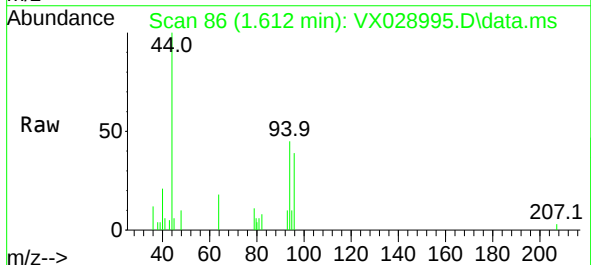


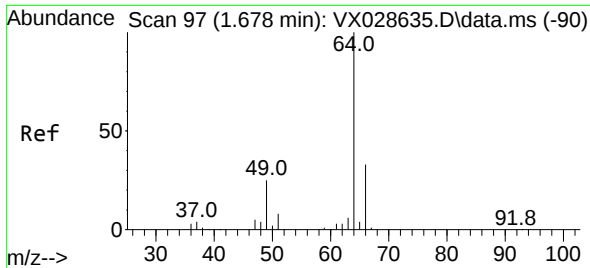

#6
Chloroethane
Concen: Below Cal
RT: 1.679 min Scan# 91
Delta R.T. 0.001 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-08DL


Tgt Ion: 64 Resp: 567
Ion Ratio Lower Upper
64 100
66 25.8 25.3 37.9

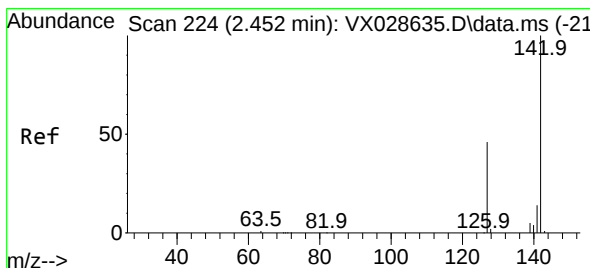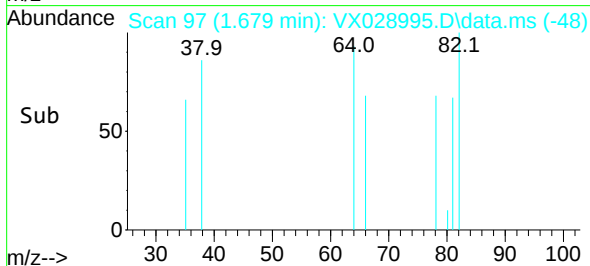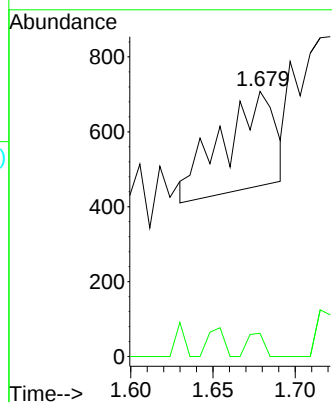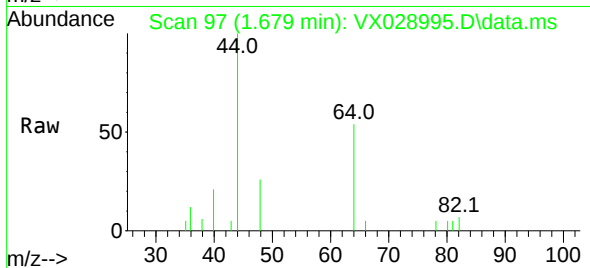

#10
Methyl Iodide
Concen: 0.240 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.013 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42

Tgt Ion: 142 Resp: 1074
Ion Ratio Lower Upper
142 100
127 45.3 33.9 50.9
141 5.9 11.4 17.2#

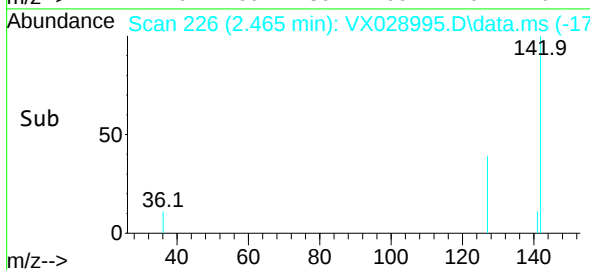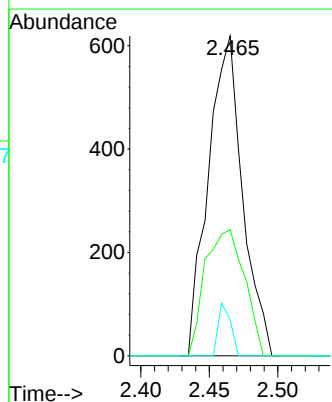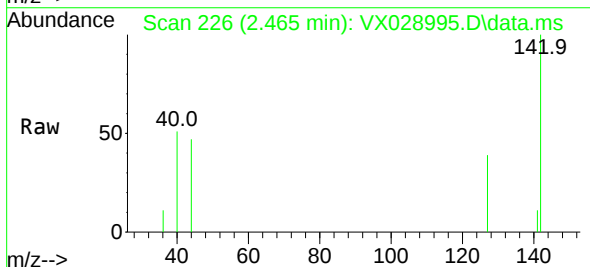

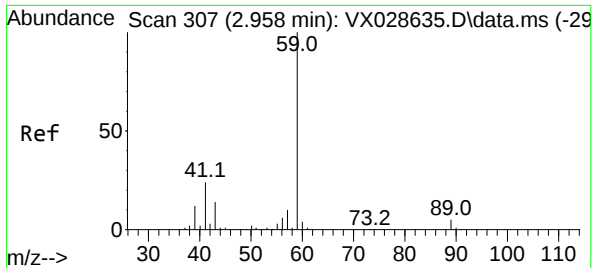

#11

Tert butyl alcohol

Concen: 4.324 ug/l

RT: 2.947 min Scan# 307

Delta R.T. -0.011 min

Lab File: VX028995.D

Acq: 26 May 2022 13:42

Instrument :

MSVOA_X

ClientSampleId :





MW-08DL

Tgt Ion: 59 Resp: 11855

Ion Ratio Lower Upper

59 100

57 1.4 8.3 12.5#

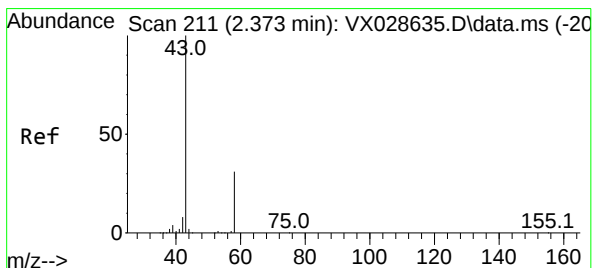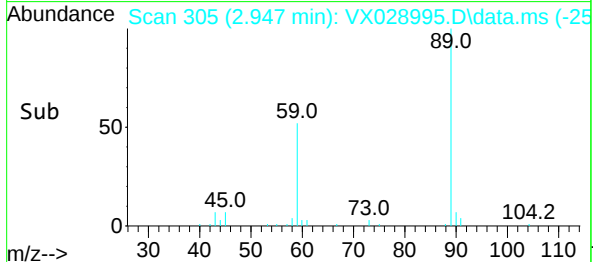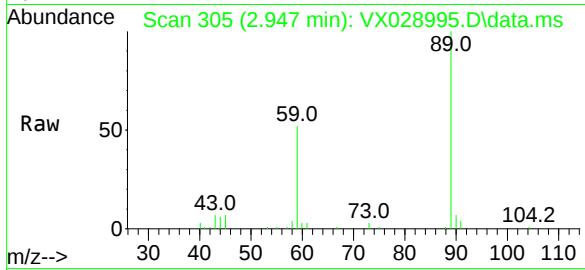

#16

Acetone

Concen: 0.616 ug/l

RT: 2.380 min Scan# 212

Delta R.T. 0.007 min

Lab File: VX028995.D




Acq: 26 May 2022 13:42


Tgt Ion: 43 Resp: 1213

Ion Ratio Lower Upper

43 100

58 35.9 28.8 43.2


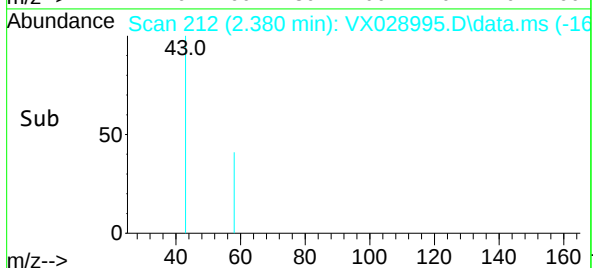
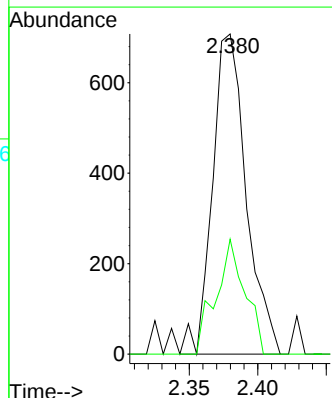
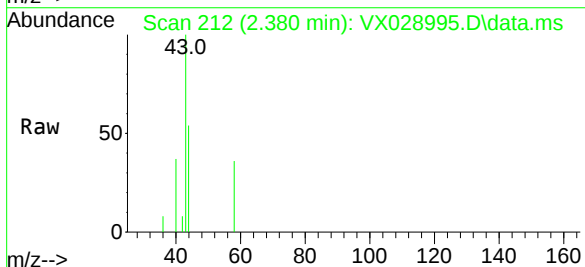




#19
Methyl tert-butyl Ether
Concen: 0.228 ug/l
RT: 3.117 min Scan# 311
Delta R.T. 0.006 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-08DL


Tgt Ion: 73 Resp: 2799
Ion Ratio Lower Upper
73 100
57 51.5 16.8 25.2#

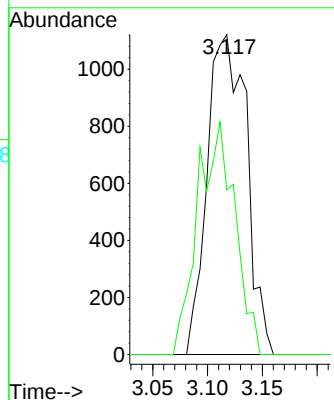

#20
Methylene Chloride
Concen: 0.448 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42


Tgt Ion: 84 Resp: 1853
Ion Ratio Lower Upper
84 100
49 102.0 85.5 128.3
51 29.9 26.6 39.8
86 58.3 51.5 77.3

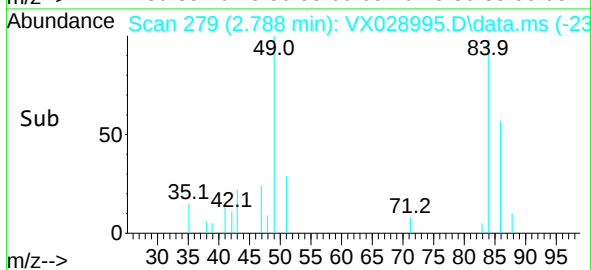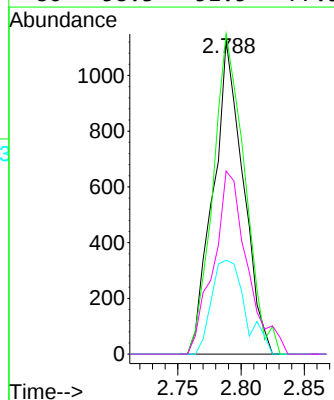






#31
Cyclohexane
Concen: 0.352 ug/l
RT: 5.477 min Scan# 718
Delta R.T. 0.013 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42

Instrument :
MSVOA_X
ClientSampleId :
MW-08DL



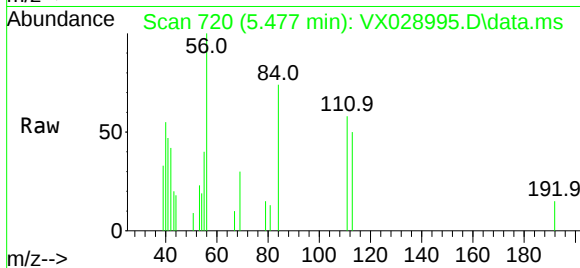



Tgt Ion: 56 Resp: 2243
Ion Ratio Lower Upper
56 100
69 29.9 26.7 40.1
84 73.8 77.2 115.8#

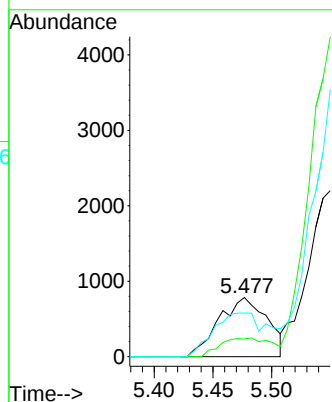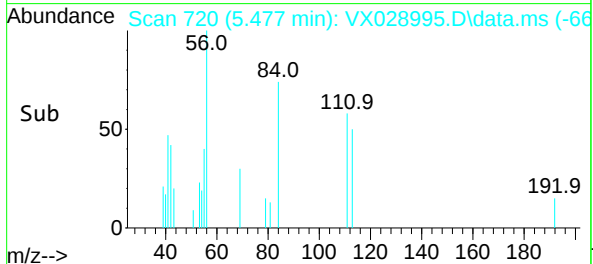

#33
1,2-Dichloroethane-d4
Concen: 48.302 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42

Tgt Ion: 65 Resp: 221800
Ion Ratio Lower Upper
65 100
67 51.1 0.0 107.4



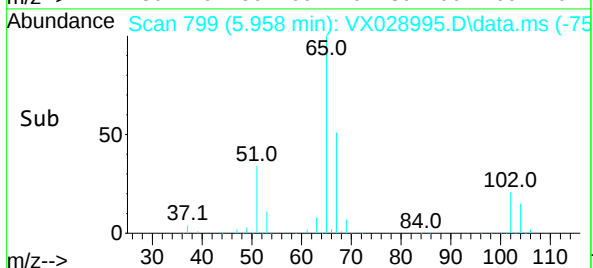
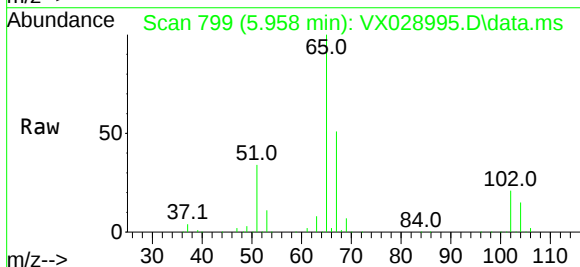




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-08DL


Tgt Ion:114 Resp: 600918
Ion Ratio Lower Upper
114 100
63 19.4 0.0 36.8
88 16.6 0.0 32.4

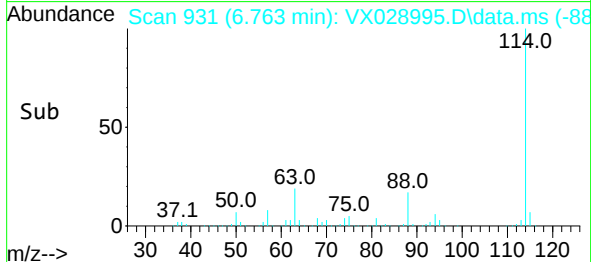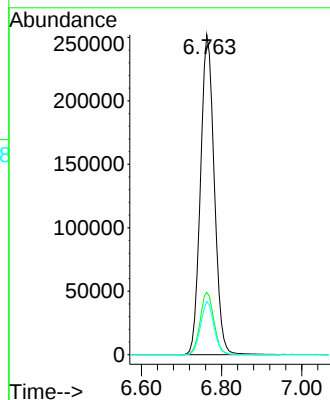

#35
Dibromofluoromethane
Concen: 49.816 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42

Tgt Ion:113 Resp: 196133
Ion Ratio Lower Upper
113 100
111 102.8 82.8 124.2
192 19.6 16.9 25.3

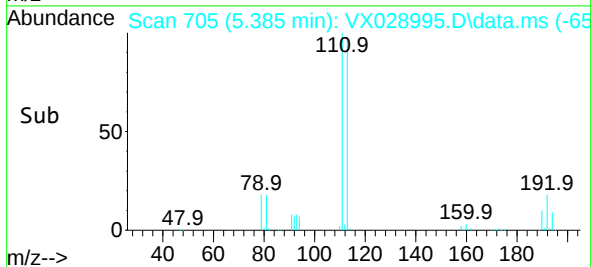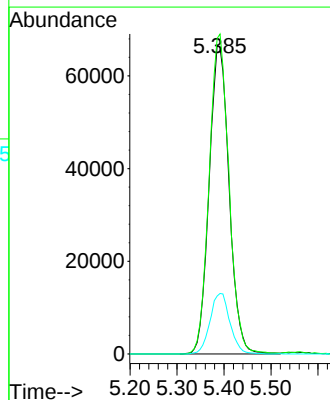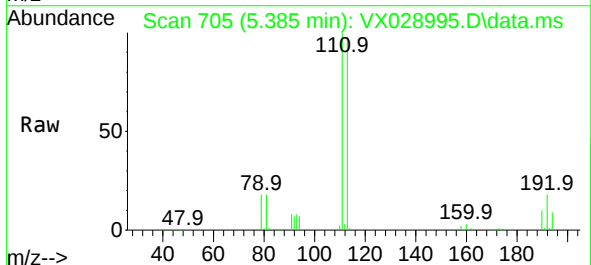



#36

1,1-Dichloropropene

Concen: 4.374 ug/l

RT: 5.556 min Scan# 71

Delta R.T. -0.134 min

Lab File: VX028995.D

Acq: 26 May 2022 13:42

Instrument :

MSVOA_X

ClientSampleId :

MW-08DL





Tgt Ion: 75 Resp: 25864

Ion Ratio Lower Upper

75 100

110 9.9 18.3 54.8#

77 0.0 24.8 37.2#

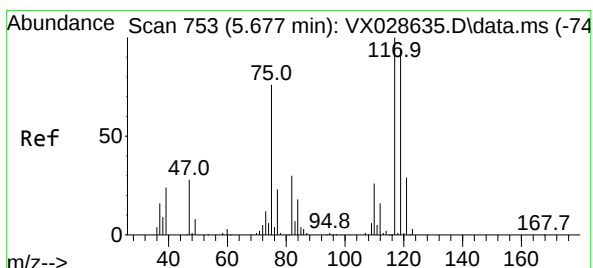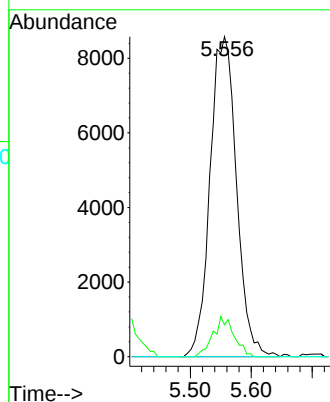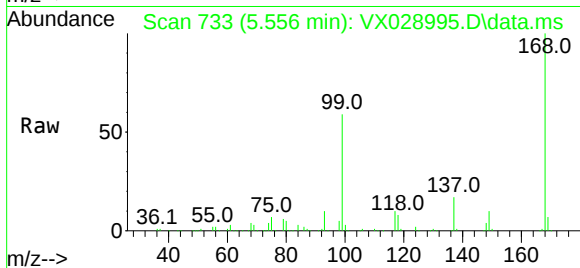

#38

Carbon Tetrachloride

Concen: 5.775 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.127 min

Lab File: VX028995.D

Acq: 26 May 2022 13:42




Tgt Ion: 117 Resp: 34367


Ion Ratio Lower Upper

117 100

119 4.4 77.3 115.9#

121 0.0 24.2 36.2#


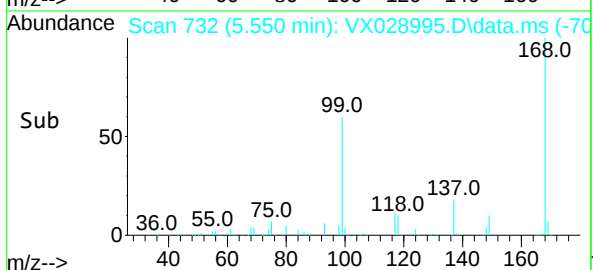
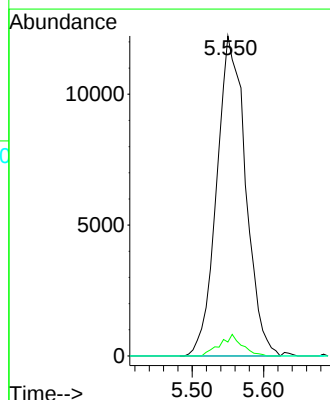
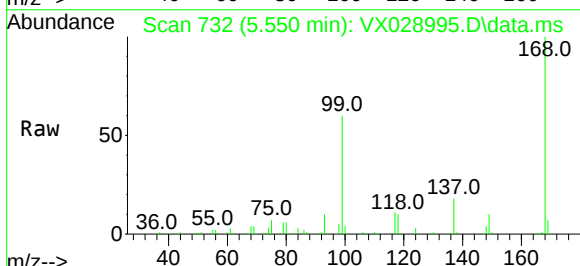




#39
Methylcyclohexane
Concen: 0.385 ug/l
RT: 7.373 min Scan# 1031
Delta R.T. -0.005 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-08DL


Tgt Ion: 83 Resp: 2614
Ion Ratio Lower Upper
83 100
55 63.3 54.6 81.8
98 37.1 37.4 56.2#

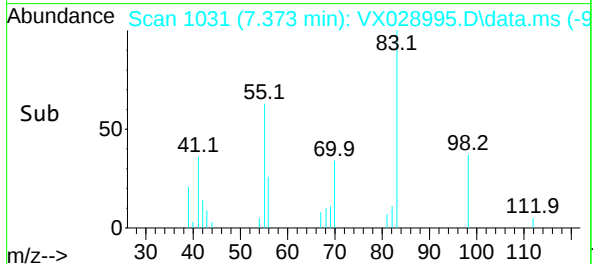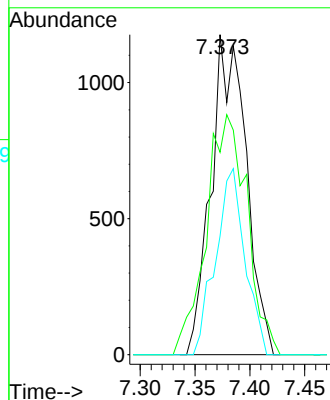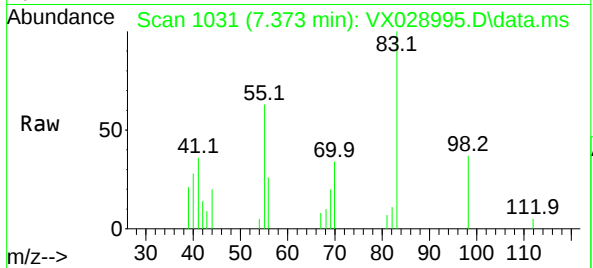

#40
Benzene
Concen: 0.840 ug/l
RT: 6.044 min Scan# 813
Delta R.T. 0.007 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42

Tgt Ion: 78 Resp: 14268
Ion Ratio Lower Upper
78 100
77 21.8 19.3 28.9


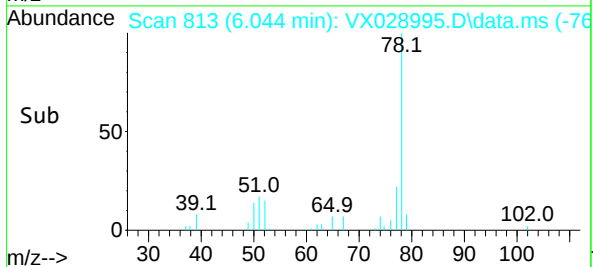
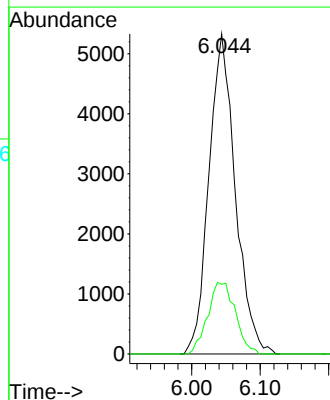
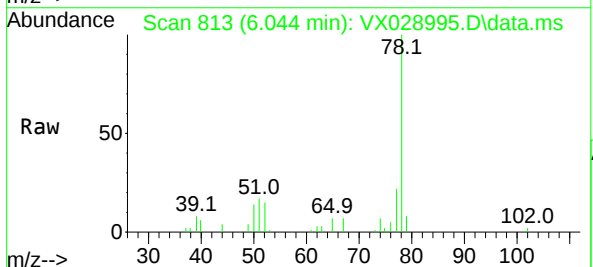




#44
Trichloroethene
Concen: 0.302 ug/l
RT: 7.123 min Scan# 94
Delta R.T. 0.001 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-08DL


Tgt Ion:130 Resp: 1392
Ion Ratio Lower Upper
130 100
95 61.5 0.0 188.8

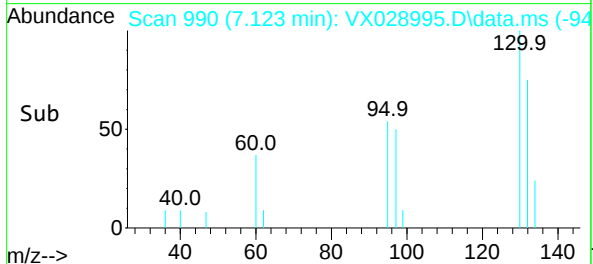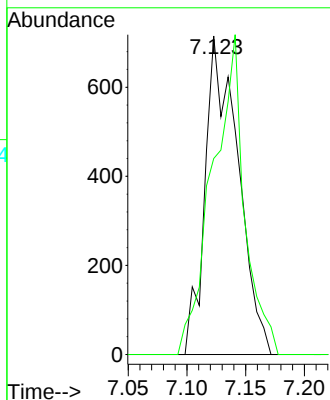

#50
Toluene-d8
Concen: 47.970 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.007 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42

Tgt Ion: 98 Resp: 712049
Ion Ratio Lower Upper
98 100
100 67.0 52.6 78.8


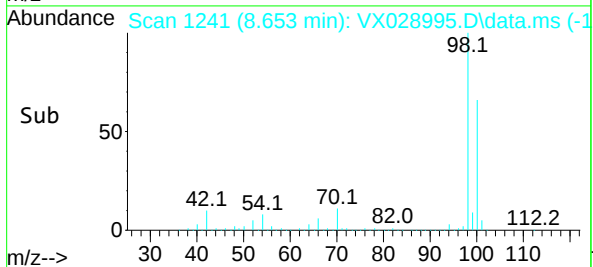
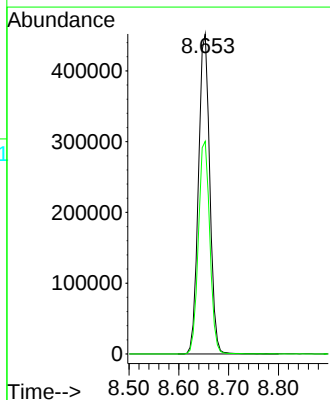
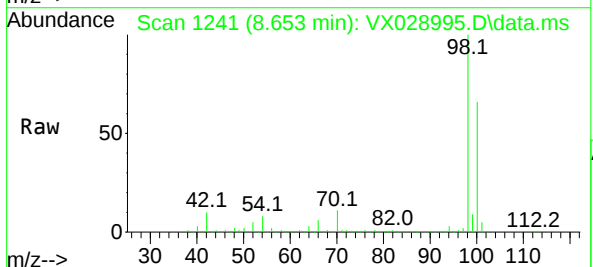




#52
Toluene
Concen: 1.204 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-08DL


Tgt Ion: 92 Resp: 13160
Ion Ratio Lower Upper
92 100
91 168.4 137.5 206.3

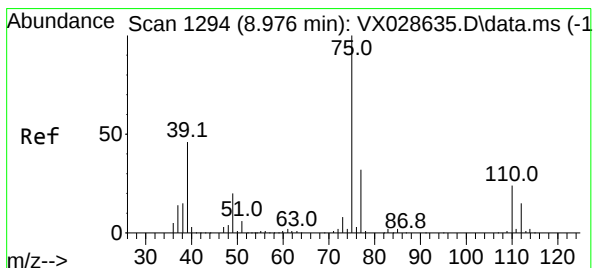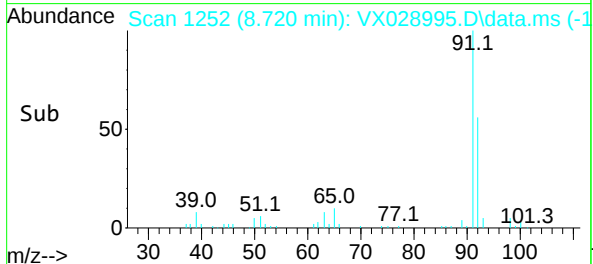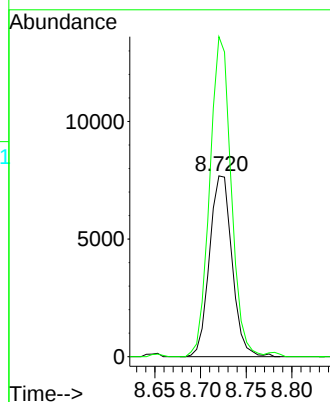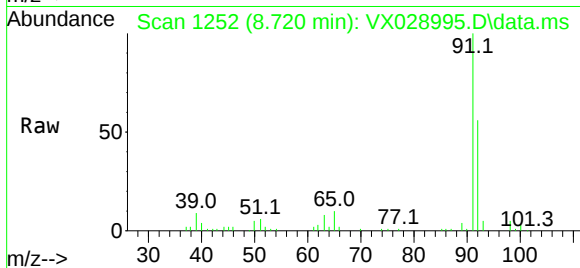

#53
t-1,3-Dichloropropene
Concen: 1.647 ug/l
RT: 8.994 min Scan# 1297
Delta R.T. 0.018 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42

Tgt Ion: 75 Resp: 43
Ion Ratio Lower Upper
75 100
77 0.0 25.4 38.0#


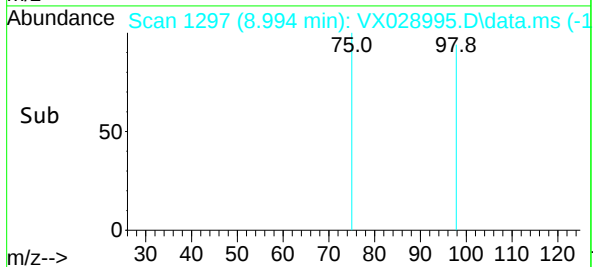
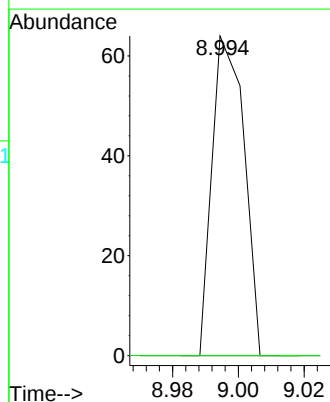
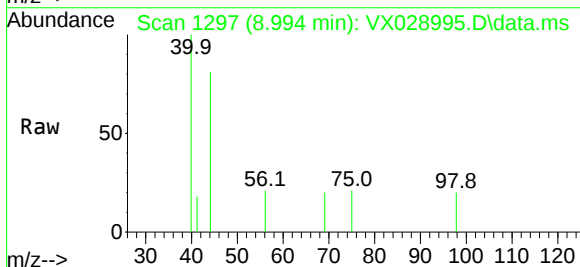




#62
4-Bromofluorobenzene
Concen: 52.678 ug/l
RT: 11.079 min Scan# 1
Delta R.T. -0.006 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-08DL


Tgt Ion: 95 Resp: 292057
Ion Ratio Lower Upper
95 100
174 77.4 0.0 163.0
176 73.6 0.0 155.0

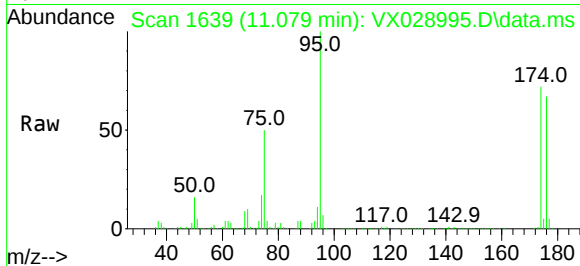

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42

Tgt Ion: 117 Resp: 580508
Ion Ratio Lower Upper
117 100
82 56.4 41.8 62.8
119 32.3 24.8 37.2

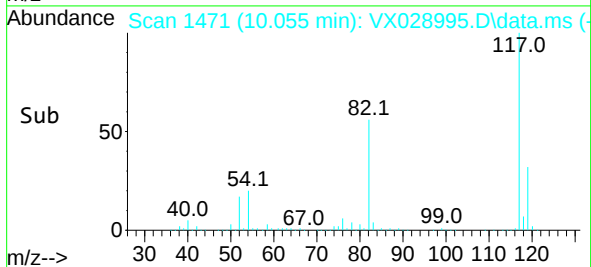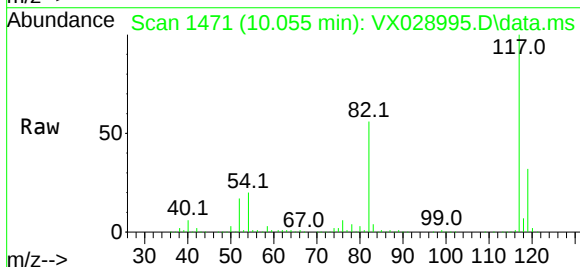

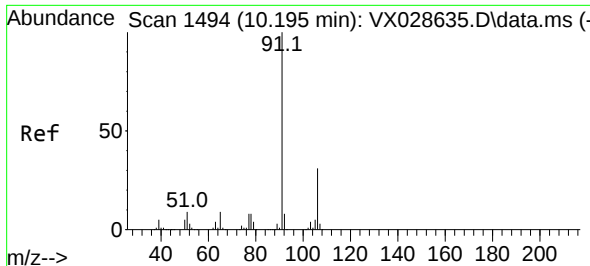

#67

Ethyl Benzene

Concen: 14.378 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX028995.D

Acq: 26 May 2022 13:42

Instrument :

MSVOA_X

ClientSampleId :





MW-08DL

Tgt Ion: 91 Resp: 317370

Ion Ratio Lower Upper

91 100

106 31.1 24.6 36.8

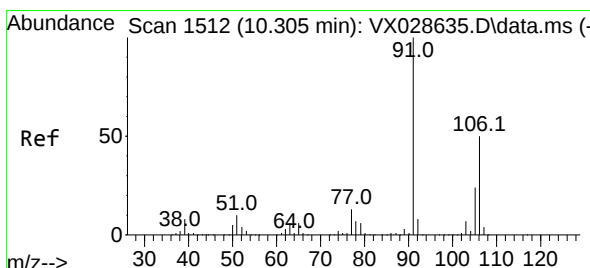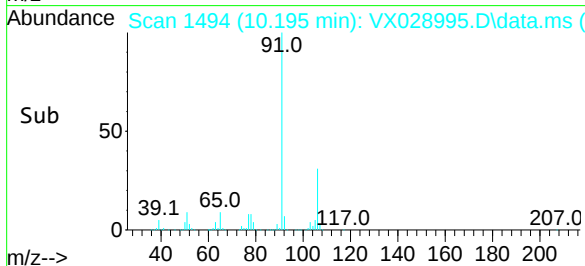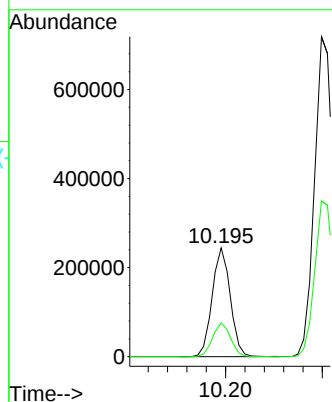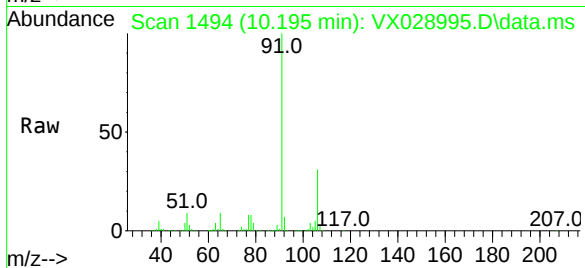

#68

m/p-Xylenes

Concen: 55.845 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. -0.006 min

Lab File: VX028995.D




Acq: 26 May 2022 13:42


Tgt Ion: 106 Resp: 479921

Ion Ratio Lower Upper

106 100

91 203.0 160.4 240.6


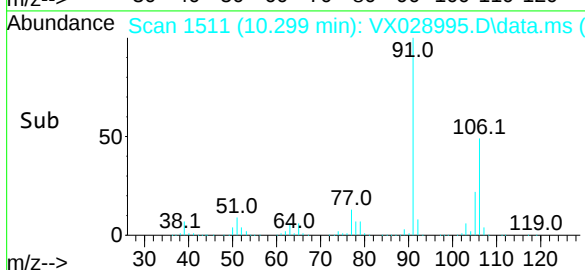

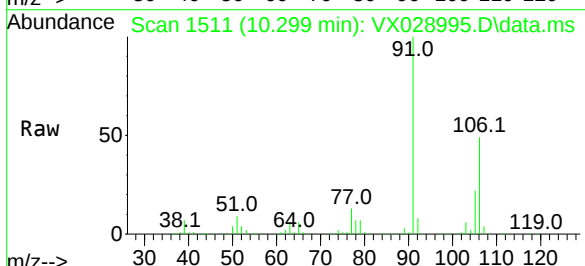




#69
o-Xylene
Concen: 27.968 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.006 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-08DL


Tgt Ion:106 Resp: 236643
Ion Ratio Lower Upper
106 100
91 214.1 106.1 318.1



#70
Styrene
Concen: 0.863 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.018 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42

Tgt Ion:104 Resp: 11855
Ion Ratio Lower Upper
104 100
78 293.2 38.6 57.8#
103 267.4 43.8 65.8#


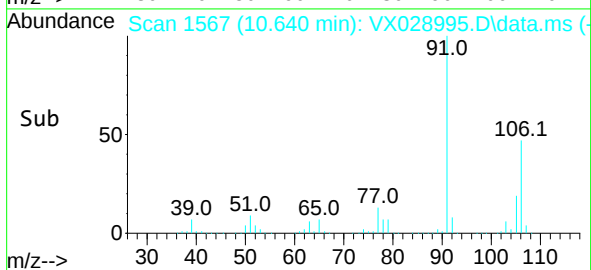

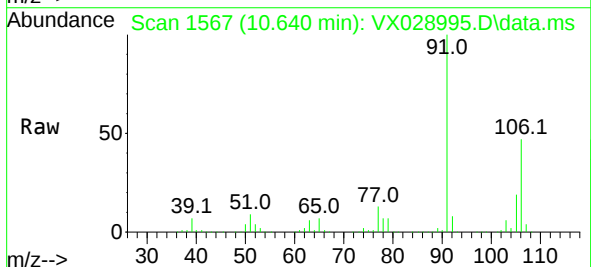




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-08DL


Tgt Ion:152 Resp: 284716
Ion Ratio Lower Upper
152 100
115 61.7 37.5 112.7
150 157.0 0.0 338.2

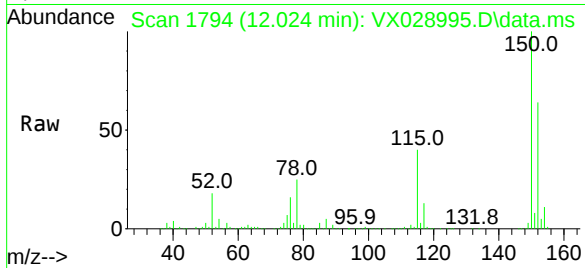

#73
Isopropylbenzene
Concen: 0.735 ug/l
RT: 10.964 min Scan# 1620
Delta R.T. 0.001 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42

Tgt Ion:105 Resp: 15866
Ion Ratio Lower Upper
105 100
120 26.2 13.5 40.5

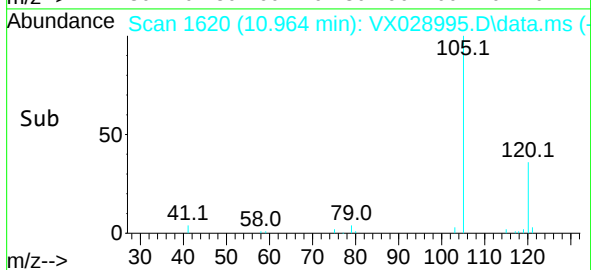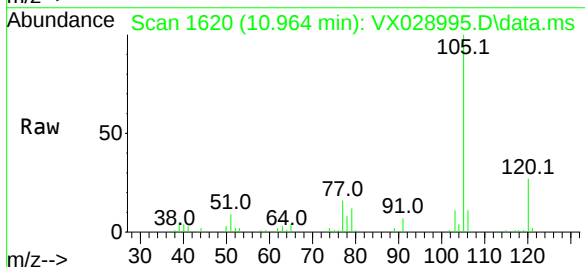



#76

1,2,3-Trichloropropane

Concen: 21.520 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.158 min

Lab File: VX028995.D

Acq: 26 May 2022 13:42

Instrument :

MSVOA_X

ClientSampleId :





MW-08DL

Tgt Ion: 75 Resp: 143491

Ion Ratio Lower Upper

75 100

77 1.2 19.4 58.2#

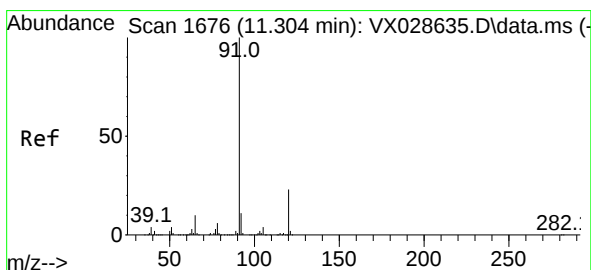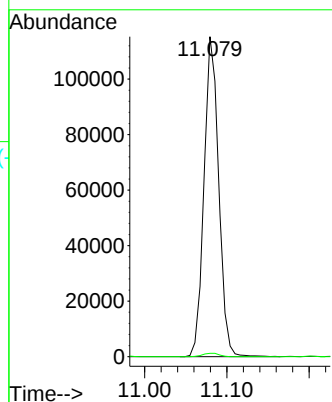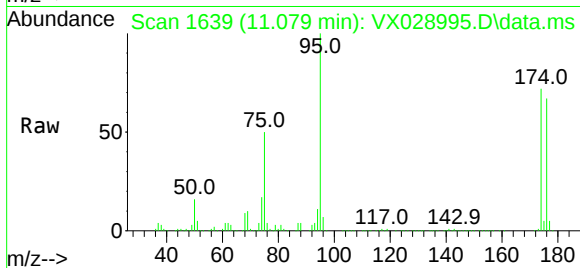

#78

n-propylbenzene

Concen: 1.662 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.001 min

Lab File: VX028995.D




Acq: 26 May 2022 13:42


Tgt Ion: 91 Resp: 41517

Ion Ratio Lower Upper

91 100

120 23.0 11.6 34.8

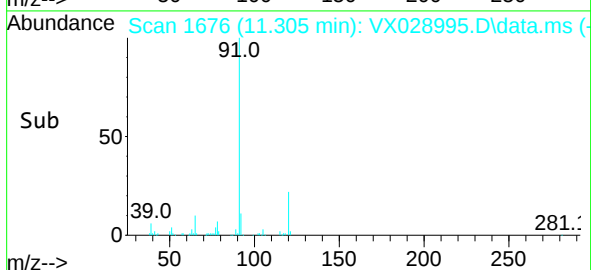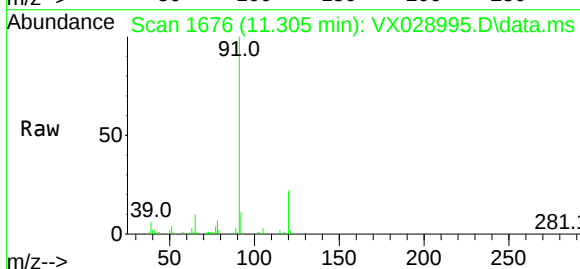



#79

2-Chlorotoluene

Concen: 2.409 ug/l

RT: 11.378 min Scan# 1

Delta R.T. 0.013 min

Lab File: VX028995.D

Acq: 26 May 2022 13:42

Instrument :

MSVOA_X

ClientSampleId :





MW-08DL

Tgt Ion: 91 Resp: 36883

Ion Ratio Lower Upper

91 100

126 0.5 17.3 51.9#

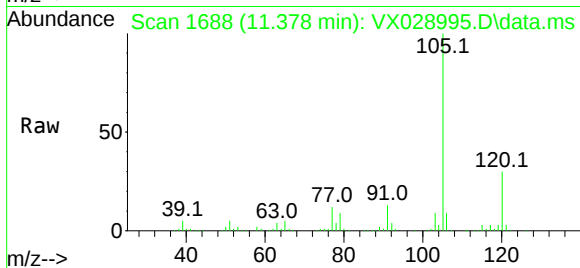

#80

1,3,5-Trimethylbenzene

Concen: 5.300 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX028995.D




Acq: 26 May 2022 13:42


Tgt Ion:105 Resp: 95347

Ion Ratio Lower Upper

105 100

120 48.8 24.3 72.9


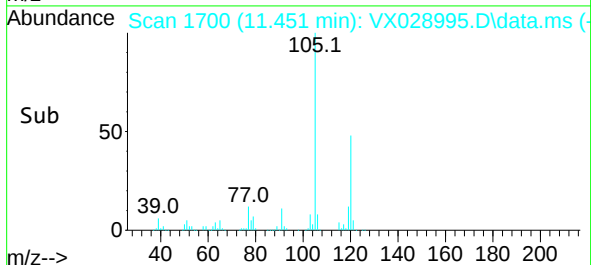
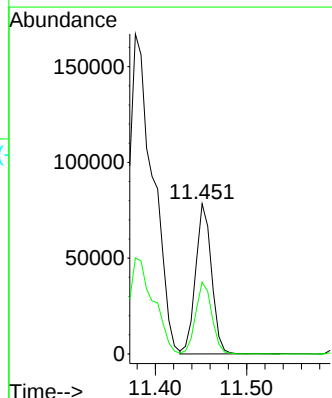
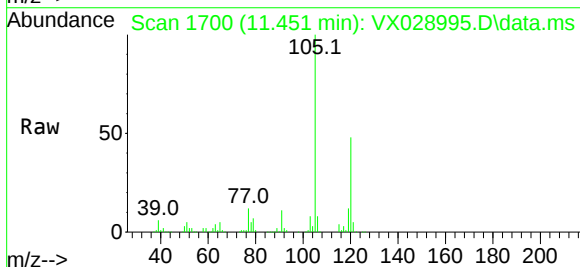




#81
trans-1,4-Dichloro-2-butene
Concen: 63.100 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-08DL


Tgt Ion: 75 Resp: 143491
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#

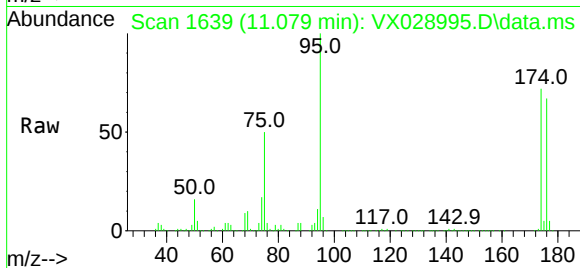

#82
4-Chlorotoluene
Concen: 0.612 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42

Tgt Ion: 91 Resp: 10829
Ion Ratio Lower Upper
91 100
126 1.7 14.9 44.5#


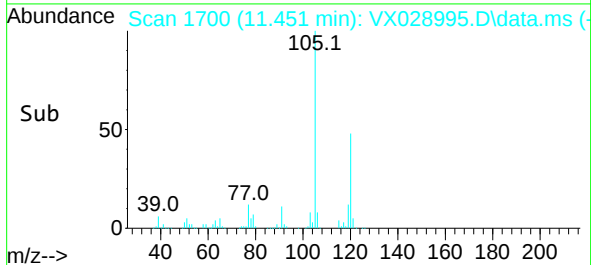

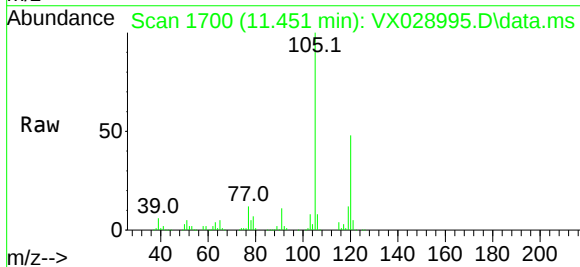




#83
tert-Butylbenzene
Concen: 0.267 ug/l
RT: 11.976 min Scan# 11
Delta R.T. 0.257 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-08DL


Tgt Ion:119 Resp: 4656
Ion Ratio Lower Upper
119 100
91 27.7 26.9 80.6
134 26.1 11.4 34.2

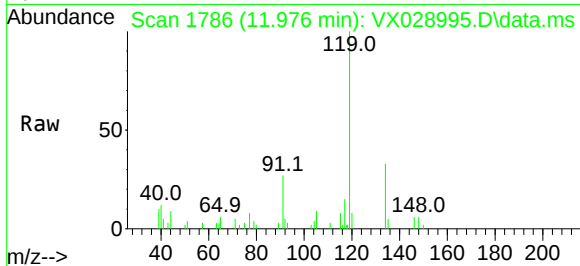

#84
1,2,4-Trimethylbenzene
Concen: 22.027 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.006 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42

Tgt Ion:105 Resp: 397401
Ion Ratio Lower Upper
105 100
120 45.2 22.6 67.8


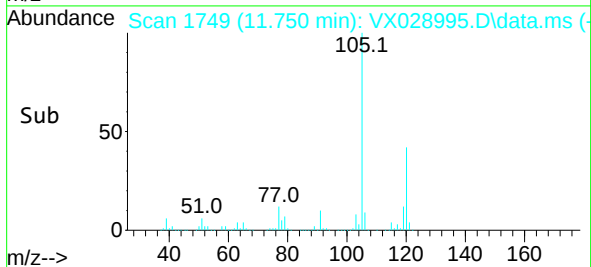

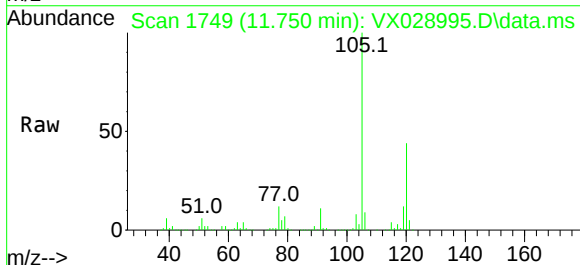




#85
 sec-Butylbenzene
 Concen: 18.495 ug/l
 RT: 11.750 min Scan# 1178
 Delta R.T. -0.140 min
 Lab File: VX028995.D
 Acq: 26 May 2022 13:42




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-08DL


Tgt Ion:105 Resp: 397401
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.2 30.4#

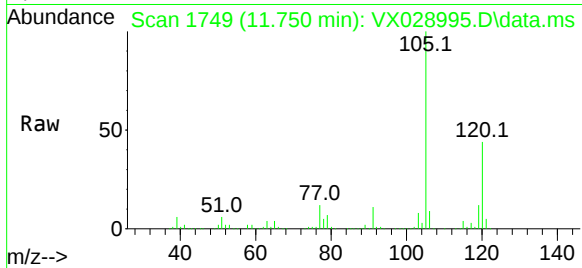

#86
 p-Isopropyltoluene
 Concen: 0.258 ug/l
 RT: 11.976 min Scan# 1786
 Delta R.T. -0.036 min
 Lab File: VX028995.D
 Acq: 26 May 2022 13:42

Tgt Ion:119 Resp: 4656
 Ion Ratio Lower Upper
 119 100
 134 26.1 13.0 39.0
 91 27.7 11.3 33.9

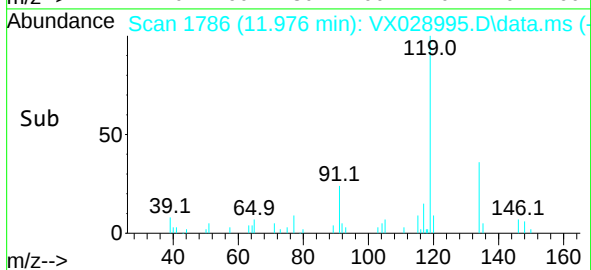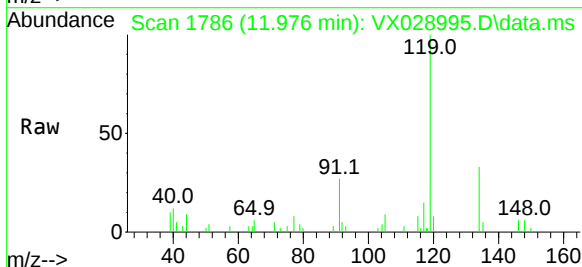



#89

n-Butylbenzene

Concen: 0.460 ug/l

RT: 12.323 min Scan# 1843

Delta R.T. -0.012 min

Lab File: VX028995.D

Acq: 26 May 2022 13:42

Instrument :

MSVOA_X

ClientSampleId :

MW-08DL





Tgt Ion: 91 Resp: 7180

Ion Ratio Lower Upper

91 100

92 26.5 27.8 83.3#

134 125.5 13.3 39.8#

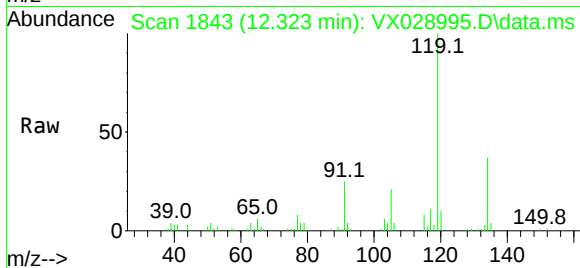

#90

Hexachloroethane

Concen: 0.923 ug/l

RT: 12.616 min Scan# 1891

Delta R.T. 0.074 min

Lab File: VX028995.D




Acq: 26 May 2022 13:42


Tgt Ion: 117 Resp: 2691

Ion Ratio Lower Upper

117 100

201 0.0 39.5 118.5#

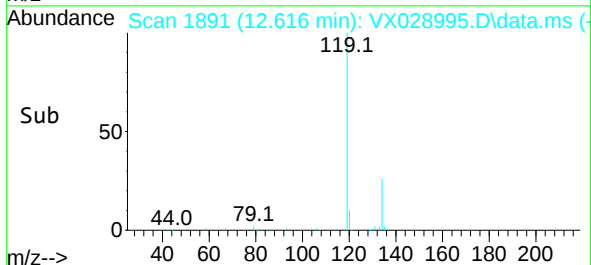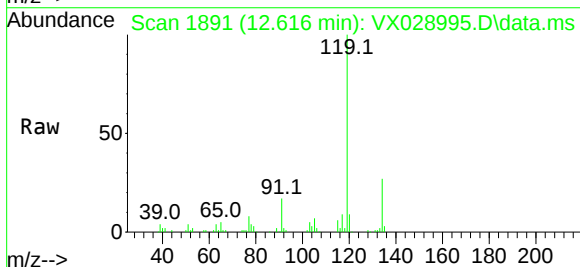

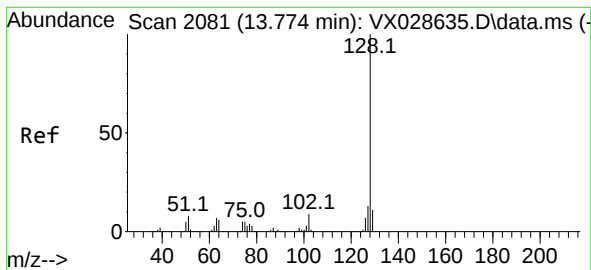

#95
Naphthalene
Concen: 6.360 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. 0.000 min
Lab File: VX028995.D
Acq: 26 May 2022 13:42

Instrument :
MSVOA_X
ClientSampleId :
MW-08DL

Tgt Ion:128 Resp: 128669
Ion Ratio Lower Upper
128 100
127 12.6 10.2 15.4
129 11.0 8.7 13.1

