
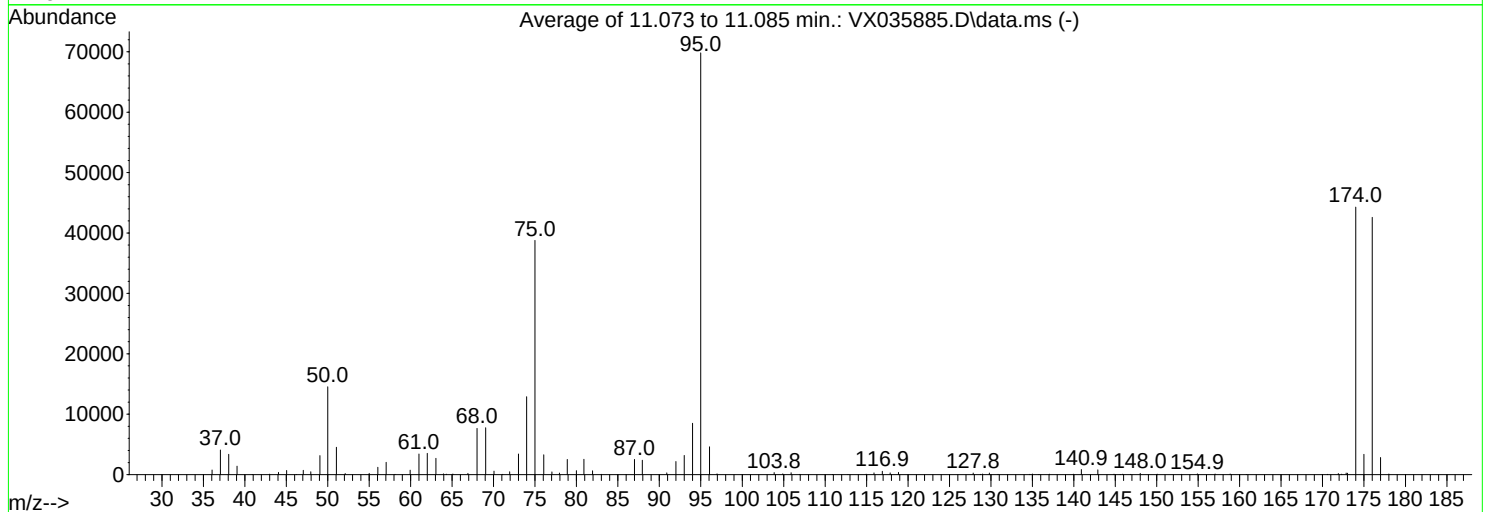


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052623\
Data File : VX035885.D
Acq On : 26 May 2023 15:26
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052623W.M
Title : SW846 8260
Last Update : Mon May 29 07:45:36 2023

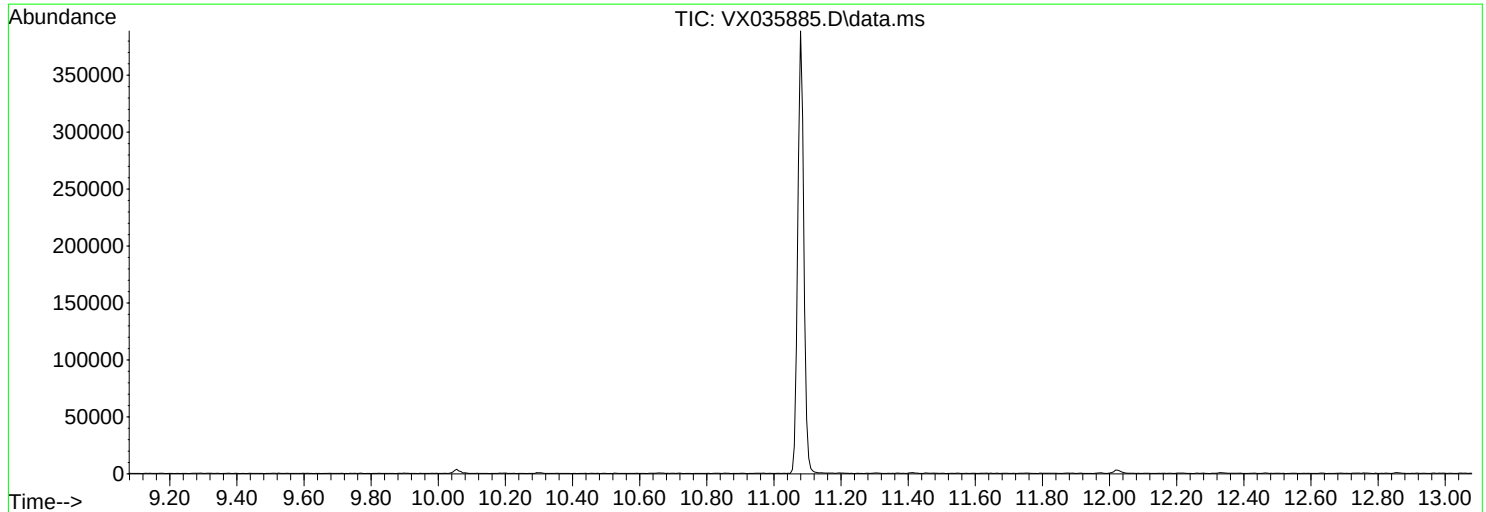

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	14554	PASS
75	95	30	60	55.5	38771	PASS
95	95	100	100	100.0	69824	PASS
96	95	5	9	6.6	4623	PASS
173	174	0.00	2	0.6	268	PASS
174	95	50	100	63.4	44285	PASS
175	174	5	9	7.6	3352	PASS
176	174	95	101	96.2	42592	PASS
177	176	5	9	6.7	2848	PASS