

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
 Data File : VX022198.D
 Acq On : 26 May 2021 15:31
 Operator : JC/MD
 Sample : M2520-03DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-03-2021-05-24DL

Quant Time: May 27 04:06:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 19 14:23:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	61868	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	130341	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	115949	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	49388	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	50299	52.70	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 105.40%			
35) Dibromofluoromethane	5.397	113	40486	48.98	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 97.96%			
50) Toluene-d8	8.653	98	160796	50.50	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 101.00%			
62) 4-Bromofluorobenzene	11.085	95	57303	48.69	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 97.38%			
Target Compounds					Qvalue	
3) Chloromethane	1.294	50	212	0.26	ug/l	92
5) Bromomethane	1.611	94	327	0.65	ug/l #	54
11) Tert butyl alcohol	2.953	59	1222	5.60	ug/l #	73
13) Acrolein	2.239	56	90	0.62	ug/l #	1
16) Acetone	2.386	43	3679	8.85	ug/l #	86
17) Carbon Disulfide	2.508	76	1089	0.59	ug/l #	75
18) Methyl Acetate	2.721	43	394	0.36	ug/l #	47
20) Methylene Chloride	2.794	84	1023	1.11	ug/l #	85
25) 2-Butanone	4.580	43	534	0.79	ug/l #	45
31) Cyclohexane	5.562	56	1843	1.54	ug/l #	1
36) 1,1-Dichloropropene	5.556	75	6287	5.22	ug/l #	48
38) Carbon Tetrachloride	5.562	117	7105	6.03	ug/l #	16
40) Benzene	6.050	78	32012	8.63	ug/l	95
52) Toluene	8.720	92	40848	17.39	ug/l	97
53) t-1,3-Dichloropropene	8.720	75	471	0.32	ug/l #	1
55) 1,1,2-Trichloroethane	9.019	97	258	0.27	ug/l #	15
67) Ethyl Benzene	10.201	91	202885	45.69	ug/l	99
68) m/p-Xylenes	10.305	106	40237	23.98	ug/l	97
69) o-Xylene	10.646	106	29887	18.31	ug/l	98
70) Styrene	10.659	104	4917	1.84	ug/l #	1
73) Isopropylbenzene	10.963	105	14097	3.37	ug/l	96
76) 1,2,3-Trichloropropane	11.085	75	29470	24.19	ug/l #	39
78) n-propylbenzene	11.305	91	6656	1.36	ug/l	100
79) 2-Chlorotoluene	11.402	91	6561	2.21	ug/l #	45
80) 1,3,5-Trimethylbenzene	11.457	105	14000	4.04	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.085	75	29470	57.31	ug/l #	12
82) 4-Chlorotoluene	11.451	91	1603	0.47	ug/l #	45
83) tert-Butylbenzene	11.975	119	3615	1.09	ug/l	73
84) 1,2,4-Trimethylbenzene	11.756	105	54507	15.63	ug/l	99
85) sec-Butylbenzene	11.756	105	54507	12.91	ug/l #	57
86) p-Isopropyltoluene	11.975	119	3615	1.01	ug/l	92
89) n-Butylbenzene	12.329	91	2785	0.84	ug/l #	9
90) Hexachloroethane	12.414	117	15566	26.41	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	12.975	75	210	0.71	ug/l #	1
95) Naphthalene	13.780	128	2234951	578.61	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
Data File : VX022198.D
Acq On : 26 May 2021 15:31
Operator : JC/MD
Sample : M2520-03DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL

Quant Time: May 27 04:06:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260
QLast Update : Wed May 19 14:23:10 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
Data File : VX022198.D
Acq On : 26 May 2021 15:31
Operator : JC/MD
Sample : M2520-03DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL

Quant Time: May 27 04:06:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260
QLast Update : Wed May 19 14:23:10 2021
Response via : Initial Calibration




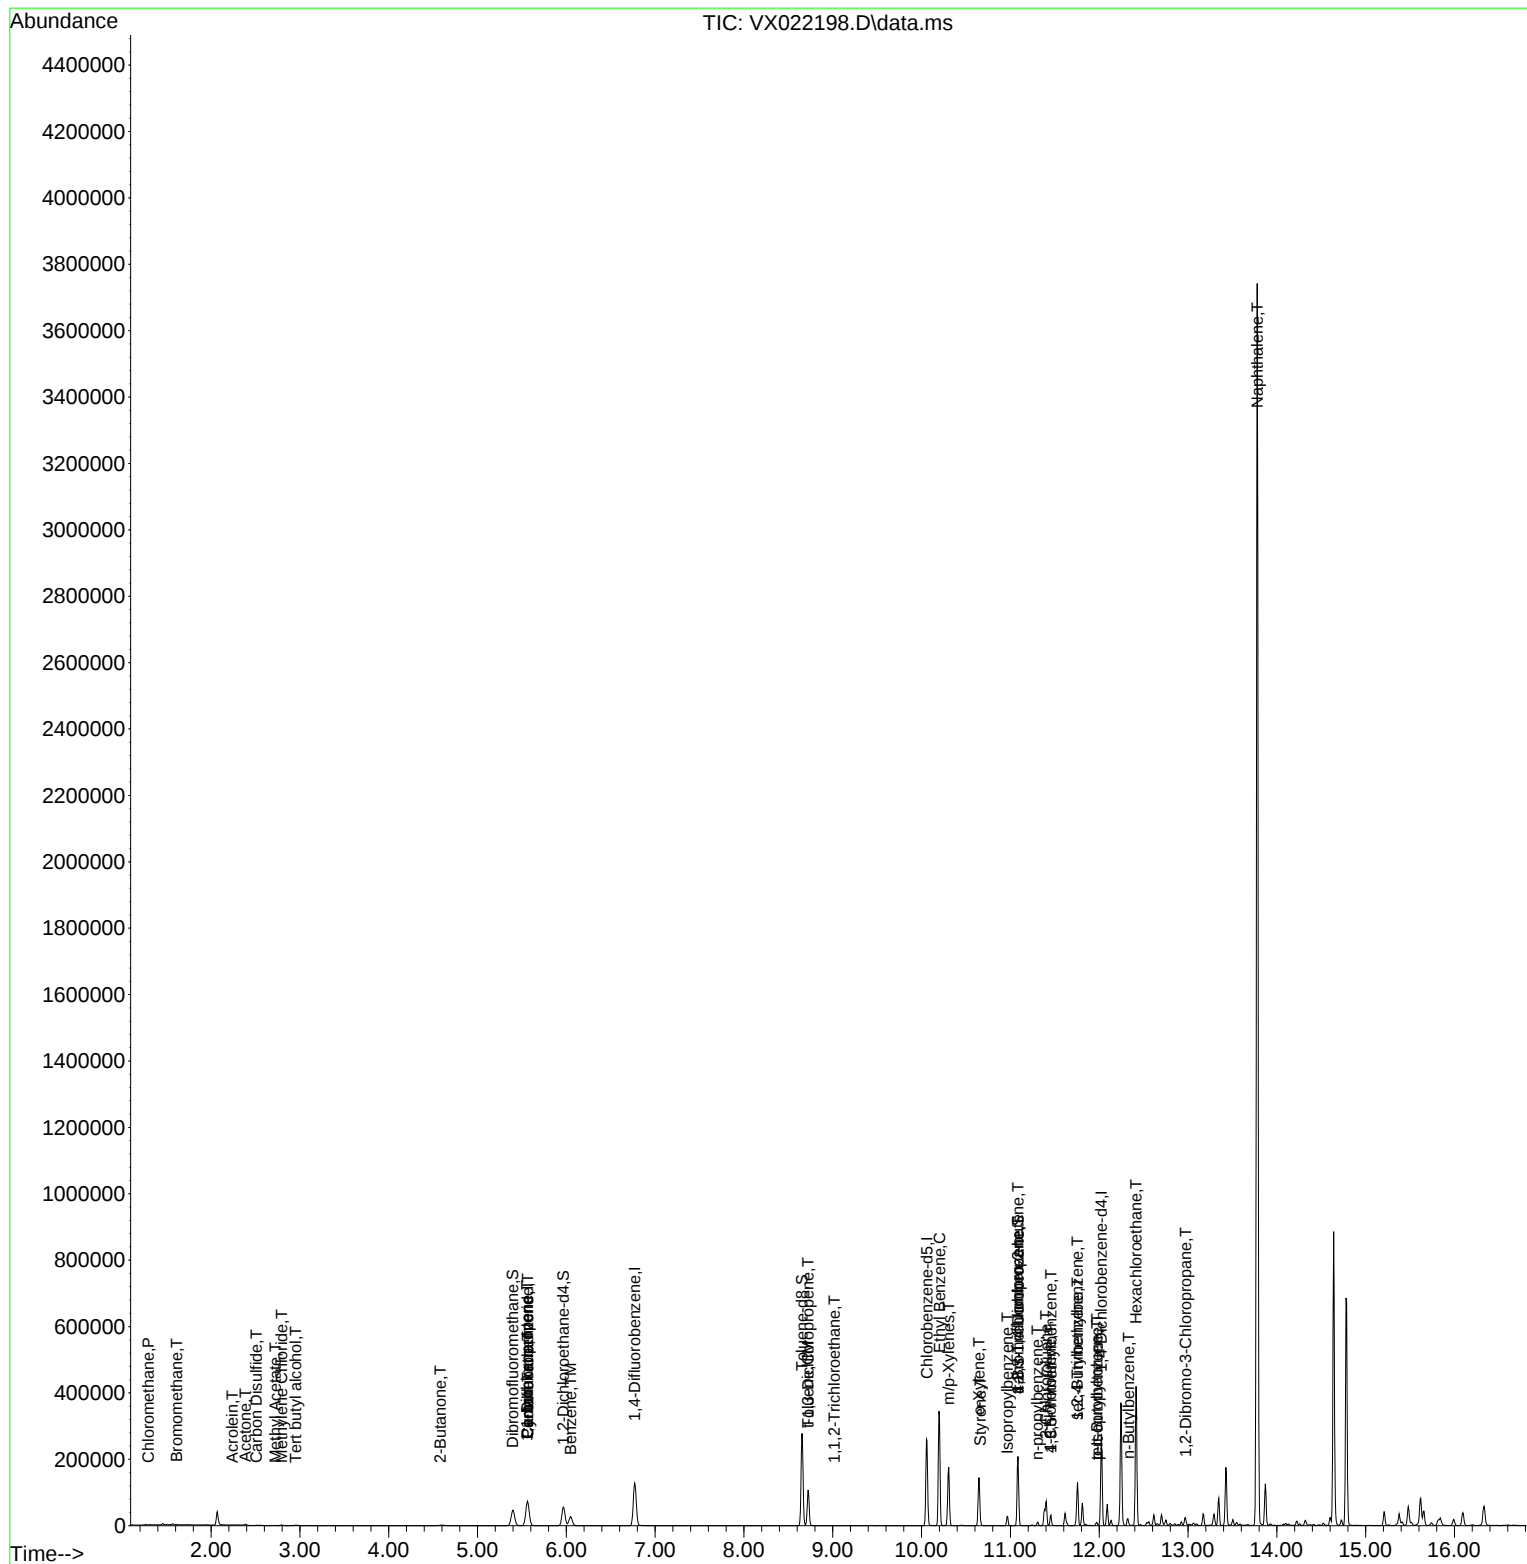




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.000 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion:168 Resp: 61868
Ion Ratio Lower Upper
168 100
99 64.3 45.8 68.6

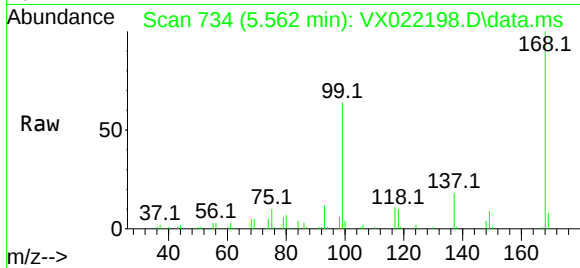

#3
Chloromethane
Concen: 0.26 ug/l
RT: 1.294 min Scan# 34
Delta R.T. -0.001 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion: 50 Resp: 212
Ion Ratio Lower Upper
50 100
52 37.5 26.4 39.6




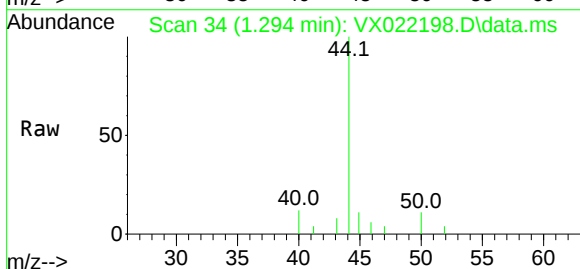


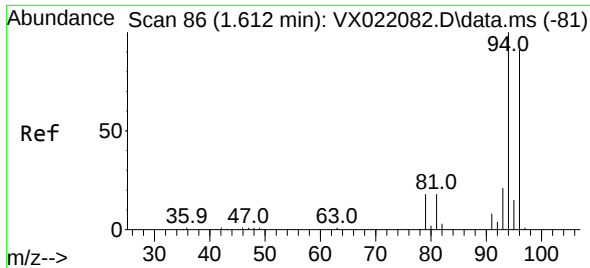

#5
Bromomethane
Concen: 0.65 ug/l
RT: 1.611 min Scan# 86
Delta R.T. -0.001 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion: 94 Resp: 327
Ion Ratio Lower Upper
94 100
96 51.0 76.4 114.6#

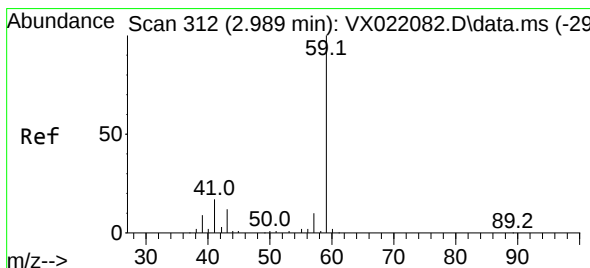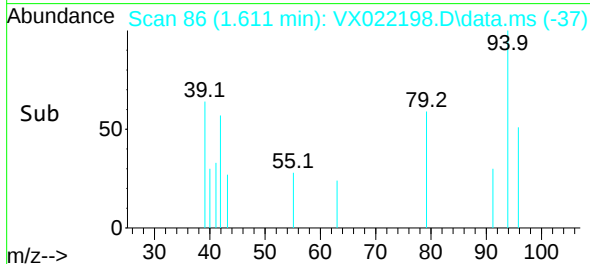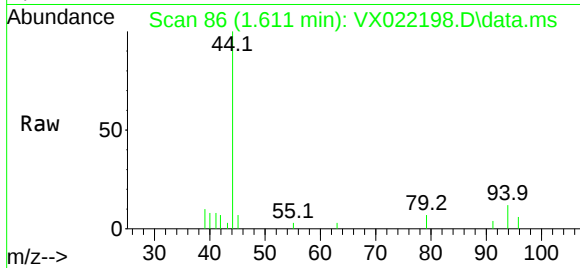

#11
Tert butyl alcohol
Concen: 5.60 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.036 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion: 59 Resp: 1222
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#


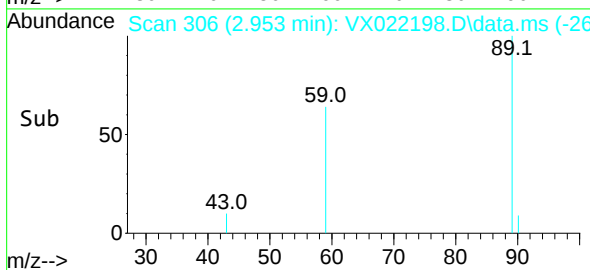

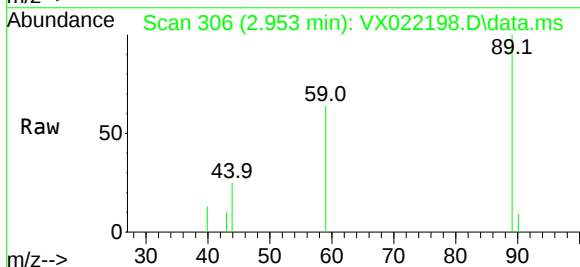


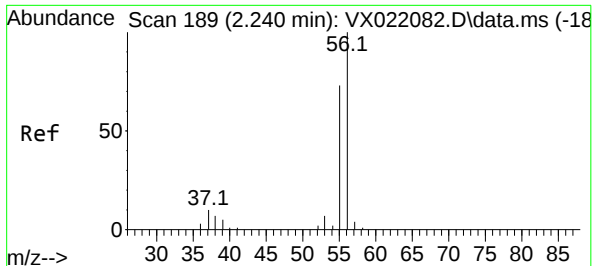

#13
Acrolein
Concen: 0.62 ug/l
RT: 2.239 min Scan# 189
Delta R.T. -0.001 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion: 56 Resp: 90
Ion Ratio Lower Upper
56 100
55 193.3 56.4 84.6#

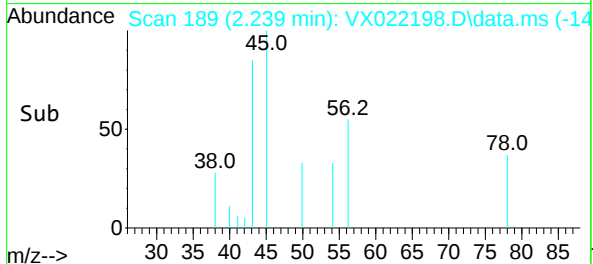

#16
Acetone
Concen: 8.85 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion: 43 Resp: 3679
Ion Ratio Lower Upper
43 100
58 26.8 27.8 41.8#




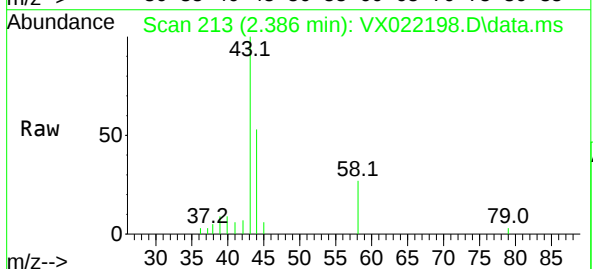


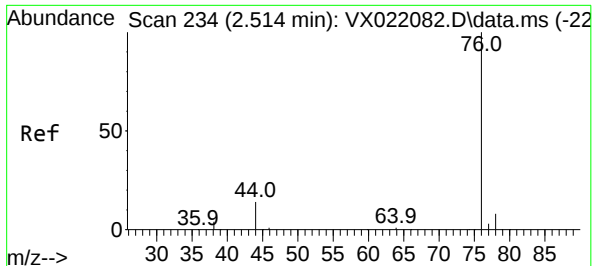

#17
Carbon Disulfide
Concen: 0.59 ug/l
RT: 2.508 min Scan# 233
Delta R.T. -0.006 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion: 76 Resp: 1089
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

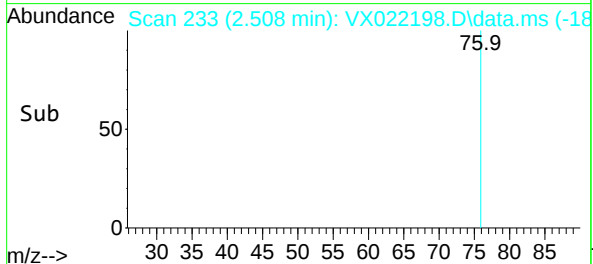

#18
Methyl Acetate
Concen: 0.36 ug/l
RT: 2.721 min Scan# 268
Delta R.T. 0.012 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion: 43 Resp: 394
Ion Ratio Lower Upper
43 100
74 0.0 21.9 32.9#


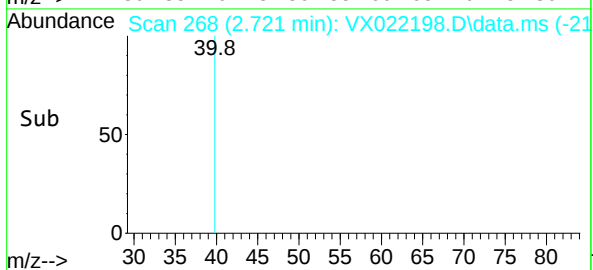

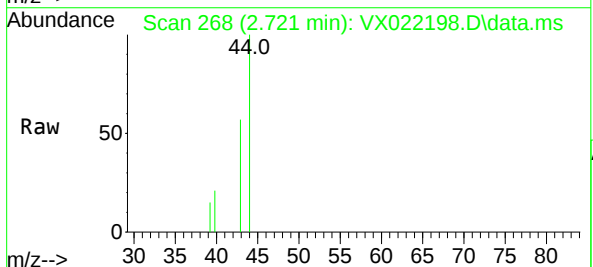




#20
Methylene Chloride
Concen: 1.11 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion:	84	Resp:	1023
Ion	Ratio	Lower	Upper
84	100		
49	96.1	88.6	132.8
51	27.2	27.0	40.6
86	49.0	50.3	75.5#

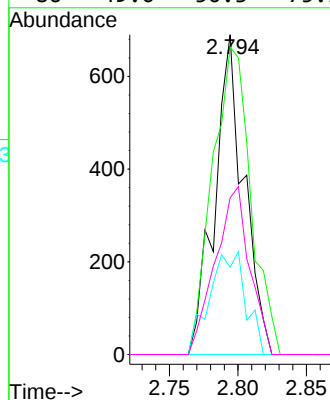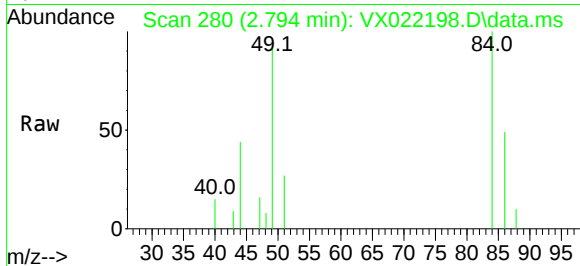

#25
2-Butanone
Concen: 0.79 ug/l
RT: 4.580 min Scan# 573
Delta R.T. 0.012 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion:	43	Resp:	534
Ion	Ratio	Lower	Upper
43	100		
72	0.0	23.7	35.5#


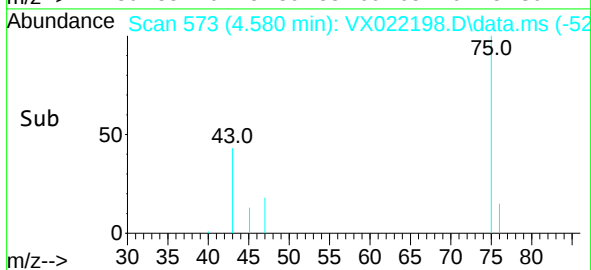
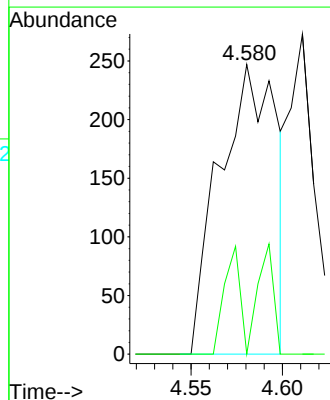
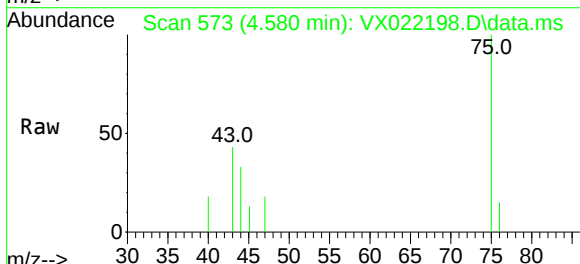


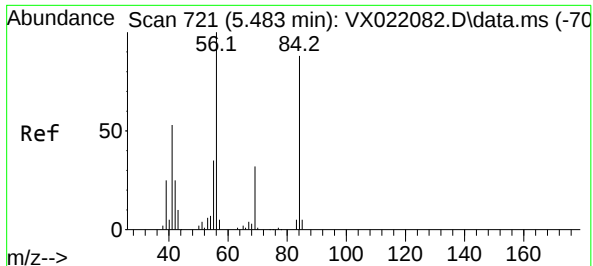

#31
Cyclohexane
Concen: 1.54 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.079 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion: 56 Resp: 1843
Ion Ratio Lower Upper
56 100
69 173.4 25.3 37.9#
84 142.5 71.4 107.0#

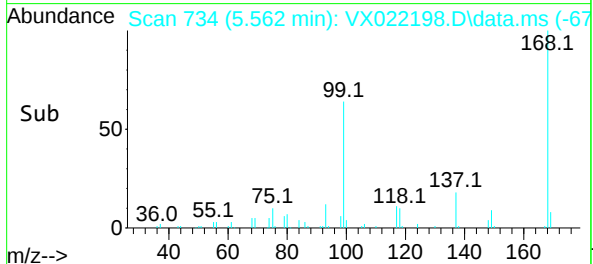

#33
1,2-Dichloroethane-d4
Concen: 52.70 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion: 65 Resp: 50299
Ion Ratio Lower Upper
65 100
67 53.3 0.0 105.4




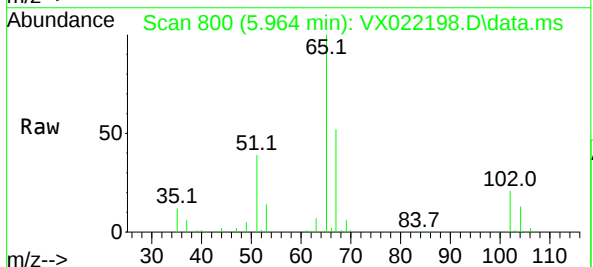


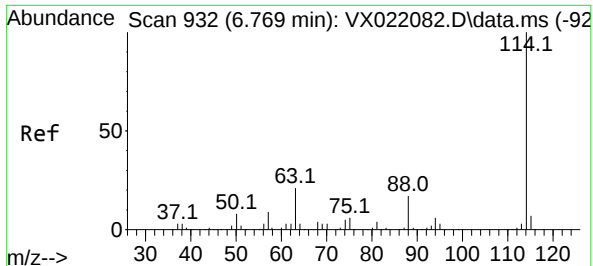

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion:114 Resp: 130341
Ion Ratio Lower Upper
114 100
63 21.9 0.0 40.8
88 16.4 0.0 32.8

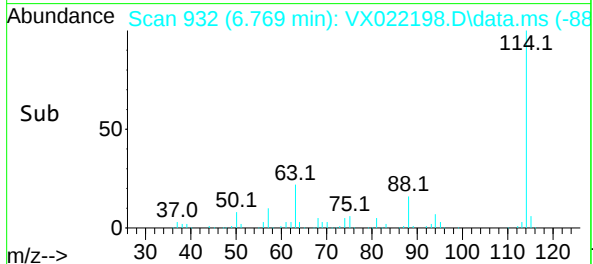

#35
Dibromofluoromethane
Concen: 48.98 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.006 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion:113 Resp: 40486
Ion Ratio Lower Upper
113 100
111 101.8 81.9 122.9
192 15.8 16.7 25.1#


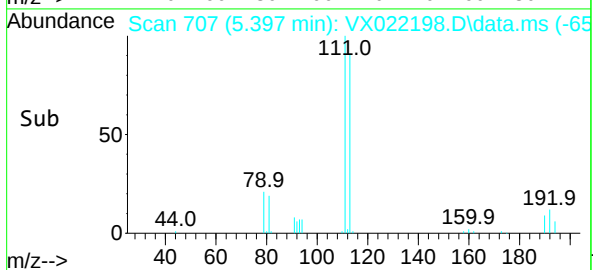

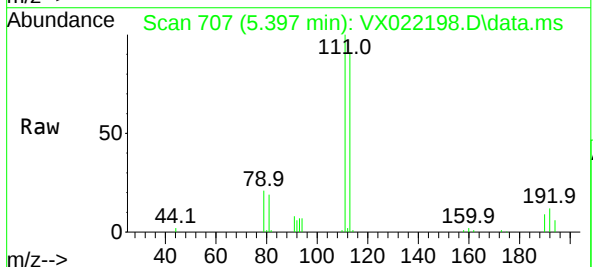




#36
1,1-Dichloropropene
Concen: 5.22 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.146 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion: 75 Resp: 6287
Ion Ratio Lower Upper
75 100
110 8.7 18.1 54.4#
77 0.0 25.3 37.9#

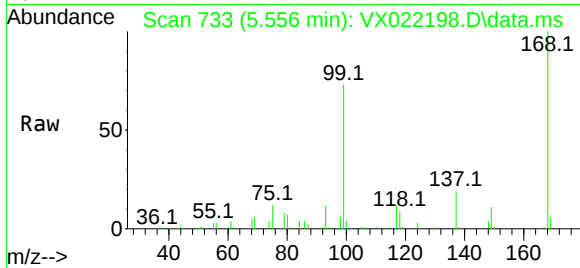

#38
Carbon Tetrachloride
Concen: 6.03 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.128 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion: 117 Resp: 7105
Ion Ratio Lower Upper
117 100
119 4.6 76.2 114.2#
121 0.0 24.8 37.2#


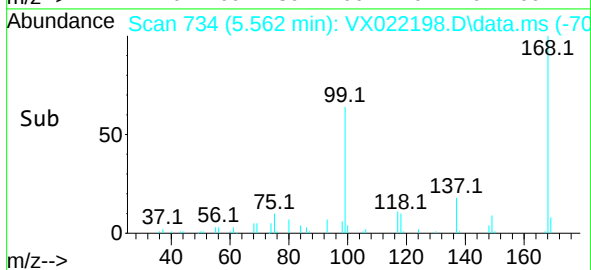

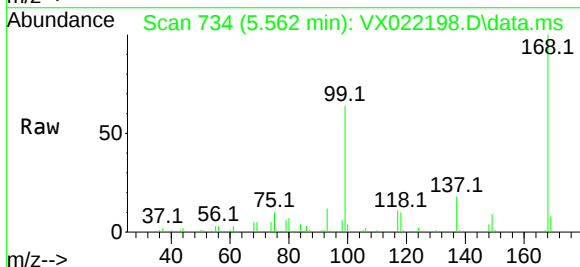


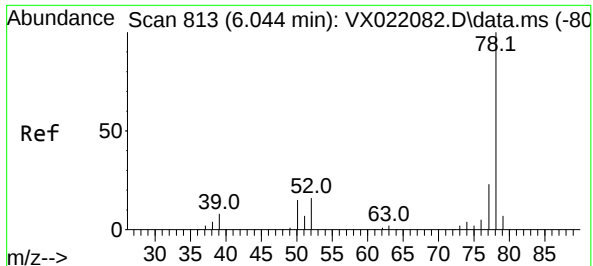

#40
Benzene
Concen: 8.63 ug/l
RT: 6.050 min Scan# 814
Delta R.T. 0.006 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion: 78 Resp: 32012
Ion Ratio Lower Upper
78 100
77 21.2 18.9 28.3

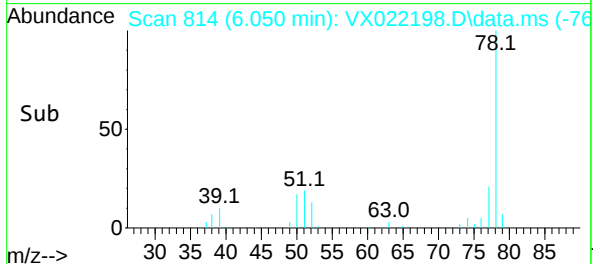

#50
Toluene-d8
Concen: 50.50 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion: 98 Resp: 160796
Ion Ratio Lower Upper
98 100
100 66.0 51.9 77.9


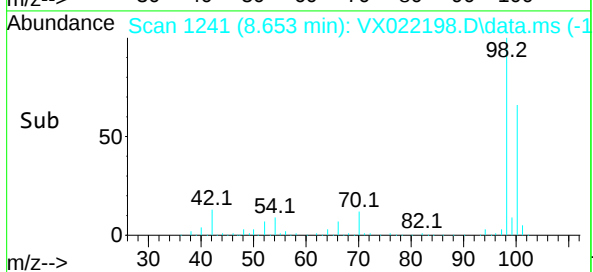

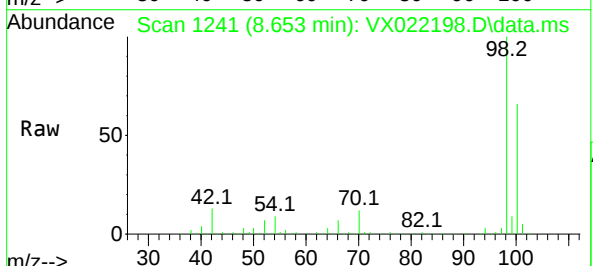




#52
Toluene
Concen: 17.39 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.006 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion: 92 Resp: 40848
Ion Ratio Lower Upper
92 100
91 167.8 137.1 205.7



#53
t-1,3-Dichloropropene
Concen: 0.32 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.262 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion: 75 Resp: 471
Ion Ratio Lower Upper
75 100
77 123.4 24.9 37.3#




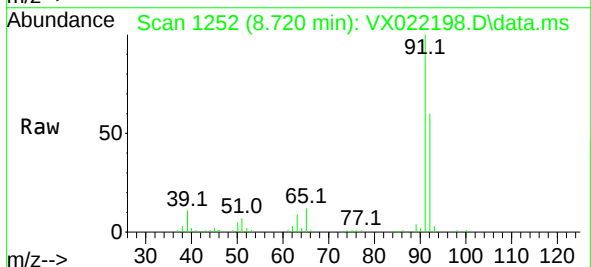




#55
1,1,2-Trichloroethane
Concen: 0.27 ug/l
RT: 9.019 min Scan# 1301
Delta R.T. -0.140 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion:	97	Resp:	258
Ion	Ratio	Lower	Upper
97	100		
83	0.0	69.3	103.9#
85	0.0	44.3	66.5#
99	0.0	50.3	75.5#



#62
4-Bromofluorobenzene
Concen: 48.69 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion:	95	Resp:	57303
Ion	Ratio	Lower	Upper
95	100		
174	64.4	0.0	154.6
176	61.5	0.0	155.8


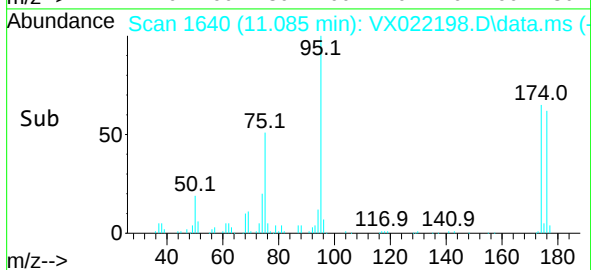

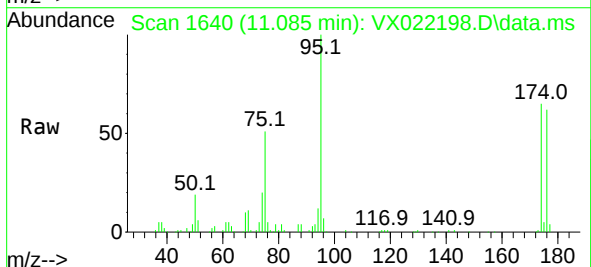




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. 0.000 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion:117 Resp: 115949
Ion Ratio Lower Upper
117 100
82 57.0 47.4 71.2
119 32.9 26.6 39.8

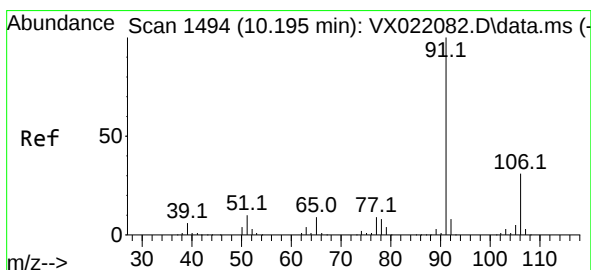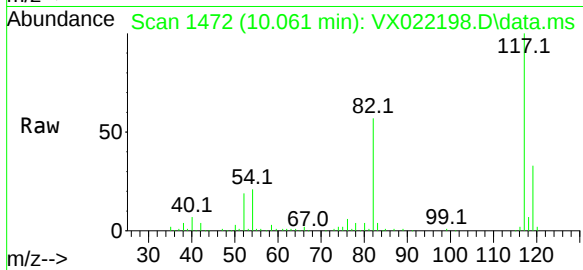

#67
Ethyl Benzene
Concen: 45.69 ug/l
RT: 10.201 min Scan# 1495
Delta R.T. 0.006 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion: 91 Resp: 202885
Ion Ratio Lower Upper
91 100
106 31.3 24.6 37.0




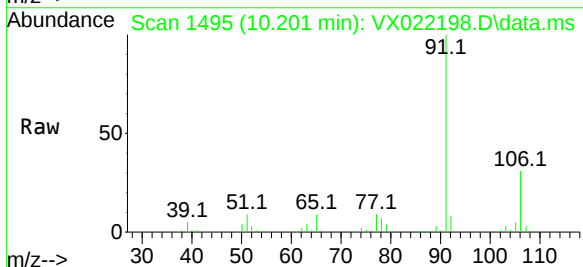




#68
m/p-Xylenes
Concen: 23.98 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion:106 Resp: 40237
Ion Ratio Lower Upper
106 100
91 208.1 162.8 244.2



#69
o-Xylene
Concen: 18.31 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.001 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion:106 Resp: 29887
Ion Ratio Lower Upper
106 100
91 213.3 108.1 324.2


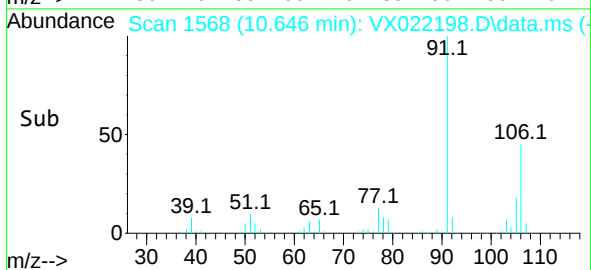

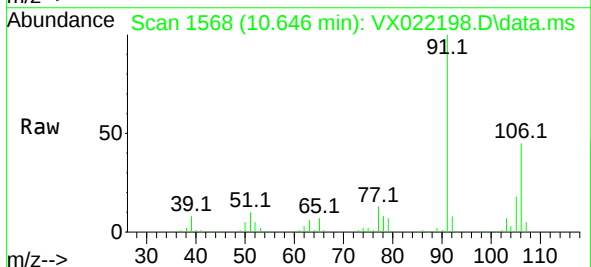




#70
Styrene
Concen: 1.84 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. -0.000 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion:104	Resp:	4917
Ion Ratio	Lower	Upper
104	100	
78	123.0	40.0 60.0#
103	122.2	43.4 65.0#

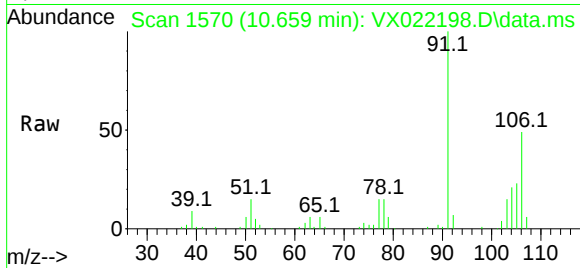

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion:152	Resp:	49388
Ion Ratio	Lower	Upper
152	100	
115	65.2	41.1 123.3
150	159.2	0.0 349.0

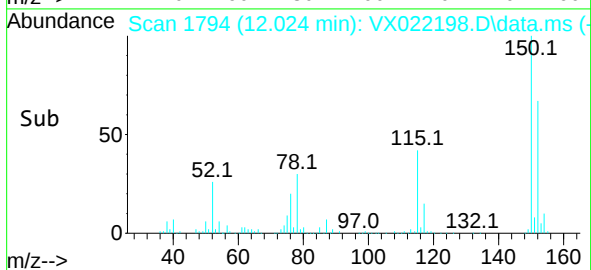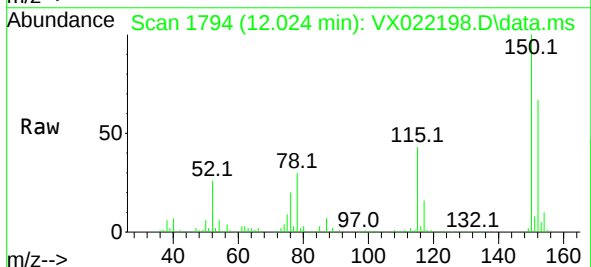



#73

Isopropylbenzene

Concen: 3.37 ug/l

RT: 10.963 min Scan# 1620

Delta R.T. -0.001 min





Lab File: VX022198.D

Acq: 26 May 2021 15:31

Tgt Ion: 105 Resp: 14097

Ion Ratio Lower Upper

105 100
120 28.3 13.2 39.6

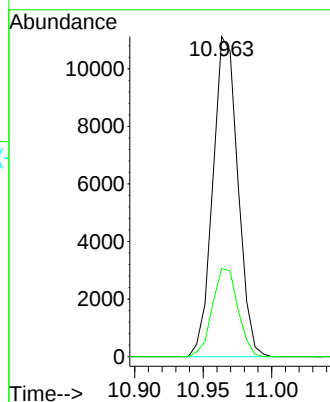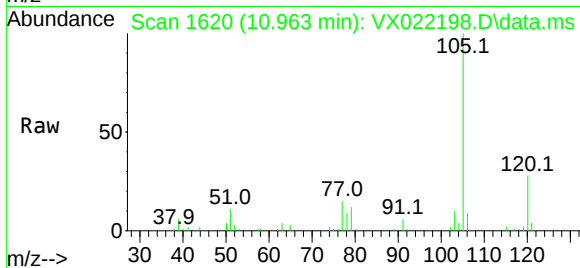

#76

1,2,3-Trichloropropane

Concen: 24.19 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. -0.159 min




Lab File: VX022198.D


Acq: 26 May 2021 15:31

Tgt Ion: 75 Resp: 29470

Ion Ratio Lower Upper

75 100
77 1.1 19.1 57.5#

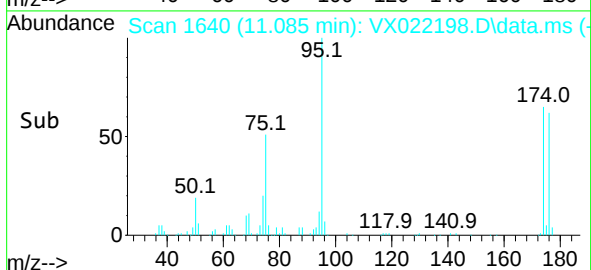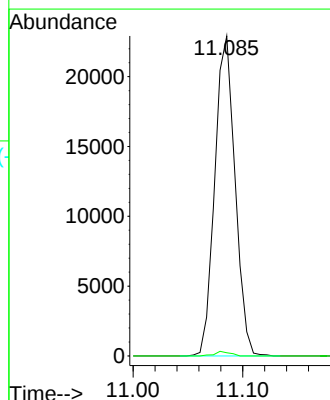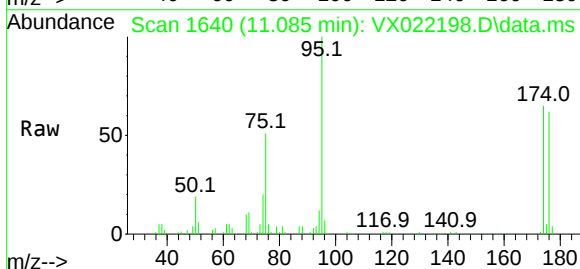

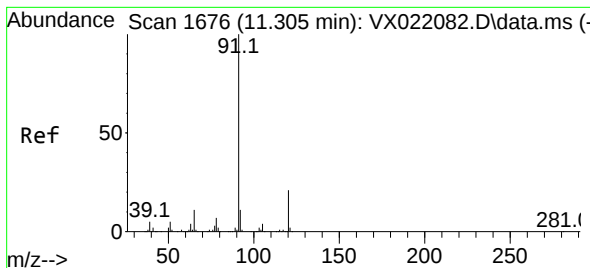

#78

n-propylbenzene

Concen: 1.36 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.000 min

Lab File: VX022198.D





Acq: 26 May 2021 15:31

Tgt Ion: 91 Resp: 6656

Ion Ratio Lower Upper

91 100

120 23.0 11.5 34.5

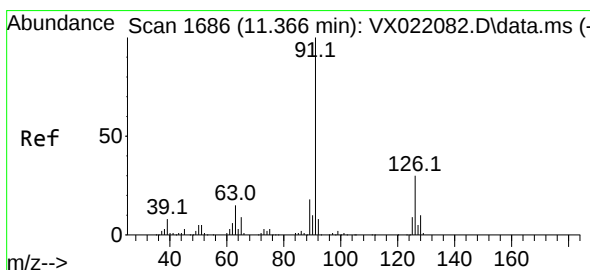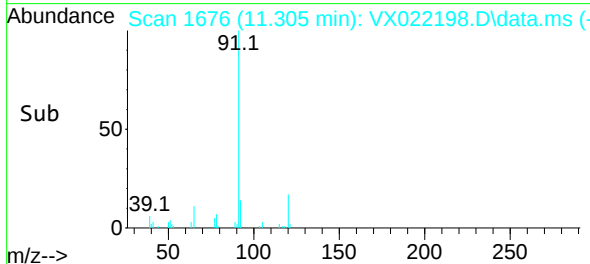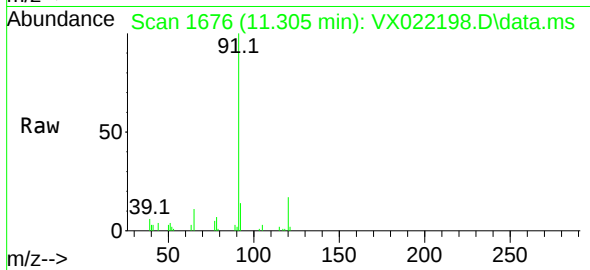

#79

2-Chlorotoluene

Concen: 2.21 ug/l

RT: 11.402 min Scan# 1692

Delta R.T. 0.036 min

Lab File: VX022198.D




Acq: 26 May 2021 15:31


Tgt Ion: 91 Resp: 6561

Ion Ratio Lower Upper

91 100

126 2.0 16.6 49.8#


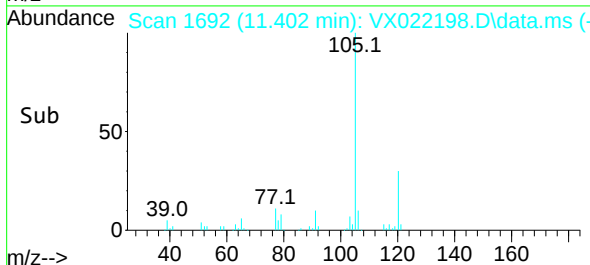

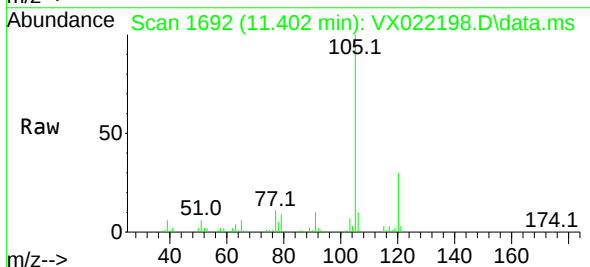




#80
1,3,5-Trimethylbenzene
Concen: 4.04 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion:105 Resp: 14000
Ion Ratio Lower Upper
105 100
120 46.4 23.8 71.5

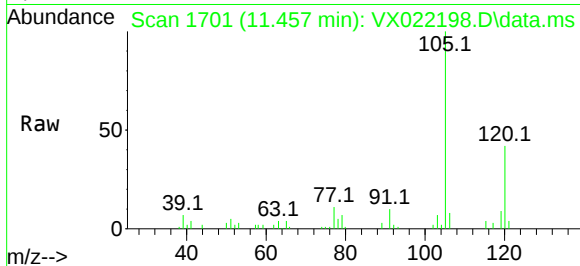

#81
trans-1,4-Dichloro-2-butene
Concen: 57.31 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.060 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion: 75 Resp: 29470
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#


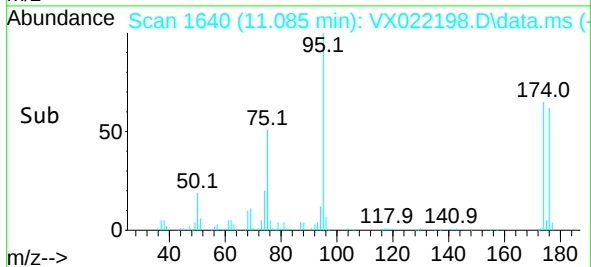

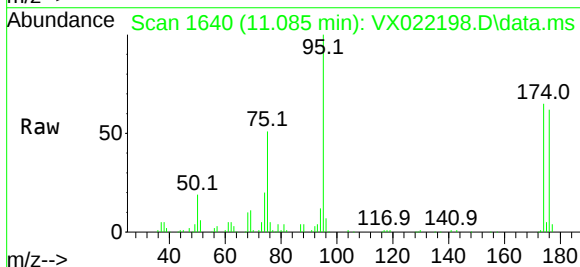




#82
4-Chlorotoluene
Concen: 0.47 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion: 91 Resp: 1603
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#

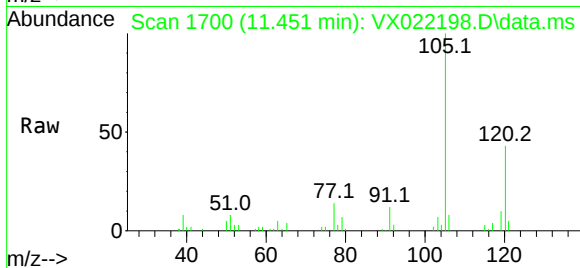

#83
tert-Butylbenzene
Concen: 1.09 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. 0.255 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion: 119 Resp: 3615
Ion Ratio Lower Upper
119 100
91 30.8 27.9 83.7
134 26.8 11.3 33.9


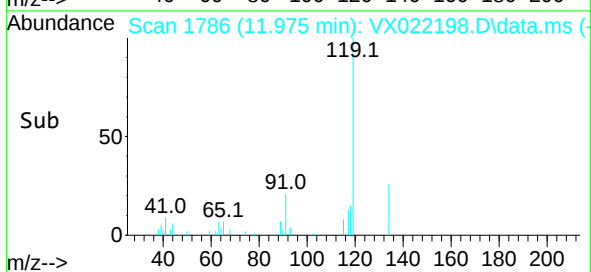

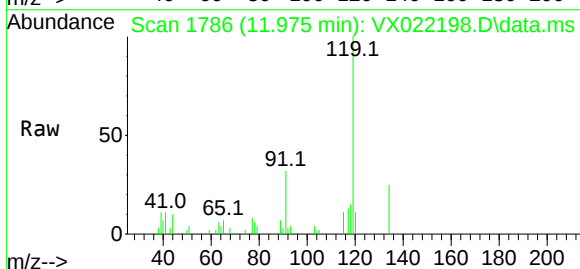




#84
1,2,4-Trimethylbenzene
Concen: 15.63 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion:105 Resp: 54507
Ion Ratio Lower Upper
105 100
120 44.5 22.4 67.3

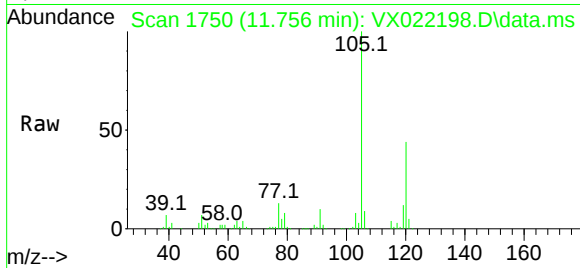

#85
sec-Butylbenzene
Concen: 12.91 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.140 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion:105 Resp: 54507
Ion Ratio Lower Upper
105 100
134 0.0 10.0 29.8#


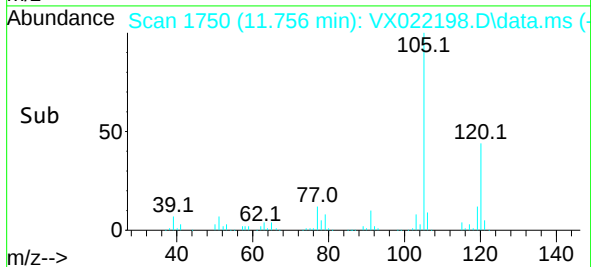

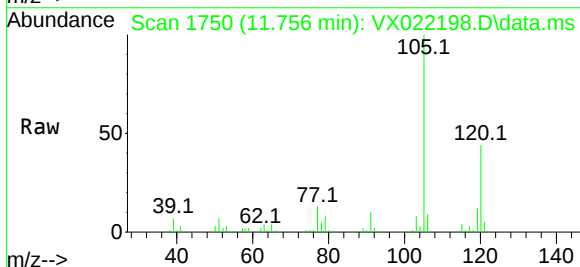




#86
p-Isopropyltoluene
Concen: 1.01 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. -0.037 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion:119 Resp: 3615
Ion Ratio Lower Upper
119 100
134 26.8 12.9 38.7
91 30.8 11.7 35.0

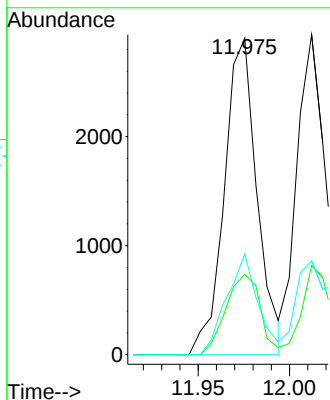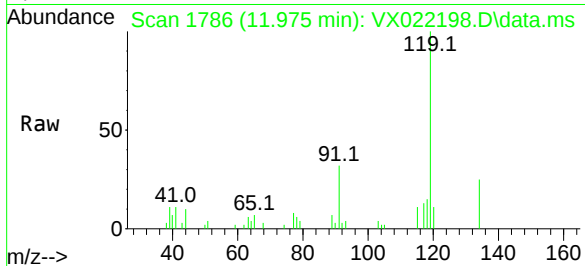

#89
n-Butylbenzene
Concen: 0.84 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. -0.006 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion: 91 Resp: 2785
Ion Ratio Lower Upper
91 100
92 23.3 27.4 82.0#
134 124.1 13.2 39.5#


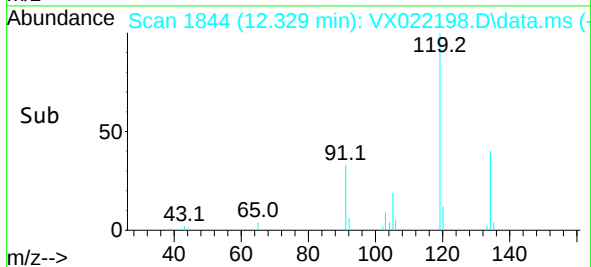
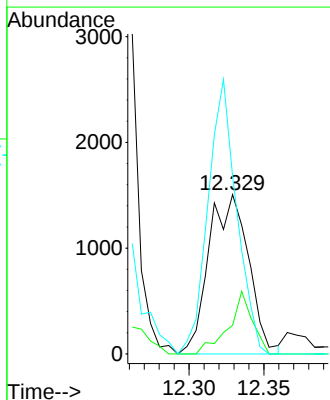
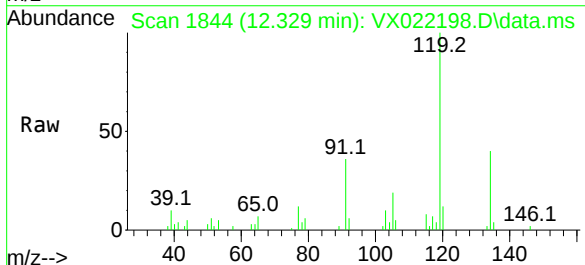




#90
Hexachloroethane
Concen: 26.41 ug/l
RT: 12.414 min Scan# 1858
Delta R.T. -0.129 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31




Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL


Tgt Ion:117 Resp: 15566
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#

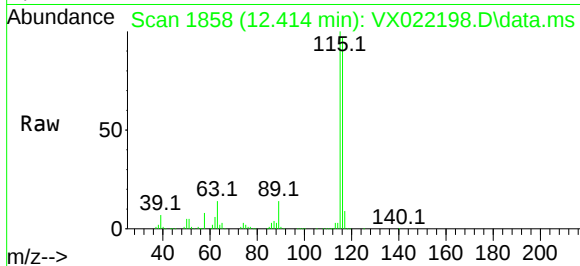

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.71 ug/l
RT: 12.975 min Scan# 1950
Delta R.T. 0.030 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Tgt Ion: 75 Resp: 210
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#

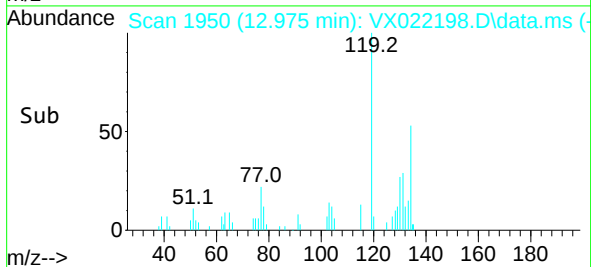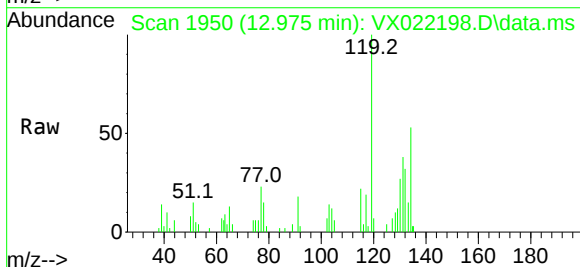

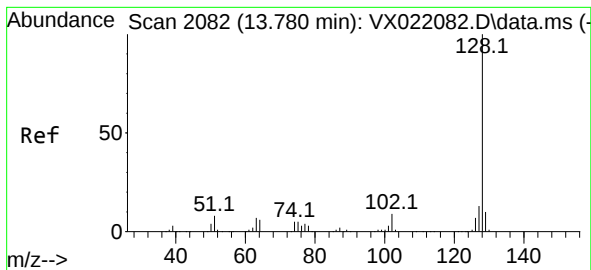

#95
Naphthalene
Concen: 578.61 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX022198.D
Acq: 26 May 2021 15:31

Instrument :
MSVOA_X
ClientSampleId :
WC-03-2021-05-24DL

Tgt Ion:128 Resp: 2234951
Ion Ratio Lower Upper
128 100
127 13.0 10.3 15.5
129 11.2 8.8 13.2

