

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
 Data File : VX022201.D
 Acq On : 26 May 2021 16:42
 Operator : JC/MD
 Sample : M2526-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MH-117T-20210525

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M

Title : SW846 8260

Signal : TIC: VX022201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.550	234	240	248	rVB	5679	10801	2.27%	0.434%
2	4.501	549	560	567	rBV4	2272	6036	1.27%	0.242%
3	5.397	695	707	720	rBV2	51355	146801	30.80%	5.894%
4	5.556	723	733	745	rBV2	78642	221456	46.46%	8.892%
5	5.964	790	800	813	rBV2	61859	163084	34.21%	6.548%
6	6.769	921	932	943	rBV3	141138	339081	71.14%	13.614%
7	7.129	984	991	1002	rVB2	53378	110707	23.23%	4.445%
8	8.653	1232	1241	1257	rBV	305365	476648	100.00%	19.138%
9	10.055	1465	1471	1479	rBV	290493	392919	82.43%	15.776%
10	11.085	1634	1640	1648	rBV	224396	284693	59.73%	11.431%
11	12.024	1789	1794	1803	rVB	276982	338377	70.99%	13.586%




Sum of corrected areas: 2490603

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
Data File : VX022201.D
Acq On : 26 May 2021 16:42
Operator : JC/MD
Sample : M2526-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-117T-20210525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

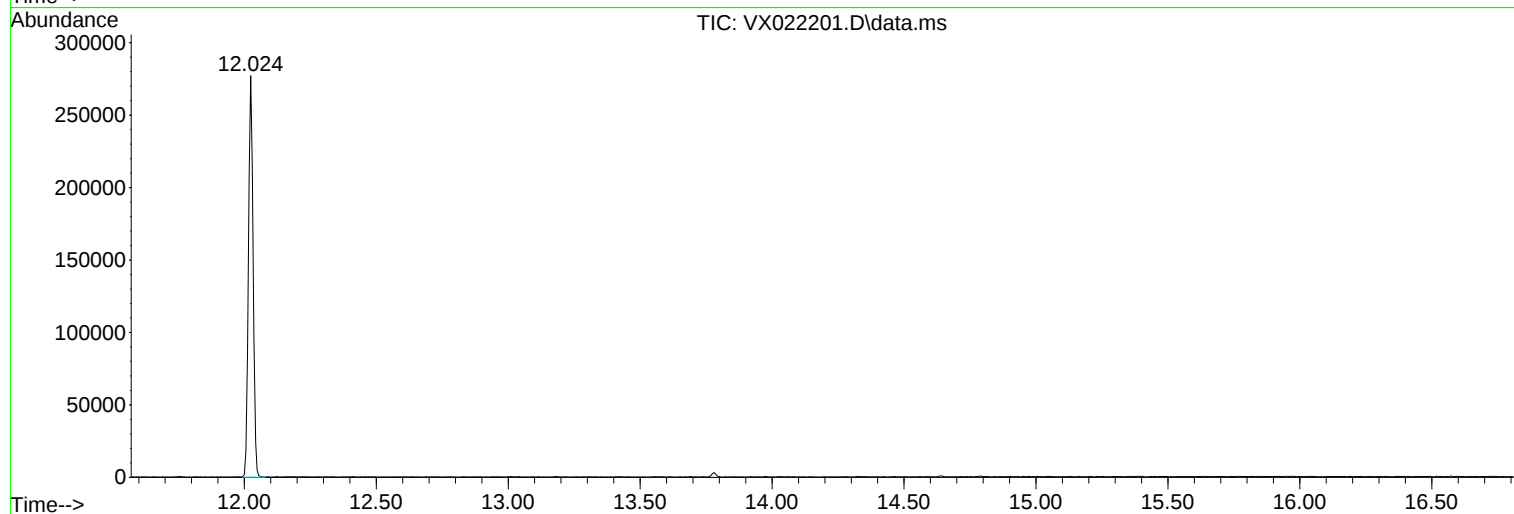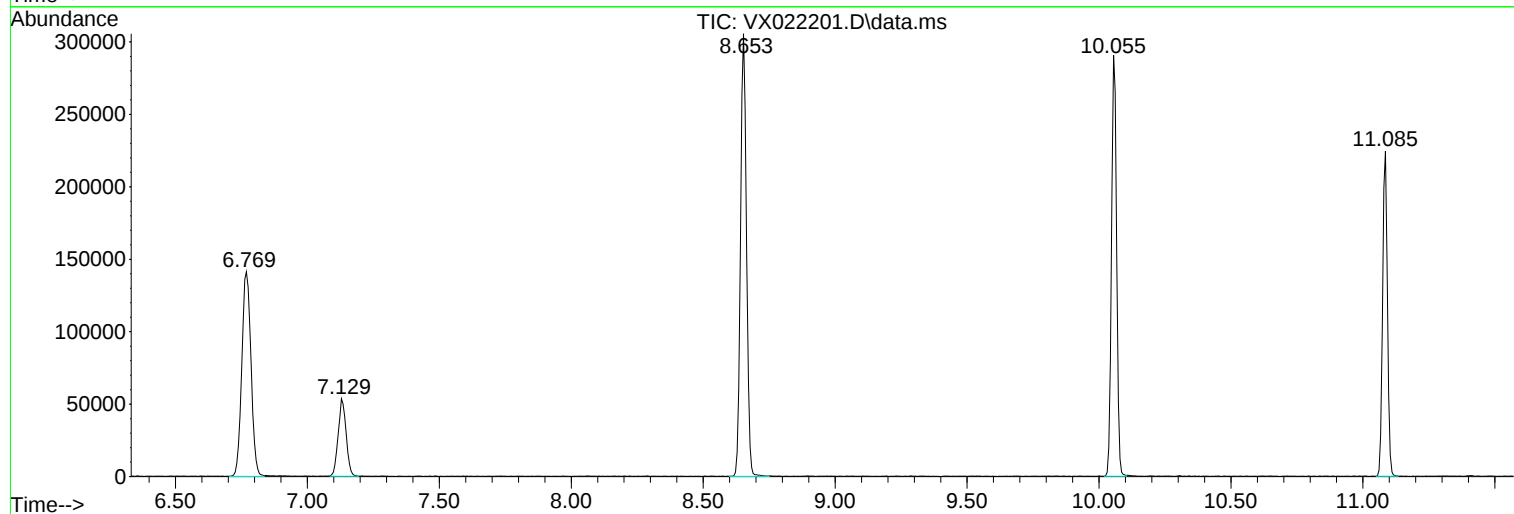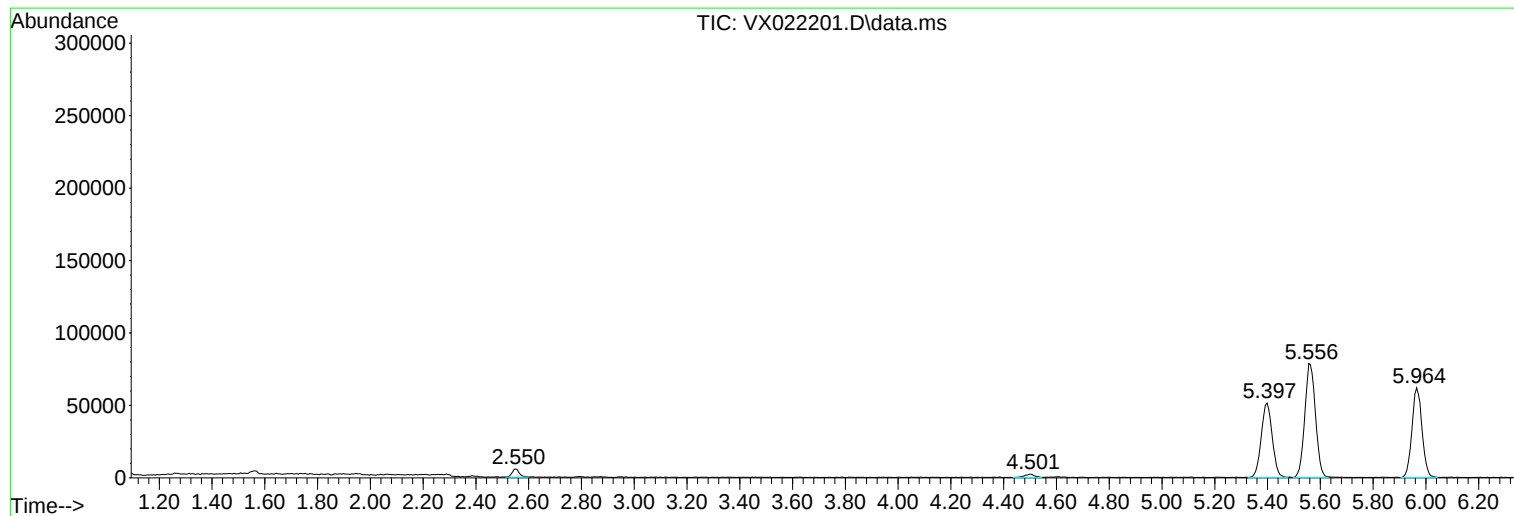

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
Data File : VX022201.D
Acq On : 26 May 2021 16:42
Operator : JC/MD
Sample : M2526-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-117T-20210525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
Data File : VX022201.D
Acq On : 26 May 2021 16:42
Operator : JC/MD
Sample : M2526-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-117T-20210525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
