

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
 Data File : VX022205.D
 Acq On : 26 May 2021 18:16
 Operator : JC/MD
 Sample : M2526-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MH-121.5T-20210525

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M

Title : SW846 8260

Signal : TIC: VX022205.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.550	232	240	248	rBV2	5180	10362	2.29%	0.465%
2	4.501	550	560	569	rBV3	4691	11767	2.60%	0.529%
3	5.397	696	707	722	rVB	48642	139608	30.85%	6.272%
4	5.562	722	734	746	rBV	76285	213481	47.17%	9.590%
5	5.964	790	800	814	rBV	61068	157366	34.77%	7.069%
6	6.769	921	932	944	rBV	135407	323946	71.58%	14.552%
7	7.135	984	992	1000	rVB2	5468	10933	2.42%	0.491%
8	8.653	1234	1241	1250	rBV	293126	452581	100.00%	20.331%
9	10.055	1466	1471	1481	rBV	269846	368575	81.44%	16.557%
10	11.085	1634	1640	1649	rVB	205790	252516	55.79%	11.344%
11	12.024	1789	1794	1801	rBV	236110	284927	62.96%	12.800%




Sum of corrected areas: 2226062

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
Data File : VX022205.D
Acq On : 26 May 2021 18:16
Operator : JC/MD
Sample : M2526-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-121.5T-20210525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

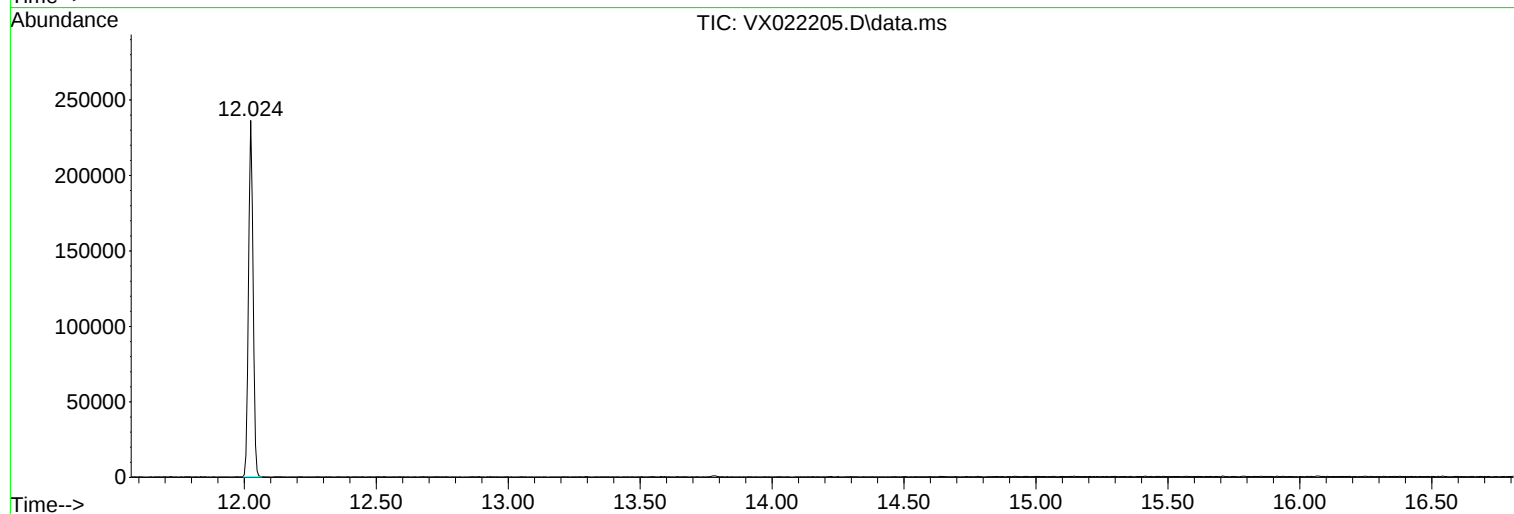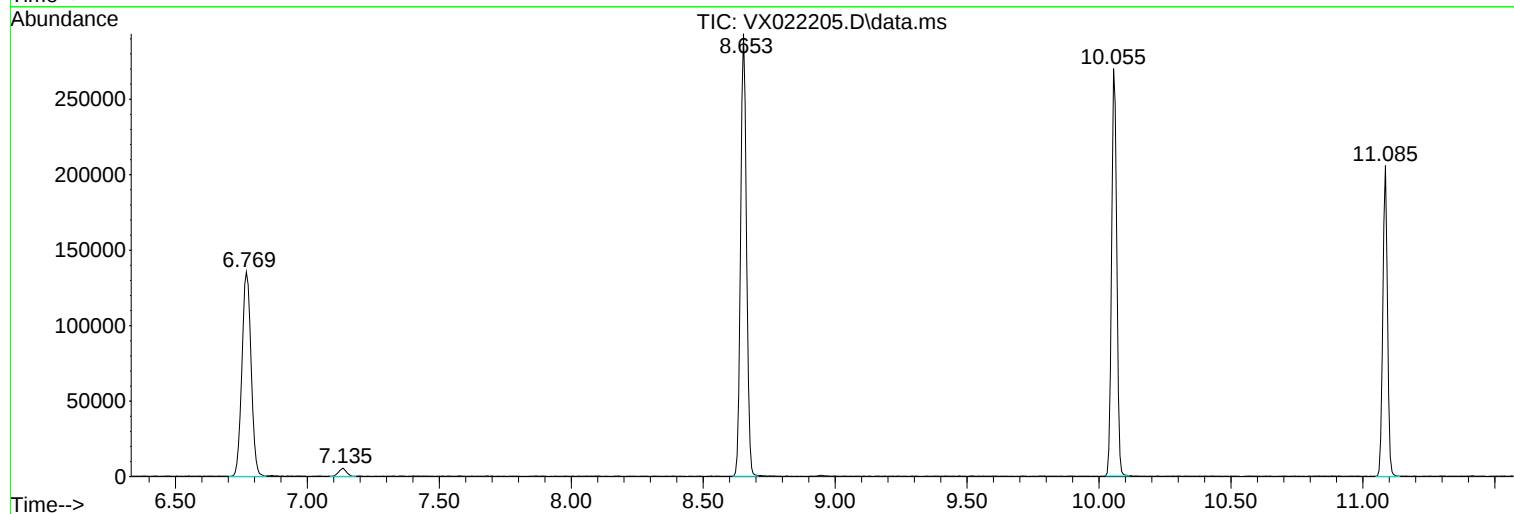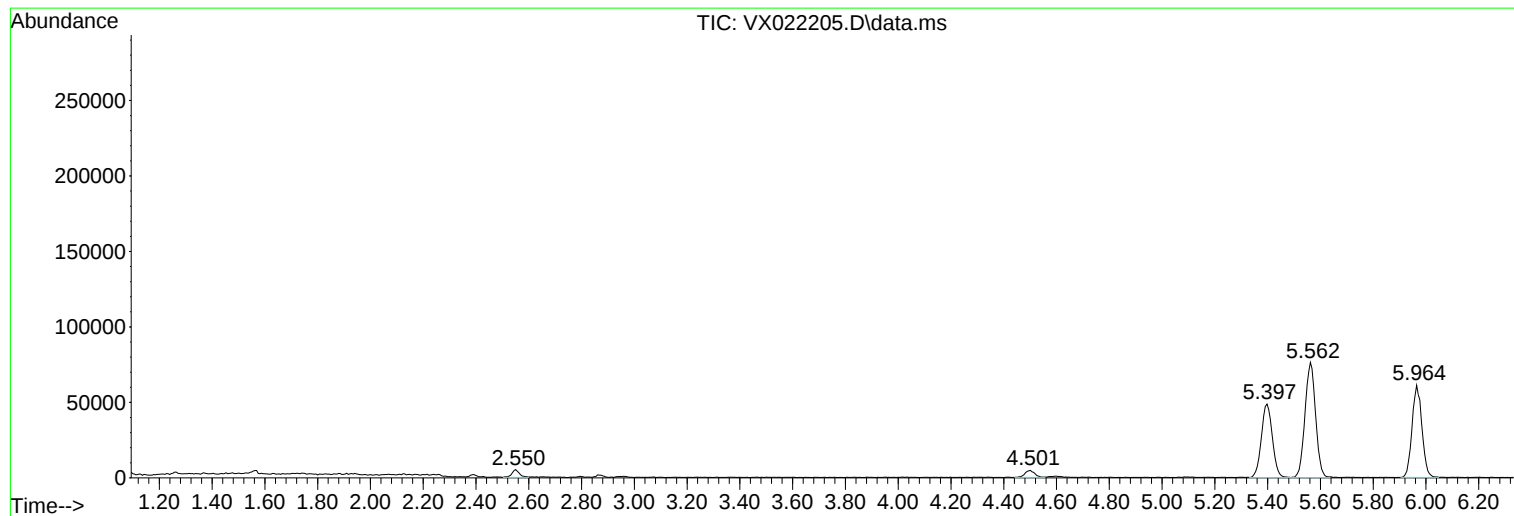

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
Data File : VX022205.D
Acq On : 26 May 2021 18:16
Operator : JC/MD
Sample : M2526-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-121.5T-20210525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
Data File : VX022205.D
Acq On : 26 May 2021 18:16
Operator : JC/MD
Sample : M2526-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-121.5T-20210525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------