

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
 Data File : VX022208.D
 Acq On : 26 May 2021 19:27
 Operator : JC/MD
 Sample : M2526-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 ROOF-DRAIN-20210525

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M

Title : SW846 8260

Signal : TIC: VX022208.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.386	208	213	219	rBV	3549	5764	1.27%	0.260%
2	2.544	233	239	249	rBV2	5879	10974	2.42%	0.496%
3	5.397	696	707	720	rBV	49127	140673	30.99%	6.356%
4	5.562	723	734	746	rVV2	76777	211490	46.59%	9.556%
5	5.964	790	800	815	rVB	62013	159375	35.11%	7.201%
6	6.769	920	932	944	rBV	140273	325052	71.61%	14.687%
7	8.653	1234	1241	1249	rBV	297562	453911	100.00%	20.509%
8	10.055	1464	1471	1485	rVB	267267	368970	81.29%	16.671%
9	11.085	1634	1640	1649	rVB	201051	252676	55.67%	11.417%
10	12.024	1789	1794	1800	rBV	235920	284329	62.64%	12.847%




Sum of corrected areas: 2213214

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
Data File : VX022208.D
Acq On : 26 May 2021 19:27
Operator : JC/MD
Sample : M2526-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ROOF-DRAIN-20210525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

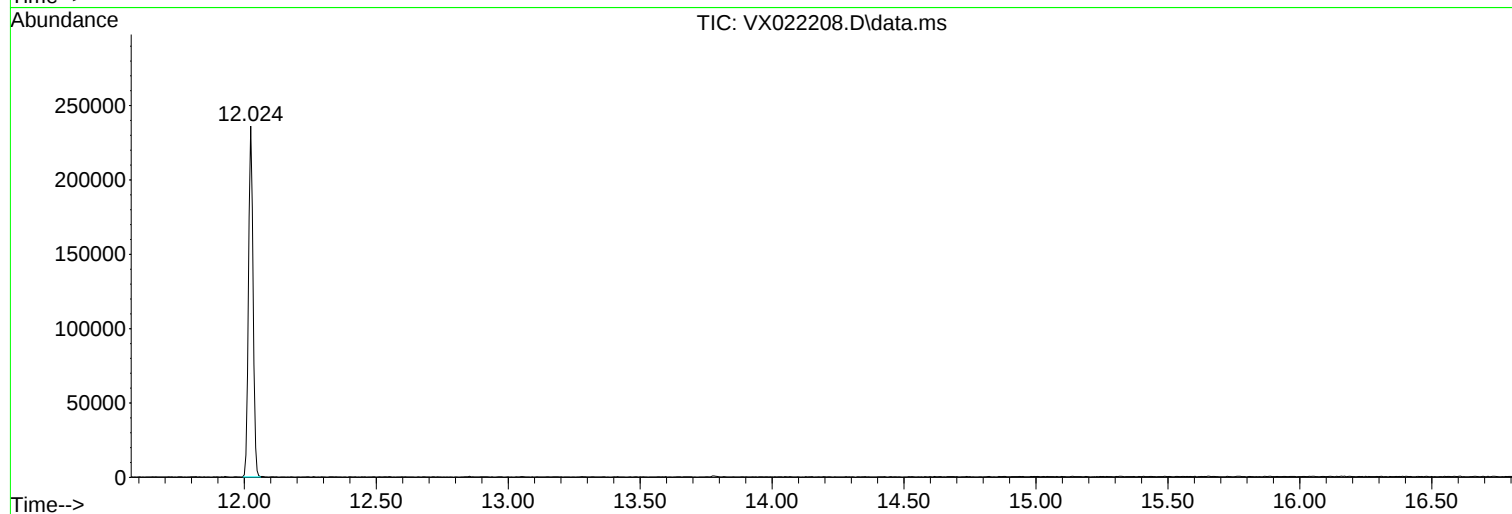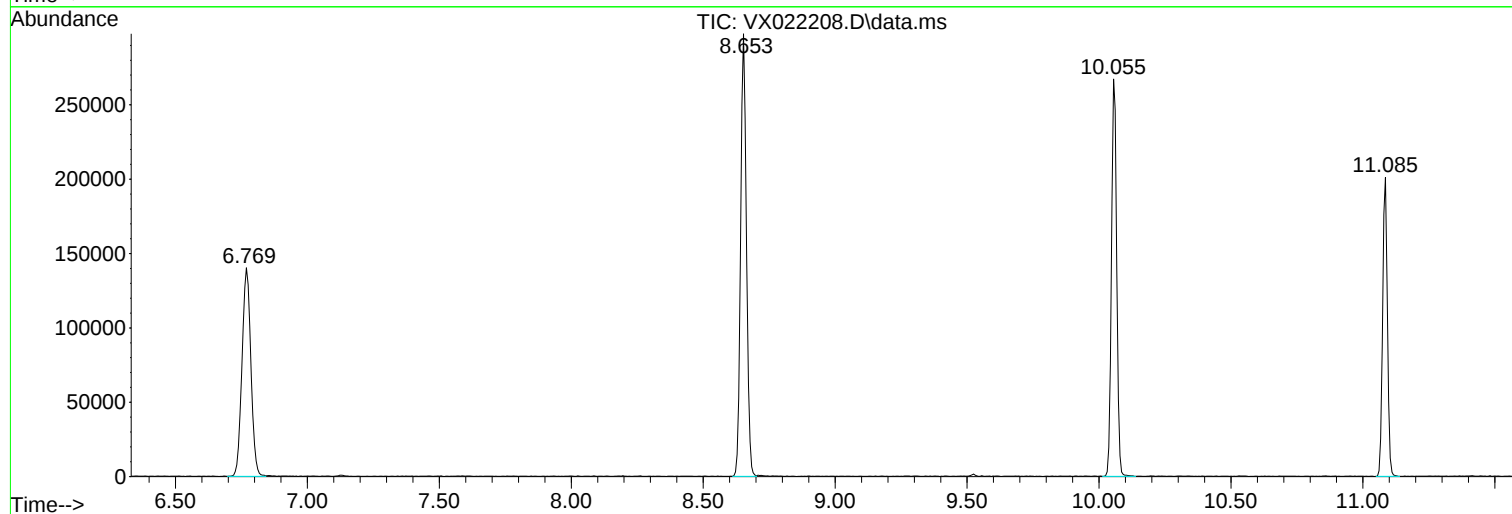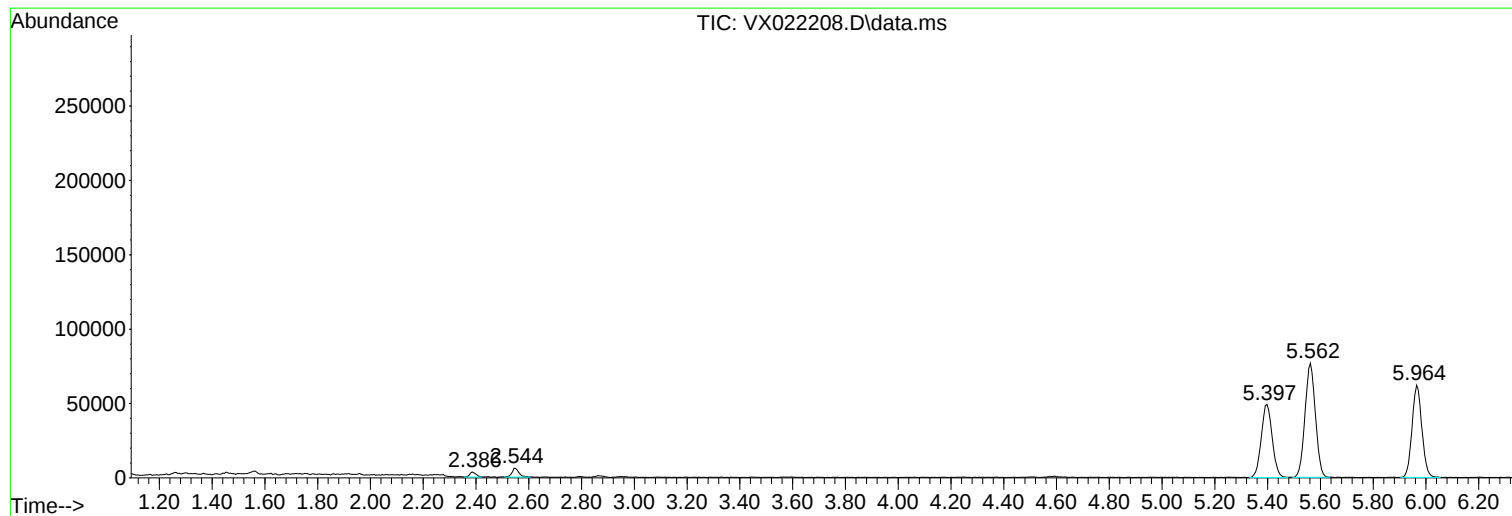

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
Data File : VX022208.D
Acq On : 26 May 2021 19:27
Operator : JC/MD
Sample : M2526-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ROOF-DRAIN-20210525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
Data File : VX022208.D
Acq On : 26 May 2021 19:27
Operator : JC/MD
Sample : M2526-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ROOF-DRAIN-20210525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
