

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
 Data File : VX022220.D
 Acq On : 27 May 2021 01:42
 Operator : JC/MD
 Sample : M2483-01 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DSN-001-SEWER-OUTLET-001

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X051321W.M

Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VX022220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.551	71	76	77	rBV4	2973	4341	1.52%	0.341%
2	1.672	94	96	101	rVB5	5054	4645	1.62%	0.365%
3	2.264	191	193	202	rVB4	1773	3626	1.27%	0.285%
4	2.398	209	215	220	rBV	4325	7770	2.71%	0.611%
5	2.581	238	245	256	rBV	54920	102711	35.89%	8.075%
6	2.788	272	279	284	rBV3	3824	6628	2.32%	0.521%
7	2.947	298	305	311	rBV	3897	8460	2.96%	0.665%
8	4.904	615	626	642	rBV2	35779	107932	37.71%	8.485%
9	5.093	650	657	658	rBV4	2829	4068	1.42%	0.320%
10	5.964	789	800	813	rVB	39483	104849	36.63%	8.243%
11	6.769	919	932	943	rBV2	86439	208387	72.81%	16.383%
12	8.653	1234	1241	1250	rBV	190245	286222	100.00%	22.502%
13	10.055	1466	1471	1481	rVB	183816	244627	85.47%	19.232%
14	11.085	1634	1640	1648	rVB	140639	177727	62.09%	13.972%




Sum of corrected areas: 1271993

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
Data File : VX022220.D
Acq On : 27 May 2021 01:42
Operator : JC/MD
Sample : M2483-01 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN-001-SEWER-OUTLET-001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X051321W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

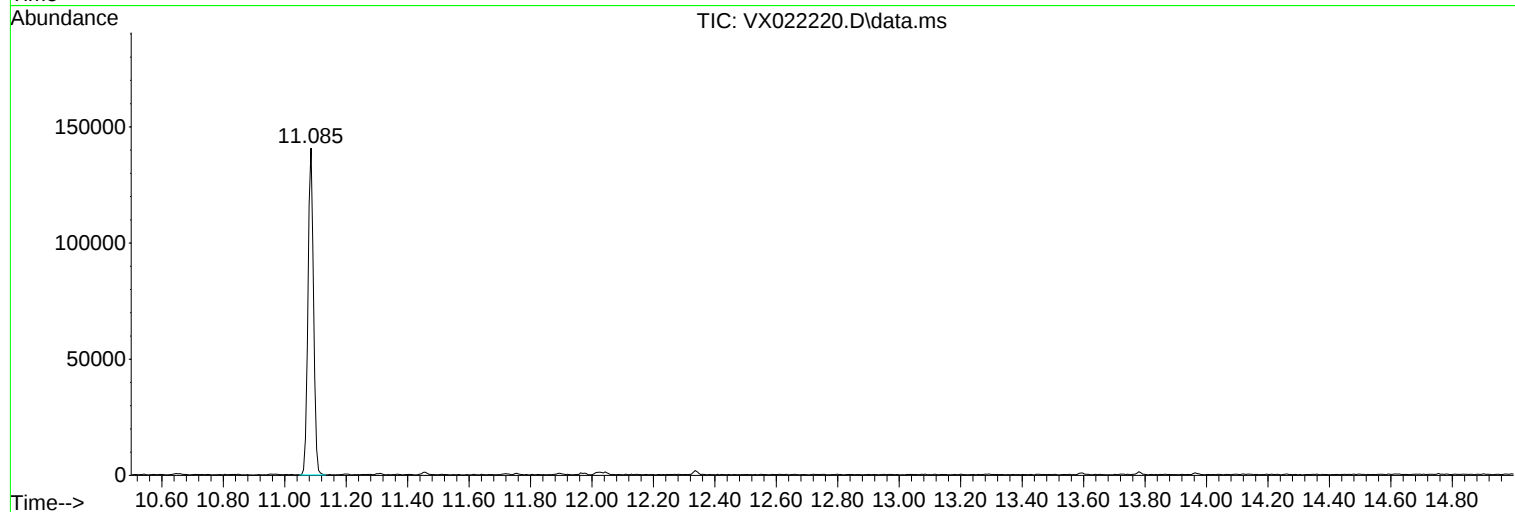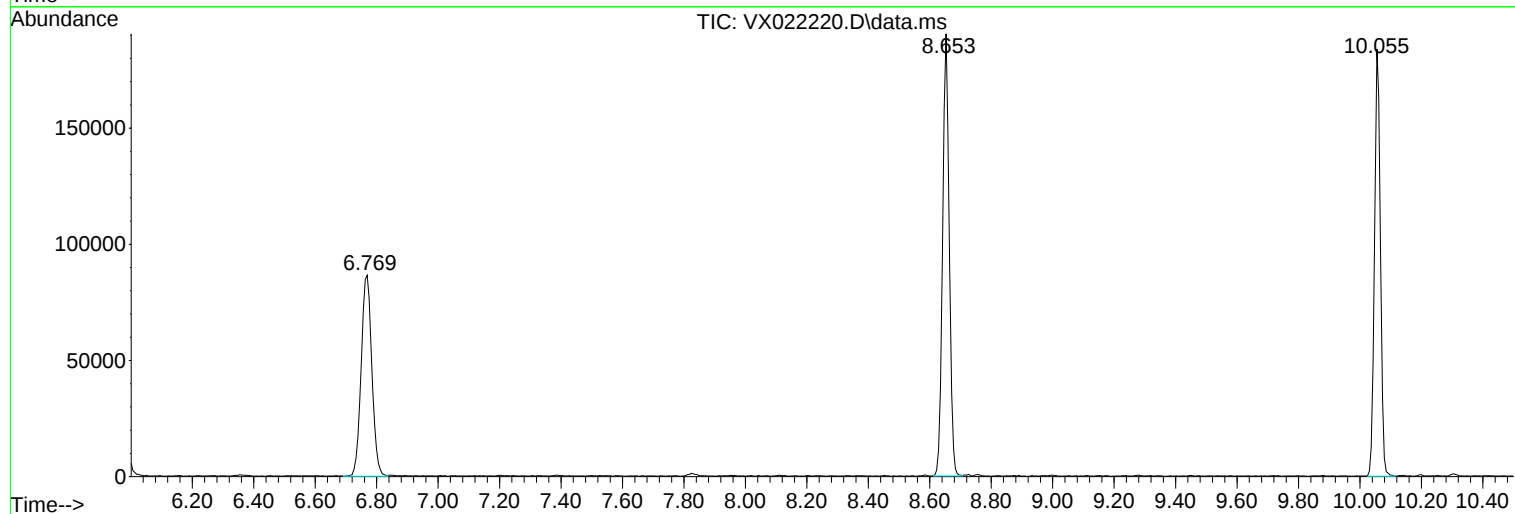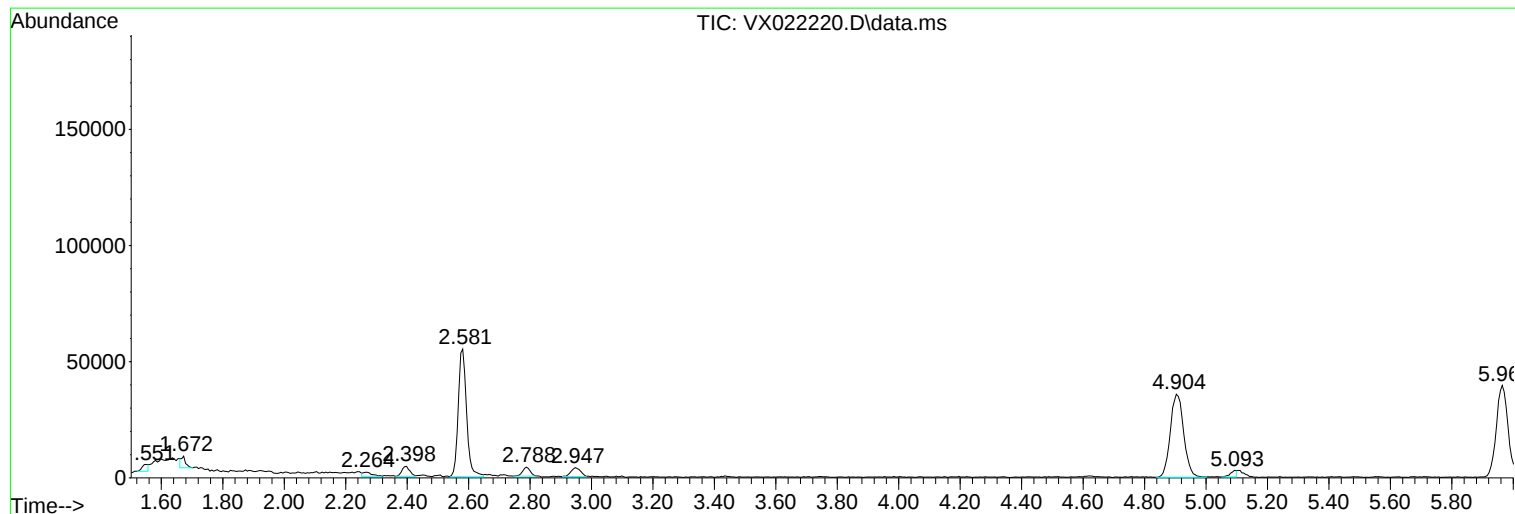

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
Data File : VX022220.D
Acq On : 27 May 2021 01:42
Operator : JC/MD
Sample : M2483-01 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN-001-SEWER-OUTLET-001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X051321W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052721\
Data File : VX022220.D
Acq On : 27 May 2021 01:42
Operator : JC/MD
Sample : M2483-01 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN-001-SEWER-OUTLET-001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X051321W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
