
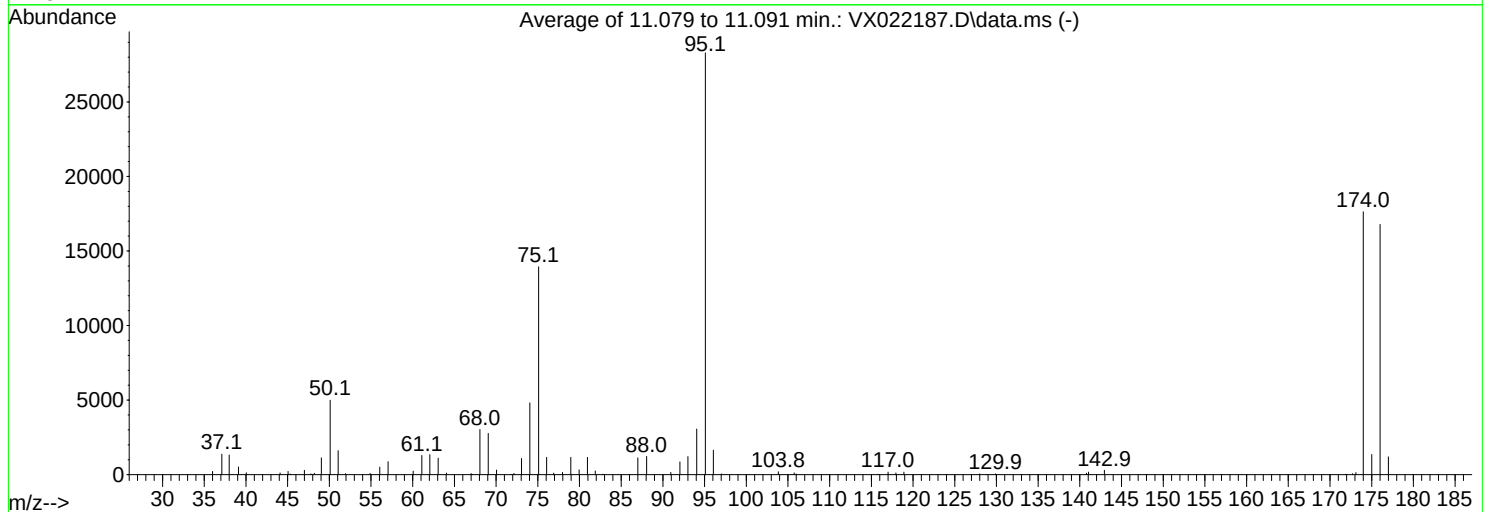


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX052721\  
 Data File : VX022187.D  
 Acq On : 26 May 2021 10:18  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051921W.M  
 Title : SW846 8260  
 Last Update : Wed May 19 14:23:10 2021

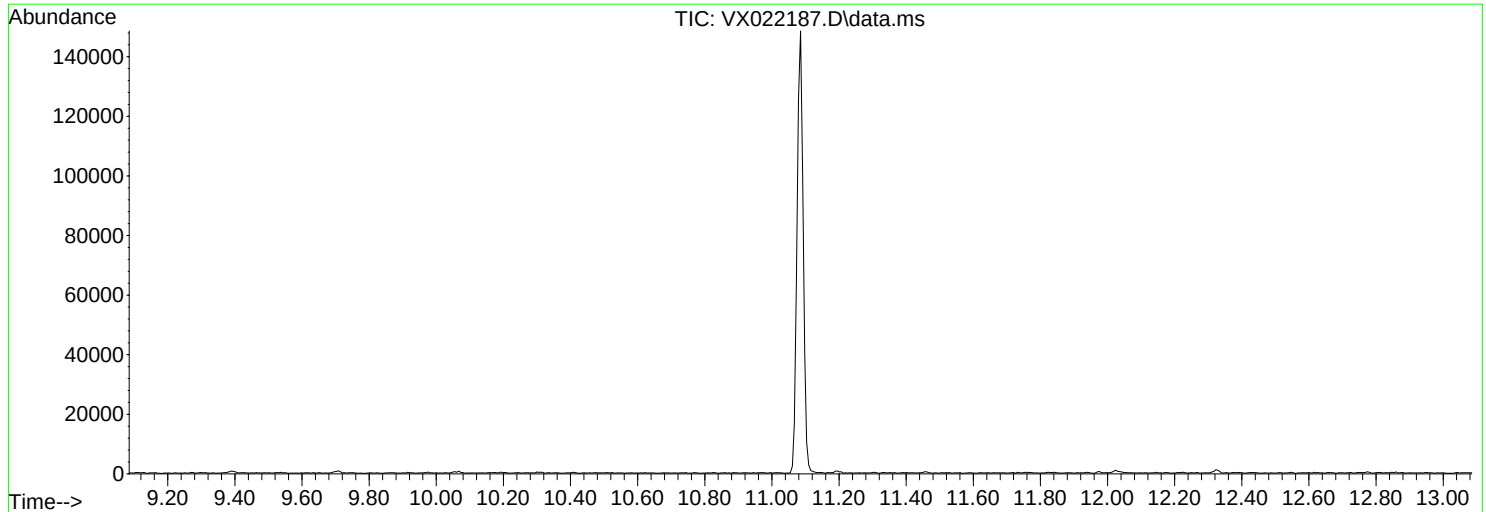

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 17.7         | 4995       | PASS                |
| 75             | 95              | 30              | 60              | 49.3         | 13940      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 28291      | PASS                |
| 96             | 95              | 5               | 9               | 5.8          | 1637       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.8          | 137        | PASS                |
| 174            | 95              | 50              | 100             | 62.3         | 17631      | PASS                |
| 175            | 174             | 5               | 9               | 7.7          | 1355       | PASS                |
| 176            | 174             | 95              | 101             | 95.2         | 16787      | PASS                |
| 177            | 176             | 5               | 9               | 7.1          | 1191       | PASS                |