

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
 Data File : VX029024.D
 Acq On : 27 May 2022 15:13
 Operator : JC/MD
 Sample : N2968-09DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-39

Quant Time: May 27 22:09:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 12 14:58:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	347738	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	610688	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	597997	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	297203	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	223645	46.918	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	93.840%		
35) Dibromofluoromethane	5.391	113	199921	49.966	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	99.940%		
50) Toluene-d8	8.653	98	731861	48.516	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	97.040%		
62) 4-Bromofluorobenzene	11.079	95	296813	52.679	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	105.360%		
Target Compounds					Qvalue	
5) Bromomethane	1.611	94	1703	Below Cal		97
6) Chloroethane	1.654	64	538	Below Cal	#	43
11) Tert butyl alcohol	2.953	59	25379	17.673	ug/l #	91
13) Acrolein	2.203	56	931	1.190	ug/l #	1
16) Acetone	2.380	43	1889	0.923	ug/l	99
19) Methyl tert-butyl Ether	3.111	73	9024	0.707	ug/l #	1
20) Methylene Chloride	2.794	84	1168	0.272	ug/l #	81
25) 2-Butanone	4.574	43	801	0.249	ug/l	99
31) Cyclohexane	5.477	56	6021	0.910	ug/l	85
36) 1,1-Dichloropropene	5.556	75	26816	4.462	ug/l #	50
38) Carbon Tetrachloride	5.556	117	36496	6.034	ug/l #	15
40) Benzene	6.044	78	359950	20.841	ug/l	97
42) 1,2-Dichloroethane	6.044	62	3536	0.555	ug/l #	73
52) Toluene	8.720	92	281530	25.339	ug/l	97
53) t-1,3-Dichloropropene	8.720	75	3183	2.088	ug/l #	1
67) Ethyl Benzene	10.195	91	702738	30.905	ug/l	99
68) m/p-Xylenes	10.305	106	713214	80.564	ug/l	100
69) o-Xylene	10.646	106	362576	41.599	ug/l	99
70) Styrene	10.646	104	19407	1.371	ug/l #	1
73) Isopropylbenzene	10.963	105	33019	1.465	ug/l	97
76) 1,2,3-Trichloropropane	11.079	75	145587	20.917	ug/l #	38
78) n-propylbenzene	11.305	91	103305	3.962	ug/l	99
79) 2-Chlorotoluene	11.378	91	47226	2.956	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.451	105	123803	6.592	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.079	75	145587	61.441	ug/l #	15
82) 4-Chlorotoluene	11.451	91	13287	0.719	ug/l #	46
83) tert-Butylbenzene	11.756	119	66226	3.642	ug/l #	53
84) 1,2,4-Trimethylbenzene	11.756	105	544144	28.894	ug/l	99
85) sec-Butylbenzene	11.756	105	544144	24.261	ug/l #	56
86) p-Isopropyltoluene	11.975	119	6619	0.352	ug/l	94
89) n-Butylbenzene	12.323	91	8796	0.539	ug/l #	19
90) Hexachloroethane	12.646	117	6199	2.037	ug/l #	10
95) Naphthalene	13.774	128	240007	11.364	ug/l	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

MSVOA_X


ClientSampleId :


MW-39

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029024.D
Acq On : 27 May 2022 15:13
Operator : JC/MD
Sample : N2968-09DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-39


Quant Time: May 27 22:09:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260
QLast Update : Thu May 12 14:58:53 2022
Response via : Initial Calibration

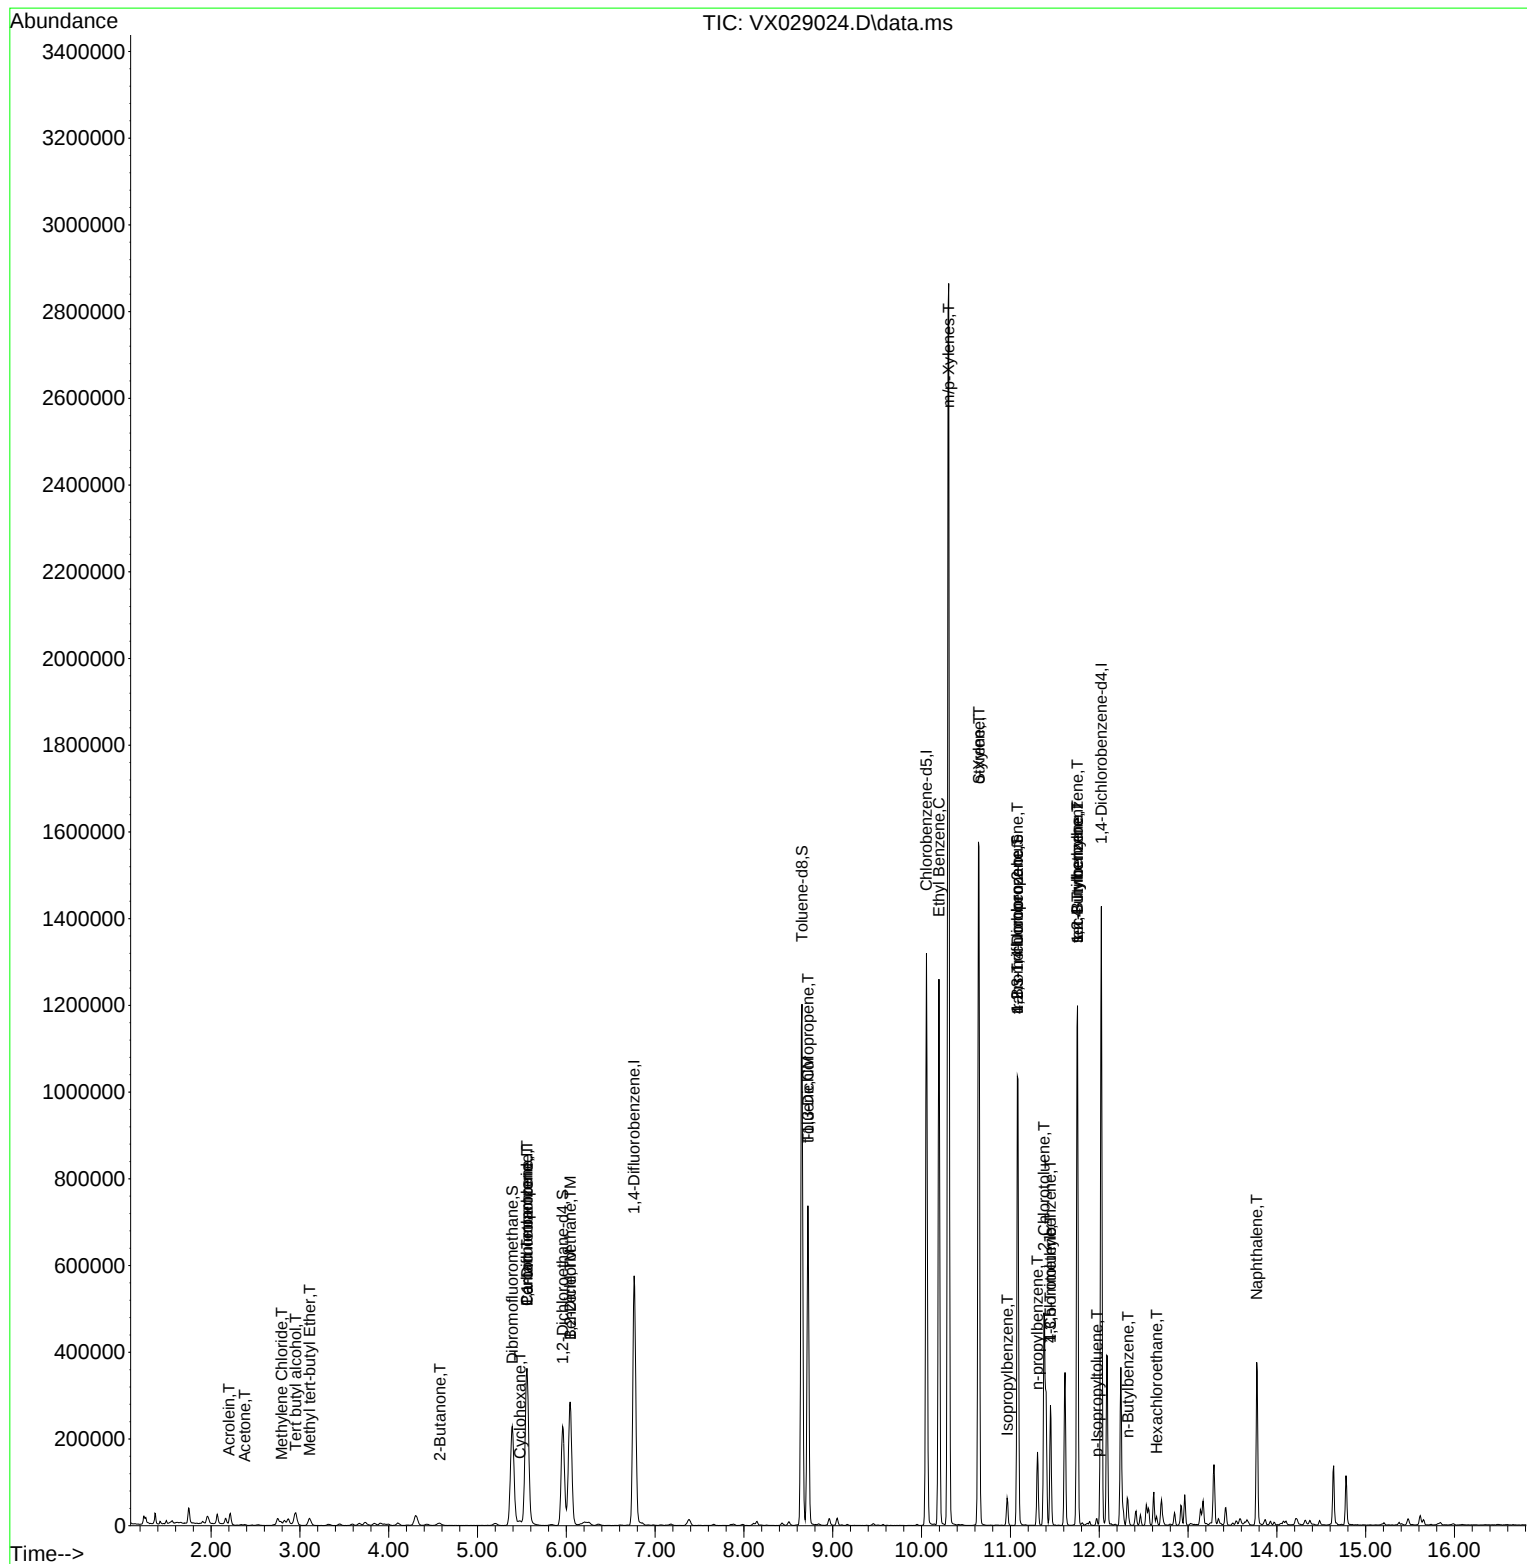






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.007 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13

Instrument :
MSVOA_X
ClientSampleId :
MW-39







Tgt Ion:168 Resp: 347738
Ion Ratio Lower Upper
168 100
99 59.9 41.7 62.5

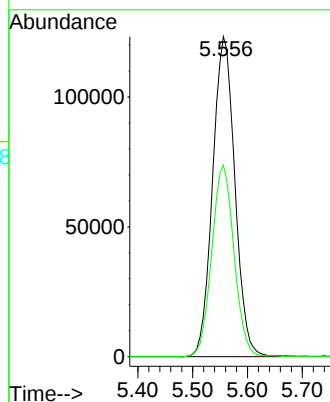

#5
Bromomethane
Concen: Below Cal
RT: 1.611 min Scan# 86
Delta R.T. 0.012 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13

Tgt Ion: 94 Resp: 1703
Ion Ratio Lower Upper
94 100
96 91.2 75.3 112.9


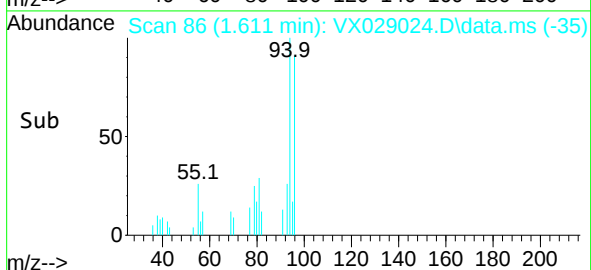
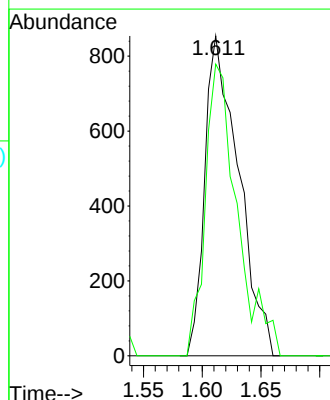



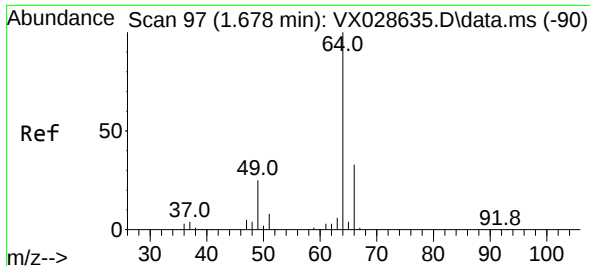

#6
Chloroethane
Concen: Below Cal
RT: 1.654 min Scan# 91
Delta R.T. -0.024 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13




Instrument :
MSVOA_X
ClientSampleId :
MW-39


Tgt Ion: 64 Resp: 538
Ion Ratio Lower Upper
64 100
66 0.0 25.3 37.9#

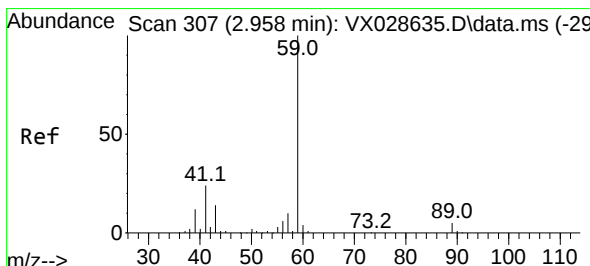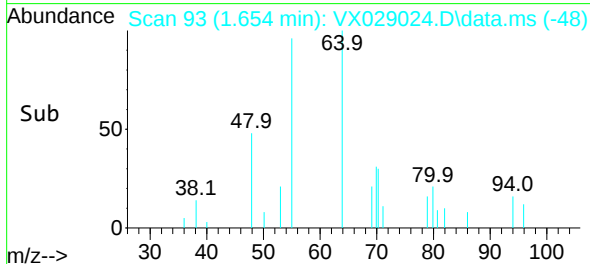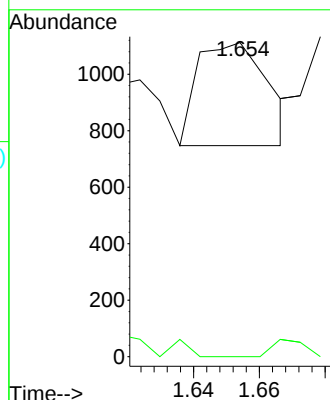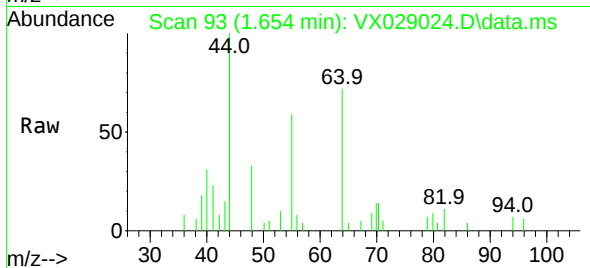

#11
Tert butyl alcohol
Concen: 17.673 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.005 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13

Tgt Ion: 59 Resp: 25379
Ion Ratio Lower Upper
59 100
57 7.0 8.3 12.5#


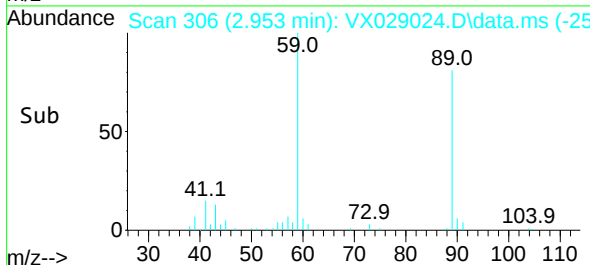
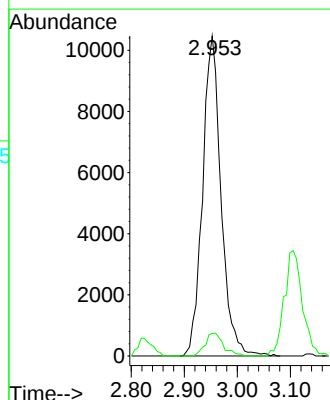
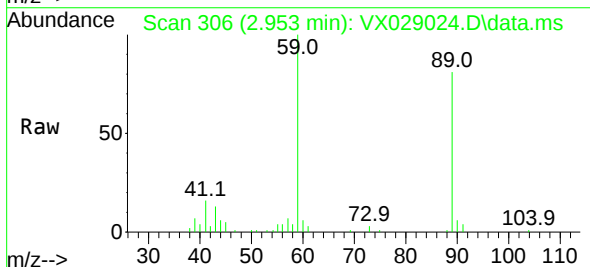




#13
Acrolein
Concen: 1.190 ug/l
RT: 2.203 min Scan# 11
Delta R.T. -0.030 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13




Instrument :
MSVOA_X
ClientSampleId :
MW-39


Tgt Ion: 56 Resp: 931
Ion Ratio Lower Upper
56 100
55 1540.4 55.0 82.6#

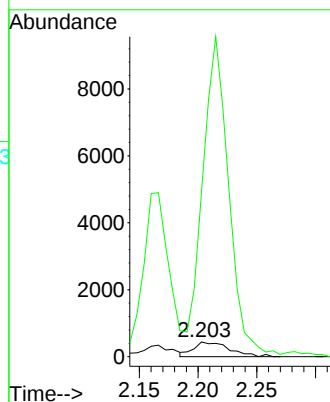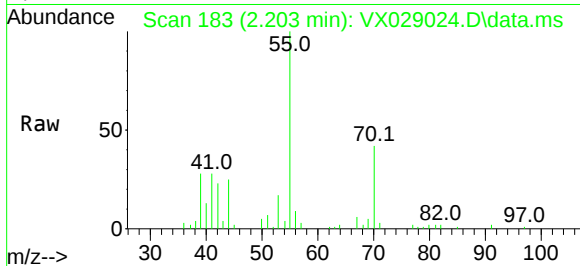

#16
Acetone
Concen: 0.923 ug/l
RT: 2.380 min Scan# 212
Delta R.T. 0.007 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13

Tgt Ion: 43 Resp: 1889
Ion Ratio Lower Upper
43 100
58 36.7 28.8 43.2


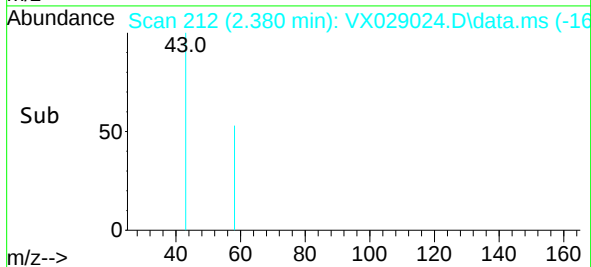
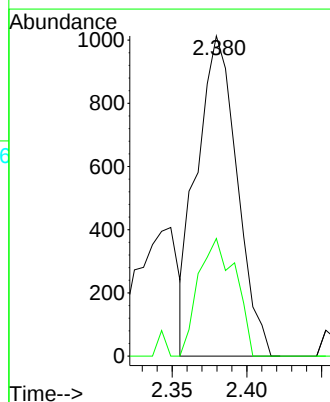
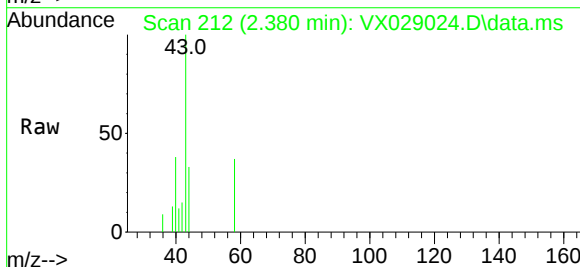




#19
Methyl tert-butyl Ether
Concen: 0.707 ug/l
RT: 3.111 min Scan# 311
Delta R.T. 0.000 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13




Instrument :
MSVOA_X
ClientSampleId :
MW-39


Tgt Ion: 73 Resp: 9024
Ion Ratio Lower Upper
73 100
57 83.2 16.8 25.2#

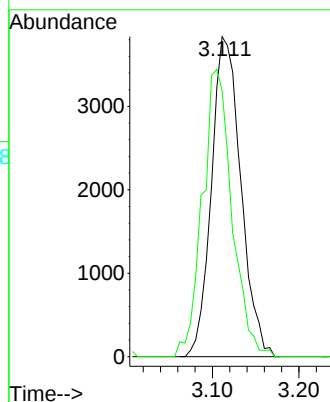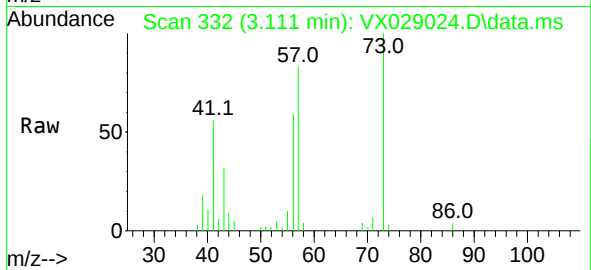

#20
Methylene Chloride
Concen: 0.272 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.006 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13

Tgt Ion: 84 Resp: 1168
Ion Ratio Lower Upper
84 100
49 81.2 85.5 128.3#
51 18.6 26.6 39.8#
86 60.5 51.5 77.3


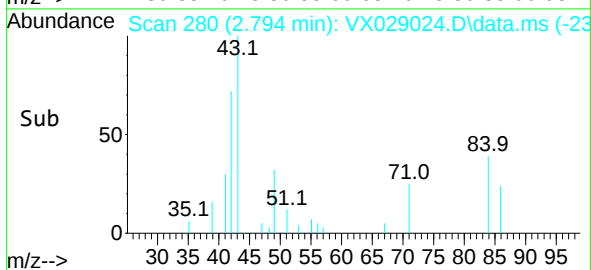
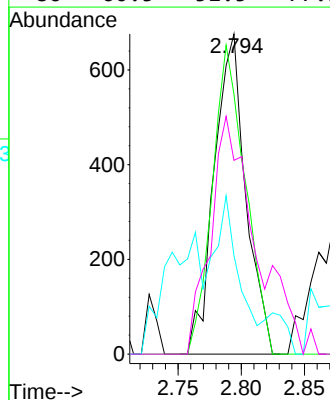
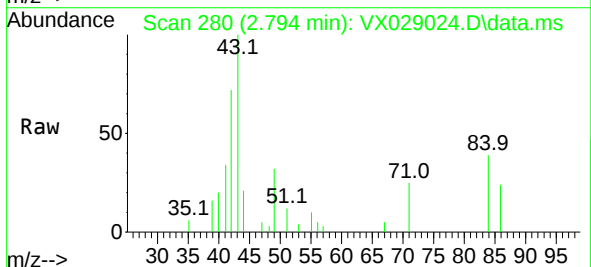




#25
2-Butanone
Concen: 0.249 ug/l
RT: 4.574 min Scan# 51
Delta R.T. 0.024 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13




Instrument :
MSVOA_X
ClientSampleId :
MW-39


Tgt Ion: 43 Resp: 801
Ion Ratio Lower Upper
43 100
72 31.1 24.4 36.6

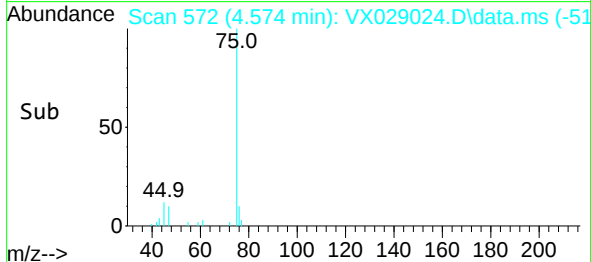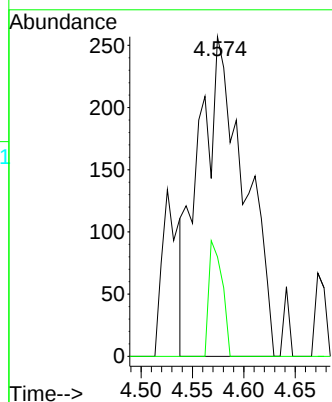

#31
Cyclohexane
Concen: 0.910 ug/l
RT: 5.477 min Scan# 720
Delta R.T. 0.013 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13

Tgt Ion: 56 Resp: 6021
Ion Ratio Lower Upper
56 100
69 29.2 26.7 40.1
84 113.2 77.2 115.8

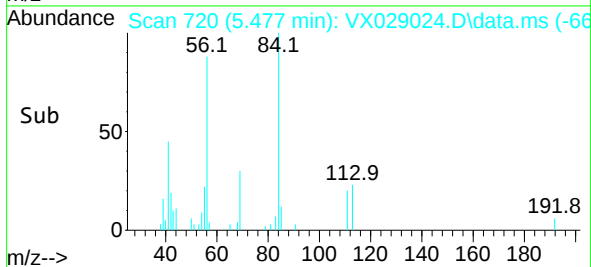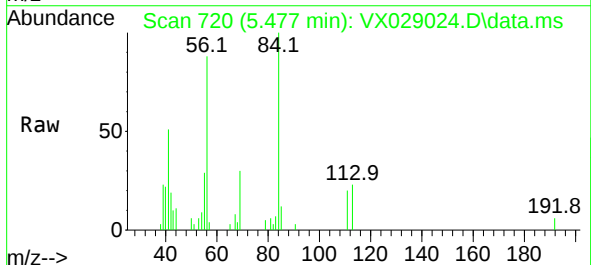

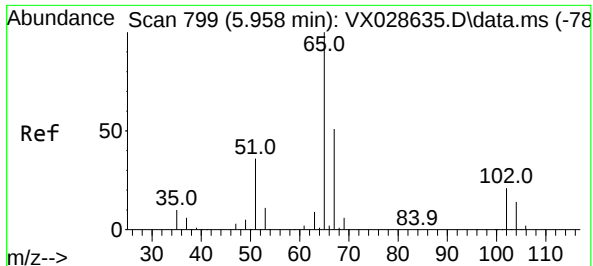

#33

1,2-Dichloroethane-d4

Concen: 46.918 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX029024.D

Acq: 27 May 2022 15:13

Instrument :

MSVOA_X

ClientSampleId :





MW-39

Tgt Ion: 65 Resp: 223645

Ion Ratio Lower Upper

65 100

67 51.9 0.0 107.4

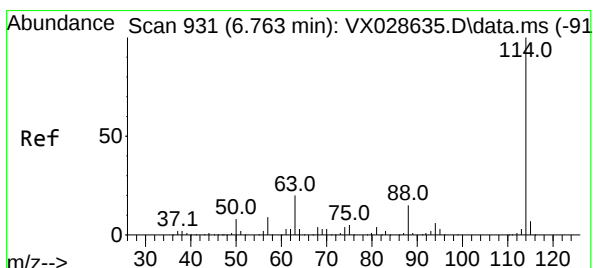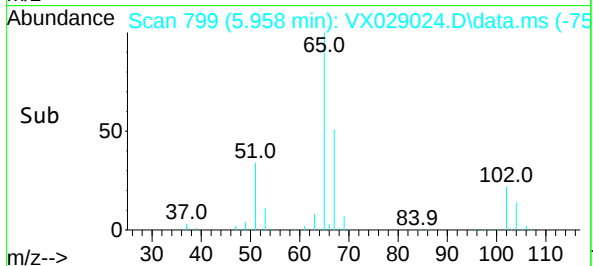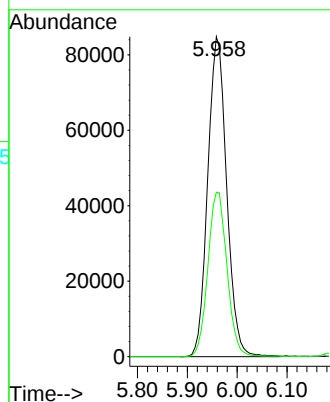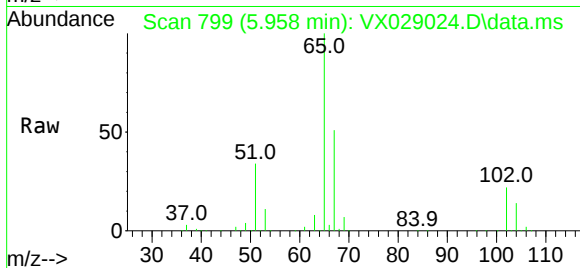

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX029024.D

Acq: 27 May 2022 15:13




Tgt Ion: 114 Resp: 610688


Ion Ratio Lower Upper

114 100

63 19.5 0.0 36.8

88 16.5 0.0 32.4

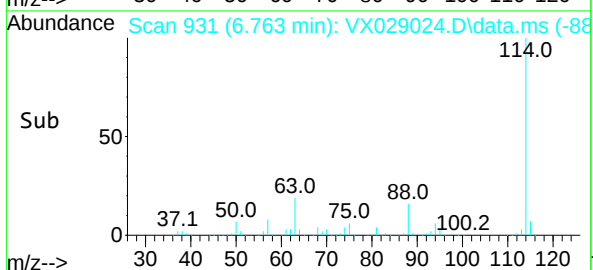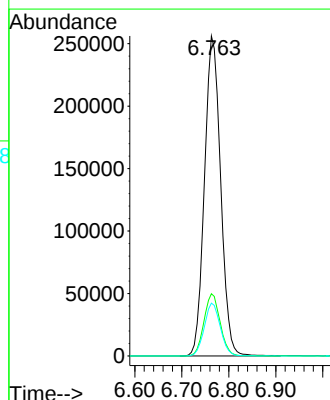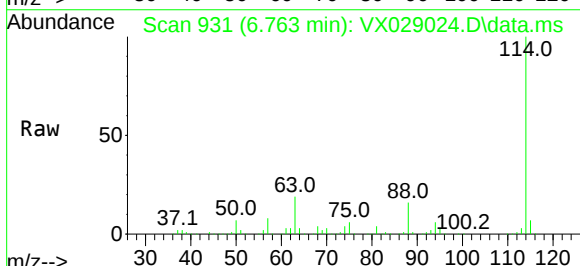

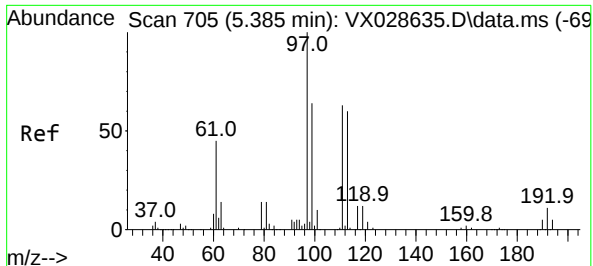

#35

Dibromofluoromethane

Concen: 49.966 ug/l

RT: 5.391 min Scan# 705

Delta R.T. 0.006 min

Lab File: VX029024.D

Acq: 27 May 2022 15:13

Instrument :

MSVOA_X

ClientSampleId :

MW-39





Tgt Ion:113 Resp: 199921

Ion Ratio Lower Upper

113 100

111 102.8 82.8 124.2

192 20.1 16.9 25.3

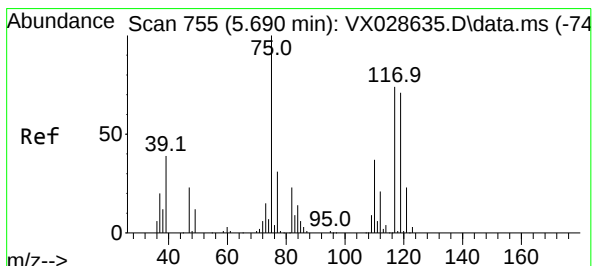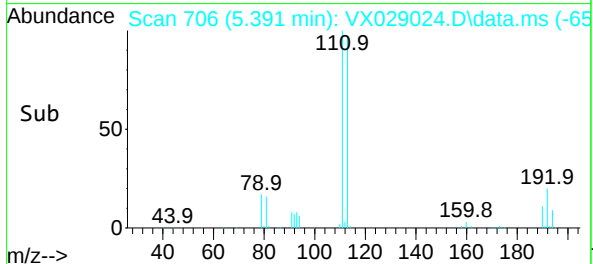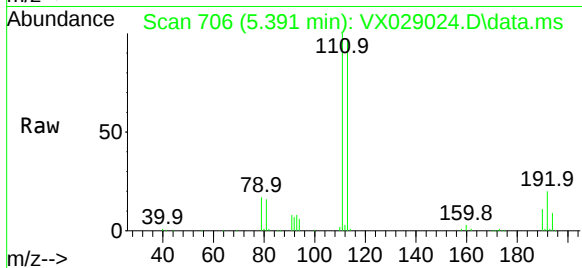

#36

1,1-Dichloropropene

Concen: 4.462 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.134 min

Lab File: VX029024.D

Acq: 27 May 2022 15:13




Tgt Ion: 75 Resp: 26816


Ion Ratio Lower Upper

75 100

110 9.9 18.3 54.8#

77 0.0 24.8 37.2#


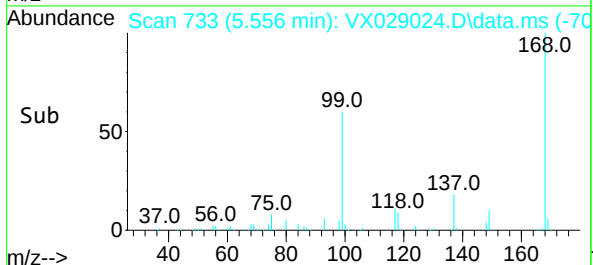
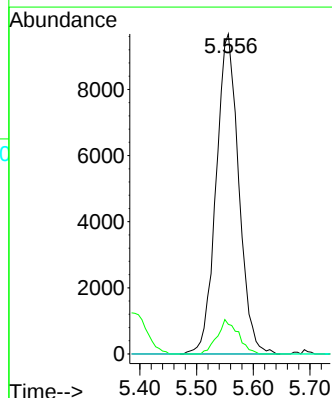
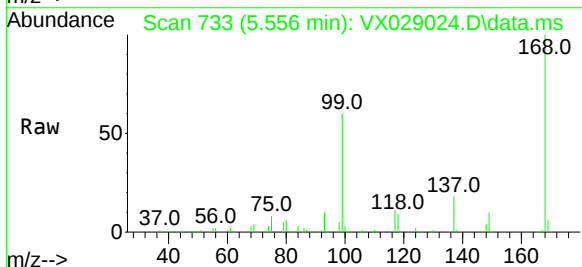


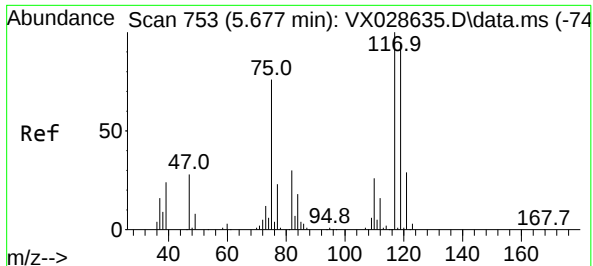

#38
Carbon Tetrachloride
Concen: 6.034 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.121 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13




Instrument :
MSVOA_X
ClientSampleId :
MW-39


Tgt Ion:117 Resp: 36496
Ion Ratio Lower Upper
117 100
119 4.4 77.3 115.9#
121 0.0 24.2 36.2#

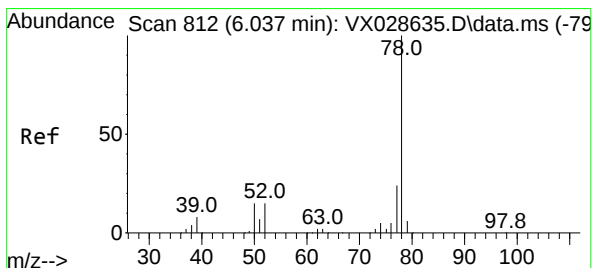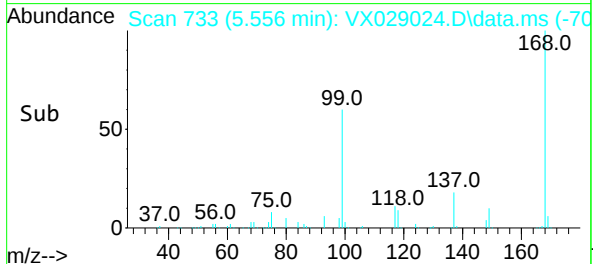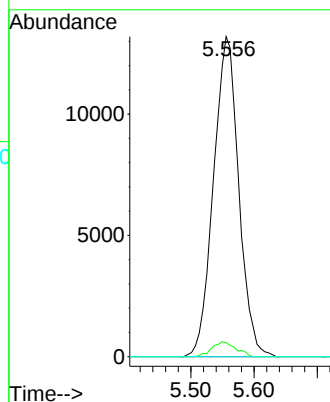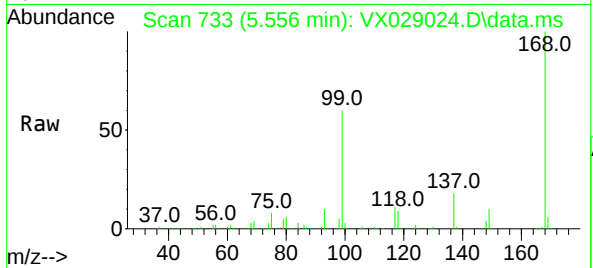

#40
Benzene
Concen: 20.841 ug/l
RT: 6.044 min Scan# 813
Delta R.T. 0.007 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13

Tgt Ion: 78 Resp: 359950
Ion Ratio Lower Upper
78 100
77 22.7 19.3 28.9

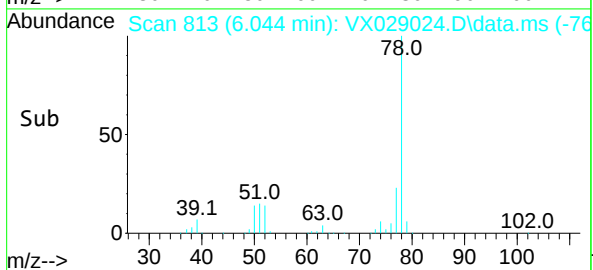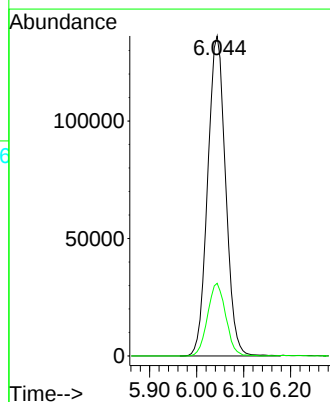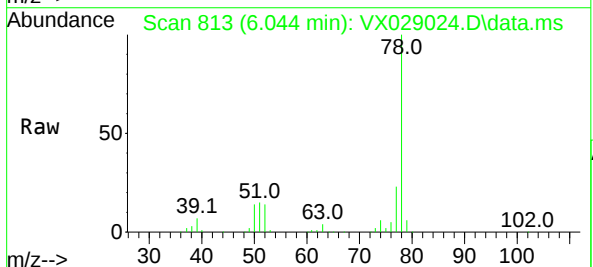



#42

1,2-Dichloroethane

Concen: 0.555 ug/l

RT: 6.044 min Scan# 81

Delta R.T. -0.042 min

Lab File: VX029024.D

Acq: 27 May 2022 15:13

Instrument :

MSVOA_X

ClientSampleId :





MW-39

Tgt Ion: 62 Resp: 3536

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.4

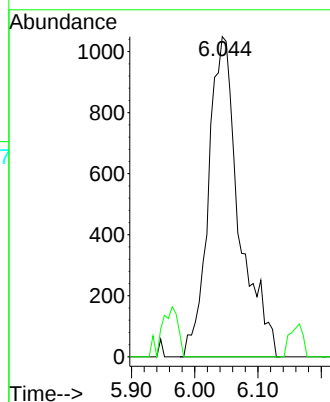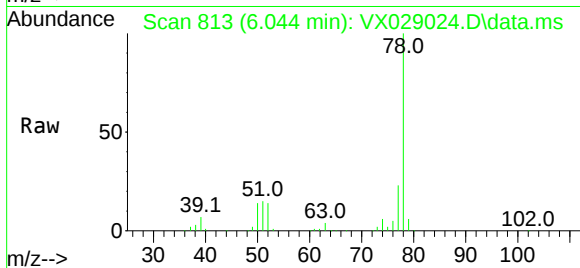

#50

Toluene-d8

Concen: 48.516 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. 0.007 min

Lab File: VX029024.D




Acq: 27 May 2022 15:13


Tgt Ion: 98 Resp: 731861

Ion Ratio Lower Upper

98 100

100 66.9 52.6 78.8



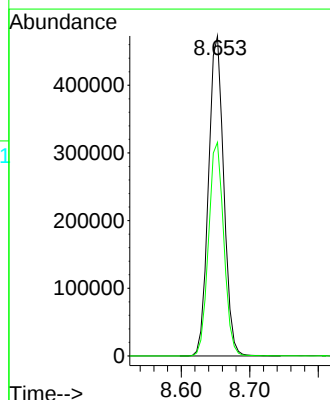
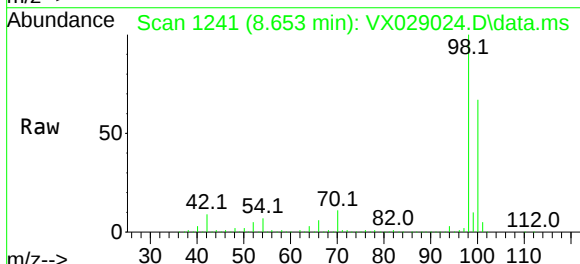




#52
Toluene
Concen: 25.339 ug/l
RT: 8.720 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13




Instrument :
MSVOA_X
ClientSampleId :
MW-39


Tgt Ion: 92 Resp: 281530
Ion Ratio Lower Upper
92 100
91 167.7 137.5 206.3

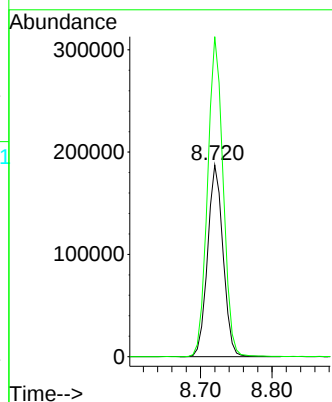

#53
t-1,3-Dichloropropene
Concen: 2.088 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.256 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13

Tgt Ion: 75 Resp: 3183
Ion Ratio Lower Upper
75 100
77 181.3 25.4 38.0#


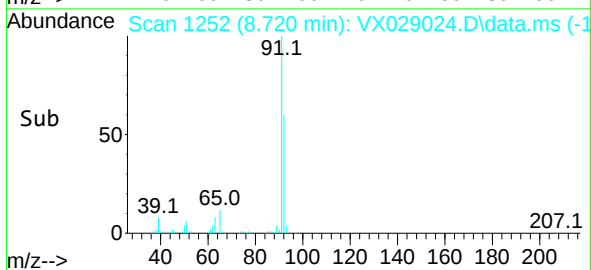
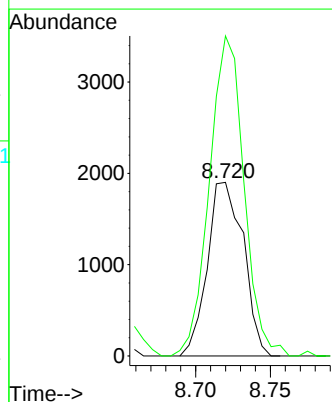
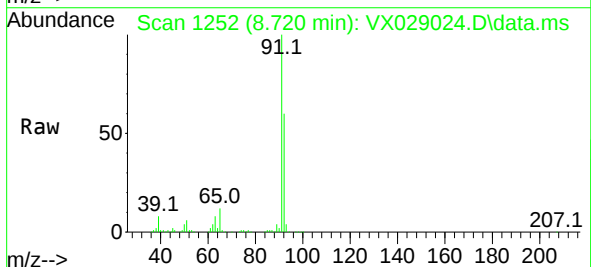




#62
4-Bromofluorobenzene
Concen: 52.679 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13




Instrument :
MSVOA_X
ClientSampleId :
MW-39


Tgt Ion: 95 Resp: 296813
Ion Ratio Lower Upper
95 100
174 77.1 0.0 163.0
176 74.7 0.0 155.0

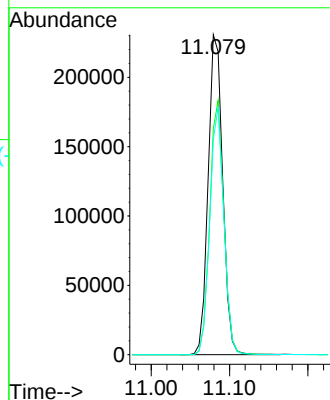

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13

Tgt Ion: 117 Resp: 597997
Ion Ratio Lower Upper
117 100
82 55.1 41.8 62.8
119 32.7 24.8 37.2


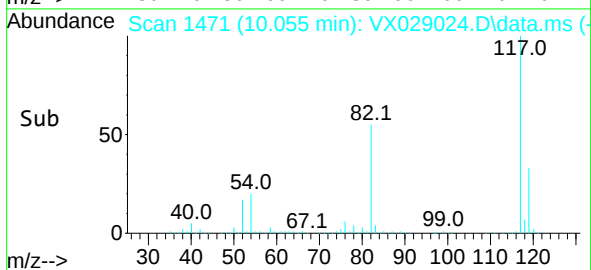
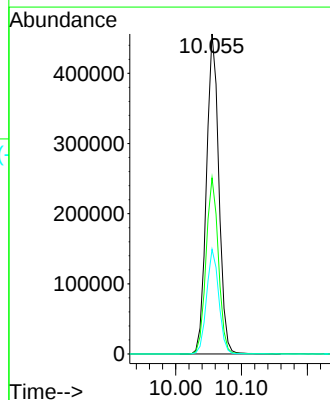





#67
Ethyl Benzene
Concen: 30.905 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13




Instrument :
MSVOA_X
ClientSampleId :
MW-39


Tgt Ion: 91 Resp: 702738
Ion Ratio Lower Upper
91 100
106 31.2 24.6 36.8

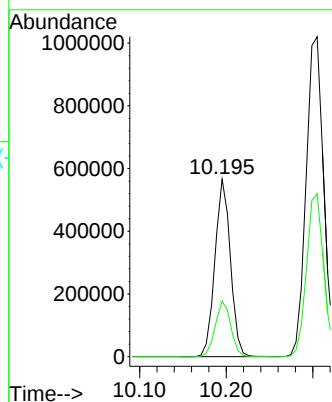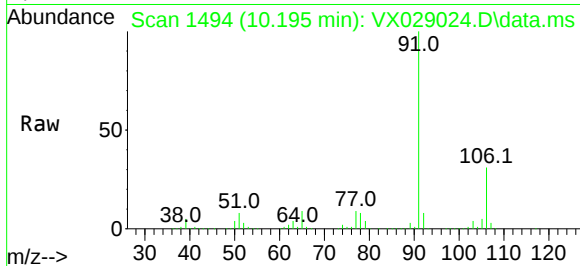

#68
m/p-Xylenes
Concen: 80.564 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13

Tgt Ion: 106 Resp: 713214
Ion Ratio Lower Upper
106 100
91 200.1 160.4 240.6


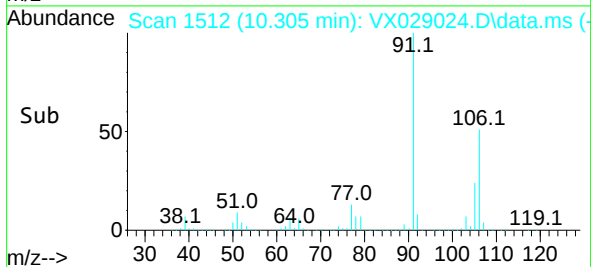
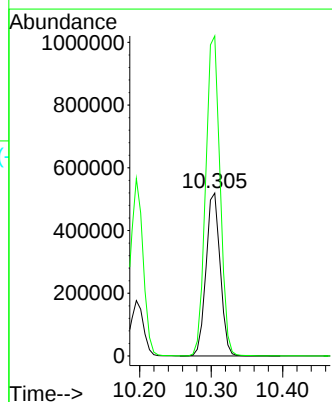
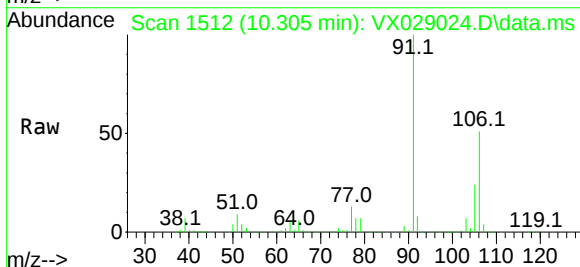




#69
o-Xylene
Concen: 41.599 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13




Instrument :
MSVOA_X
ClientSampleId :
MW-39


Tgt Ion:106 Resp: 362576
Ion Ratio Lower Upper
106 100
91 213.2 106.1 318.1

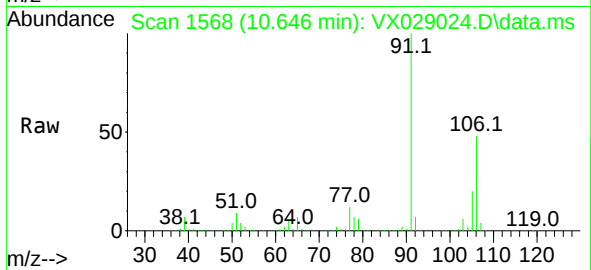

#70
Styrene
Concen: 1.371 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.012 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13

Tgt Ion:104 Resp: 19407
Ion Ratio Lower Upper
104 100
78 275.3 38.6 57.8#
103 252.9 43.8 65.8#



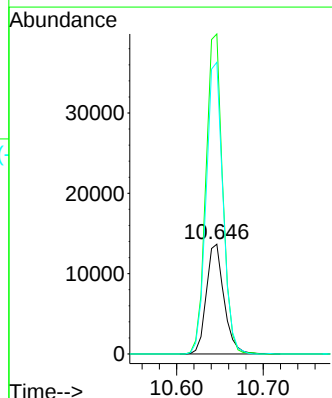
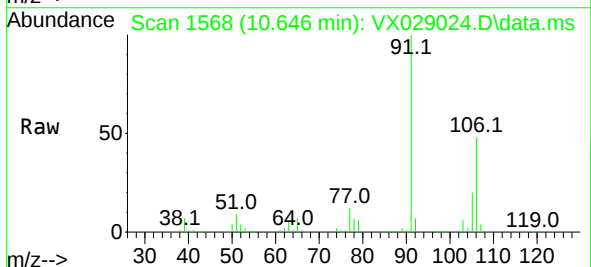




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13




Instrument :
MSVOA_X
ClientSampleId :
MW-39


Tgt Ion:152 Resp: 297203
Ion Ratio Lower Upper
152 100
115 60.6 37.5 112.7
150 154.6 0.0 338.2

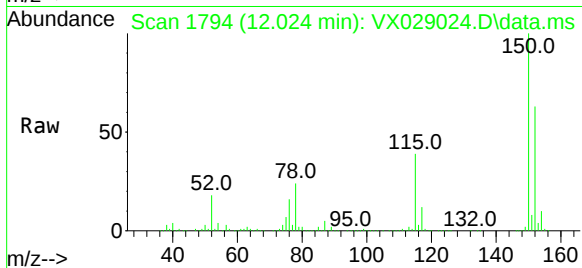

#73
Isopropylbenzene
Concen: 1.465 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13

Tgt Ion:105 Resp: 33019
Ion Ratio Lower Upper
105 100
120 25.6 13.5 40.5


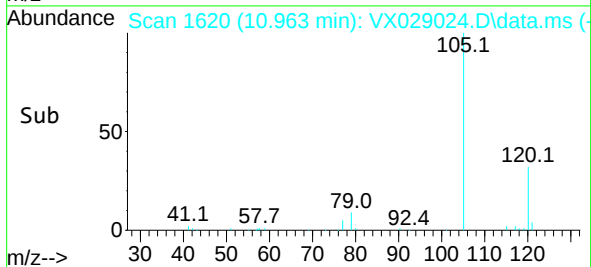

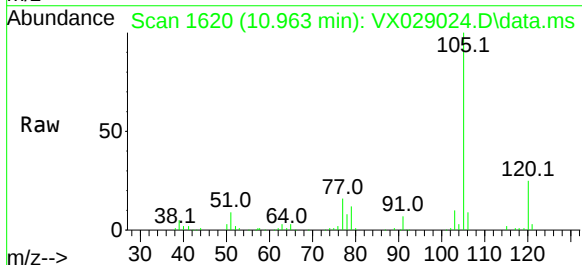




#76
1,2,3-Trichloropropane
Concen: 20.917 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13




Instrument :
MSVOA_X
ClientSampleId :
MW-39


Tgt Ion: 75 Resp: 145587
Ion Ratio Lower Upper
75 100
77 1.2 19.4 58.2#

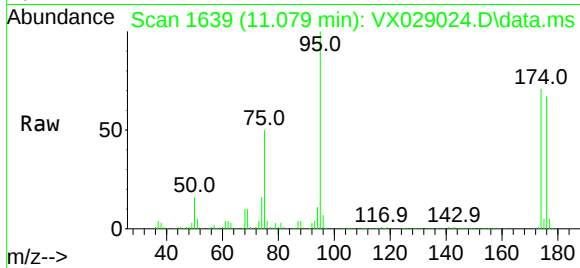

#78
n-propylbenzene
Concen: 3.962 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.001 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13

Tgt Ion: 91 Resp: 103305
Ion Ratio Lower Upper
91 100
120 23.7 11.6 34.8

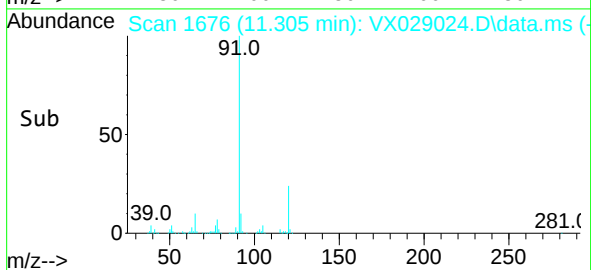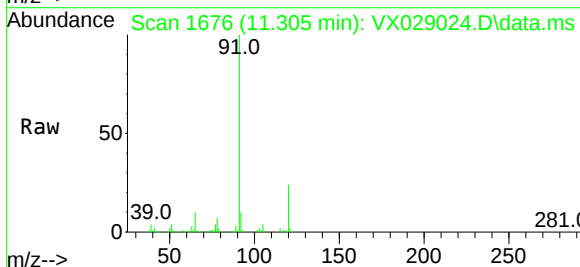



#79

2-Chlorotoluene

Concen: 2.956 ug/l

RT: 11.378 min Scan# 1

Delta R.T. 0.013 min

Lab File: VX029024.D

Acq: 27 May 2022 15:13

Instrument :

MSVOA_X

ClientSampleId :





MW-39

Tgt Ion: 91 Resp: 47226

Ion Ratio Lower Upper

91 100

126 0.2 17.3 51.9#

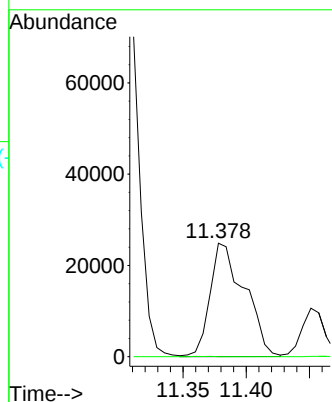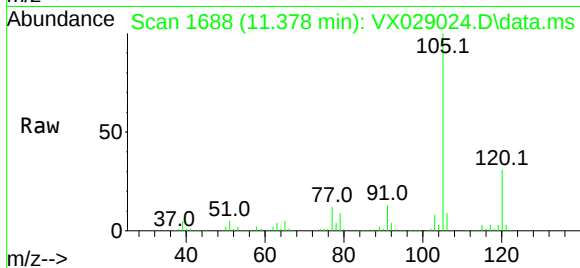

#80

1,3,5-Trimethylbenzene

Concen: 6.592 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX029024.D




Acq: 27 May 2022 15:13


Tgt Ion:105 Resp: 123803

Ion Ratio Lower Upper

105 100

120 48.4 24.3 72.9




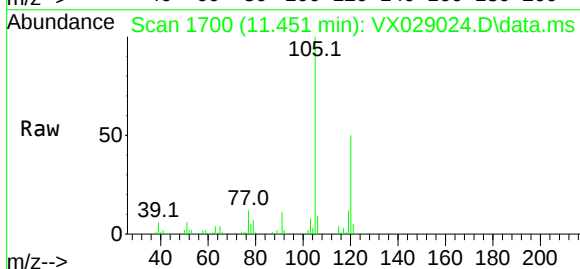




#81
trans-1,4-Dichloro-2-butene
Concen: 61.441 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13




Instrument :
MSVOA_X
ClientSampleId :
MW-39


Tgt Ion: 75 Resp: 145587
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#

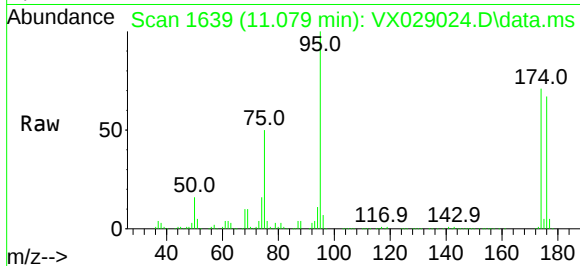

#82
4-Chlorotoluene
Concen: 0.719 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13

Tgt Ion: 91 Resp: 13287
Ion Ratio Lower Upper
91 100
126 0.7 14.9 44.5#


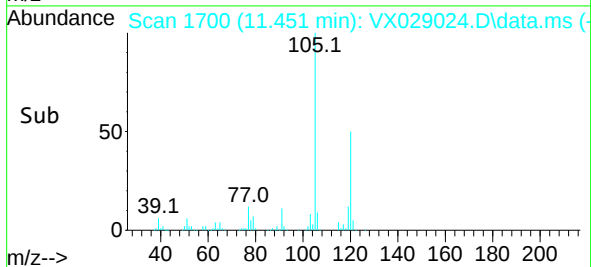

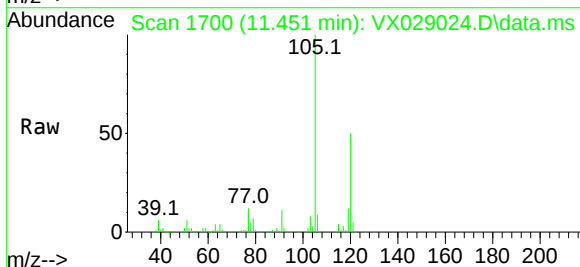




#83
tert-Butylbenzene
Concen: 3.642 ug/l
RT: 11.756 min Scan# 11
Delta R.T. 0.037 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13




Instrument :
MSVOA_X
ClientSampleId :
MW-39


Tgt Ion:119 Resp: 66226
Ion Ratio Lower Upper
119 100
91 87.3 26.9 80.6#
134 0.0 11.4 34.2#

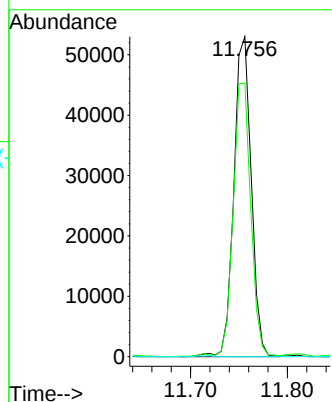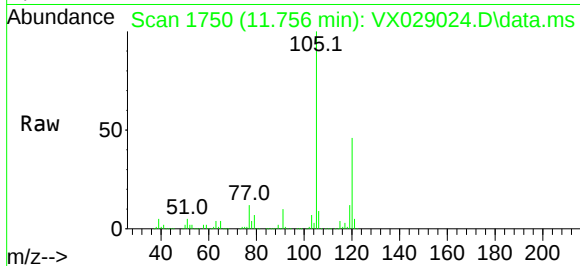

#84
1,2,4-Trimethylbenzene
Concen: 28.894 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13

Tgt Ion:105 Resp: 544144
Ion Ratio Lower Upper
105 100
120 45.6 22.6 67.8


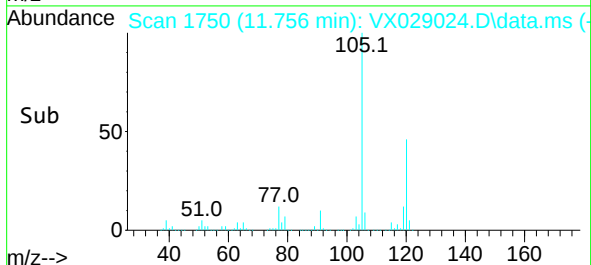

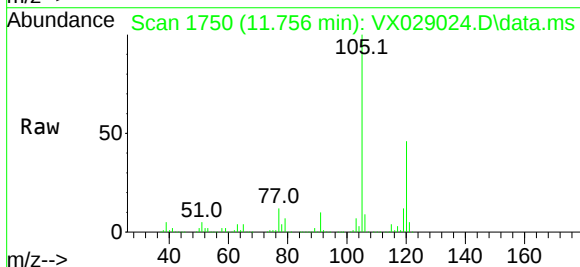




#85
 sec-Butylbenzene
 Concen: 24.261 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. -0.134 min
 Lab File: VX029024.D
 Acq: 27 May 2022 15:13




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-39


Tgt Ion:105 Resp: 544144
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.2 30.4#

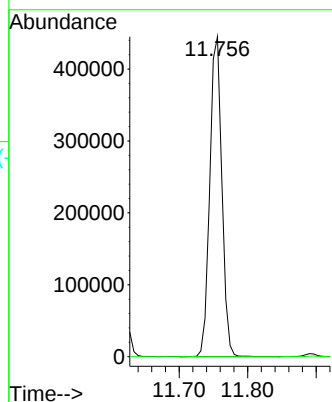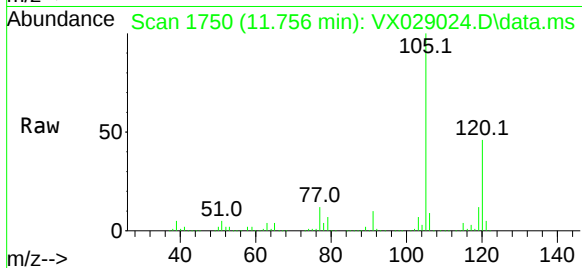

#86
 p-Isopropyltoluene
 Concen: 0.352 ug/l
 RT: 11.975 min Scan# 1786
 Delta R.T. -0.037 min
 Lab File: VX029024.D
 Acq: 27 May 2022 15:13

Tgt Ion:119 Resp: 6619
 Ion Ratio Lower Upper
 119 100
 134 28.2 13.0 39.0
 91 26.0 11.3 33.9

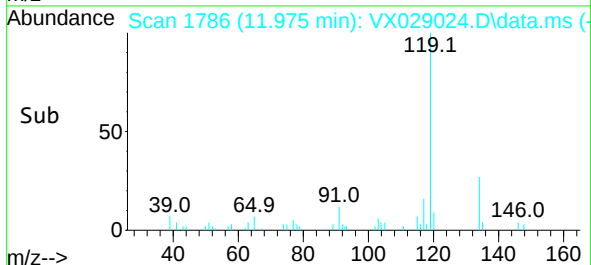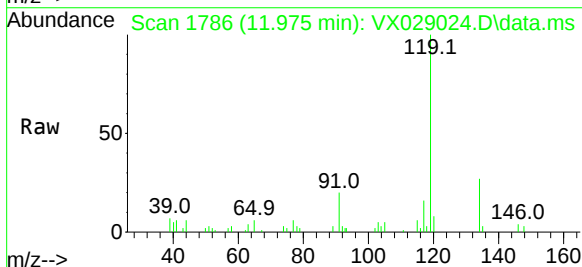



#89

n-Butylbenzene

Concen: 0.539 ug/l

RT: 12.323 min Scan# 1843

Delta R.T. -0.012 min

Lab File: VX029024.D

Acq: 27 May 2022 15:13

Instrument :

MSVOA_X

ClientSampleId :

MW-39





Tgt Ion: 91 Resp: 8796

Ion Ratio Lower Upper

91 100

92 28.1 27.8 83.3

134 114.3 13.3 39.8#

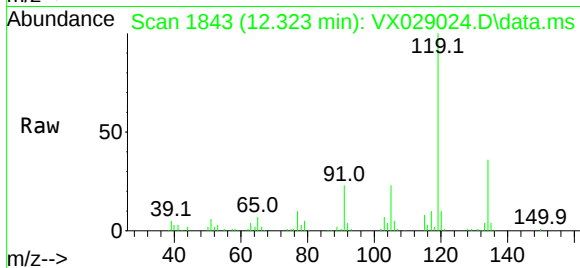

#90

Hexachloroethane

Concen: 2.037 ug/l

RT: 12.646 min Scan# 1896

Delta R.T. 0.104 min

Lab File: VX029024.D




Acq: 27 May 2022 15:13


Tgt Ion: 117 Resp: 6199

Ion Ratio Lower Upper

117 100

201 0.0 39.5 118.5#

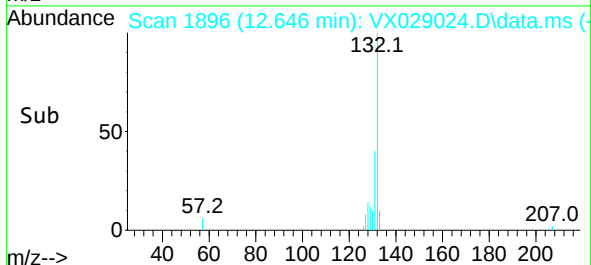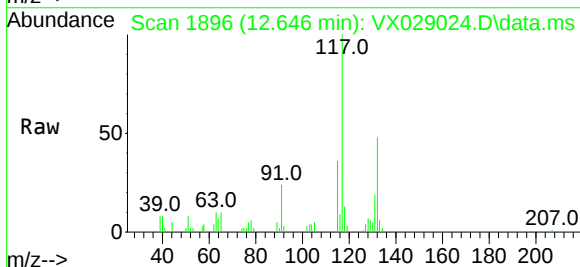



#95
Naphthalene
Concen: 11.364 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX029024.D
Acq: 27 May 2022 15:13

Instrument :
MSVOA_X
ClientSampleId :
MW-39

Tgt Ion:128 Resp: 240007
Ion Ratio Lower Upper
128 100
127 12.9 10.2 15.4
129 11.0 8.7 13.1

