

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
 Data File : VX029030.D
 Acq On : 27 May 2022 17:34
 Operator : JC/MD
 Sample : N2968-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-31

Quant Time: May 27 22:10:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 12 14:58:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	335213	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	595520	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	579026	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	277755	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	216831	47.189	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	94.380%
35) Dibromofluoromethane	5.391	113	195572	50.124	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	100.240%
50) Toluene-d8	8.653	98	708443	48.159	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	96.320%
62) 4-Bromofluorobenzene	11.085	95	282551	51.425	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	102.860%
Target Compounds						
					Qvalue	
5) Bromomethane	1.611	94	1072	Below Cal		89
6) Chloroethane	1.636	64	423	Below Cal	#	59
11) Tert butyl alcohol	2.959	59	80771	77.318	ug/l	100
15) Acrylonitrile	3.117	53	7199	3.252	ug/l	# 30
16) Acetone	2.386	43	4040	2.049	ug/l	# 87
19) Methyl tert-butyl Ether	3.117	73	700222	56.876	ug/l	99
22) Diisopropyl ether	3.763	45	23278	1.958	ug/l	# 86
23) Vinyl Acetate	3.757	43	12284	1.198	ug/l	# 66
25) 2-Butanone	4.574	43	1135	0.367	ug/l	# 80
31) Cyclohexane	5.477	56	9078	1.423	ug/l	# 90
36) 1,1-Dichloropropene	5.556	75	25584	4.366	ug/l	# 49
38) Carbon Tetrachloride	5.550	117	35321	5.989	ug/l	# 15
39) Methylcyclohexane	7.379	83	4979	0.741	ug/l	91
40) Benzene	6.044	78	216154	12.834	ug/l	99
42) 1,2-Dichloroethane	6.050	62	2362	0.380	ug/l	# 73
51) 4-Methyl-2-Pentanone	8.580	43	1422	0.225	ug/l	# 80
52) Toluene	8.720	92	5821	0.537	ug/l	94
53) t-1,3-Dichloropropene	8.726	75	29	1.645	ug/l	# 43
67) Ethyl Benzene	10.195	91	50527	2.295	ug/l	100
68) m/p-Xylenes	10.305	106	26017	3.035	ug/l	99
69) o-Xylene	10.646	106	6533	0.774	ug/l	95
73) Isopropylbenzene	10.963	105	51397	2.440	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	139965	21.517	ug/l	# 38
78) n-propylbenzene	11.305	91	51790	2.126	ug/l	99
79) 2-Chlorotoluene	11.305	91	51790	3.468	ug/l	# 40
80) 1,3,5-Trimethylbenzene	11.451	105	5797	0.330	ug/l	96
81) trans-1,4-Dichloro-2-b...	11.079	75	139965	63.093	ug/l	# 15
82) 4-Chlorotoluene	11.305	91	51790	3.000	ug/l	# 45
84) 1,2,4-Trimethylbenzene	11.756	105	15787	0.897	ug/l	96
85) sec-Butylbenzene	11.896	105	6443	0.307	ug/l	# 67
89) n-Butylbenzene	12.335	91	3119	0.205	ug/l	# 51
90) Hexachloroethane	12.646	117	8488	2.984	ug/l	# 10
95) Naphthalene	13.780	128	34811	1.764	ug/l	# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
MW-31

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029030.D
Acq On : 27 May 2022 17:34
Operator : JC/MD
Sample : N2968-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-31

Quant Time: May 27 22:10:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260
QLast Update : Thu May 12 14:58:53 2022
Response via : Initial Calibration




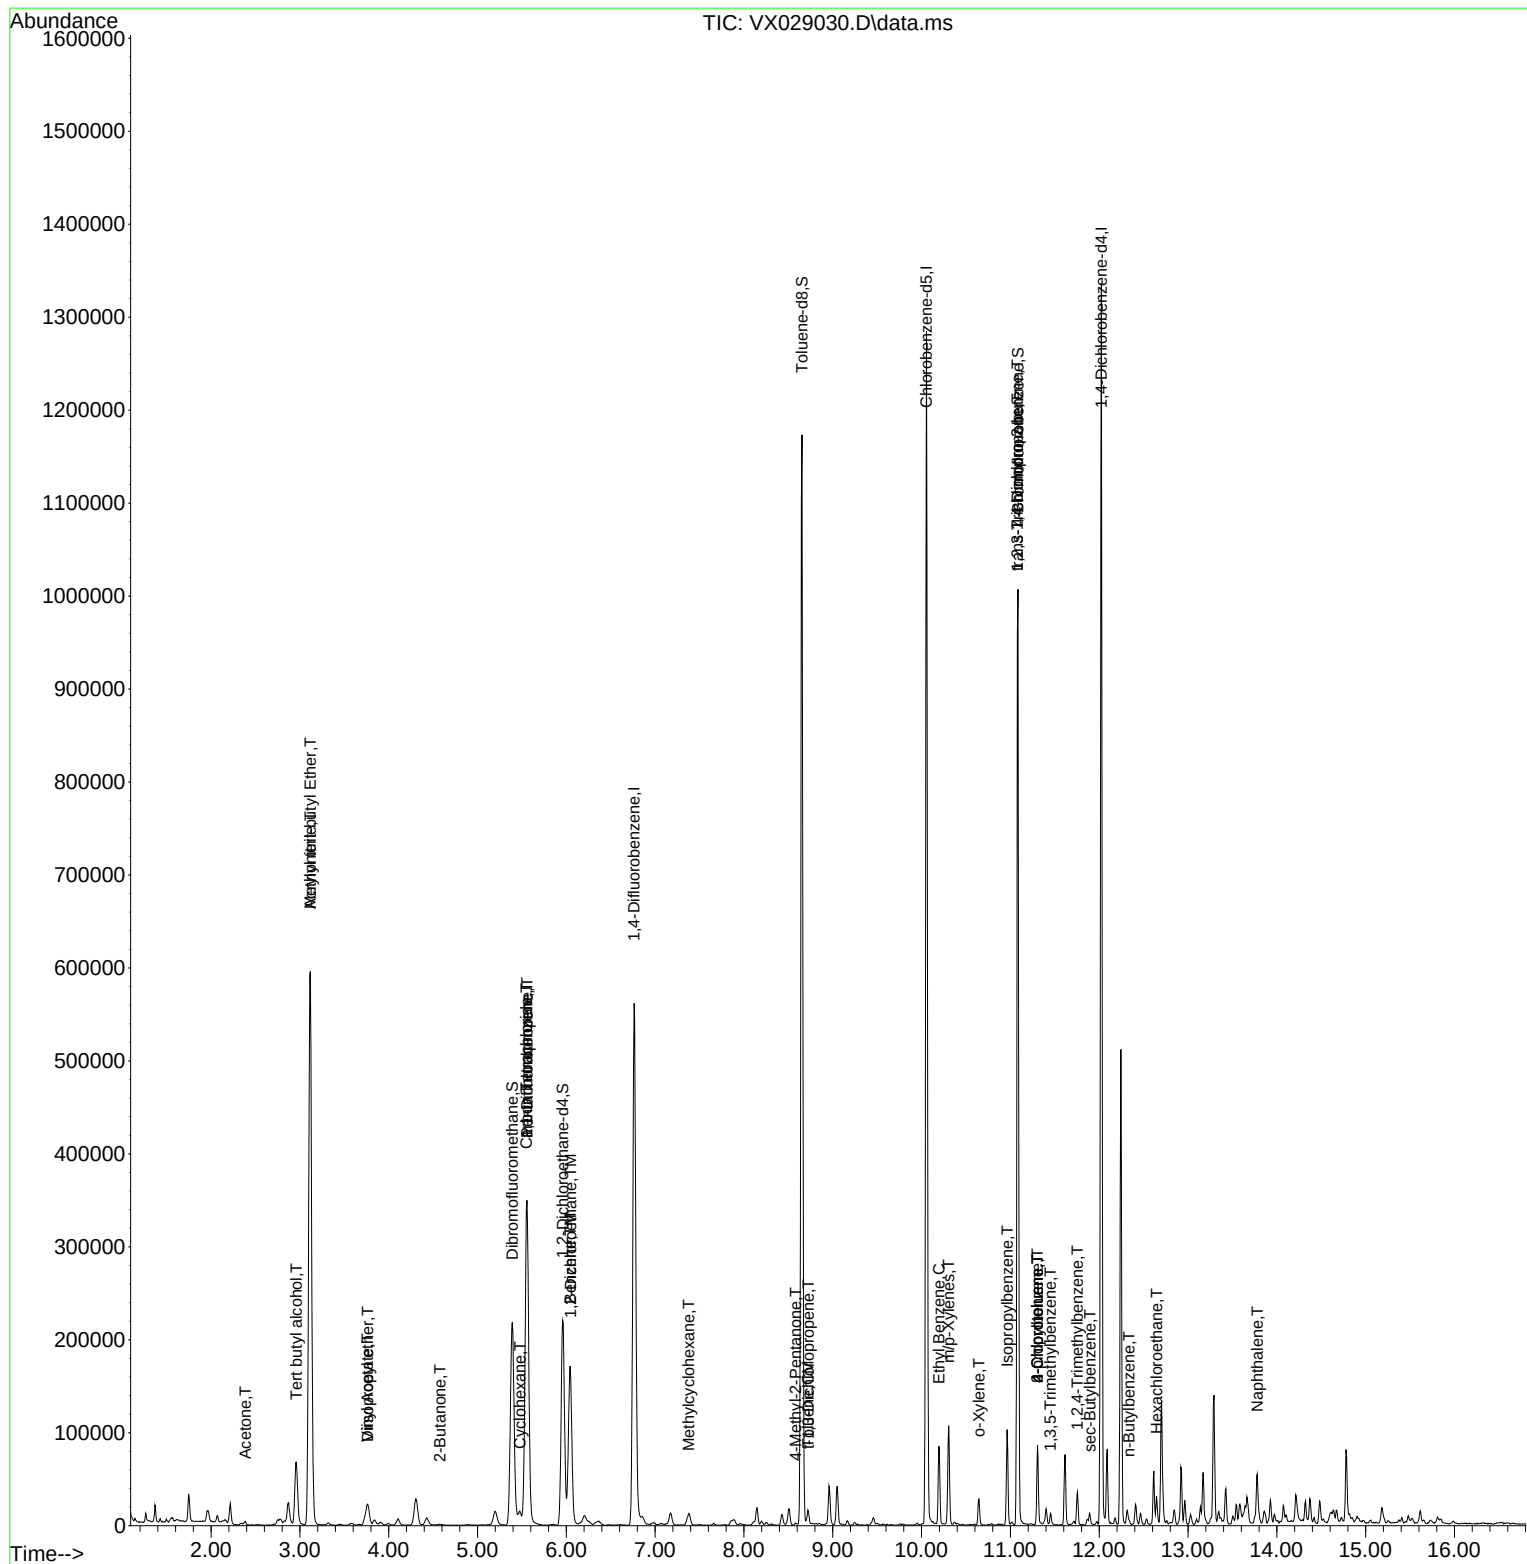


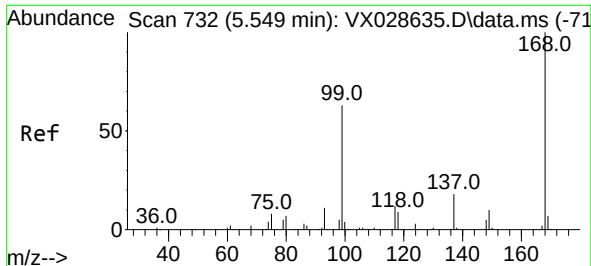

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.007 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34




Instrument :
MSVOA_X
ClientSampleId :
MW-31


Tgt Ion:168 Resp: 335213
Ion Ratio Lower Upper
168 100
99 60.3 41.7 62.5



#5
Bromomethane
Concen: Below Cal
RT: 1.611 min Scan# 86
Delta R.T. 0.012 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34

Tgt Ion: 94 Resp: 1072
Ion Ratio Lower Upper
94 100
96 104.9 75.3 112.9




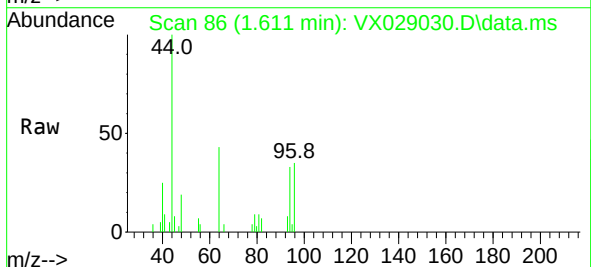


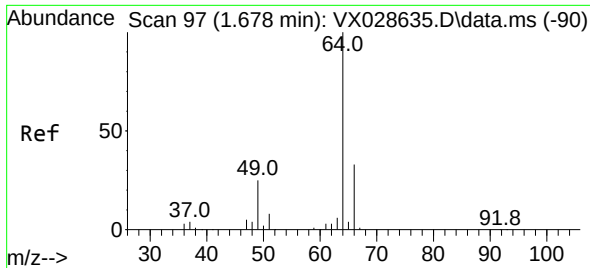

#6
Chloroethane
Concen: Below Cal
RT: 1.636 min Scan# 90
Delta R.T. -0.042 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34




Instrument :
MSVOA_X
ClientSampleId :
MW-31


Tgt Ion: 64 Resp: 423
Ion Ratio Lower Upper
64 100
66 8.8 25.3 37.9#

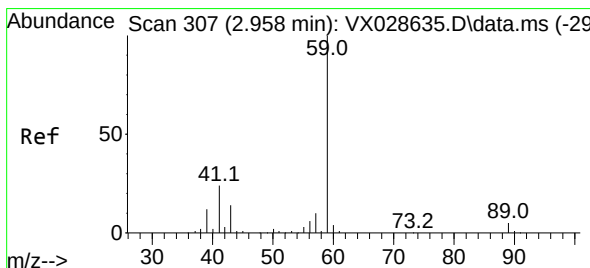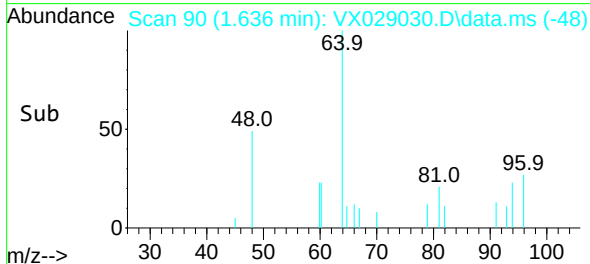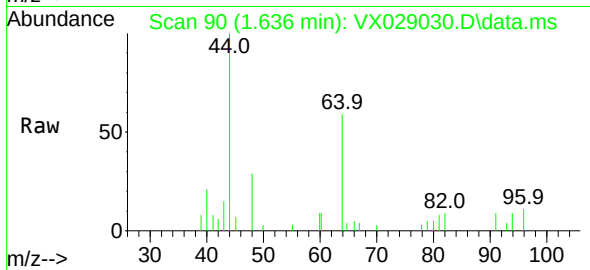

#11
Tert butyl alcohol
Concen: 77.318 ug/l
RT: 2.959 min Scan# 307
Delta R.T. 0.001 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34

Tgt Ion: 59 Resp: 80771
Ion Ratio Lower Upper
59 100
57 10.3 8.3 12.5


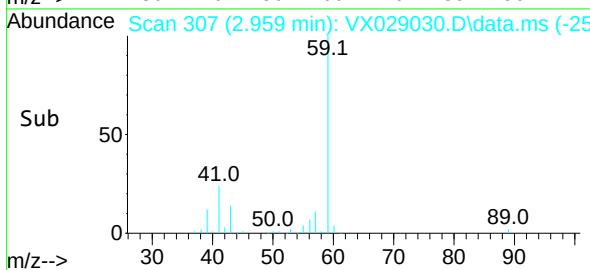

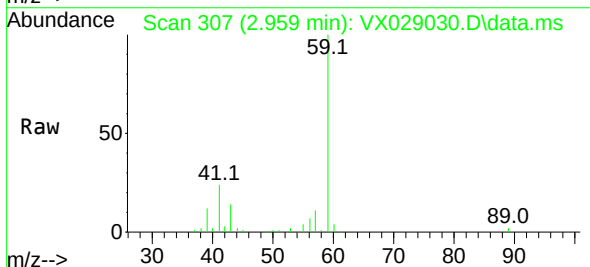


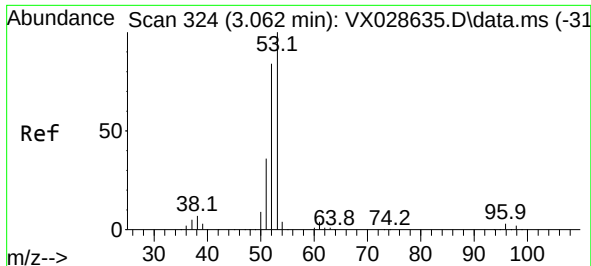

#15
Acrylonitrile
Concen: 3.252 ug/l
RT: 3.117 min Scan# 31
Delta R.T. 0.055 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34




Instrument :
MSVOA_X
ClientSampleId :
MW-31


Tgt Ion: 53 Resp: 7199
Ion Ratio Lower Upper
53 100
52 19.7 65.7 98.5#
51 76.5 28.4 42.6#

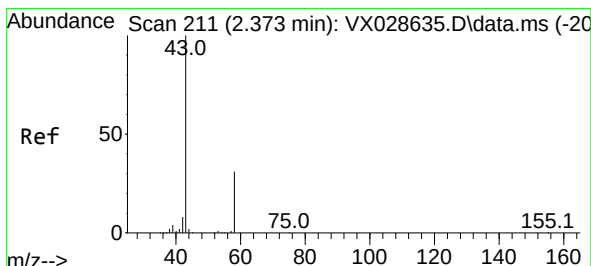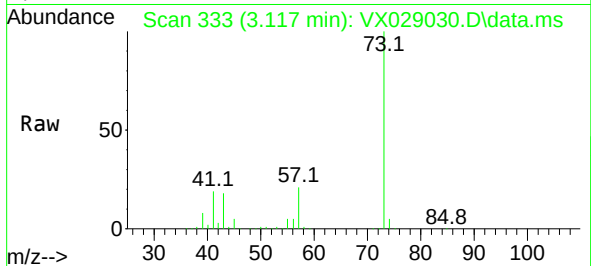

#16
Acetone
Concen: 2.049 ug/l
RT: 2.386 min Scan# 213
Delta R.T. 0.013 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34

Tgt Ion: 43 Resp: 4040
Ion Ratio Lower Upper
43 100
58 28.5 28.8 43.2#


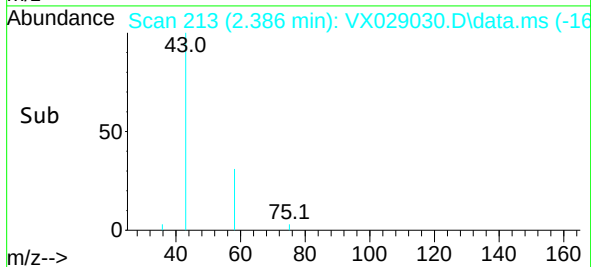

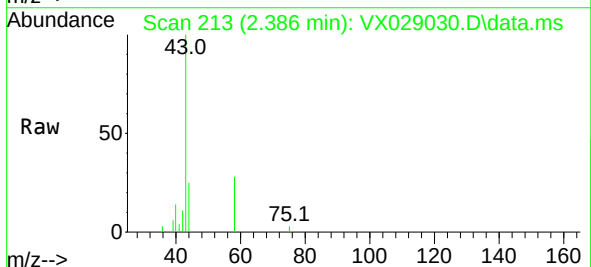




#19
Methyl tert-butyl Ether
Concen: 56.876 ug/l
RT: 3.117 min Scan# 311
Delta R.T. 0.006 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34




Instrument :
MSVOA_X
ClientSampleId :
MW-31


Tgt Ion: 73 Resp: 700222
Ion Ratio Lower Upper
73 100
57 21.4 16.8 25.2

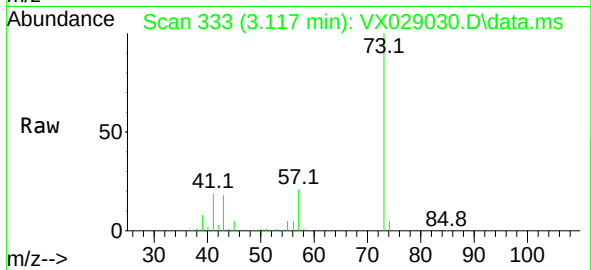

#22
Diisopropyl ether
Concen: 1.958 ug/l
RT: 3.763 min Scan# 439
Delta R.T. 0.006 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34

Tgt Ion: 45 Resp: 23278
Ion Ratio Lower Upper
45 100
43 46.8 50.8 76.2#
87 29.7 26.6 39.8
59 12.7 10.5 15.7


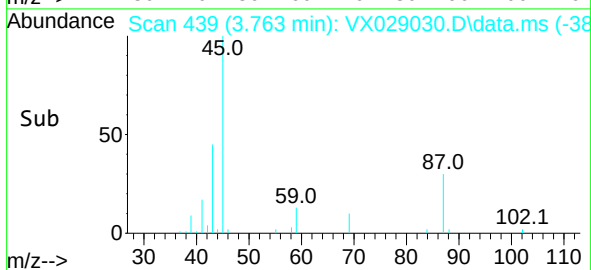

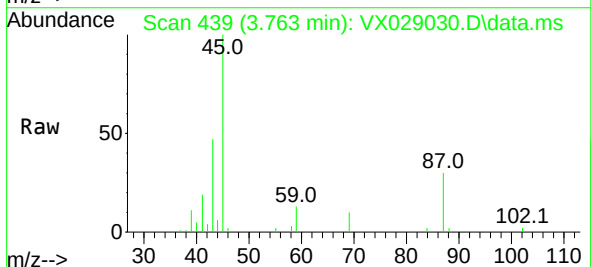


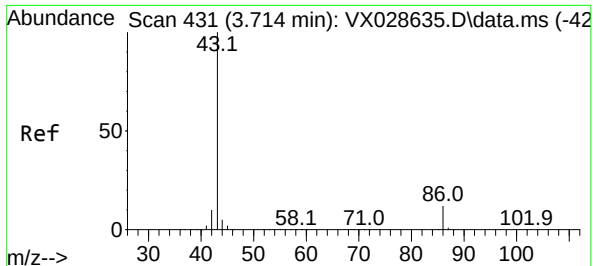

#23
 Vinyl Acetate
 Concen: 1.198 ug/l
 RT: 3.757 min Scan# 41
 Delta R.T. 0.043 min
 Lab File: VX029030.D
 Acq: 27 May 2022 17:34




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-31


Tgt Ion: 43 Resp: 12284
 Ion Ratio Lower Upper
 43 100
 86 0.0 10.8 16.2#

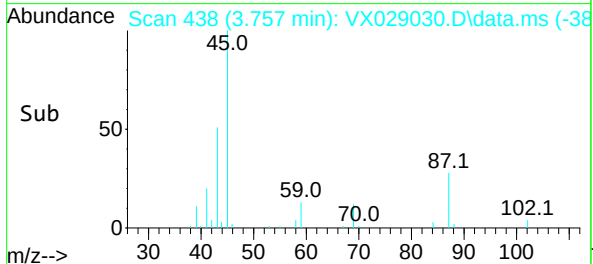

#25
 2-Butanone
 Concen: 0.367 ug/l
 RT: 4.574 min Scan# 572
 Delta R.T. 0.024 min
 Lab File: VX029030.D
 Acq: 27 May 2022 17:34

Tgt Ion: 43 Resp: 1135
 Ion Ratio Lower Upper
 43 100
 72 19.5 24.4 36.6#


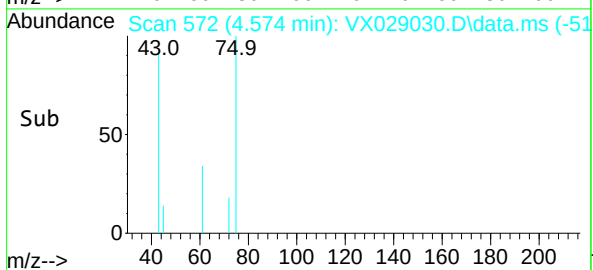

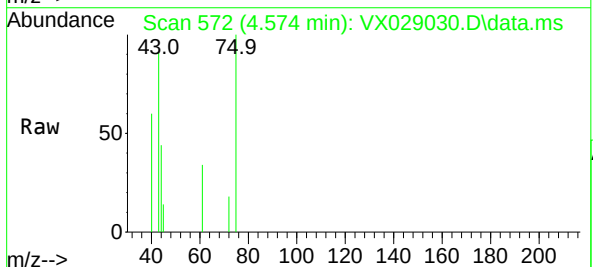


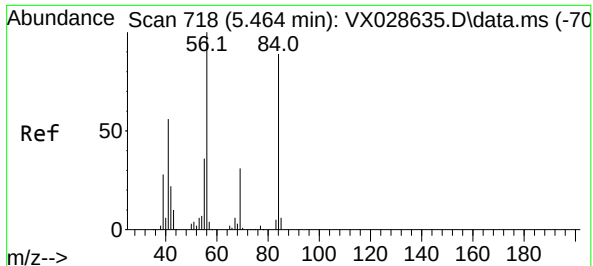

#31
Cyclohexane
Concen: 1.423 ug/l
RT: 5.477 min Scan# 718
Delta R.T. 0.013 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34




Instrument :
MSVOA_X
ClientSampleId :
MW-31


Tgt Ion: 56 Resp: 9078
Ion Ratio Lower Upper
56 100
69 20.3 26.7 40.1#
84 91.4 77.2 115.8

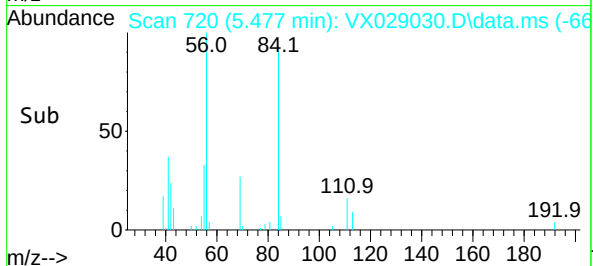

#33
1,2-Dichloroethane-d4
Concen: 47.189 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34

Tgt Ion: 65 Resp: 216831
Ion Ratio Lower Upper
65 100
67 52.1 0.0 107.4


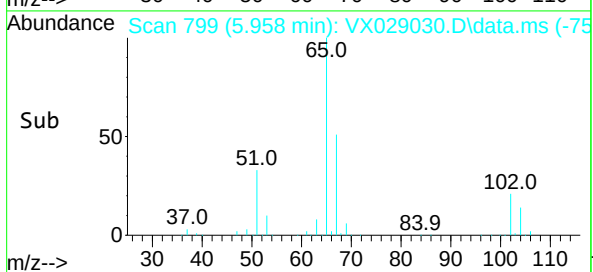

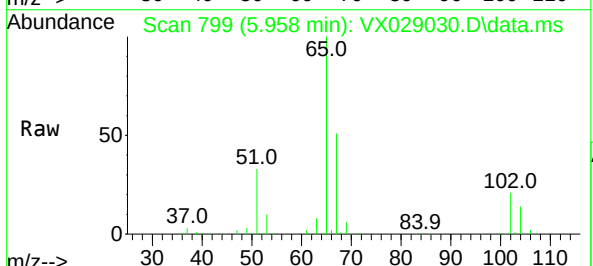


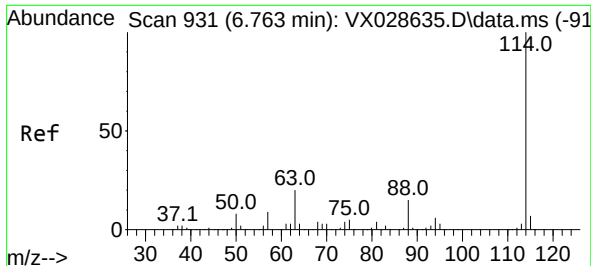

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34




Instrument :
MSVOA_X
ClientSampleId :
MW-31


Tgt Ion:114 Resp: 595520
Ion Ratio Lower Upper
114 100
63 19.1 0.0 36.8
88 16.5 0.0 32.4

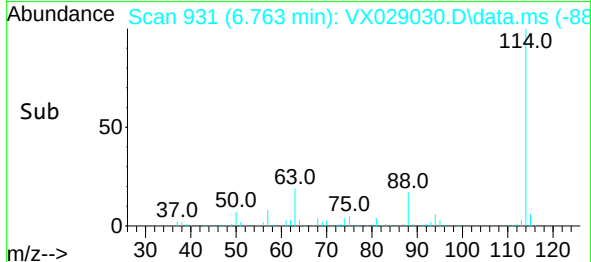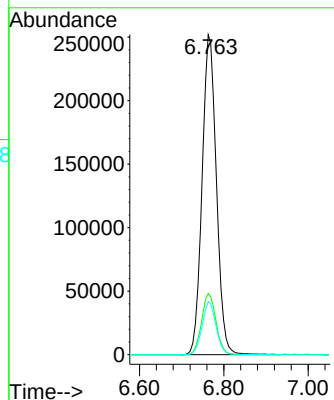

#35
Dibromofluoromethane
Concen: 50.124 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34

Tgt Ion:113 Resp: 195572
Ion Ratio Lower Upper
113 100
111 102.1 82.8 124.2
192 19.5 16.9 25.3


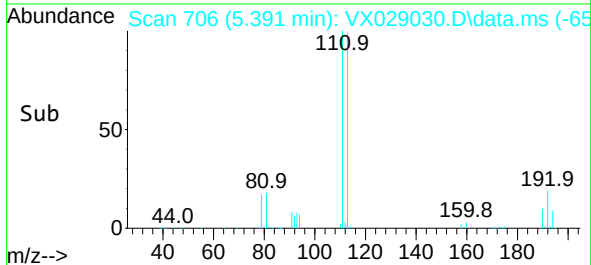
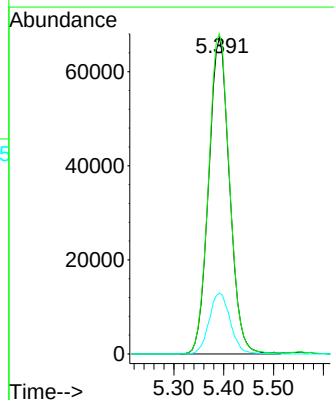
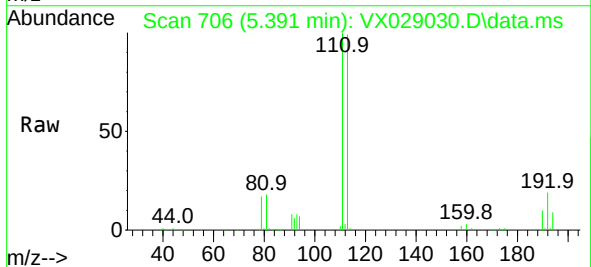


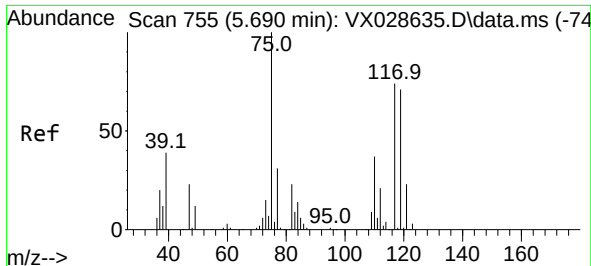

#36
1,1-Dichloropropene
Concen: 4.366 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34




Instrument :
MSVOA_X
ClientSampleId :
MW-31


Tgt Ion: 75 Resp: 25584
Ion Ratio Lower Upper
75 100
110 9.4 18.3 54.8#
77 0.0 24.8 37.2#

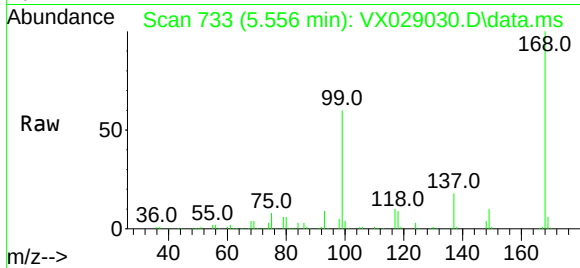

#38
Carbon Tetrachloride
Concen: 5.989 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.127 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34

Tgt Ion: 117 Resp: 35321
Ion Ratio Lower Upper
117 100
119 4.1 77.3 115.9#
121 0.0 24.2 36.2#




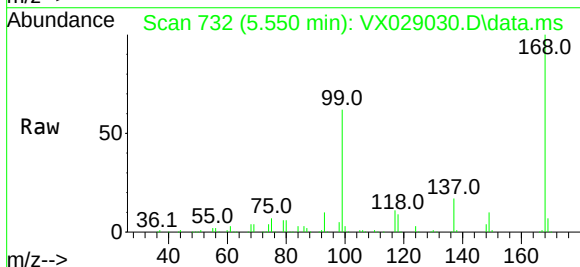




#39
Methylcyclohexane
Concen: 0.741 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. 0.001 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34




Instrument :
MSVOA_X
ClientSampleId :
MW-31


Tgt Ion: 83 Resp: 4979
Ion Ratio Lower Upper
83 100
55 79.5 54.6 81.8
98 45.9 37.4 56.2

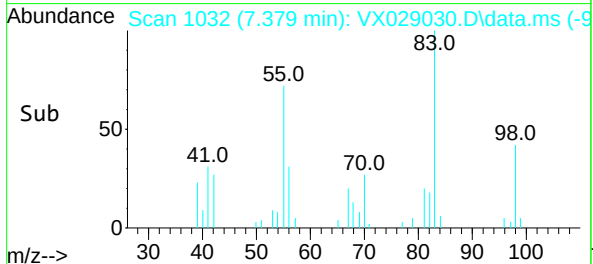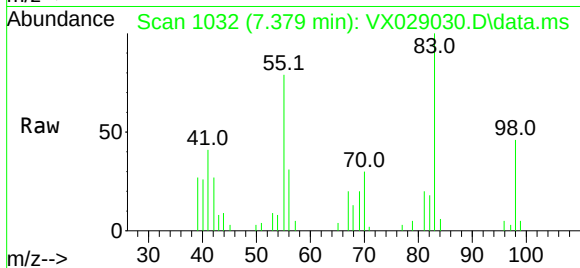

#40
Benzene
Concen: 12.834 ug/l
RT: 6.044 min Scan# 813
Delta R.T. 0.007 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34

Tgt Ion: 78 Resp: 216154
Ion Ratio Lower Upper
78 100
77 23.7 19.3 28.9

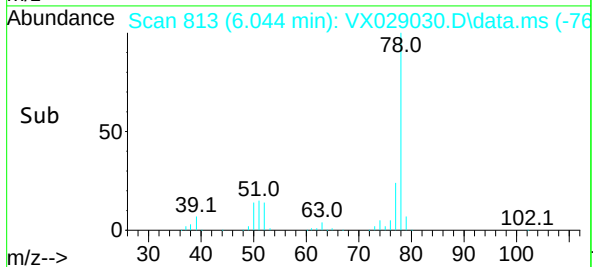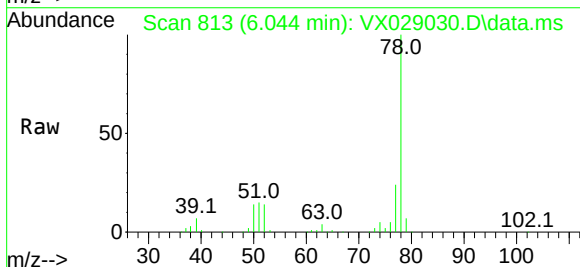

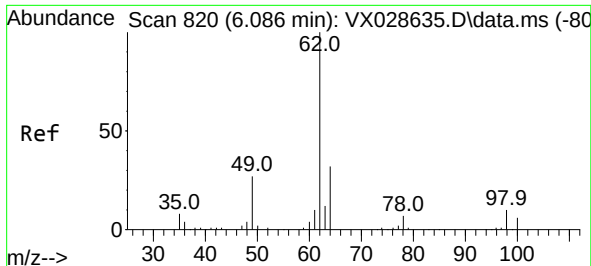

#42

1,2-Dichloroethane

Concen: 0.380 ug/l

RT: 6.050 min Scan# 81

Delta R.T. -0.036 min

Lab File: VX029030.D

Acq: 27 May 2022 17:34

Instrument :

MSVOA_X

ClientSampleId :





MW-31

Tgt Ion: 62 Resp: 2362

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.4

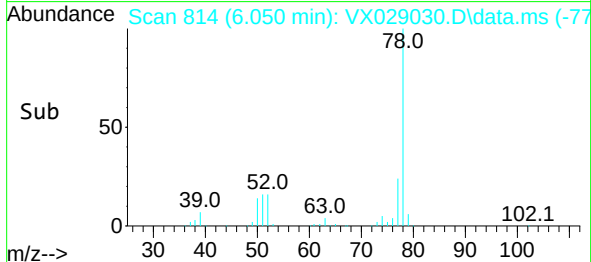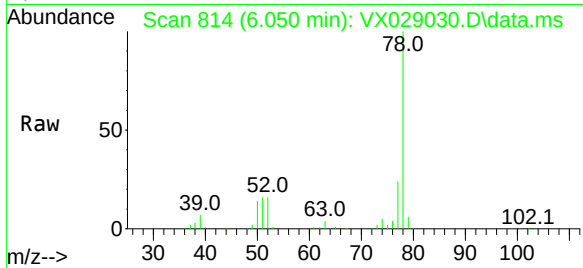

#50

Toluene-d8

Concen: 48.159 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. 0.007 min

Lab File: VX029030.D




Acq: 27 May 2022 17:34


Tgt Ion: 98 Resp: 708443

Ion Ratio Lower Upper

98 100

100 66.9 52.6 78.8


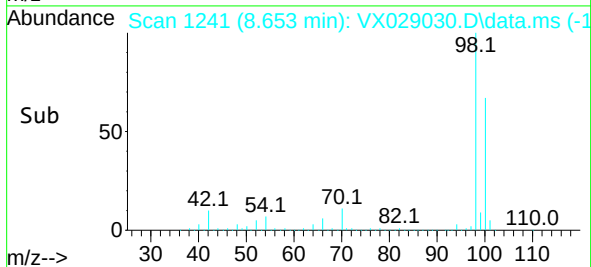

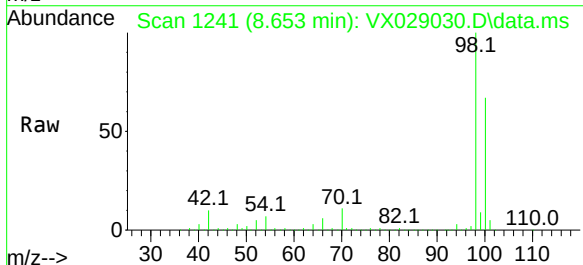


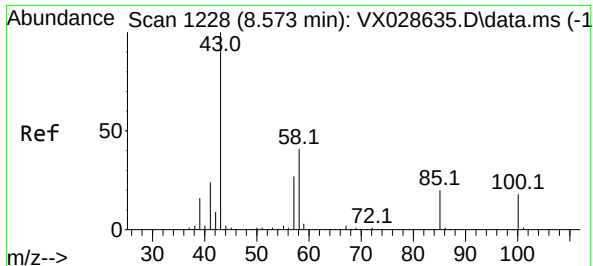

#51
4-Methyl-2-Pentanone
Concen: 0.225 ug/l
RT: 8.580 min Scan# 11
Delta R.T. 0.007 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34




Instrument :
MSVOA_X
ClientSampleId :
MW-31


Tgt Ion: 43 Resp: 1422
Ion Ratio Lower Upper
43 100
58 31.8 36.1 54.1#

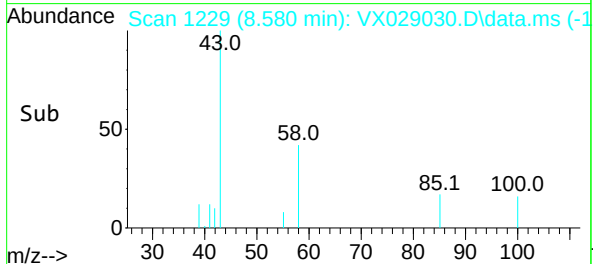

#52
Toluene
Concen: 0.537 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34

Tgt Ion: 92 Resp: 5821
Ion Ratio Lower Upper
92 100
91 163.2 137.5 206.3


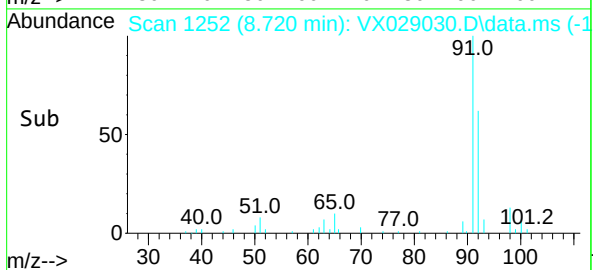

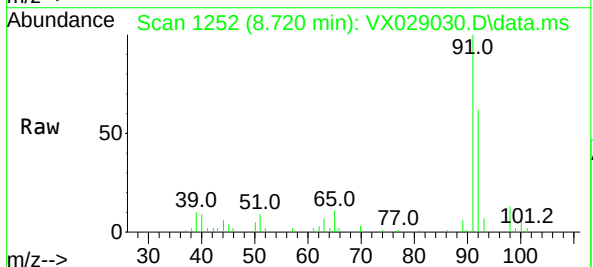




#53
t-1,3-Dichloropropene
Concen: 1.645 ug/l
RT: 8.726 min Scan# 11
Delta R.T. -0.250 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34




Instrument :
MSVOA_X
ClientSampleId :
MW-31


Tgt Ion: 75 Resp: 29
Ion Ratio Lower Upper
75 100
77 0.0 25.4 38.0#

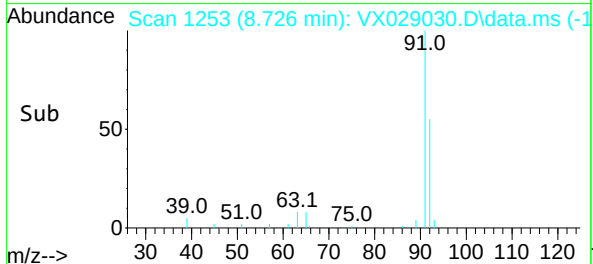

#62
4-Bromofluorobenzene
Concen: 51.425 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34

Tgt Ion: 95 Resp: 282551
Ion Ratio Lower Upper
95 100
174 77.9 0.0 163.0
176 75.0 0.0 155.0


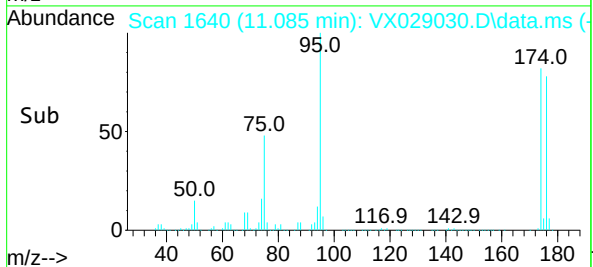

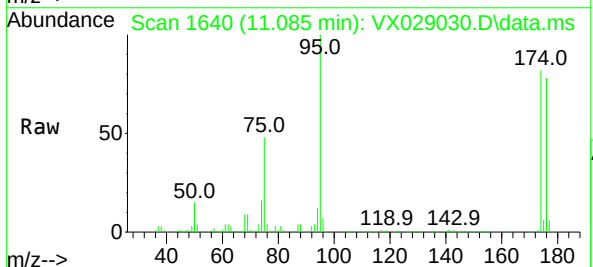




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34




Instrument :
MSVOA_X
ClientSampleId :
MW-31


Tgt Ion:117 Resp: 579026
Ion Ratio Lower Upper
117 100
82 54.5 41.8 62.8
119 31.9 24.8 37.2

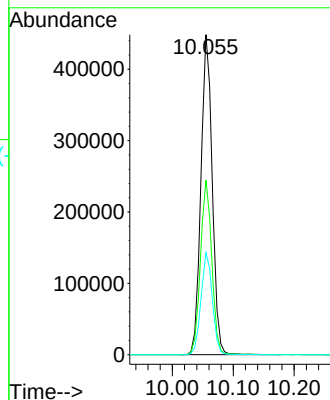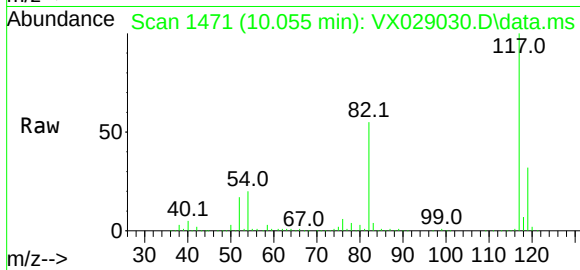

#67
Ethyl Benzene
Concen: 2.295 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34

Tgt Ion: 91 Resp: 50527
Ion Ratio Lower Upper
91 100
106 31.0 24.6 36.8



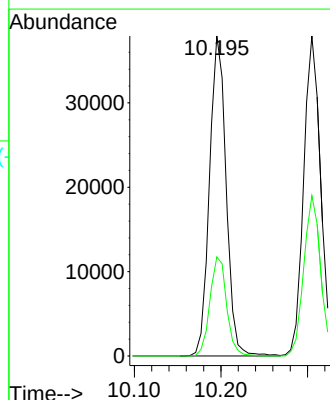
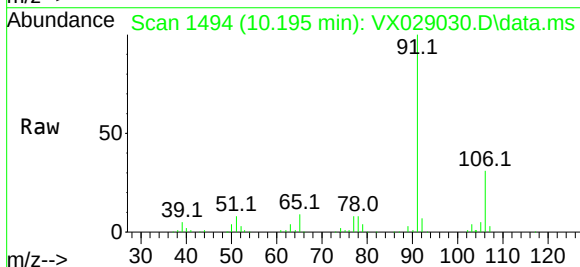




#68
m/p-Xylenes
Concen: 3.035 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34




Instrument :
MSVOA_X
ClientSampleId :
MW-31


Tgt Ion:106 Resp: 26017
Ion Ratio Lower Upper
106 100
91 199.2 160.4 240.6

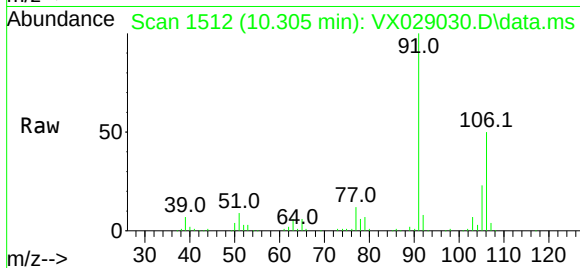

#69
o-Xylene
Concen: 0.774 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34

Tgt Ion:106 Resp: 6533
Ion Ratio Lower Upper
106 100
91 219.4 106.1 318.1


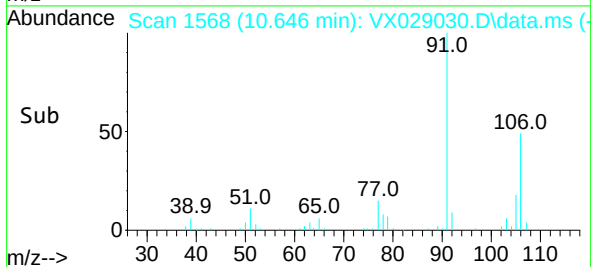

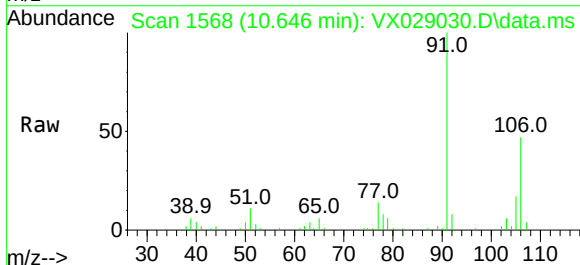




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34




Instrument :
MSVOA_X
ClientSampleId :
MW-31


Tgt Ion:152 Resp: 277755
Ion Ratio Lower Upper
152 100
115 60.9 37.5 112.7
150 156.5 0.0 338.2

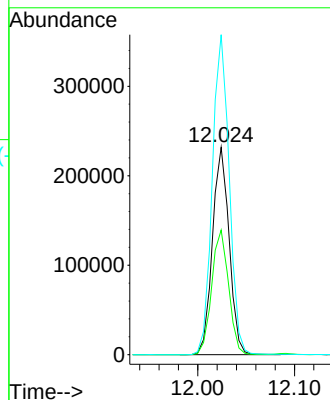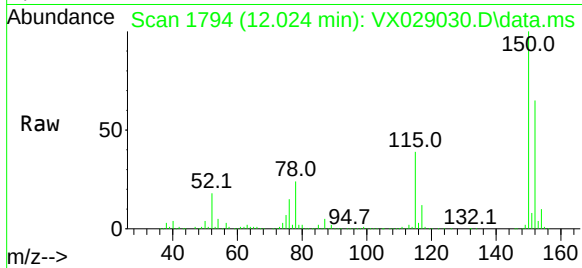

#73
Isopropylbenzene
Concen: 2.440 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34

Tgt Ion:105 Resp: 51397
Ion Ratio Lower Upper
105 100
120 26.4 13.5 40.5


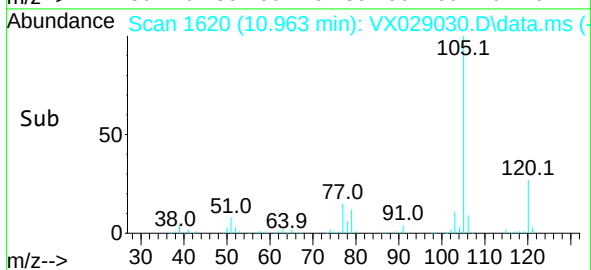
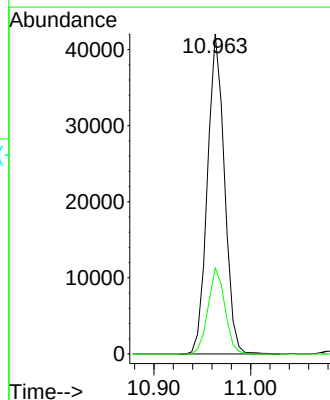
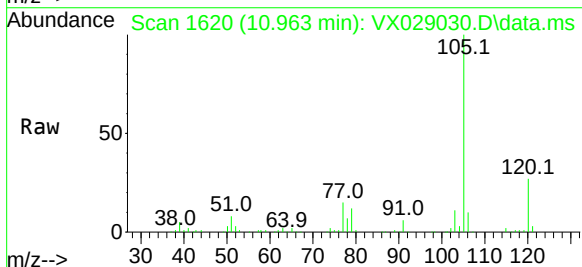




#76
1,2,3-Trichloropropane
Concen: 21.517 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34




Instrument :
MSVOA_X
ClientSampleId :
MW-31


Tgt Ion: 75 Resp: 139965
Ion Ratio Lower Upper
75 100
77 1.1 19.4 58.2#

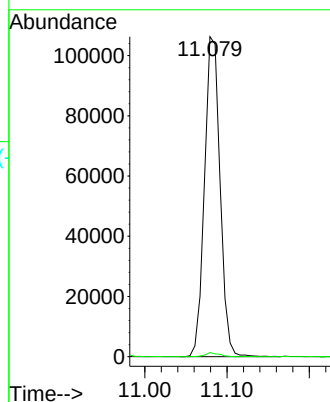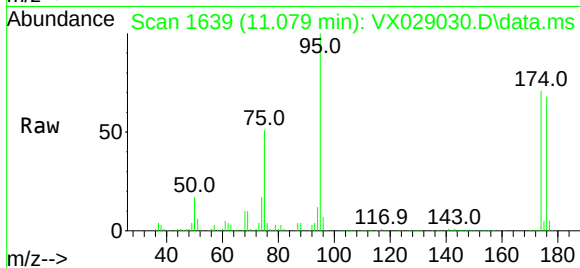

#78
n-propylbenzene
Concen: 2.126 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.001 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34

Tgt Ion: 91 Resp: 51790
Ion Ratio Lower Upper
91 100
120 22.6 11.6 34.8

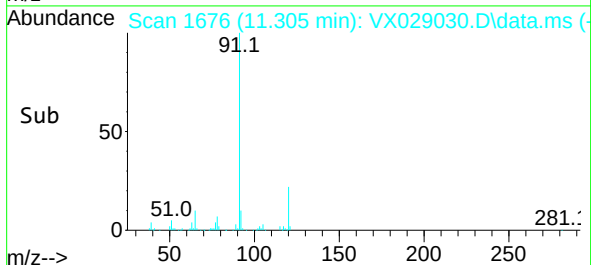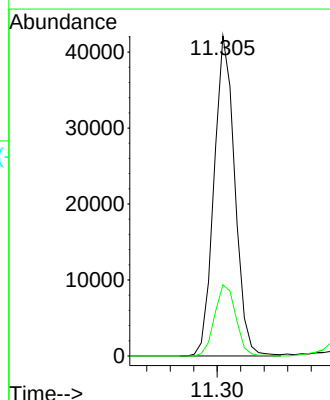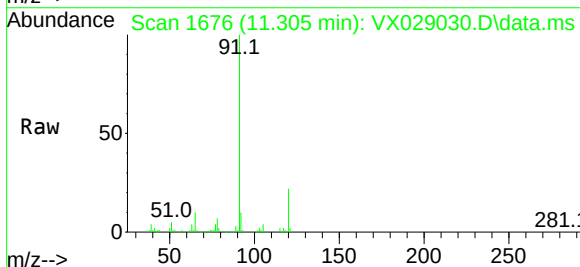



#79

2-Chlorotoluene

Concen: 3.468 ug/l

RT: 11.305 min Scan# 1

Delta R.T. -0.060 min

Lab File: VX029030.D

Acq: 27 May 2022 17:34

Instrument :

MSVOA_X

ClientSampleId :





MW-31

Tgt Ion: 91 Resp: 51790

Ion Ratio Lower Upper

91 100

126 0.0 17.3 51.9#

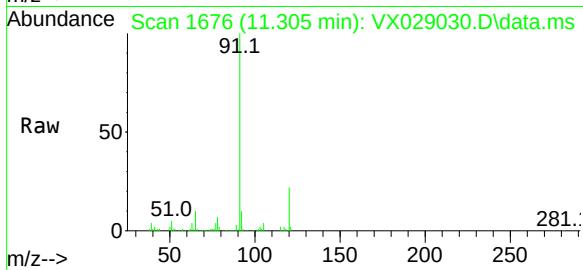

#80

1,3,5-Trimethylbenzene

Concen: 0.330 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX029030.D




Acq: 27 May 2022 17:34


Tgt Ion: 105 Resp: 5797

Ion Ratio Lower Upper

105 100

120 45.7 24.3 72.9


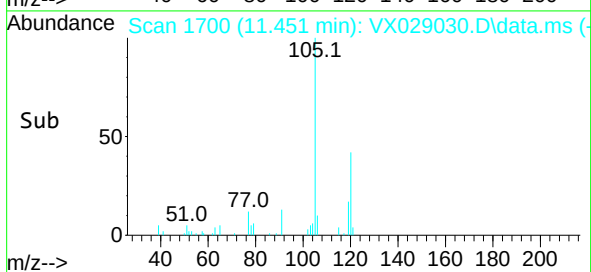

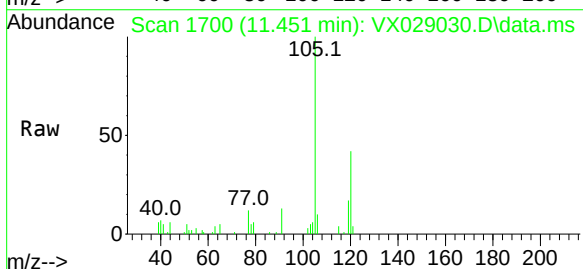




#81
trans-1,4-Dichloro-2-butene
Concen: 63.093 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34




Instrument :
MSVOA_X
ClientSampleId :
MW-31


Tgt Ion: 75 Resp: 139965
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#

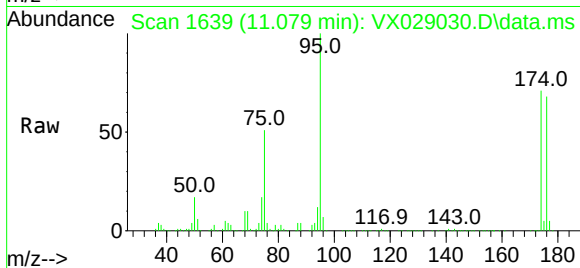

#82
4-Chlorotoluene
Concen: 3.000 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.152 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34

Tgt Ion: 91 Resp: 51790
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#


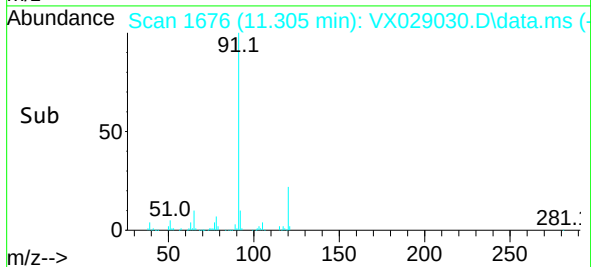

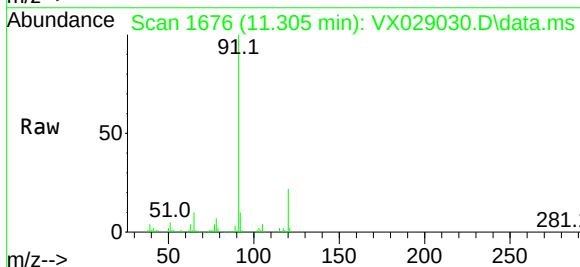


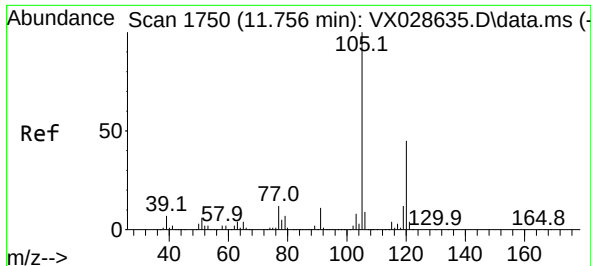

#84
1,2,4-Trimethylbenzene
Concen: 0.897 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34




Instrument :
MSVOA_X
ClientSampleId :
MW-31


Tgt Ion:105 Resp: 15787
Ion Ratio Lower Upper
105 100
120 47.8 22.6 67.8

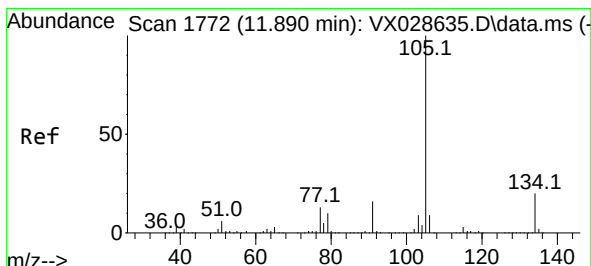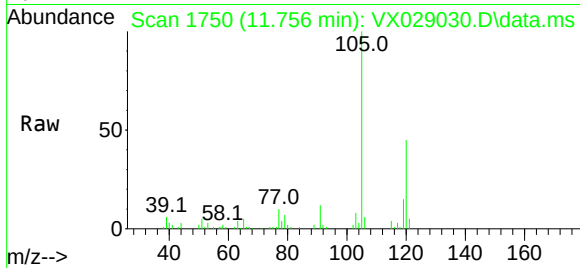

#85
sec-Butylbenzene
Concen: 0.307 ug/l
RT: 11.896 min Scan# 1773
Delta R.T. 0.006 min
Lab File: VX029030.D
Acq: 27 May 2022 17:34

Tgt Ion:105 Resp: 6443
Ion Ratio Lower Upper
105 100
134 35.4 10.2 30.4#

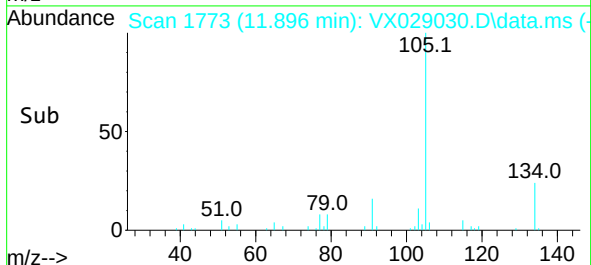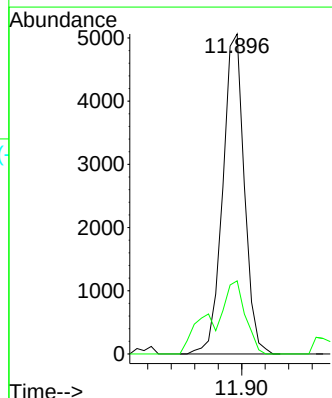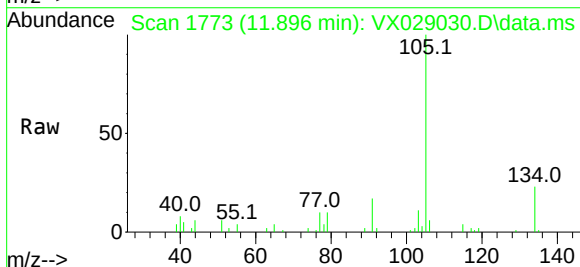



#89

n-Butylbenzene

Concen: 0.205 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. 0.000 min

Lab File: VX029030.D

Acq: 27 May 2022 17:34

Instrument :

MSVOA_X

ClientSampleId :

MW-31





Tgt Ion: 91 Resp: 3119

Ion Ratio Lower Upper

91 100

92 35.2 27.8 83.3

134 75.1 13.3 39.8#

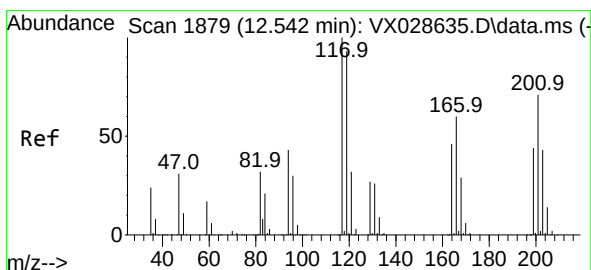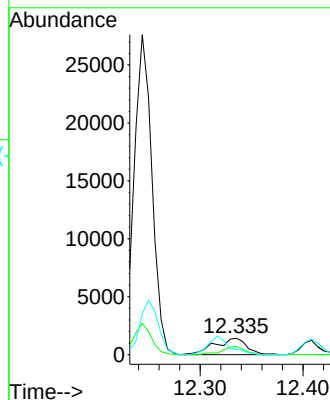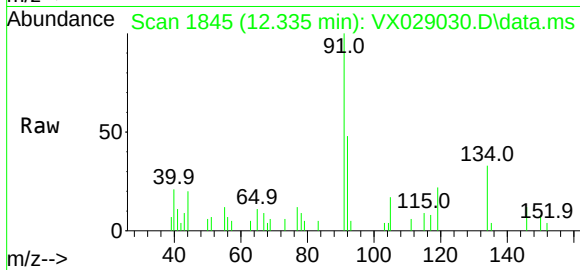

#90

Hexachloroethane

Concen: 2.984 ug/l

RT: 12.646 min Scan# 1896

Delta R.T. 0.104 min

Lab File: VX029030.D




Acq: 27 May 2022 17:34


Tgt Ion: 117 Resp: 8488

Ion Ratio Lower Upper

117 100


201 0.0 39.5 118.5#

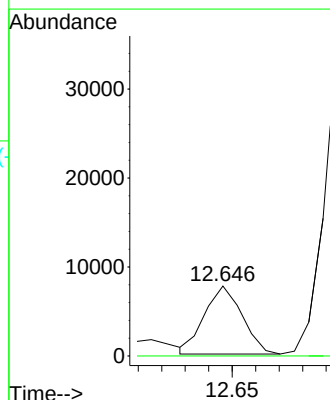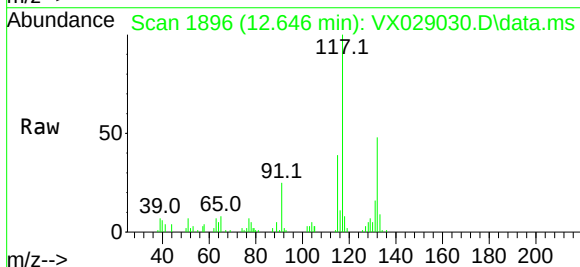



#95
 Naphthalene
 Concen: 1.764 ug/l
 RT: 13.780 min Scan# 2081
 Delta R.T. 0.006 min
 Lab File: VX029030.D
 Acq: 27 May 2022 17:34

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-31

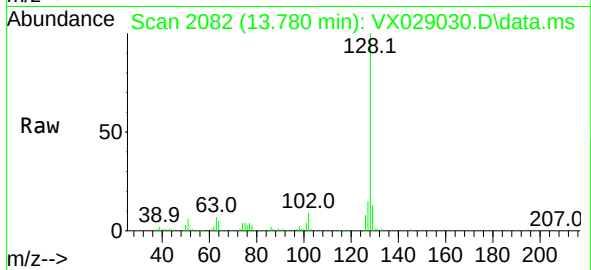

Tgt Ion	Ratio	Lower	Upper
128	100		
127	13.4	10.2	15.4
129	13.8	8.7	13.1

