

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029018.D
Acq On : 27 May 2022 12:19
Operator : JC/MD
Sample : VX0527WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0527WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M

Title : SW846 8260

Signal : TIC: VX029018.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.483	189	229	230	rBV3	114407	697146	36.02%	4.875%
2	2.947	297	305	312	rBV	17357	39151	2.02%	0.274%
3	5.385	693	705	720	rBV2	229608	674379	34.84%	4.716%
4	5.550	720	732	749	rVB	374348	1053945	54.45%	7.370%
5	5.952	788	798	815	rBV	236596	629846	32.54%	4.405%
6	6.757	920	930	949	rBV	599580	1423193	73.53%	9.952%
7	8.647	1233	1240	1250	rBV	1252174	1935515	100.00%	13.535%
8	9.787	1419	1427	1443	rBV	693191	1327303	68.58%	9.282%
9	10.055	1465	1471	1481	rBV	1352918	1767504	91.32%	12.360%
10	11.079	1634	1639	1654	rBV	1073168	1369340	70.75%	9.576%
11	11.463	1696	1702	1719	rVB	1157743	1676959	86.64%	11.727%
12	12.024	1788	1794	1804	rBV	1390123	1705745	88.13%	11.928%




Sum of corrected areas: 14300026

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029018.D
Acq On : 27 May 2022 12:19
Operator : JC/MD
Sample : VX0527WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0527WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

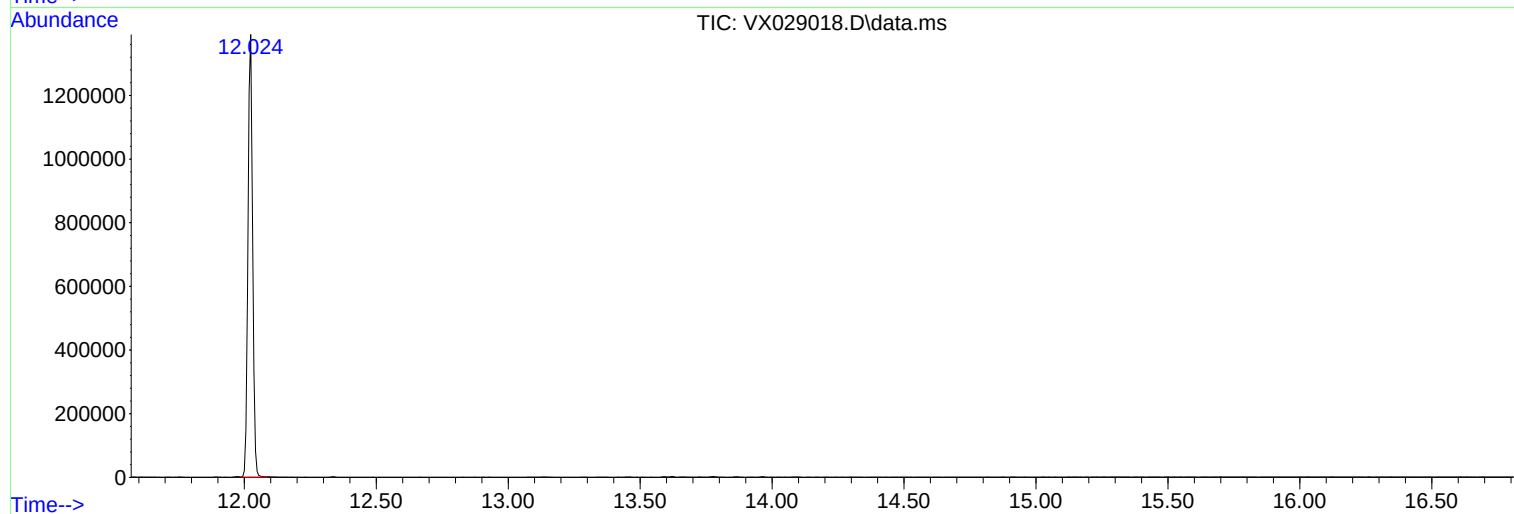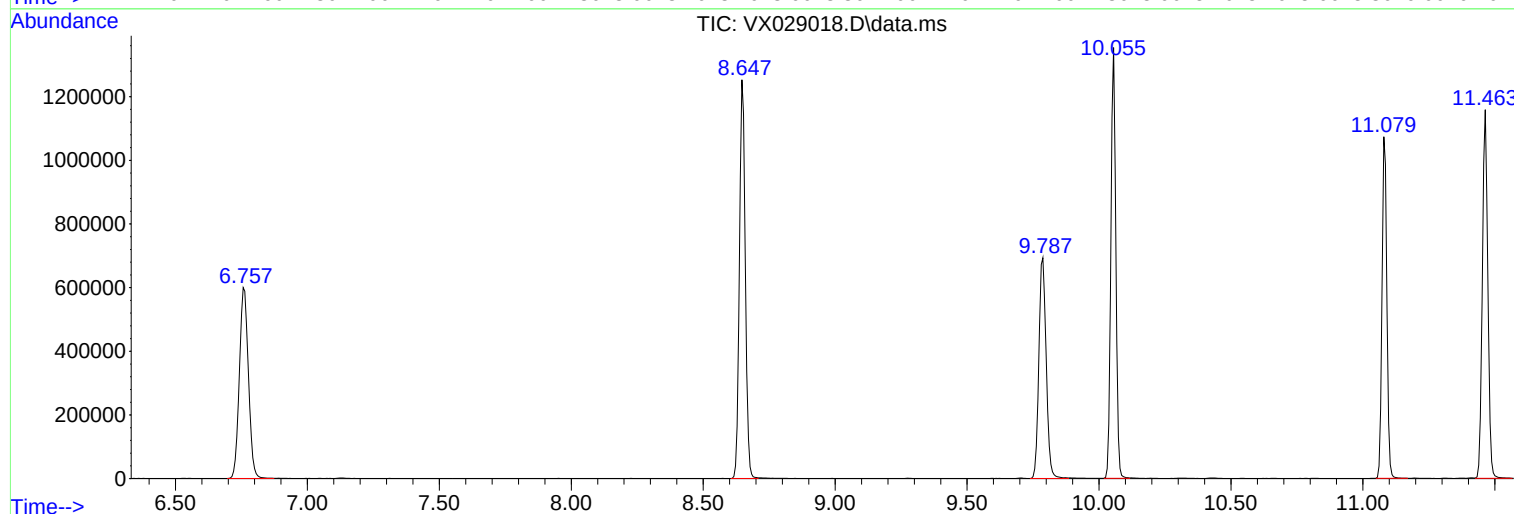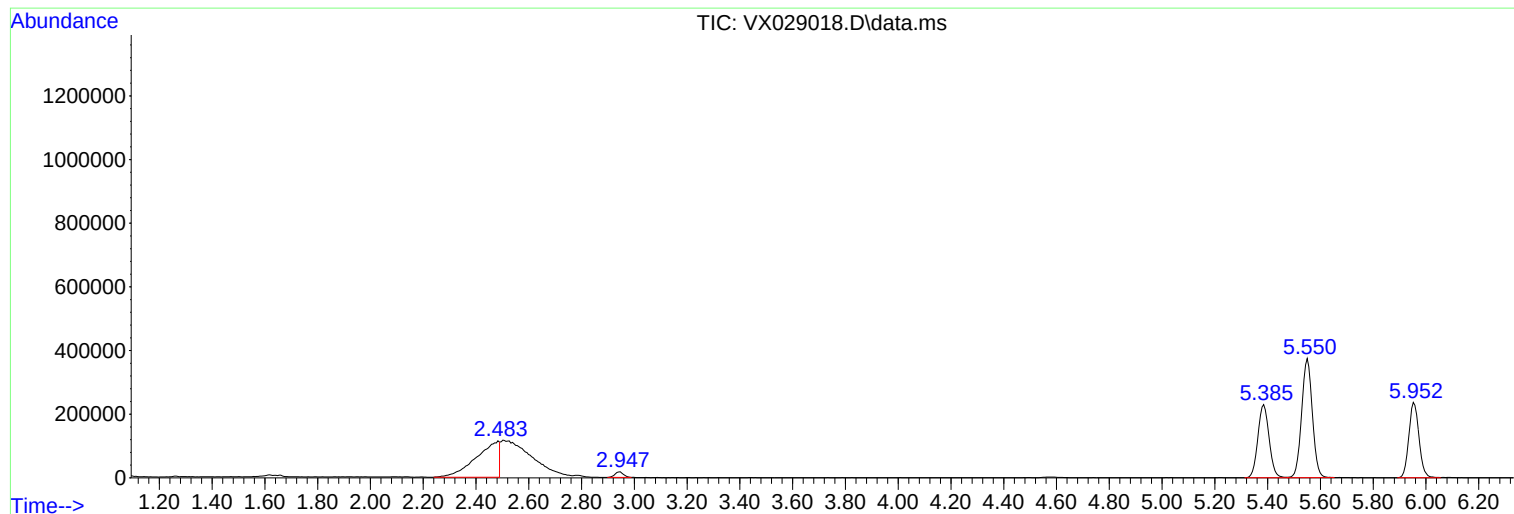

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029018.D
Acq On : 27 May 2022 12:19
Operator : JC/MD
Sample : VX0527WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0527WBL01










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzene, 1-bromo-3-fluoro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.787	37.55 ug/l	1327300	Chlorobenzene-d5	10.055

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1-bromo-3-fluoro-	174	C6H4BrF	001073-06-9	95
2			Benzene, 1-bromo-2-fluoro-	174	C6H4BrF	001072-85-1	94
3			p-Bromofluorobenzene	174	C6H4BrF	000460-00-4	93
4			4(1H)-Pyrimidinone, 5-bromo-	174	C4H3BrN2O	019808-30-1	37
5			6-Ethynyl-4-methoxy-2H-1,3-benzo...	176	C10H8O3	1000388-14-3	14

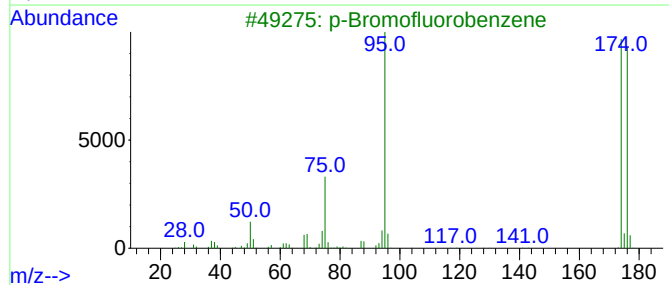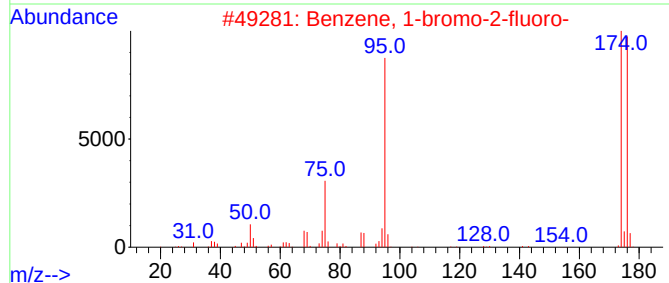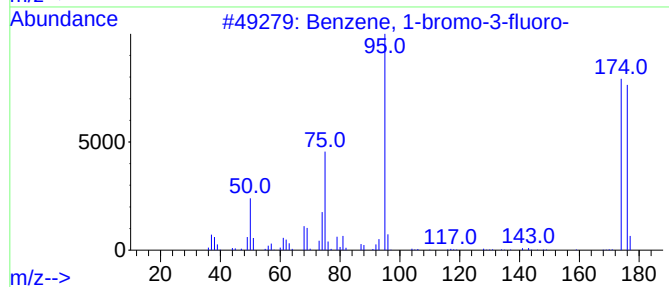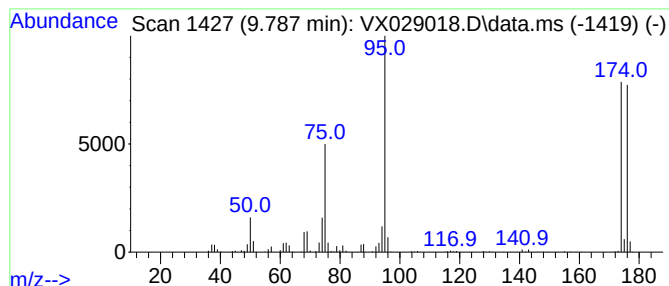

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029018.D
Acq On : 27 May 2022 12:19
Operator : JC/MD
Sample : VX0527WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0527WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1-brom...	9.787	37.5	ug/l	1327300	3	10.055	1767500	50.0