

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
 Data File : VX029023.D
 Acq On : 27 May 2022 14:50
 Operator : JC/MD
 Sample : N2968-05 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-27

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Title : SW846 8260

Signal : TIC: VX029023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	32	rBV	20031	34750	1.87%	0.267%
2	2.953	297	306	319	rVB2	31823	75586	4.06%	0.581%
3	3.117	324	333	344	rVB2	15143	37061	1.99%	0.285%
4	5.391	694	706	720	rBV	223960	653795	35.09%	5.029%
5	5.556	722	733	749	rVB	350078	1008682	54.14%	7.758%
6	5.958	789	799	806	rBV	232045	602167	32.32%	4.632%
7	6.043	806	813	826	rVB	282023	750608	40.29%	5.773%
8	6.763	921	931	948	rBV	572151	1366582	73.35%	10.511%
9	8.653	1234	1241	1248	rBV	1184802	1863037	100.00%	14.330%
10	8.720	1248	1252	1261	rVB	59506	96381	5.17%	0.741%
11	10.055	1465	1471	1487	rBV	1257384	1687477	90.58%	12.980%
12	10.195	1489	1494	1500	rBV	224680	291591	15.65%	2.243%
13	10.305	1506	1512	1520	rBV	285656	377866	20.28%	2.906%
14	10.646	1562	1568	1579	rBV	166682	223486	12.00%	1.719%
15	11.085	1634	1640	1648	rBV	1020794	1324826	71.11%	10.190%
16	11.305	1671	1676	1683	rBV	25972	33808	1.81%	0.260%
17	11.384	1683	1689	1690	rVV	38128	48911	2.63%	0.376%
18	11.402	1690	1692	1697	rVV	35922	42812	2.30%	0.329%
19	11.451	1697	1700	1711	rVB	26528	35448	1.90%	0.273%
20	11.616	1721	1727	1732	rBV	58312	72621	3.90%	0.559%
21	11.756	1745	1750	1756	rVB	167555	207665	11.15%	1.597%
22	12.024	1788	1794	1800	rBV	1358905	1651032	88.62%	12.699%
23	12.091	1800	1805	1811	rVB	75557	97985	5.26%	0.754%
24	12.244	1824	1830	1838	rBV	107806	134892	7.24%	1.038%
25	12.701	1901	1905	1912	rVB2	16105	22103	1.19%	0.170%
26	13.140	1969	1977	1981	rBV	47435	72148	3.87%	0.555%
27	13.292	1997	2002	2007	rVB2	35495	48487	2.60%	0.373%
28	13.774	2076	2081	2088	rBV	70174	94261	5.06%	0.725%
29	14.640	2218	2223	2231	rVB	14439	19198	1.03%	0.148%
30	14.780	2240	2246	2251	rBV	20012	25817	1.39%	0.199%




Sum of corrected areas: 13001083

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029023.D
Acq On : 27 May 2022 14:50
Operator : JC/MD
Sample : N2968-05 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

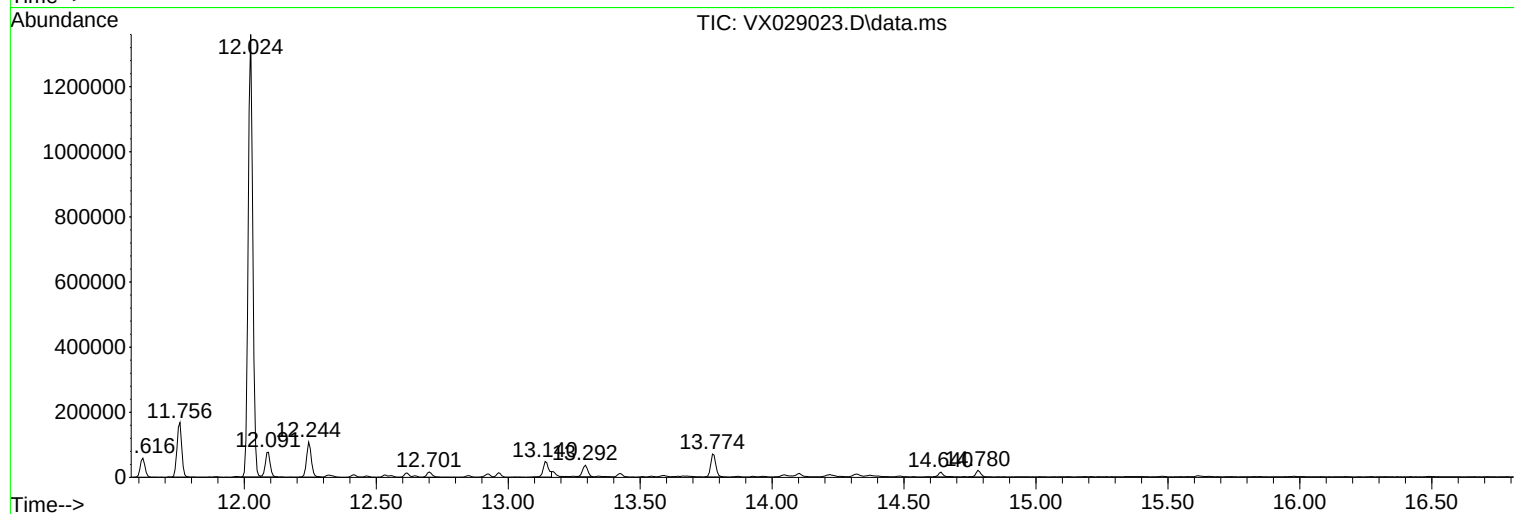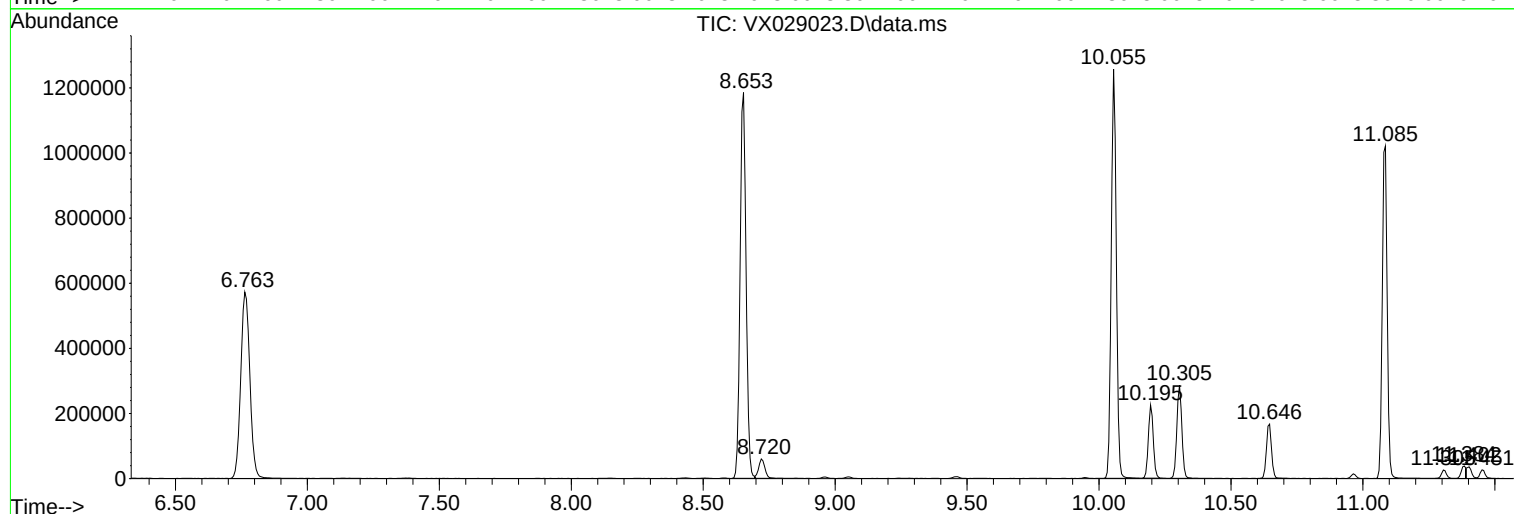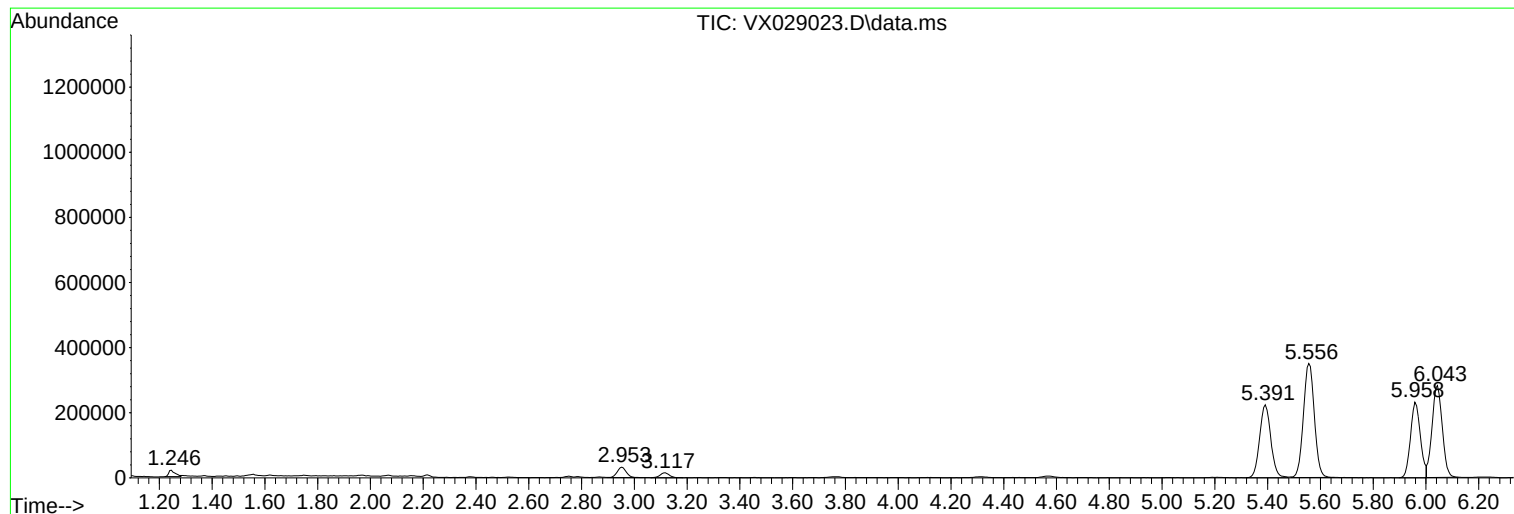

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029023.D
Acq On : 27 May 2022 14:50
Operator : JC/MD
Sample : N2968-05 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029023.D
Acq On : 27 May 2022 14:50
Operator : JC/MD
Sample : N2968-05 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc