

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
 Data File : VX029034.D
 Acq On : 27 May 2022 19:07
 Operator : JC/MD
 Sample : N2968-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-45

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M

Title : SW846 8260

Signal : TIC: VX029034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	18	26	41	rBV	23699	53010	2.86%	0.516%
2	2.532	229	237	248	rBV	18334	35148	1.90%	0.342%
3	2.947	296	305	314	rBV	13276	30559	1.65%	0.298%
4	5.391	694	706	722	rBV2	221089	648175	35.01%	6.315%
5	5.556	722	733	749	rVB	354188	995522	53.77%	9.699%
6	5.958	789	799	822	rBV	230510	604047	32.63%	5.885%
7	6.763	921	931	951	rBV	573121	1355161	73.20%	13.203%
8	8.653	1234	1241	1256	rBV	1177835	1851279	100.00%	18.037%
9	10.055	1465	1471	1489	rBV	1265283	1695796	91.60%	16.522%
10	11.079	1634	1639	1653	rBV	1002711	1330270	71.86%	12.961%
11	12.024	1788	1794	1802	rBV	1366112	1664854	89.93%	16.221%




Sum of corrected areas: 10263821

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029034.D
Acq On : 27 May 2022 19:07
Operator : JC/MD
Sample : N2968-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

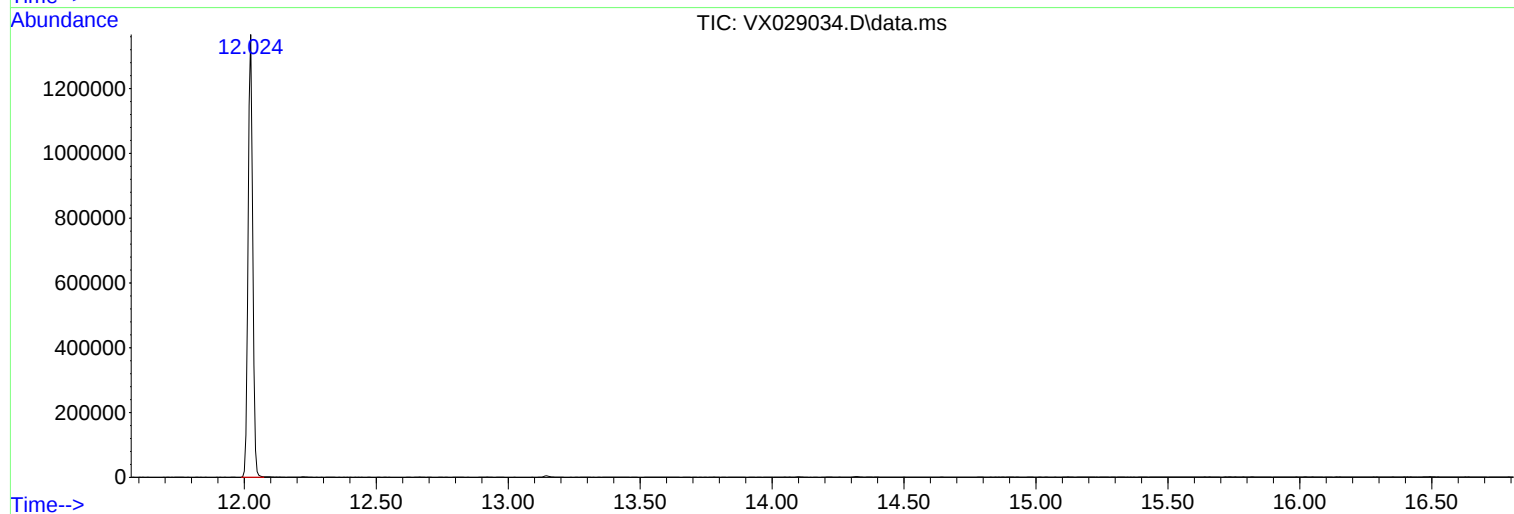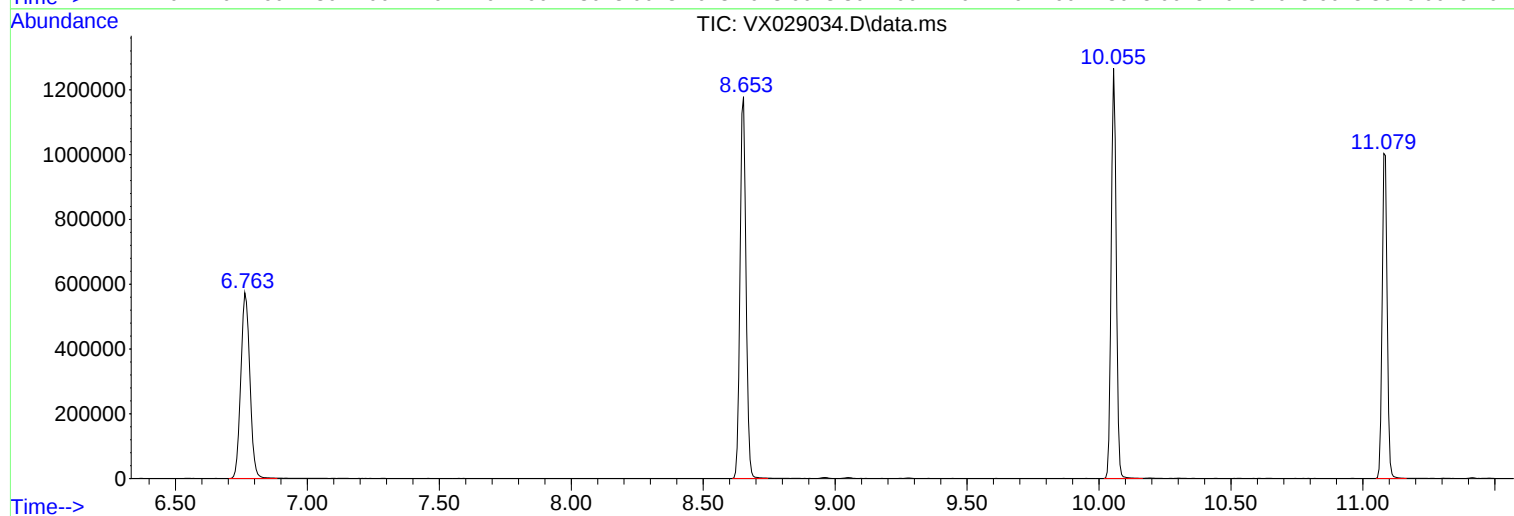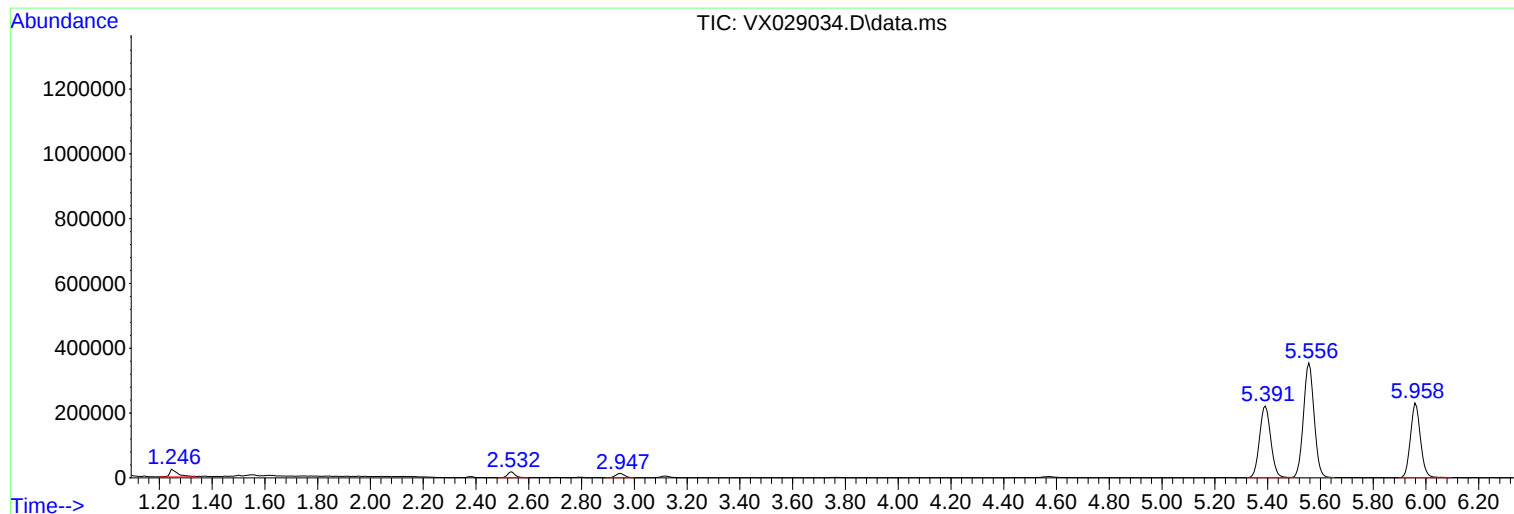

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029034.D
Acq On : 27 May 2022 19:07
Operator : JC/MD
Sample : N2968-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029034.D
Acq On : 27 May 2022 19:07
Operator : JC/MD
Sample : N2968-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------