

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
 Data File : VX029047.D
 Acq On : 28 May 2022 01:19
 Operator : JC/MD
 Sample : N3022-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RB06-20220525

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M

Title : SW846 8260

Signal : TIC: VX029047.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	25	31	40	rBV4	8819	22188	1.17%	0.214%
2	2.380	205	212	222	rBV	21784	36072	1.91%	0.349%
3	2.538	230	238	252	rBV2	21520	50928	2.70%	0.492%
4	5.385	693	705	720	rBV	226579	662594	35.07%	6.405%
5	5.556	721	733	748	rVB	360390	1020361	54.01%	9.864%
6	5.958	785	799	820	rBV	232810	617360	32.68%	5.968%
7	6.763	921	931	949	rBV	588721	1385431	73.34%	13.393%
8	8.653	1234	1241	1256	rBV	1185878	1889133	100.00%	18.263%
9	10.055	1465	1471	1488	rBV	1268312	1701740	90.08%	16.451%
10	11.079	1634	1639	1652	rBV	1002509	1319934	69.87%	12.760%
11	12.024	1788	1794	1804	rBV	1348816	1638454	86.73%	15.839%




Sum of corrected areas: 10344195

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029047.D
Acq On : 28 May 2022 01:19
Operator : JC/MD
Sample : N3022-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RB06-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

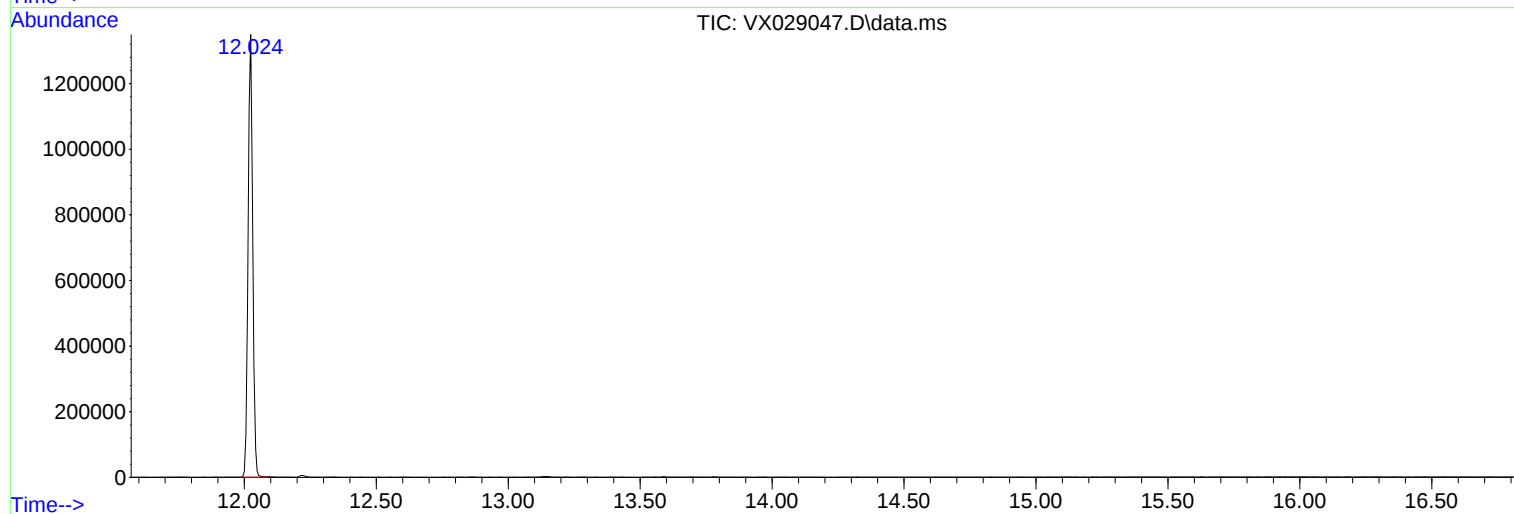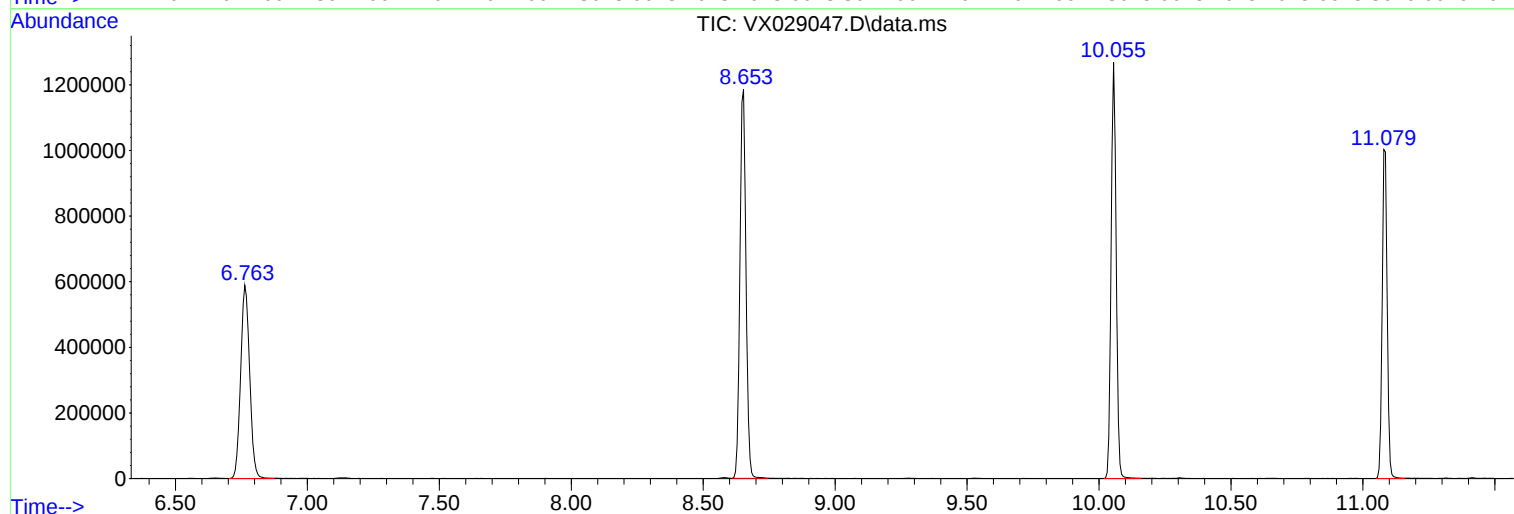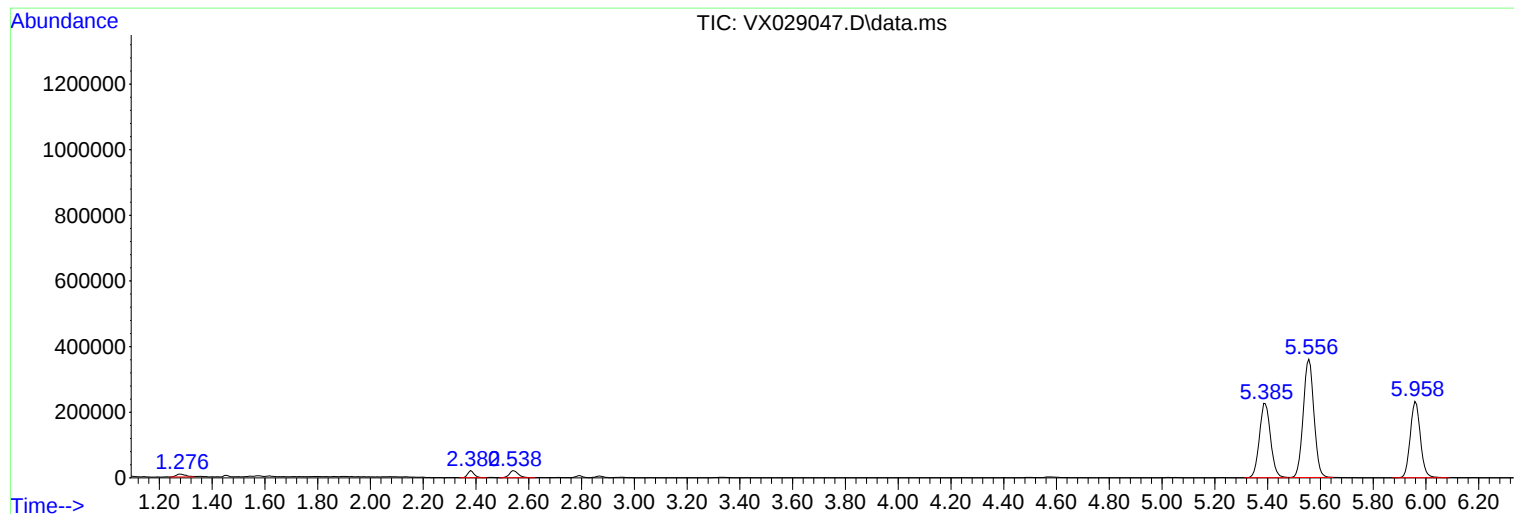

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029047.D
Acq On : 28 May 2022 01:19
Operator : JC/MD
Sample : N3022-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RB06-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029047.D
Acq On : 28 May 2022 01:19
Operator : JC/MD
Sample : N3022-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RB06-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc