

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029056.D
Acq On : 28 May 2022 04:49
Operator : JC/MD
Sample : N3022-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
08BR-20220525

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M

Title : SW846 8260

Signal : TIC: VX029056.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.330	197	204	210	rBV2	55110	106154	2.53%	0.750%
2	4.495	548	559	575	rBV	71092	197651	4.72%	1.397%
3	5.391	694	706	721	rBV	217004	628165	14.99%	4.441%
4	5.556	722	733	749	rVB	336623	955304	22.80%	6.754%
5	5.958	785	799	817	rBV	218962	581453	13.88%	4.111%
6	6.763	921	931	948	rBV	550762	1304842	31.15%	9.225%
7	7.128	981	991	1015	rBV	1952880	4189244	100.00%	29.617%
8	8.653	1234	1241	1258	rBV	1130728	1791877	42.77%	12.668%
9	10.055	1465	1471	1482	rBV	1229969	1613691	38.52%	11.408%
10	11.085	1634	1640	1652	rBV	949050	1245411	29.73%	8.805%
11	12.024	1788	1794	1804	rBV	1248001	1530971	36.55%	10.824%




Sum of corrected areas: 14144763

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029056.D
Acq On : 28 May 2022 04:49
Operator : JC/MD
Sample : N3022-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
08BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

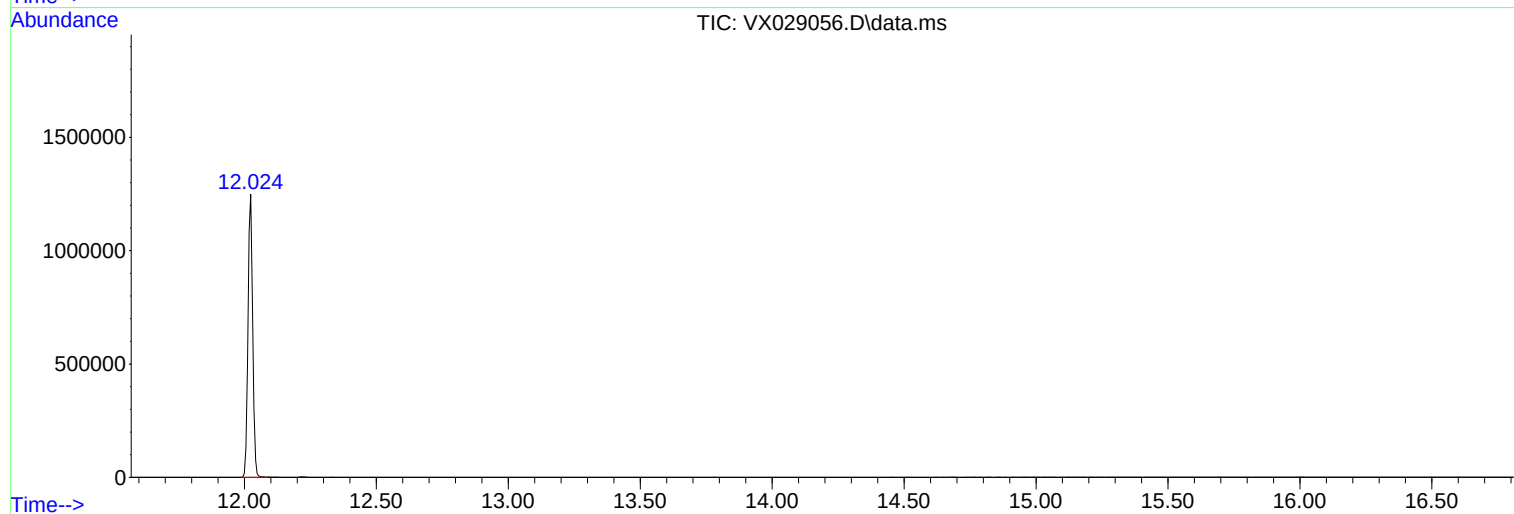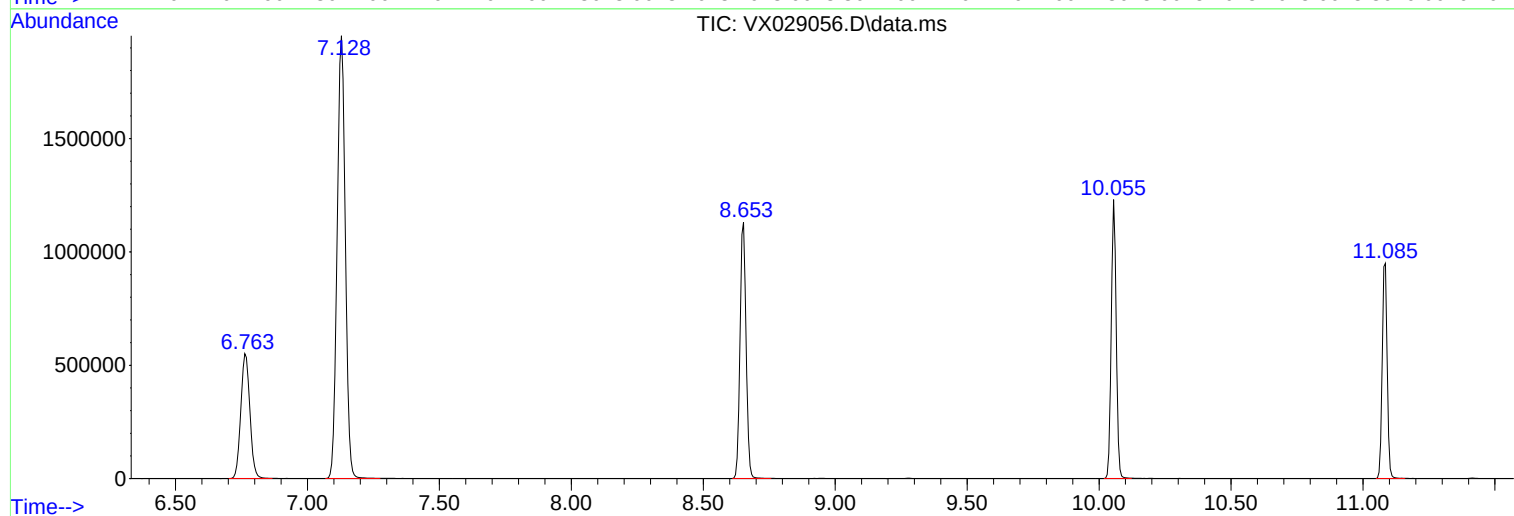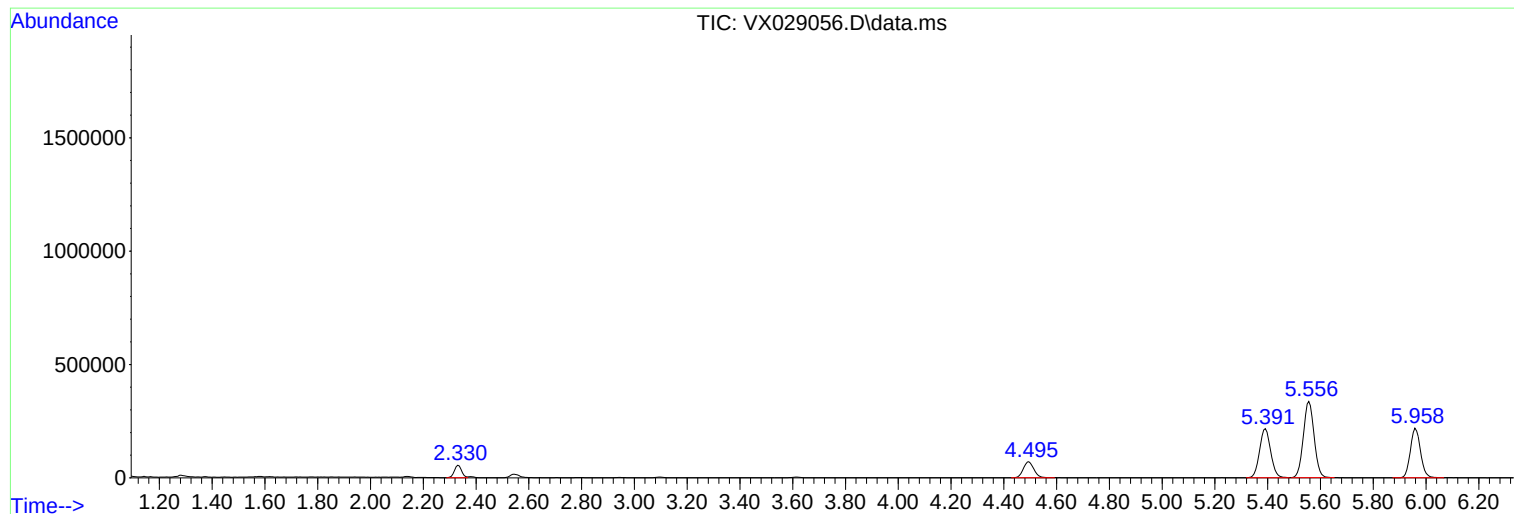

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029056.D
Acq On : 28 May 2022 04:49
Operator : JC/MD
Sample : N3022-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
08BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029056.D
Acq On : 28 May 2022 04:49
Operator : JC/MD
Sample : N3022-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
08BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc