

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
 Data File : VX029058.D
 Acq On : 28 May 2022 05:36
 Operator : JC/MD
 Sample : N3022-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP03-20220525

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M

Title : SW846 8260

Signal : TIC: VX029058.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	55	rVB	660970	637899	1.39%	0.745%
2	4.495	544	559	587	rBV	10595254	29433793	64.14%	34.382%
3	5.391	694	706	721	rBV	213784	620588	1.35%	0.725%
4	5.556	721	733	751	rVB2	339771	955280	2.08%	1.116%
5	5.958	788	799	817	rBV	215931	573482	1.25%	0.670%
6	6.763	921	931	944	rBV	540538	1294703	2.82%	1.512%
7	7.135	980	992	1021	rBV	20340320	45890735	100.00%	53.606%
8	8.653	1234	1241	1251	rBV	1121470	1765010	3.85%	2.062%
9	10.055	1465	1471	1490	rBV	1218263	1609164	3.51%	1.880%
10	11.085	1634	1640	1654	rBV	958083	1252736	2.73%	1.463%
11	12.024	1788	1794	1803	rBV	1265897	1573594	3.43%	1.838%




Sum of corrected areas: 85606984

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029058.D
Acq On : 28 May 2022 05:36
Operator : JC/MD
Sample : N3022-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP03-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

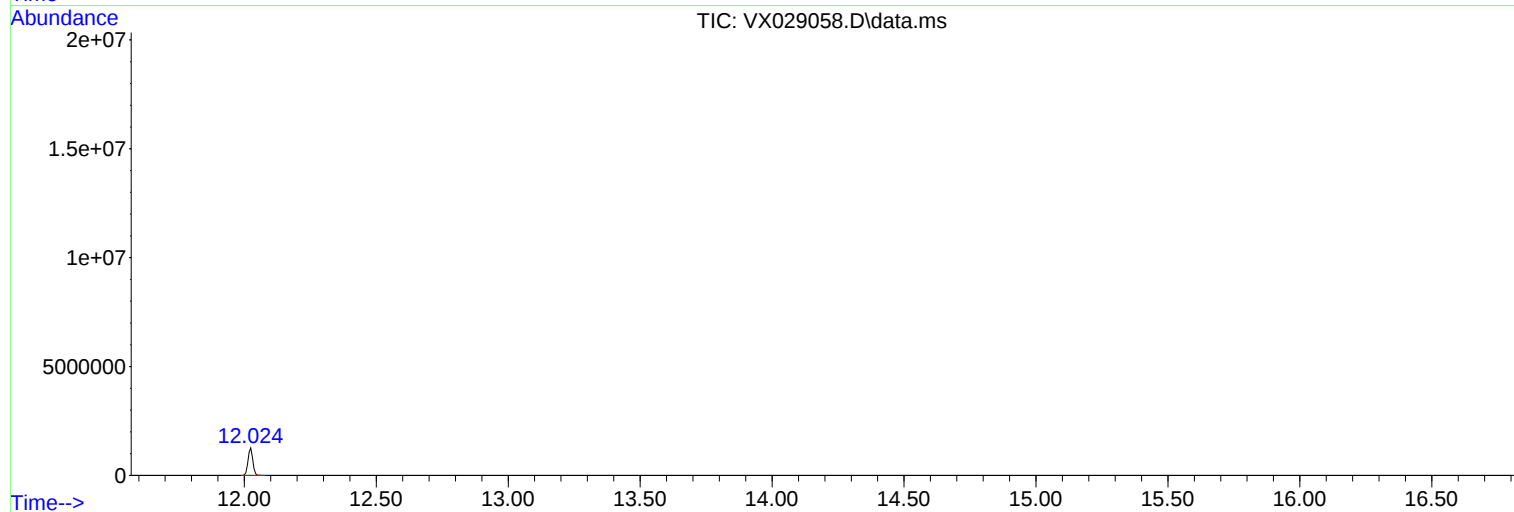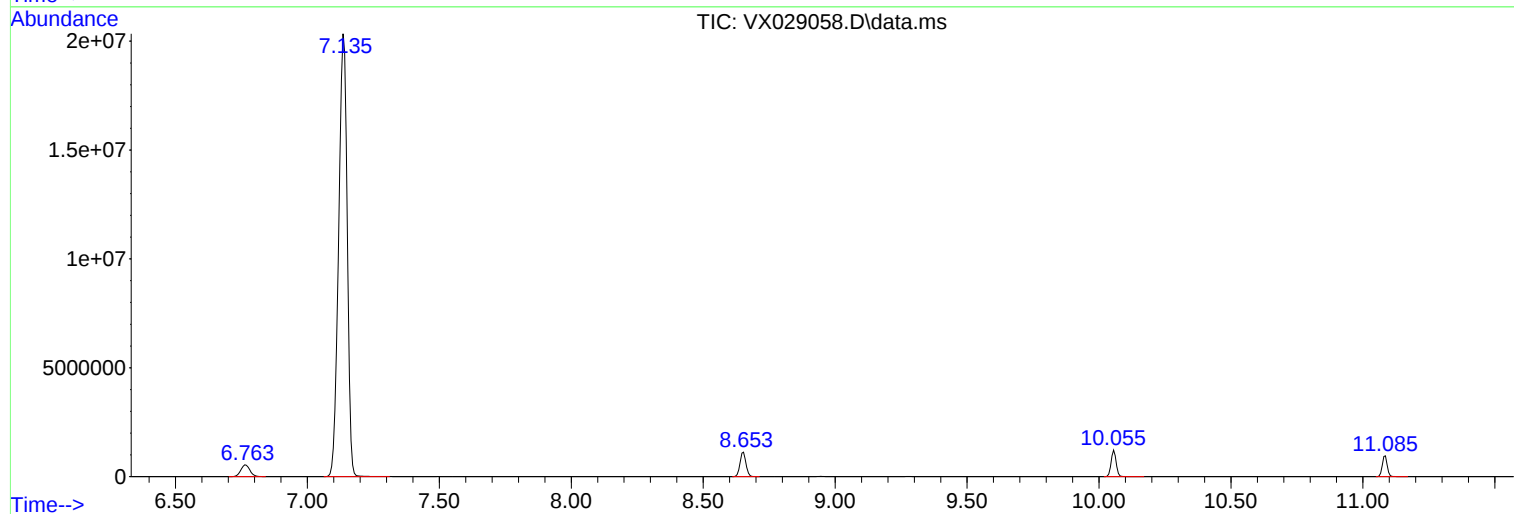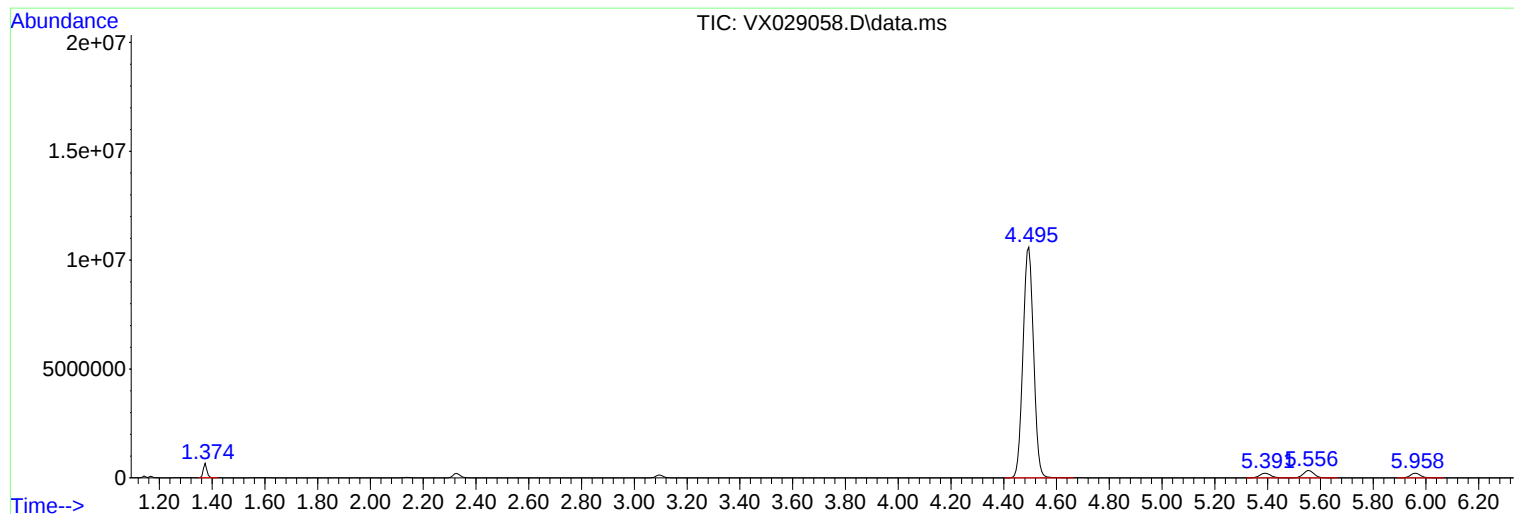

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029058.D
Acq On : 28 May 2022 05:36
Operator : JC/MD
Sample : N3022-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP03-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052722\
Data File : VX029058.D
Acq On : 28 May 2022 05:36
Operator : JC/MD
Sample : N3022-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP03-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------