

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX052821\  
 Data File : VX022240.D  
 Acq On : 27 May 2021 18:14  
 Operator : JC/MD  
 Sample : M2526-18DL 50X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 18 Sample Multiplier: 1


Instrument :  
 MSVOA\_X  
 ClientSampleId :

Quant Time: May 28 01:33:45 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051921W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed May 19 14:23:10 2021  
 Response via : Initial Calibration

| Compound                      | R.T.           | QIon | Response           | Conc  | Units | Dev(Min) |
|-------------------------------|----------------|------|--------------------|-------|-------|----------|
| -----                         |                |      |                    |       |       |          |
| Internal Standards            |                |      |                    |       |       |          |
| 1) Pentafluorobenzene         | 5.562          | 168  | 68534              | 50.00 | ug/l  | # 0.00   |
| 34) 1,4-Difluorobenzene       | 6.769          | 114  | 142074             | 50.00 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5          | 10.055         | 117  | 124250             | 50.00 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 12.024         | 152  | 46299              | 50.00 | ug/l  | 0.00     |
|                               |                |      |                    |       |       |          |
| System Monitoring Compounds   |                |      |                    |       |       |          |
| 33) 1,2-Dichloroethane-d4     | 5.964          | 65   | 55535              | 52.53 | ug/l  | 0.00     |
| Spiked Amount 50.000          | Range 78 - 117 |      | Recovery = 105.06% |       |       |          |
| 35) Dibromofluoromethane      | 5.391          | 113  | 42323              | 46.98 | ug/l  | 0.00     |
| Spiked Amount 50.000          | Range 75 - 124 |      | Recovery = 93.96%  |       |       |          |
| 50) Toluene-d8                | 8.653          | 98   | 174590             | 50.31 | ug/l  | 0.00     |
| Spiked Amount 50.000          | Range 92 - 112 |      | Recovery = 100.62% |       |       |          |
| 62) 4-Bromofluorobenzene      | 11.085         | 95   | 58626              | 45.70 | ug/l  | 0.00     |
| Spiked Amount 50.000          | Range 83 - 123 |      | Recovery = 91.40%  |       |       |          |
|                               |                |      |                    |       |       |          |
| Target Compounds              |                |      |                    |       |       | Qvalue   |
| 2) Dichlorodifluoromethane    | 1.173          | 85   | 212                | 0.25  | ug/l  | # 42     |
| 5) Bromomethane               | 1.612          | 94   | 302                | 0.54  | ug/l  | # 54     |
| 10) Methyl Iodide             | 2.447          | 142  | 265                | 0.30  | ug/l  | # 84     |
| 11) Tert butyl alcohol        | 2.947          | 59   | 1909               | 7.89  | ug/l  | # 73     |
| 12) 1,1-Dichloroethene        | 2.325          | 96   | 362                | 0.46  | ug/l  | # 48     |
| 13) Acrolein                  | 2.258          | 56   | 138                | 0.86  | ug/l  | # 54     |
| 16) Acetone                   | 2.386          | 43   | 796                | 1.73  | ug/l  | # 80     |
| 17) Carbon Disulfide          | 2.520          | 76   | 467                | 0.23  | ug/l  | # 75     |
| 20) Methylene Chloride        | 2.794          | 84   | 844                | 0.83  | ug/l  | # 84     |
| 21) trans-1,2-Dichloroethene  | 3.105          | 96   | 466                | 0.55  | ug/l  | 86       |
| 27) cis-1,2-Dichloroethene    | 4.495          | 96   | 14751              | 14.20 | ug/l  | 90       |
| 31) Cyclohexane               | 5.556          | 56   | 1989               | 1.50  | ug/l  | # 15     |
| 36) 1,1-Dichloropropene       | 5.562          | 75   | 6424               | 4.89  | ug/l  | # 48     |
| 38) Carbon Tetrachloride      | 5.568          | 117  | 7835               | 6.10  | ug/l  | # 17     |
| 44) Trichloroethene           | 7.129          | 130  | 60150              | 59.88 | ug/l  | 98       |
| 68) m/p-Xylenes               | 10.305         | 106  | 386                | 0.21  | ug/l  | # 46     |
| 76) 1,2,3-Trichloropropane    | 11.085         | 75   | 30656              | 26.84 | ug/l  | # 39     |
| 78) n-propylbenzene           | 11.305         | 91   | 1107               | 0.24  | ug/l  | 98       |
| 81) trans-1,4-Dichloro-2-b... | 11.085         | 75   | 30656              | 63.59 | ug/l  | # 12     |
| 84) 1,2,4-Trimethylbenzene    | 11.756         | 105  | 1278               | 0.39  | ug/l  | 83       |
| 88) 1,4-Dichlorobenzene       | 12.049         | 146  | 356                | 0.21  | ug/l  | # 25     |
| 89) n-Butylbenzene            | 12.335         | 91   | 749                | 0.24  | ug/l  | 82       |
| 90) Hexachloroethane          | 12.707         | 117  | 125                | 0.23  | ug/l  | # 9      |
| 93) 1,2,4-Trichlorobenzene    | 13.591         | 180  | 228                | 0.25  | ug/l  | 90       |
| 94) Hexachlorobutadiene       | 13.719         | 225  | 140                | 0.39  | ug/l  | # 19     |
| 95) Naphthalene               | 13.780         | 128  | 960                | 0.27  | ug/l  | 98       |
| -----                         |                |      |                    |       |       |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Quant Time: May 28 01:33:45 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051921W.M  
Quant Title : SW846 8260  
QLast Update : Wed May 19 14:23:10 2021  
Response via : Initial Calibration

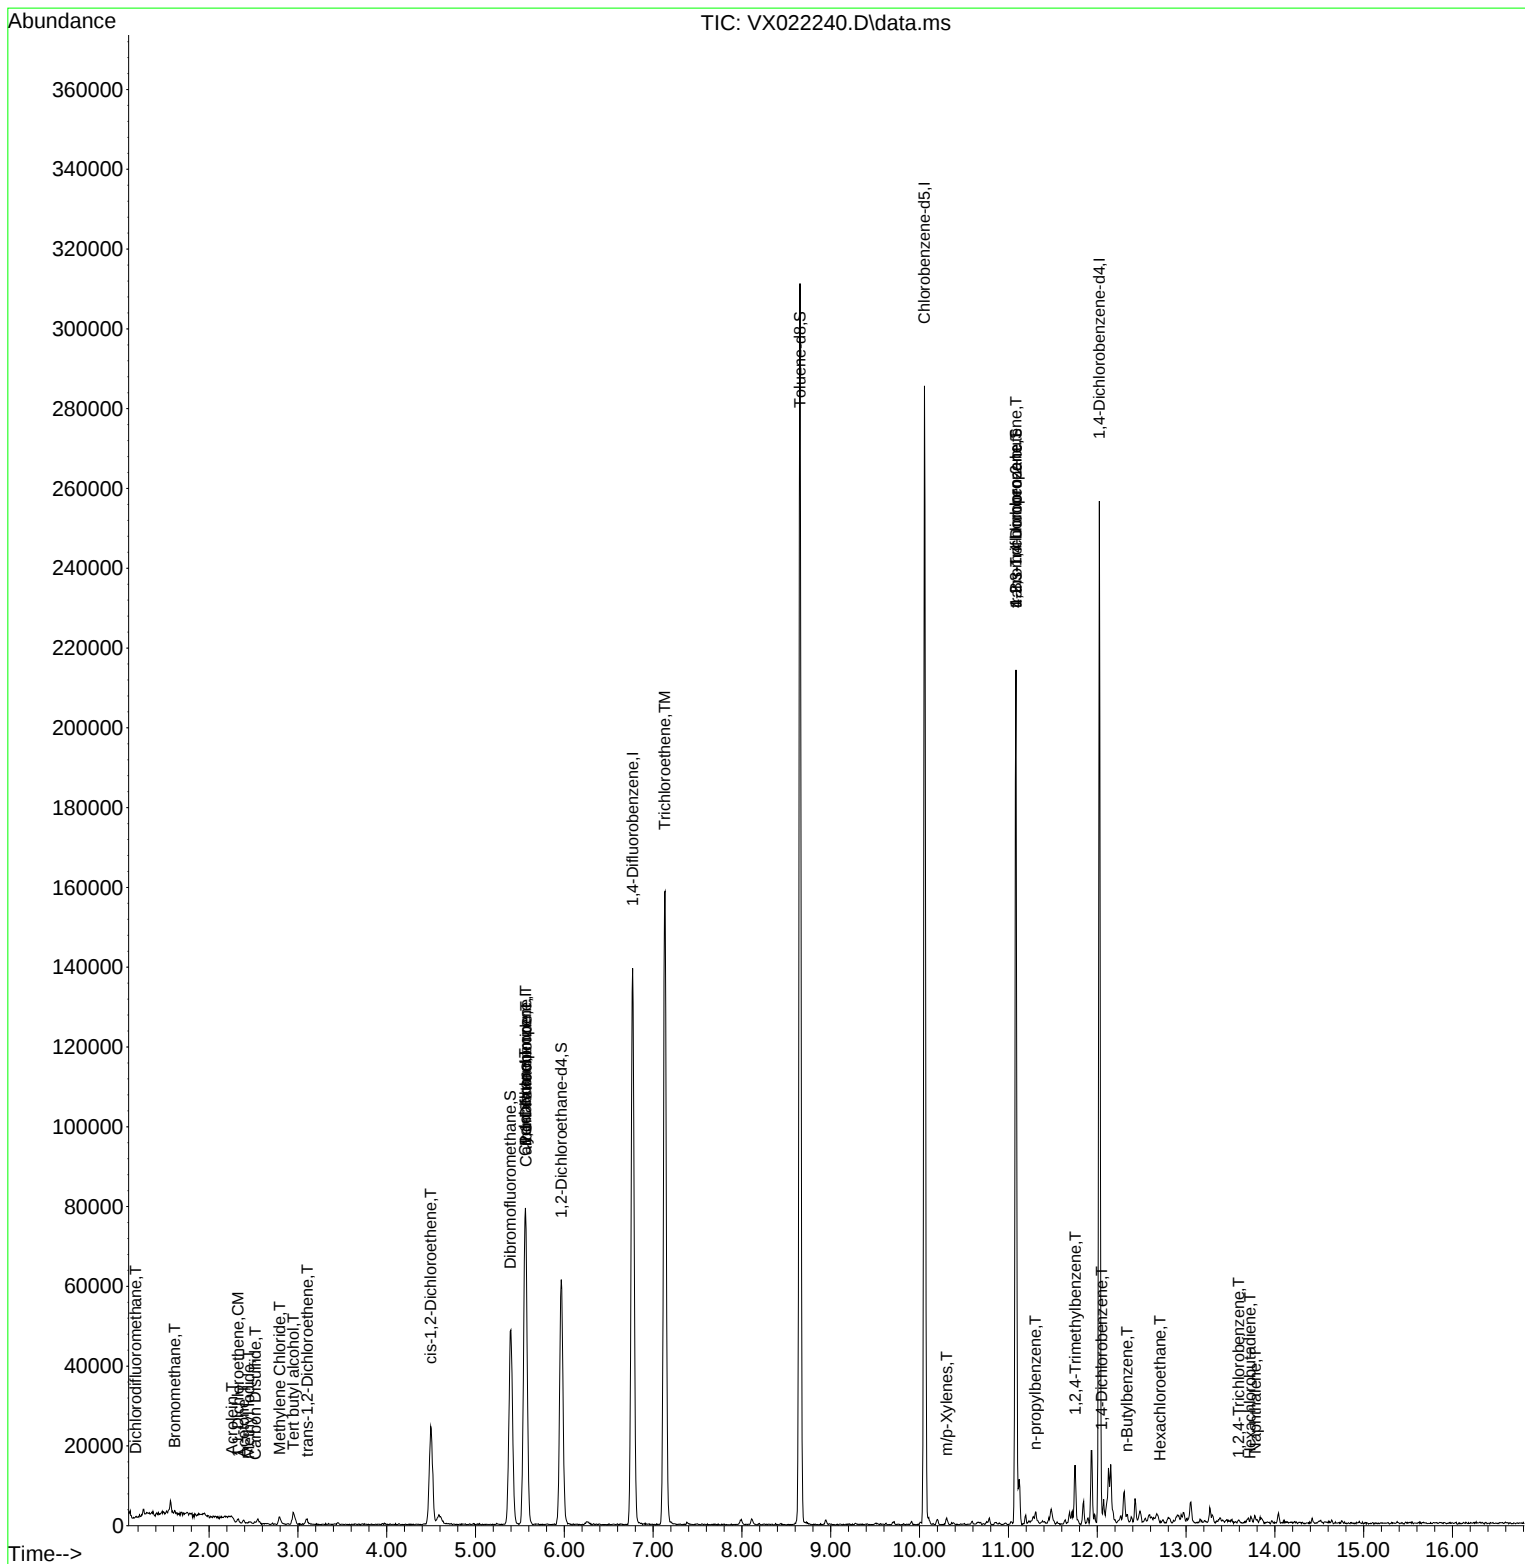






#1  
Pentafluorobenzene  
Concen: 50.00 ug/l  
RT: 5.562 min Scan# 734  
Delta R.T. 0.000 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14

Instrument :  
MSVOA\_X  
ClientSampled :







Tgt Ion:168 Resp: 68534  
Ion Ratio Lower Upper  
168 100  
99 69.8 45.8 68.6#



#2  
Dichlorodifluoromethane  
Concen: 0.25 ug/l  
RT: 1.173 min Scan# 14  
Delta R.T. 0.006 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14

Tgt Ion: 85 Resp: 212  
Ion Ratio Lower Upper  
85 100  
87 0.0 16.4 49.2#


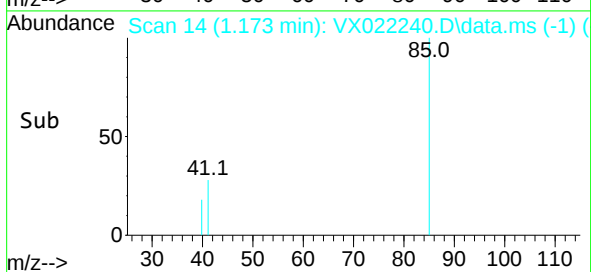




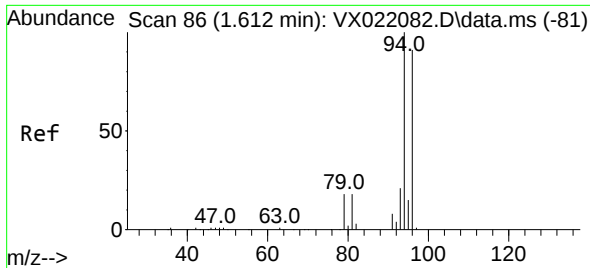

#5  
Bromomethane  
Concen: 0.54 ug/l  
RT: 1.612 min Scan# 86  
Delta R.T. -0.000 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 94 Resp: 302  
Ion Ratio Lower Upper  
94 100  
96 50.4 76.4 114.6#

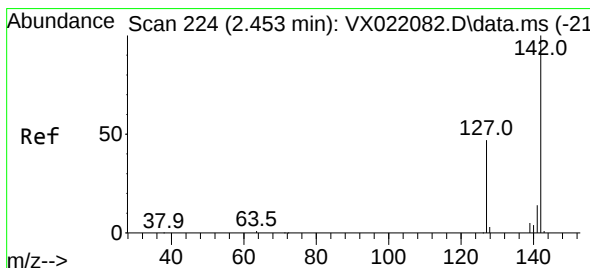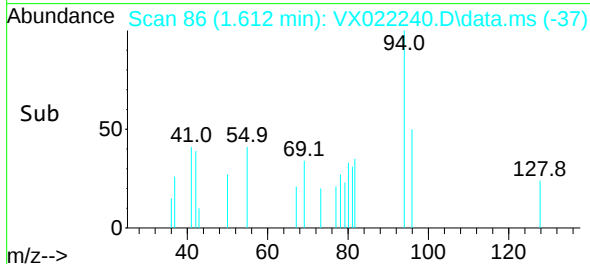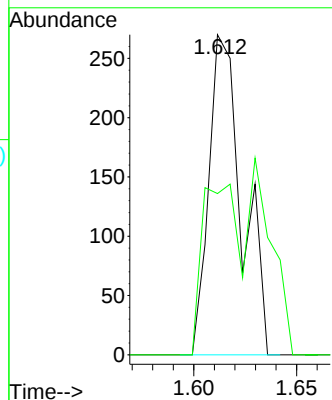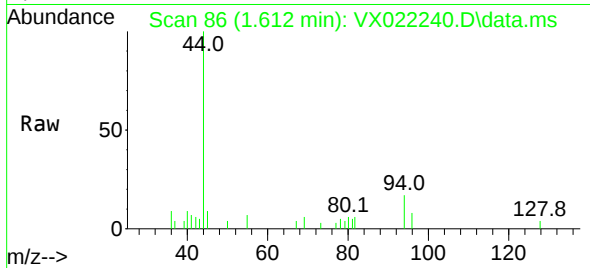

#10  
Methyl Iodide  
Concen: 0.30 ug/l  
RT: 2.447 min Scan# 223  
Delta R.T. -0.006 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14

Tgt Ion: 142 Resp: 265  
Ion Ratio Lower Upper  
142 100  
127 35.5 33.3 49.9  
141 0.0 11.4 17.0#

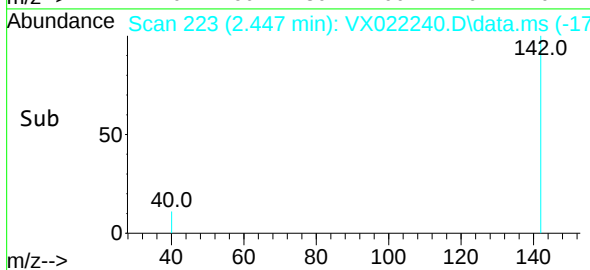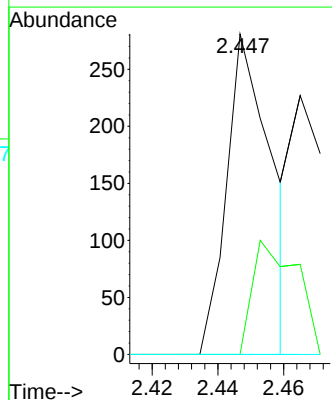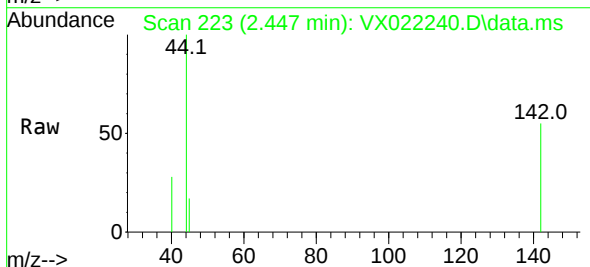




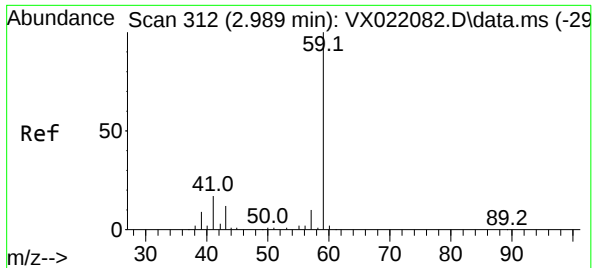


#11

Tert butyl alcohol  
Concen: 7.89 ug/l  
RT: 2.947 min Scan# 305  
Delta R.T. -0.042 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14

Instrument :  
MSVOA\_X  
ClientSampled :




Tgt Ion: 59 Resp: 1909  
Ion Ratio Lower Upper  
59 100  
57 0.0 7.8 11.8#

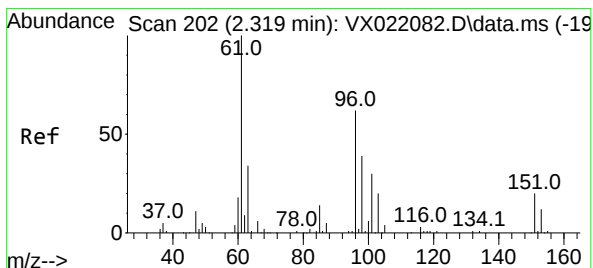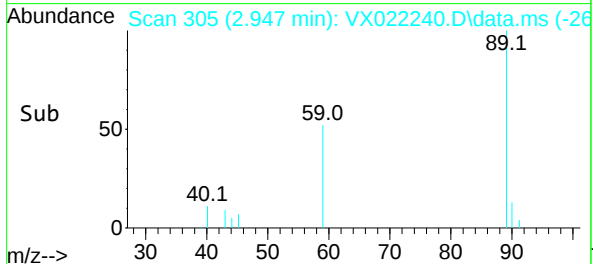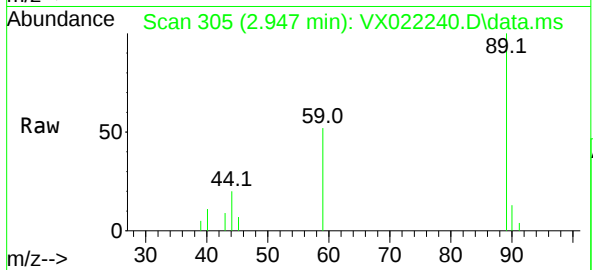


#12

1,1-Dichloroethene  
Concen: 0.46 ug/l  
RT: 2.325 min Scan# 203  
Delta R.T. 0.006 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14


Tgt Ion: 96 Resp: 362  
Ion Ratio Lower Upper  
96 100  
61 74.2 124.6 187.0#  
98 42.6 50.6 76.0#

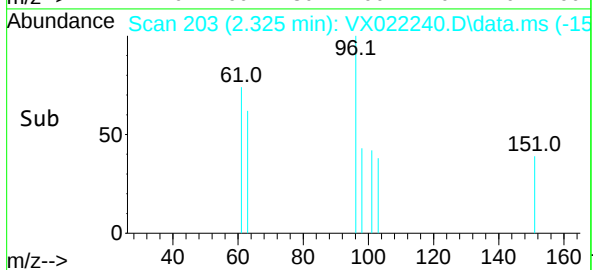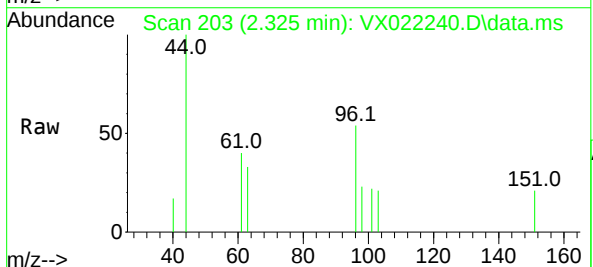






#13  
Acrolein  
Concen: 0.86 ug/l  
RT: 2.258 min Scan# 192  
Delta R.T. 0.018 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14

Instrument :  
MSVOA\_X  
ClientSampled :



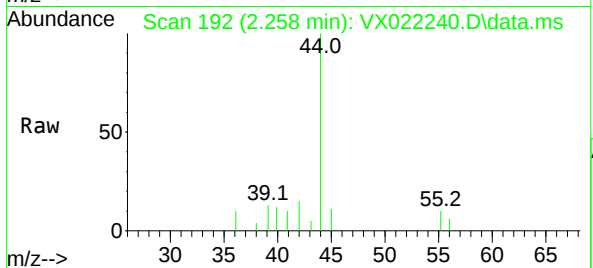



Tgt Ion: 56 Resp: 138  
Ion Ratio Lower Upper  
56 100  
55 108.7 56.4 84.6#

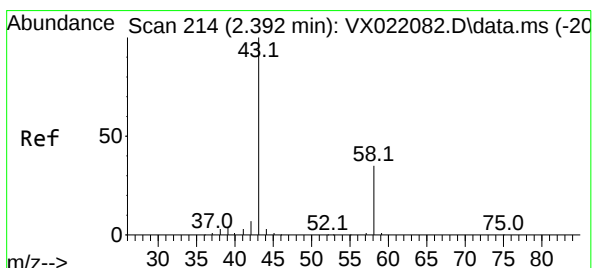

#16  
Acetone  
Concen: 1.73 ug/l  
RT: 2.386 min Scan# 213  
Delta R.T. -0.006 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14


Tgt Ion: 43 Resp: 796  
Ion Ratio Lower Upper  
43 100  
58 23.4 27.8 41.8#

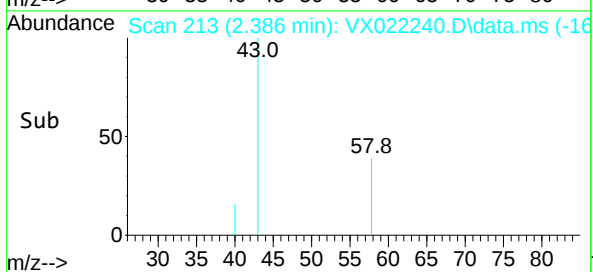






#17  
Carbon Disulfide  
Concen: 0.23 ug/l  
RT: 2.520 min Scan# 235  
Delta R.T. 0.006 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14

Instrument :  
MSVOA\_X  
ClientSampled :



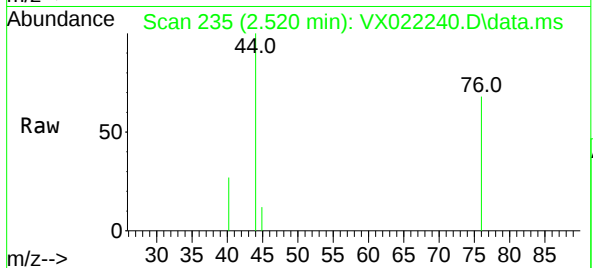



Tgt Ion: 76 Resp: 467  
Ion Ratio Lower Upper  
76 100  
78 0.0 7.2 10.8#

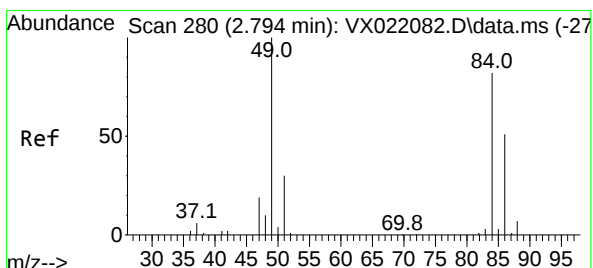

#20  
Methylene Chloride  
Concen: 0.83 ug/l  
RT: 2.794 min Scan# 280  
Delta R.T. 0.000 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14


Tgt Ion: 84 Resp: 844  
Ion Ratio Lower Upper  
84 100  
49 96.6 88.6 132.8  
51 24.6 27.0 40.6#  
86 78.6 50.3 75.5#

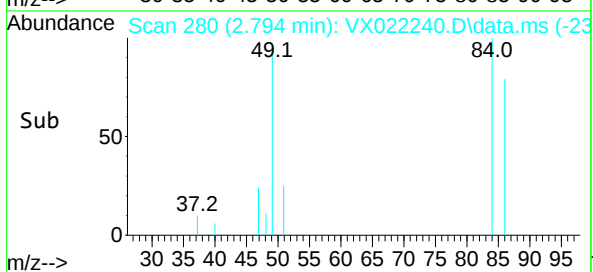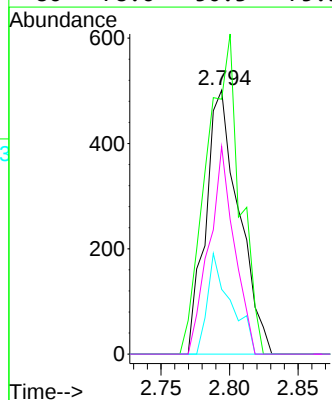






#21  
trans-1,2-Dichloroethene  
Concen: 0.55 ug/l  
RT: 3.105 min Scan# 331  
Delta R.T. 0.006 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14

Instrument :  
MSVOA\_X  
ClientSampled :



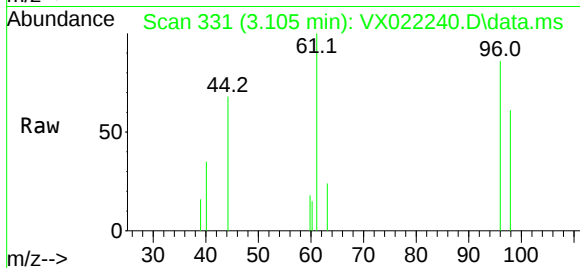



Tgt Ion: 96 Resp: 466  
Ion Ratio Lower Upper  
96 100  
61 116.3 107.7 161.5  
98 70.3 50.4 75.6

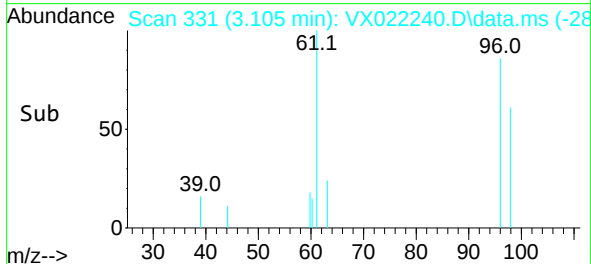

#27  
cis-1,2-Dichloroethene  
Concen: 14.20 ug/l  
RT: 4.495 min Scan# 559  
Delta R.T. 0.000 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14


Tgt Ion: 96 Resp: 14751  
Ion Ratio Lower Upper  
96 100  
61 125.5 0.0 285.6  
98 65.3 0.0 129.6

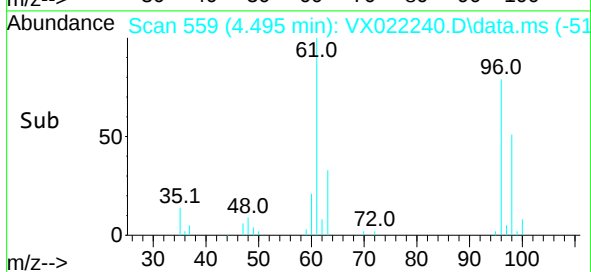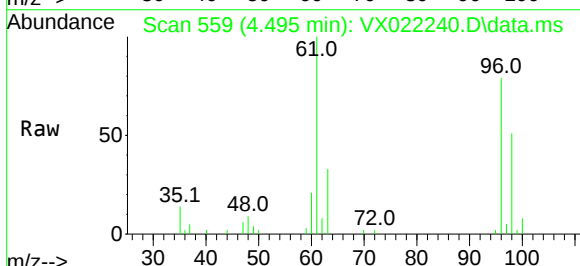






#31  
Cyclohexane  
Concen: 1.50 ug/l  
RT: 5.556 min Scan# 733  
Delta R.T. 0.073 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14


Instrument :  
MSVOA\_X  
ClientSampleId :

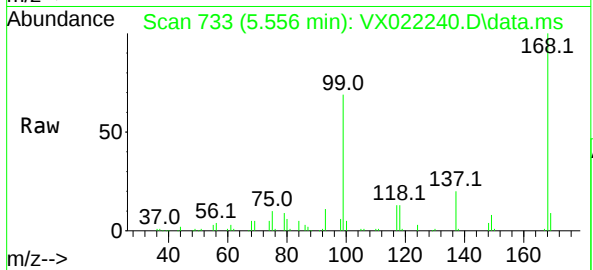



Tgt Ion: 56 Resp: 1989  
Ion Ratio Lower Upper  
56 100  
69 142.2 25.3 37.9#  
84 130.6 71.4 107.0#

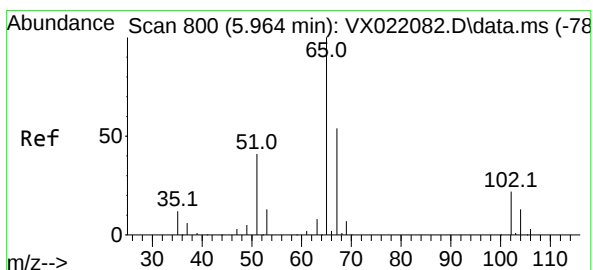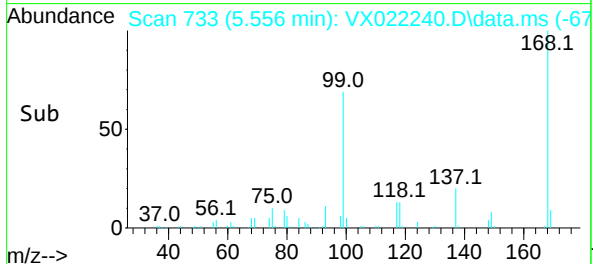


#33  
1,2-Dichloroethane-d4  
Concen: 52.53 ug/l  
RT: 5.964 min Scan# 800  
Delta R.T. 0.000 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14

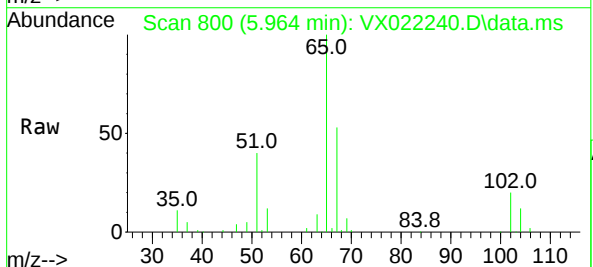

Tgt Ion: 65 Resp: 55535  
Ion Ratio Lower Upper  
65 100  
67 53.1 0.0 105.4



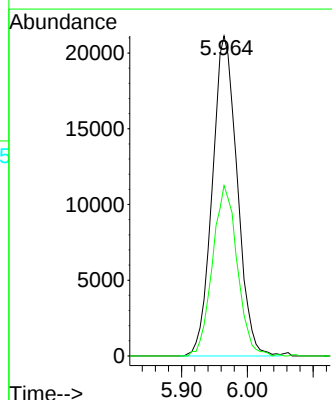
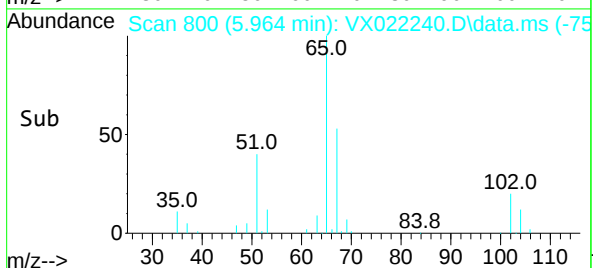




#34  
1,4-Difluorobenzene  
Concen: 50.00 ug/l  
RT: 6.769 min Scan# 932  
Delta R.T. 0.000 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion:114 Resp: 142074  
Ion Ratio Lower Upper  
114 100  
63 21.2 0.0 40.8  
88 16.0 0.0 32.8

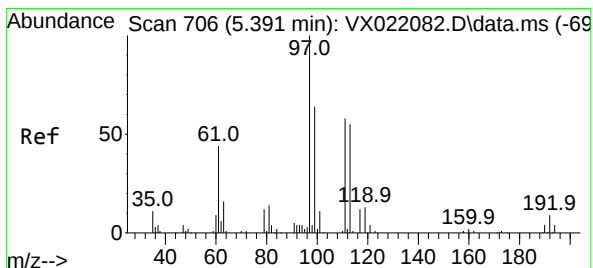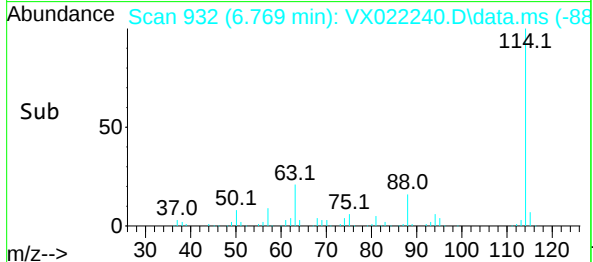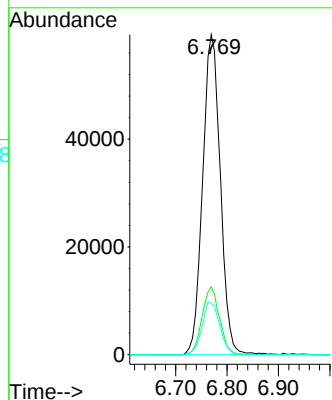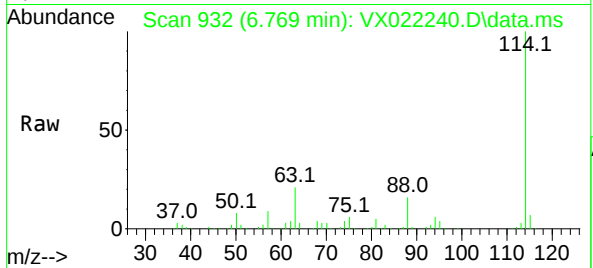

#35  
Dibromofluoromethane  
Concen: 46.98 ug/l  
RT: 5.391 min Scan# 706  
Delta R.T. 0.000 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14

Tgt Ion:113 Resp: 42323  
Ion Ratio Lower Upper  
113 100  
111 102.7 81.9 122.9  
192 15.8 16.7 25.1#

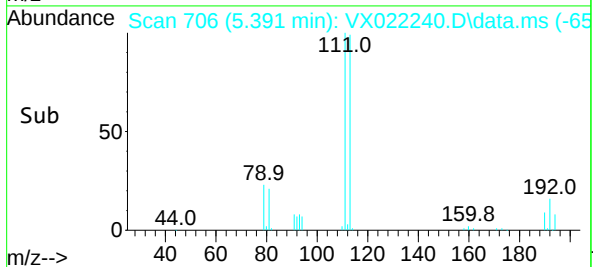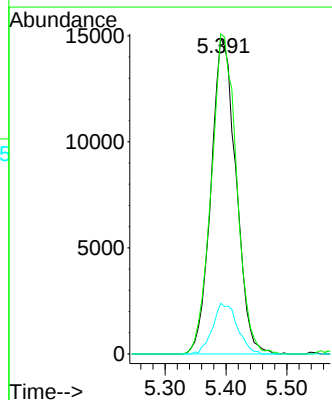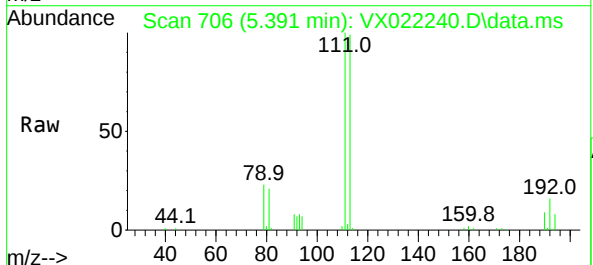



#36

1,1-Dichloropropene

Concen: 4.89 ug/l

RT: 5.562 min Scan# 734





Delta R.T. -0.140 min

Lab File: VX022240.D

Acq: 27 May 2021 18:14

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 75    | Resp: | 6424  |
| Ion      | Ratio | Lower | Upper |
| 75       | 100   |       |       |
| 110      | 8.7   | 18.1  | 54.4# |
| 77       | 0.0   | 25.3  | 37.9# |

Instrument :  
MSVOA\_X  
ClientSampleId :

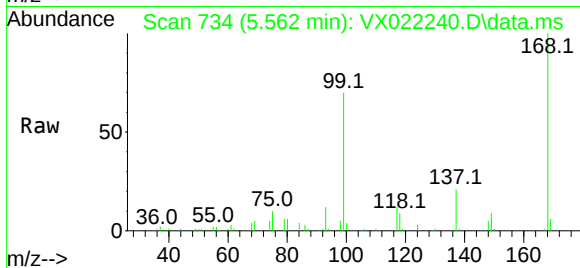

#38

Carbon Tetrachloride

Concen: 6.10 ug/l




RT: 5.568 min Scan# 735


Delta R.T. -0.122 min

Lab File: VX022240.D

Acq: 27 May 2021 18:14

|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 117   | Resp: | 7835   |
| Ion      | Ratio | Lower | Upper  |
| 117      | 100   |       |        |
| 119      | 5.4   | 76.2  | 114.2# |
| 121      | 0.0   | 24.8  | 37.2#  |


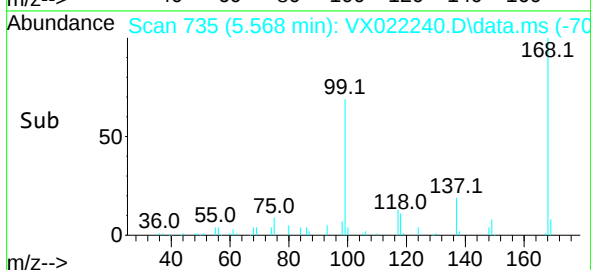
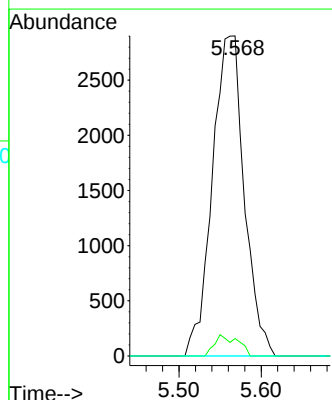
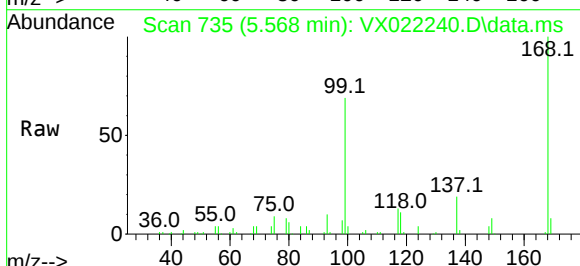




#44  
Trichloroethene  
Concen: 59.88 ug/l  
RT: 7.129 min Scan# 991  
Delta R.T. -0.000 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14




Instrument :  
MSVOA\_X  
ClientSampled :


Tgt Ion:130 Resp: 60150  
Ion Ratio Lower Upper  
130 100  
95 101.5 0.0 198.0

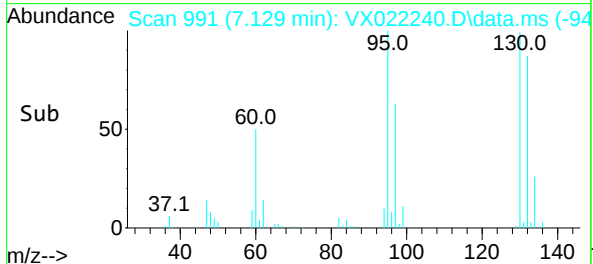

#50  
Toluene-d8  
Concen: 50.31 ug/l  
RT: 8.653 min Scan# 1241  
Delta R.T. -0.000 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14

Tgt Ion: 98 Resp: 174590  
Ion Ratio Lower Upper  
98 100  
100 66.3 51.9 77.9


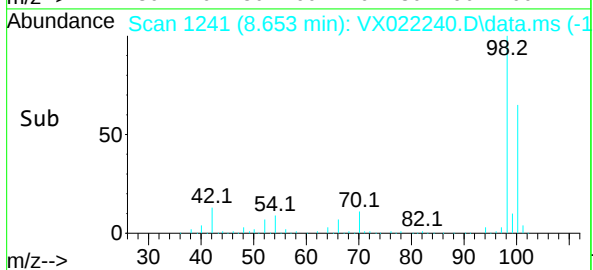

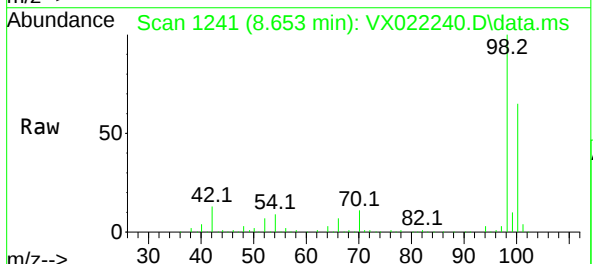




#62  
4-Bromofluorobenzene  
Concen: 45.70 ug/l  
RT: 11.085 min Scan# 1640  
Delta R.T. 0.000 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 95 Resp: 58626  
Ion Ratio Lower Upper  
95 100  
174 64.0 0.0 154.6  
176 60.3 0.0 155.8

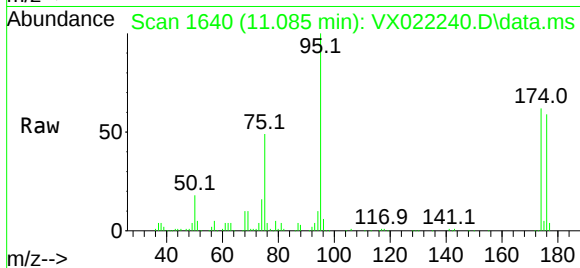

#63  
Chlorobenzene-d5  
Concen: 50.00 ug/l  
RT: 10.055 min Scan# 1471  
Delta R.T. -0.006 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14

Tgt Ion: 117 Resp: 124250  
Ion Ratio Lower Upper  
117 100  
82 57.5 47.4 71.2  
119 31.9 26.6 39.8


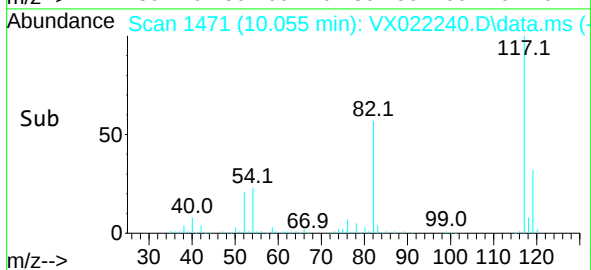

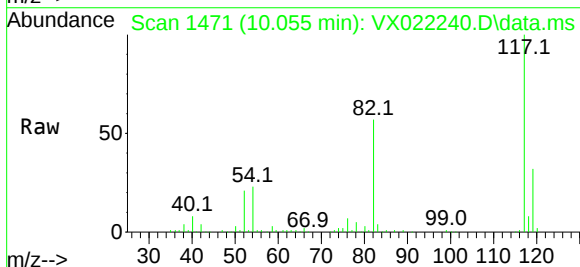




#68  
m/p-Xylenes  
Concen: 0.21 ug/l  
RT: 10.305 min Scan# 1512  
Delta R.T. 0.000 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion:106 Resp: 386  
Ion Ratio Lower Upper  
106 100  
91 286.5 162.8 244.2#

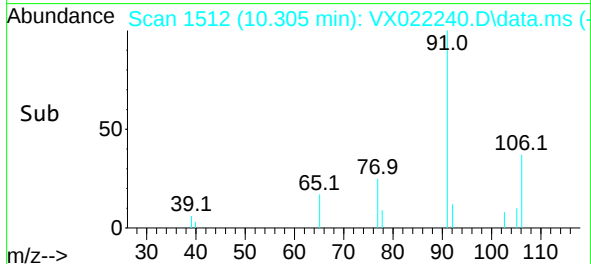

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.00 ug/l  
RT: 12.024 min Scan# 1794  
Delta R.T. 0.000 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14

Tgt Ion:152 Resp: 46299  
Ion Ratio Lower Upper  
152 100  
115 65.7 41.1 123.3  
150 158.1 0.0 349.0


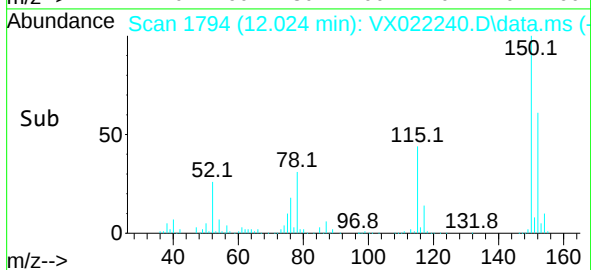

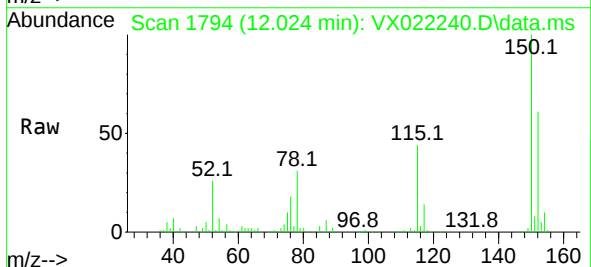




#76  
1,2,3-Trichloropropane  
Concen: 26.84 ug/l  
RT: 11.085 min Scan# 1640  
Delta R.T. -0.159 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14




Instrument :  
MSVOA\_X  
ClientSampled :


Tgt Ion: 75 Resp: 30656  
Ion Ratio Lower Upper  
75 100  
77 1.3 19.1 57.5#

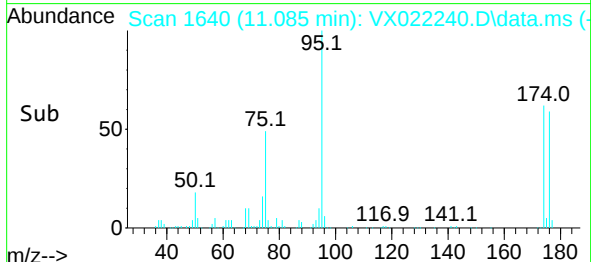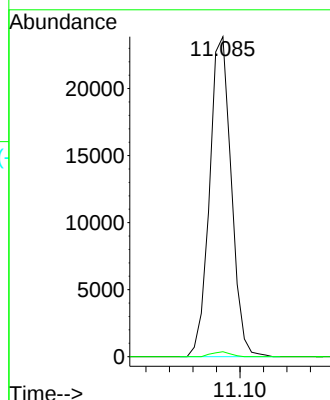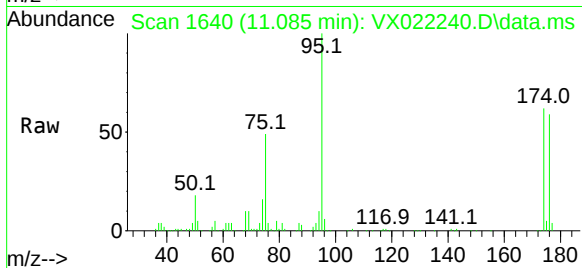

#78  
n-propylbenzene  
Concen: 0.24 ug/l  
RT: 11.305 min Scan# 1676  
Delta R.T. -0.000 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14

Tgt Ion: 91 Resp: 1107  
Ion Ratio Lower Upper  
91 100  
120 23.9 11.5 34.5


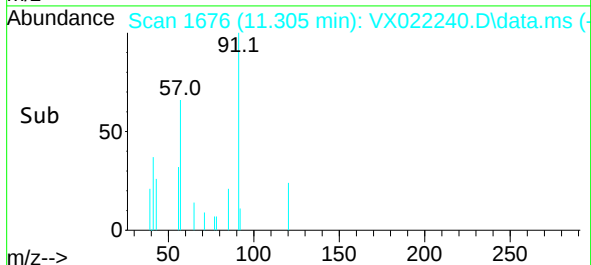
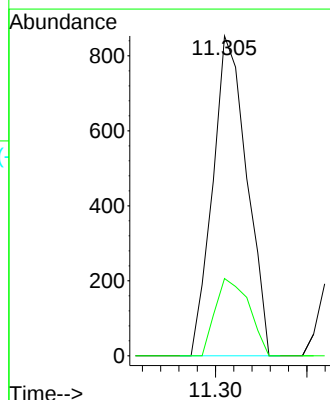
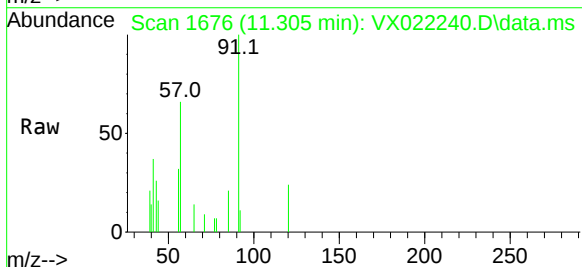




#81  
trans-1,4-Dichloro-2-butene  
Concen: 63.59 ug/l  
RT: 11.085 min Scan# 1640  
Delta R.T. 0.060 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14




Instrument :  
MSVOA\_X  
ClientSampled :


Tgt Ion: 75 Resp: 30656  
Ion Ratio Lower Upper  
75 100  
53 0.0 74.5 111.7#  
89 0.0 37.9 56.9#

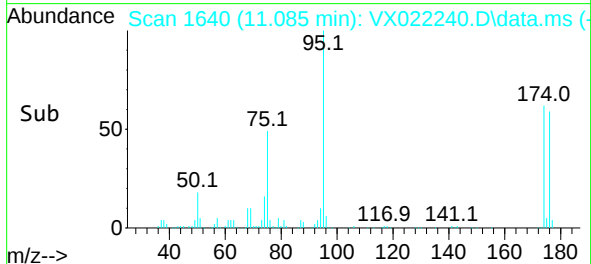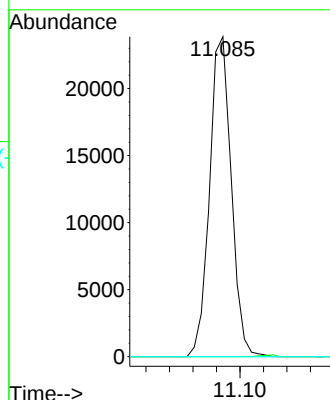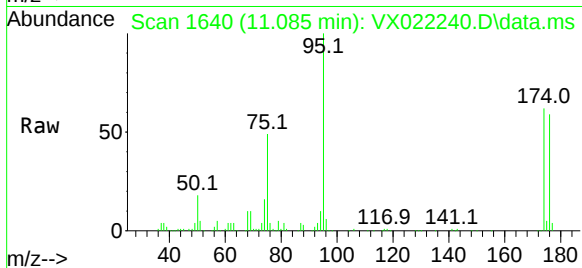

#84  
1,2,4-Trimethylbenzene  
Concen: 0.39 ug/l  
RT: 11.756 min Scan# 1750  
Delta R.T. 0.000 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14

Tgt Ion: 105 Resp: 1278  
Ion Ratio Lower Upper  
105 100  
120 34.0 22.4 67.3



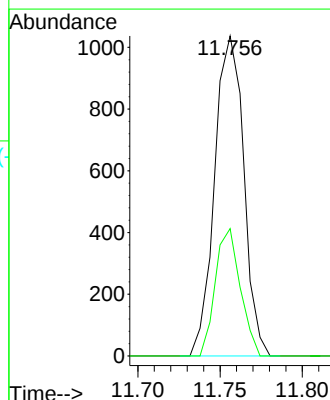
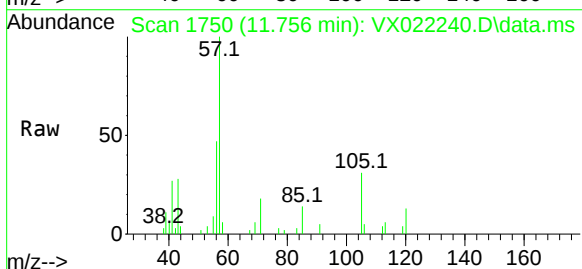




#88  
1,4-Dichlorobenzene  
Concen: 0.21 ug/l  
RT: 12.049 min Scan# 1798  
Delta R.T. 0.006 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14




Instrument :  
MSVOA\_X  
ClientSampled :


Tgt Ion:146 Resp: 356  
Ion Ratio Lower Upper  
146 100  
111 0.0 19.6 58.8#  
148 0.0 31.6 95.0#

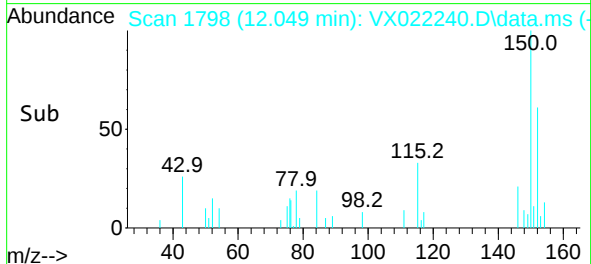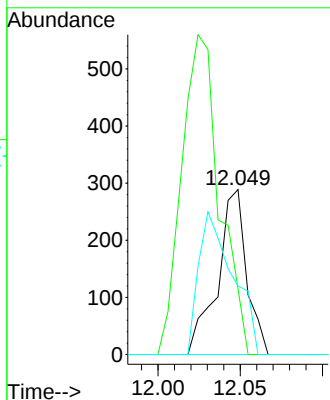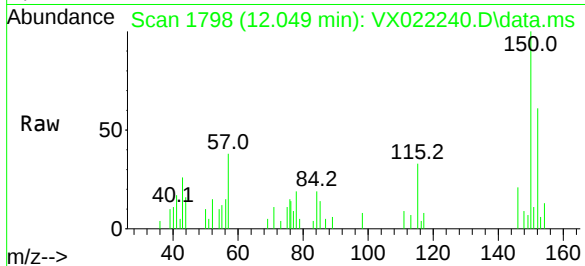

#89  
n-Butylbenzene  
Concen: 0.24 ug/l  
RT: 12.335 min Scan# 1845  
Delta R.T. 0.000 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14


Tgt Ion: 91 Resp: 749  
Ion Ratio Lower Upper  
91 100  
92 44.1 27.4 82.0  
134 38.9 13.2 39.5

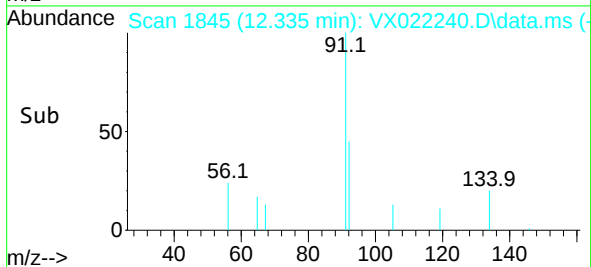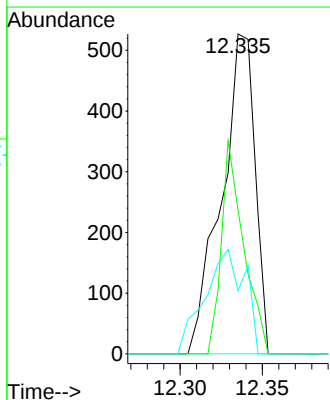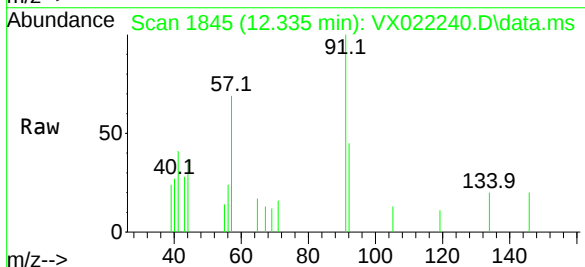






#90  
Hexachloroethane  
Concen: 0.23 ug/l  
RT: 12.707 min Scan# 1906  
Delta R.T. 0.164 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14


Instrument :  
MSVOA\_X  
ClientSampled :

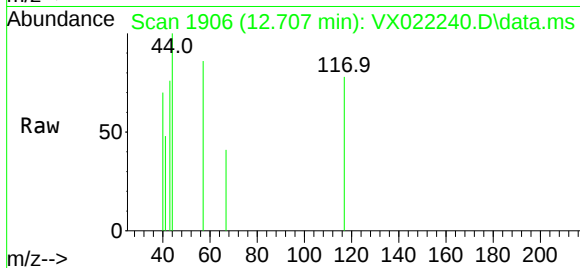



Tgt Ion:117 Resp: 125  
Ion Ratio Lower Upper  
117 100  
201 0.0 40.4 121.2#

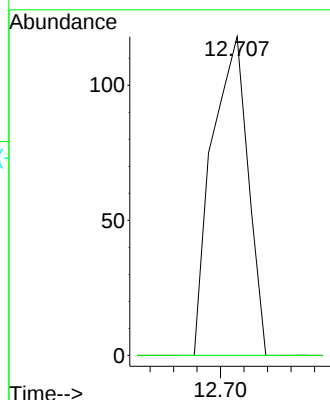


#93  
1,2,4-Trichlorobenzene  
Concen: 0.25 ug/l  
RT: 13.591 min Scan# 2051  
Delta R.T. 0.000 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14

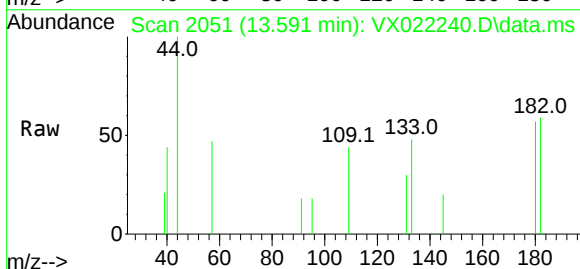


Tgt Ion:180 Resp: 228  
Ion Ratio Lower Upper  
180 100  
182 89.9 47.7 143.1  
145 18.0 15.0 45.0

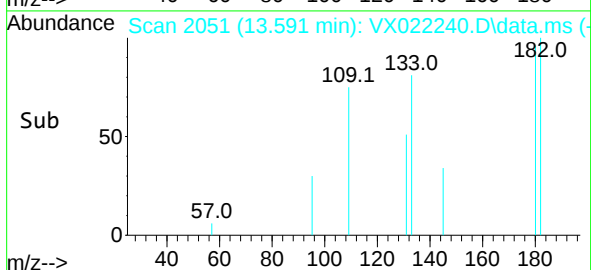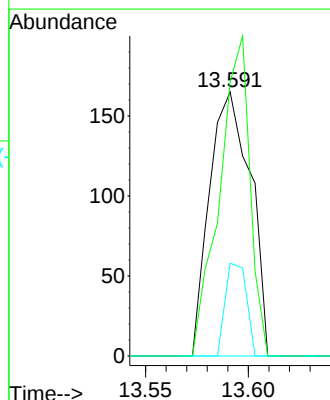






#94  
Hexachlorobutadiene  
Concen: 0.39 ug/l  
RT: 13.719 min Scan# 2072  
Delta R.T. -0.012 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14


Instrument :  
MSVOA\_X  
ClientSampled :

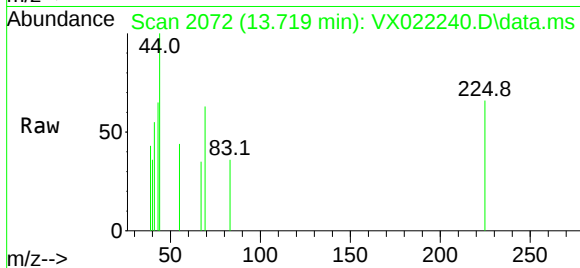

Tgt Ion:225 Resp: 140  
Ion Ratio Lower Upper  
225 100  
223 0.0 31.1 93.2#  
227 0.0 31.6 95.0#



#95  
Naphthalene  
Concen: 0.27 ug/l  
RT: 13.780 min Scan# 2082  
Delta R.T. 0.000 min  
Lab File: VX022240.D  
Acq: 27 May 2021 18:14

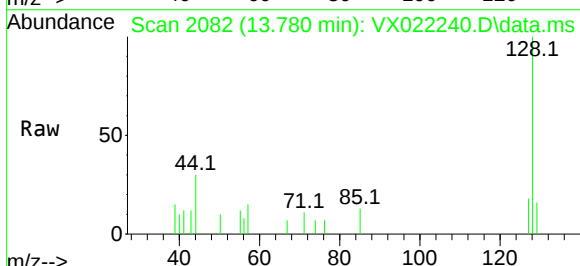

Tgt Ion:128 Resp: 960  
Ion Ratio Lower Upper  
128 100  
127 11.8 10.3 15.5  
129 11.5 8.8 13.2

