

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052821\
 Data File : VX022246.D
 Acq On : 27 May 2021 20:35
 Operator : JC/MD
 Sample : M2520-02 40X
 Misc : 15.039g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-02-2021-05-24


Quant Time: May 28 01:35:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 19 14:23:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	70286	50.00	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.769	114	143203	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	128253	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	53525	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	56850	52.43	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 104.86%			
35) Dibromofluoromethane	5.397	113	43388	47.78	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 95.56%			
50) Toluene-d8	8.653	98	177794	50.82	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 101.64%			
62) 4-Bromofluorobenzene	11.085	95	63604	49.19	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 98.38%			
Target Compounds						Qvalue
3) Chloromethane	1.294	50	202	0.22	ug/l	# 88
5) Bromomethane	1.605	94	243	0.43	ug/l	82
10) Methyl Iodide	2.465	142	382	0.43	ug/l	# 89
11) Tert butyl alcohol	2.959	59	858	3.46	ug/l	# 73
13) Acrolein	2.148	56	49	0.30	ug/l	# 1
15) Acrylonitrile	3.068	53	111	0.23	ug/l	# 36
16) Acetone	2.386	43	542	1.15	ug/l	# 83
17) Carbon Disulfide	2.514	76	496	0.24	ug/l	# 75
18) Methyl Acetate	2.703	43	273	0.22	ug/l	# 47
20) Methylene Chloride	2.794	84	624	0.60	ug/l	# 85
31) Cyclohexane	5.550	56	1836	1.35	ug/l	# 27
36) 1,1-Dichloropropene	5.556	75	6476	4.89	ug/l	# 47
38) Carbon Tetrachloride	5.556	117	7555	5.83	ug/l	# 15
44) Trichloroethene	7.123	130	337	0.33	ug/l	77
51) 4-Methyl-2-Pentanone	8.653	43	937	0.59	ug/l	# 1
67) Ethyl Benzene	10.195	91	77015	15.68	ug/l	96
68) m/p-Xylenes	10.305	106	1880	1.01	ug/l	96
69) o-Xylene	10.652	106	1699	0.94	ug/l	85
73) Isopropylbenzene	10.969	105	13502	2.98	ug/l	100
76) 1,2,3-Trichloropropane	11.085	75	32781	24.83	ug/l	# 39
78) n-propylbenzene	11.305	91	5357	1.01	ug/l	99
80) 1,3,5-Trimethylbenzene	11.451	105	1539	0.41	ug/l	83
81) trans-1,4-Dichloro-2-b...	11.085	75	32781	58.82	ug/l	# 12
83) tert-Butylbenzene	11.975	119	4139	1.15	ug/l	70
84) 1,2,4-Trimethylbenzene	11.756	105	51465	13.62	ug/l	97
85) sec-Butylbenzene	11.756	105	51465	11.25	ug/l	# 57
86) p-Isopropyltoluene	12.012	119	5211	1.35	ug/l	90
89) n-Butylbenzene	12.329	91	4292	1.20	ug/l	# 37
90) Hexachloroethane	12.701	117	13077	20.47	ug/l	# 9
92) 1,2-Dibromo-3-Chloropr...	12.969	75	200	0.62	ug/l	# 1
93) 1,2,4-Trichlorobenzene	13.591	180	368	0.34	ug/l	# 40
95) Naphthalene	13.780	128	1391229	332.34	ug/l	100
96) 1,2,3-Trichlorobenzene	13.963	180	263	0.24	ug/l	# 12

(#) = qualifier out of range (m) = manual integration (+) = signals summed





Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24

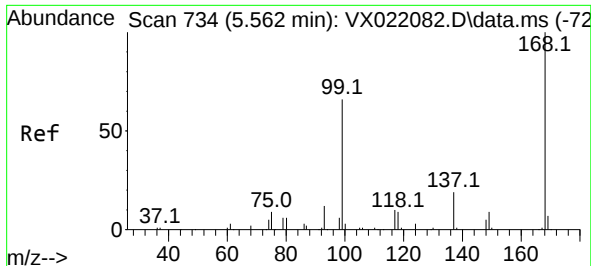

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion:168 Resp: 70286
Ion Ratio Lower Upper
168 100
99 69.7 45.8 68.6#

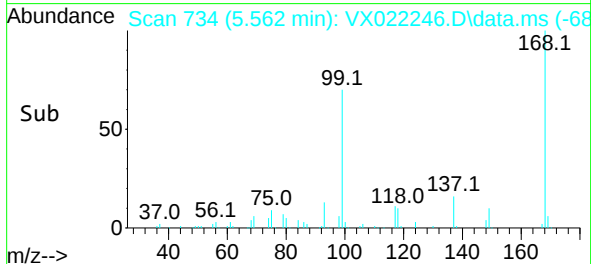

#3
Chloromethane
Concen: 0.22 ug/l
RT: 1.294 min Scan# 34
Delta R.T. -0.001 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35

Tgt Ion: 50 Resp: 202
Ion Ratio Lower Upper
50 100
52 26.2 26.4 39.6#


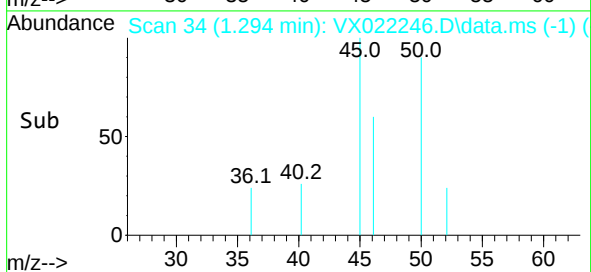

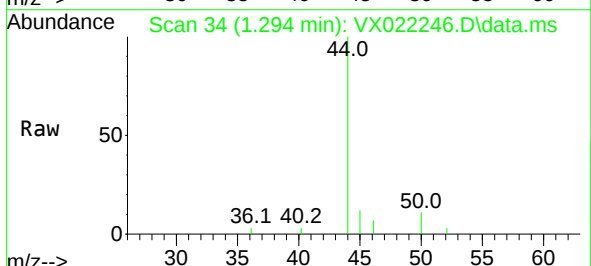


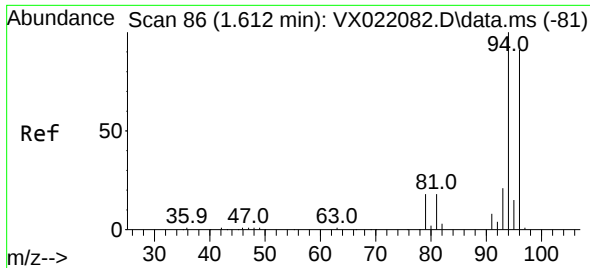

#5
Bromomethane
Concen: 0.43 ug/l
RT: 1.605 min Scan# 85
Delta R.T. -0.007 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion: 94 Resp: 243
Ion Ratio Lower Upper
94 100
96 78.0 76.4 114.6

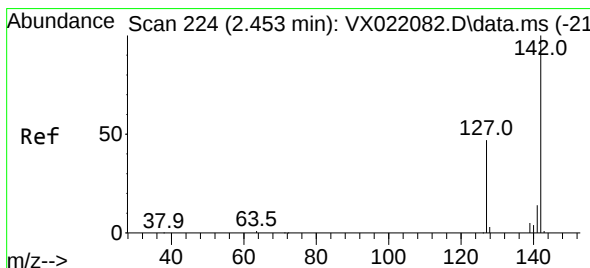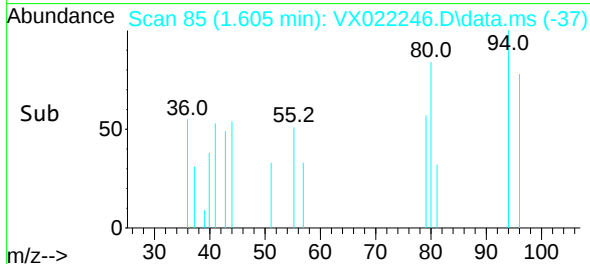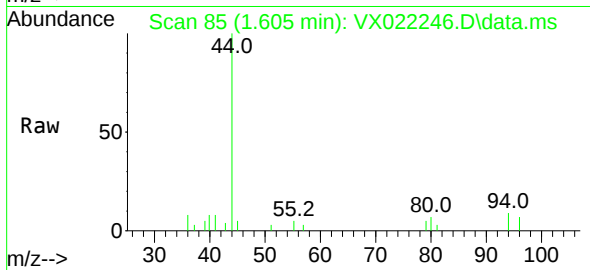

#10
Methyl Iodide
Concen: 0.43 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.012 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35

Tgt Ion: 142 Resp: 382
Ion Ratio Lower Upper
142 100
127 43.7 33.3 49.9
141 0.0 11.4 17.0#

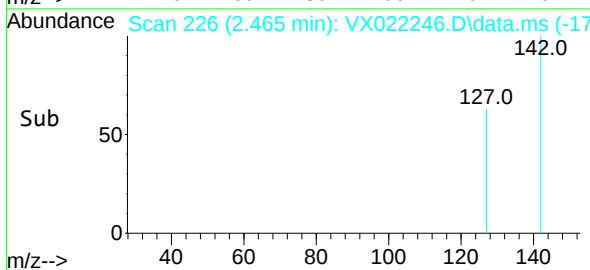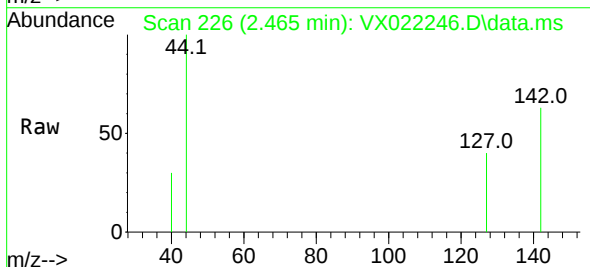




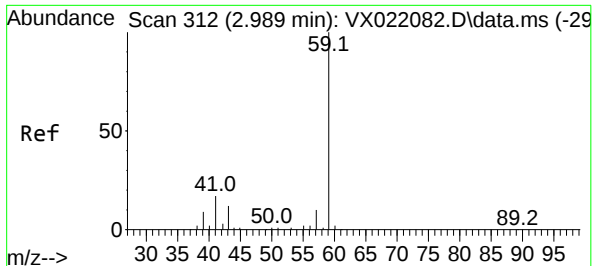


#11

Tert butyl alcohol
Concen: 3.46 ug/l
RT: 2.959 min Scan# 307
Delta R.T. -0.030 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35

Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24




Tgt Ion: 59 Resp: 858
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#

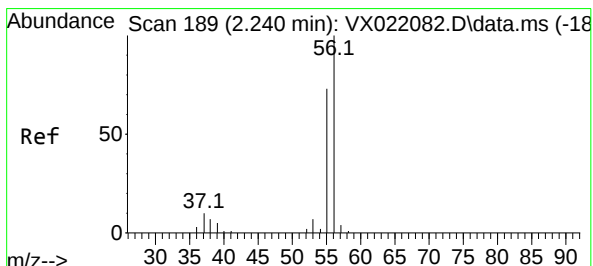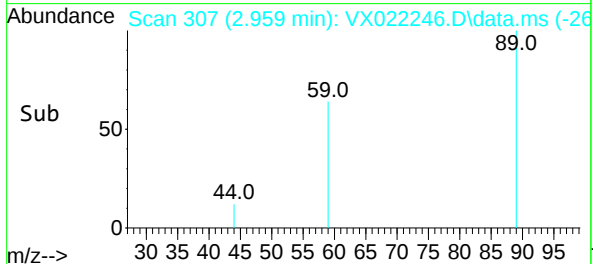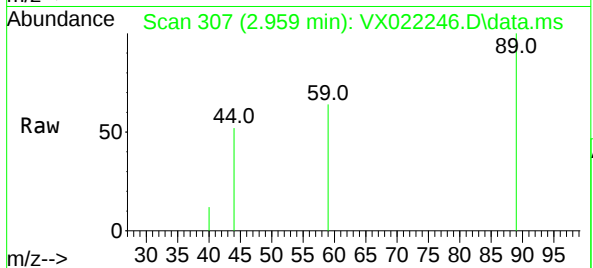


#13

Acrolein
Concen: 0.30 ug/l
RT: 2.148 min Scan# 174
Delta R.T. -0.092 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35

Tgt Ion: 56 Resp: 49
Ion Ratio Lower Upper
56 100
55 326.5 56.4 84.6#


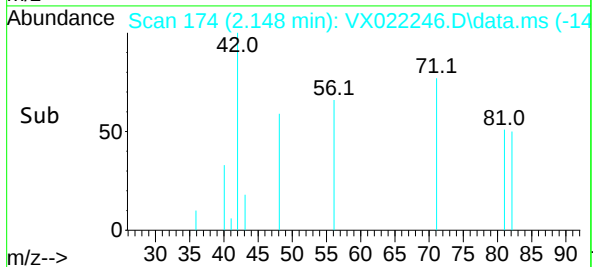

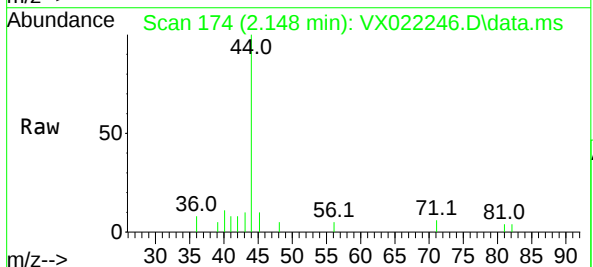


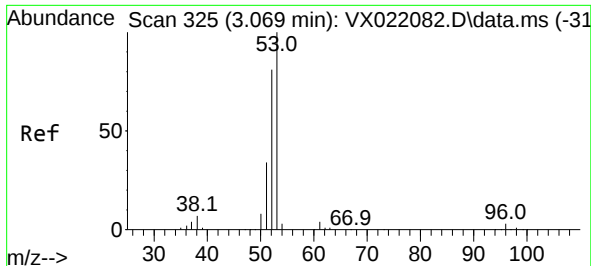

#15
Acrylonitrile
Concen: 0.23 ug/l
RT: 3.068 min Scan# 325
Delta R.T. -0.001 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion: 53	Resp:	111
Ion Ratio	Lower	Upper
53	100	
52	22.5	65.3 97.9#
51	0.0	28.2 42.2#

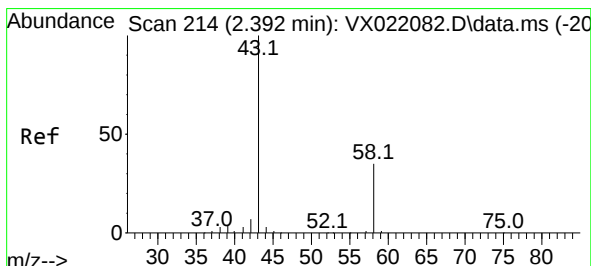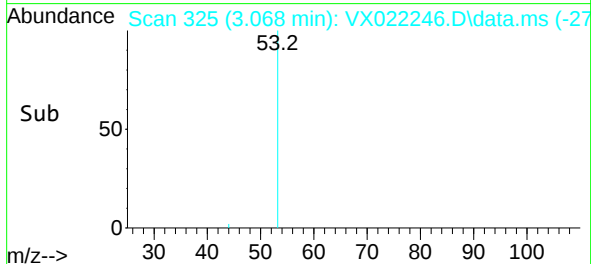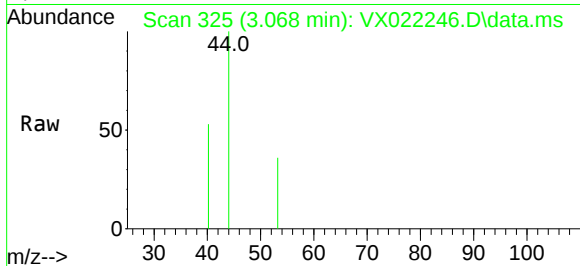

#16
Acetone
Concen: 1.15 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35

Tgt Ion: 43	Resp:	542
Ion Ratio	Lower	Upper
43	100	
58	25.0	27.8 41.8#


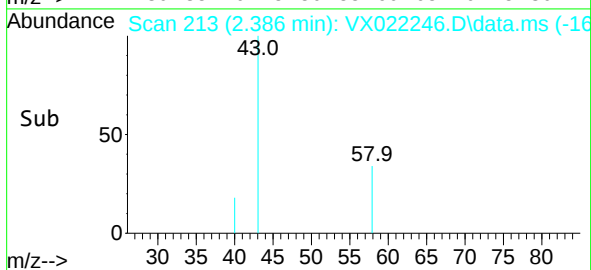

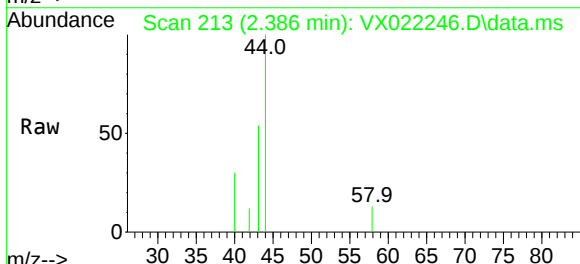


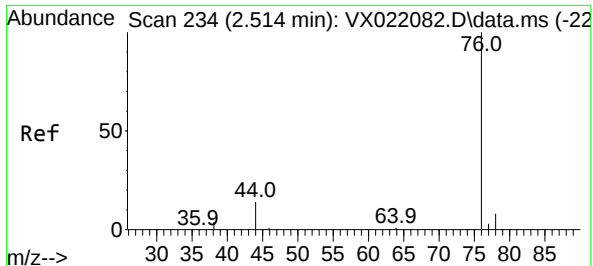

#17
Carbon Disulfide
Concen: 0.24 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion: 76 Resp: 496
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

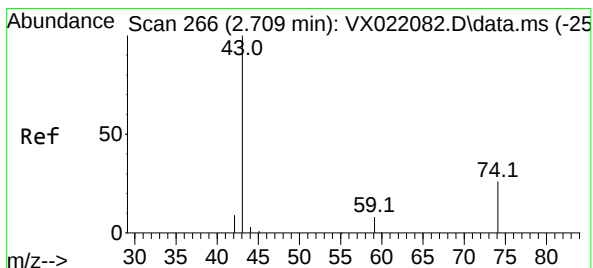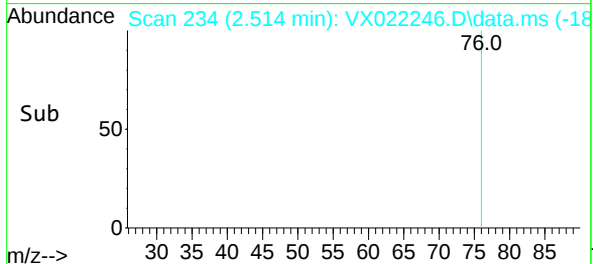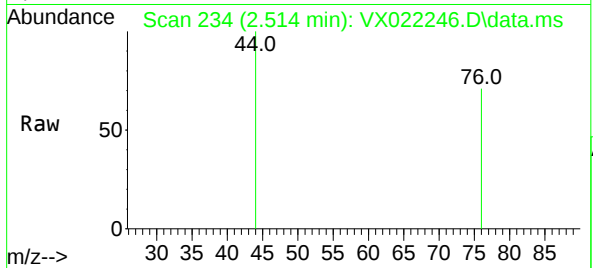

#18
Methyl Acetate
Concen: 0.22 ug/l
RT: 2.703 min Scan# 265
Delta R.T. -0.006 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35

Tgt Ion: 43 Resp: 273
Ion Ratio Lower Upper
43 100
74 0.0 21.9 32.9#

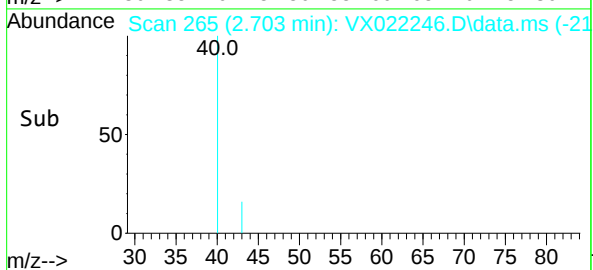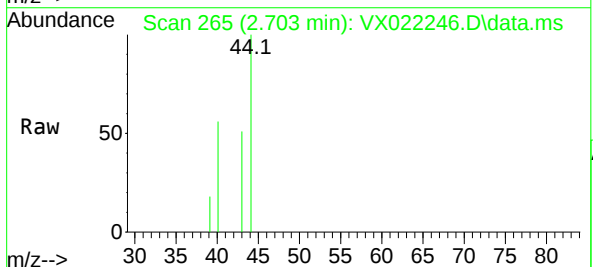

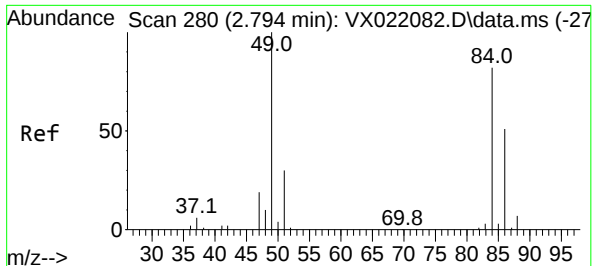

#20

Methylene Chloride

Concen: 0.60 ug/l

RT: 2.794 min Scan# 280

Delta R.T. 0.000 min

Lab File: VX022246.D

Acq: 27 May 2021 20:35

Tgt Ion: 84 Resp: 624





Ion Ratio Lower Upper

84 100

49 107.4 88.6 132.8

51 41.4 27.0 40.6#

86 91.0 50.3 75.5#

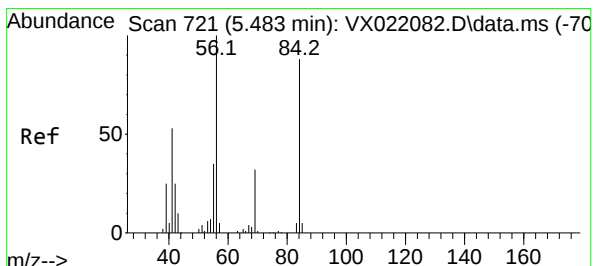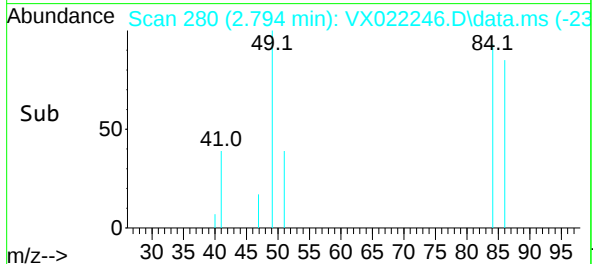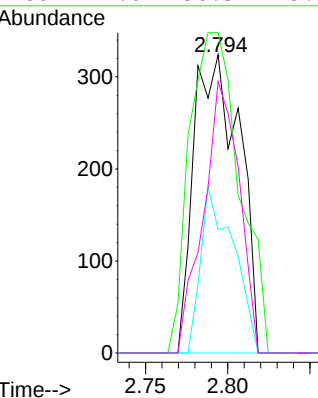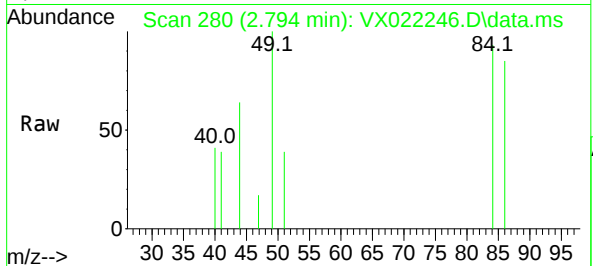

#31

Cyclohexane

Concen: 1.35 ug/l

RT: 5.550 min Scan# 732

Delta R.T. 0.067 min

Lab File: VX022246.D

Acq: 27 May 2021 20:35




Tgt Ion: 56 Resp: 1836


Ion Ratio Lower Upper

56 100

69 132.4 25.3 37.9#

84 120.9 71.4 107.0#

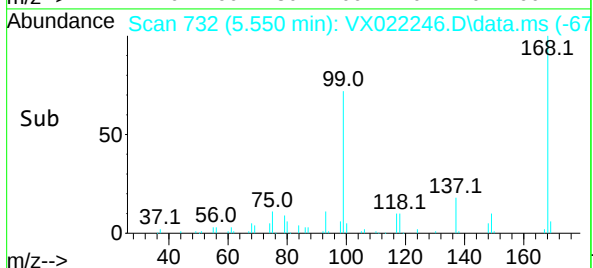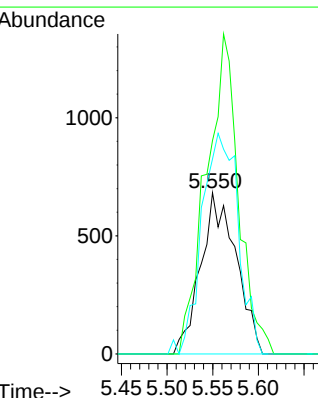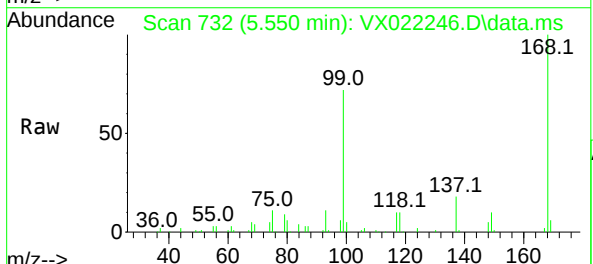

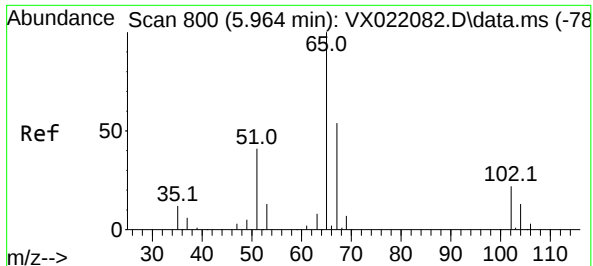

#33

1,2-Dichloroethane-d4

Concen: 52.43 ug/l

RT: 5.964 min Scan# 800

Delta R.T. 0.000 min

Lab File: VX022246.D

Acq: 27 May 2021 20:35

Tgt Ion: 65 Resp: 56850

Ion Ratio Lower Upper

65 100





67 51.8 0.0 105.4

Instrument :

MSVOA_X

ClientSampleId :

WC-02-2021-05-24

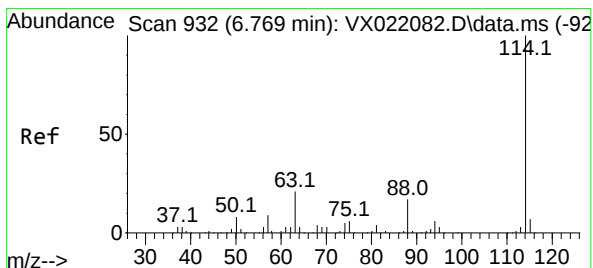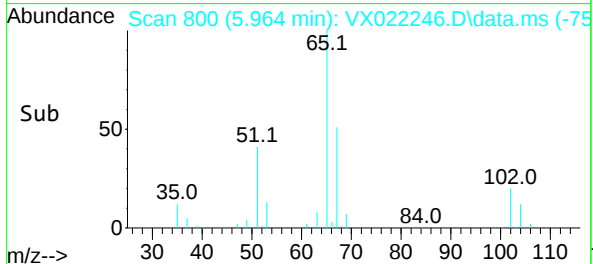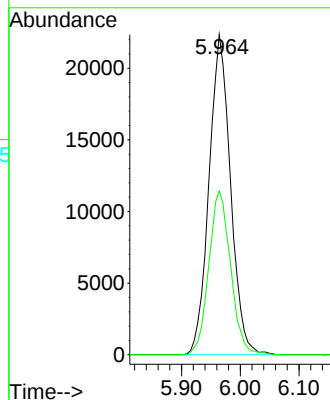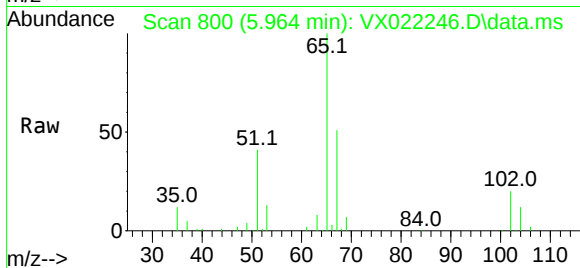

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.769 min Scan# 932

Delta R.T. -0.000 min

Lab File: VX022246.D

Acq: 27 May 2021 20:35




Tgt Ion: 114 Resp: 143203


Ion Ratio Lower Upper

114 100

63 21.3 0.0 40.8

88 15.3 0.0 32.8

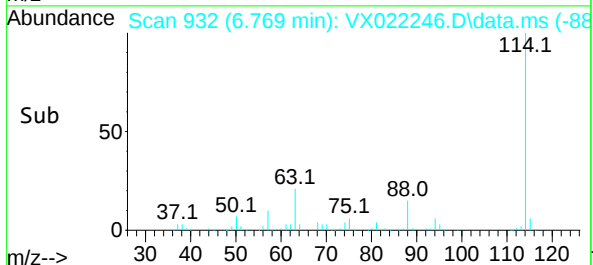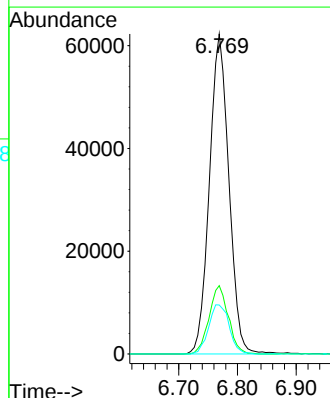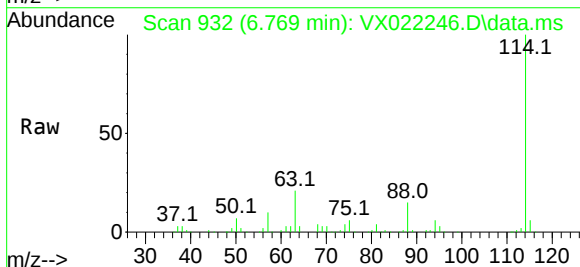

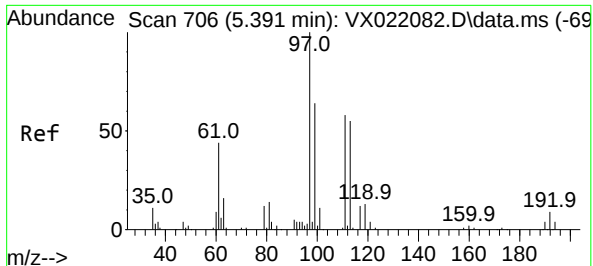

#35

Dibromofluoromethane

Concen: 47.78 ug/l

RT: 5.397 min Scan# 707

Delta R.T. 0.006 min

Lab File: VX022246.D

Acq: 27 May 2021 20:35





Tgt Ion:113 Resp: 43388

Ion Ratio Lower Upper

113 100

111 101.6 81.9 122.9

192 15.4 16.7 25.1#

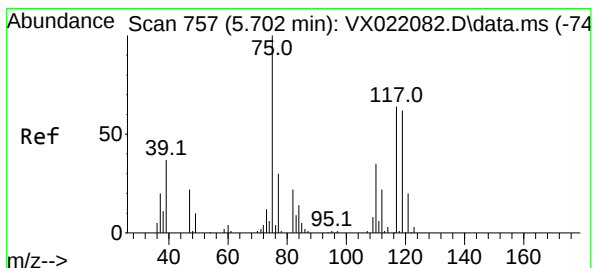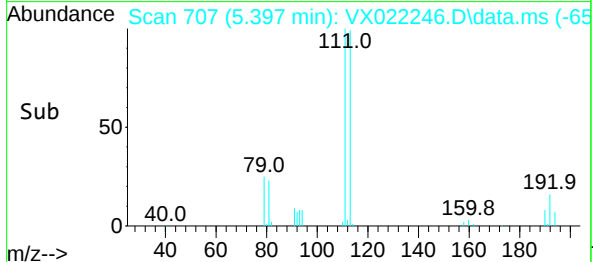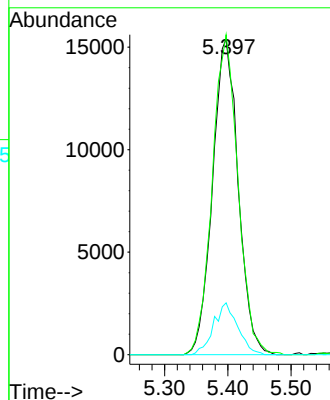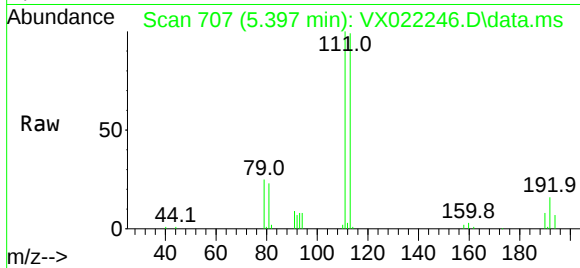

#36

1,1-Dichloropropene

Concen: 4.89 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.146 min

Lab File: VX022246.D

Acq: 27 May 2021 20:35




Tgt Ion: 75 Resp: 6476


Ion Ratio Lower Upper

75 100

110 7.4 18.1 54.4#


77 0.0 25.3 37.9#

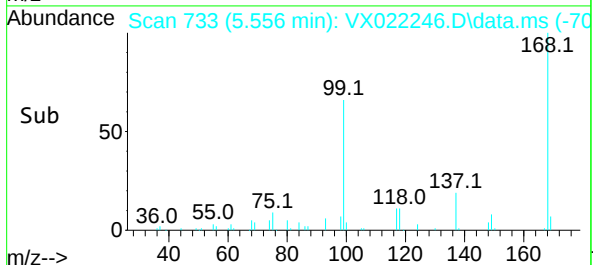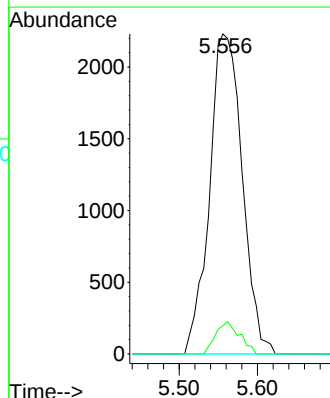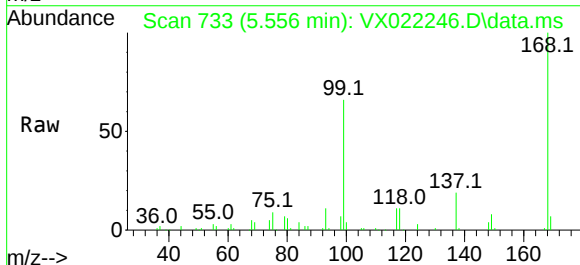



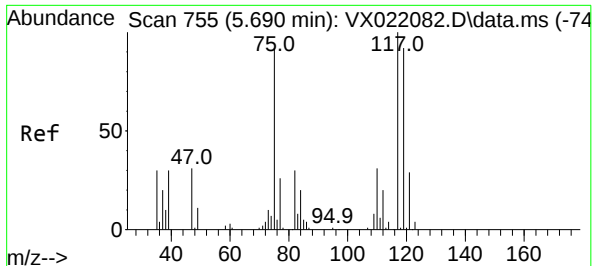


#38
Carbon Tetrachloride
Concen: 5.83 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.134 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35

Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24



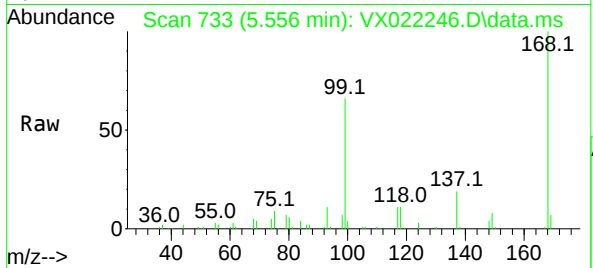



Tgt Ion:117 Resp: 7555
Ion Ratio Lower Upper
117 100
119 3.8 76.2 114.2#
121 0.0 24.8 37.2#

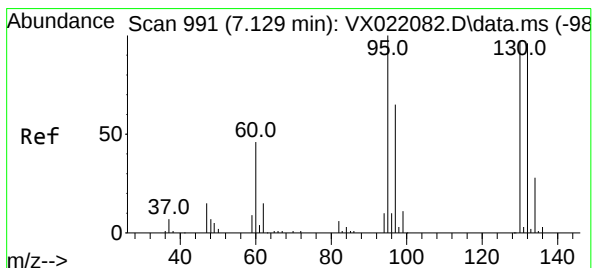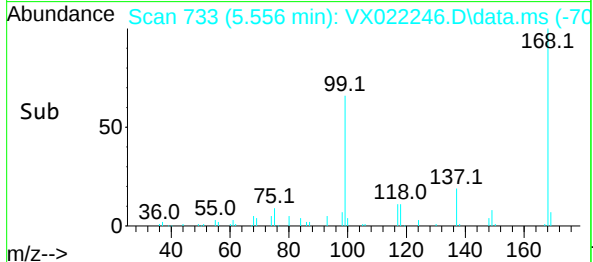

#44
Trichloroethene
Concen: 0.33 ug/l
RT: 7.123 min Scan# 990
Delta R.T. -0.006 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35

Tgt Ion:130 Resp: 337
Ion Ratio Lower Upper
130 100
95 76.5 0.0 198.0


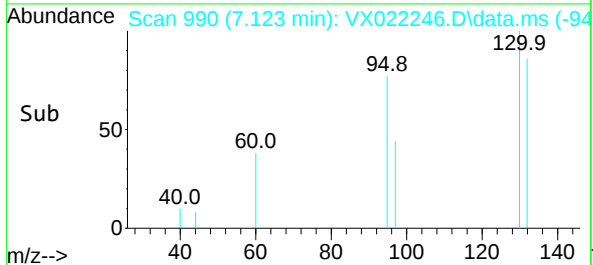

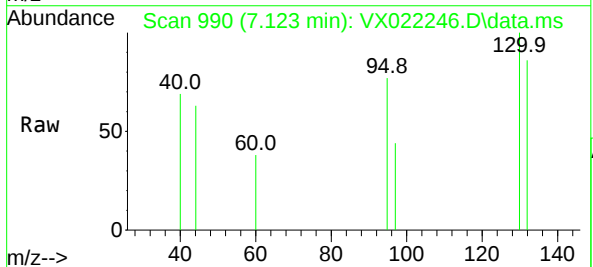




#50
Toluene-d8
Concen: 50.82 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion: 98 Resp: 177794
Ion Ratio Lower Upper
98 100
100 65.4 51.9 77.9

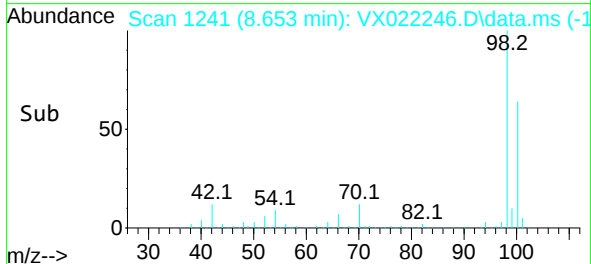

#51
4-Methyl-2-Pentanone
Concen: 0.59 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.073 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35

Tgt Ion: 43 Resp: 937
Ion Ratio Lower Upper
43 100
58 160.2 35.4 53.0#


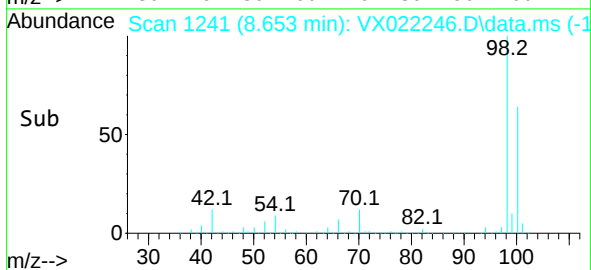

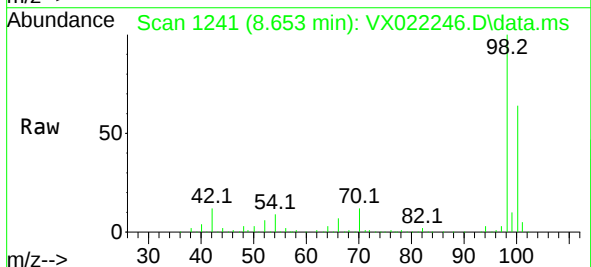




#62
4-Bromofluorobenzene
Concen: 49.19 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion: 95 Resp: 63604
Ion Ratio Lower Upper
95 100
174 62.6 0.0 154.6
176 61.5 0.0 155.8

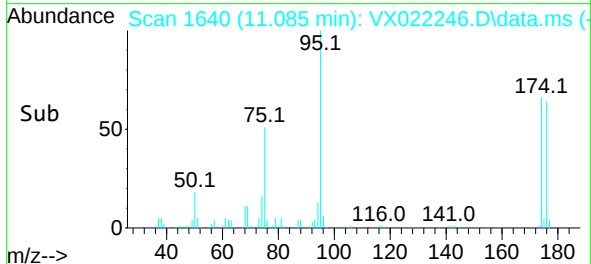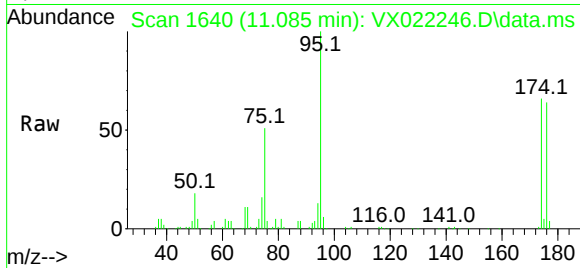

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35

Tgt Ion: 117 Resp: 128253
Ion Ratio Lower Upper
117 100
82 60.9 47.4 71.2
119 32.1 26.6 39.8


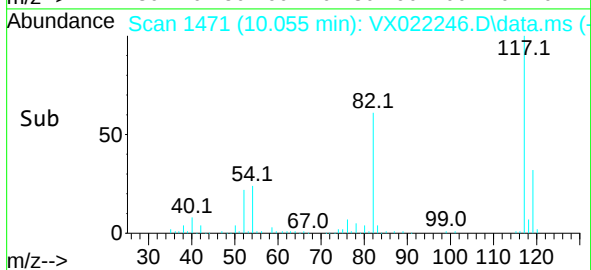

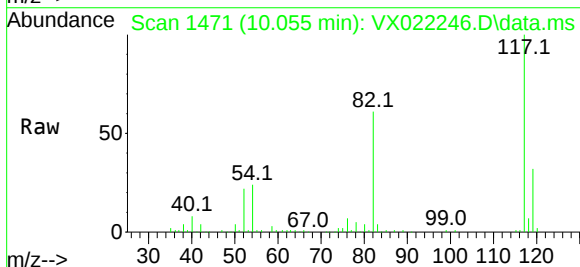




#67
Ethyl Benzene
Concen: 15.68 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion: 91 Resp: 77015
Ion Ratio Lower Upper
91 100
106 28.7 24.6 37.0

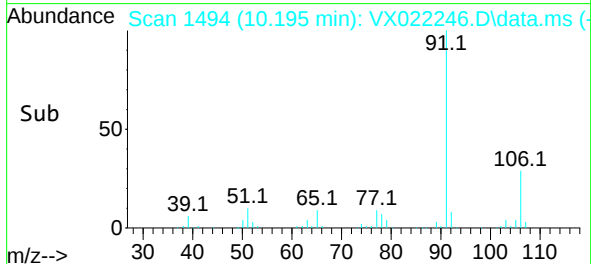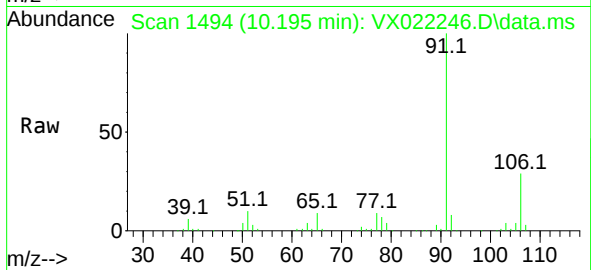

#68
m/p-Xylenes
Concen: 1.01 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35

Tgt Ion: 106 Resp: 1880
Ion Ratio Lower Upper
106 100
91 210.4 162.8 244.2


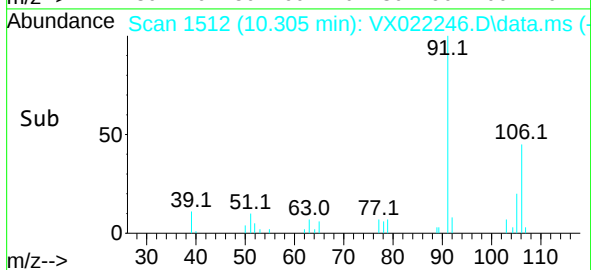

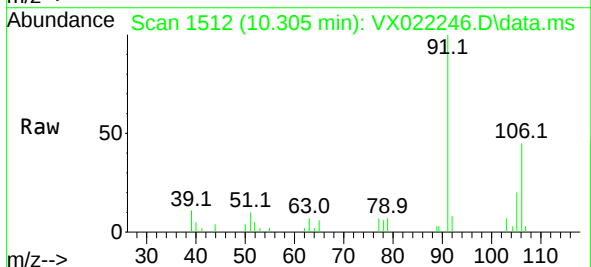




#69
o-Xylene
Concen: 0.94 ug/l
RT: 10.652 min Scan# 1569
Delta R.T. 0.005 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion:106 Resp: 1699
Ion Ratio Lower Upper
106 100
91 239.4 108.1 324.2

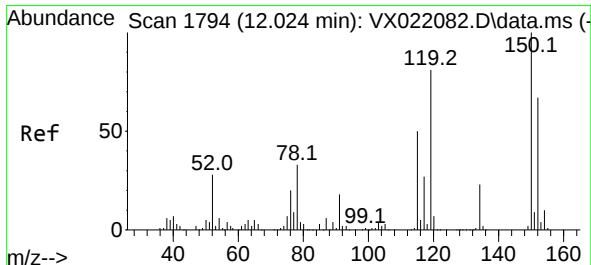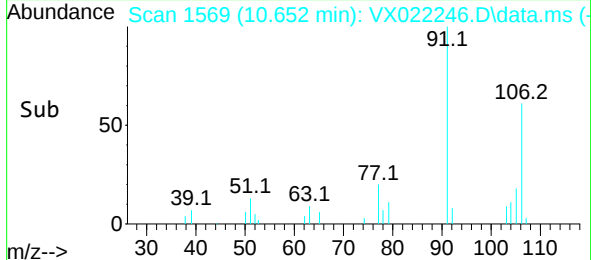

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35

Tgt Ion:152 Resp: 53525
Ion Ratio Lower Upper
152 100
115 68.5 41.1 123.3
150 159.7 0.0 349.0

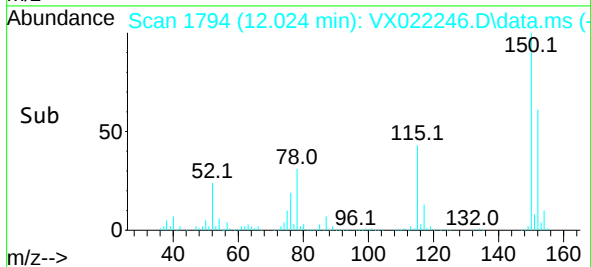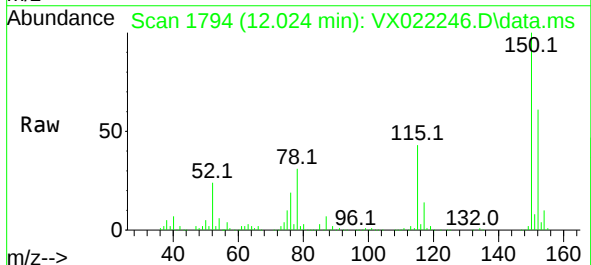



#73

Isopropylbenzene

Concen: 2.98 ug/l

RT: 10.969 min Scan# 1621

Delta R.T. 0.005 min

Lab File: VX022246.D





Acq: 27 May 2021 20:35

Tgt Ion: 105 Resp: 13502

Ion Ratio Lower Upper

105 100

120 26.3 13.2 39.6

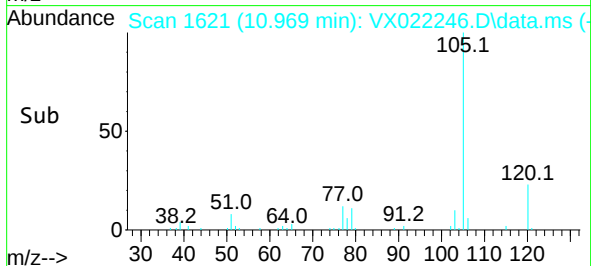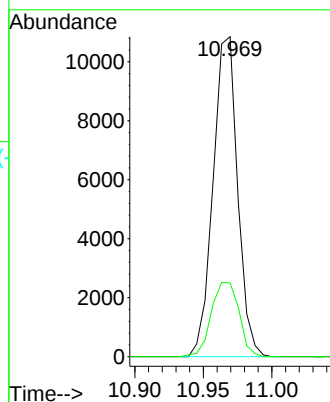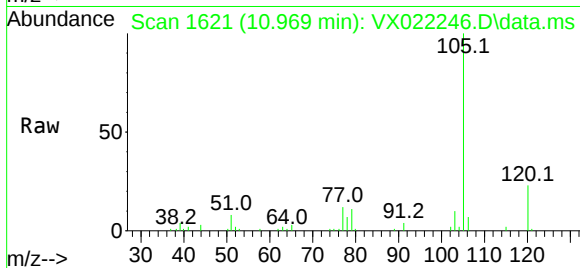

#76

1,2,3-Trichloropropane

Concen: 24.83 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. -0.159 min

Lab File: VX022246.D




Acq: 27 May 2021 20:35


Tgt Ion: 75 Resp: 32781

Ion Ratio Lower Upper

75 100

77 1.2 19.1 57.5#

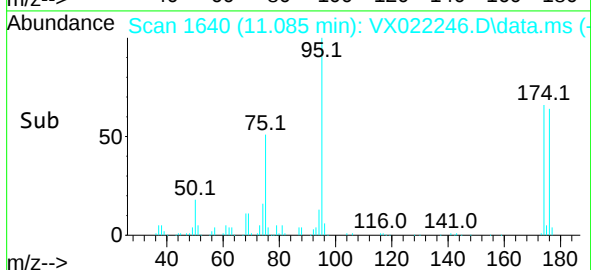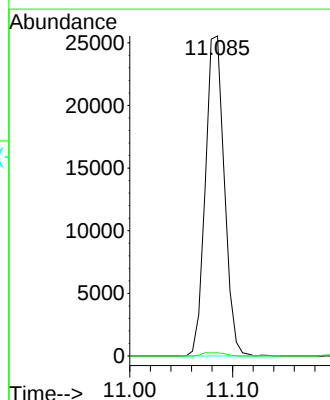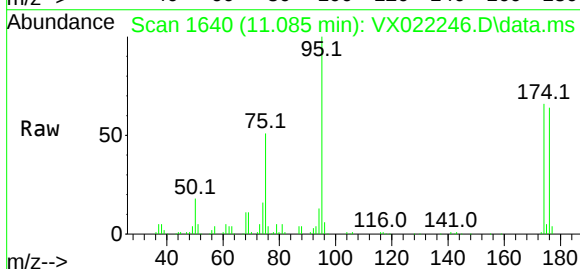

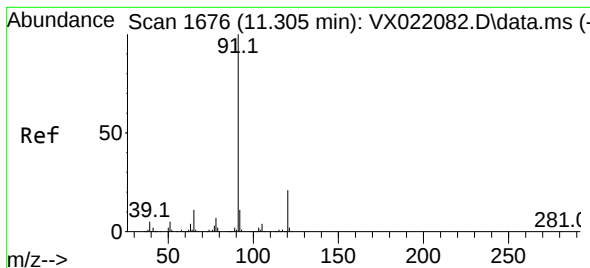

#78

n-propylbenzene

Concen: 1.01 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.000 min

Lab File: VX022246.D

Acq: 27 May 2021 20:35

Instrument :

MSVOA_X

ClientSampleId :





WC-02-2021-05-24

Tgt Ion: 91 Resp: 5357

Ion Ratio Lower Upper

91 100

120 23.7 11.5 34.5

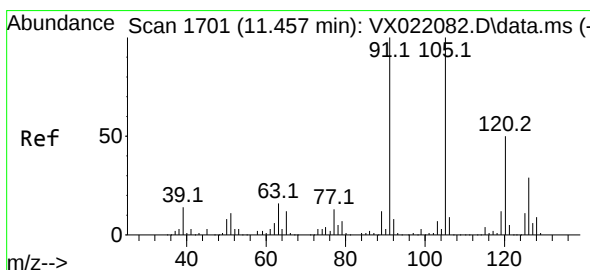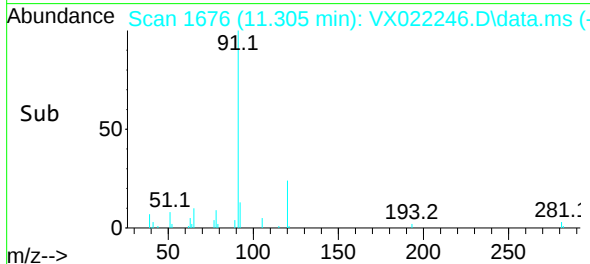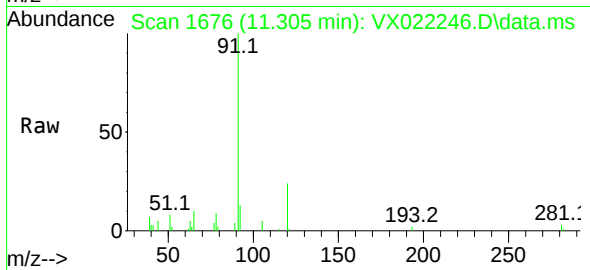

#80

1,3,5-Trimethylbenzene

Concen: 0.41 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. -0.006 min

Lab File: VX022246.D




Acq: 27 May 2021 20:35


Tgt Ion: 105 Resp: 1539

Ion Ratio Lower Upper

105 100

120 36.5 23.8 71.5


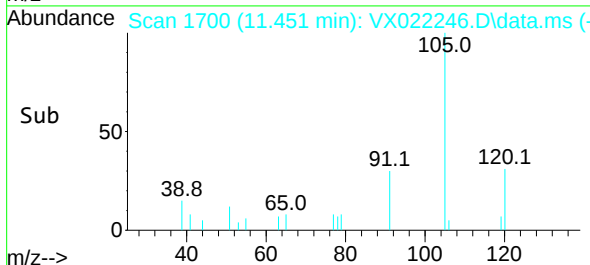

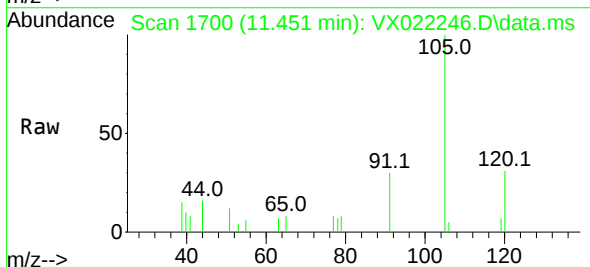




#81
 trans-1,4-Dichloro-2-butene
 Concen: 58.82 ug/l
 RT: 11.085 min Scan# 1640
 Delta R.T. 0.060 min
 Lab File: VX022246.D
 Acq: 27 May 2021 20:35




Instrument :
 MSVOA_X
 ClientSampleId :
 WC-02-2021-05-24


Tgt Ion: 75 Resp: 32781
 Ion Ratio Lower Upper
 75 100
 53 0.0 74.5 111.7#
 89 0.0 37.9 56.9#

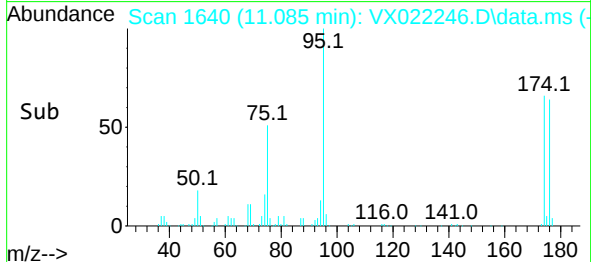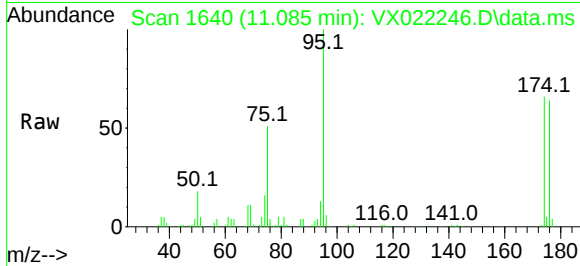

#83
 tert-Butylbenzene
 Concen: 1.15 ug/l
 RT: 11.975 min Scan# 1786
 Delta R.T. 0.255 min
 Lab File: VX022246.D
 Acq: 27 May 2021 20:35

Tgt Ion: 119 Resp: 4139
 Ion Ratio Lower Upper
 119 100
 91 29.8 27.9 83.7
 134 30.9 11.3 33.9


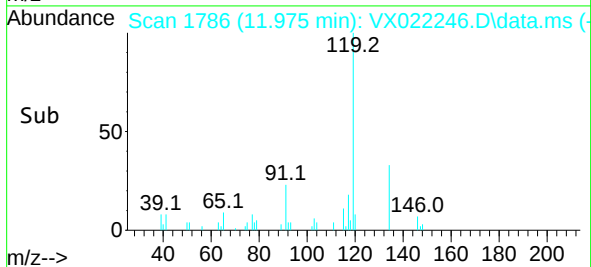

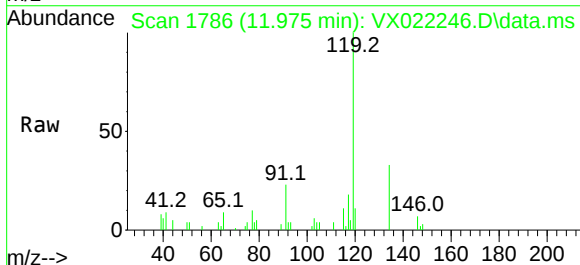


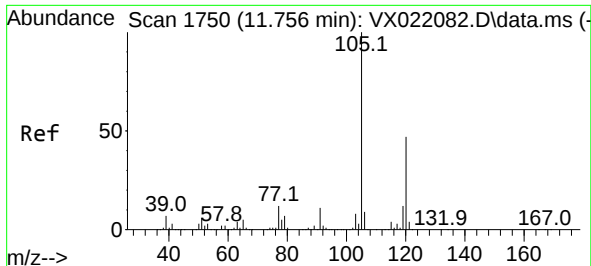

#84
1,2,4-Trimethylbenzene
Concen: 13.62 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion:105 Resp: 51465
Ion Ratio Lower Upper
105 100
120 42.9 22.4 67.3

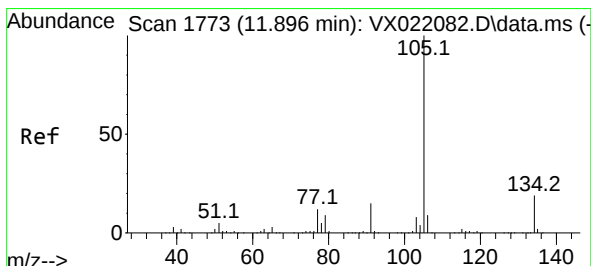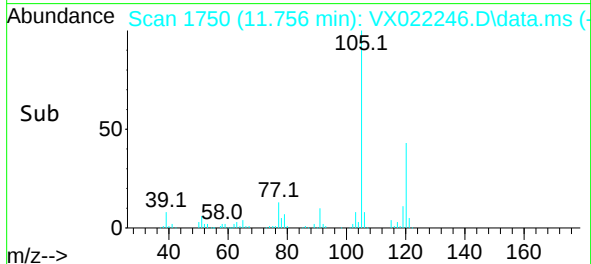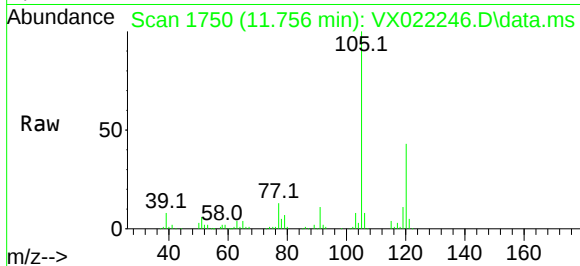

#85
sec-Butylbenzene
Concen: 11.25 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.140 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35

Tgt Ion:105 Resp: 51465
Ion Ratio Lower Upper
105 100
134 0.0 10.0 29.8#


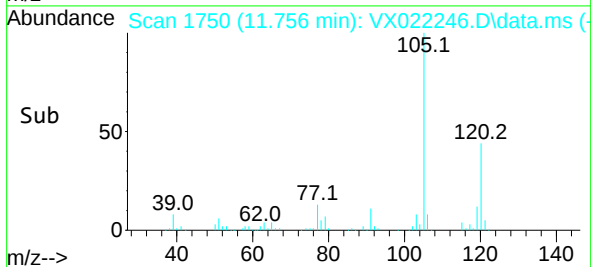

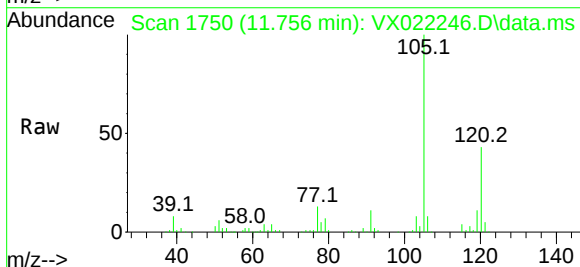




#86
p-Isopropyltoluene
Concen: 1.35 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. -0.000 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion:119 Resp: 5211
Ion Ratio Lower Upper
119 100
134 25.8 12.9 38.7
91 33.4 11.7 35.0

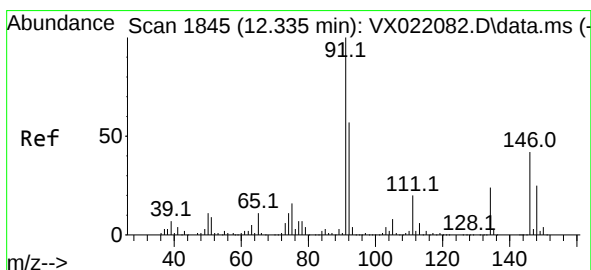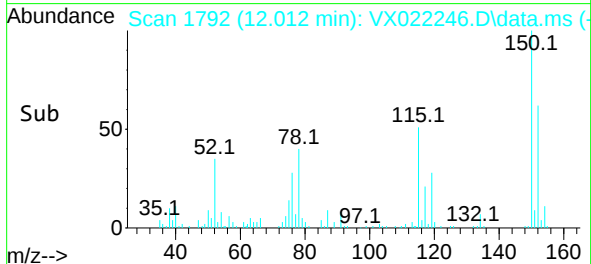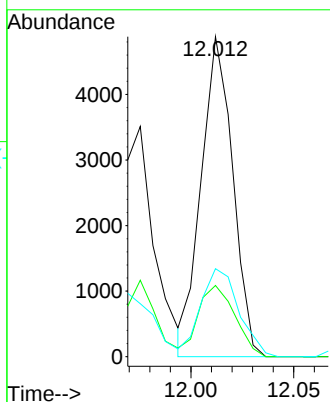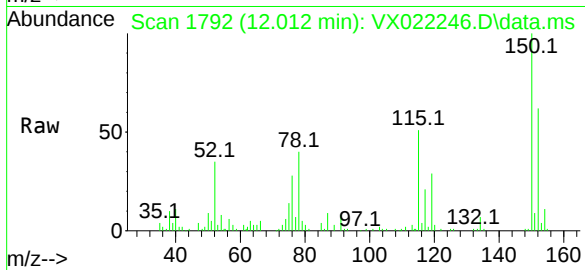

#89
n-Butylbenzene
Concen: 1.20 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. -0.006 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35

Tgt Ion: 91 Resp: 4292
Ion Ratio Lower Upper
91 100
92 29.1 27.4 82.0
134 87.3 13.2 39.5#


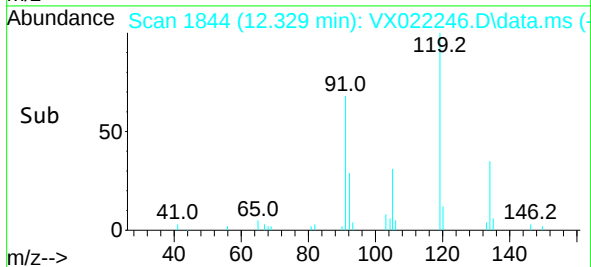
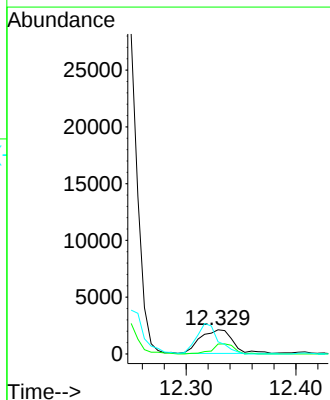
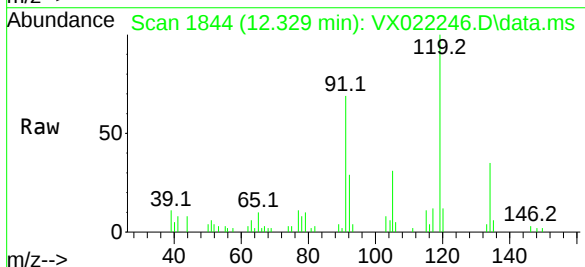




#90
Hexachloroethane
Concen: 20.47 ug/l
RT: 12.701 min Scan# 1905
Delta R.T. 0.158 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion:117 Resp: 13077
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#

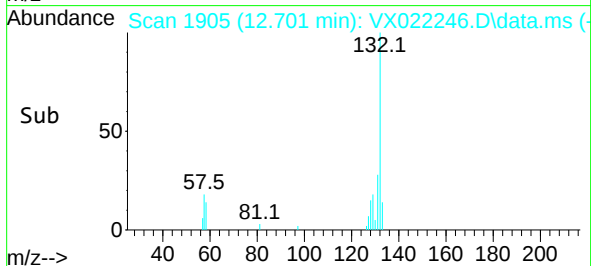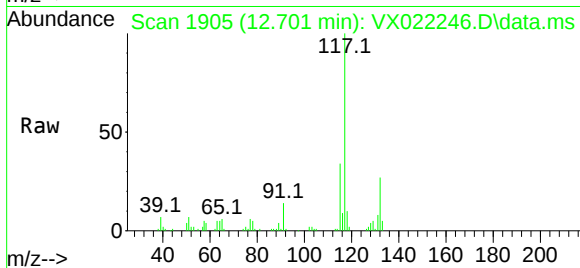

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.62 ug/l
RT: 12.969 min Scan# 1949
Delta R.T. 0.024 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35

Tgt Ion: 75 Resp: 200
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#




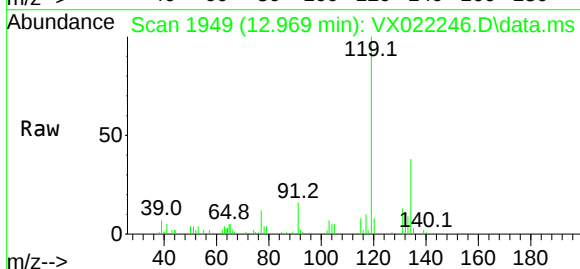




#93
1,2,4-Trichlorobenzene
Concen: 0.34 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. -0.000 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion:180 Resp: 368
Ion Ratio Lower Upper
180 100
182 77.2 47.7 143.1
145 133.4 15.0 45.0#

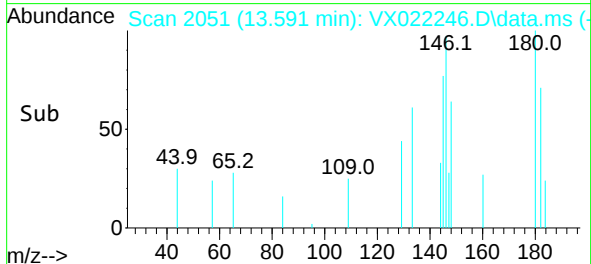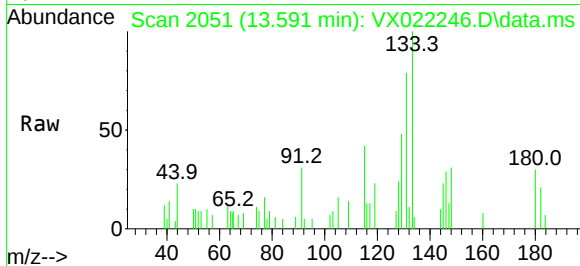

#95
Naphthalene
Concen: 332.34 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX022246.D
Acq: 27 May 2021 20:35


Tgt Ion:128 Resp: 1391229
Ion Ratio Lower Upper
128 100
127 12.7 10.3 15.5
129 11.1 8.8 13.2

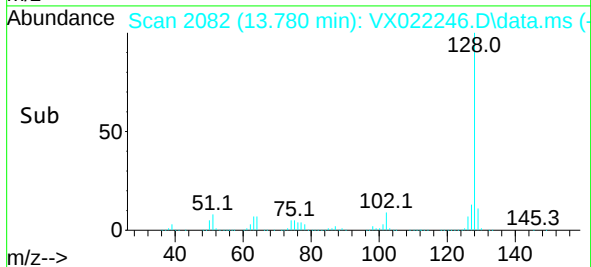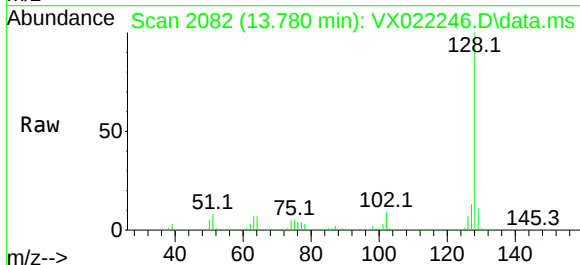

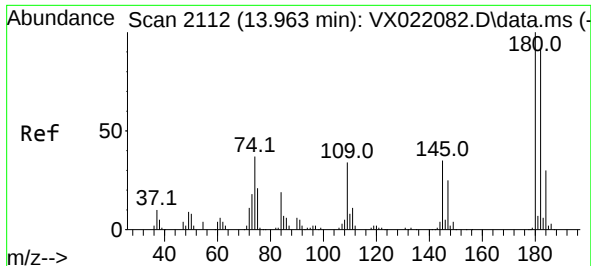

#96
 1,2,3-Trichlorobenzene
 Concen: 0.24 ug/l
 RT: 13.963 min Scan# 2112
 Delta R.T. -0.000 min
 Lab File: VX022246.D
 Acq: 27 May 2021 20:35

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-02-2021-05-24

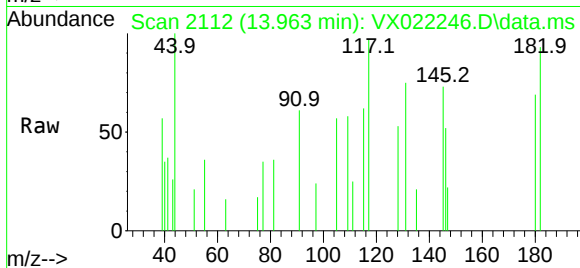

Tgt Ion:180	Resp:	263
Ion	Ratio	Lower Upper
180	100	
182	107.6	47.6 142.9
145	206.8	16.1 48.3#

