
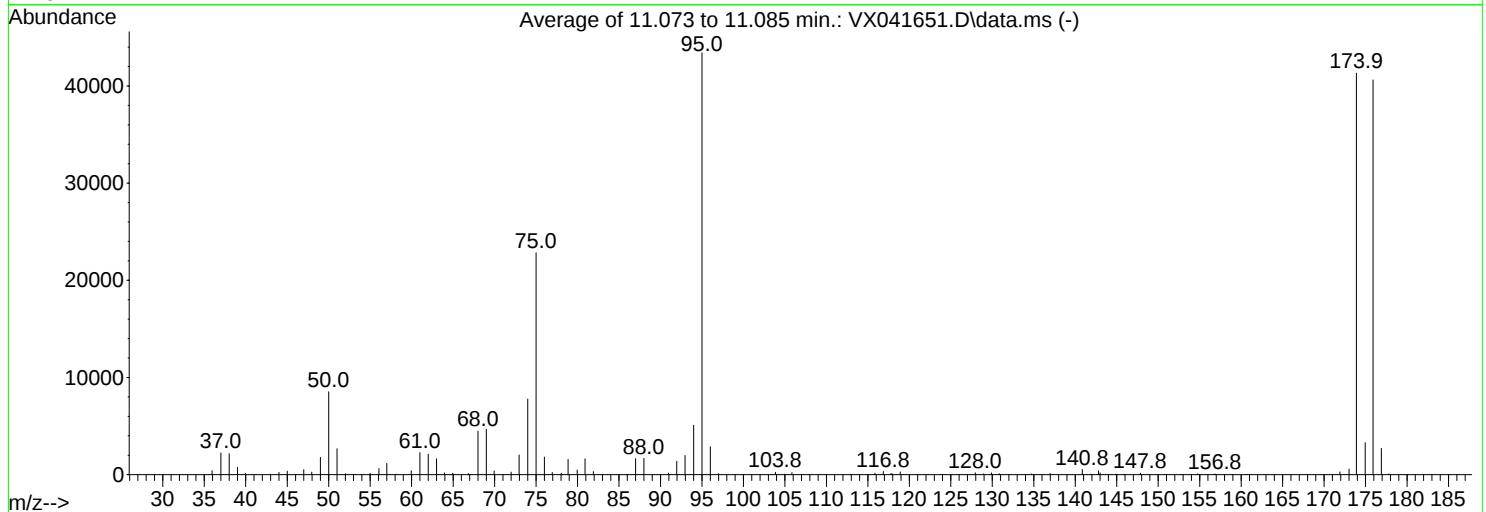


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052824\
Data File : VX041651.D
Acq On : 28 May 2024 08:44
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X051524W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu May 16 05:13:13 2024

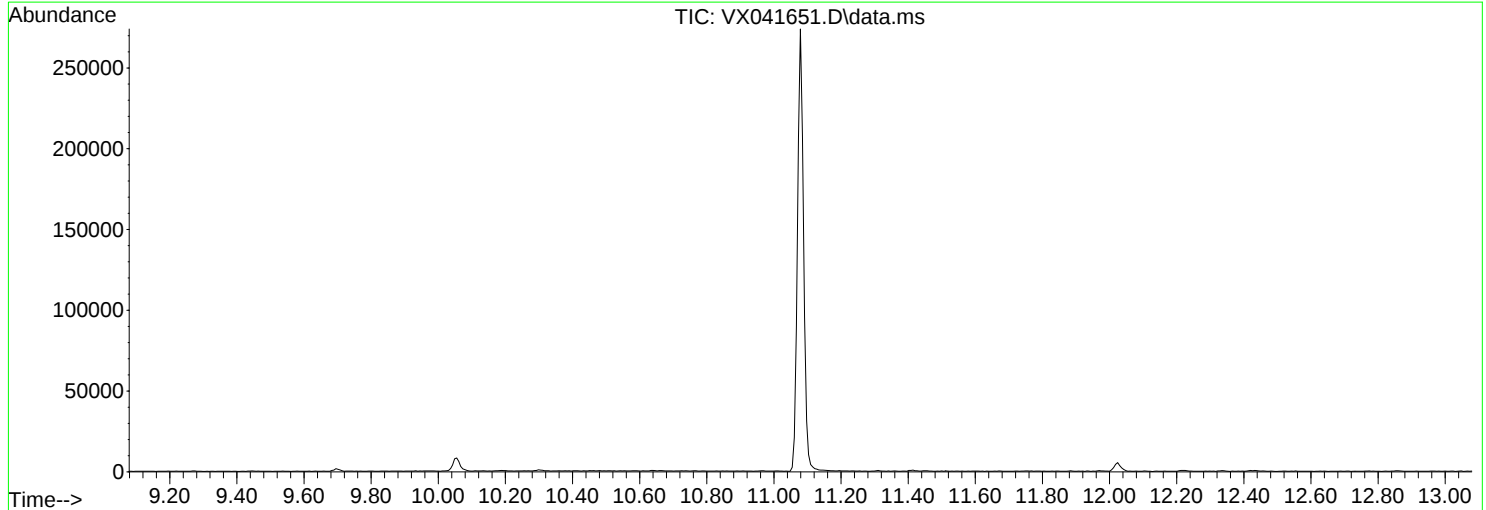

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	8535	PASS
75	95	30	60	52.6	22835	PASS
95	95	100	100	100.0	43408	PASS
96	95	5	9	6.6	2865	PASS
173	174	0.00	2	1.4	574	PASS
174	95	50	100	95.2	41323	PASS
175	174	5	9	8.0	3299	PASS
176	174	95	101	98.3	40627	PASS
177	176	5	9	6.7	2706	PASS